


DELAYED SWEEP OSCILLOSCOPE

CS-2070

70MHz 4-CHANNEL OSCILLOSCOPE

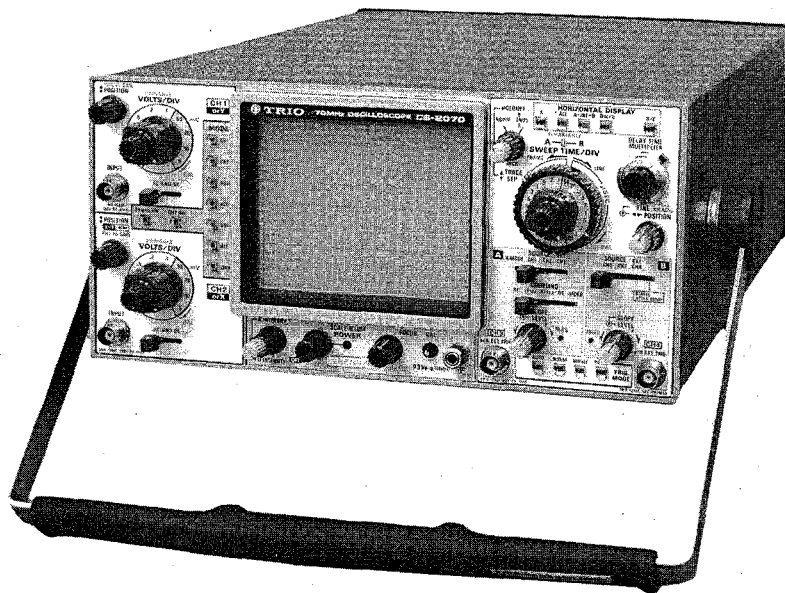

Serial Number 2110001 ~ 3060100

 **TRIO**

CONTENTS

SPECIFICATIONS	1-1	VERTICAL PREAMPLIFIER.....	6-11
CIRCUIT DESCRIPTION	2-1	VERTICAL OUTPUT AMP	6-17
BLOCK DIAGRAM	2-4	SWEEP ROTARY.....	6-18
MAINTENANCE	3-1	TRIG SWEEP.....	6-19
REMOVAL OF CASE.....	3-1	HORIZONTAL OUTPUT AMP.....	6-25
REMOVING/INSTALLING CRT.....	3-1	HORIZONTAL MODE CONTROL.....	6-26
REPLACING SWITCHING		A TRIG SWITCH.....	6-28
POWER SUPPLY	3-2	B TRIG SWITCH	6-29
TROUBLESHOOTING	3-2	POWER BLANKING.....	6-30
ADJUSTMENT	4-1	PC BOARD AND SCHEMATIC	
ADJUSTMENT OF POWER SUPPLY AND CRT.....	4-2	DIAGRAM	7-1
ADJUSTMENT OF VERTICAL AXIS (I).....	4-5	VERTICAL ATTENUATOR.....	7-2
ADJUSTMENT OF A, B TRIG AMPLIFIER.....	4-9	VERTICAL PREAMPLIFIER.....	7-4
ADJUSTMENT OF VERTICAL AXIS (II).....	4-10	VERTICAL OUTPUT AMP	7-6
ADJUSTMENT OF HORIZONTAL SWEEP	4-12	SWEEP ROTARY.....	7-8
ADJUSTMENT OF X-Y OPERATION.....	4-16	TRIG SWEEP.....	7-10
ADJUSTMENT OF TRIGGERING.....	4-16	HORIZONTAL OUTPUT AMP.....	7-12
OPERATING CHECKS.....	4-19	HORIZONTAL MODE CONTROL.....	7-14
TROUBLESHOOTING	5-1	A TRIG SWITCH.....	7-16
PARTS LIST AND DISASSEMBLY	6-1	B TRIG SWITCH	7-18
MAIN SHASSIS.....	6-2	POWER BLANKING.....	7-20
VERTICAL ATTENUATOR.....	6-9	SEMICONDUCTOR	8-1

SPECIFICATIONS

CRT

Model:	150CTM31
Display area:	8 × 10 div (1 div = 1 cm)
Type:	Rectangular, with internal graticule
Accelerating potential:	12 kV

VERTICAL AXIS (Channel 1 and Channel 2 identical specifications)

Sensitivity:	5 mV/div to 5V/div (X1 mode) 1 mV/div to 1V/div (X5 mode) 500 μV/div (Cascaded operation, CH1 to CH2)
Accuracy:	±3% (10 ~ 35°C) ±5% (0 ~ 50°C) ±8% (Cascaded operation, CH1 to CH2)
Attenuator:	5 mV/div to 5V/div in 1-2-5 sequence, all 10 ranges with fine adjustment.
Input resistance:	1 MΩ ±2%
Input capacitance:	Approx. 28 pF
Frequency response:	(Include × 5 GAIN mode)
DC:	DC to 70 MHz (-3 dB) DC to 80 MHz (-6 dB) DC to 40 MHz (-3 dB) (Cascaded operation, CH1 to CH2)
AC:	5 Hz to 70 MHz (-3 dB) 5 Hz to 80 MHz (-6 dB) 7 Hz to 40 MHz (-3 dB) (Cascaded operation, CH1, to CH2)
Risetime:	5ns
Signal delay time:	Approx 20ns as displayed on CRT screen
Crosstalk:	-40 dB minimum
Operating modes:	
CH1	CH1, single trace
CH2	CH2, single trace
DUAL	CH1 and CH2, dual trace
ADD	CH1 + CH2 (added) display
QUAD	CH1 ~ CH4, four trace
ALT	Two or four waveforms, alternating
CHOP	Two or four waveforms, chopped
CHOP frequency:	Approx 250 kHz
Polarity reversal:	CH2 only
Maximum input voltage:	500 Vp-p or 250V (DC + AC peak)
Maximum undistorted amplitude:	8 division, minimum (DC to 70 MHz)
Bandwidth limiting:	Vertical system bandwidth with the 20 MHz BW pushbutton switch pushed is approximately 20 MHz)

VERTICAL AXIS (Channel 3 and Channel 4 common specifications)

Sensitivity:	0.1V/div. ±3%
Input resistance:	1 MΩ ±2%
Input capacitance:	Approx. 28 pF
Input coupling mode:	DC only
Frequency response:	DC to 70 MHz (-3 dB) DC to 80 MHz (-6 dB)
Risetime:	5 ns
Signal delay time:	Same as CH1 and CH2
Maximum allowable voltage	
DC component:	±0.5V or less (AC + DC)
AC component:	1 Vp-p or less
Maximum input voltage:	50V (DC + AC peak)

HORIZONTAL AXIS (CH2 input)

Modes:	X-Y mode is switch selectable (HORIZONTAL DISPLAY)
X-Y mode:	CH1: Y-axis CH2: X-axis
Sensitivity:	Same as CH2
Accuracy:	Same as CH2
Input resistance:	Same as CH2
Input capacitance:	Same as CH2
Frequency response:	
DC:	DC to 5 MHz (-3 dB) DC to 6 MHz (-6 dB)
AC:	5 Hz to 5 MHz (-3 dB) 5 Hz to 6 MHz (-6 dB)
X-Y phase difference:	Less than 3° at 100 kHz

SWEEP

Modes (switchable with the HORIZONTAL DISPLAY switch):	
A	A Sweep
ALT	B Sweep waveform is displayed as an intensified portion of the A Sweep and B Sweep alternating
A-INT-B	Duration of the B Sweep is displayed as an intensified portion of the A Sweep.
B DLY'D	Delayed B sweep
X-Y	X-Y display mode
A Sweep time:	50ns/div to 0.5s/div in 22 ranges, in 1-2-5 sequence, vernier control provides fully adjustable sweep time between steps.
B Sweep time:	50ns/div to 50ms/div in 19 ranges, in 1-2-5 sequence.
Accuracy:	±3% (10 ~ 35°C) ±6% (0 ~ 50°C)
Sweep magnification:	X10 ±5% (10 ~ 35°C) ±7% (0 ~ 50°C)

SPECIFICATIONS

Linearity: 50ns/div to 0.5s/div $\pm 3\%$
 ($\pm 5\%$ with X10 magnification)
HOLD OFF: Continuously adjustable for A
 Sweep hold off time from
 NORM to X5.
Trace separation: B positionable up to 4
 divisions separated from A
 Sweep, continuously adjustable.
Delay method: Continuous delay, SYNC delay
Delay time: 0.2 to 10 times the sweep time
 from 200ns to 0.5s, continu-
 ously adjustable.
Time difference measurement accuracy:
 $\pm 2\%$ (10 ~ 35 °C)
 $\pm 4\%$ (0 ~ 50 °C)
Delay jitter: 1/20000 of the full scale
 sweep time.

TRIGGERING

A TRIG

A trigger modes: AUTO, NORM, SINGLE,
Trigger source: V MODE, CH1, CH2, EXT CH3
Coupling modes: AC, LF_{REJ}, HF_{REJ}, DC, VIDEO
 VIDEO-LINE sync automatically
 selected at sweep times of
 50 μ s/div to 50ns/div.
 VIDEO-FRAME sync automatically
 selected at sweep times
 of 0.5s/div to 0.1ms/div.
Trigger level: $\pm 90^\circ$ adjustable
Polarity: + / -

B TRIG

Trigger source: CH1, CH2, EXT CH4, STARTS
 AFTER DELAY
Coupling modes: AC only
Trigger level: $\pm 90^\circ$ adjustable
Polarity: + / -

TRIGGER SENSITIVITY (A AND B)

COUPLING	FREQ RANGE	MINIMUM SYNC AMPLITUDE	
		INT	EXT
DC	DC ~ 20 MHz	0.5div	50 mV
	DC ~ 70 MHz	1.5div	150 mV
AC	Same as for DC but with increased minimum level for below 20 Hz		
AC HF _{REJ}	Increased minimum level below 20 Hz and above 30 kHz		
AC LF _{REJ}	Increased minimum level below 30 kHz		
VIDEO	FRAME/LINE	0.5div	50 mV

AUTO: Same as above specifications for above 30 Hz.
Jitter: 1ns maximum at 70 MHz at
 5ns/div sweep rate (X10 MAG on)

CALIBRATING VOLTAGE

1 kHz $\pm 3\%$ Positive square wave
 0.3V $\pm 1\%$ (10 ~ 35 °C)
 $\pm 2\%$ (0 ~ 50 °C)

INTENSITY MODULATION

Input signal: TTL level, intensity increasing
 with more positive levels
Input impedance: Approx. 10 k Ω
Usable frequency range: DC to 10 MHz
Maximum input voltage: 50V (DC + AC peak)

VERTICAL AXIS OUTPUT

Output voltage: Sampled CH1 output
 50 mVp-p/div (into 50 Ω load)
Output impedance: Approx. 50 Ω
Frequency response: DC to 70 MHz (-3 dB)
 (into 50 Ω load)

TRACE ROTATION

Electrical, adjustable

POWER SUPPLY

Line voltage: LOW: 90 ~ 132V
 HIGH: 180 ~ 264V
Line frequency: 50/60 Hz
Power consumption: Approx. 56W

DIMENSIONS

Width: 284 mm (328 mm)
Height: 138 mm (150 mm)
Depth: 400 mm (471 mm)
 () dimensions include pro-
 trusions from basic case out-
 line dimensions.

WEIGHT

7.4 kg

ACCESSORIES

PC-29 Probes..... 2
 Instruction Manual..... 1
 Handbook..... 1
 AC power cord..... 1
 Probe holder..... 1

OPTION

Accessory Bag (MC-78)
 Panel Cover (MD-85)

ENVIRONMENT

**Operating temperature and
 humidity for guaranteed
 specifications:** 10 ~ 35 °C, 85% maximum RH
Full operating range: 0 ~ 50 °C, 90% maximum RH
Storage temperature: -20 ~ 55 °C
and humidity range: 80% maximum
Altitude:
 Operating: 5000 m
 Non-operating: 12000 m

CIRCUIT DESCRIPTION

VERTICAL ATTENUATOR

The CS-2070 input attenuator consists of two stages of attenuation-on having 1/2, 1/4 and 1/10 steps and the other having either 1/10 or 1/100 attenuation to form an overall ten point attenuator in 1-2-5 sequence.

The signal from the attenuator is passed to a dual FET impedance conversion circuit (Q1). Its output is sent to IC12. Variable gain is achieved by varying the emitter resistance of IC12.

The output of IC12 is sent to the vertical pre-amp. The arrangement for CH2 is the same as for CH1.

VERTICAL MODE LOGIC CIRCUIT

Instead of the usual mechanical switches used on other instruments the CS-2070 makes use of electronic switching. The switches themselves generate a single pulse output when operated so that the various combinations of switches and holding of selected modes must be done with external logic circuitry. The circuit that accomplishes this is the Vertical Mode Logic Circuit. The pulses generated when the switches are operated are shaped by a schmitt trigger circuit and sent to the rest of the circuitry. IC6 is a latch used to hold a single pulse. The input signal, passing through the circuit formed by D5-D11 and IC3, IC2 and IC7 is a delayed pulse which acts as the trigger for IC6. In this way IC6 holds the data that represents the fact that a switch has been depressed. IC4 acts as a logical single pole double throw switch to select one of DUAL/QUAD and ALT/CHOP. CH2 inverter and 20MHz BW switching functions are managed (ON-OFF) by IC10 which acts as a SPST switch. The output of IC4 is also latched into IC6. The output of IC6 is used to drive the vertical mode LED's through IC8, IC11, IC5 and IC9.

VERTICAL PRE-AMP CIRCUIT

The CS-2070 has four pre-amp circuits to allow 4-channel operation. The output of the vertical attenuator is fed to IC1, an amplifier.

For CH2 an inverting stage, IC2, is provided to allow switched inversion of that channel only. Q2 and Q3 form the CH1 position circuit.

Q50 and Q51 form the CH2 position circuit which operates in a similar fashion to the circuit for CH1. Q4 and Q5 are x1 amplifier stages (for CH1) and Q6, Q7 are x5 amplifier stages. The circuit formed by Q8 and Q9 is used to switch between x1 and x5 gain for CH1. For CH2, Q52/Q53 and Q54/Q55 along with Q56 and Q57 have the same functions. Q10/Q11 and Q19/Q20 for a cascoded amplifier. Q18 and Q21 in combination with Q19 and Q20 form a switching circuit. This circuit is used to turn the CH1 signal on and off.

Q12 and Q13 form the trigger amplifier. The trigger signal passes through the buffer output amplifier formed by Q14 and Q15, being converted to 50Ω impedance and is sent to the A trigger switch circuit. For channel 1 only, the vertical signal passes through the stage formed by Q16 and Q17 to

the rear panel connector for CH1 output. The circuit configuration for CH2, CH3 and CH4 is similar except that the CH3 and CH4 position adjustment is accomplished by means of PCB mounted trimmers VR1 and VR2.

The CH1 through CH4 signals are amplified by the output amplifier formed at the base side of the emitter follower formed by Q42 and Q43. This amplifier consists of Q44 and Q45 whose output is sent to the delay line.

Q38/Q39 and Q40/Q41 for the trigger amplifier which sends the signal of the output amplifier to the A trigger switch circuit and acts as the V MODE trigger source. Q37 acts as the load resistance switch for the ADD mode. Q33-Q36 form the 20MHz bandwidth circuit which limit the vertical bandwidth to -3dB down at 20MHz.

CH1 through CH4 signals are switched by the logic circuit formed by IC3 - IC7 in accordance with the vertical mode and horizontal mode selected.

VERTICAL OUTPUT AMPLIFIER

The signal from the delay line is sent to the vertical output amplifier. Q1, Q2, Q3 and Q4 form a cascoded differential input amplifier. Q11 forms a bias current stabilization circuit.

Q7 - Q10 form the final output stage.

Q5 forms the trace separation circuit.

A TRIGGER SWITCH CIRCUIT

The CH1-CH4, V MODE signals are sent to the A trigger switch circuit. S1 is the trigger source switch with S2 acting as the trigger coupling selection switch.

Q3 and Q4 form the VIDEO sync circuit which detects the trigger signal of the TV picture signal for stable display.

Q6 and Q7 form an impedance converting emitter follower circuit to lower the output impedance to drive the next stage. Q8 and Q9 form a circuit which is used to improve the CMRR. This circuit is a feedback amplifier. IC1 is a cascode amplifier used as the polarity reversal (inversion) circuit for the trigger signal. Q10 forms an impedance conversion stage used to convert the output of the IC1 stage to 50Ω for output to the horizontal sweep unit.

B TRIGGER SWITCH CIRCUIT

Basically this circuit operates as does the A trigger switch circuit. Q1 accepts the CH2 trigger input and uses this signal to form the X signal for X-Y operation. Other aspects of operation are the same as the A trigger switch circuit.

SWEEP ROTARY CIRCUIT

This circuit is a part of the sweep circuit, but is located on a separate board. It is composed of a rotary switch to select the sweep time and resistors of the HOLDOFF circuit.

CIRCUIT DESCRIPTION

HORIZONTAL SWEEP CIRCUIT

This sweep circuit uses a constant current integrated circuit to obtain sawtooth waveform by charging capacitor with constant current.

Q14, Q16, and Q18 form the circuit that switches the sweep time capacitor for A sweep. In the case of B sweep the same operation is carried out by transistors Q43, Q45 and Q47. Q13, Q15 and Q17 form the circuit that switches holdoff capacitor for A sweep.

The voltage supplied by the constant voltage circuit is converted to a constant current source by the voltage setting circuit comprised of IC3a and transistor Q8 and the resistor which is selected by the rotary switch.

This current is used to charge the sweep time capacitor, and result in a rise voltage at the capacitor terminals. This voltage is sent to a high impedance buffer amplifier composed of Q19 and Q20.

When the output of this amplifier reaches a constant voltage value, IC7d is switched on and IC2b flip-flop is reset. At the same time IC2a is set.

The output of IC2 turns on Q7 and enshorts the sweep time capacitor.

The terminal output voltage of the capacitor falls. In addition the constant current circuit which is composed of Q22 charges one of the following holdoff capacitors; C13, C19, or C23. The terminal voltage of the capacitor increases step by step. When this terminal voltage goes beyond the threshold level Q23 is turned on.

The output of Q23 turns on the SCHMIDT trigger circuit which is composed of IC2b. The output of IC2b cancels the set condition of IC2a and sweep is once again started. The trigger signal synchronizes IC2a through IC1a, IC1b.

It cancels the set of the flip-flop when it is in the set state and starts the sweep which is synchronized to the trigger signal. The SCHMITT trigger circuit is composed of IC1a and IC1b. The trigger signal which is smoothed by IC1a and IC1b is supplied to IC1c, Q3 and Q4. When there is a trigger signal, IC1d gate is closed and IC2a operates as the master slave flip-flop.

When there is no trigger signal IC2a opens the gate of IC1d and operates R-S flip-flop. This is the auto free run circuit.

Q24 to Q26 form the delay sweep level detection circuit.

When the voltage level increases as set by DELAY TIME MULTIPLIER, Q24 is turned on and triggers IC8a gate. IC8a and IC10b compose the logic differential circuit. It makes constant width pulse which activates IC5b and starts B sweep circuit is approximately the same as A sweep circuit, but it does not have 3 low speed ranges. IC4d gate is selected from master slave flip-flop using B STARTS AFTER DELAY switch, and has trigger priority to R-S flip-flop.

The sweep can be started from the voltage level set by the DELAY TIME MULTIPLIER. A sweep horizontal position adjustment is carried out by Q53, and B sweep by Q54. The selection of HORIZONTAL DISPLAY is carried out by Q55 to Q58.

A and B sweep waveforms are synthesized by Q55 and Q58 collectors and X-Y signal is also synthesized at this point by Q59.

The signal through Q60 enhances CMRR and is sent to next stage by Q62 and Q63. Q64 and Q65, and Q66 and Q67 are selected times one and times ten (X1 and X10) by Q69 and Q68 respectively. The impedance is converted to 50 ohms and is sent to the horizontal output amplifier by Q70 and Q71.

The trace SEP circuit is composed of Q78 to Q80 and two different bias voltages are sent to the vertical output amplifier by the A and B sweep signals.

IC8d is the reset-pulse generator circuit in the case of signal sweep operation and also produces the blanking control signal when it is necessary to produce horizontal display using IC13a, IC14a and IC14e.

This circuit combines the sweep and chop signal using IC11a, IC11b, IC11c, IC11d and IC12d. The impedance is converted in Q72 to Q75.

This signal becomes the input signal of the blanking circuit. The signal in the case of DUAL or QUAD setting of the vertical axis mode is produced in IC12a IC12b, IC13b, IC14c, IC14d, IC15a, IC15b, IC15c and IC15d and D48 to D50. IC12a and IC12b comprise the chop oscillator. The vertical mode logic and horizontal mode logic signal switch this oscillator on and off.

In the case of oscillation stopping this oscillator produces an alternate signal output.

On receiving a signal from IC14e, the output of IC12a and IC12b is turned off in the case of vertical axis single trace operation by IC15d.

However this output can be supplied in another case. The output of Q77 is supplied to the vertical amplifier and the output is separated into chop and alternate signals.

HORIZONTAL MODE CONTROL CIRCUIT

The switch states are latched by IC4 and IC7 which effectively makes these non-locking switches into locking types functionally.

For horizontal display D1-D9 and IC1d-IC1f are used to hold 3 bits of coded status information. Waveform shaping is used in the IC1 circuit to prevent misoperation. Diodes D10-D12 and IC2c-IC2e and IC3d form a circuit that is used to detect what switch of the horizontal group has been depressed.

The detected switch data is entered into the register IC4 which then holds the switch status. IC5 is a tri-state buffer.

IC6 is used to restore the encoded switches status information on a one to one basis for all functions. Switch status held until a particular switch is pressed for a second time.

The output of IC6 is used to drive an LED and as a control signal for blanking and sweep switching. The operation of the trigger mode switch input is the same as for the horizontal display switch group. Diodes D13-D16 and IC1a and IC1b are used to encode 2 bits of switch status information for this switch group after pulse shaping is done. D17, D18 IC2a, IC2b, IC2f and IC3a determine whether an input is present, writing into the register IC7a and IC7b the appropriate status information.

This register holds the switch status encoded information until IC8 is used to cancel, or return the status information based on alternate operation of the switches. Similar to the

CIRCUIT DESCRIPTION

horizontal display switch group, once depressed a switch mode is maintained until the switch is depressed once more. IC5a, IC5b, and IC5c are tri-state buffers. IC9a, IC9b, and IC9d—IC9f along with Q1—Q3 form buffers for the switch LED's and sweep circuit. The output from the trigger mode reset switch is pulse shaped and sent to the trigger sweep circuit.

This circuit holds data even when the instrument's power supply switch is turned OFF. That control is performed by Q4, D19, D20, D31, D100, IC3 and IC8a.

D19 and D20 form a power supply based on the capacitor for memory. IC3b and IC3c detect the power OFF condition and generate a memory save signal. The output of the above circuit forms the set of control signals used to control the vertical mode logic circuitry.

CALIBRATING VOLTAGE CIRCUIT

Q11 and Q12 form a multivibrator circuit which generates a signal which is subsequently converted to a low impedance by means of Q10 for output as the calibration signal. IC17 is used to regulate the voltage generated by this calibration circuit.

CH3 and CH4 INPUT CIRCUITS

These circuits consist of buffer amplifier. The signal from the input terminal (BNC) is impedance converted with the circuit formed by Q13a, Q13b, Q14 and Q15 and sent to the vertical pre-amplifier. The operation and configuration of the CH4 circuit is similar to the CH3 circuit.

HORIZONTAL OUTPUT AMPLIFIER

The signal from the horizontal sweep circuit is amplified by the differential amplifier formed by Q1 and Q2. The output signal of this circuit is then passed to the emitter follower circuit formed by Q5 and Q6 for impedance conversion to enable driving the circuit formed by Q7 and Q8. Q9 and Q10 form a voltage regulation circuit which serves as the DC load for Q7 and Q8 respectively with AC peaking performed by means of C15 and C16. Q11 and Q12 form an auto-bias circuit which automatically controls the operating point of the output stage.

SWITCHING POWER SUPPLY UNIT

Although the CS-2070 is light and compact, and make use of a switching regulator type power supply.

Input of either 100V or 200V is rectified and a smoothing capacitor is used to generate a smooth DC output of approximately 200V.

Next, a power transistor is used to convert this output to an AC voltage which is used to drive a compact type converter transformer. The transformer used has 6 bifilar windings which create six separate outputs which are then rectified and smoothed to provide the supply for the blanking unit directly. One of the outputs is compared with a reference voltage to form an error voltage used for regulation. The error voltage is sent to the error voltage amplifier, the output

of which is used to control the base of the power transistor. This output is isolated from the primary by means of a photocoupler.

POWER BLANKING UNIT

The five remaining outputs from the switching regulator power supply are further regulated using a series regulation method. This accomplished with Q1, Q3—Q6. IC1a, IC1b, IC2a and IC2b are error voltage amplifiers. The +20V derived by use of a resistance voltage divider. A conventional high voltage DC-DC converter is used. Q25—Q27 are error voltage amplifiers with Q29 acting as a control transistor. The CS-2070 provides independent A and B sweep intensity controls. This function is implemented by means of the circuit formed by Q13—Q15. Q17 forms the external intensity (Z-axis) modulation circuit which accepts an input and results in brighter displays for increasing inputs.

The signals from these circuits are combined at the base of Q18 to drive Q19. Q20 forms the DC load for Q19 with C25 acting to provide AC peaking for this circuit. Q21 and Q22 form the auto-focus circuit which apply a signal to the focus electrodes of a reverse phase from the blanking signal. Q23 and Q24 act to restore the DC component of the blanking and auto-focus circuits by using differential amplifiers for isolation. Q8 controls scale illumination with Q9 and Q10 controlling the adjustment of trace rotation.


HIGH VOLTAGE UNIT

The post-acceleration voltage of the CS-2070 is 12 kV requiring the high voltage unit to be protected from the hands of the user if safety is to be maintained.

This protection also is required to prevent leakage.

To achieve this goal, the high voltage unit of the CS-2070 has been encapsulated in resin to form a high voltage "block". In the block are the high voltage DC to DC converter as well as the 1.7 kV cathode voltage supplies rectifier. In addition to the anode cap which makes available 10 kV, the block has 1.7 kV DC and 6.3V AC outputs.


BLOCK DIAGRAM

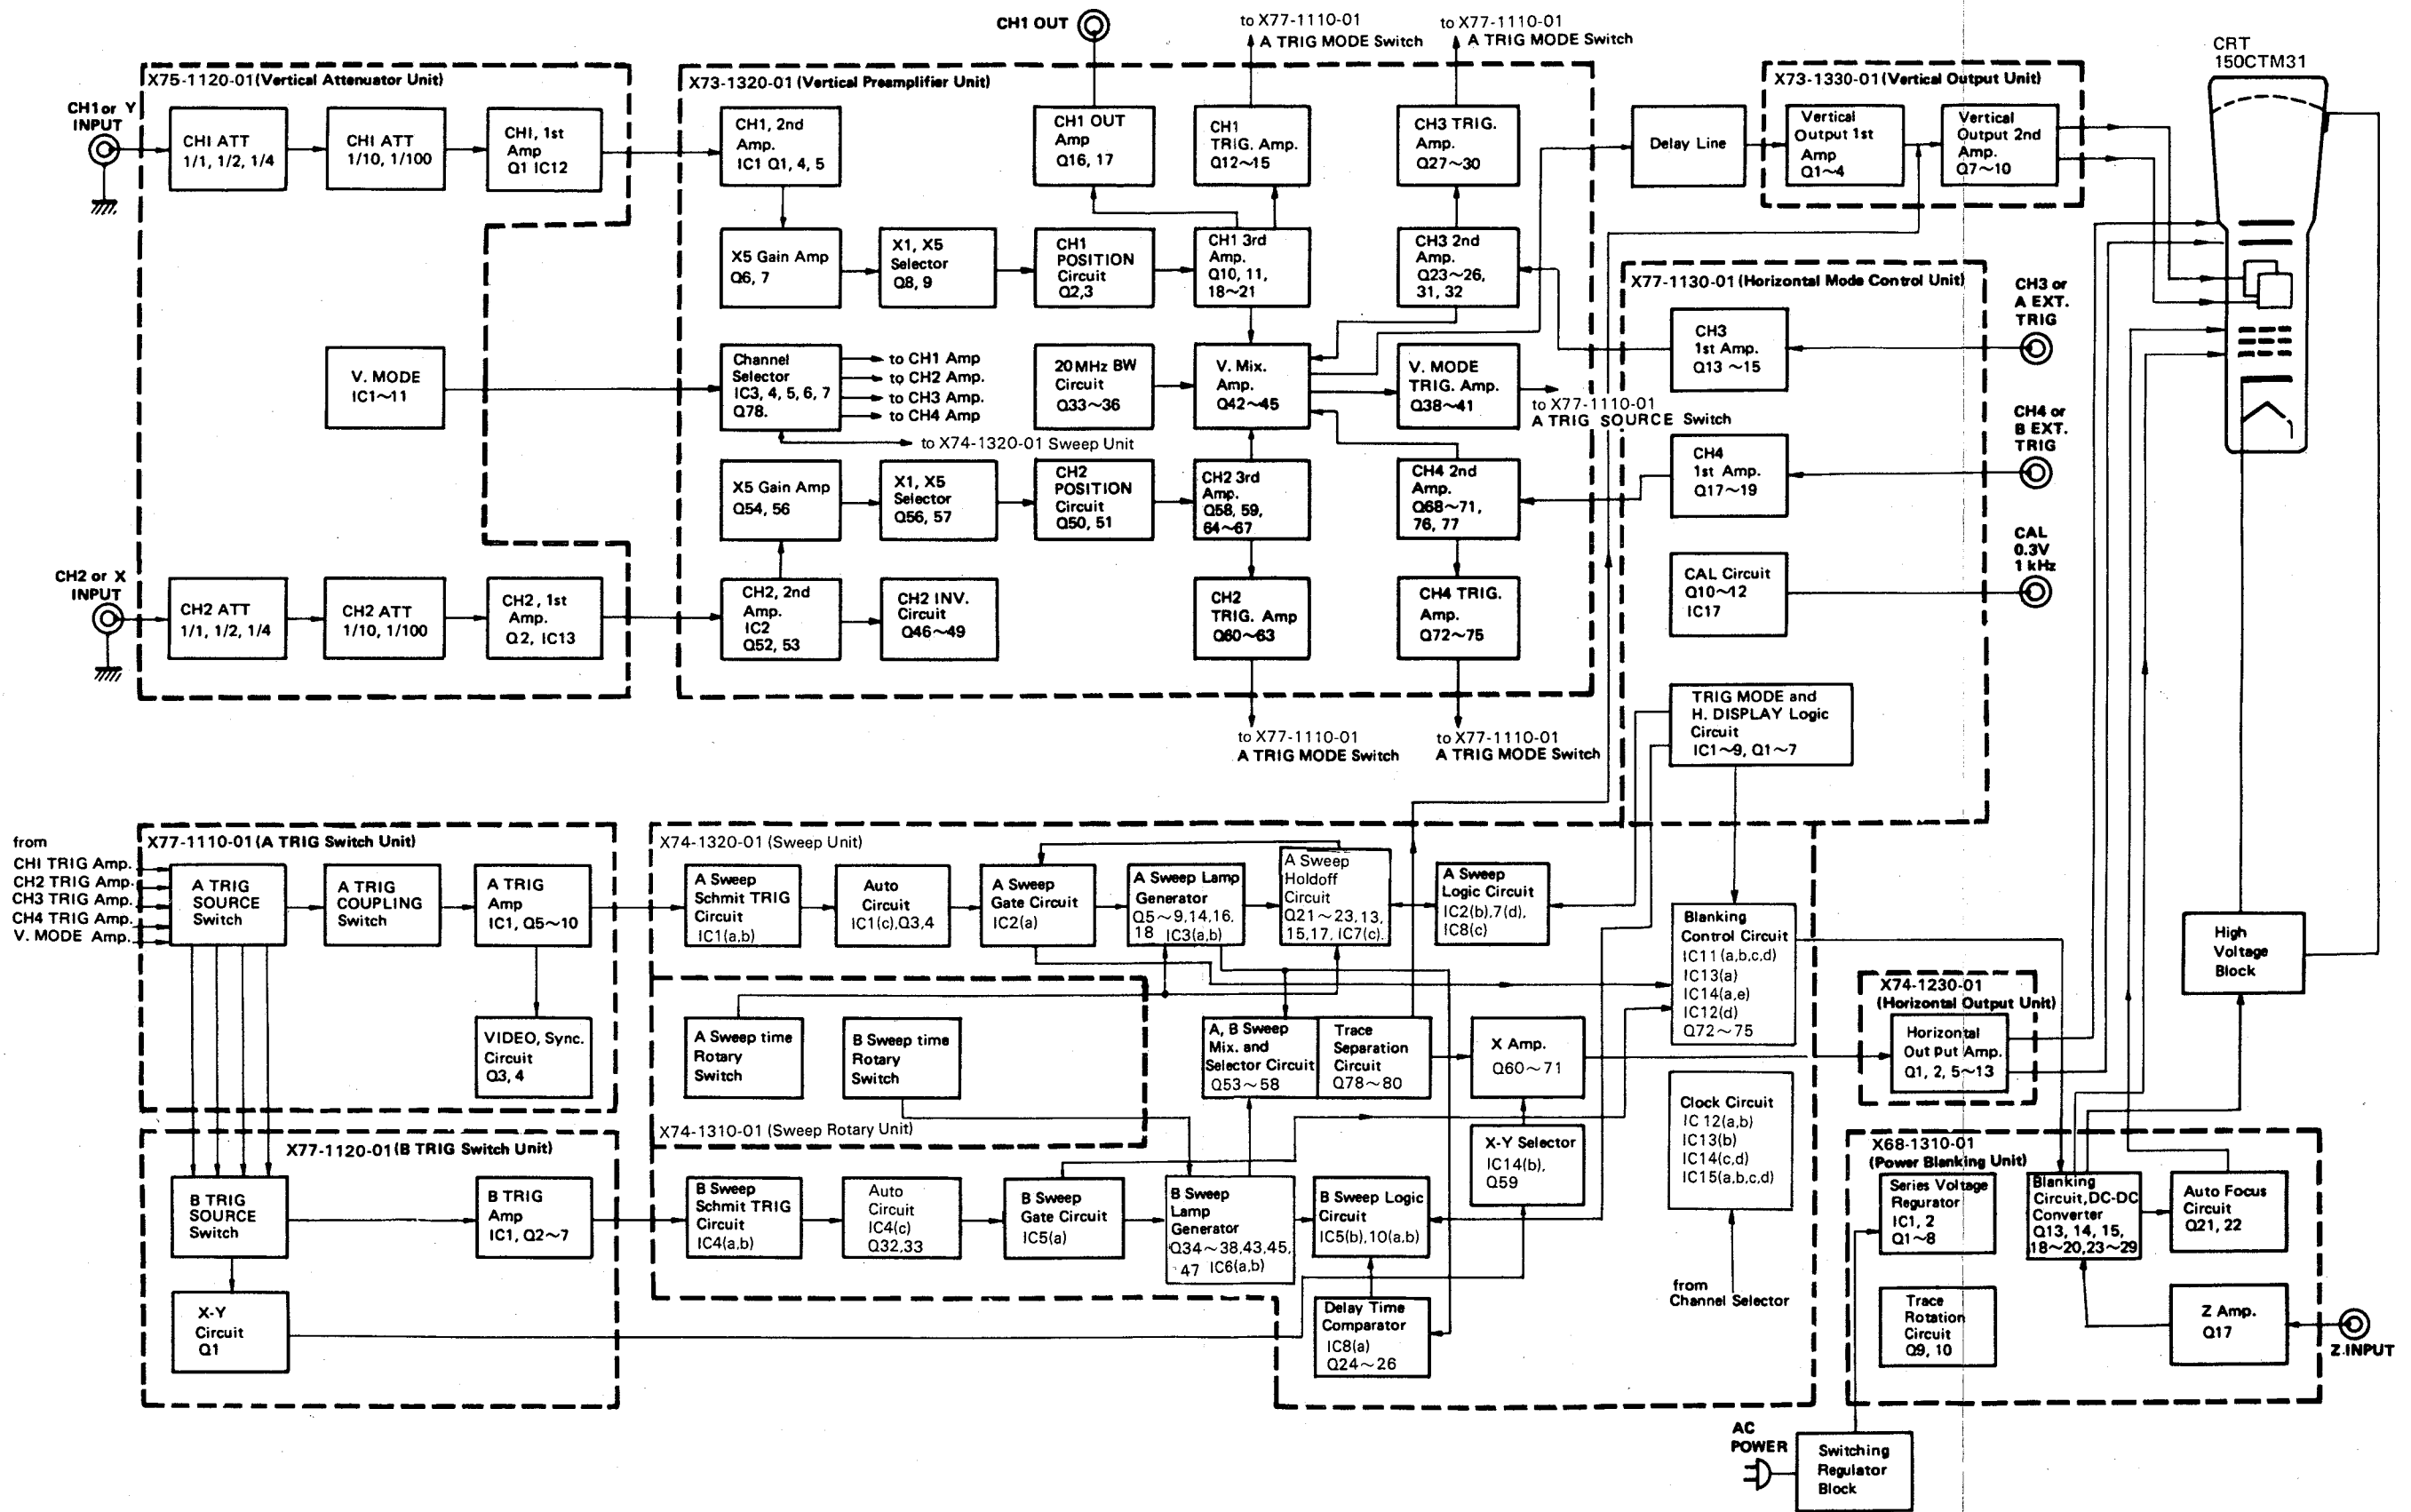

MAINTENANCE

REPLACING SWITCHING POWER SUPPLY

The switching power supply is housed in the shield case located at the rear. To remove the switching power supply, remove the horizontal logic circuitry (right) and vertical preamplifier (left) and remove the retaining screws which fix the shield case to the frame.

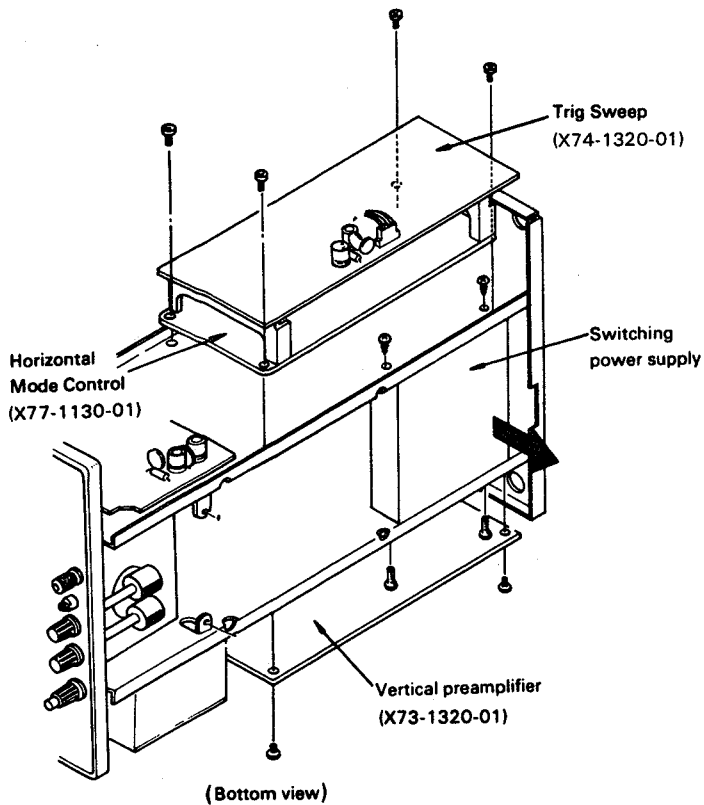

Replacing switching power supply

TROUBLESHOOTING

1. Confirm that the voltage selector is set to the correct position.
2. If one of the mode LEDs does not light, the unit will not operate correctly. When using the unit, confirm that the LED lights up.
3. To service the unit effectively, isolate the failure first. Then, remove the case and check the wiring, P.C.B. pattern and parts.
4. A low voltage power supply will affect the circuitry. Do not use the low voltage power supply for checking.

ADJUSTMENT

To obtain the best performance, periodically accurately calibrate the unit.

Sometimes, only one mode need be calibrated, while at other times, all modes should be calibrated.

When one mode is calibrated, it must be noted that the other modes may be affected. When calibrating all modes, perform the calibration in the specified sequence.

The following calibration required an accurate measuring instrument and an insulated adjusting flat blade screw-driver. If they are not available, contact your dealer.

For optimum adjustment, turn the power on and warm up the CS-2070 sufficiently (more than 30 minutes) before starting.

CAUTION:

Calibrate the unit under the following condition.

Temperature: 10 — 35°C

Humidity: Less than 85%

POWER SUPPLY VOLTAGE

Before calibrating the unit, check the power supply voltage.

Voltage selector: LOW: 90 — 132V

HIGH: 180 — 264V

50/60 Hz

TEST EQUIPMENT REQUIRED

The following instrument or their equivalent should be used for making adjustments.

Test Equipment	Model	Minimum Specification
Digital Multi-Meter	DL-720 (TRIO)	Impedance: More than 10 MΩ, Measuring range: 0.01V to 199V
Sine-Wave Generator	SG-502 (Tektronix)	Frequency: 10 Hz to 10 MHz, constant voltage over tuning range
Sine-Wave Generator	SG-503 (Tektronix)	Frequency: 50 kHz to 100 MHz, Output impedance: 50Ω, constant voltage over tuning range.
Square-Wave Generator	PG-506 (Tektronix)	Output signal: 1 kHz, Amplitude: 10 mVp-p to 10 Vp-p, Accuracy: within ±1%, Rise time: 35ns or less (1 MHz, 1ns or less)
Q Meter	4343B (YHP)	—
Color Pattern Generator	CG-911A (TRIO)	—
Oscilloscope	475A (Tektronix)	Sensitivity: More than 5 mV Frequency response: More than 250 MHz
Time-Marker Generator	TG-501 (Tektronix)	Time mark: 0.5s to 0.1μs repetitive waveform, accuracy: within 0.1%
High-Voltage Probe	—	Input Impedance: 1000 MΩ
Termination	TA-57 (TRIO)	Impedance: 50Ω
Attenuator	011-0059-02	—20 dB attenuation (50Ω)

Test Equipment	Model	Minimum Specification
Power Meter	2041 (YEW)	—
Auto transformer (variable)	SD-265 (Tektronix)	—
Current Probe	P6302 AM-503 (Tektronix)	—
Frequency Counter	FC-754A (TRIO)	—

PREPARATION FOR ADJUSTMENT

Control Setting

The control settings listed below must be used for each adjustment procedure. Exceptions to these settings will be noted as they occur. After completing a adjustment, return the controls to the following settings.

Power Section

POWER ON

CRT Control Section

A INTEN Between 12 and 3 o'clock position
 B INTEN Between 12 and 3 o'clock position
 FOCUS Optimum position
 SCALE ILLUM Arbitrary position

Vertical Section

VARIABLE (CH1 and CH2) CAL
 ▲ POSITION (CH1 and CH2) 12 o'clock position
 AC-GND-DC (CH1 and CH2) AC
 VOLTS/DIV (CH1 and CH2) 5V/DIV
 × 5 GAIN OFF

Horizontal Sweep Section

A SWEEP TIME/DIV 0.1ms/DIV
 B SWEEP TIME/DIV 0.1ms/DIV
 A VAR CAL
 DELAY TIME MULTIPLIER Arbitrary position
 ▲ TRACE SEP. Fully CCW
 HOLDOFF NORM
 B ENDS A OFF
 ► POSITION 12 o'clock position
 FINE PULL × 10 MAG 12 o'clock position (× 10 MAG OFF)

TRIG. Section

A TRIG SOURCE V. MODE
 A COUPLING AC
 A TRIG LEVEL 12 o'clock position
 A TRIG SLOPE +
 B TRIG SOURCE CH1
 B TRIG LEVEL 12 o'clock position
 B TRIG SLOPE +

Mode Section

V. MODE CH1
 20MHz BW OFF
 CH2 INV OFF
 TRIG. MODE AUTO
 HORIZONTAL DISPLAY A

MAINTENANCE


REMOVAL OF CASE

1. Pull out CH3 and CH4 POSITION knobs.
2. Remove the 4 screws located at the rear of the case and the 1 located at bottom with a \oplus screwdriver. Carefully slide the body forward from the case.
3. To install the body in the case, place the case horizontally and slide the body into the case using the rails located at the bottom of the case. Then, place the body vertically and engage the case front edge into the front panel groove.

4. Temporarily insert the case retaining screws and then tighten them evenly.
5. Install the CH3 and CH4 POSITION knobs.

CAUTION:

A voltage of 12 kV is applied to the CRT socket and anode cap. Before removing the case, turn the power off and pull out the power plug. After removing the case, take care not to touch them.

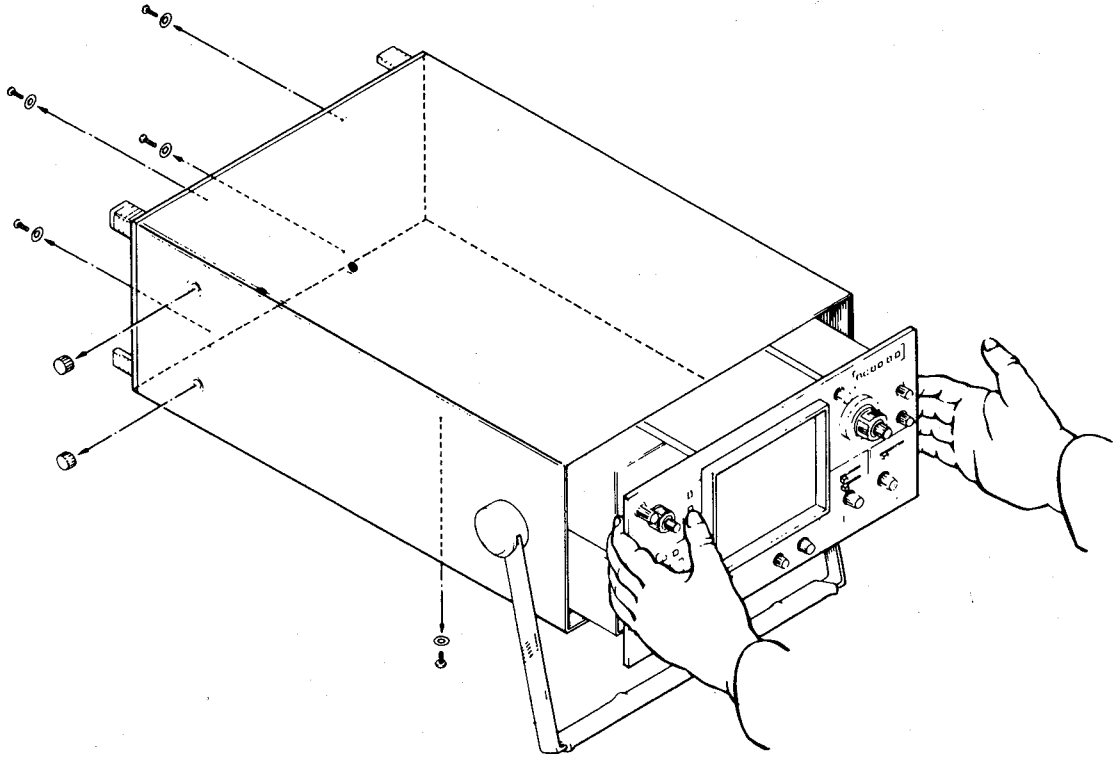


REMOVING/INSTALLING CRT

1. When servicing CRT, do not loosen the CRT band. Only remove the CRT retaining screws, then slide the CRT backward and raise the socket. The CRT can be removed easily.
2. Insert the CRT from the socket side until the CRT comes in contact with the shield plate and tighten the CRT band retaining screws.
3. As slots are provided in the CRT bracket, the CRT can be moved right and left, and back and forth. As the bracket is inclined by 45° , the CRT can be positioned in an arbitrary position. To fix the CRT, fix the CRT band, then fix the bracket.


CAUTION:

A high tension voltage is remained at the anode of the CRT. Before removing the CRT, connect the anode to the ground via a 100 k Ω load for 5 seconds to discharge the voltage.



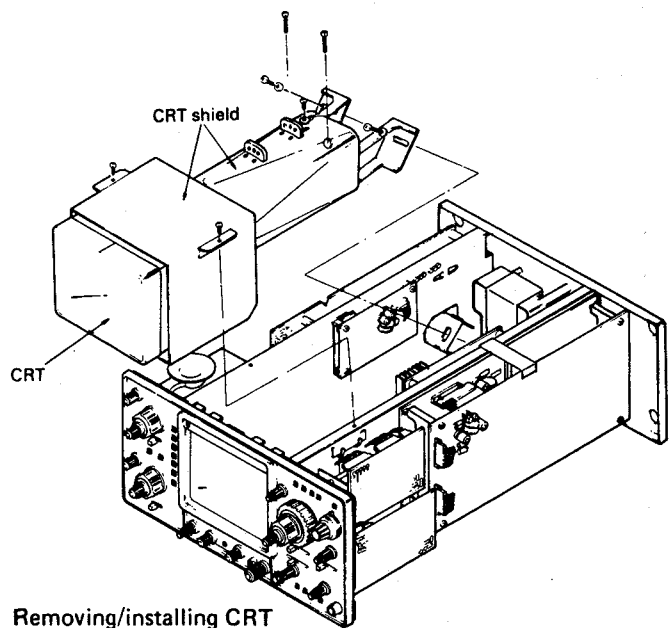


Removing/installing CRT


ADJUSTMENT

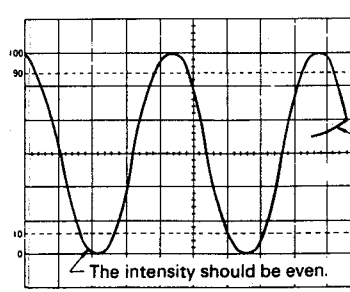Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark																											
ADJUSTMENT OF POWER SUPPLY AND CRT																																		
Checking of Power Supply		X68-1310	475A DL-720		(1) Measurement and checking of voltages at P27 and P30 pins <table border="1" style="margin-left: auto; margin-right: auto; border-collapse: collapse;"> <thead> <tr> <th></th> <th>1P</th> <th>2P</th> <th>3P</th> <th>4P</th> <th>5P</th> <th>6P</th> <th>7P</th> <th>8P</th> </tr> </thead> <tbody> <tr> <td>P27</td> <td>+120V</td> <td>+55±1V</td> <td>20V</td> <td></td> <td></td> <td>+5.2V</td> <td>+10V</td> <td>-10V</td> </tr> <tr> <td>P30</td> <td>24V±2V</td> <td>55V</td> <td></td> <td>130V ±3V</td> <td>7V±0.5V</td> <td>12V +1.5V-0.5V</td> <td>-12V +0.5V-1.5V</td> <td></td> </tr> </tbody> </table>		1P	2P	3P	4P	5P	6P	7P	8P	P27	+120V	+55±1V	20V			+5.2V	+10V	-10V	P30	24V±2V	55V		130V ±3V	7V±0.5V	12V +1.5V-0.5V	-12V +0.5V-1.5V			
	1P	2P	3P	4P	5P	6P	7P	8P																										
P27	+120V	+55±1V	20V			+5.2V	+10V	-10V																										
P30	24V±2V	55V		130V ±3V	7V±0.5V	12V +1.5V-0.5V	-12V +0.5V-1.5V																											
Adjustment of 1.6kV	VR7	X68-1310	DL-720 High voltage probe		(2) Measure the voltage on 2P of P33 and adjust VR7 to obtain 1.6kV.																													
Coarse adjustment of ASTIG and FOCUS	VR9 FOCUS Knob	X68-1310		H. DISPLAY: X-Y CH1, CH2 AC-GND-DC: GND A INTENSITY: 3 o'clock 20 MHz B.W: ON	(1) Operate \blacktriangleleft POSITION knobs for CH1 and CH2 to position the spot in the center of the CRT screen. (2) Adjust VR9 to make the spot round and smaller.																													
Adjustment of A INTENSITY	VR5	X68-1310		H.DISPLAY: X-Y A. INTENSITY: 9 o'clock CH1, CH2 AC-GND-DC: GND 20 MHz B.W: ON	Adjust VR5 so that the spot on the CRT screen disappears when A INTENSITY is set in the position of 9 o'clock. < Check > (1) Make sure that the spot on the CRT screen increases in brightness when A INTENSITY is turned CW and that the trace becomes almost extinguished when A INTENSITY is turned CCW (9 o'clock position).																													
Checking of B INTENSITY				H. DISPLAY: ALT V. MODE: CH1 TRIG. MODE: AUTO B TRIG. SOURCE: STARTS AFTER DELAY CH1, AC-GND-DC: AC B SWEEP TIME/DIV: 0.1ms	(1) Operate \blacktriangleleft TRACE SEP to cause B sweep line in the center of the CRT screen. (2) Make adjust so that the trace becomes extinguished when B INTENSITY is turned to fully CCW. when B INTENSITY is turned CCW. (3) Make adjust so that the trace becomes extinguished when B INTENSITY is turned to fully CCW.																													
Adjustment of Blanking	TC2	X68-1310	SG-502	H.DISPLAY: A V.MODE: CH1 TRIG. MODE: AUTO A TRIG SOURCE: V.MODE A COUPLING: AC A INTENSITY: Fully CW CH1. AC-GND-DC: AC A SWEEP TIME/DIV: 0.05μs	(1) Apply a sine wave signal of 10 MHz to CH1 INPUT and operate \blacktriangleleft POSITION, \blacktriangleleft POSITION and CH1 VOLTS/DIV to bring out a waveform with a vertical amplitude of 6 div on the screen. (2) Make adjustment so that there is no unevenness in intensity of the trace at the waveform starting point and there is no retrace.																													
Adjustment of Z-axis Input Blanking	TC1	X68-1310	SG-503	H. DISPLAY: A V. MODE: CH1 TRIG. MODE: AUTO A. TRIG SOURCE: V. MODE CH1 AC-GND-DC: DC VOLTS/DIV: 2V	(1) Set A SWEEP TIME/DIV at 5μs and apply a 1MHz sine wave signal of 10Vp-p to CH1 INPUT so that a waveform with a vertical amplitude of 5 div appears on the screen. (2) Apply the same signal above to the Z INPUT, and turn A INTENSITY CCW so that the dark and bright area of the waveform are distinct. (3) Adjust so that the bright area of the sine waveform is symmetrical to the peak point.																													


ADJUSTMENT

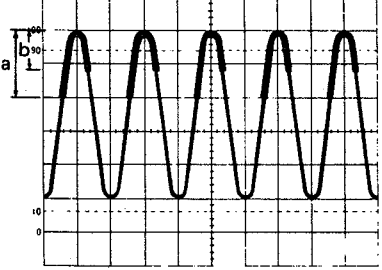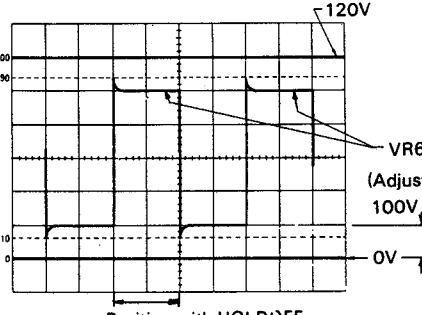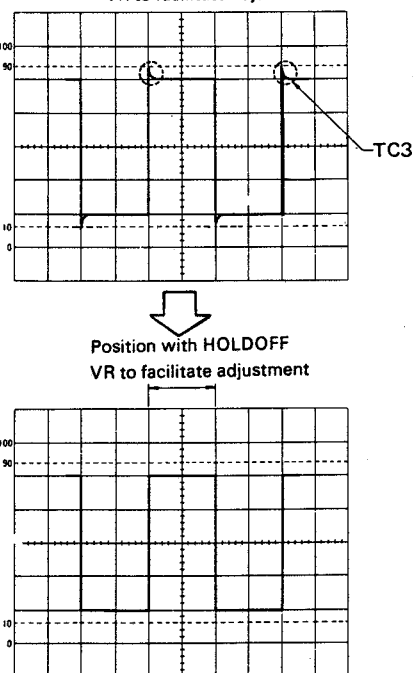Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
							
Adjustment of Auto FOCUS Level	VR6	X68-1310	475A Probe (1/10)	H. DISPLAY: A A. INTENSITY: Fully CW TRIG. MODE: AUTO V. MODE: CH1: A. TRIG SOURCE: V. MODE A. SWEEP TIME/DIV: 20μs HOLDOFF: NORM	<ol style="list-style-type: none"> (1) Set the oscilloscope (475A) for the vertical axis sensitivity at 2V/div. (2) Observe the waveform of AUTO FOCUS circuit (F.TP pattern) with a probe and make adjustment so that DC level of top of the square wave is approx. 100V (4.5~5 div.) 		<p>< Note > Be sure that the AC-GND-DC selector switch of the oscilloscope (475A) is at "DC" position.</p>
Adjustment of Auto FOCUS wave Forming	TC3	X68-1310		H. DISPLAY: A A INTENSITY: Fully CW TRIG MODE: AUTO V. MODE: CH1 A. TRIG SOURCE: V.MODE A SWEEP TIME/DIV: 20μs HOLDOFF: NORM	Make adjustment so that the above-mentioned circuit has an ideal waveform.		
Adjustment of ASTIG and FOCUS	VR9 FOCUS knob	X68-1310		H. DISPLAY: X-Y CH1, CH2 AC-GND-DC: GND A. INTENSITY: 3 o'clock	<ol style="list-style-type: none"> (1) Operate \updownarrow POSITION for CH1 and CH2 so that the bright spot is brought into the center of the CRT screen. (2) Make adjustment to make the spot round and smaller. <p>< Check ></p> <ol style="list-style-type: none"> (1) Make sure that the bright spot grows larger when the FOCUS knob is turned CW or CCW. (2) Make sure that the FOCUS knob is in a position within the range of 9 and 3 o'clock when the spot is smallest. (3) The most ideal point should be obtained by repeating the above operations and adjustment. 		<p>< Note > Be sure to bring the bright spot into the center of the CRT screen. It may be difficult to obtain the correct adjusting position near the edge of the screen due to the CRT peripheral blur.</p>

ADJUSTMENT

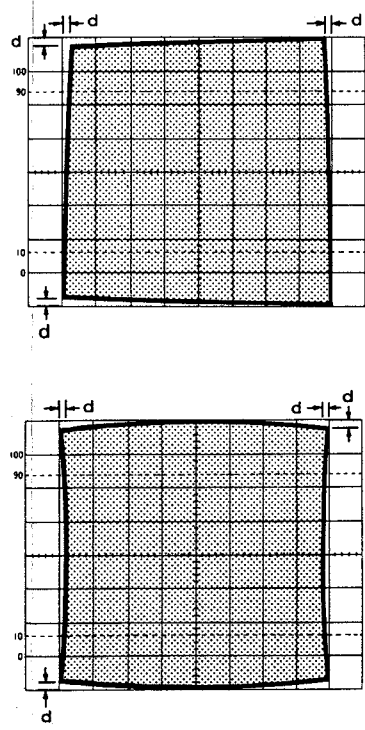Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Adjustment of Trace Rotation	VR2	X68-1310		H.DISPLAY: A V. MODE: CH1 TRIG. MODE: AUTO CH1, AC-GND-DC: GND	(1) Operate \updownarrow POSITION for CH1 to move the trace to the center of the CRT screen. (2) Make adjustment to align the trace with the horizontal center graticule line. < Check > (1) Make sure that the trace moves more than 0.3 div (10°) up and down from the horizontal center graticule line at its righthand end.		< Note > When the trace does not appear fully across the screen, make proper adjustment by operating VR9 (X74-1320) and VR7 (X74-1320)
Adjustment of Perpendicularity	VR3	X68-1310	SG-502	H. DISPLAY: X-Y CH1, CH2 AC-GND-DC: AC	(1) Apply a 1 kHz sine wave to CH1 INPUT and adjust the oscillator (SG-502) output to produce a waveform with a vertical amplitude of 8 div. (2) Operate \updownarrow POSITION knobs for CH1 and CH2 to produce a trace in the center of the CRT screen. (3) Make adjustment so that the trace is vertical (within $90^\circ \pm 1^\circ$) < Check > Make sure that the trace moves more than 0.1 div left and right at the topmost end of the vertical center graticule line. Readjust the trace rotation.		
Adjustment of Pattern Distortion	VR10	X68-1310	SG-502	H.DISPLAY: X-Y CH1, CH2 AC-GND-DC: AC	(1) Apply a sine wave signal of 100 kHz to CH1 INPUT and a sine wave signal of 1 kHz to CH2 INPUT and adjust the oscillator output to produce a square with the sides of 8 div on the CRT screen. (2) Adjust VR10 so that the horizontal and vertical bendings are less than 0.2 div.	 <p style="text-align: center;">$d = 0.2 \text{ div. or less}$</p>	




ADJUSTMENT

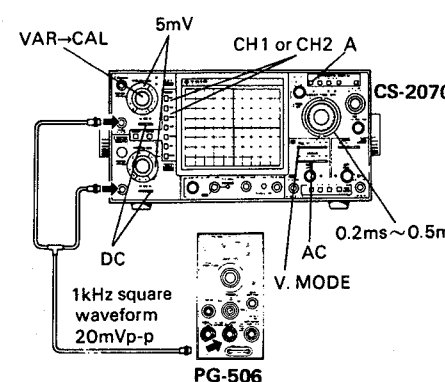Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Adjustment of CRT Center	VR1	X73-1330		H. DISPLAY: A V. MODE: CH1 TRIG. MODE: AUTO CH1. AC-GND-DC: GND	Short-circuit the test point of X73-1320 and adjust VR1 so that the trace becomes aligned with the horizontal center graticule line.		
ADJUSTMENT OF VERTICAL AXIS (I)							
Adjustment of CH1 DC BAL	VR1	X75-1120		H. DISPLAY: A V. MODE: CH1 TRIG. MODE: AUTO CH1. AC-GND-DC: GND CH1. VOLTS/DIV: 5mV	(1) Turn CH1 VARIABLE knob to fully CCW. (2) Adjust CH1 \downarrow POSITION so that the trace becomes aligned with the horizontal center graticule line on the CRT screen. (3) Turn VARIABLE to CAL and make adjustment so that the trace becomes aligned with the horizontal center graticule line on the CRT screen. (4) Repeat the above procedure. < Check > Movement of trace Less than 0.8 div.		< Note > If the trace does not come to the center of the screen even when \downarrow POSITION is operated, adjust VR4 (X73-1320).
Adjustment of CH2 DC BAL	VR2	X75-1120		H. DISPLAY: A V. MODE: CH2 TRIG. MODE: AUTO CH2. AC-GND-DC: GND CH2. VOLTS/DIV: 5 mV	Same with the adjustment of CH1 DC BAL		< Note > CH2 position center can be adjusted by VR14 (X73-1-320).
Adjustment of CH1 Gain	VR3	X73-1320	BNC-BNC cord T junction PG-506 50 Ω Termination	H. DISPLAY: A V. MODE: CH1 TRIG. MODE: AUTO A. TRIG SOURCE: V.MODE CH1. AC-GND-DC: DC CH1. VOLTS/DIV: 5mV V. VAR: CAL 20 MHz B.W: ON	(1) Apply a square wave signal of 20 mVp-p, 1 kHz to CH1 and CH2 INPUT. (2) V. MODE select to CH1 and operate CH1 and CH2 \downarrow POSITION to produce a waveform in the center of the CRT screen. (3) Synchronize by operating A TRIG LEVEL. (4) Adjust VR3 so that the vertical amplitude of the waveform becomes 4 div. < Check > Turn CH1 VOLTS/DIV and input a reference signal so that the vertical amplitude will be 4 to 6 div in each range. Sensitivity error within $\pm 3\%$		< Reference > Method of calculation of sensitivity error $\text{Sensitivity error} = \frac{a - b}{b} \times 100\%$ a = CRT screen amplitude b = Input signal voltage / (VOLTS/DIV) (Example): CRT screen amplitude: 4.2 div Input signal: 20mVp-p 1 kHz square wave VOLTS/DIV: 5mV Sensitivity error $= \frac{4.2 \text{ div} - 20\text{mV}/5\text{mV}}{20\text{mV}/5\text{mV}} \times 100 = 5\%$
Adjustment of CH2 Gain	VR13	X73-1320		H. DISPLAY: A V. MODE: CH2 TRIG MODE: AUTO A TRIG SOURCE: V.MODE CH2 AC-GND-DC: DC CH2 VOLTS/DIV: 5mV V. VAR: CAL 20 MHz B.W: ON	(1) With V. MODE selected to CH2, turn VOLTS/DIV to 5mV and perform the same operations as described above to make adjustment and check. < Check > (1) Select V. MODE to DUAL and ALT position and turn VOLTS/DIV for CH1 and CH2 and apply a square wave of 20mVp-p, 1 kHz to CH1 INPUT. Make sure that CH1 and CH2 have the same amplitude.		< Note > Overshoot or tilt might appear to the reference signal of 1 kHz square wave. In this case, make corase adjustment of square wave characteristics.



ADJUSTMENT

Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
					(2) Switch V. MODE to ADD and A. TRIG SOURCE to CH1 (CH2) and press CH2 INV pushbutton switch (the lamp will go on when this switch is pressed and it will go off when pressed again). Operate \updownarrow POSITION for CH1 and CH2 to produce a single trace in the center of the CRT screen. If a single and straight trace cannot be obtained, adjust VR3 again. <u>Channel error: Within 3%</u>		
Adjustment of CH1 \updownarrow POSITION and CH2 \updownarrow POSITION	VR4 VR14	X73-1320 X73-1320		V. MODE: DUAL, ALT H.DISPLAY: A TRIG.MODE: AUTO CH1, CH2 VOLTS/DIV: 5mV CH1, CH2 AC-GND-DC: GND CH1, CH2 \updownarrow POSITION: 12 o'clock A SWEEP TIME/DIV: 0.1ms	Adjust VR4 and VR14 so that the CH1 and CH2 traces become aligned with the horizontal center graticule line on the CRT screen. < Check > (1) The deviation from the horizontal center graticule line on the CRT screen must be within ± 1 div. (2) When \updownarrow POSITION for both CH1 and CH2 is turned fully CW, the trace must move upward more than 4 div and when the knob is turned fully CCW the trace must move downward more than 4 div.		
Adjustment of CH2 INV Position	VR15	X73-1320			Press CH2 INV (the lamp is on) and adjust VR15 to bring the trace to its position at CH2 NORM (the lamp is off). < Check > (1) Vertical deviation between CH2 NORM and INV : within ± 0.5 div (2) Press CH2 INV and turn CH2 \updownarrow POSITION fully CW and see if the trace moves more than 4 div upward and it moves more than 4 div downward when the knob is turned fully CCW.		
Adjustment of CH1 X5 Gain and CH2 X5 Gain	VR6 VR17	X73-1320 X73-1320	PG-506	H. DISPLAY: A V. MODE: DUAL, ALT TRIG.MODE: AUTO CH1, CH2 VOLTS/DIV: 5mV CH1, CH2 AC-GND-DC: DC CH1, CH2 X5 GAIN: PULL A SWEEP TIME/DIV: 0.2ms V.VAR: CAL	(1) Apply a square wave signal of 5 mVp-p to CH1 INPUT and make adjustment so that the CRT screen amplitude becomes 5 div. (2) Apply the same signal to CH2 and make the similar adjustment. < Check > (1) The sensitivity error must be within $\pm 3\%$. (2) For both CH1 and CH2, the lamp must go on when PULL X5 GAIN is pulled and go off when the button is pressed. (3) The UNCAL lamp must go off when VARIABLE is operated to CAL and go on when the knob is turned to UNCAL. (CCW)		< Note > If no waveform appears on the screen when the knob is pulled, make coarse adjustment by operating X5 Gain Position Adjustment. CH1: VR5 (X73-1320) CH2: VR16 (X73-1320)
Adjustment of CH1 X 5 Gain Position and CH2 X 5 Gain Position	VR5 VR16	X73-1320 X73-1320		H. DISPLAY: A V. MODE: DUAL, ALT TRIG. MODE: AUTO CH1, CH2 VOLTS/DIV: 5mV CH1, CH2 AC-GND-DC: GND CH1, CH2 X5 GAIN: PULL CH1, CH2 \updownarrow POSITION: 12 o'clock A SWEEP TIME/DIV: 0.1ms	Adjust VR5 and VR16 so that the trace of CH1 and CH2 become aligned with the horizontal center graticule line on the CRT screen. < Check > The distance from the center graticule line must be within ± 1 div.		< Note > If sometimes happens that the trace grows thicker at X5 GAIN, thus making it difficult to obtain proper adjustment. In this case, press 20 MHz BW (the lamp is on) button switch to make the line thinner.


ADJUSTMENT

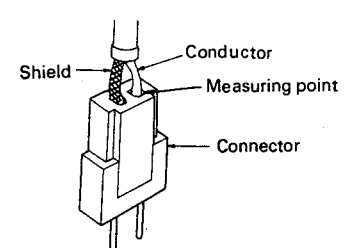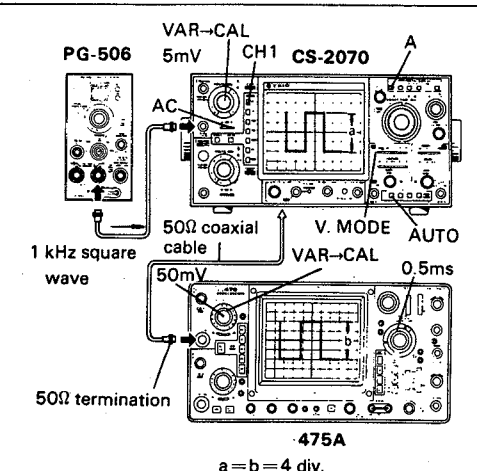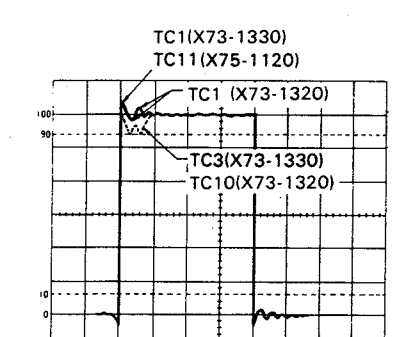Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark															
Adjustment of CH1 DC Trig Level CH2 DC Trig Level CH3 DC Trig Level CH4 DC Trig Level	VR7 VR19 VR10 VR20	X73-1320 X73-1320 X73-1320 X73-1320	DL-720	H. DISPLAY: A V. MODE: QUAD CH1, CH2 AC-GND-DC: GND TRIG. MODE: AUTO	(1) Operate CH1 and CH2 \updownarrow POSITION and CH3 and CH4 \updownarrow POSITION to align the trace with each other on the center of the CRT screen. (2) Make adjustment so that the voltage at all the check points may be zero ($-0.008 \sim +0.008V$).		< Note > Use the connector lead for making measurement at the check points. Adjust the voltage in the conductor to zero.															
					<table border="1" style="margin-left: auto; margin-right: auto;"> <thead> <tr> <th>Item of Adj.</th> <th>Adj. Control</th> <th>Check point</th> </tr> </thead> <tbody> <tr> <td>CH1 DC Trig Level</td> <td>VR7</td> <td>P15 (X73-1320)</td> </tr> <tr> <td>CH2 DC Trig Level</td> <td>VR19</td> <td>P16 (X73-1320)</td> </tr> <tr> <td>CH3 DC Trig Level</td> <td>VR10</td> <td>P17 (X73-1320)</td> </tr> <tr> <td>CH4 DC Trig Level</td> <td>VR20</td> <td>P18 (X73-1320)</td> </tr> </tbody> </table>	Item of Adj.	Adj. Control	Check point	CH1 DC Trig Level	VR7	P15 (X73-1320)	CH2 DC Trig Level	VR19	P16 (X73-1320)	CH3 DC Trig Level	VR10	P17 (X73-1320)	CH4 DC Trig Level	VR20	P18 (X73-1320)		
Item of Adj.	Adj. Control	Check point																				
CH1 DC Trig Level	VR7	P15 (X73-1320)																				
CH2 DC Trig Level	VR19	P16 (X73-1320)																				
CH3 DC Trig Level	VR10	P17 (X73-1320)																				
CH4 DC Trig Level	VR20	P18 (X73-1320)																				
Adjustment of V. MODE Trig DC Level	VR22	X73-1320		V. MODE: CH1 CH1, AC-GND-DC: GND	(1) Operate CH1 \updownarrow POSITION to align the trace with horizontal center graticule line on the CRT screen. (2) Make adjustment so that the voltage in the conductor of the connector P19 is zero ($-0.008 \sim +0.008V$).																	
Adjustment of CH1 OUT Gain	VR8	X73-1320	475A 50 Ω Termination 50 Ω coaxial cable PG-506	H.DISPLAY: A V. MODE: CH1 TRIG MODE: AUTO CH1 AC-GND-DC: AC CH1 VOLTS/DIV: 5mV V. VAR: CAL	(1) Set the vertical axis sensitivity of oscilloscope (475A) to 50mV and AC-GND-DC to DC. (2) Connect the cable to CH1 OUT on the rear panel of CS-2070 and oscilloscope (475A) via the 50 Ω termination. (3) Apply a 1 kHz square wave signal to CH1 INPUT and adjust the oscillator output and \updownarrow POSITION so that the amplitude may be 2 div upward and downward from the horizontal center graticule line on the CRT screen. (4) Make adjustment so that the oscilloscope (475A) waveform becomes 4 div.																	
Adjustment of CH1 OUT DC Level	VR9	X73-1320	DL-720	H.DISPLAY: A V. MODE: CH1 CH1 AC-GND-DC: GND TRIG. MODE: AUTO	(1) Operate CH1 \updownarrow POSITION to align the trace with the horizontal center graticule line on the CRT screen. (2) Make adjustment so that the voltage in the connector P21 (X73-1320) becomes less than 0V ($\pm 10mV$).																	
Adjustment of Square wave Characteristics of CH1 5mV and 0.5V Ranges	TC3 TC1 TC10 TC11 TC1 TC9 TC7 TC23	X73-1330 X73-1320 X73-1320 X75-1120 X73-1330 X73-1320 X75-1120 X75-1120	PG-506 50 Ω 20dB Attenuator 50 Ω coaxial cable (BNC-BNC) 475A 50 Ω Termination	H. DISPLAY: A TRIG MODE: AUTO CH1, CH2 AC-GND-DC: DC CH1, CH2 VOLTS/DIV: 5mV ATRIG SOURCE: CH1 COUPLING: AC A TRIG SLOPE: + V VAR: CAL	(1) Set V. MODE to CH1 and repeatedly apply a 1 MHz squarewave signal to CH1 INPUT from the squarewave oscillator and adjust the oscillator output so that the amplitude becomes 6 div. In doing this, the input terminal must be terminated to match the output impedance of the oscillator, when the output impedance is 50 Ω termination. (2) Adjust TC3, TC1, TC10, TC11 and TC1 to shape the square wave on the CRT screen (CS-2070) as illustrated at right. At the same time, adjust TC9 to shape the square wave on the CRT screen of 475A. (3) Rotate VOLTS/DIV to 0.5V and adjust TC7 and TC23 so that the quality of square waveform becomes the best.		(1) Adjust A SWEEP TIME/DIV between 0.05 μs and 0.2 μs so that the waveform is visible. (2) As all measuring instruments are affected, repeat the adjustment individually.															


ADJUSTMENT

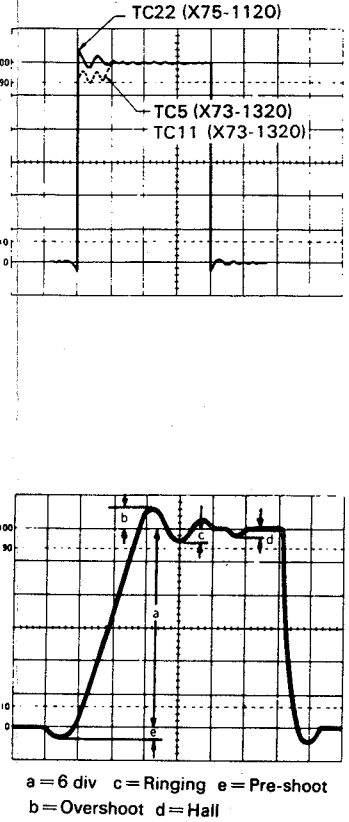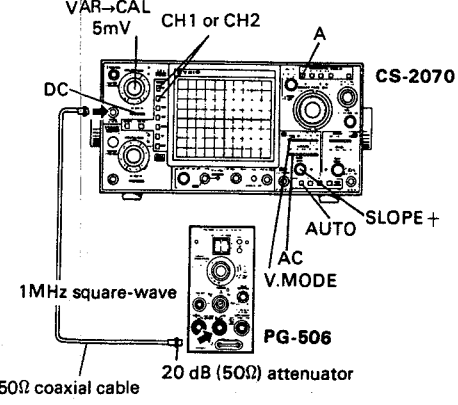Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Adjustment of Square wave Characteristics of CH2 5mV and 0.5V Ranges	TC5 TC22 TC11 TC18 TC24	X73-1320 X75-1120 X73-1320 X75-1120 X75-1120	PG-506 50Ω 20dB Attenuator 50Ω coaxial cable (BNC-BNC) 475A 50Ω Termination	A TRIG SOURCE: CH2	<p>(1) Set V. MODE to CH2 and make adjustment to obtain the same waveform as in the case of CH1.</p> <p>(2) Rotate the VOLTS/DIV to 0.5V and adjust TC18 and TC24 to obtain the square waveform as in the case of CH1.</p> <p>< Check ></p> <p>(1) With VOLTS/DIV remaining at 5mV, check the waveform quality when A. SWEEP TIME/DIV is changed by varying the squarewave frequency, from 100kHz to 10kHz, 1kHz and back to 100Hz sequentially.</p> <p style="border: 1px solid black; display: inline-block; padding: 2px;">Overshoot Less than 8%</p>		
Adjustment of Square wave Characteristics of CH1 X5 GAIN	TC2	X73-1320	PG-506 50Ω Termination 50Ω, 20dB Attenuator 50Ω coaxial cable (BNC-BNC)	H. DISPLAY: A TRIG MODE: AUTO CH1, CH2 AC-GND-DC: DC CH1, CH2 VOLTS/DIV: 5mV A TRIG SOURCE: CH1 COUPLING: AC A TRIG SLOPE: + V. VAR: CAL	<p>(1) With V. MODE being set to CH1, pull the PULL X5 GAIN and apply 1 MHz squarewave signal to CH1 INPUT to produce a waveform quality of 6 div on the CRT screen.</p> <p>(2) Make adjustment to improve the waveform quality</p> <p>< Check ></p> <p style="border: 1px solid black; display: inline-block; padding: 2px;">Overshoot less than 8%.</p>		<p>< Note ></p> <p>Terminate the input terminal of oscilloscope to match the output impedance of the oscillator.</p>
Adjustment of Square wave Characteristics of CH2 X5 GAIN	TC6	X73-1320		A TRIG SOURCE: CH2	<p>(1) With V. MODE set to CH2, apply 1 MHz square wave signal to CH2 INPUT and make the same adjustment as in the case of CH1.</p> <p>< Check ></p> <p style="border: 1px solid black; display: inline-block; padding: 2px;">Overshoot less than 8%.</p>		

ADJUSTMENT

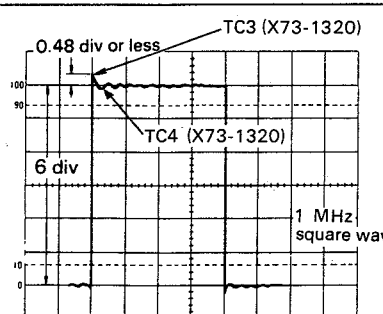Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark																																																																								
Adjustment of CH1 ATT CH2 ATT		X75-1120	4343B PG-506	H.DISPLAY: A CH1 AC-GND-DC: DC A TRIG SOURCE: V. MODE A SWEEP TIME/DIV: 0.2ms V.VAR: CAL	<p>(1) Shaping of waveform Apply 1 kHz squarewave signal to CH1 and CH2 INPUT and adjust the oscillator output to produce a waveform of 5~6 div. In doing this, make adjustment so that the waveform quality of each range is equal to that of the 5mV range.</p> <p>(2) Input capacity Connect a Q-meter (4343B) to CH1 and CH2 INPUT and make adjustment so that the input capacity of each range is equal to that of the 5mV range.</p> <p>CH1 Reference range: 5mV Range CH2 Reference range: 5mV Range</p> <table border="1" style="width: 100%; border-collapse: collapse; text-align: center;"> <thead> <tr> <th>Sequence</th> <th colspan="2">Adjustment</th> <th>Adj. control</th> <th>Sequence</th> <th colspan="2">Adjustment</th> <th>Adj. control</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>10mV range</td> <td>Wave Shape</td> <td>TC4</td> <td>1</td> <td>10mV range</td> <td>Wave Shape</td> <td>TC15</td> </tr> <tr> <td>2</td> <td>20mV range</td> <td>Wave Shape</td> <td>TC5</td> <td>2</td> <td>20mV range</td> <td>Wave Shape</td> <td>TC16</td> </tr> <tr> <td>3</td> <td>50mV range</td> <td>Wave Shape</td> <td>TC6</td> <td>3</td> <td>50mV range</td> <td>Wave Shape</td> <td>TC17</td> </tr> <tr> <td>4</td> <td>0.5V range</td> <td>Wave Shape</td> <td>TC10</td> <td>4</td> <td>0.5V range</td> <td>Wave Shape</td> <td>TC21</td> </tr> <tr> <td>5</td> <td>10mV range</td> <td>Input Capacity</td> <td>TC1</td> <td>5</td> <td>10mV range</td> <td>Input Capacity</td> <td>TC12</td> </tr> <tr> <td>6</td> <td>20mV range</td> <td>Input Capacity</td> <td>TC2</td> <td>6</td> <td>20mV range</td> <td>Input Capacity</td> <td>TC13</td> </tr> <tr> <td>7</td> <td>50mV range</td> <td>Input Capacity</td> <td>TC3</td> <td>7</td> <td>50mV range</td> <td>Input Capacity</td> <td>TC14</td> </tr> <tr> <td>8</td> <td>0.5V range</td> <td>Input Capacity</td> <td>TC8</td> <td>8</td> <td>0.5V range</td> <td>Input Capacity</td> <td>TC19</td> </tr> </tbody> </table>	Sequence	Adjustment		Adj. control	Sequence	Adjustment		Adj. control	1	10mV range	Wave Shape	TC4	1	10mV range	Wave Shape	TC15	2	20mV range	Wave Shape	TC5	2	20mV range	Wave Shape	TC16	3	50mV range	Wave Shape	TC6	3	50mV range	Wave Shape	TC17	4	0.5V range	Wave Shape	TC10	4	0.5V range	Wave Shape	TC21	5	10mV range	Input Capacity	TC1	5	10mV range	Input Capacity	TC12	6	20mV range	Input Capacity	TC2	6	20mV range	Input Capacity	TC13	7	50mV range	Input Capacity	TC3	7	50mV range	Input Capacity	TC14	8	0.5V range	Input Capacity	TC8	8	0.5V range	Input Capacity	TC19		<p>< Note ></p> <p>(1) Be sure to make the adjustment with the shield case being fitted in place.</p> <p>(2) If smearing or overshoot occurs to the square wave at 0.1V or 0.2V range, at 0.1V range, adjust TC1 (CH1) or TC12 (CH2) and at 0.2V range, TC2 (CH1) or TC13 (CH2).</p> <p>* Input capacity should be in the specification.</p>
Sequence	Adjustment		Adj. control	Sequence	Adjustment		Adj. control																																																																								
1	10mV range	Wave Shape	TC4	1	10mV range	Wave Shape	TC15																																																																								
2	20mV range	Wave Shape	TC5	2	20mV range	Wave Shape	TC16																																																																								
3	50mV range	Wave Shape	TC6	3	50mV range	Wave Shape	TC17																																																																								
4	0.5V range	Wave Shape	TC10	4	0.5V range	Wave Shape	TC21																																																																								
5	10mV range	Input Capacity	TC1	5	10mV range	Input Capacity	TC12																																																																								
6	20mV range	Input Capacity	TC2	6	20mV range	Input Capacity	TC13																																																																								
7	50mV range	Input Capacity	TC3	7	50mV range	Input Capacity	TC14																																																																								
8	0.5V range	Input Capacity	TC8	8	0.5V range	Input Capacity	TC19																																																																								
ADJUSTMENT OF A, B TRIG AMPLIFIERS																																																																															
Adjustment of CH3 Gain and CH4 Gain	VR11 VR21	X73-1320 X73-1320	PG506	H.DISPLAY: A V.MODE: QUAD. ALT A TRIG SOURCE: EXT CH3 B TRIG SOURCE: EXT CH4 A SWEEP TIME/DIV: 0.2ms TRIG MODE: AUTO CH1, CH2 AC-GND-DC: GND	<p>(1) Apply a 1 kHz squarewave signal simultaneously to CH3 and CH4 INPUT and adjust A TRIG LEVEL and B TRIG LEVEL to obtain synchronization. Operate CH3 and CH4 POSITION to bring the pattern to the center of the CRT screen.</p> <p>(2) Make adjustment so that the amplitude of CH3 and CH4 becomes 5 div., respectively.</p> <p>< Check > Sensitivity error must be within $\pm 3\%$. (See to Reference for the adjustment of CH1 Gain)</p> <table border="1" style="width: 100%; border-collapse: collapse; text-align: center;"> <tr> <td>Sensitivity error</td> <td>within $\pm 3\%$.</td> </tr> </table>	Sensitivity error	within $\pm 3\%$.		<p>< Note ></p> <p>If tilt or overshoot occurs to the 1 kHz waveform, refer to the section devoted to CH3 and CH4 waveform shaping.</p>																																																																						
Sensitivity error	within $\pm 3\%$.																																																																														
CH3 Waveform Shaping	TC4(Medium range) TC3(Ultra high range)	X73-1320 X73-1320	PG-506	H.DISPLAY: A V. MODE: QUAD. ALT A TRIG SOURCE: EXT CH3 A SWEEP TIME/DIV: 0.2ms TRIG MODE: AUTO CH1, CH2 AC-GND-DC: GND	<p>(1) Apply a 1 kHz square wave signal of fast rise time to CH3 INPUT and adjust the oscillator output to produce a waveform of 6 div on the CRT screen.</p> <p>(2) Produce a waveform of 6 div in the same manner and adjust TC3 to obtain the similar waveform as (1) above.</p> <p>(3) With A. SOURCE to EXT CH3 adjust the oscillator output and frequency to produce a square waveform of 1 MHz 6 div on the CRT screen and shape the waveform in the medium and ultra-high ranges.</p> <p>< Check > Overshoot less than 8%</p>		<p>< Note ></p> <p>(1) When shaping the waveform, terminate the input terminal of oscilloscope to match the output impedance of the oscillator</p> <p>(2) Before making 1 MHz waveshape, be sure to adjust input capacity EXT CH3 (TC1)</p>																																																																								



ADJUSTMENT

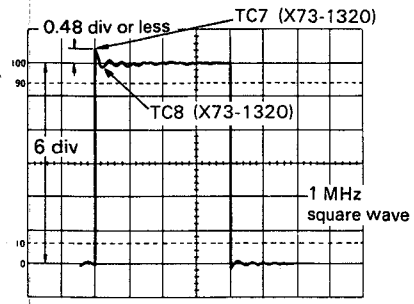Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
CH4 Wave form Shapping	TC8(Medium range) TC7(Ultra high range)	X73-1320 X73-1320	PG-506	H.DISPLAY: A V.MODE: QUAD.ALT A TRIG SOURCE: EXT CH3 B TRIG SOURCE: EXT CH4 A SWEEP TIME/DIV: 0.2ms B SWEEP TIME/DIV: 0.2ms	(1) Apply 1kHz and 1 MHz square wave signals of fast rise time to both CH3 and CH4 INPUT and take the same steps as in (1) above to shape the waveform. < Check > Overshoot less than 8%.		< Note > Before making 1 MHz wave shape, be sure to adjust input capacity EXT CH4 (TC4)
Adjustment of CH3 Input Capacity	TC1	X77-1130	4343B	A TRIG SOURCE: EXT CH3 B TRIG SOURCE: EXT CH4	Make adjustment so that the input capacity of CH3 becomes equal to the value of CH1 5mV range (28pF ± 2pF).		< Note > Be sure to make adjustment of input capacity after making 1 kHz square wave waveshape.
Adjustment of CH4 Input Capacity	TC4	X77-1130		Adjust the input capacity in the same manner as CH3. < Check > Check the input capacity in the same manner as CH3. Overshoot less than 8%.	< Note > Be sure to make adjustment of input capacity after making 1 kHz square wave waveshape.		
ADJUSTMENT OF VERTICAL AXIS (II)							
Check of 1 MHz Square wave Characteristics Square wave Characteristics of CH1 and CH2			PG-506 50Ω Termination	H.DISPLAY: A A. TRIG SOURCE: V.MODE A.SWEEP TIME/DIV: 0.2μs~ 0.05μs TRIG.MODE: AUTO A COUPLING: AC	(1) Check the squarewave characteristics of CH1 and CH2 5mV range. Turn the VOLTS/DIV knob for each channel to adjust the oscillator output so that CH1 and CH2 will produce a waveform of 6 div, respectively. (2) The overshoot must be less than 8% for each range.		< Note > As the VOLTS/DIV is manually rotated, the amplitude of 6 divs cannot be obtained amplitude.
Square wave Characteristics of CH3 and CH4				H. DISPLAY: ALT V.MODE: QUAD. ALT A.TRIG SOURCE: EXT CH3 B TRIG SOURCE: EXT CH4	Apply a 1 MHz squarewave signal to CH3 and CH4 INPUT and see if the overshoot is less than 8% at this time.		
Check of CH1 and CH2 Frequency Characteristics			SG-503 50Ω coaxial cable (BNC-BNC) 50Ω 20dB attenuator 50Ω Termination.	H. DISPLAY: A TRIG MODE: AUTO A. TRIG SOURCE: V. MODE A COUPLING: AC CH1, CH2 AC-GND-DC: DC A SWEEP TIME/DIV: 2μs~ 0.05μs	(1) With CH1 VOLTS/DIV set to 5 mV, apply a sine wave signal of 50kHz to INPUT and adjust the oscillator output to produce a waveform of 6 div on the CRT screen. (2) When the frequency is varied to 70 MHz with the oscillator output remaining unchanged, the amplitude on the screen must be over 4.25 div and there must be no sudden dips and peaks during attenuation. (3) Perform the same operations for CH2. Frequency characteristic 70MHz: less than -3 dB (4) When the specification are not satisfied, readjust the 1 MHz squarewave characteristics.		

ADJUSTMENT

Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Check of CH3 and CH4 Frequency Characteristics			SG-503 50Ω coaxial cable (BNC-BNC) 50Ω 20dB attenuator 50Ω Termination.	H. DISPLAY: ALT V.MODE: QUAD.ALT TRIG. MODE: AUTO A TRIG SOURCE: EXT CH3 B. TRIG SOURCE: EXT CH4	(1) Apply sine wave signals of 50 kHz to both CH3 and CH4 INPUT and adjust the oscillator output to produce a waveform of 6 div on the CRT screen. (2) When the frequency is changed to 70 MHz with the oscillator output remaining unchanged, the amplitude on the screen must be over 4.25 div. Frequency characteristic 70MHz : less than -3 dB (3) Perform the same operations for CH4. (4) When the specification are not satisfied, readjust the 1 MHz squarewave characteristics.		
Check of CH1 and CH2 X5 GAIN Frequency Characteristics			SG-503 50Ω Termination	H.DISPLAY: A A TRIG SOURCE: V. MODE TRIG.MODE: AUTO CH1, CH2 AC-GND-DC: DC CH1, CH2 VOLTS/DIV: 5mV CH1, CH2 X5 GAIN: PULL	(1) With V. MODE set to CH1, apply a sine wave signal of 50 kHz to CH1 INPUT and adjust the oscillator output to produce a waveform of 6 div on the CRT screen. (2) When the frequency is varied to 70MHz with the oscillator output remaining unchanged, the amplitude on the screen must be over 4.25 div. (3) Set V. MODE to CH2 and make a similar check. X5 GAIN frequency characteristic 70MHz: less than -3 dB.		
Check of 20MHz BW Frequency Characteristics			SG-503 50Ω Termination	H.DISPLAY: A V.MODE: CH1 A TRIG SOURCE: V.MODE CH1 AC-GND-DC: DC CH1 VOLTS/DIV: 5mV 20MHz BW: ON TRIG MODE: AUTO	(1) Apply a sine wave signal of 50kHz to CH1 INPUT to produce a waveform of 6 div. (2) Vary the frequency of the input signal without changing the oscillator output and read the frequency at which the amplitude on the screen becomes 4.25 div. This frequency must be within the specification limits. 20MHz BW Frequency characteristics Frequency of -3 dB: 16 MHz - 24 MHz.		
Adjustment of CH1 OUT Frequency Characteristics	TC9	X73-1320	475A 50Ω Termination (through type) 50Ω coaxial cord (BNC-BNC) SG-503	CH1 AC-GND-DC: AC CH1 VOLTS/DIV: 5mV CH1 POSITION: 12 o'clock	(1) With the vertical axis sensitivity of 475A set to 50mV, lead a 50Ω coaxial cable from CH1 OUT and terminate it with 50Ω termination and connect it to CH1 OUT of 475A. (2) Apply a sine wave signal of 50kHz to CH1 INPUT and adjust the oscillator output so that the vertical amplitude of 475A becomes 6 div. When the frequency is varied to 70 MHz without changing the oscillator output, adjust TC9 so that the amplitude on the CRT screen of 475A becomes over 4.25 div. CH1 OUT frequency characteristic 70MHz: less than -3 dB		<p>< Note > If the squarewave characteristics of CH1 PREAMP and V OUTPUT AMP are readjusted the squarewave characteristic and frequency characteristic will also change.</p>
Adjustment of CAL Output	VR1 VR2	X77-1130 X77-1130	475A FC-754A DL-720		(1) Short-circuit TP2 (X77 - 1130) and adjust VR1 so that the voltage at CAL output terminal becomes 0.3V ±1%. (2) Set the vertical axis sensitivity of 475A to 5mV and the sweep time to 0.2 ms. (3) Lead a probe from the calibration voltage output terminal (CAL) of CS-2070 and connect it to CH1 INPUT of 475A. (4) Adjust VR2 so that the frequency becomes 1 kHz. < Check > Check the duty ratio. Frequency: Within 1 kHz ±3%. Output voltage: Within 0.3 Vp-p ±1%. Duty ratio: Within (50 ±2)%		<p>< Note > For checking the frequency, a frequency counter (FC-754A) may be used.</p>



ADJUSTMENT

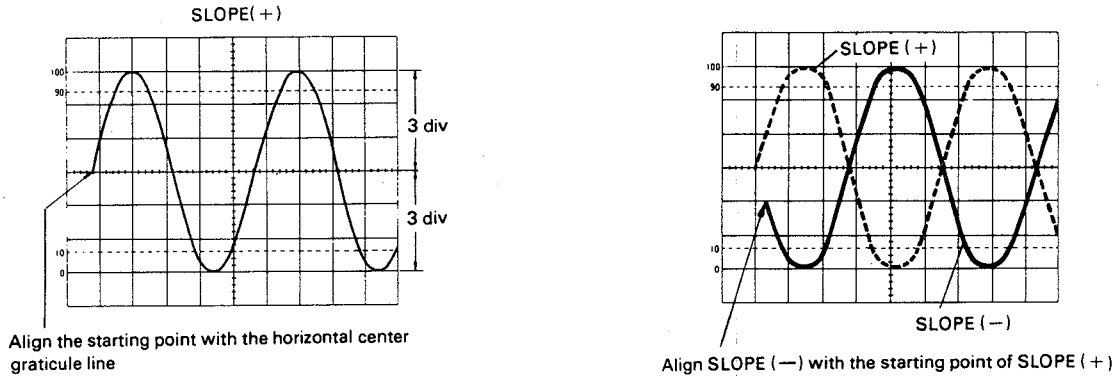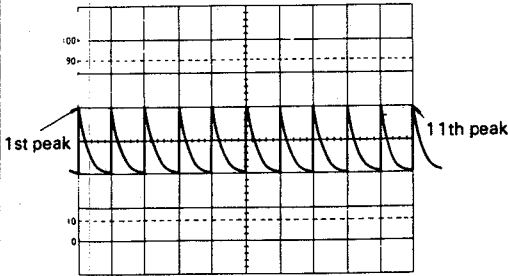Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
ADJUSTMENT OF HORIZONTAL SWEEP							
Coarse Adjustment of A and B Trigger Center and SLOPE (Coarse Adjustment of A Trigger Center and SLOPE)	VR2	X77-1110	SG-502	H.DISPLAY: A V.MODE: CH1 TRIG MODE: AUTO CH1 AC-GND-DC: AC	(1) Apply a sine wave signal of 1 kHz to CH1 INPUT and adjust the oscilloscope output and \updownarrow position to produce a waveform of amplitude 3 div above and below the horizontal center graticule line on the CRT screen. (2) Adjust VR2 so that the starting point of the waveform is aligned with the horizontal center graticule line on the CRT screen. (3) Set TRIG. SLOPE to (-) and adjust VR3 to bring the starting point to the position of the starting point of the waveform produced when TRIG. SLOPE is set to (+).	 <p style="text-align: center;">Align the starting point with the horizontal center graticule line</p> <p style="text-align: center;">Align SLOPE (-) with the starting point of SLOPE (+)</p>	
	VR3	X77-1110		A SWEEP TIME/DIV: 0.2ms A TRIG SOURCE: V. MODE A COUPLING: AC TRIG LEVEL: 12 o'clock TRIG SLOPE: +			
(Coarse Adjustment of B Trigger Center and SLOPE)	VR2	X77-1120	SG-502	H.DISPLAY: ALT V.MODE: CH1 A TRIG SOURCE: V. MODE B TRIG SOURCE: CH1 B TRIG LEVEL: 12 o'clock B TRIG SLOPE: +	(1) Set A. INTEN to Fully CCW. (2) Apply a sine wave signal of 1 kHz to CH1 INPUT and adjust the oscillator output and \updownarrow position to produce a waveform of amplitude 3 div above and below the horizontal center graticule line on the CRT screen. (3) Next, set TRIG. SLOPE to (-) and make adjustment to bring the starting point of the waveform to the position of the starting point of the waveform produce when TRIG. SLOPE is set to (+).		
	VR3	X77-1120		A SWEEP TIME/DIV: 0.5ms B SWEEP TIME/DIV: 0.2ms TRIG. MODE: AUTO \updownarrow TRACE SEP: NORM			
Adjustment of A Sweep Time	VR9	X74-1320	TG-501	H.DISPLAY: A V.MODE: CH1 A TRIG SOURCE: V. MODE A SWEEP TIME/DIV: 0.5ms TRIG MODE: AUTO A. VAR: CAL	(1) Apply a marker signal of 0.5 ms to CH1 INPUT. (2) Operate \blacktriangleleft POSITION to bring the first peak of the marker signal to the left end of the graticule line and adjust VR9 for the 11th peak to the right end of the graticule line.		< Note > When TG-501 is used, set CH1 AC-GND-DC to AC, VOLTS/DIV to 0.5V/div, thru 50 Ω termination.

ADJUSTMENT

Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Adjustment of B Sweep Time	VR10	X74-1320	TG-501	H.DISPLAY: ALT V.MODE: CH1 A. TRIG SOURCE: V. MODE B. TRIG SOURCE: CH1 A SWEEP TIME/DIV: 0.5ms B SWEEP TIME/DIV: 0.5ms TRIG.MODE: AUTO A,B TRIG.SLOPE: + A,B INTEN: Fully CW DELAY TIME MULTI: 0.20	<ol style="list-style-type: none"> Apply a marker signal of 0.5 ms to CH1 INPUT. On the screen A and B sweeps of CH1 input signal will appear. Operate \updownarrow TRACE SEP to bring these sweeps into the positions where they can be easily adjusted. Make adjustment so that the first peak of B sweep is brought to the left end of the graticule line on the screen and the 11th peak to the right end of graticule line on the screen. Make sure that A and B TRIG'D lamps are on. 		<p>< Note ></p> <ol style="list-style-type: none"> When TG-501 is used, the knobs must be operated in the same manner as described above. If the 11th peak is not visible, adjust VR7 (X74-1320) Sweep Length The B sweep time will not change even if A VAR is turned.
Adjustment of A Sweep Length	VR7	X74-1320		H. DISPLAY: A V. MODE: CH1 A TRIG SOURCE: V. MODE A SWEEP TIME/DIV: 0.5 ms TRIG MODE: AUTO	<ol style="list-style-type: none"> Apply a marker signal of 0.5 ms to CH1 INPUT. Make adjustment so that the total length is 11 div. 		<p>< Note ></p> <p>Turn \leftarrow POSITION to shift the base line two markers to the left then you can see the 12th time marker with the graticule area.</p>
Adjustment of B Sweep Length	VR8	X74-1320		H. DISPLAY: ALT V. MODE: CH1 A TRIG SOURCE: V. MODE B TRIG SOURCE: CH1 A SWEEP TIME/DIV: 0.5 ms B SWEEP TIME/DIV: 0.5ms TRIG MODE: AUTO A, B TRIG SLOPE: + A, B INTEN: Fully CW DELAY TIME MULTI: 0.20	<ol style="list-style-type: none"> Apply a marker signal of 0.5 ms to CH1 INPUT. A and B sweeps will appear on the screen. Use \updownarrow TRACE SEP to separate them. Make adjustment so that the total length of B sweep is 11 div. 		
Adjustment of A Sweep Position	VR12	X74-1320		H.DISPLAY: A V. MODE: CH1 A TRIG SOURCE: V. MODE A SWEEP TIME/DIV: 0.5 ms TRIG MODE: AUTO	<ol style="list-style-type: none"> Set CH1 AC-GND-DC to GND to bring the trace to the center of the CRT screen. Set the FINE knob of \leftarrow POSITION to 12 o'clock. Turn \updownarrow POSITION fully CW without turning the FINE knob and note the deviation between the starting point of the trace and the center of the screen. Next, turn \leftarrow POSITION fully CCW and measure the distance between the ending point of the trace and the center of the screen. Make adjustment so that these deviations will have the same width. <p style="border: 1px solid black; padding: 2px; display: inline-block;">Width error less than 1 div.</p>		


ADJUSTMENT

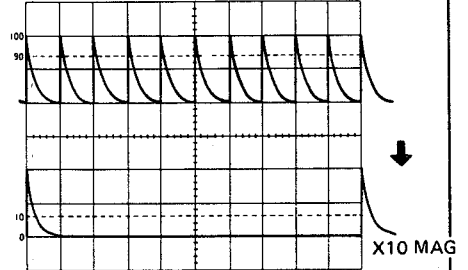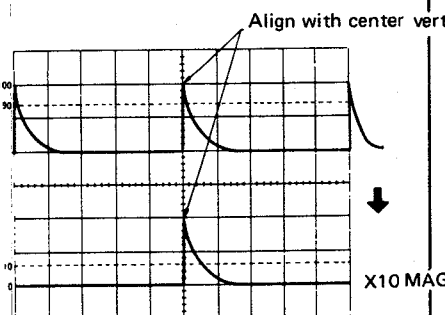Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Adjustment of B Sweep Position	VR11	X74-1320	TG-501	H.DISPLAY: ALT V.MODE: CH1 A TRIG SOURCE: V. MODE B TRIG SOURCE: CH1 A,B SWEEP TIME/DIV: 0.5ms TRIG MODE: AUTO A, B TRIG SLOPE: + A, B INTEN: Fully CW DELAY TIME MULTI: 0.20	(1) Apply a marker signal of 0.5 ms to CH1 INPUT and align the first peak of A sweep to the leftmost division of the CRT screen. (2) Operate ∇ TRACE SEP to separate A sweep and B sweep and set A. VAR to CAL. (3) Make adjustment so that the starting point of B sweep is aligned with that of A sweep in the horizontal position. < Check > Operate ∇ TRACE SEP so that A sweep and B sweep are superimposed on one another and make sure that their starting points coincide with each other.		
Adjustment of X10 MAG Gain	VR13	X74-1320	TG-501	H.DISPLAY: A V.MODE: CH1 A TRIG SOURCE: V.MODE A SWEEP TIME/DIV: 0.1ms TRIG MODE: AUTO CH1, VOLTS/DIV: 1V CH1, AC-GND-DC: DC	(1) Apply a marker signal of 0.1 ms to CH1 INPUT to produce a waveform of vertical amplitude of about 2 div. (2) Align the first peak of the marker signal with the left end of the graticule line on the CRT screen and the 11th peak with the right end and pull the X10 MAG switch. (3) Make adjustment so that the peak-to-peak distance is 10 div. < Check > Specification 10 times $\pm 5\%$		
Adjustment of X10 MAG Center	VR14	X74-1320		H. DISPLAY: A V. MODE: CH1 A TRIG SOURCE: V. MODE A SWEEP TIME/DIV: 0.1ms A. VAR: CAL TRIG. MODE: AUTO A. TRIG SLOPE: +	(1) Apply a marker signal of 0.5 ms to CH1 INPUT to produce 3 peaks waveform on the CRT screen. (2) Operate $\blacktriangleleft \blacktriangleright$ POSITION to bring the central peak to the vertical center graticule line on the screen. (3) Make adjustment so that the waveform will be aligned with the vertical center graticule line on the screen when the FINE knob is pulled out (X10 MAG position). < Check > Repeatedly push and pull the FINE knob to make sure that the center of the waveform does not move. Deviation less than 1 div.		
Adjustment of MAG Center and Gain					Recheck the center at $\times 10$ MAG and Gain.		
Adjustment of A Sweep Time 50 ms, 5 μ s and 0.1 μ s	VR2 (50 ms) VR1 (5 μ s) TC1 (0.1 μ s)	X74-1320	TG-501	H. DISPLAY: A V. MODE: CH1 A. TRIG SOURCE: V. MODE TRIG. MODE: AUTO A VAR: CAL	(1) With A. SWEEP TIME/DIV set to 50 ms, apply a marker signal of 50 ms to CH1 INPUT. (2) Adjust VR2 so that the first peak of the marker signal is aligned with the left end of the graticule on the screen and the 11th peak with the right end. (3) Next, Rotate the A SWEEP TIME/DIV to 5 μ s and apply a 5 μ s time marker to CH1 INPUT and adjust VR1 in the same manner as (2) (4) Next, A SWEEP TIME/DIV to 0.1 μ s and with 0.1 μ s time marker to CH1 INPUT, adjust TC1 in the same manner as (2)		






ADJUSTMENT

Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Adjustment of B Sweep Time 50 ms, 5 μ s and 0.1 μ s	VR4 (50 ms) VR3 (5 μ s) TC2 (0.1 μ s)	X74-1320		H.DISPLAY: ALT V.MODE: CH1 A TRIG SOURCE: V. MODE B TRIG SOURCE: CH1 TRIG MODE: AUTO A, B TRIG SLOPE: + A, B INTEN: Fully CW DELAY TIME MULTI: 1.00	<ol style="list-style-type: none"> Set A and B SWEEP TIME/DIV to 50 ms and apply a marker signal of 50 ms to CH1. Operate \downarrow TRACE SEP to separate A sweep and B sweep to be in the positions where adjustment can be made easily. Adjust VR4 so that the first peak of the marker signal is aligned with the left end of the graticule line on the screen and the 11th peak with the right end. Rotate A and B SWEEP TIME/DIV to 5 μs and apply a 5 μs time marker to CH1 INPUT and adjust VR3 in the same manner as (3) Next, A SWEEP TIME/DIV to 0.1 μs and with 0.1 μs time marker to CH1 INPUT, adjust TC2 in the same manner as (3). 		
Adjustment of 0.05 μ s A Sweep Linearity	TC3	X74-1320		H.DISPLAY: A V.MODE: CH1 A TRIG SOURCE: V MODE A SWEEP TIME/DIV: 0.05 μ s A. VAR: CAL TRIG. MODE: AUTO A. TRIG SLOPE: +	<ol style="list-style-type: none"> Apply a marker signal to CH1 INPUT. Make adjustment so that the total length of the waveform is 11 div. 		
Adjustment of 0.05 μ s B Sweep Linearity	TC4	X74-1320		H.DISPLAY: ALT V.MODE: CH1 A TRIG SOURCE: V. MODE B TRIG SOURCE: CH1 TRIG MODE: AUTO A, B TRIG SLOPE: + A, B INTEN: Fully CW DELAY TIME MULTI: 1.00	<ol style="list-style-type: none"> With A SWEEP TIME/DIV to 0.05 μs and B SWEEP TIME/DIV to 0.05 μs, apply a marker signal of 0.05 μs to CH1 INPUT. Operate \downarrow TRACE SEP to separate A sweep and B sweep into the positions where they can be easily adjusted. Make adjustment so that the total length of the waveform is 11 div. 		
Check of Sweep Time Error in All the Range [I] [II]				H.DISPLAY: A V. MODE: CH1 A TRIG SOURCE: V. MODE TRIG. MODE: AUTO A VAR: CAL	<ol style="list-style-type: none"> Apply a reference time marker signal for each range of A SWEEP TIME/DIV. Measure the time error rate and make sure it is within the specification limits. Specification Within $\pm 3\%$. 		
				H. DISPLAY: ALT V. MODE: CH1 A TRIG SOURCE: V. MODE B TRIG SOURCE: CH1 A. VAR: CAL TRIG. MODE: AUTO A, B TRIG SLOPE: + A, B INTEN: Fully CW DELAY TIME MULTI: 1.00	<ol style="list-style-type: none"> Operate \downarrow TRACE SEP to separate A sweep and B sweep into the positions where they can be easily adjusted. Apply a reference time marker signal in each of all the ranges (50 ms—0.05 μs) of B sweep. Measure the time error rate and make sure it is within the specification limits. Specification Within $\pm 3\%$. 		







ADJUSTMENT

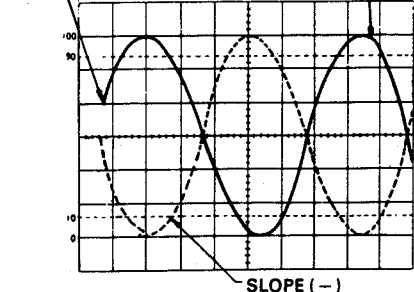Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
ADJUSTMENT OF X - Y OPERATION							
Adjustment of X Position Center	VR15	X74-1320		H.DISPLAY: A V. MODE: DUAL, ALT CH1, CH2 VOLTS/DIV: 5mV CH1, CH2 AC-GND-DC: GND A TRIG SOURCE: CH1 TRIG. MODE: AUTO A SWEEP TIME/DIV: 0.1ms	(1) Operate \updownarrow POSITION for both CH1 and CH2 to superimpose the two traces on one another in the center of the CRT screen. (2) Make adjustment so that the bright spot comes to the center of the screen when H. DISPLAY is switched in X-Y. < Check > Operate CH2 \updownarrow POSITION and make sure that the spot will move as described below. (1) When the knob is turned counterclockwise, the spot moves leftward more than 5 div. (2) When the knob is turned clockwise, the spot moves rightward more than 5 div.		< Note > When making X-Y adjustment, do not set both CH1 and CH2 to X5. GAIN.
Adjustment of X Gain	VR18	X73-1320	PG-506	H.DISPLAY: X-Y CH2 AC-GND-DC: AC CH2 VOLTS/DIV: 5mV	(1) Apply a square wave signal of 20 mVp-p 1 kHz to CH2 INPUT and make adjustment so that the horizontal amplitude is 4 div.		
Readjustment of X Position Center and X Gain					Readjust X position Center and X Gain.		
Check of X Axis Frequency Characteristic			SG-502	H. DISPLAY: X-Y CH2 AC-GND-DC: DC CH2 VOLTS/DIV: 5mV	(1) Apply a sine wave signal of 1 kHz to CH2 INPUT and adjust the oscillator output to produce a waveform of 10 div. (2) When the frequency is varied to 5 MHz without changing the oscillator output, the amplitude must be over 7.1 div (-3 dB).		
ADJUSTMENT OF TRIGGERING							
Adjustment of A Trig Slope	VR3	X77-1110	SG-502	H.DISPLAY: A V.MODE: CH1 A TRIG SOURCE: V. MODE A COUPLING: AC CH1, CH2 AC-GND-DC: AC CH1, CH2 VOLTS/DIV: 5mV A SWEEP TIME/DIV: 0.2ms A TRIG SLOPE: + TRIG MODE: AUTO	(1) Apply a sine wave signal of 1 kHz to CH1 INPUT and adjust the oscillator output to produce a waveform of 4~6 div on the CRT screen. (2) Operate A TRIG LEVEL and CH1 \updownarrow POSITION so that the waveform may have an amplitude equally above and below the horizontal center graticule line on the CRT screen. (3) Set A TRIG SLOPE to (-) and make adjustment so that the starting point of the waveform will be in the position of the starting point of the waveform when A TRIG SLOPE is in the (+) position. < Check > (1) Repeatedly turn the A TRIG SLOPE knob from (+) to (-) and make sure that the starting points are in the same positions. (2) Make sure that the rise slope of the waveform will be synchronized when the A TRIG SLOPE knob is in the (+) position and the fall slope will be synchronized when the knob is in the (-) position. (3) Feed the same signal to CH2 and set V MODE to CH2 to produce a waveform of CH2 and make sure that the rise slope of the waveform is synchronized when the A TRIG SLOPE knob is at (+) and the fall slope is synchronized when it is at (-) position.	Align SLOPE (+) with the horizontal center graticule line SLOPE (+) 	

ADJUSTMENT

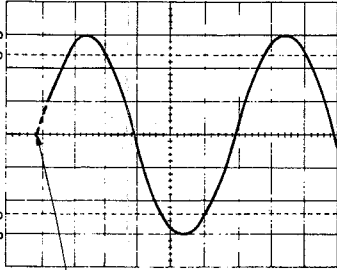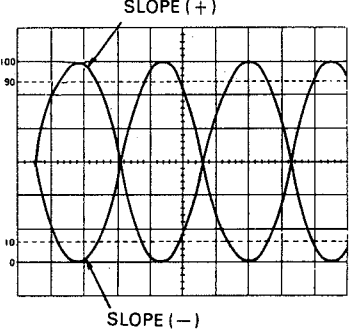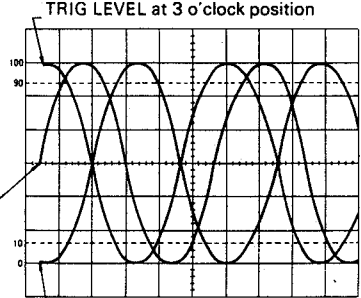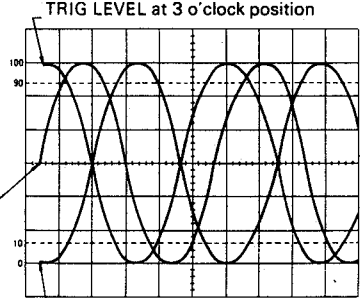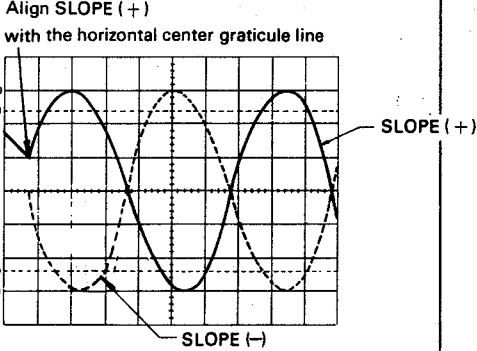Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Adjustment A Trig Level Center	VR2	X77-1110	SG-502	H.DISPLAY: A V.MODE: CH1 A TRIG SOURCE: V. MODE A. COUPLING: AC CH1, CH2 AC-GND-DC: AC CH1, CH2 VOLTS/DIV: 5mV A SWEEP TIME/DIV: 0.2ms A TRIG SLOPE: + TRIG MODE: AUTO	<ol style="list-style-type: none"> (1) Set A TRIG LEVEL to 12 o'clock. (2) Apply a sine wave signal of 1 kHz to CH1 INPUT and adjust the oscillator output to produce a waveform of 4~6 div on the CRT screen. (3) Operate CH1 \blacktriangledown POSITION to move the waveform so that its amplitude is equally above and below the horizontal center graticule line on the CRT screen. (4) Make adjustment so that the starting point of the waveform is on the horizontal center graticule line on the CRT screen. <p>< Check ></p> <ol style="list-style-type: none"> (1) When A TRIG SLOPE is alternately turned to (+) and (-), the starting point must be always on the horizontal center graticule line. (2) With A TRIG SLOPE remaining in the position of (+), turn TRIG LEVEL clockwise toward 3 o'clock from near 9 o'clock and see if the waveform is as shown at right. (3) Adjust the oscillator output so that the waveform amplitude becomes 0.5 div and make sure that synchronization can be obtained by A TRIG LEVEL. <div style="display: flex; justify-content: space-around; align-items: flex-end;"> <div style="text-align: center;">  <p>Align the starting point with the horizontal center graticule line</p> </div> <div style="text-align: center;">  <p>SLOPE (+) SLOPE (-)</p> </div> <div style="text-align: center;">  <p>TRIG LEVEL at 3 o'clock position TRIG LEVEL at 9 o'clock position TRIG LEVEL at 12 o'clock position</p> </div> </div>	 <p>TRIG LEVEL at 3 o'clock position TRIG LEVEL at 9 o'clock position TRIG LEVEL at 12 o'clock position</p>	
Adjustment of B Trig Slope	VR3	X77-1120	SG-502	H.DISPLAY: ALT V.MODE: CH1 A TRIG SOURCE: V. MODE B TRIG SOURCE: CH1 A COUPLING: AC CH1, CH2 AC-GND-DC: AC CH1, CH2 VOLTS/DIV: 5mV A, B SWEEP TIME/DIV: 0.2ms A. VAR: CAL A, B TRIG.SLOPE: + TRIG MODE: AUTO A, B INTEN: Fully CW	<ol style="list-style-type: none"> (1) Apply a sine wave signal of 1 kHz to CH1 INPUT and adjust the oscillator output to produce a waveform of 4~6 div on the CRT screen. (2) Operate A TRIG LEVEL, B TRIG LEVEL and CH1 \blacktriangledown POSITION to move waveform so that its amplitude is equally above and below the horizontal center graticule line on the screen. (3) Set A INTEN to CCW and B INTEN to an arbitrary position near 3 o'clock. (4) Set B TRIG SLOPE to (-) and make adjustment so that the starting point of the waveform comes to the same position of the starting point of waveform when B TRIG SLOPE is in the (-) position. <p>< Check ></p> <ol style="list-style-type: none"> (1) Turn B TRIG SLOPE knob alternately to (+) and (-) and make sure that the starting point is always on the horizontal center graticule line. (2) When B TRIG SLOPE is in the (+) position, the rise slope of the waveform should be synchronized and its fall slope be synchronized at (-). (3) Apply the same signal to CH2 and set V. MODE to CH2 to produce a waveform of B sweep of CH2 on the screen to make sure that the rise slope of the waveform is synchronized when B TRIG SLOPE is at (+) and the fall slope is synchronized at (-). 	 <p>Align SLOPE (+) with the horizontal center graticule line SLOPE (+) SLOPE (-)</p>	

ADJUSTMENT

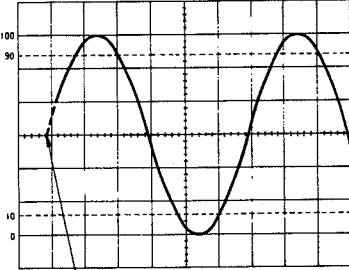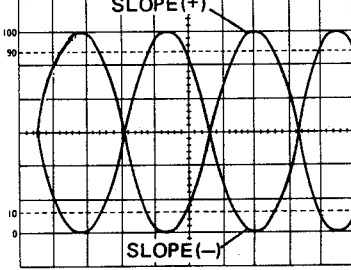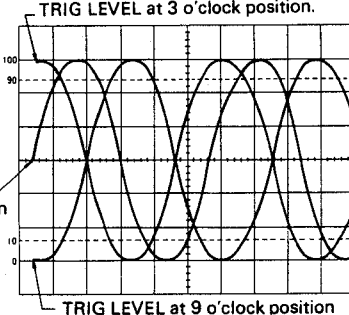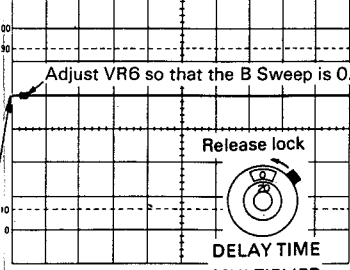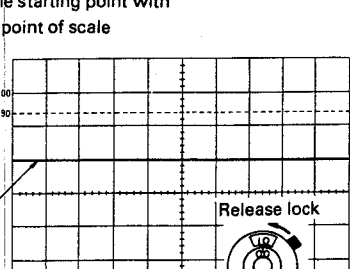Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
Adjustment of B Trig Level Center	VR2	X77-1120	SG-502	H.DISPLAY: ALT V. MODE: CH1 A COUPLING: AC CH1, CH2 AC-GND-DC: AC CH1, CH2 VOLTS/DIV: 5mV A, B SWEEP TIME/DIV: 0.2ms A. VAR: CAL B. TRIG SOURCE: CH1	<ol style="list-style-type: none"> (1) Turn B TRIG LEVEL knob to 12 o'clock. (2) Apply a sine wave signal of 1 kHz to CH1 INPUT and adjust the oscillator output to produce a waveform of 4~6 div on the CRT screen. (3) Operate CH1 \blacktriangle POSITION so that the waveform has an amplitude equally above and below the horizontal center graticule line on the screen. (4) Turn A INTEN to CCW and B INTEN to a position near 3 o'clock and make adjustment so that the starting point of the waveform is on the horizontal center graticule line. <p>< Check ></p> <ol style="list-style-type: none"> (1) Turn B TRIG SLOPE alternately to (+) and (-) and make sure that the starting point of the waveform is always on the horizontal center graticule line. (2) With B TRIG SLOPE knob remaining in the (+) position, turn TRIG LEVEL knob clockwise toward 3 o'clock from near 9 o'clock and see if the waveform appear as shown at right. (3) Adjust the oscillator output so that the waveform amplitude becomes 0.5 div and make sure that synchronization is obtained at this time by operating B TRIG LEVEL. <div style="display: flex; justify-content: space-around; align-items: flex-end;"> <div style="text-align: center;">  <p>Align the starting point with horizontal center graticule line</p> </div> <div style="text-align: center;">  </div> <div style="text-align: center;">  </div> </div>		
Adjustment of DELAY TIME MULTIPLIER	VR6 VR5	X74-1320 X74-1320		H. DISPLAY: ALT V. MODE: CH1 CH1 AC-GND-DC: GND TRIG MODE: AUTO A SWEEP TIME/DIV: 0.1ms B SWEEP TIME/DIV: 1 μ s \blacktriangle TRACE SEP: NORM B SOURCE : START AFTER DELAY	<ol style="list-style-type: none"> (1) Set DELAY TIME MULTIPLIER to 0.20. (2) Operate A INTEN and B INTEN properly to make B trace brighter and A trace light dimmer. (3) Operate \blacktriangle POSITION to bring the starting point of A trace to the left end of the graticule line on the CRT screen. (4) Make adjustment so that B trace may appear as shown at right. (5) Next, set DELAY TIME MULTIPLIER to 10:00. Make adjustment so that B trace may appear as shown at right. (6) Repeat (1) thru (5) 2 or 3 times. <p>< Check ></p> Set DELAY TIME MULTIPLIER to 5.00 and make sure that the starting point of B trace is in a position within 5 div \pm 0.2 div from the left end of the screen.	<div style="text-align: center;">  <p>Adjust VR6 so that the B Sweep is 0.2 div. A Sweep</p> </div> <div style="text-align: center;">  <p>Align the starting point with the left point of scale</p> </div> <div style="text-align: center;">  <p>Align the starting point with the vertical graticule line (VR5) B Sweep</p> </div>	



ADJUSTMENT

Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark
OPERATING CHECKS							
Check of Triggering Sensitivity			SG-502 SG-503 475A	V.MODE: CH1 CH1 VOLTS/DIV: 5mV A,B SWEEP TIME/DIV: arbitrary position CH1 AC-GND-DC: AC TRIG MODE: NORM	<p>(1) Make measurements of triggering sensitivity according to the table given below. (For both A and B sweeps)</p> <p>[I] A Sweep, INT</p> <p>(1) Set H DISPLAY to A and A TRIG SOURCE to CH1.</p> <p>(2) Apply a sine wave signal to CH1 INPUT, vary the oscillator output and operate A TRIG LEVEL to measure the minimum synchronizing amplitude on the CRT screen. When doing this, make sure that the A TRIG' D lamp is on.</p> <p>Check synchronization by each check frequency.</p> <p>[II] B Sweep, INT</p> <p>(1) Set H DISPLAY to B DLY'D, A TRIG SOURCE to CH1 and B TRIG SOURCE to CH1.</p> <p>(2) Apply a sine wave to CH1 INPUT, vary the oscillator output and operate B TRIG LEVEL to measure the minimum synchronizing amplitude. When doing this, make sure that the A TRIG'D and B TRIG'D lamps are on.</p> <p>Check synchronization by each frequency.</p> <p>[III] A Sweep, EXT</p> <p>(1) Set H DISPLAY to A and A TRIG SOURCE to EXT CH3.</p> <p>(2) Apply a signal of the same voltage simultaneously to CH1 and CH4 INPUT.</p> <p>(3) Operate CH1 VOLTS/DIV to produce a waveform of 6 div on the CRT screen.</p> <p>(4) Vary the oscillator output and operate A TRIG LEVEL to measure the minimum synchronizing amplitude by the oscilloscope (475A).</p> <p>Check synchronization by each check frequency.</p> <p>When doing this, make sure that A TRIG'D lamp is on.</p> <p>[IV] B Sweep, EXT</p> <p>(1) Set H DISPLAY to ALT, A TRIG SOURCE to CH1 and B TRIG SOURCE to EXT CH4.</p> <p>(2) Apply a signal of the same voltage simultaneously to CH1 and CH4 INPUT.</p> <p>(3) Operate CH1 VOLTS/DIV to produce a waveform of 6 div on the CRT screen.</p> <p>(4) Operate B TRIG LEVEL and A TRIG LEVEL to synchronize both A sweep and B sweep.</p> <p>(5) Vary the oscillator output and operate B TRIG LEVEL and measure the minimum synchronizing amplitude by the oscilloscope (475A). Check synchronization by each check frequency.</p> <p>(6) Make sure that the B TRIG'D lamp is on.</p>		




ADJUSTMENT

Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark																																														
					<p>[V] Check of triggering sensitivity</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th rowspan="2">COUPLING (TRIG. SOURCE)</th> <th rowspan="2">FREQ RANGE (Hz)</th> <th colspan="2">Trig. sensitivity (Min. sync amplitude)</th> </tr> <tr> <th>TRIG. SOURCE V.MODE (CH1 or CH2)</th> <th>TRIG SOURCE EXT CH3 or CH4</th> </tr> </thead> <tbody> <tr> <td>AC</td> <td>20Hz ~ 20MHz ~ 70MHz</td> <td>0.5div 1.5div</td> <td>50mVp-p 150mVp-p</td> </tr> <tr> <td>DC</td> <td>DC ~ 20MHz ~ 70MHz</td> <td>0.5div 1.5div</td> <td>50mVp-p 150mVp-p</td> </tr> <tr> <td>AC HF_{REJ}</td> <td>1kHz 1MHz</td> <td>0.5div Not to be synchronized at 1 div</td> <td>50mVp-p Not to be synchronized at 100mVp-p</td> </tr> <tr> <td>AC LF_{REJ}</td> <td>1MHz 1kHz</td> <td>0.5div Not to be synchronized at 1 div</td> <td>50mVp-p Not to be synchronized at 100mVp-p</td> </tr> <tr> <td>VIDEO</td> <td>VIDEO signal FRAME LINE</td> <td>0.5div</td> <td>50mVp-p</td> </tr> </tbody> </table> <p>[VI] Check of triggering sensitivity by TRIG. MODE H.DISPLAY : A, A SOURCE : AC</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th rowspan="2">COUPLING (TRIG. SOURCE)</th> <th rowspan="2">FREQ RANGE (Hz)</th> <th colspan="2">Trig. sensitivity (Min. sync amplitude)</th> </tr> <tr> <th>TRIG SOURCE V.MODE (CH1 or CH2)</th> <th>TRIG. SOURCE EXT</th> </tr> </thead> <tbody> <tr> <td>AUTO</td> <td>30Hz ~ 20MHz ~ 70MHz</td> <td>0.5div 1.5div</td> <td>50mVp-p 150mVp-p</td> </tr> </tbody> </table> <p>[VII] Check of trig source (A sweep) ① TRIG MODE: AUTO, H.DISPLAY: A ② Applied different signals to CH1 ~ CH4 and operate A SOURCE as described below and make sure to operate as follow.</p> <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 15%;">A SOURCE</th> <th style="width: 85%;">Operation</th> </tr> </thead> <tbody> <tr> <td>V.MODE</td> <td> V.MODE→CH1 The signal of CH1 is synchronized with A sweep V.MODE→CH2 The signal of CH2 is synchronized with A sweep V.MODE→DUAL, ALT When the signals of CH1 and CH2 are superimposed on one another they are synchronized with the A sweep of CH1 and CH2, respectively, but there will be no synchronization when there is no signal V.MODE→DUAL, CHOP No Sync. V.MODE→ADD Synchronized with the signal of CH2 when CH1 + CH2 (CH1 - CH2 at CH2 INV) V.MODE→QUAD, ALT When the signals of CH1 ~ CH4 are superimposed on one another on the CRT screen, the signals will be synchronized with the A sweep of CH1 ~ CH4 respectively but there will be no sync when there is no signal. V.MODE→QUAD, CHOP No Sync. </td> </tr> <tr> <td>CH1</td> <td>The signal of CH1 is synchronized with A sweep</td> </tr> <tr> <td>CH2</td> <td>The signal of CH2 is synchronized with A sweep</td> </tr> <tr> <td>EXT CH3</td> <td>The signal of CH3 is synchronized with A sweep</td> </tr> </tbody> </table> <p>③ Check sync by the lighting of A TRIG'D lamp</p>	COUPLING (TRIG. SOURCE)	FREQ RANGE (Hz)	Trig. sensitivity (Min. sync amplitude)		TRIG. SOURCE V.MODE (CH1 or CH2)	TRIG SOURCE EXT CH3 or CH4	AC	20Hz ~ 20MHz ~ 70MHz	0.5div 1.5div	50mVp-p 150mVp-p	DC	DC ~ 20MHz ~ 70MHz	0.5div 1.5div	50mVp-p 150mVp-p	AC HF _{REJ}	1kHz 1MHz	0.5div Not to be synchronized at 1 div	50mVp-p Not to be synchronized at 100mVp-p	AC LF _{REJ}	1MHz 1kHz	0.5div Not to be synchronized at 1 div	50mVp-p Not to be synchronized at 100mVp-p	VIDEO	VIDEO signal FRAME LINE	0.5div	50mVp-p	COUPLING (TRIG. SOURCE)	FREQ RANGE (Hz)	Trig. sensitivity (Min. sync amplitude)		TRIG SOURCE V.MODE (CH1 or CH2)	TRIG. SOURCE EXT	AUTO	30Hz ~ 20MHz ~ 70MHz	0.5div 1.5div	50mVp-p 150mVp-p	A SOURCE	Operation	V.MODE	V.MODE→CH1 The signal of CH1 is synchronized with A sweep V.MODE→CH2 The signal of CH2 is synchronized with A sweep V.MODE→DUAL, ALT When the signals of CH1 and CH2 are superimposed on one another they are synchronized with the A sweep of CH1 and CH2, respectively, but there will be no synchronization when there is no signal V.MODE→DUAL, CHOP No Sync. V.MODE→ADD Synchronized with the signal of CH2 when CH1 + CH2 (CH1 - CH2 at CH2 INV) V.MODE→QUAD, ALT When the signals of CH1 ~ CH4 are superimposed on one another on the CRT screen, the signals will be synchronized with the A sweep of CH1 ~ CH4 respectively but there will be no sync when there is no signal. V.MODE→QUAD, CHOP No Sync.	CH1	The signal of CH1 is synchronized with A sweep	CH2	The signal of CH2 is synchronized with A sweep	EXT CH3	The signal of CH3 is synchronized with A sweep		
COUPLING (TRIG. SOURCE)	FREQ RANGE (Hz)	Trig. sensitivity (Min. sync amplitude)																																																			
		TRIG. SOURCE V.MODE (CH1 or CH2)	TRIG SOURCE EXT CH3 or CH4																																																		
AC	20Hz ~ 20MHz ~ 70MHz	0.5div 1.5div	50mVp-p 150mVp-p																																																		
DC	DC ~ 20MHz ~ 70MHz	0.5div 1.5div	50mVp-p 150mVp-p																																																		
AC HF _{REJ}	1kHz 1MHz	0.5div Not to be synchronized at 1 div	50mVp-p Not to be synchronized at 100mVp-p																																																		
AC LF _{REJ}	1MHz 1kHz	0.5div Not to be synchronized at 1 div	50mVp-p Not to be synchronized at 100mVp-p																																																		
VIDEO	VIDEO signal FRAME LINE	0.5div	50mVp-p																																																		
COUPLING (TRIG. SOURCE)	FREQ RANGE (Hz)	Trig. sensitivity (Min. sync amplitude)																																																			
		TRIG SOURCE V.MODE (CH1 or CH2)	TRIG. SOURCE EXT																																																		
AUTO	30Hz ~ 20MHz ~ 70MHz	0.5div 1.5div	50mVp-p 150mVp-p																																																		
A SOURCE	Operation																																																				
V.MODE	V.MODE→CH1 The signal of CH1 is synchronized with A sweep V.MODE→CH2 The signal of CH2 is synchronized with A sweep V.MODE→DUAL, ALT When the signals of CH1 and CH2 are superimposed on one another they are synchronized with the A sweep of CH1 and CH2, respectively, but there will be no synchronization when there is no signal V.MODE→DUAL, CHOP No Sync. V.MODE→ADD Synchronized with the signal of CH2 when CH1 + CH2 (CH1 - CH2 at CH2 INV) V.MODE→QUAD, ALT When the signals of CH1 ~ CH4 are superimposed on one another on the CRT screen, the signals will be synchronized with the A sweep of CH1 ~ CH4 respectively but there will be no sync when there is no signal. V.MODE→QUAD, CHOP No Sync.																																																				
CH1	The signal of CH1 is synchronized with A sweep																																																				
CH2	The signal of CH2 is synchronized with A sweep																																																				
EXT CH3	The signal of CH3 is synchronized with A sweep																																																				

ADJUSTMENT

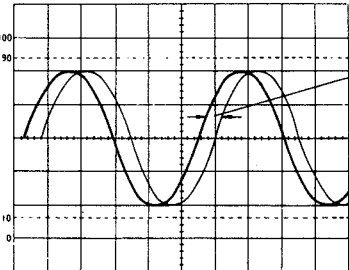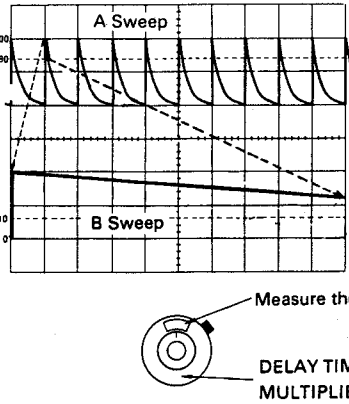
Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark								
					<p>[VIII] Check of trig source (B sweep)</p> <p>(1) Set H DISPLAY to A, TRIG MODE to AUTO, V MODE to DUAL, ALT and A TRIG SOURCE to V MODE.</p> <p>(2) Apply different signals to CH1, CH2 and CH4 and superimpose the signals of CH1 and CH2 on one another on the CRT screen and synchronize them by A TRIG LEVEL.</p> <p>(3) Set H DISPLAY to B DLY'D and operate B SOURCE as described below to check the synchronization.</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <thead> <tr> <th>B TRIG SOURCE</th> <th>Operation</th> </tr> </thead> <tbody> <tr> <td>CH1</td> <td>The signal of CH1 is synchronized with B sweep.</td> </tr> <tr> <td>CH2</td> <td>The signal of CH2 is synchronized with B sweep.</td> </tr> <tr> <td>EXT CH4</td> <td>The signal of CH4 is synchronized with B sweep.</td> </tr> </tbody> </table> <p>(4) Make sure that the B TRIG'D lamp is on.</p>	B TRIG SOURCE	Operation	CH1	The signal of CH1 is synchronized with B sweep.	CH2	The signal of CH2 is synchronized with B sweep.	EXT CH4	The signal of CH4 is synchronized with B sweep.		
B TRIG SOURCE	Operation														
CH1	The signal of CH1 is synchronized with B sweep.														
CH2	The signal of CH2 is synchronized with B sweep.														
EXT CH4	The signal of CH4 is synchronized with B sweep.														
Check of Jitter			SG503	<p>H.DISPLAY: A A.TRIG SOURCE: CH1 TRIG MODE: NORM A COUPLING: AC A SWEEP TIME/DIV: 0.05μs CH1 VOLTS/DIV: 0.1V CH1 AC-GND-DC: AC X10 MAG: PULL HOLD OFF: NORM</p>	<p>(1) Apply a sine wave signal of 70 MHz to CH1 INPUT and adjust the oscillator output to produce a waveform of 4 div on the CRT screen.</p> <p>(2) Operate A TRIG LEVEL to find a point where the jitter is minimized.</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td>Jitter</td> <td>Less than 0.2 div</td> </tr> </table>	Jitter	Less than 0.2 div								
Jitter	Less than 0.2 div														
Operational Check of DELAY TIME MULTIPLIER			TG-501	<p>H.DISPLAY: ALT A, B TRIG SOURCE: CH1 TRIG MODE: AUTO V. MODE: CH1 B SOURCE: STARTS AFTER DELAY CH1 AC-GND-DC: AC A SWEEP TIME/DIV: 1ms B SWEEP TIME/DIV: 5μs</p>	<p>(1) Apply a marker signal of 1 ms to CH1 INPUT produce a waveform of 2~3 div on the CRT screen.</p> <p>(2) Operate \updownarrow TRACE SEP to separate B sweep and A sweep.</p> <p>(3) Operate $\leftarrow \rightarrow$ POSITION to align the first peak of the waveform with the left end of the screen.</p> <p>(4) Adjust A INTEN and B INTEN to bring the waveform into the positions where they can be easily visible.</p> <p>(5) Operate DELAY TIME MULTIPLIER so that the patterns of the screen appear as shown at right (the second peak of the A sweep should be intensity modulated and should be aligned with the left end of B sweep scale) and note the dial reading at this time.</p>		<p>< Note > When TG-501 is used, CH1 VOLTS/DIV should be set to 0.5V thru 50Ω termination.</p>								

ADJUSTMENT

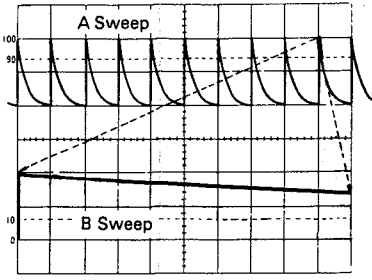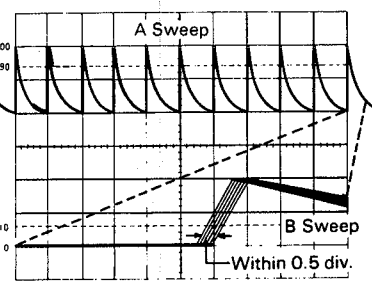
Item	Adjustment Control	P.C.B No.	Test Equipment	Control Setting	Adjustment and Check	Illustration	Remark		
					<p>(6) Turn DELAY TIME MULTIPLIER and operate \leftrightarrow POSITION so that what is shown at right will happen at the 10th peak and note the dial reading at this time.</p> <p>(7) Make the following calculation from the dial reading to make sure that the error is within the specification limits. $(B) - (A) = 8.00 \pm 0.2$</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td>Time multiplication error</td> <td>within $\pm 2\%$</td> </tr> </table>	Time multiplication error	within $\pm 2\%$	 <p style="text-align: center;">Measure the dial reading</p> 	
Time multiplication error	within $\pm 2\%$								
Check of DELAY TIME Jitter			TG-501	<p>H.DISPLAY: ALT A TRIG SOURCE: CH1 B TRIG SOURCE: CH2 TRIG MODE: AUTO V. MODE: CH1 B SOURCE: STARTS AFTER DELAY B ENDS A: ON CH1 AC-GND-DC: AC A SWEEP TIME/DIV: 1ms B SWEEP TIME/DIV: 1μs</p>	<p>(1) Apply a marker signal of 1 ms to CH1 INPUT to produce a waveform of 2~3 div on the CRT screen</p> <p>(2) Operate \updownarrow TRACE SEP to separate A sweep and B sweep.</p> <p>(3) Operate DELAY TIME MULTIPLIER to obtain the patterns as shown at right. (DELAY TIME MULTIPLIER is to be set to about 1.00).</p> <p>(4) Make sure that the jitter of B sweep is less than 0.5 div at this time.</p> <table border="1" style="margin-left: auto; margin-right: auto;"> <tr> <td>Specification</td> <td>Less than 1/20,000</td> </tr> </table>	Specification	Less than 1/20,000		
Specification	Less than 1/20,000								

ADJUSTMENT


X73-1320-01

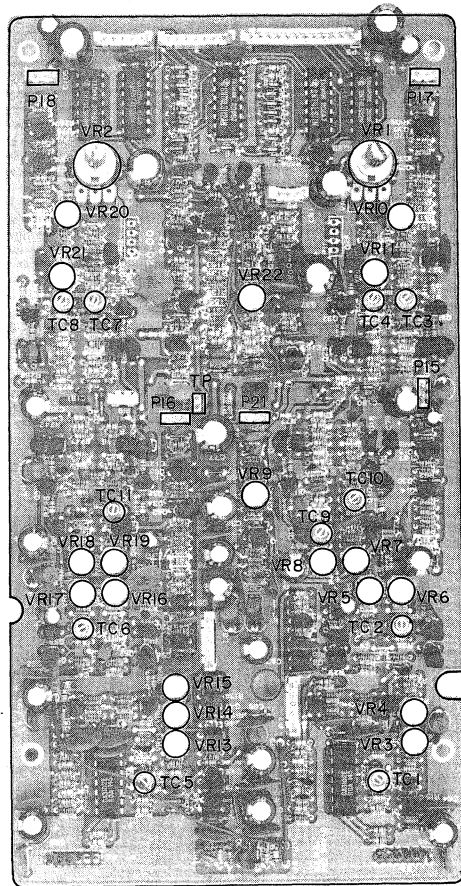


X74-1320-01

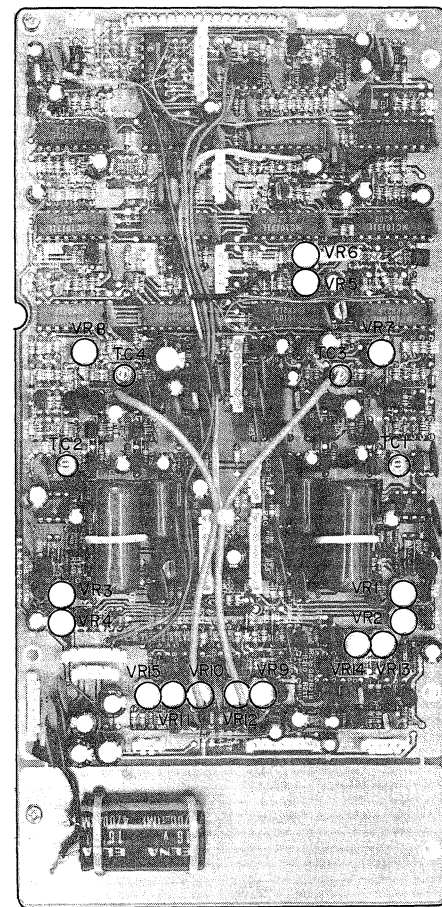


X75-1120-01

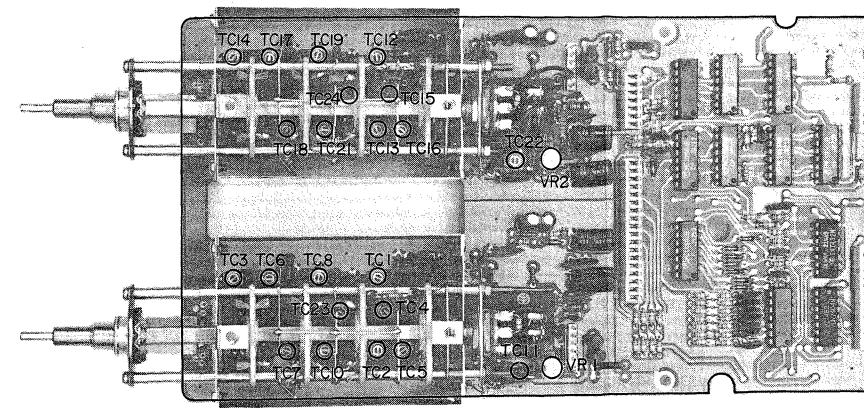


X77-1130-01

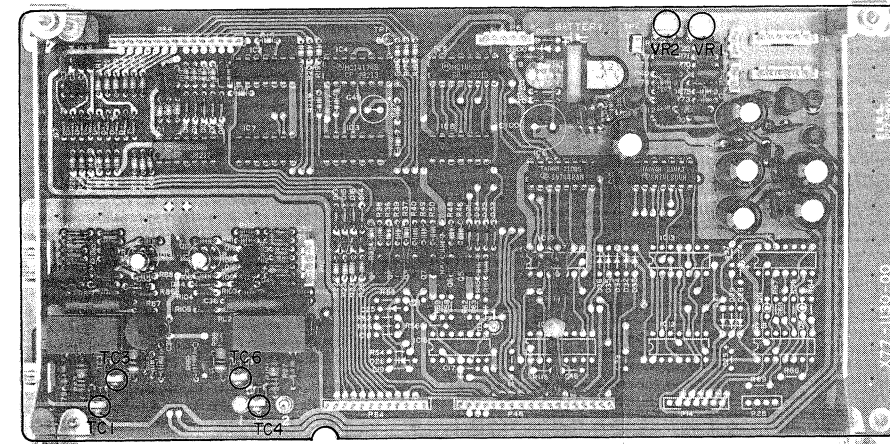


X73-1330-01

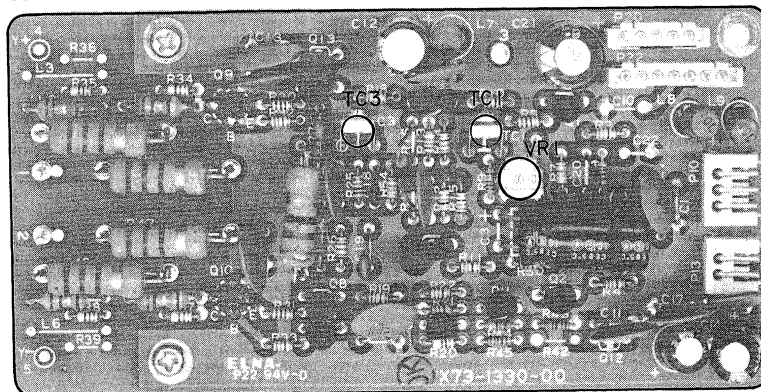


X77-1110-01

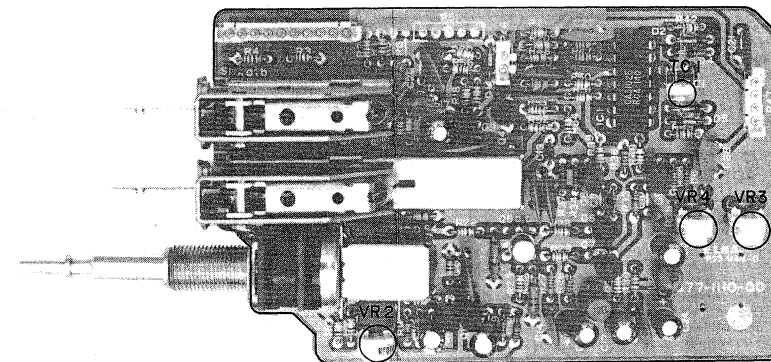




X68-1310-01

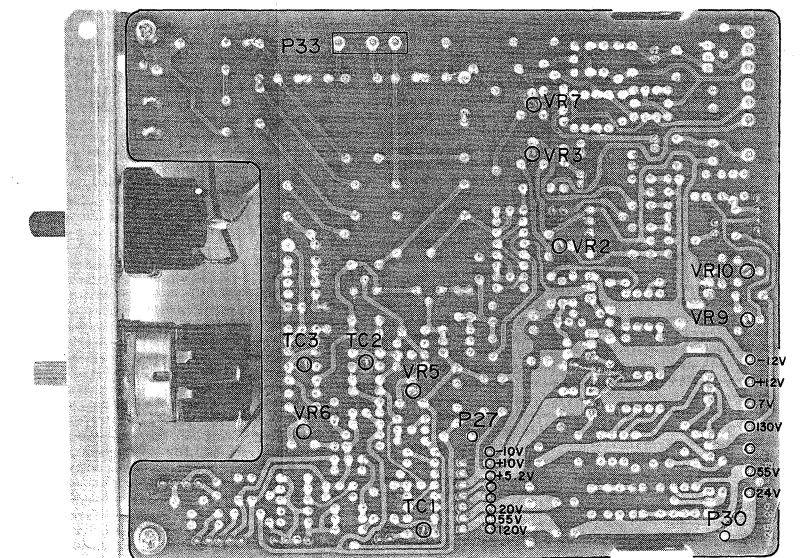

X77-1120-01



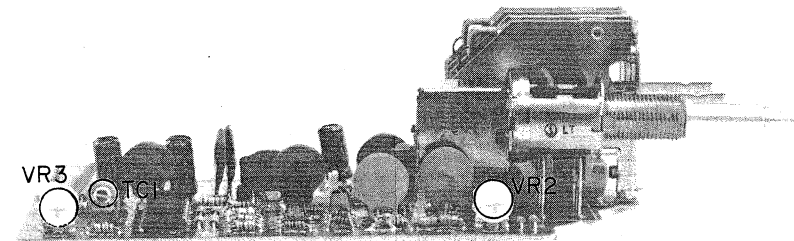


TROUBLESHOOTING

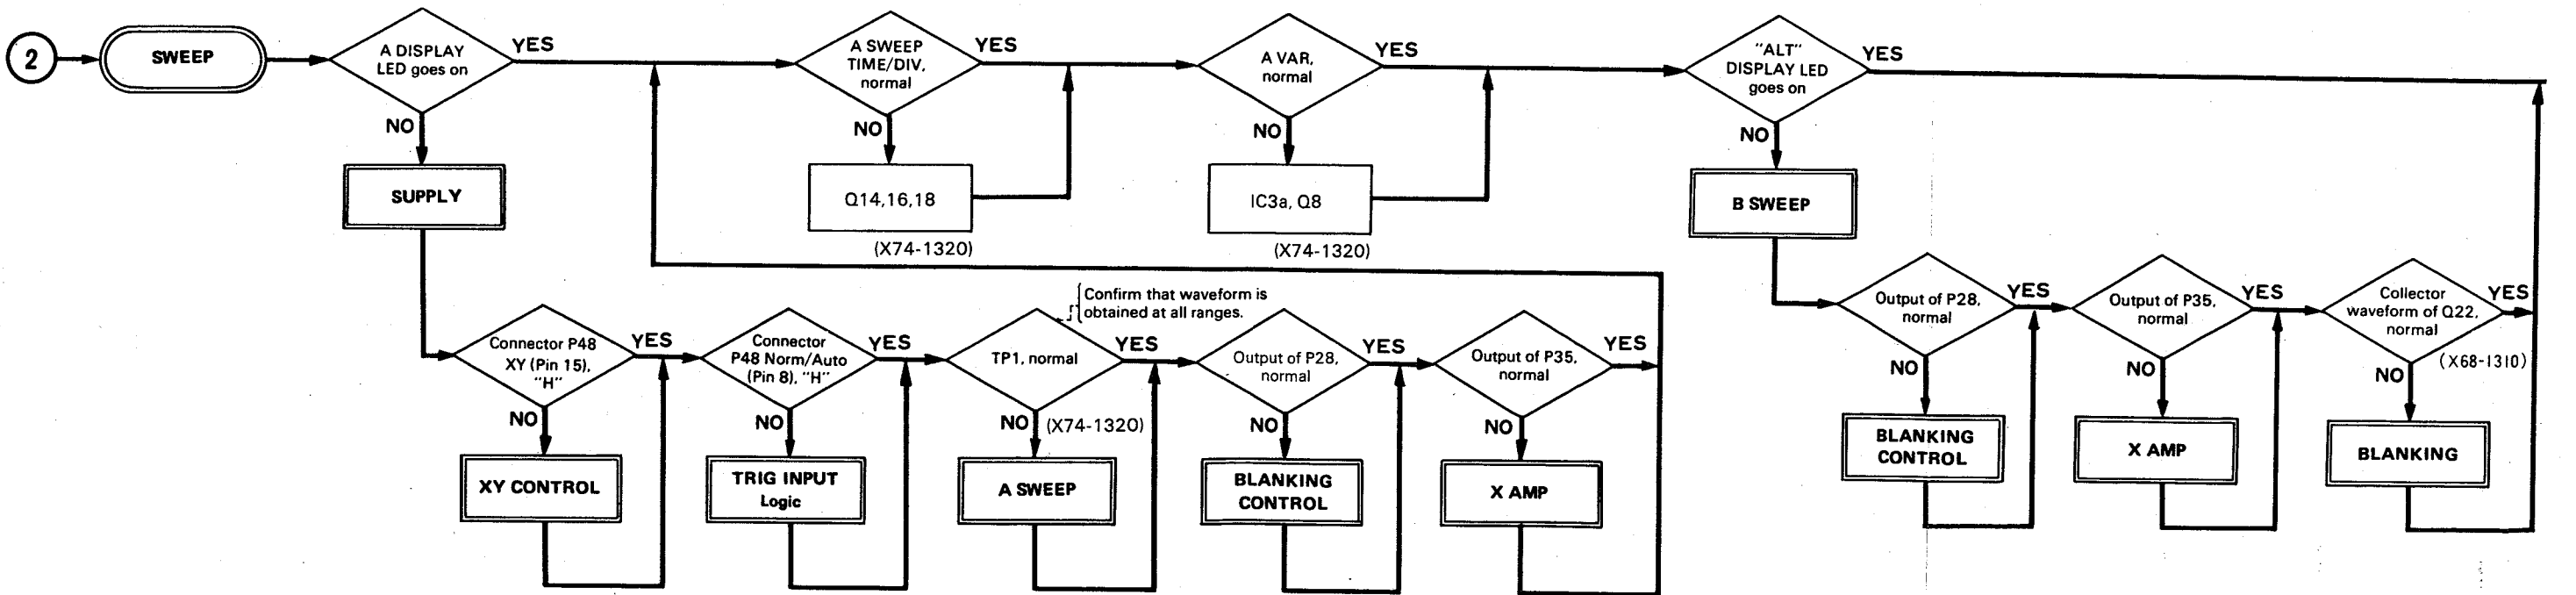
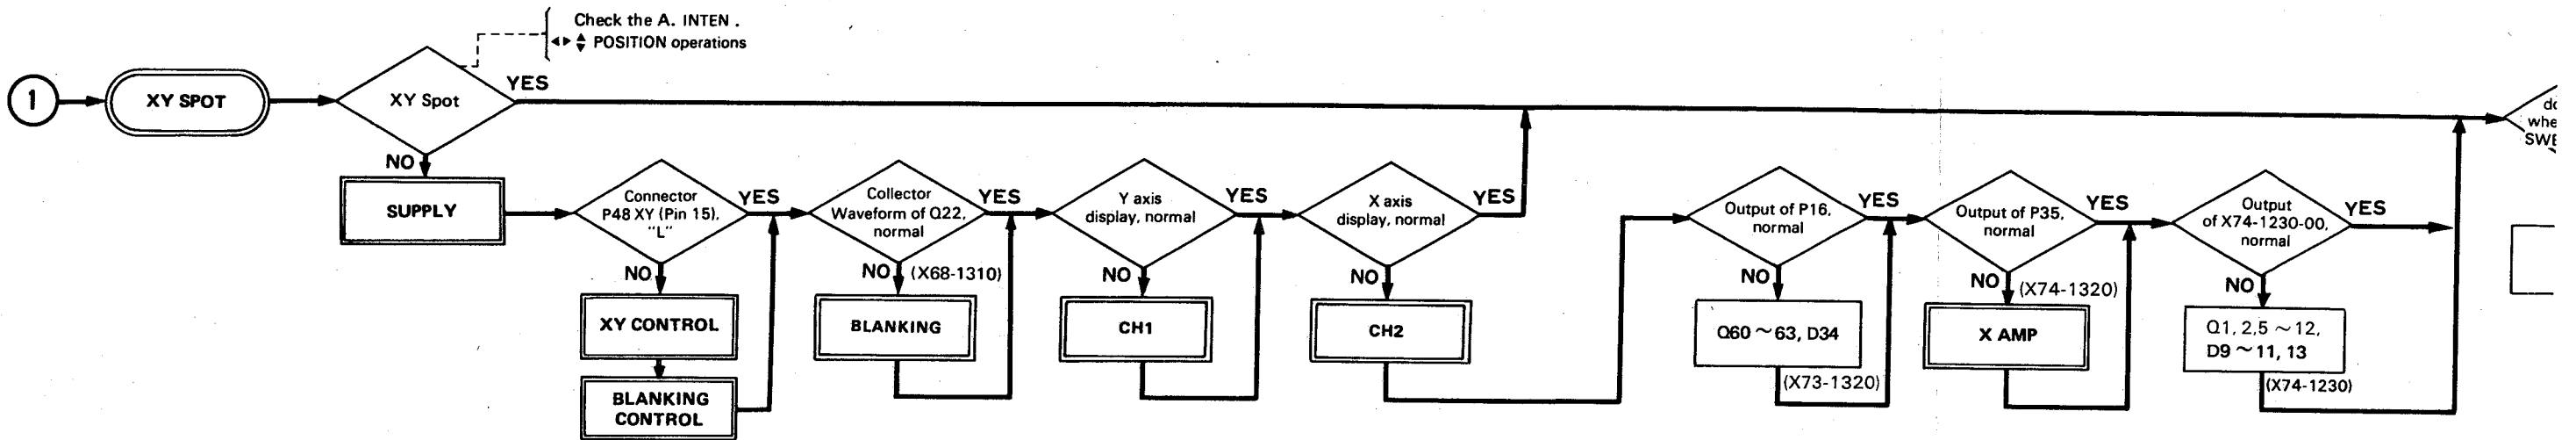
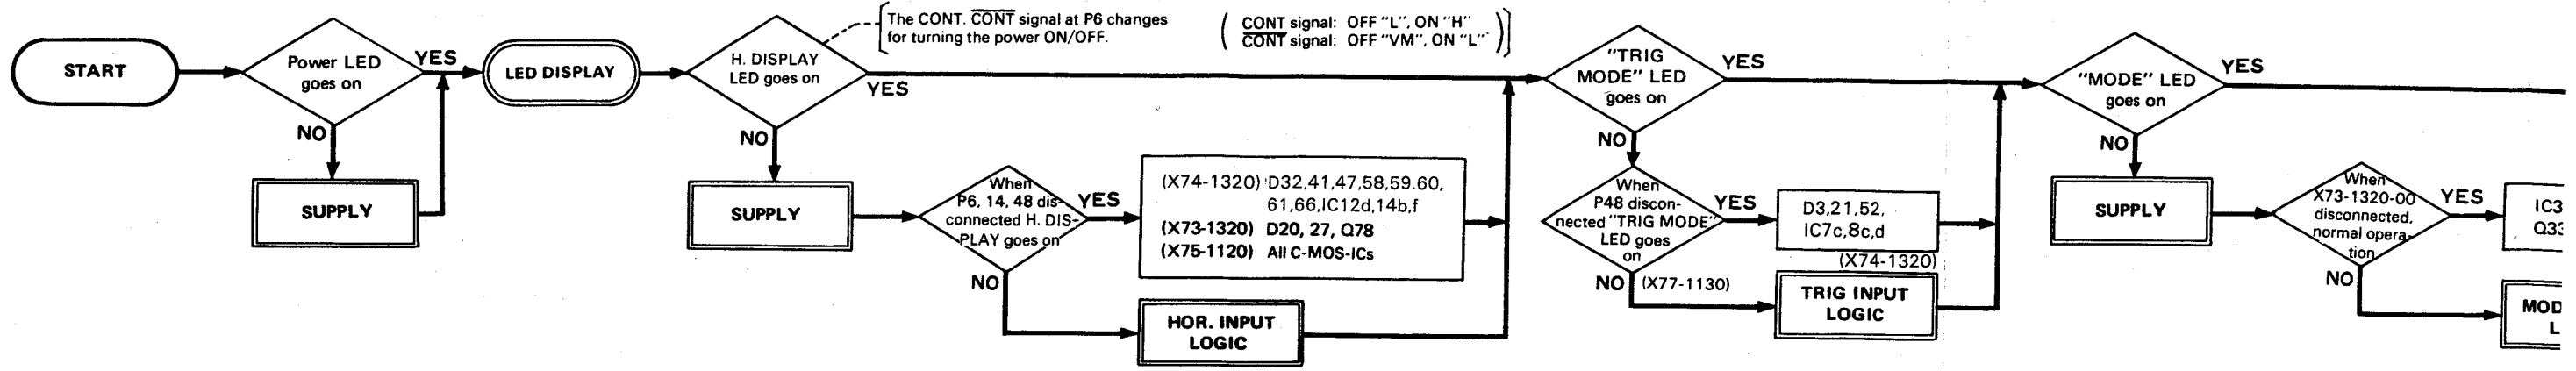


TROUBLESHOOTING

CONT signal: OFF "L", ON "H"
 CONT signal: OFF "VM", ON "L"

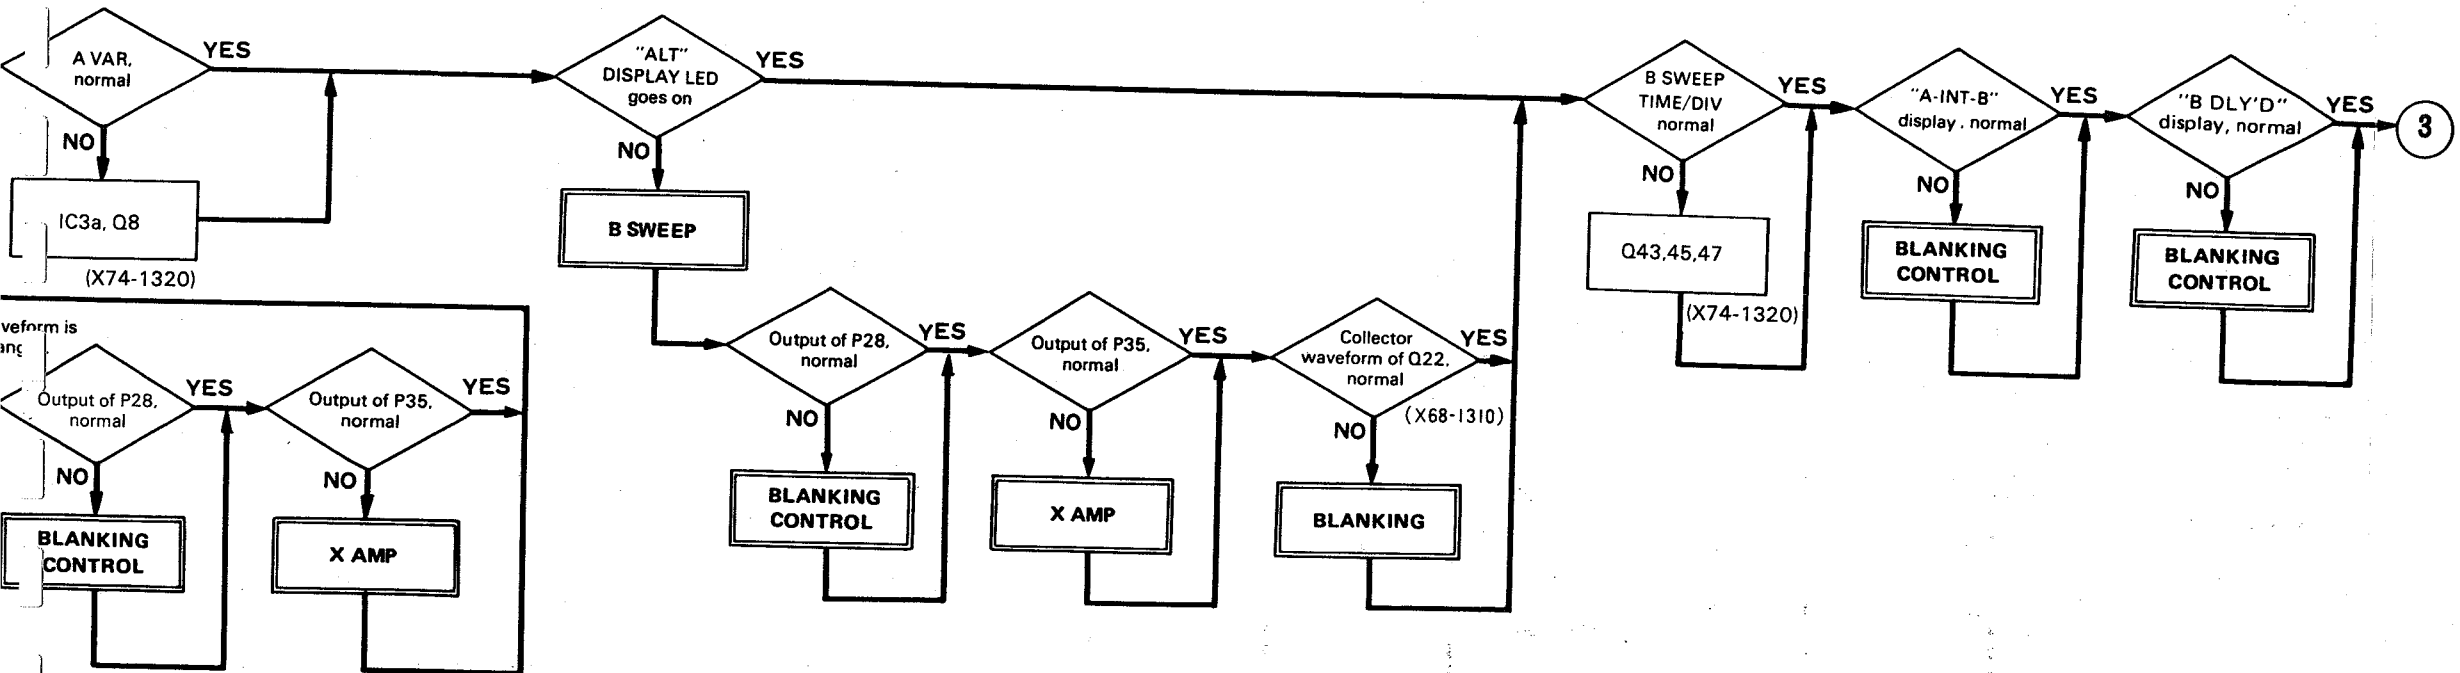
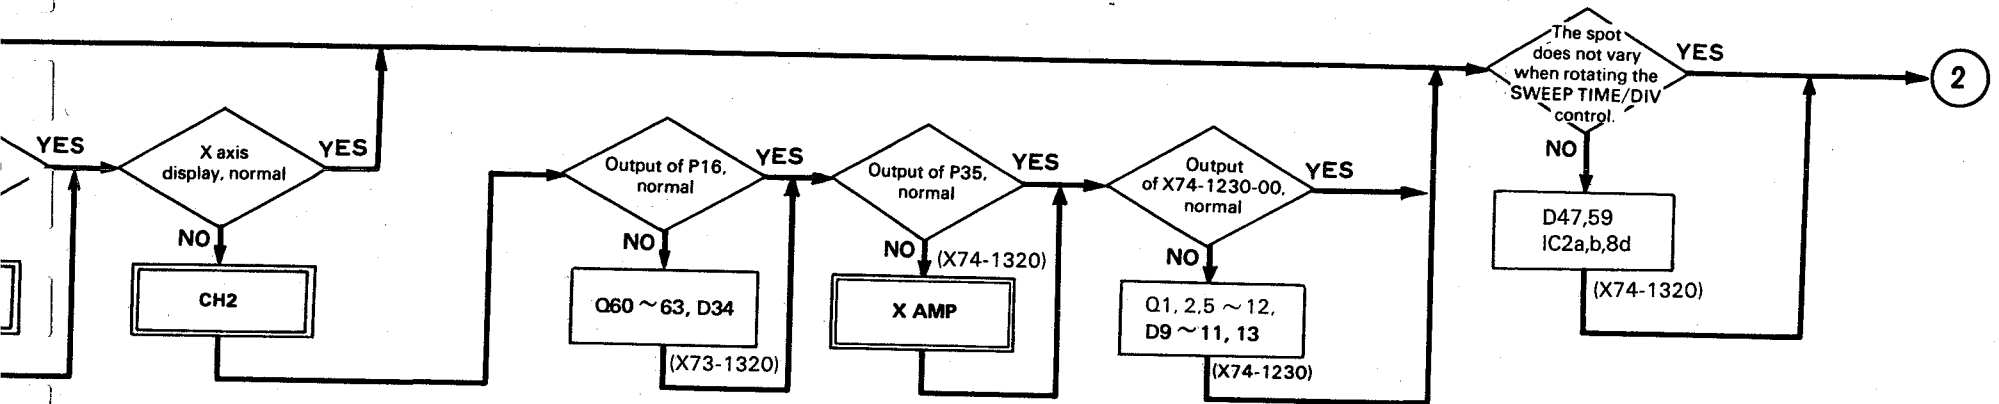
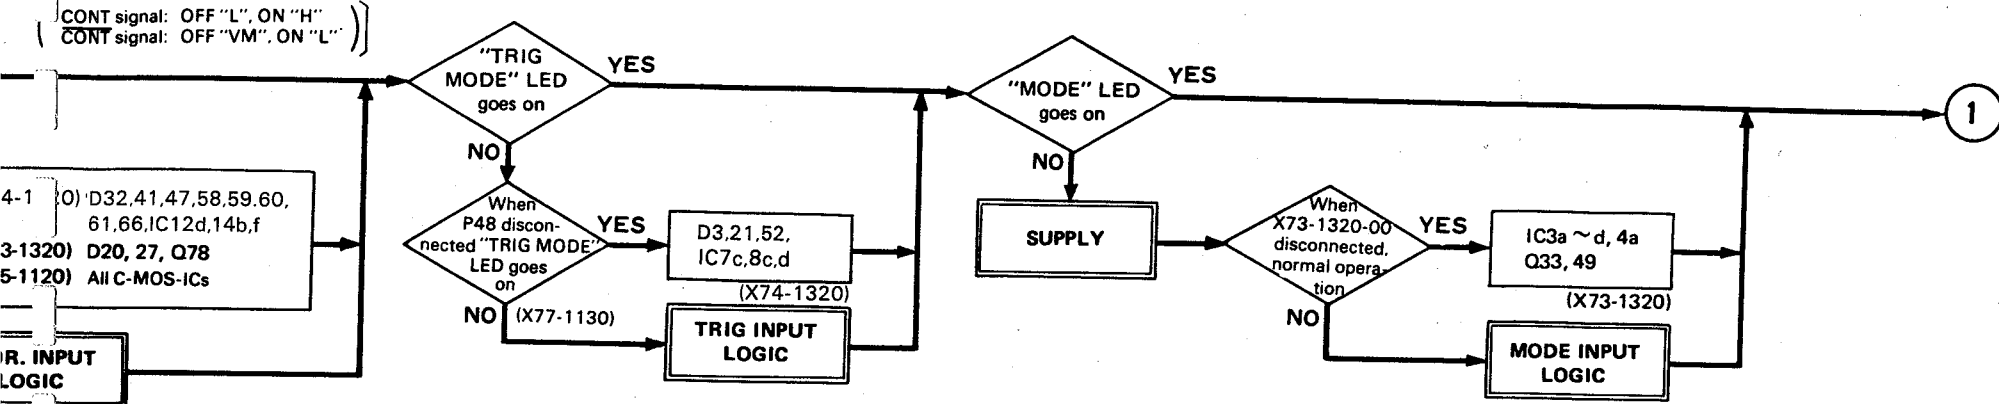


TROUBLESHOOTING

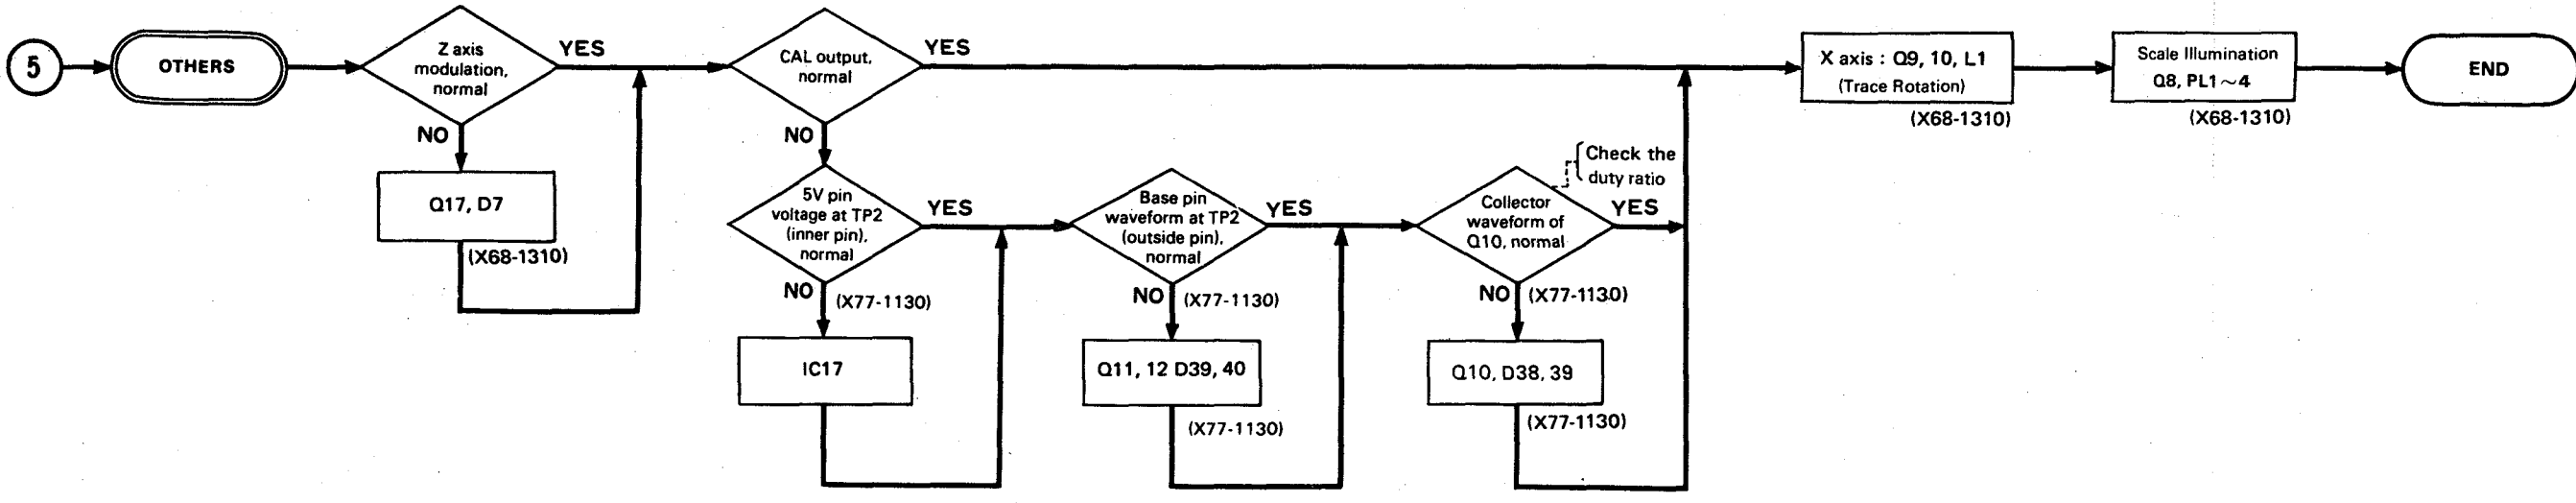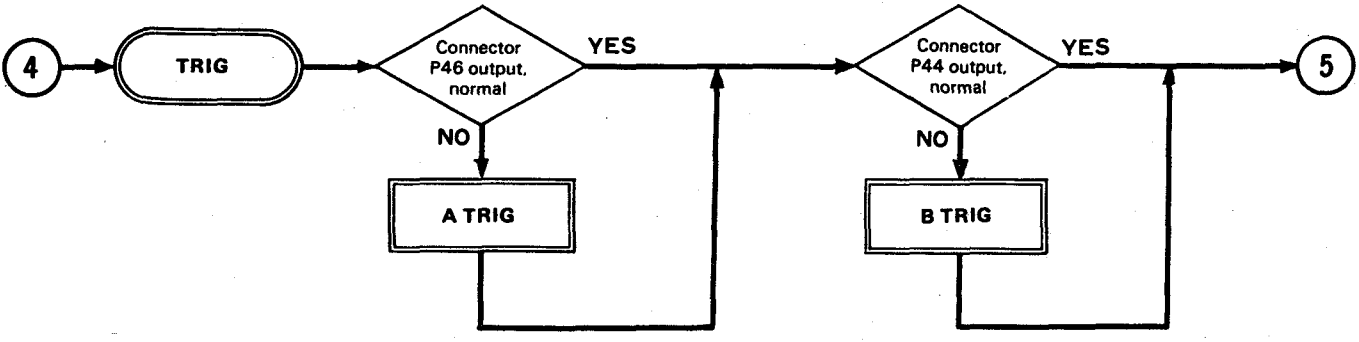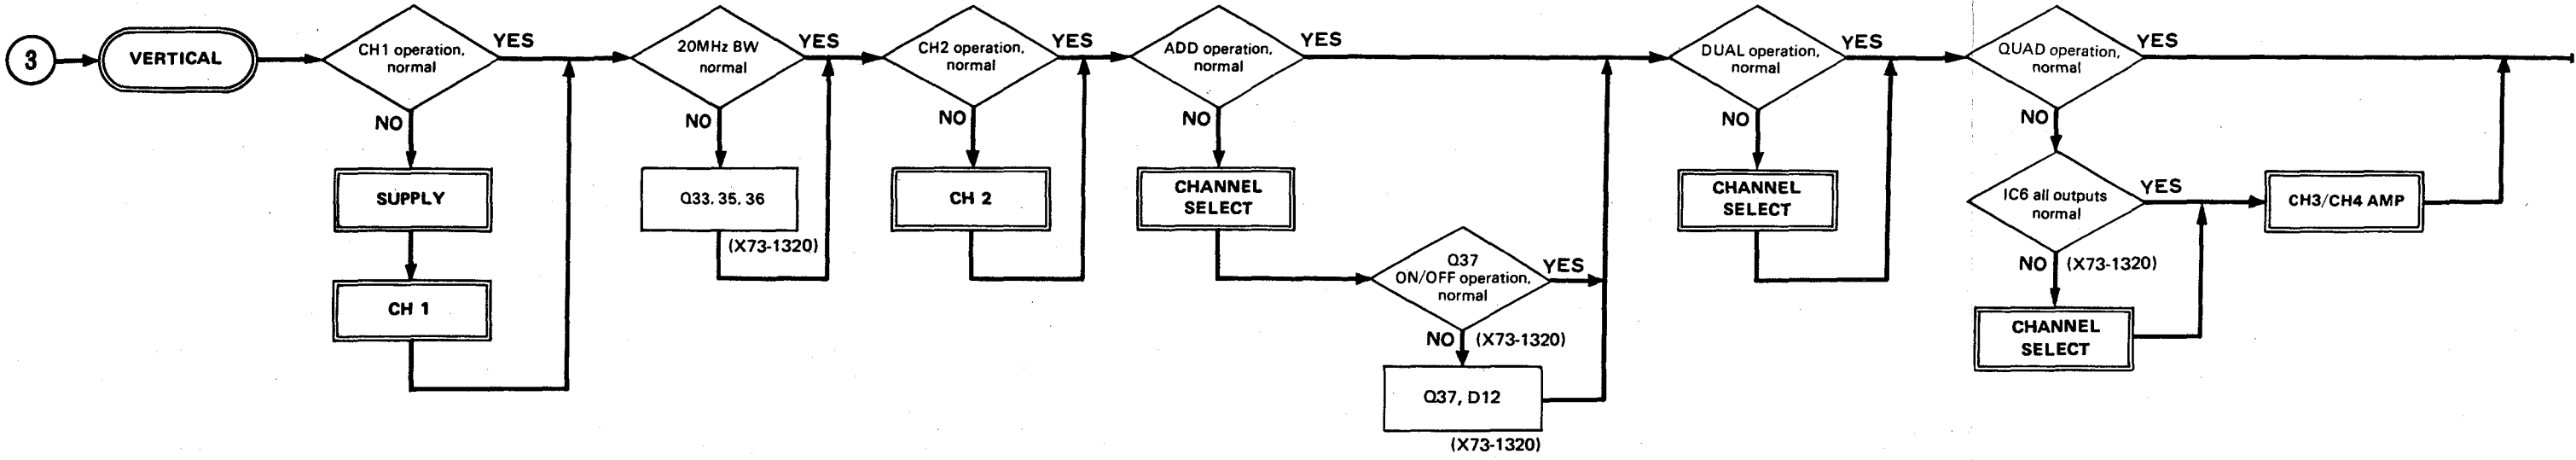

Colle
I
Colle




TROUBLESHOOTING

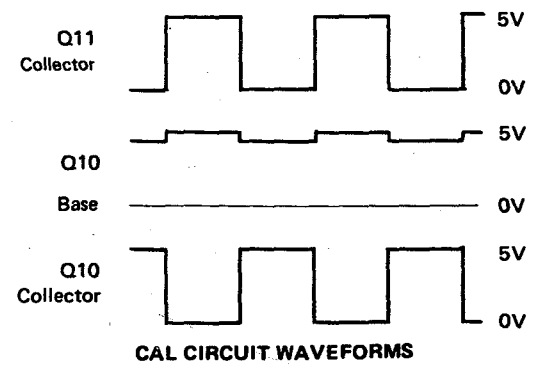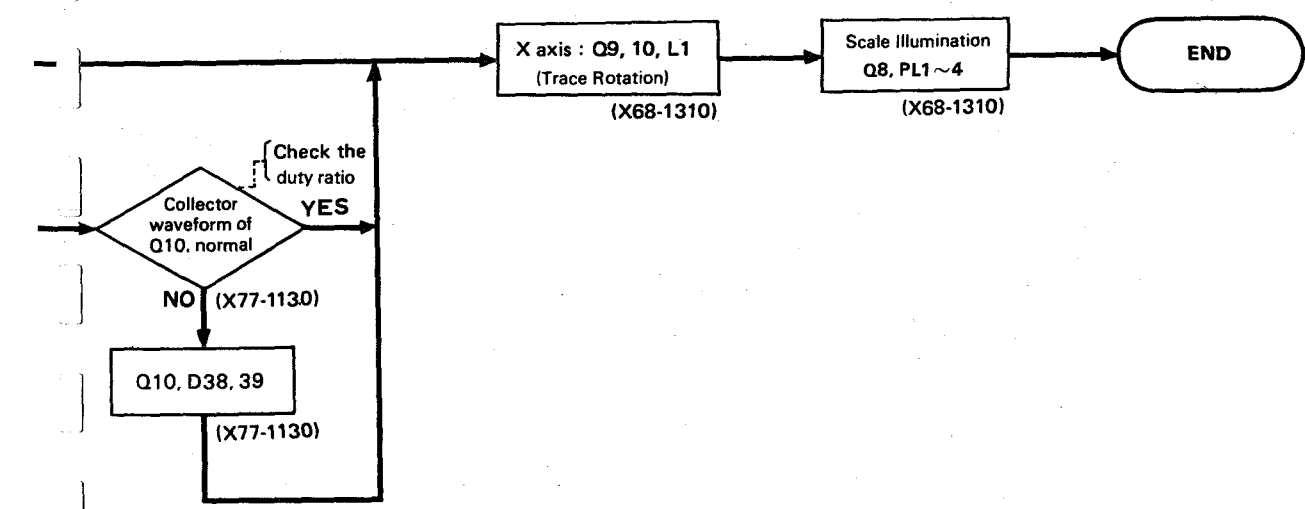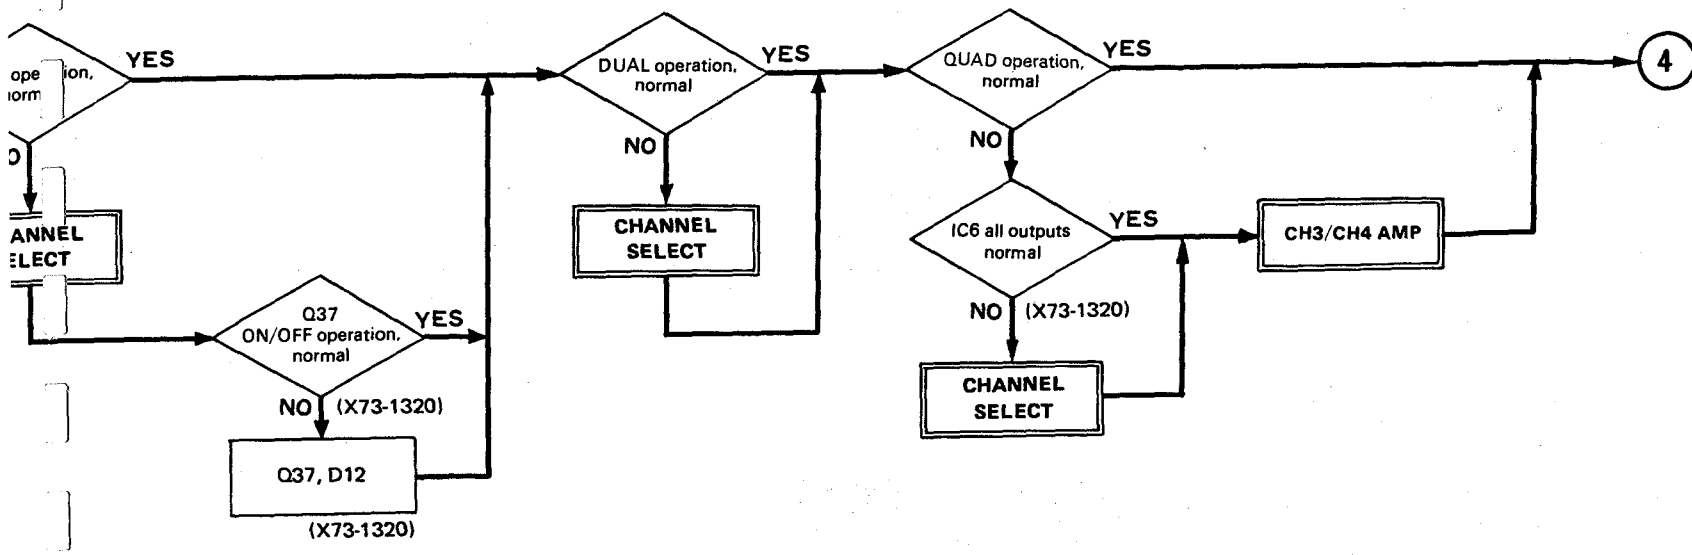




TROUBLESHOOTING

(POWER SUPPLY OF EACH VOLTAGE)


If the power supply voltage is not normal, find the defective unit referring to the below flowchart.

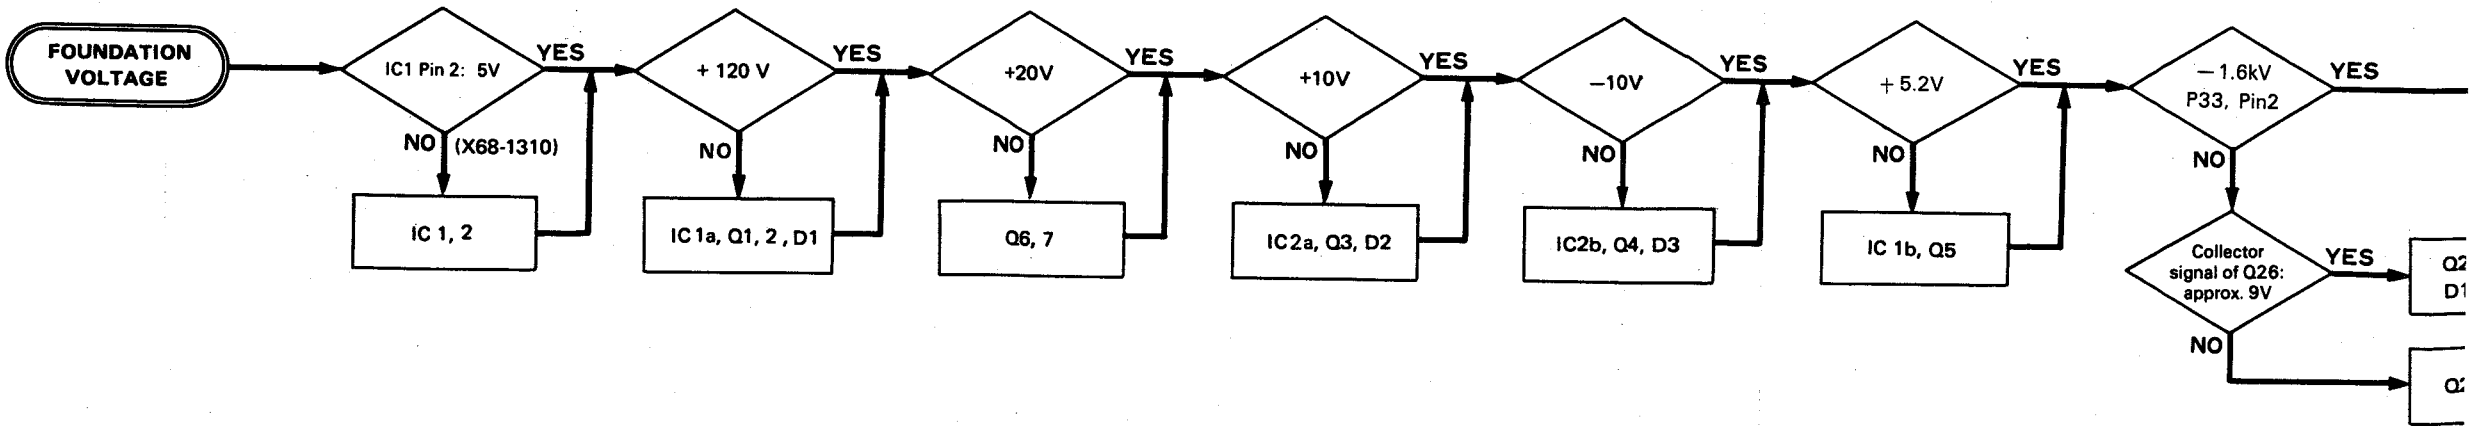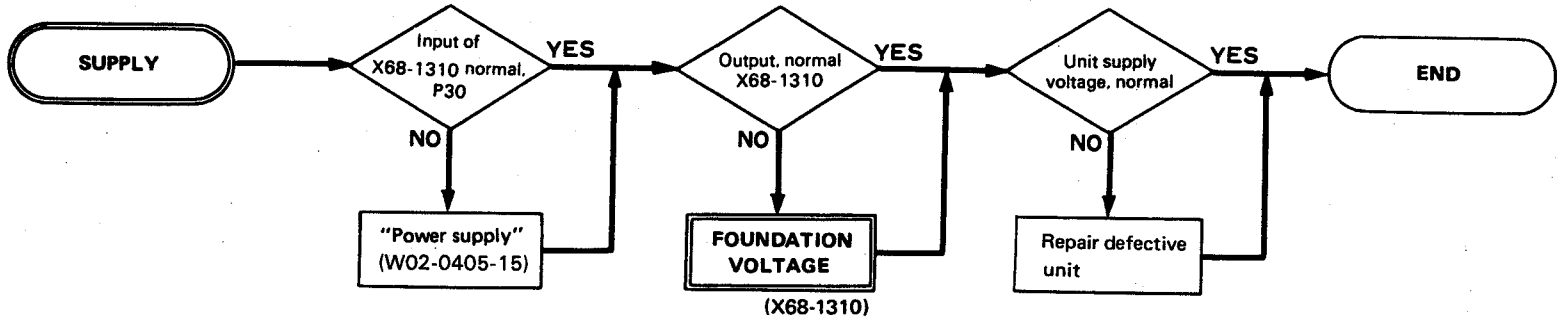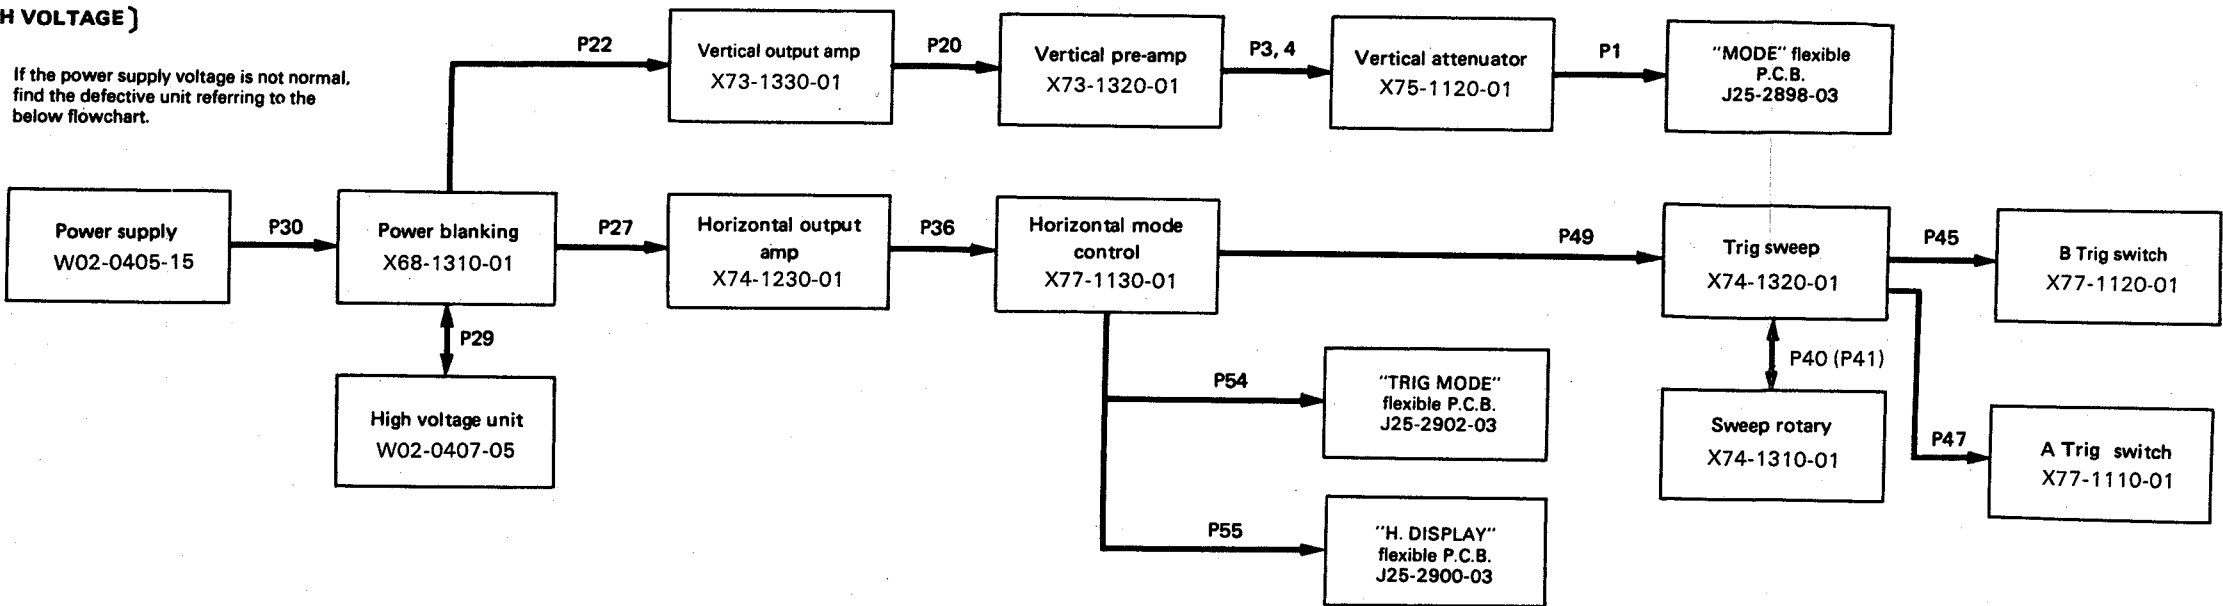

TROUBLESHOOTING

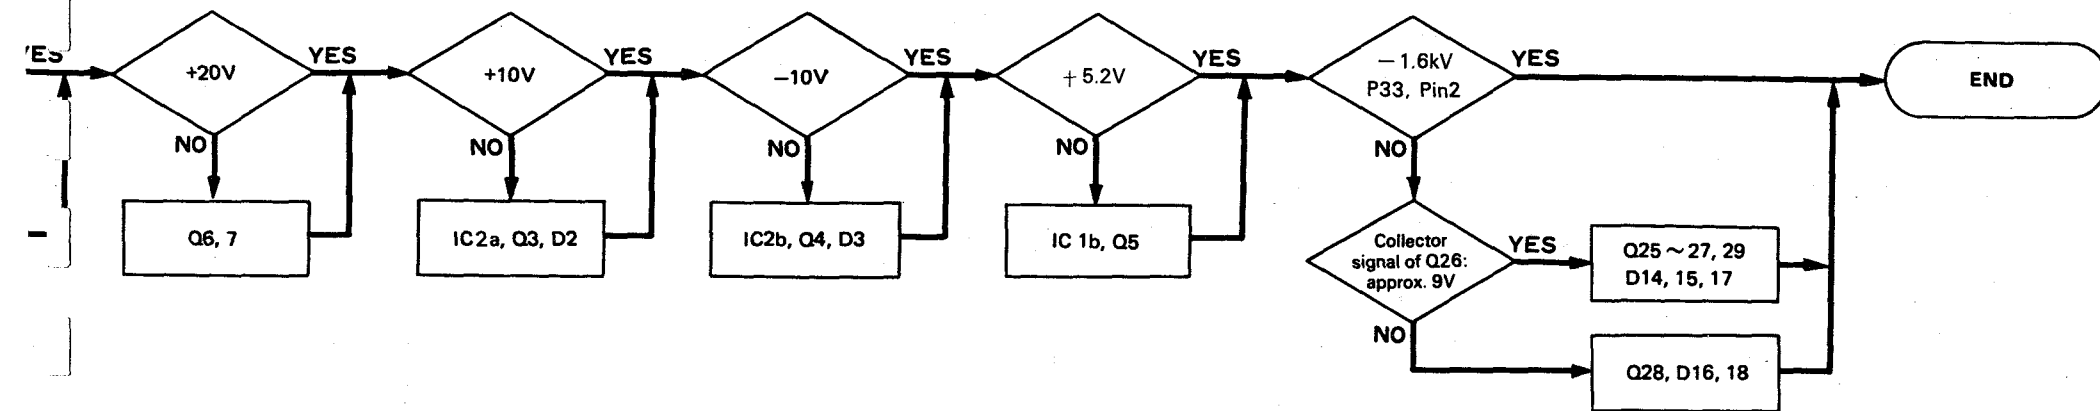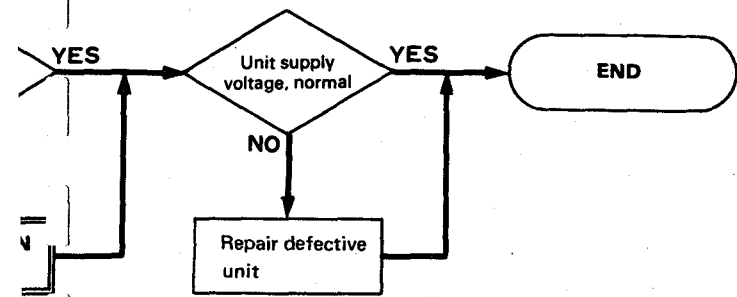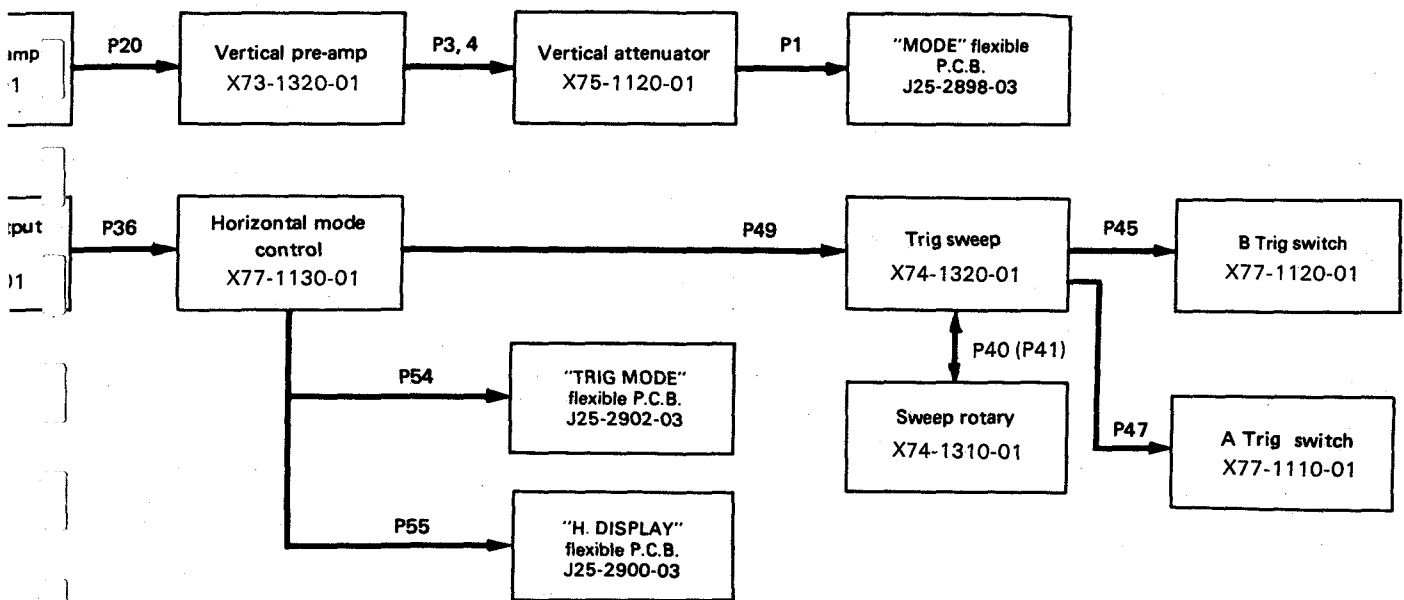


TROUBLESHOOTING

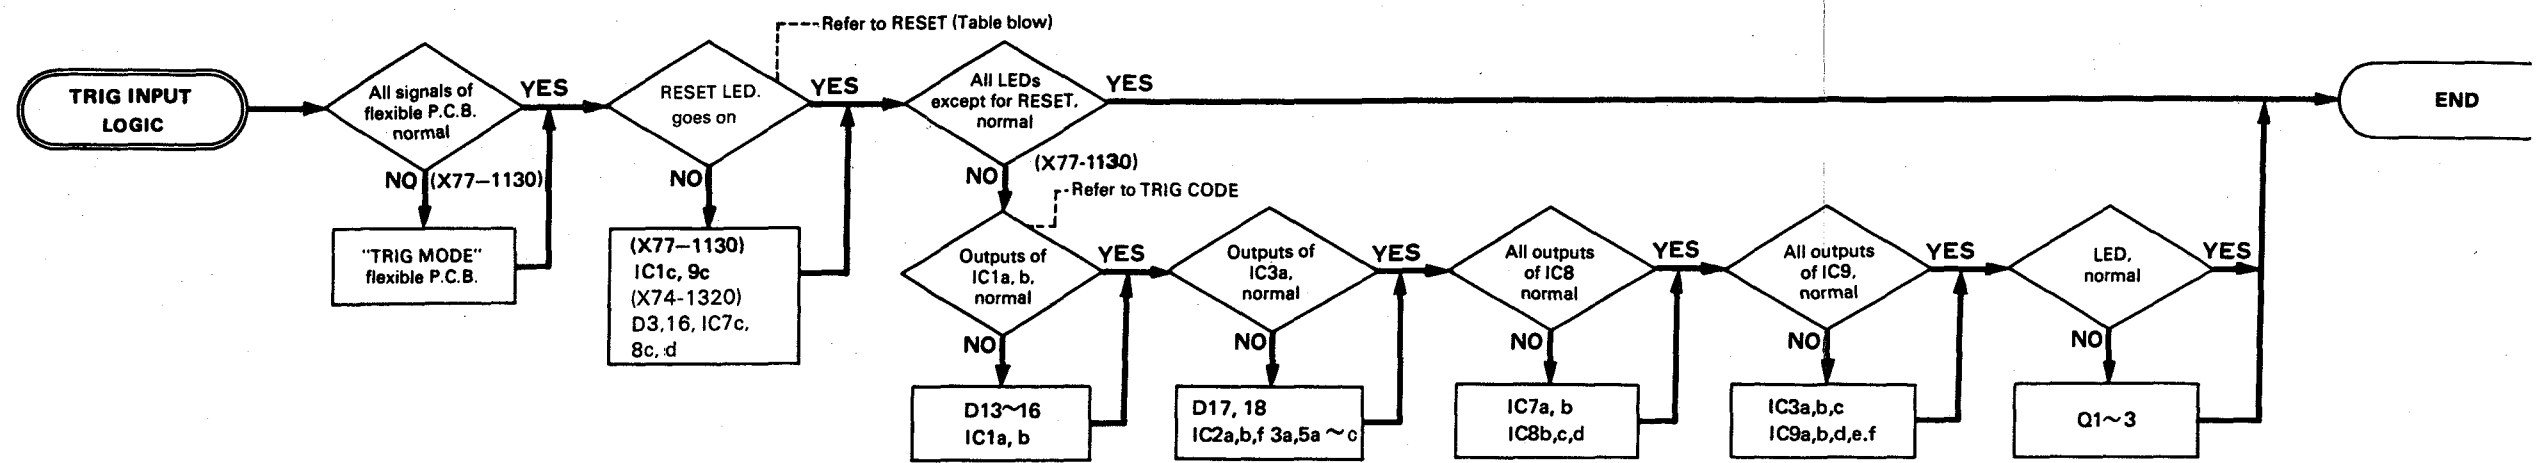


RESET (TRIG MODE "SINGLE")

RESET	Q1	Q1+1	
PUSH (TRIG MODE SINGLE)	P48 10Pin	IC2b 3 Pin	IC3a 3 Pin
		L	L

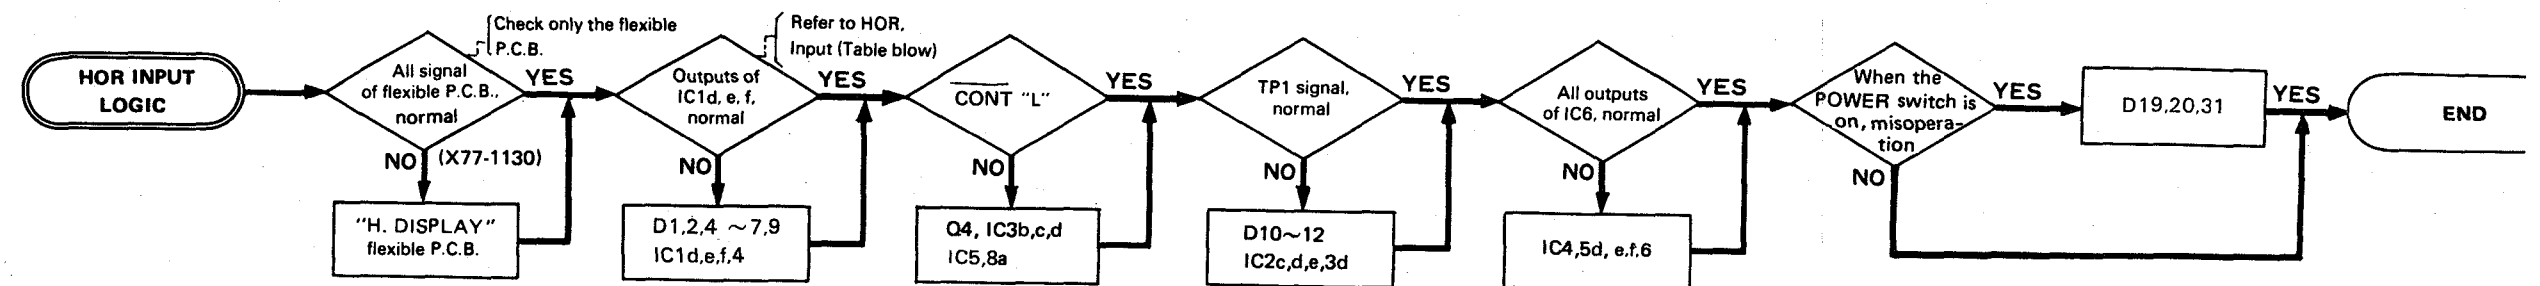

TROUBLESHOOTING

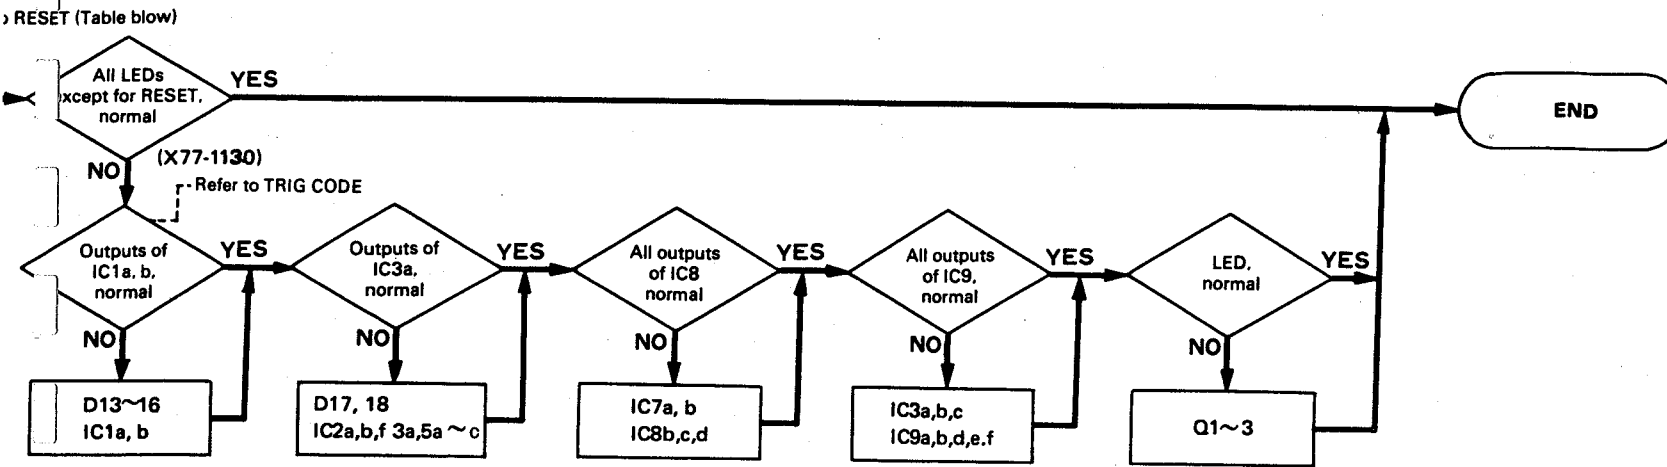


RESET (TRIG MODE "SINGLE")

RESET	Q1	Q1+1
PUSH (TRIG MODE SINGLE)	P48 10Pin	IC2b 3 Pin IC3a 3 Pin
		L L

TRIG CODE

TRIG MODE PUSH	Qt			Qt+1											
	IC1		IC3	IC7				IC8-4	IC8-11	IC8-10	IC9				
	4 Pin	2 Pin	3 Pin	13 Pin	12 Pin	1 Pin	2 Pin	IC5-3	IC5-5	IC5-7	8 Pin	10 Pin	12 Pin	4 Pin	2 Pin
AUTO		L		H	L	L	H	L	H	H	H	L	L	H	H
NORM	L			L	H	H	L	H	L	H	L	H	L	L	H
SINGLE				H	L	H	L	H	H	L	L	L	H	H	L

Qt : Logical value when the switch is depressed.
Qt + 1: Logical value after the switch is depressed.




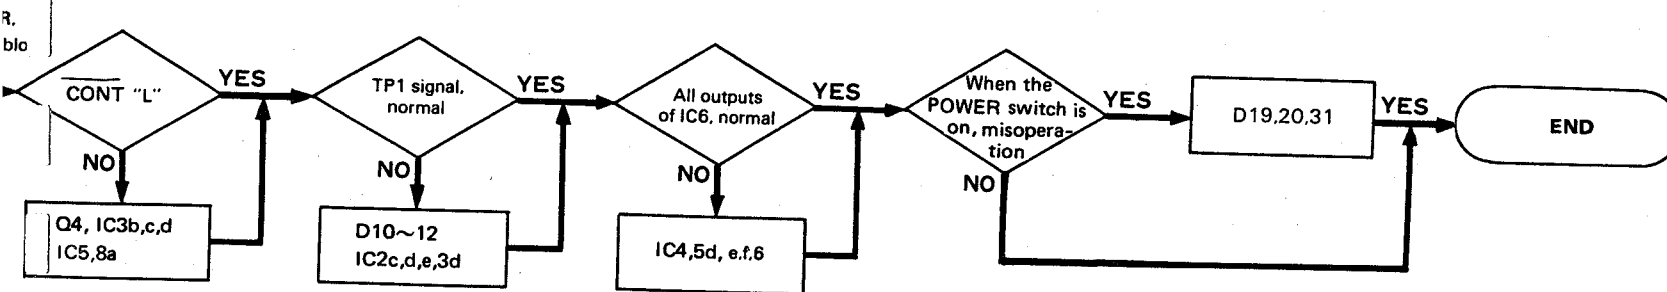


HOR. INPUT

H.DISPLAY PUSH	Qt				Qt+1										
	IC1 OUTPUT			TP1	IC5 1 pin 15 pin	IC4 2 pin 13 pin	IC4 5 pin 11 pin	IC4 7 pin 9 pin	IC6 OUTPUT						
	12f	10e	8 d		2	3	4	5	6	7	OTHER OUTPUT				
A	L	L			L	L	L	H	L	H	H	H	H	H	H
ALT	L		L		L	L	H	L	H	L	H	H	H	H	H
A-INT-B	L				L	L	H	H	H	H	L	H	H	H	H
B		L	L		L	H	L	L	H	H	H	L	H	H	H
X-Y			L		L	H	H	L	H	H	H	H	L	H	H

Qt : Logical value when the switch is depressed.
Qt + 1: Logical value after the switch is depressed.

TROUBLESHOOTING

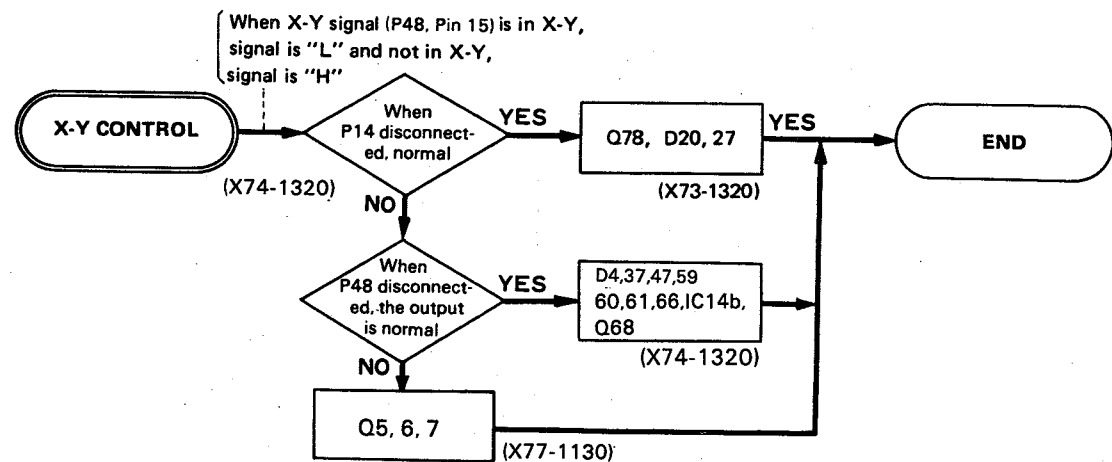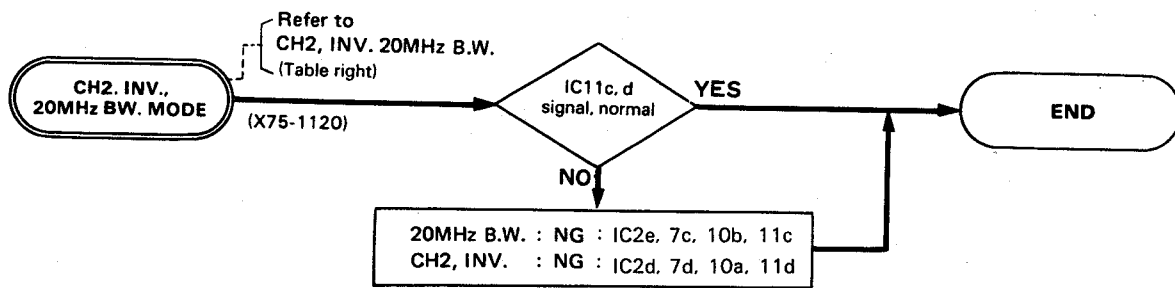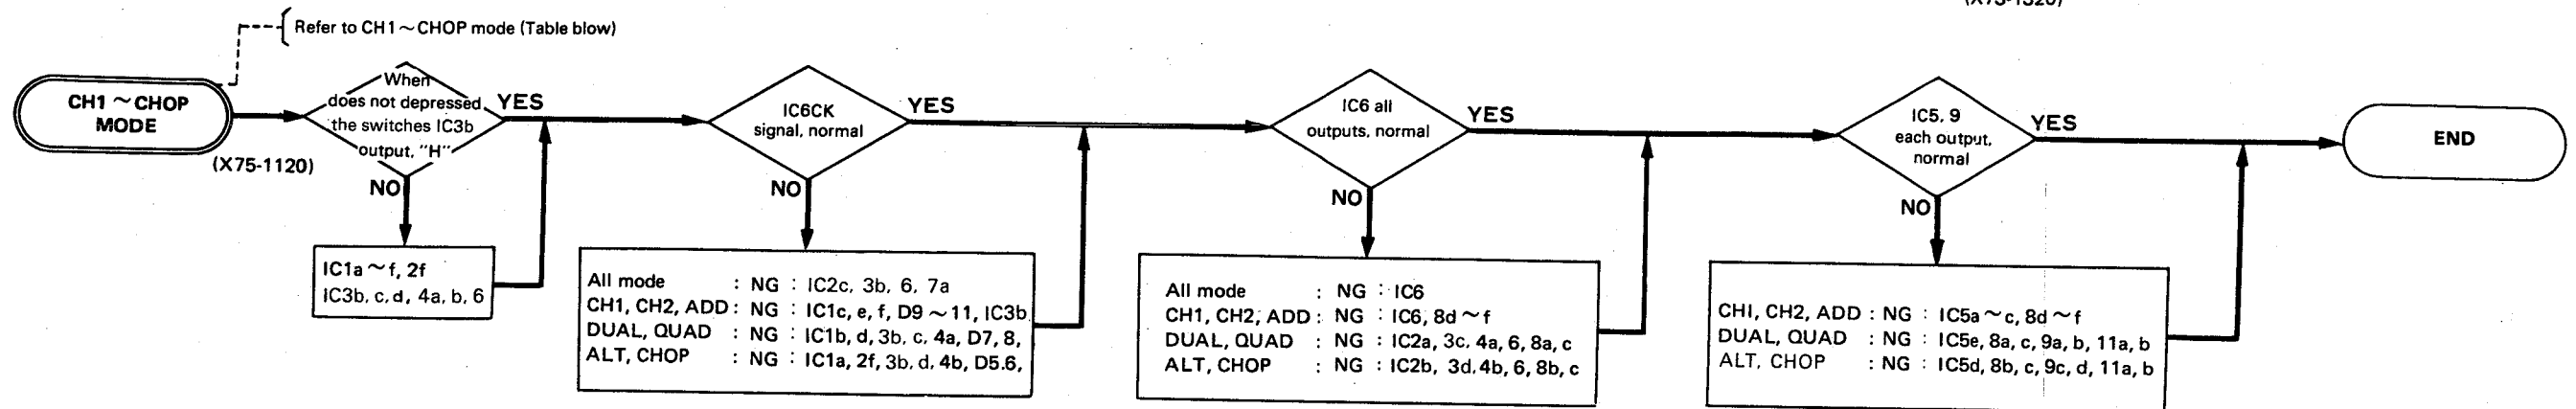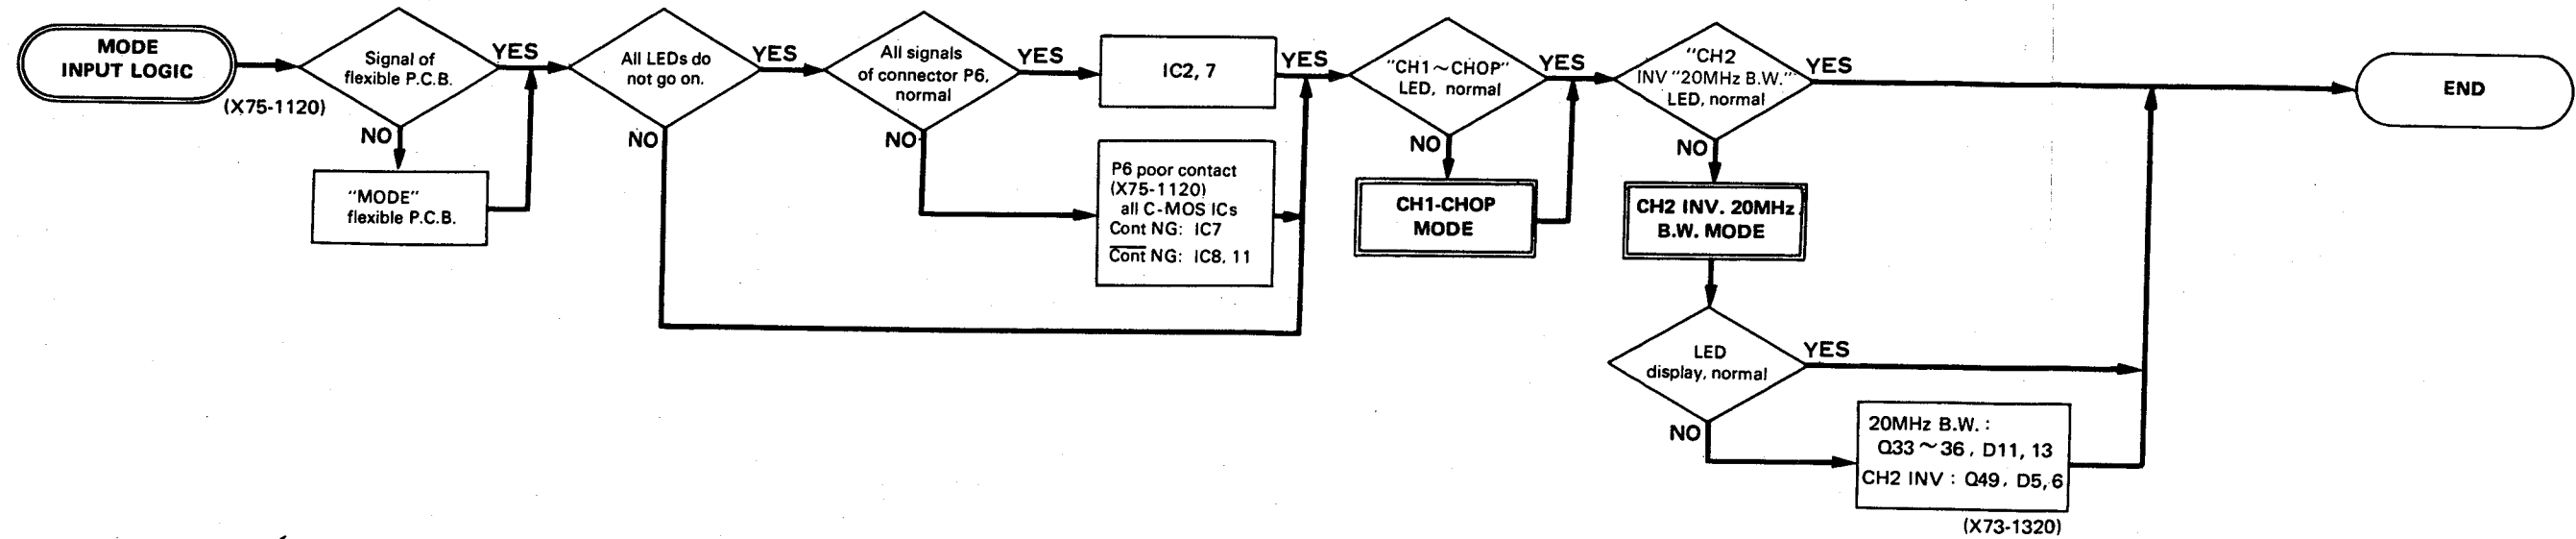

CH2 INV.

CH2 INV	Qt	Qt + 1
	IC10a INPUT	IC10a OUTPUT
PUSH	(T)	(Qa)

20MHz B.W.



20MHz B.W. PUSH	Qt	Qt + 1
	IC 10b INPUT	IC10b OUTPUT
	(T)	(Qb)

CH1 ~ CHOP MODE

"MODE"	Qt				Q5
	IC3b IN / OUT			IC6	
PUSH	IN Pin 5	IN Pin 6	OUT Pin 4	CK	
CH1	L				H
CH2	L				L
DUAL		L			L
ADD	L				L
QUAD		L			L
ALT		L			L
CHOP		L			L

Qt : Logical value when the switch is depressed
 Qt + 1 : Logical value after the switch is depressed
 Qkt : Indicates that Qkt which is the logical value depressed is output when the switch is depressed

TROUBLESHOOTING

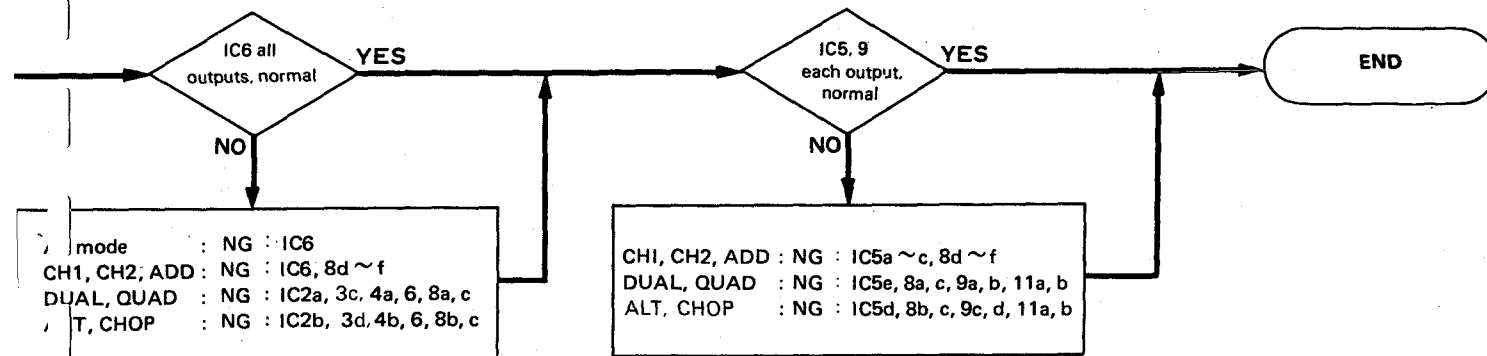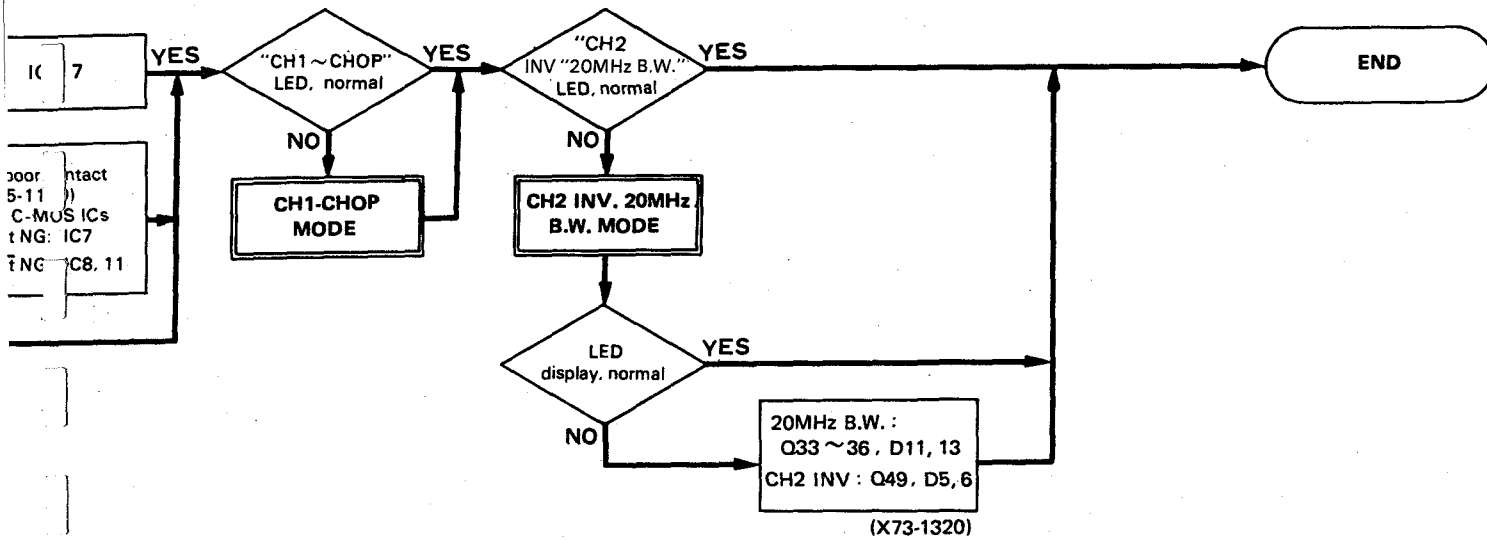

CH2 INV.

	Qt	Qt + 1
CH2 INV	IC10a INPUT	IC10a OUTPUT
PUSH	(T)	(Qa)

20MHz B.W.



	Qt	Qt + 1
20MHz B.W.	IC 10b INPUT	IC10b OUTPUT
PUSH	(T)	(Qb)

CH1~CHOP MODE

"MODE"	Qt				Qt + 1														
	IC3b IN/OUT			IC6 CK	CH1/CH2/ADD						IC6 Q2	DUAL/QUAD				ALT/CHOP			
	IN Pin 5	IN Pin 6	OUT Pin 4		IC6			IC5				IC4a Qa	IC6 Qo	IC9 OUTPUT		IC4b Qb	IC6 Q1	IC9 OUTPUT	
				Q5	Q4	Q3	a	b	c			b	a			c	d		
CH1	L			H	L	L	L	H	H	H	Qat	Qat	H	H	Qbt	Qbt	H	H	
CH2	L			L	H	L	H	L	H	H	Qat	Qat	H	H	Qbt	Qbt	H	H	
DUAL		L		L	L	L	H	H	H	L	L	L	L	H	Qbt	Qbt	Q1t	Q1t	
ADD	L			L	L	H	H	H	L	H	Qat	Qat	H	H	Qbt	Qbt	H	H	
QUAD		L		L	L	L	H	H	H	L	H	H	H	L	Qbt	Qbt	Q1t	Q1t	
ALT		L		L	L	L	H	H	H	L	Qat	Qat	Qot	\overline{Qot}	H	L	L	H	
CHOP		L		L	L	L	H	H	H	L	Qat	Qat	Qot	\overline{Qot}	L	H	H	L	

Qt : Logical value when the switch is depressed.
 Qt + 1 : Logical value after the switch is depressed.
 Qkt : Indicates that Qkt which is the logical value before the switch is depressed is output when the switch is depressed.

TROUBLESHOOTING

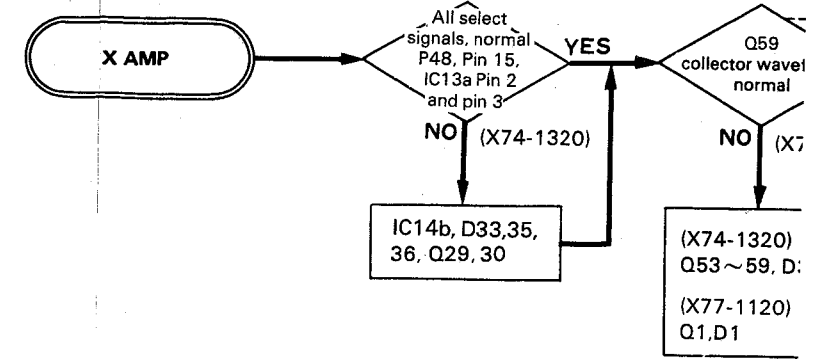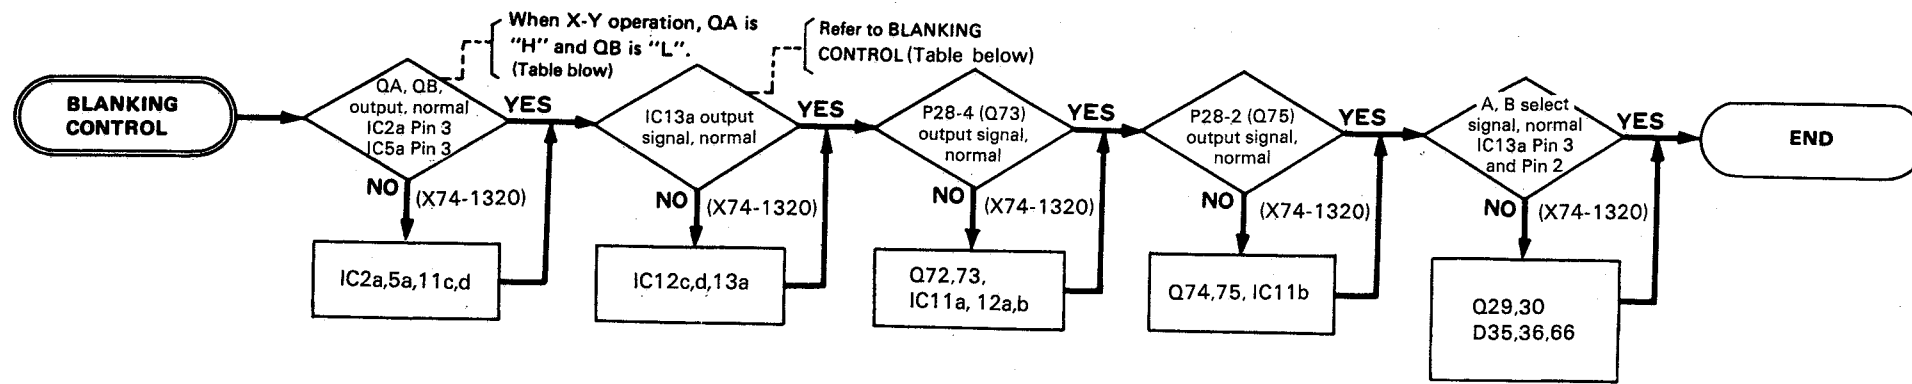


BLANKING CONTROL

H DISPLAY	P48 X-Y BUFFER 15Pin	IC13a				IC12d OUT	P28	
		IN		OUT			A. blanking 4Pin	B. blanking 2Pin
		S	R	Q	\bar{Q}		QA	QB
A	H	H	L	H	L	H	QA	H
ALT	H	L	L	TOGGLE		H	QA*	QB
A-INT-B	H	H	L	H	L	H	QA	QB
B-DLY'D	H	L	H	L	H	H	H	QB
X-Y	L	H	L	H	L	H	L	H


The $\bar{Q}A$ and $\bar{Q}B$ in the table show the reverse phase of QA and AB described.

- *1 Complex waveform IC 11b and QA signals.
- *2 Complex waveform IC11b output. When CHOP operation, output of P28 is complex CHOP signal waveform.






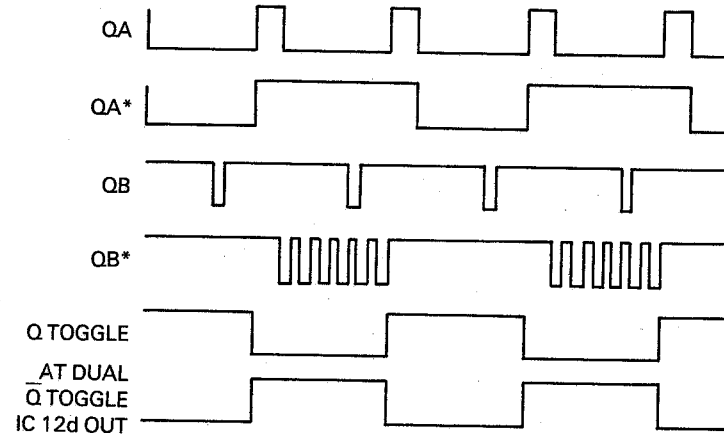


RELATIONSHIP BETWEEN A, B SWEEP AND QA, QB





- < A
- IC2a 3 Pin
- IC5a 3 Pin
- IC13a Q
- IC13a \bar{Q}
- IC12d
- Q73 (E)
- Q75 (E)
- <
- IC2a 3 Pin
- IC5a 3 Pin
- IC13a Q
- IC13a \bar{Q}
- IC12d
- Q73
- Q75

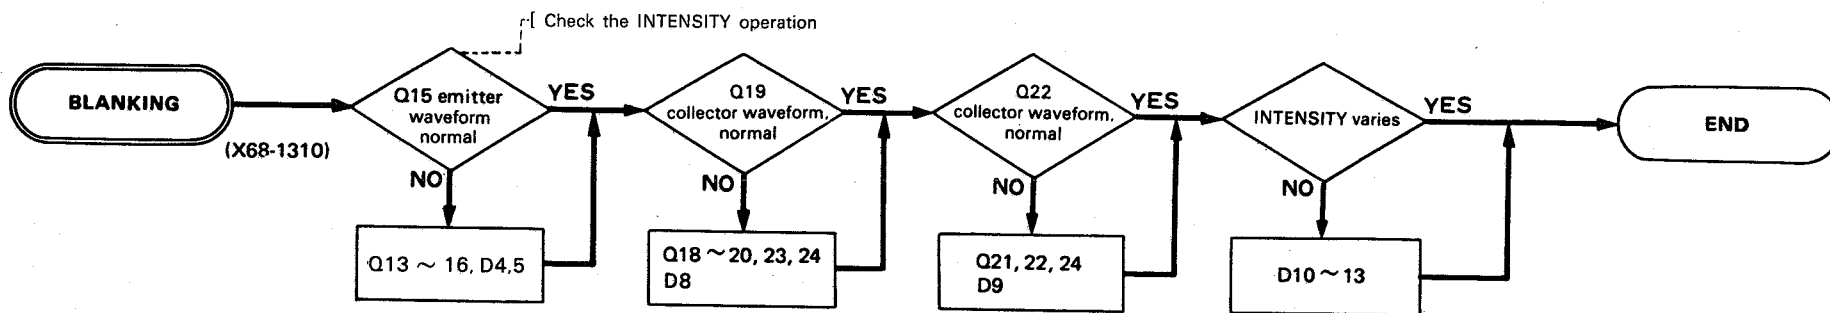





TROUBLESHOOTING

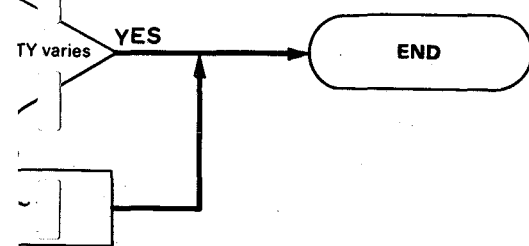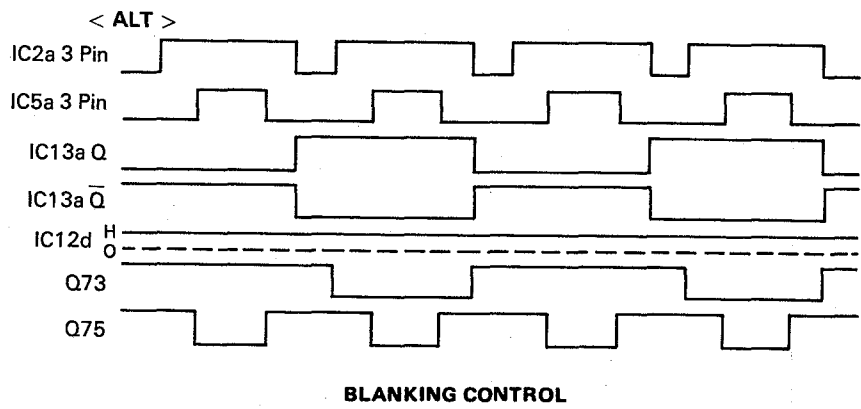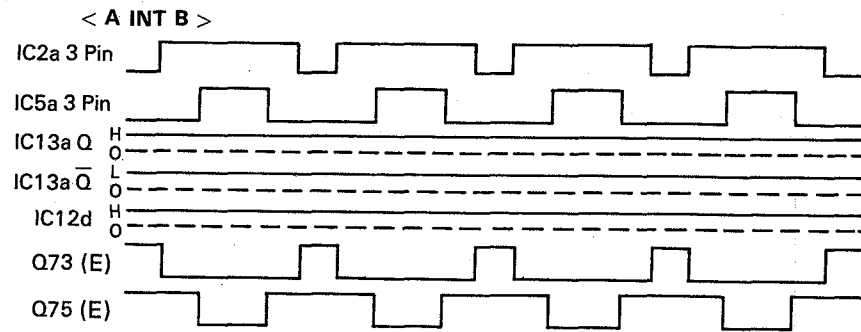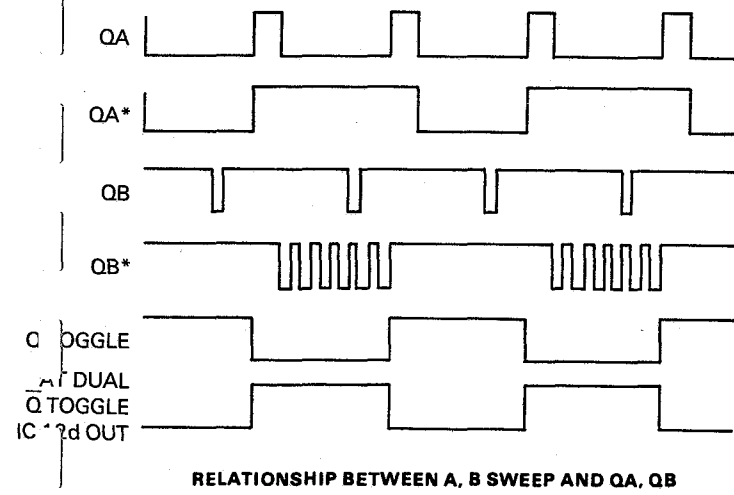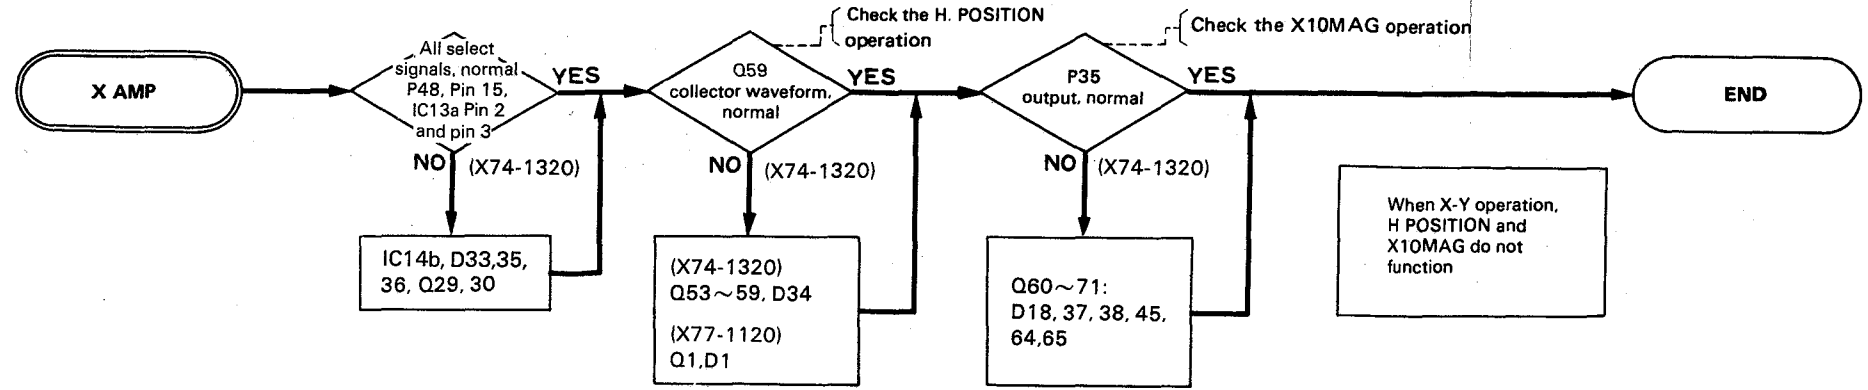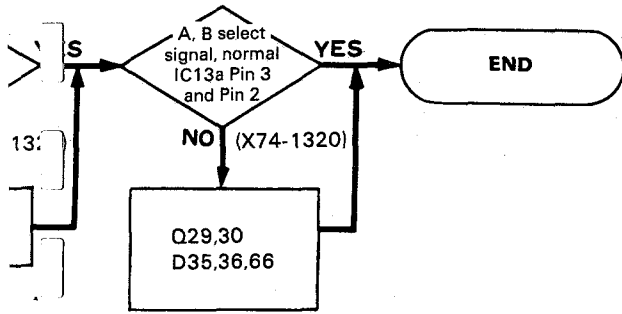


TROUBLESHOOTING

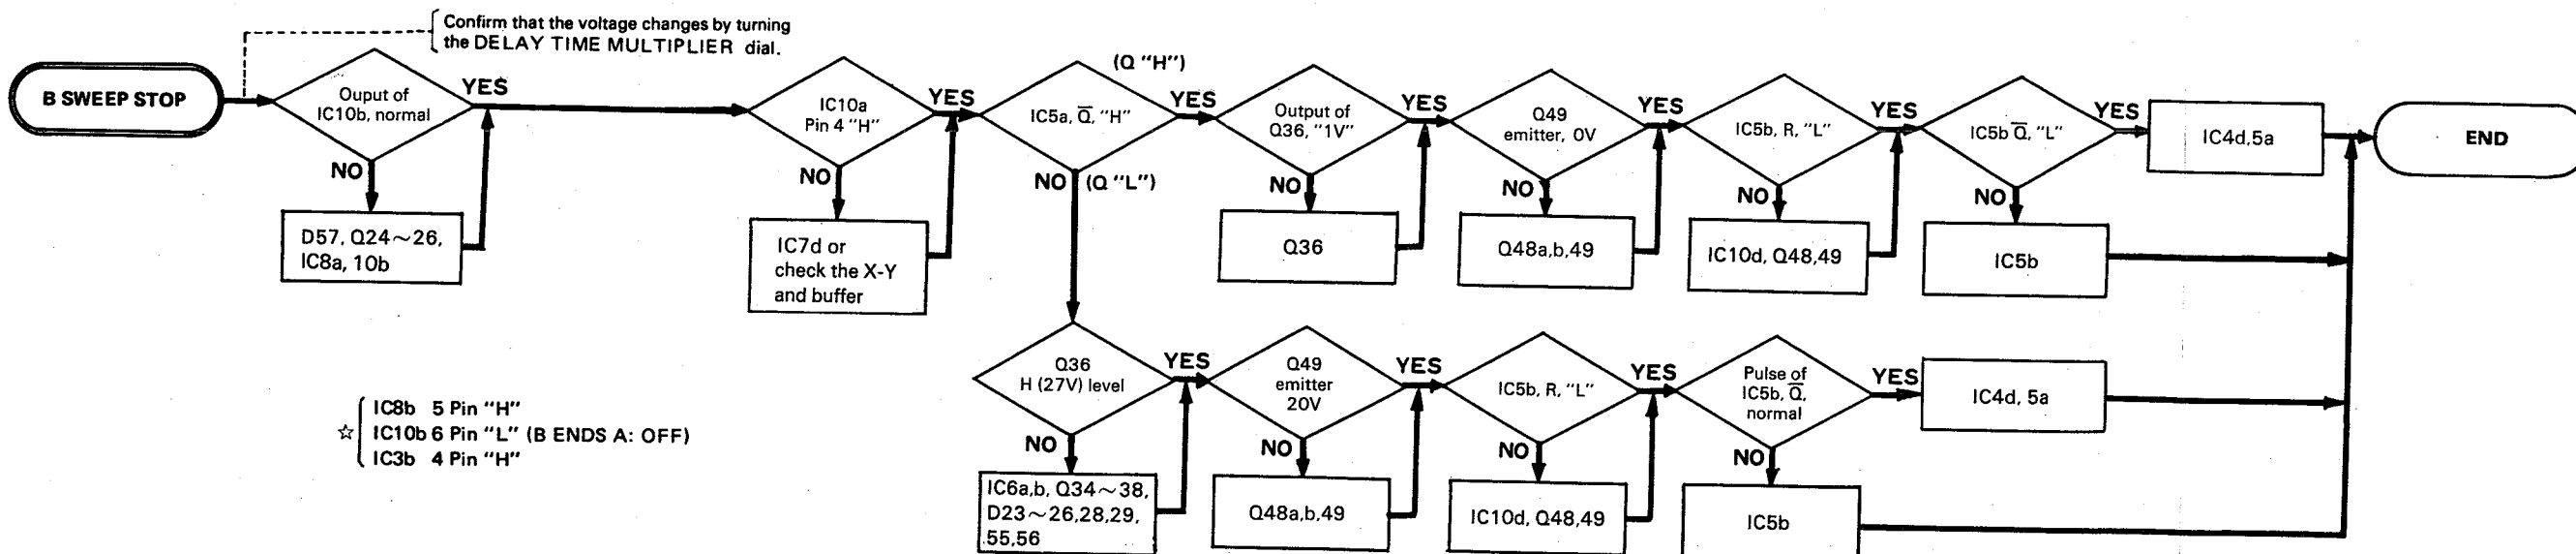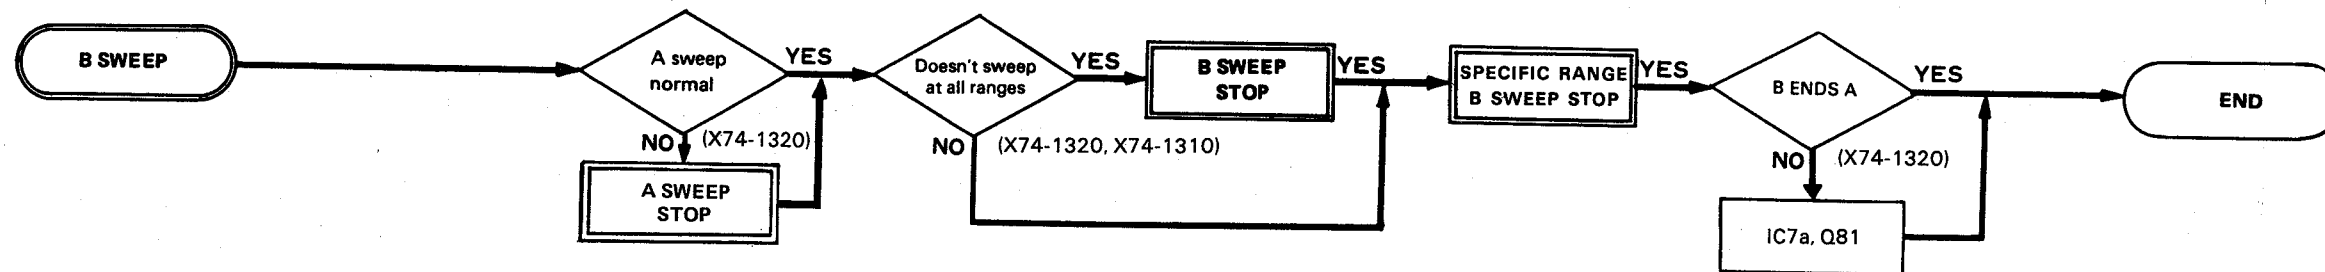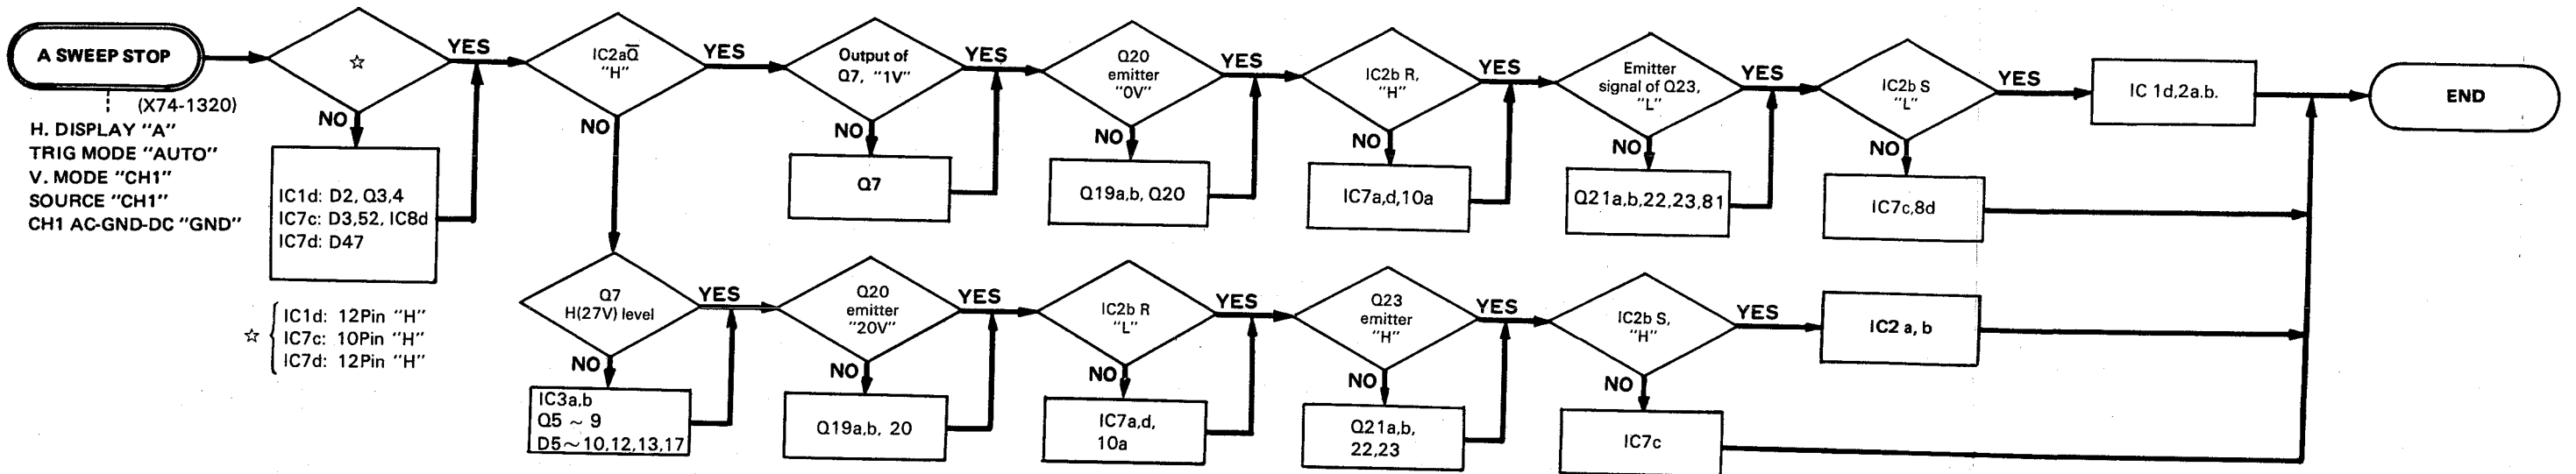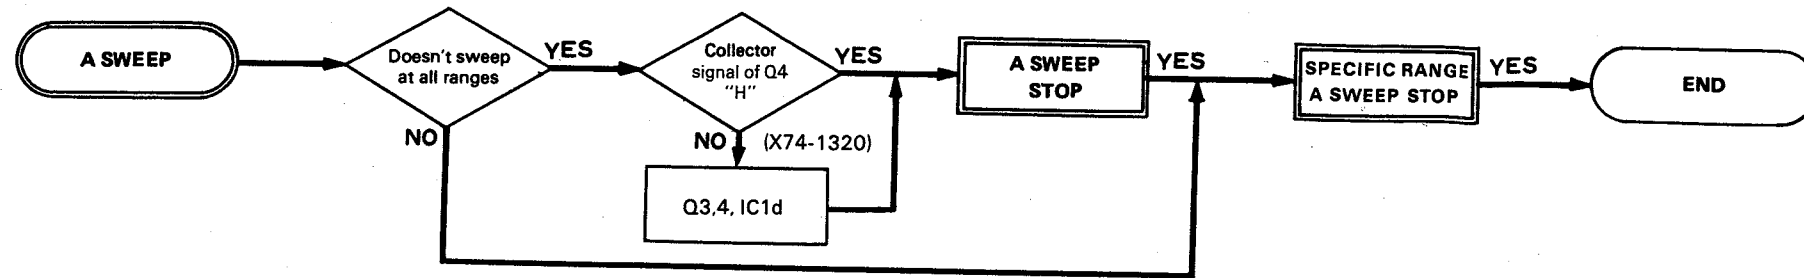

TROUBLESHOOTING

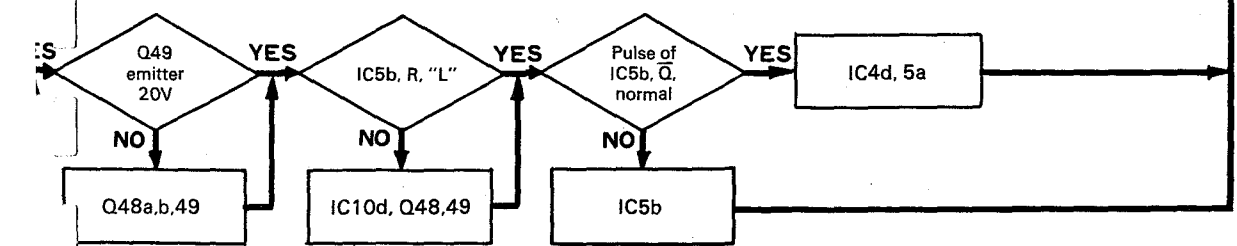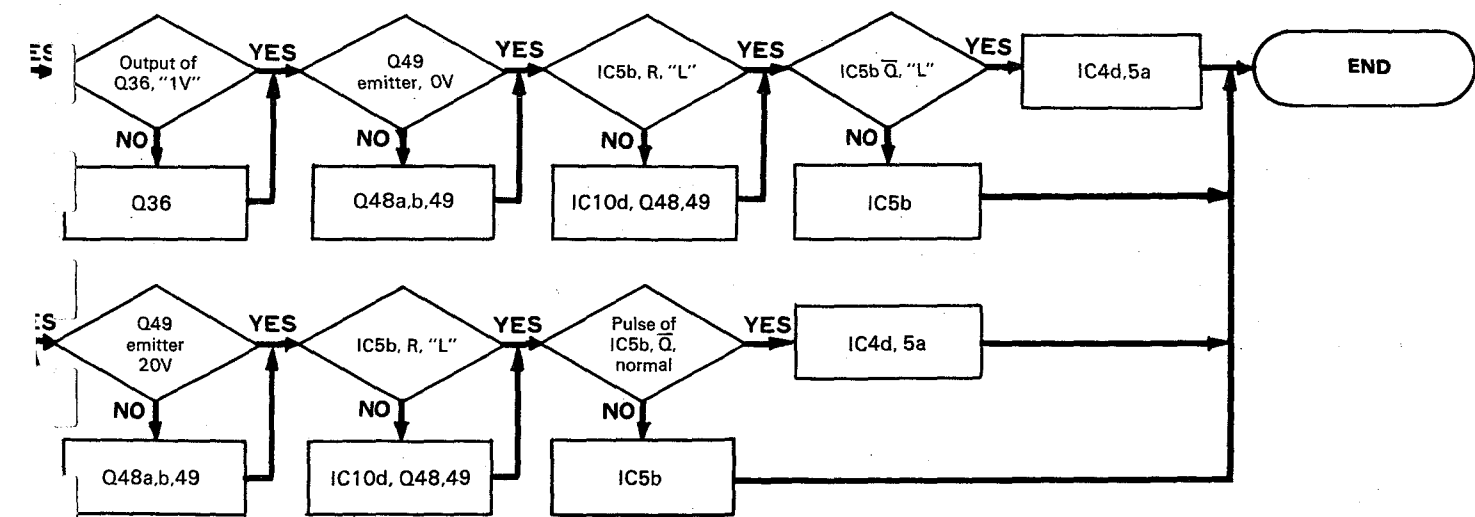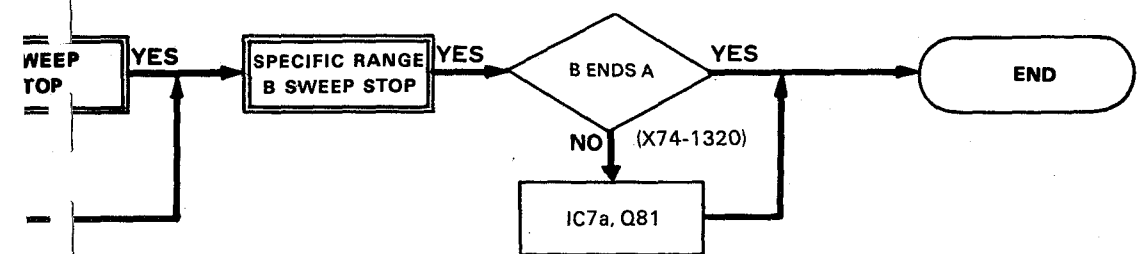
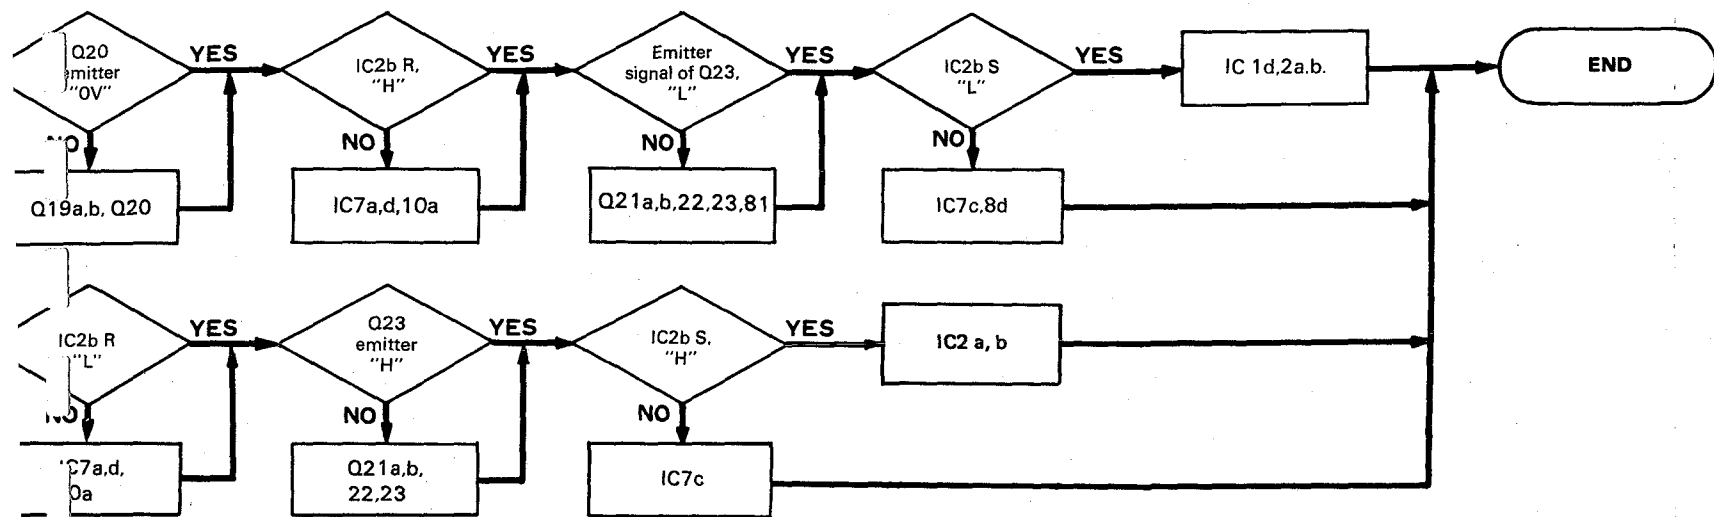


Waveform in Sweep circuit (X74-1320-01)
(Input signal 1 kHz, SWEEP TIME 1 ms/div)


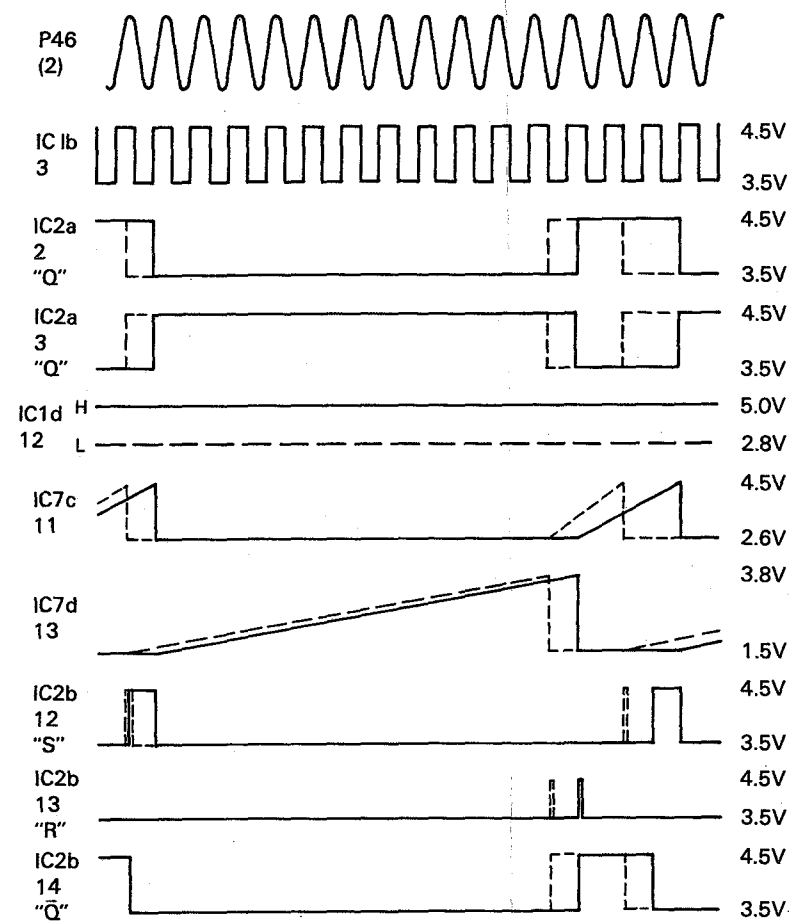


Broke-line auto free run
(at non-signal)






TROUBLESHOOTING

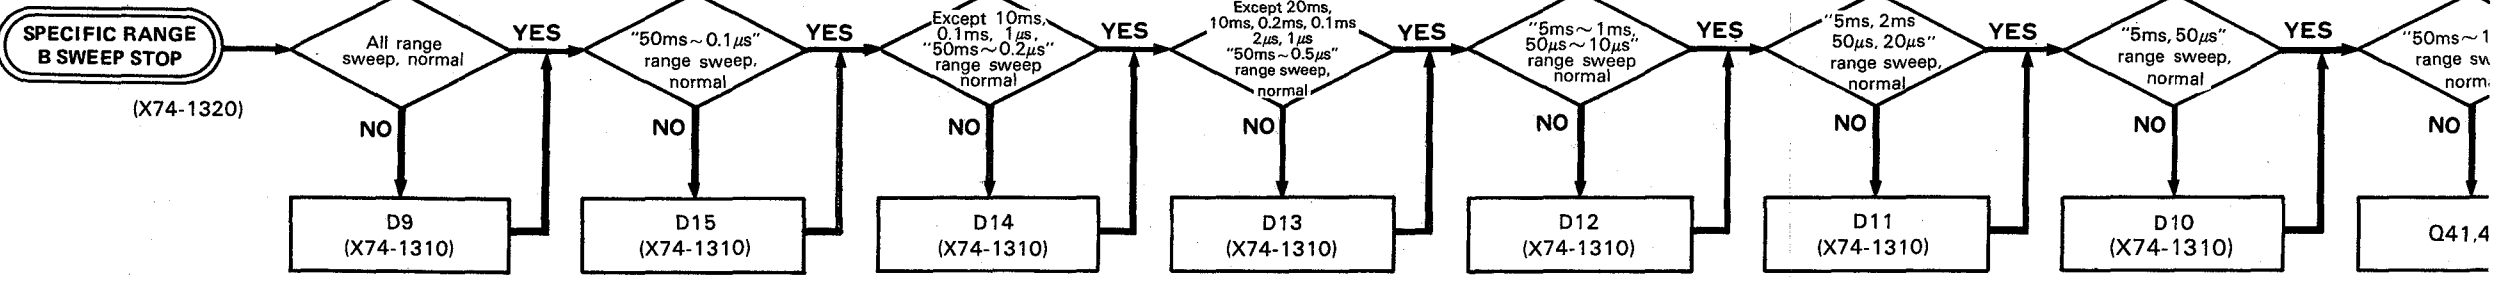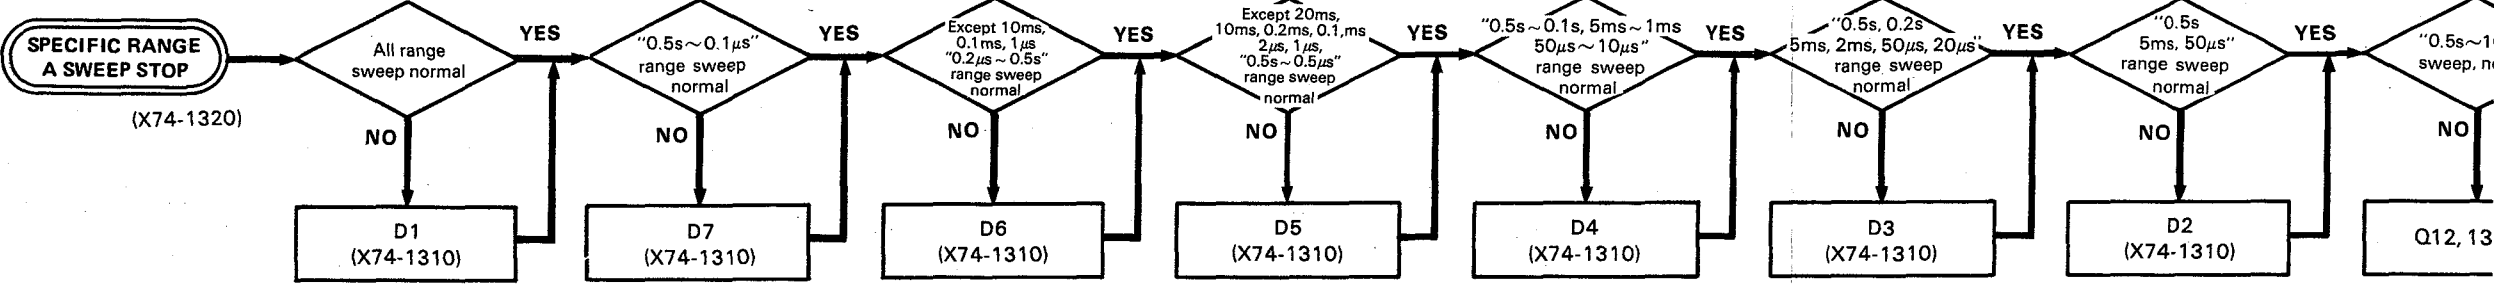

TROUBLESHOOTING

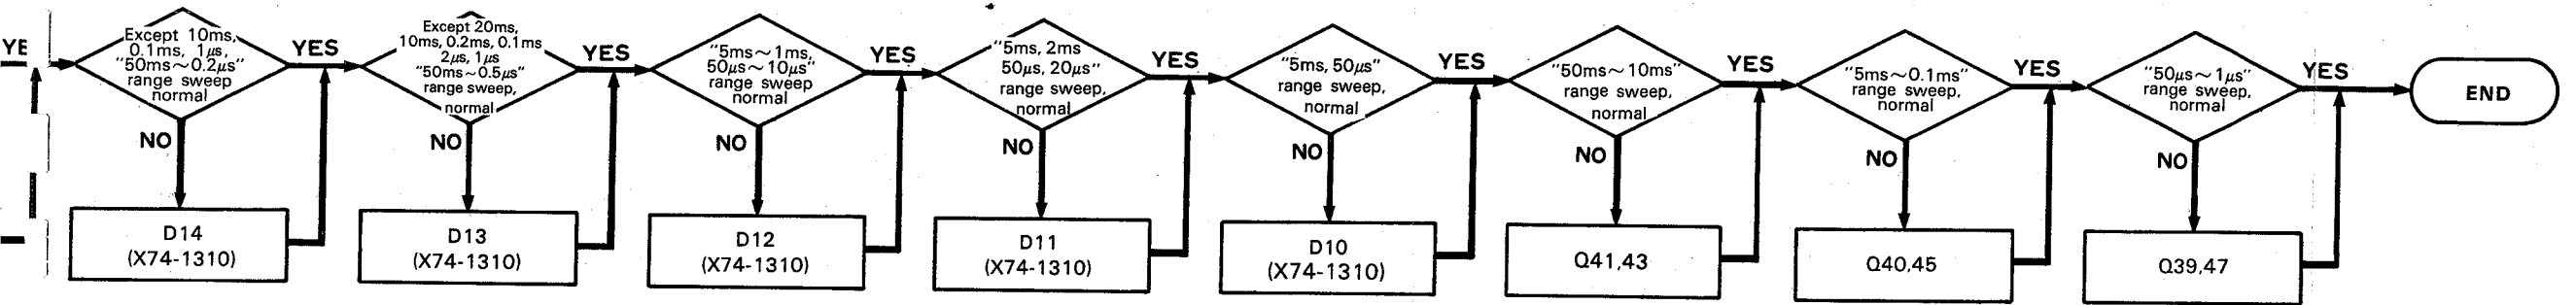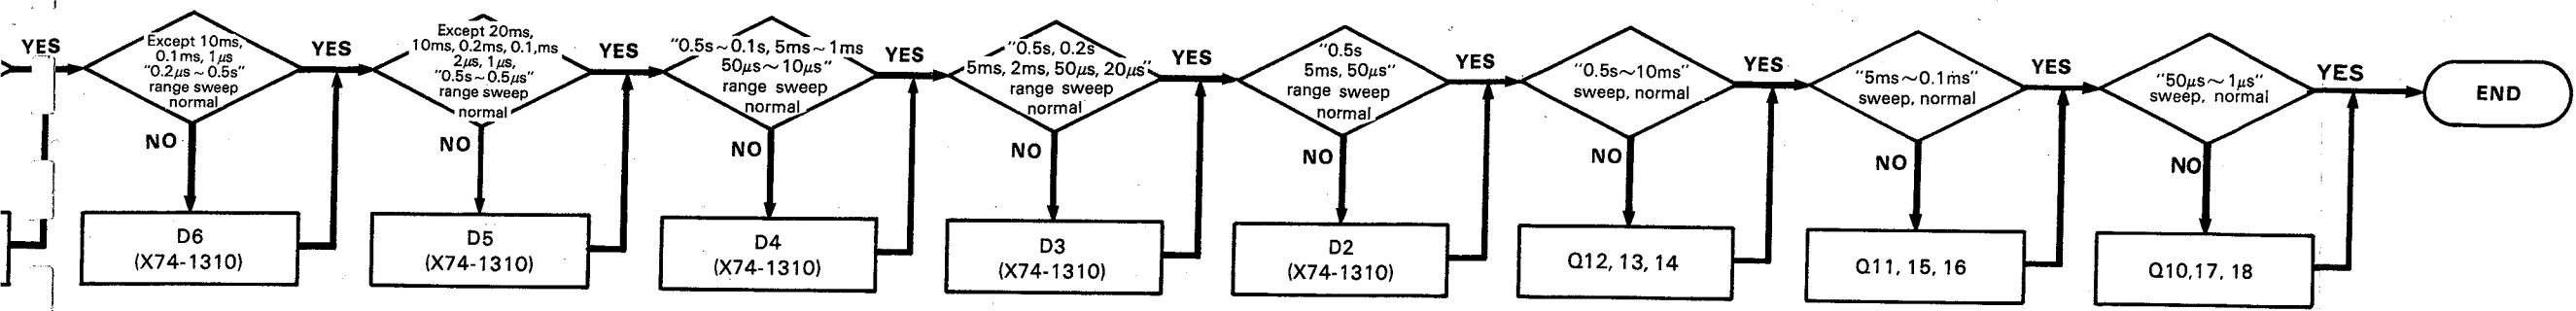

TROUBLESHOOTING

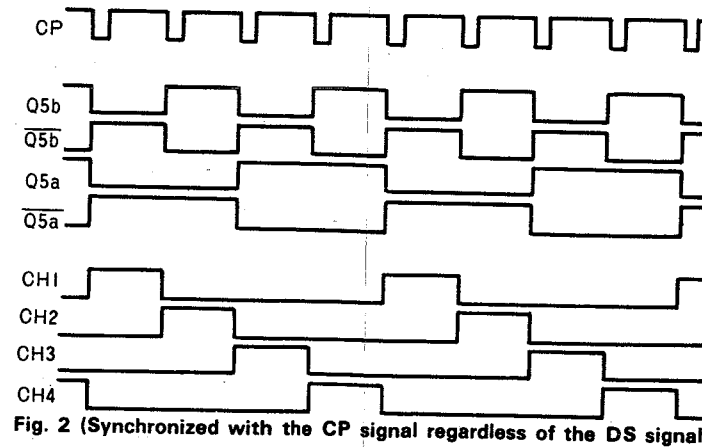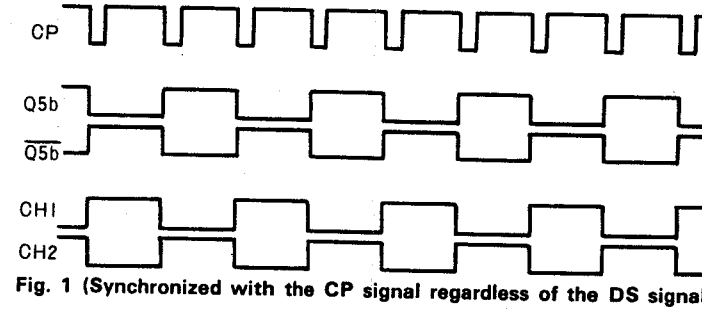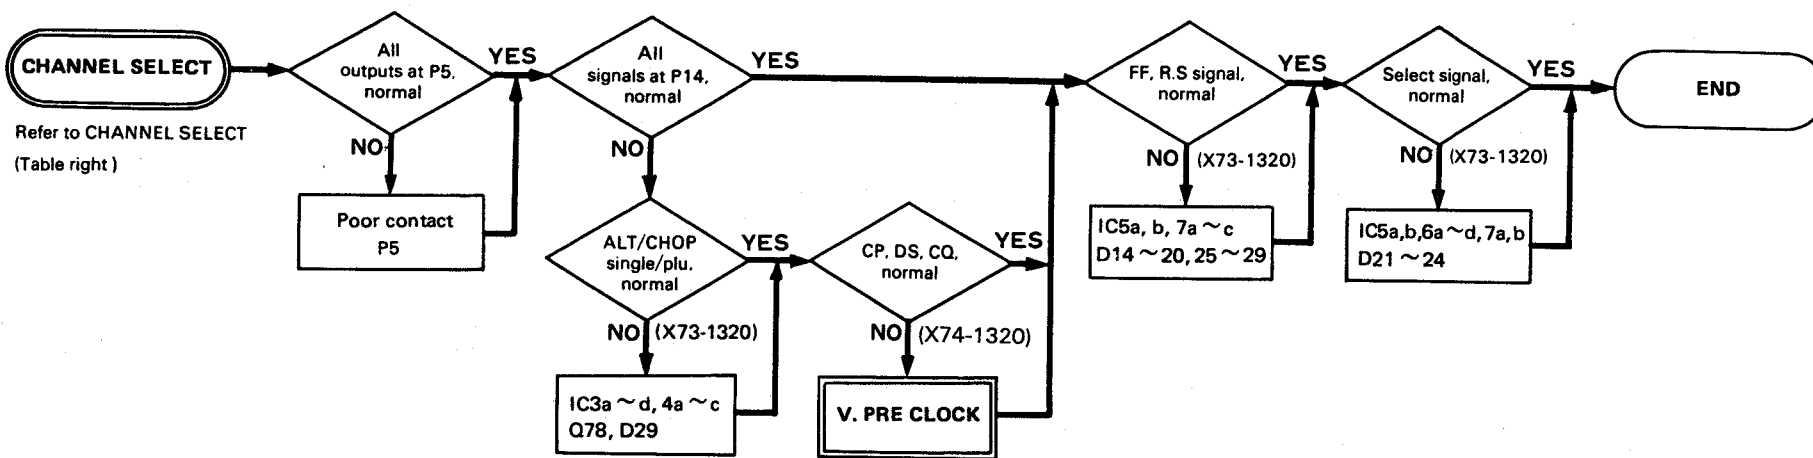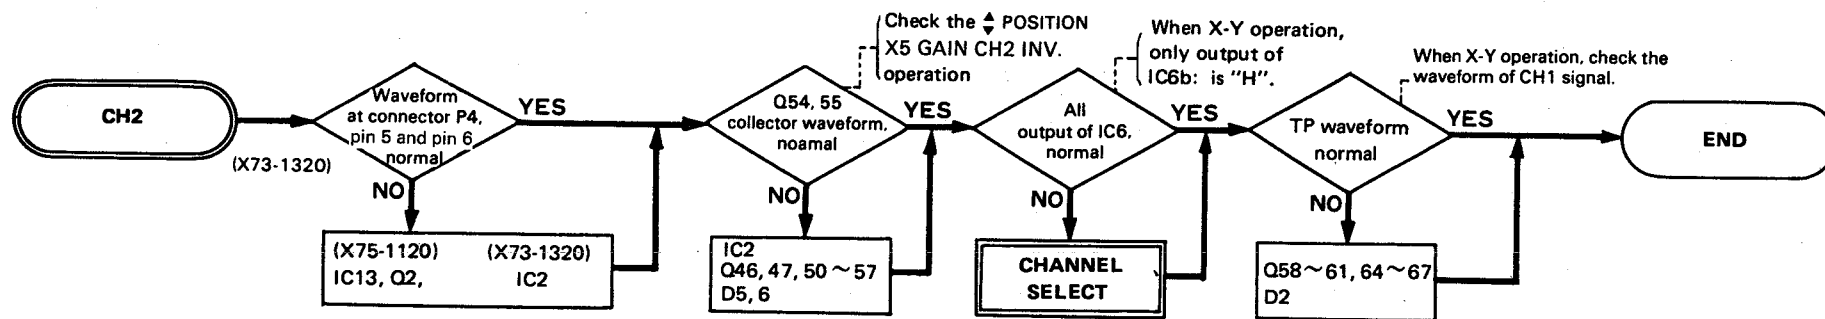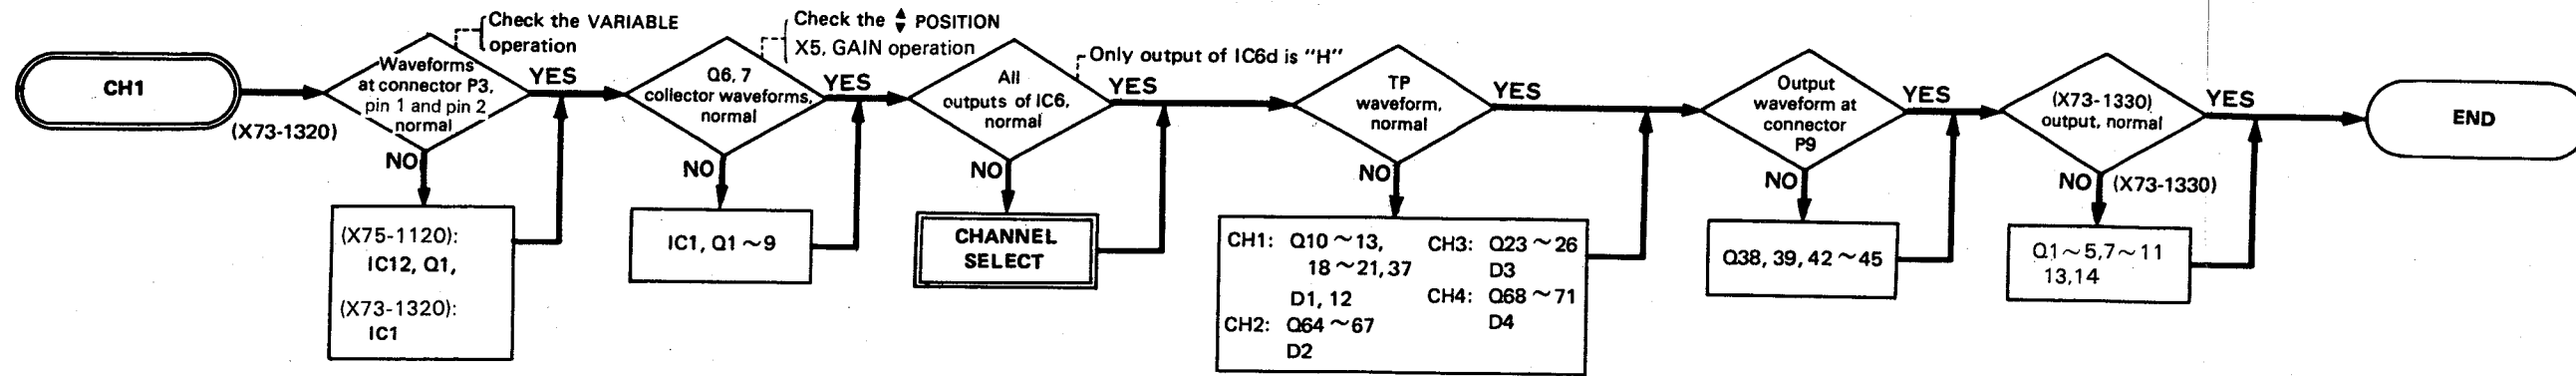

TROUBLESHOOTING

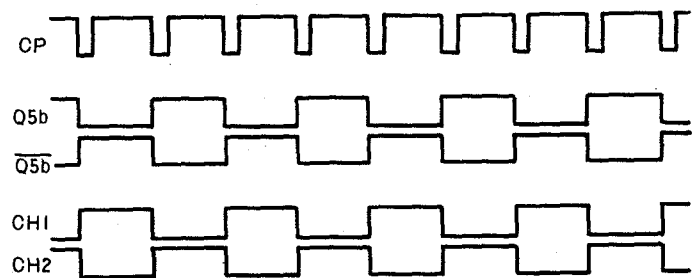
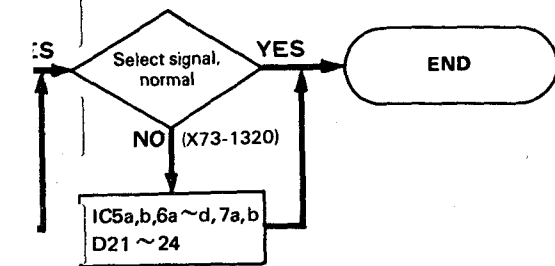
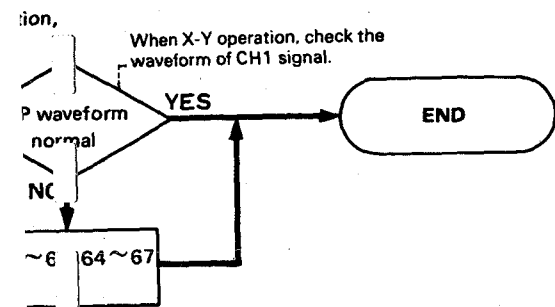
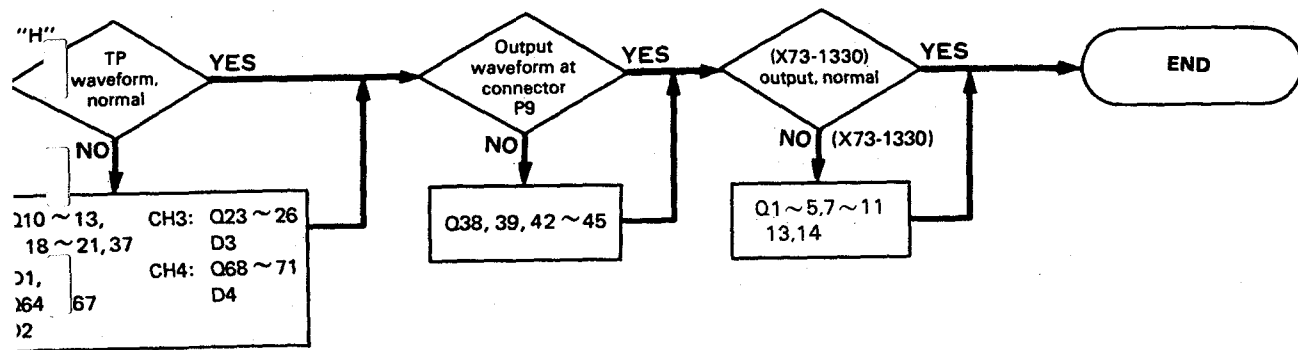


Fig. 1 (Synchronized with the CP signal regardless of the DS signal)

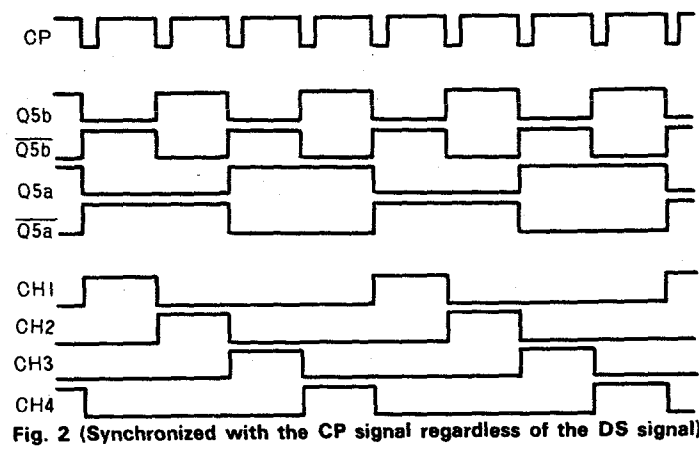






Fig. 2 (Synchronized with the CP signal regardless of the DS signal)

CHANNEL SELECT

SWEEP OPERATION		MODE INPUT LOG OUTPUT (P5) signal										VERTICAL CLOCK (P14)				FLIP-FLOP PRESET, CLEAR signal				FLIP-FLOP OUTPUT signal				CHANNEL SELECT signal			
		CHI	CH2	DU	ADD	ALT	ALT	Single	CP	DS	CO	R5b	S5b	R5a	Q5b	Q5b	Q5a	Q5a	CHI	CH2	CH3	CH4					
		AL	AL	ENOP	plu																						
Except the DUAL SWEEP	CHI	L	H	H	H	H	L	L	L	L	X	L	H	L	L	H	L	H	L	L	L						
	CH2	H	L	H	H	H	L	L	L	L	X	H	L	L	H	L	L	H	L	H	L	L					
	ADD	H	H	H	L	H	L	L	L	L	X	L	L	L	H	H	L	H	H	H	L	L					
	DUAL	ALT	H	H	L		L	L				L	H	H	L	TOGGLE	L	H	Fig1	L	L						
QUAD	CHOP	H	H		H	H	H	H				L	H	H													
	ALT			H		L	L								H	TOGGLE	TOGGLE				Fig2						
	CHOP				H	H																					
X-Y operation		X	X	X	X	X	X	H	H	L	L	L	H	L	L	H	L	H	H	L	L	L					

(Note) "X" H or L

TROUBLESHOOTING

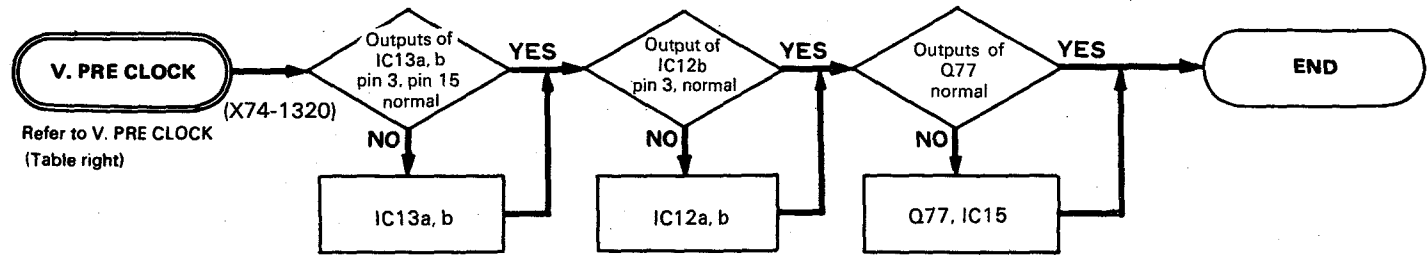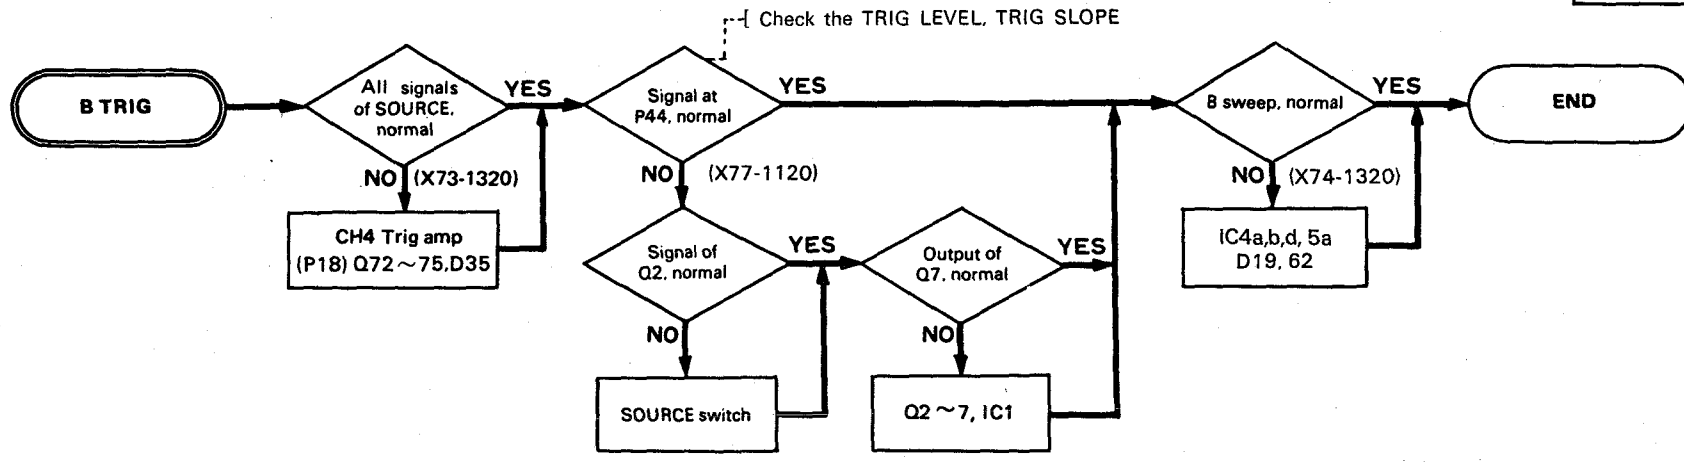
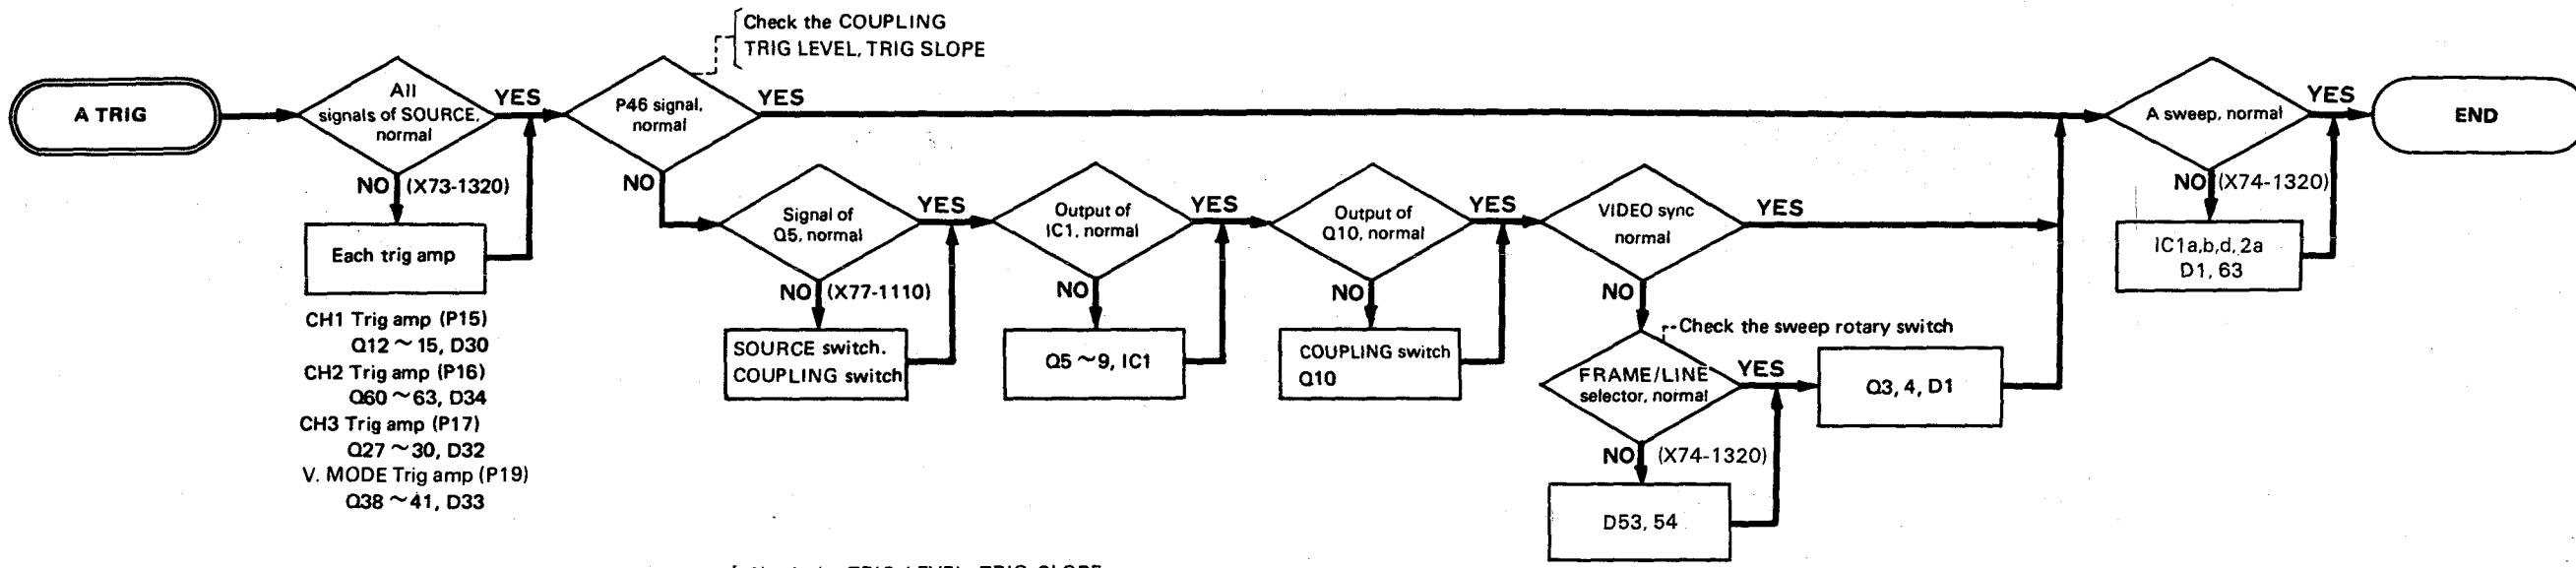
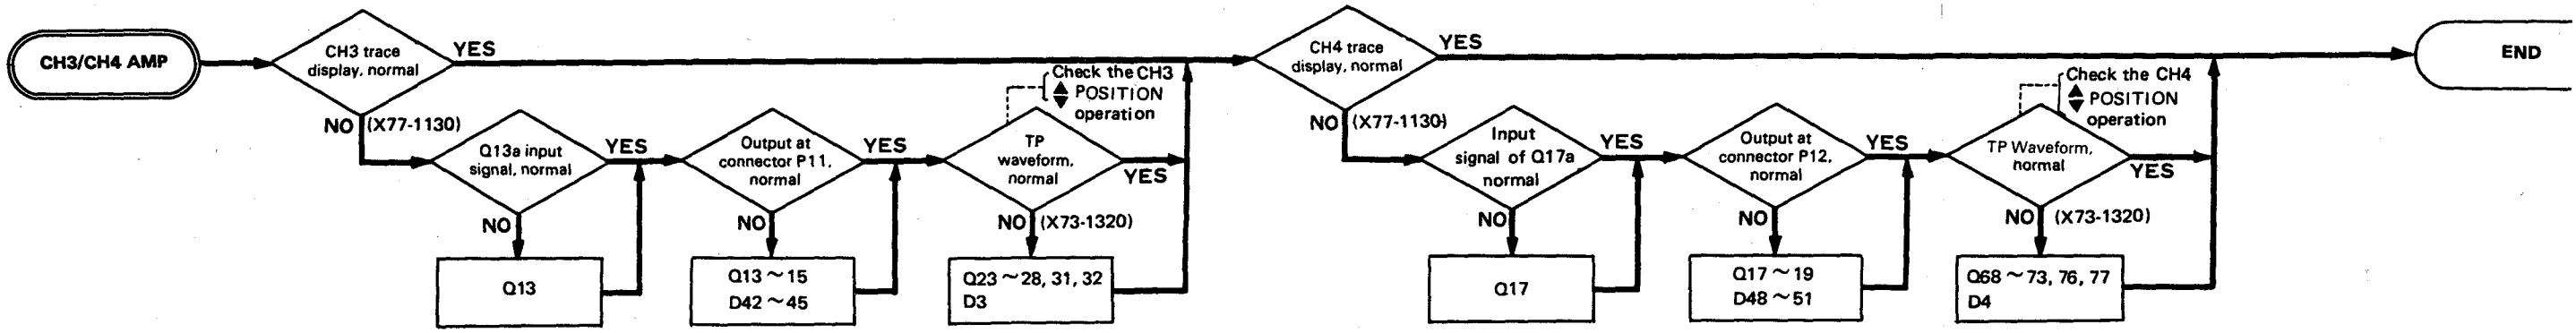


V. PRE CLOCK

MODE	INPUT		OUTPUT				DS*4	DISPLA		
	ALT	Single CHOP	IC14d	IC15a,b	IC15c,d	CP				
SWEEP Operation	CH1	L	L	H	Refer to the right table.	QA*1	QA*2	H	H.	
	CH2	L	L	H		QA*1	QA*2	H		
	DUAL	ALT	L	H		H	CHOP Osc.	CHOP Pulse	H	A
		CHOP	H	H		L	QA*1	QA*2	H	ALT
QUAD	ALT	L	H	H	CHOP Osc.	CHOP Pulse	H	A-INT-I		
	CHOP	H	H	L	CHOP Osc. *3	CHOP Pulse *3	H	B DLYI		
X-Y Operation	DUAL, ALT, QUAD, ALT, OTHER	L, H	H	DUAL, ALT, QUAD, ALT, OTHER	L, H			H	X-Y	

Each signal of IC16a, CP, DS vary by H. DISPLAY.

TROUBLESHOOTING

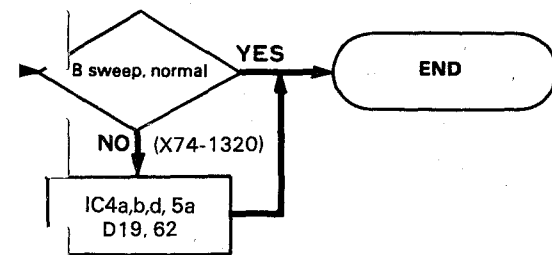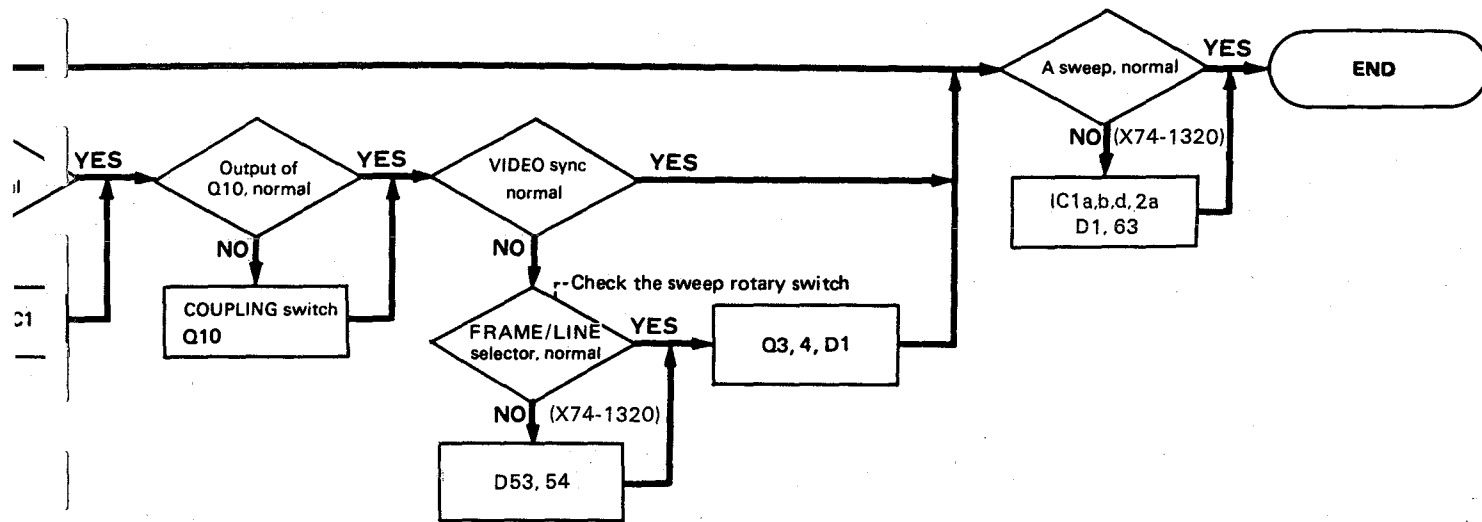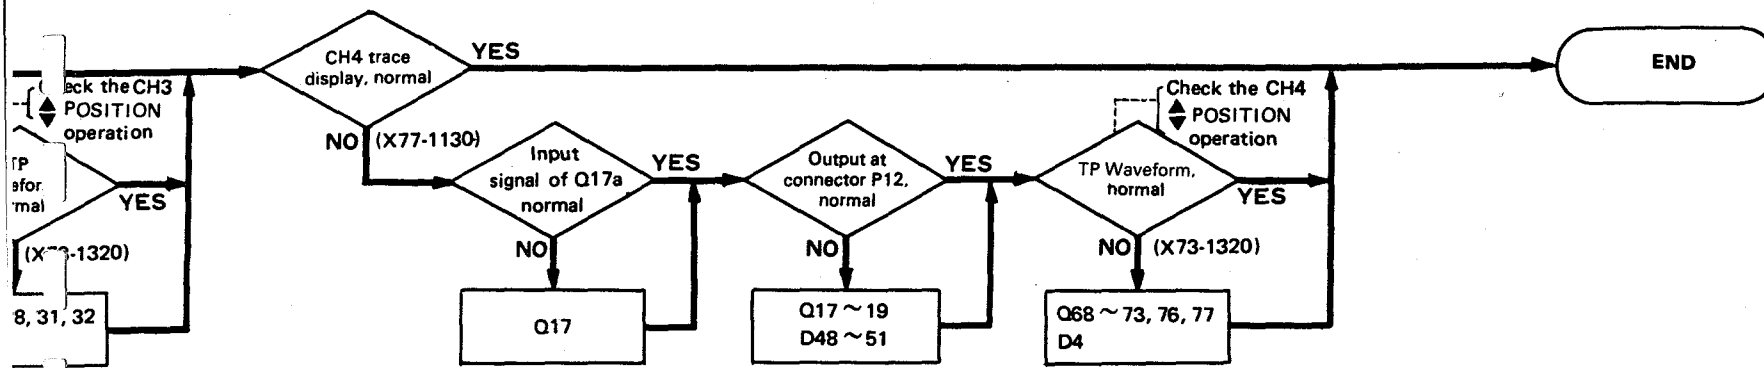

V. PRE CLOCK

	MODE	INPUT		OUTPUT					
		ALT	CHOP	Single PLU	IC14d	IC15a,b	IC15c,d	CP	DS*4
SWEEP Operation	CH1	L	L	H	Refer to the right table.	QA*1	QA*2	H	
	CH2	L	L	H		QA*1	QA*2	H	
	DUAL	ALT	L	H		H	QA*1	QA*2	H
		CHOP	H	H		L	CHOP Osc.	CHOP Pulse	H
	ADD	L	L	H		QA*1	QA*2	H	
	QUAD	ALT	L	H		H	QA*1	QA*2	H
		CHOP	H	H		L	CHOP Osc.	CHOP Pulse	H
	X-Y Operation	DUAL,ALT QUAD,ALT OTHER	L L H	H		DUAL,ALT QUAD,ALT OTHER	CHOP Osc. *3	CHOP Pulse *3	H


Each signal of IC16a, CP, DS vary by H. DISPLAY.

H. DISPLAY	IC15b Pin 7	IC15b Pin 6	IC15a, b OUTPUT	CQ	IC13a Q
DISPLAY	L	L	QA	L	H
A	L	L	QA	L	H
ALT	H	L	L	L	*5
A-INT-B	L	L	QA	L	H
B DLY'D	L	L	QA	L	L
X-Y	H	L	L	L	H

* 1. H. DISPLAY: ALT
CH1, CH2 ADD: L




H. DISPLAY: DUAL
CH1, CH2 ADD: QA



* 2. H. DISPLAY: ALT
CH1, CH2 ADD: H




H. DISPLAY: DUAL
CH1 CH2 ADD: QA




* 3. MODE: DUAL ALT, QUAD ALT: L

* 4. H. DISPLAY: DUAL



* 5. Waveform



PARTS LIST

Unless otherwise specified, all resistors are $\pm 5\%$, 1/6W and all capacitor's voltage ratings are 50WV.

The specifications and parts list and schematic diagram may be changed without notice owing to a technical innovation.


ABBREVIATIONS

Resistor	
RD	Carbon
RN	Metal film
RS	Metal film
RC	Solid
MG	Metal glaze
VR	Variable or semi-fixed
Capacitor	
CC	Ceramic
CK	Ceramic
CE	Electrolytic
CM	Mica
CQ	Mylar (Polypropylen)
TC	Ceramic trimmer
MF	Metal film
SCC	Semiconductor ceramic
Semiconductor	
TR	Transistor
FET	Field effect transistor

The part No. of each connector is stamped or color-coded. The color-coding is as follows.

Black	Brown	Red	Orange	Yellow	Green	Blue	Purple	Grey	White
0	1	2	3	4	5	6	7	8	9

[Example]

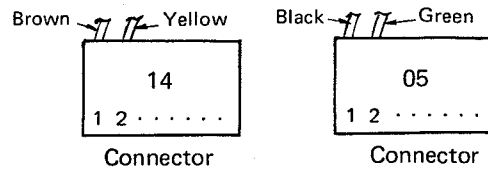

Each connector can be classified by the color of pin 1 and pin 2.

PARTS LIST


MAIN CHASSIS

Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.	
1-1		A13-0731-42	Frame		
1-2		A13-0732-12	Frame		
1-3		A20-2756-15	Die-casting panel		
1-4		A21-1006-04	Decorative panel		
1-5		A21-1007-04	Decorative panel		
1-6		A21-0884-04	Decorative panel		
1-7		A22-0817-33	Sub panel		
1-8		A23-1627-12	Rear panel		
1-9		A33-0501-14	Reflector		
1-10		D23-0801-04	Spacer		
1-11		F15-0720-04	Blind cover		
1-12		B19-0723-03	Filter		
1-13		B20-0921-04	Floating core		
1-14		B30-0903-15	LED		
1-15		E18-0351-05	Power connector		
1-16		E04-0251-05	BNC jack		
1-17		E21-0654-04	CAL terminal		
1-18		F10-1553-14	Shield plate for CH3		
1-19		E21-0657-04	GND terminal		
1-20		E29-0504-05	Teflon terminal		
1-21		F10-1557-04	Eearth band		
1-22		E23-0513-05	Earth lug		
1-23		E23-0520-05	Earth lug		
1-24		F05-1224-05	Fuse 1.2A		
1-25		F15-0138-04	Felt		
1-26		F15-0716-14	Spacer		
1-27		E23-0522-14	Earth plate		
1-28		J13-0038-05	Fuse holder		
1-29		J19-1624-04	Stopper		
1-30		J21-2927-04	Ring-antirun		
1-31		J21-2871-14	Bracket (For D.L.)		
1-32		J29-0505-04	Retainer clamp		
1-33		J39-0506-04	Spacer		
1-34		J42-0512-04	Mounting rubber (For CRT)		
1-35		J42-0513-04	Mounting rubber (For CRT)		
1-36		J42-0514-04	Mounting rubber (For lamp)		
1-37		J61-0511-05	Wire saddle		
1-38		K21-0819-03	Knob		
1-39		K21-0821-14	Knob		
1-40		K21-0831-24	Knob		
1-41		K21-0832-14	Knob		
1-42		K21-0833-14	Knob		
1-43		K21-0837-24	Knob		
1-44		K21-0838-03	Knob		
1-45		K27-0526-04	Lever knob		
1-46		L76-0104-05	Delay line		
1-47	S29	S31-2004-05	Slide switch		
1-48			Power thermister 4W-25V		
1-49	VR1	R01-1507-05	Variable resistor 3 kΩB		
	VR2	R01-1507-05	Variable resistor 3 kΩB		
1-50	VR4a	R06-2502-05	Variable resistor 5 kΩB		
	VR4b	R06-2502-05	Variable resistor 5 kΩB		
1-51	VR3a	R23-2501-05	Variable resistor 5 kΩB		
	VR3b	R23-2501-05	Variable resistor 5 kΩB		
1-52	VR5	R29-0504-05	Potential meter 1 kΩB		
1-53		002-0006-05	Shield gasket		
1-54		N08-0609-04	Post (Hex)		
1-55		N10-2030-41	Nut (Hex) M3		
1-56		N10-2060-46	Nut (Hex) M6		
1-57		N14-0602-34	Nut		
1-58		N14-0609-04	Nut		
1-59					
1-60		N16-0030-46	Lockwasher (For M3)		
1-61		N17-1030-41	Lockwasher (For M3)		
1-62					
1-63		N19-0702-04	Flat washer		


PARTS LIST

DISASSEMBLY

Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
1-64		N19-0704-04	Flat washer	
1-65				
1-66		N30-3006-46	Pan-head screw M3 × 6	
1-67		N30-3008-41	Pan-head screw M3 × 8	
1-68		N32-2606-46	Flat-head screw M2.6 × 6	
1-69		N32-3006-46	Flat-head screw M3 × 6	
1-70		N89-3006-46	Screw (Tapping) 3 × 6	
1-71		N89-3008-46	Screw (Tapping) 3 × 8	
1-72		N89-3010-46	Screw (Tapping) 3 × 10	
1-73		N09-0707-05	Flat-head screw (Tapping) (3 × 18)	
1-74		W02-0407-05	High voltage block	
1-75		W02-0405-15	Switching power block	
1-76		X68-1310-01	Power blanking unit	
1-77		R03-3502-15	Variable resistor 10 kΩB	
1-78		R05-8001-05	Variable resistor 3 MΩB	
1-79		R23-1501-05	Variable resistor 1 kΩB	
1-80		F02-0503-04	Heat sink	
1-81		J21-2930-04	Bracket (For VR)	
1-82		N09-0078-05	Screw M3 × 6 (Plastic)	
1-83		X73-1320-01	Vertical pre amp unit	
1-84		X73-1330-01	Vertical output unit	
1-85		F02-0501-04	Heat sink	
1-86		X74-1320-01	Trig sweep unit	
1-87		X74-1230-01	Horizontal output amp unit	
1-88		F01-0827-04	Heat sink	
1-89		X74-1310-01	Sweep rotary unit	
1-90		S02-2504-15	Rotary switch	
1-91		X75-1120-01	Vertical ATT unit	
1-92		X77-1110-01	A trig switch unit	
1-93		S33-2501-05	Lever switch	
1-94		S32-4008-05	Lever switch	
1-95		R01-2516-05	Variable resistor 5 kΩB	
1-96		X77-1120-01	B trig switch unit	
1-97		S37-2005-05	Lever switch	
1-98		R01-2515-05	Variable resistor 5 kΩB	
1-99		X77-1130-01	Horizontal mode control unit	
1-100		J25-2900-03	Printed circuit board	
1-101		K27-0524-14	Push knob	
1-102	S10	S40-1504-05	Tact switch	
	S11	S40-1504-05	Tact switch	
	S12	S40-1504-05	Tact switch	
	S13	S40-1504-05	Tact switch	
	S15	S40-1504-05	Tact switch	
	S16	S40-1504-05	Tact switch	
	S17	S40-1504-05	Tact switch	
	S18	S40-1504-05	Tact switch	
	S19	S40-1504-05	Tact switch	
1-103		J25-2902-03	Printed circuit board	
1-104		G01-0906-14	Spring	
1-105		J39-0509-04	Supporter for P.C.B.	
1-106			LED K-14LN322GP	
1-107		F11-0963-03	Shield case	

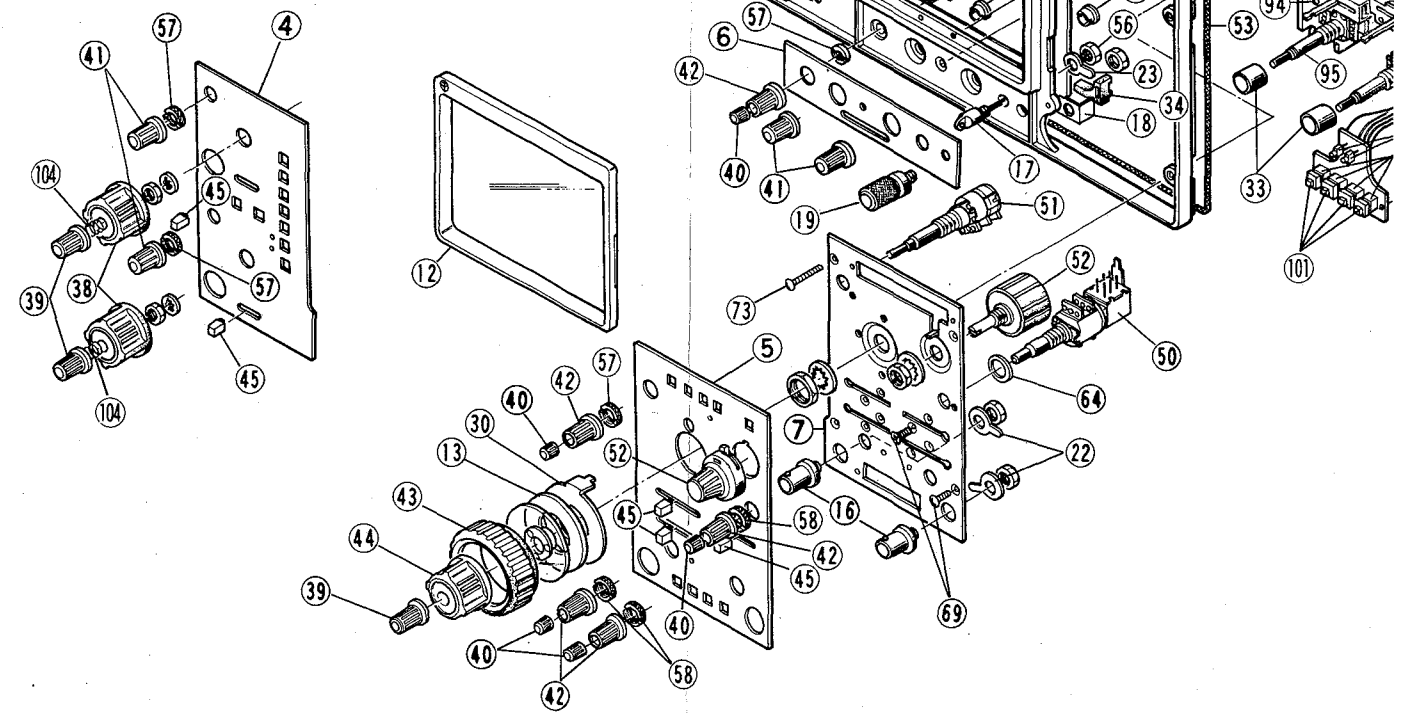

DISASSEMBLY

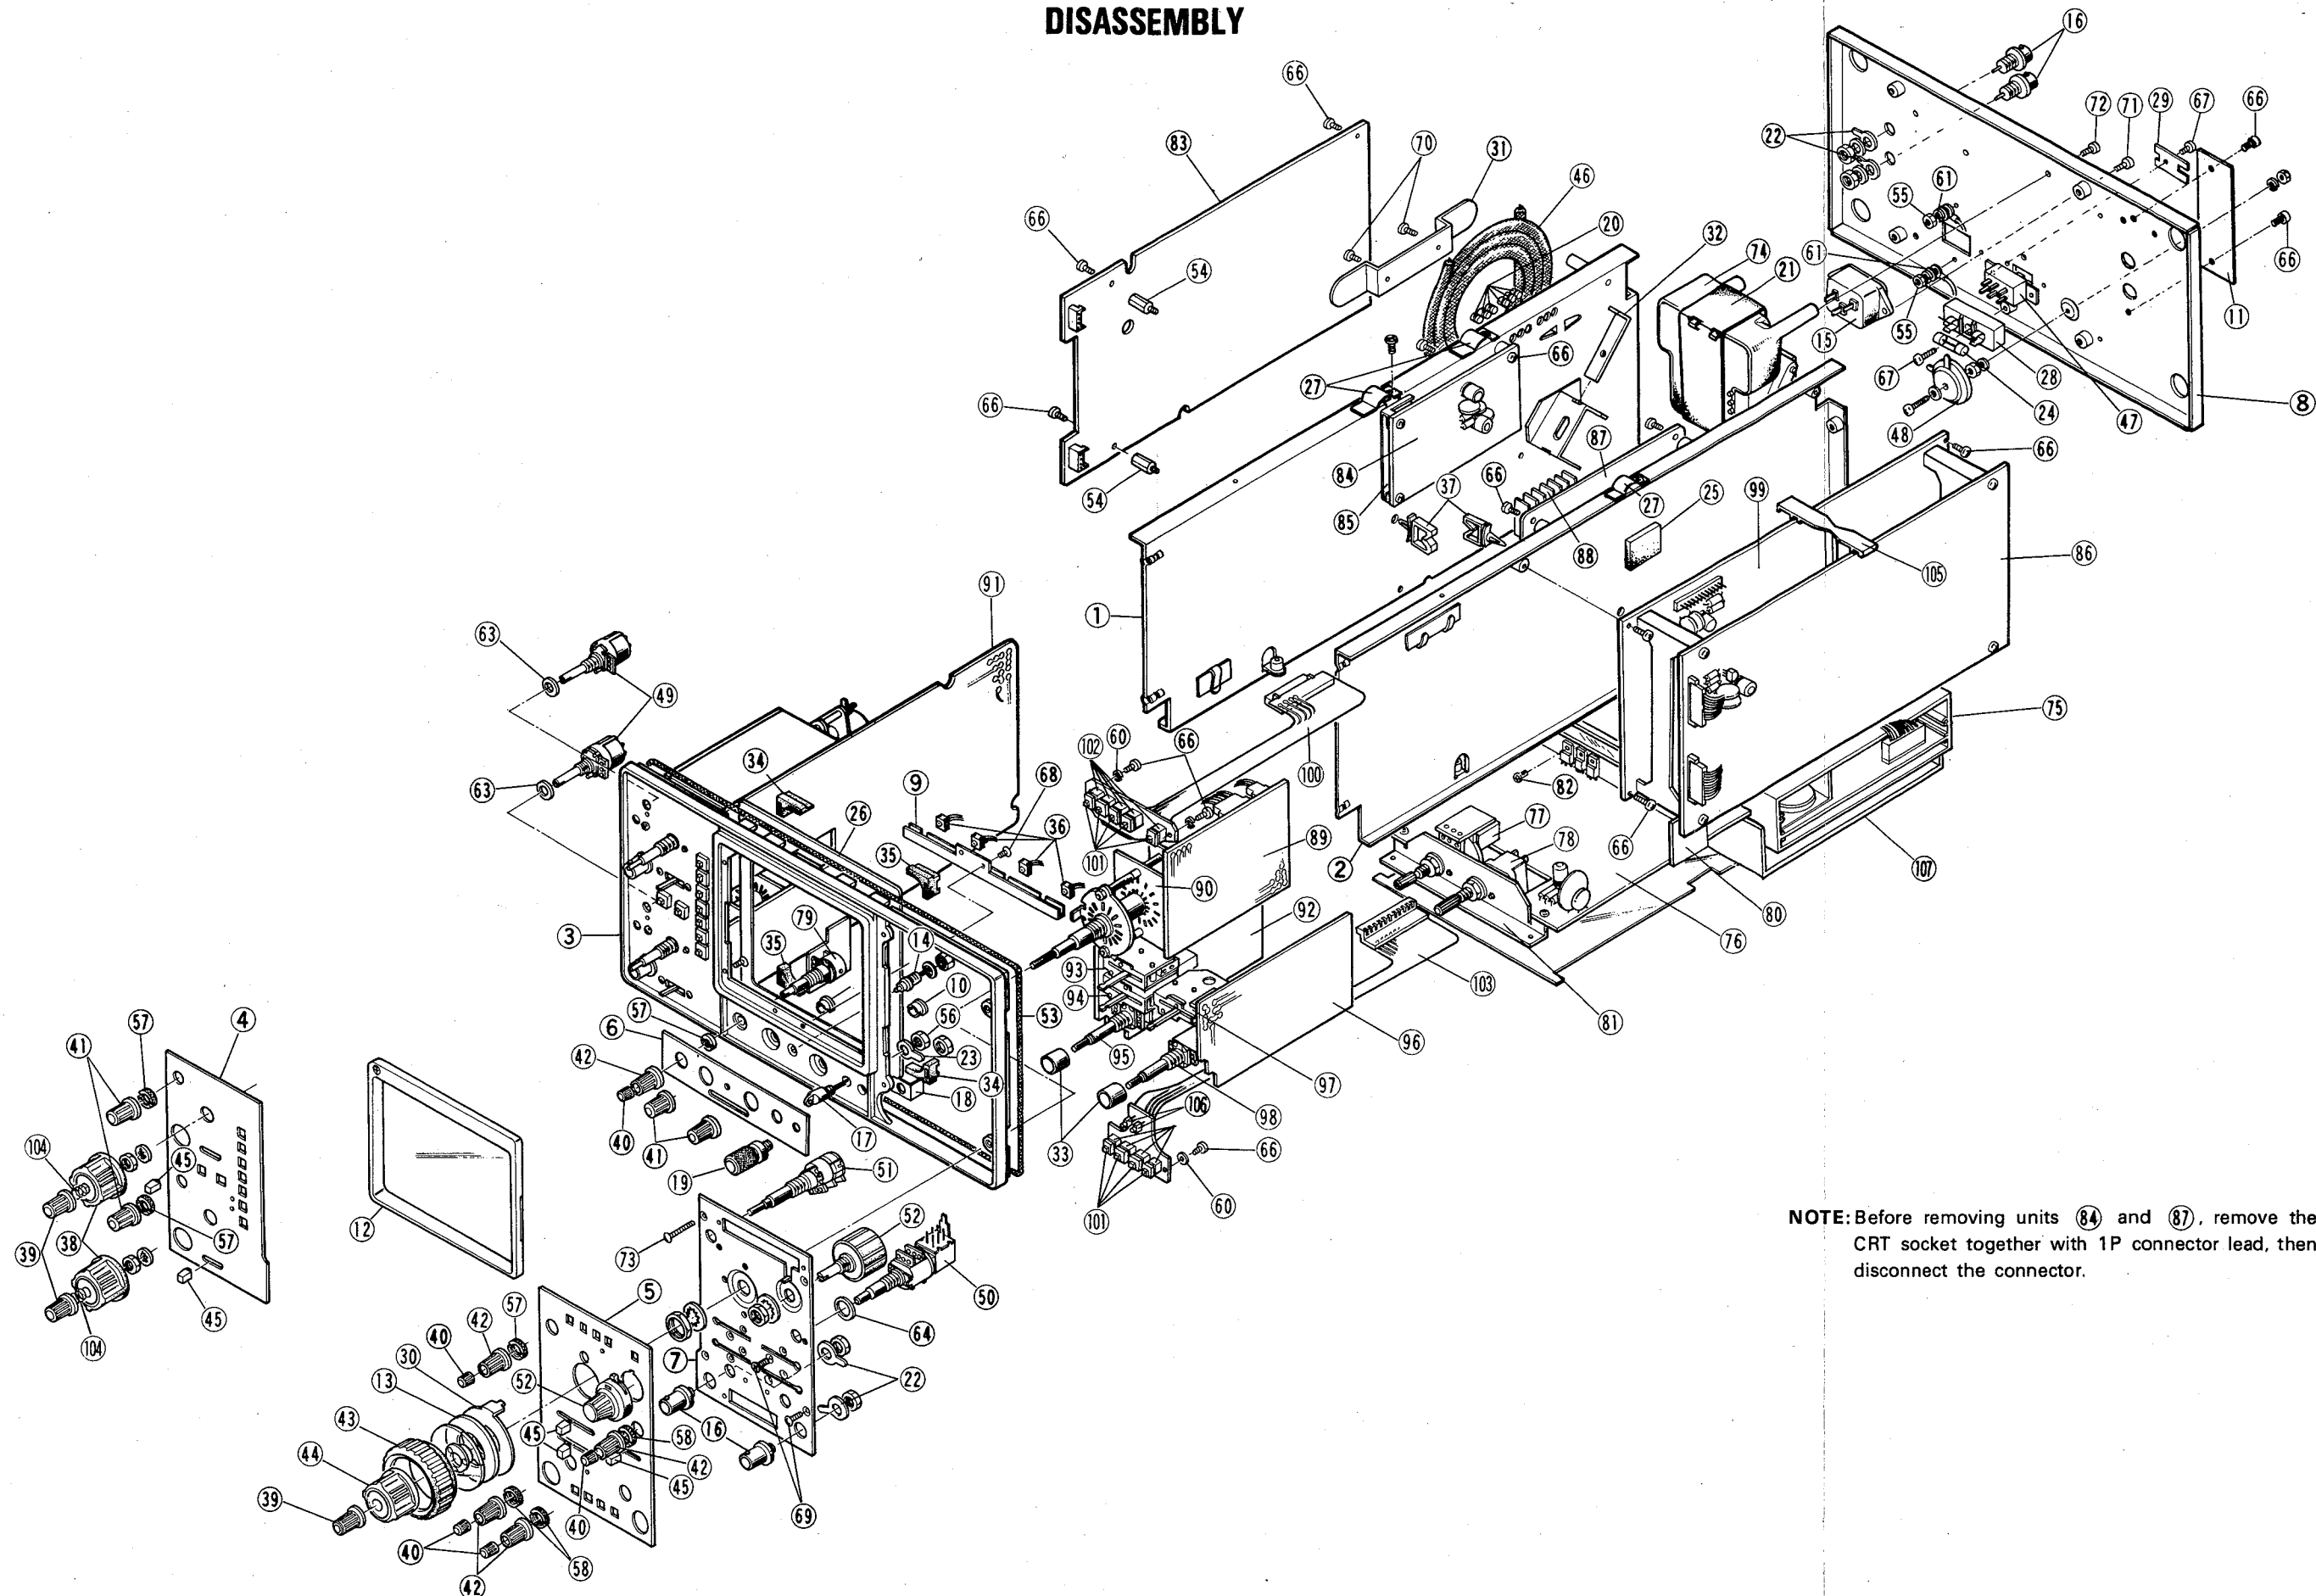

NOTE: Before removing units ⑧④ and ⑧⑦, remove the CRT socket together with 1P connector lead, then disconnect the connector.

PARTS LIST


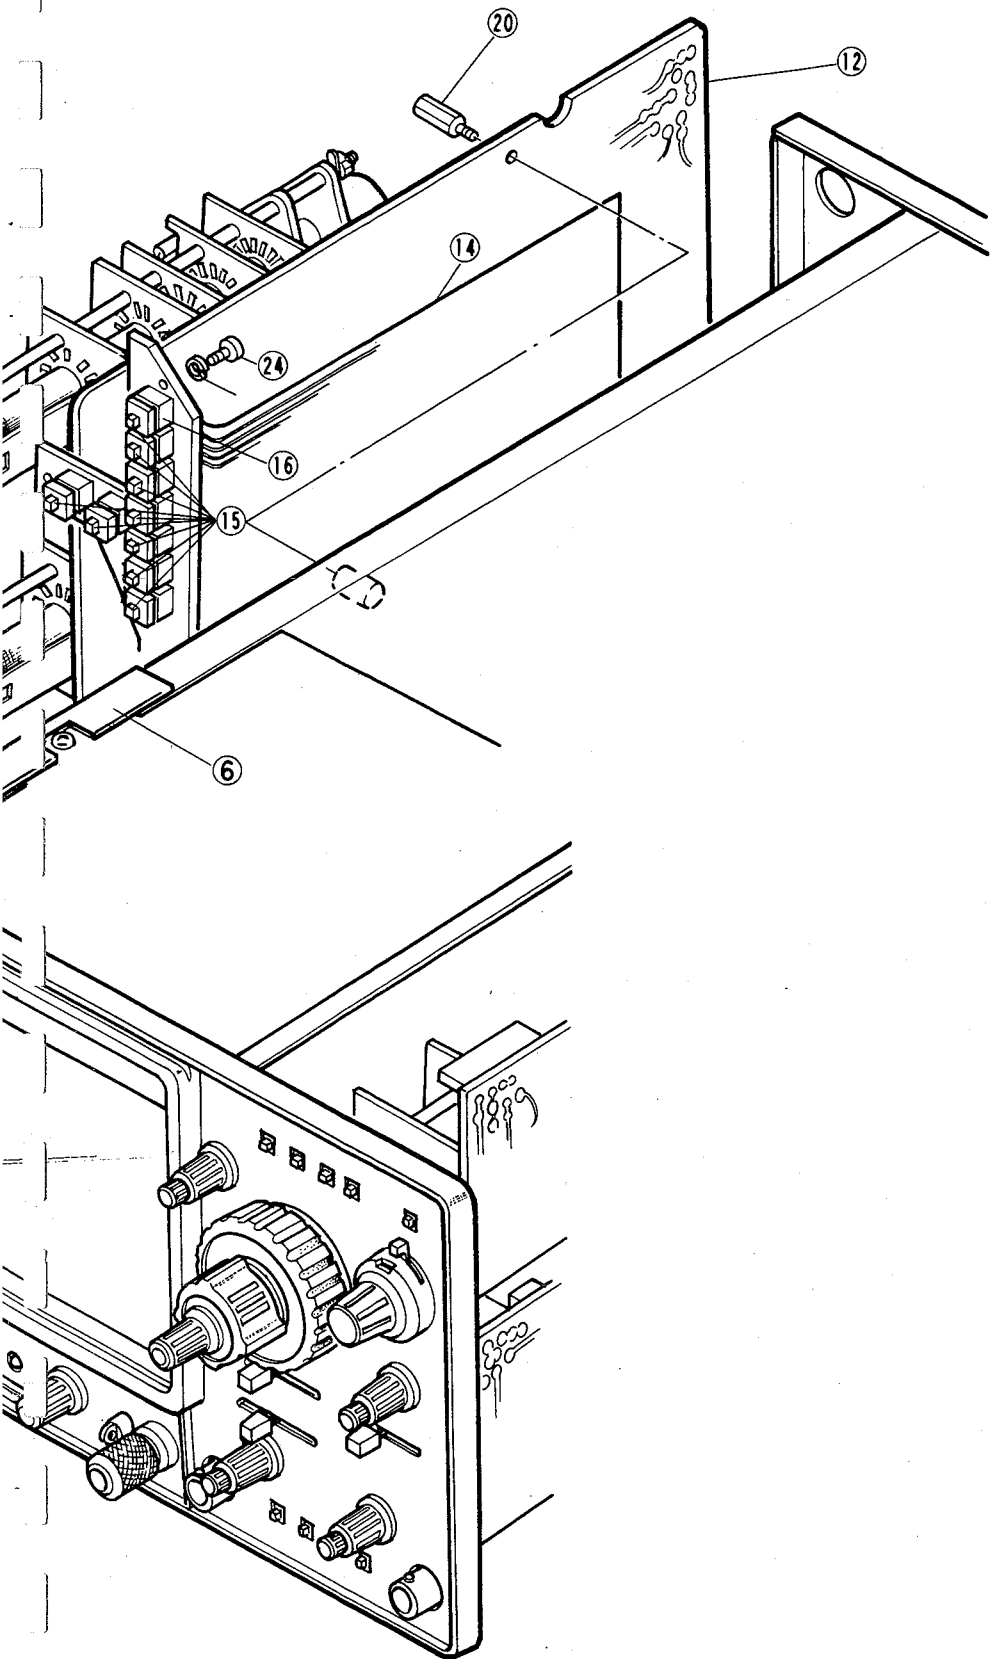


Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
2-1		A22-0823-03	Sub panel	
2-2		E04-0251-05	BNC jack	
2-3		E23-0519-04	Earth lug	
2-4		No use		
2-5	S25	S31-2506-05	Slide switch	
	S26	S31-2506-05	Slide switch	
2-6		G13-0714-04	Cushion	
2-7		E23-0521-04	Earth terminal	
2-8		F11-0961-04	Shield case	
2-9		F11-0964-04	Shield case	
2-10		F11-0965-04	Shield case	
2-11		F11-0966-04	Shield case	
2-12		X75-1120-01	Vertical ATT unit	
2-13		S01-4503-05	Rotary switch	
2-14		J25-2898-03	Printed circuit board	
2-15		K27-0524-14	Push knob	
2-16	S1	S40-1504-05	Tact switch	
	S2	S40-1504-05	Tact switch	
	S3	S40-1504-05	Tact switch	
	S4	S40-1504-05	Tact switch	
	S5	S40-1504-05	Tact switch	
	S6	S40-1504-05	Tact switch	
	S7	S40-1504-05	Tact switch	
	S8	S40-1504-05	Tact switch	
	S9	S40-1504-05	Tact switch	
2-17		No use		
2-18		No use		
2-19		No use		
2-20		N08-0609-04	Post (Hex)	
2-21		N16-0026-46	Lockwasher	
2-22		N16-0030-46	Lockwasher	
2-23		N30-2604-46	Pan-head screw M2.6 x 4	
2-24		N30-3006-46	Pan-head screw M3 x 6	
2-25		N32-2004-46	Flat-head screw M2 x 4	
2-26		N32-3006-46	Flat-head screw M3 x 6	
2-27		N09-0707-05	Flat-head screw (Tapping) 3 x 18	


PARTS LIST

DISASSEMBL

Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
3-1		E01-1403-05	CRT socket	
3-2		E31-0564-05	Leadwire with connector	
3-3		F11-0976-02	CRT shield	
3-4		F11-0975-03	CRT shield	
3-5		G13-0715-04	Cable retainer	
3-6		G16-0602-04	Reflector sheet	
3-7		G16-0603-04	Reflector sheet	
3-8		J19-1623-04	CRT band	
3-9		J21-2925-03	Bracket (For CRT)	
3-10		J21-2926-03	Bracket (For CRT)	
3-11			CRT, 15OCTM31	
3-12		L39-0515-05	Rotator coil	
3-13		G13-0714-04	Cushion	
3-14		N15-1030-41	Lockwasher	
3-15		N16-0030-46	Lockwasher	
3-16		N30-3035-46	Pan-head screw 3 x 35	
3-17		N30-3008-46	Pan-head screw M4 x 8	
3-18		N89-3006-46	Screw (Tapping) 3 x 6	
3-19		N89-3010-41	Screw (Tapping) 3 x 10	

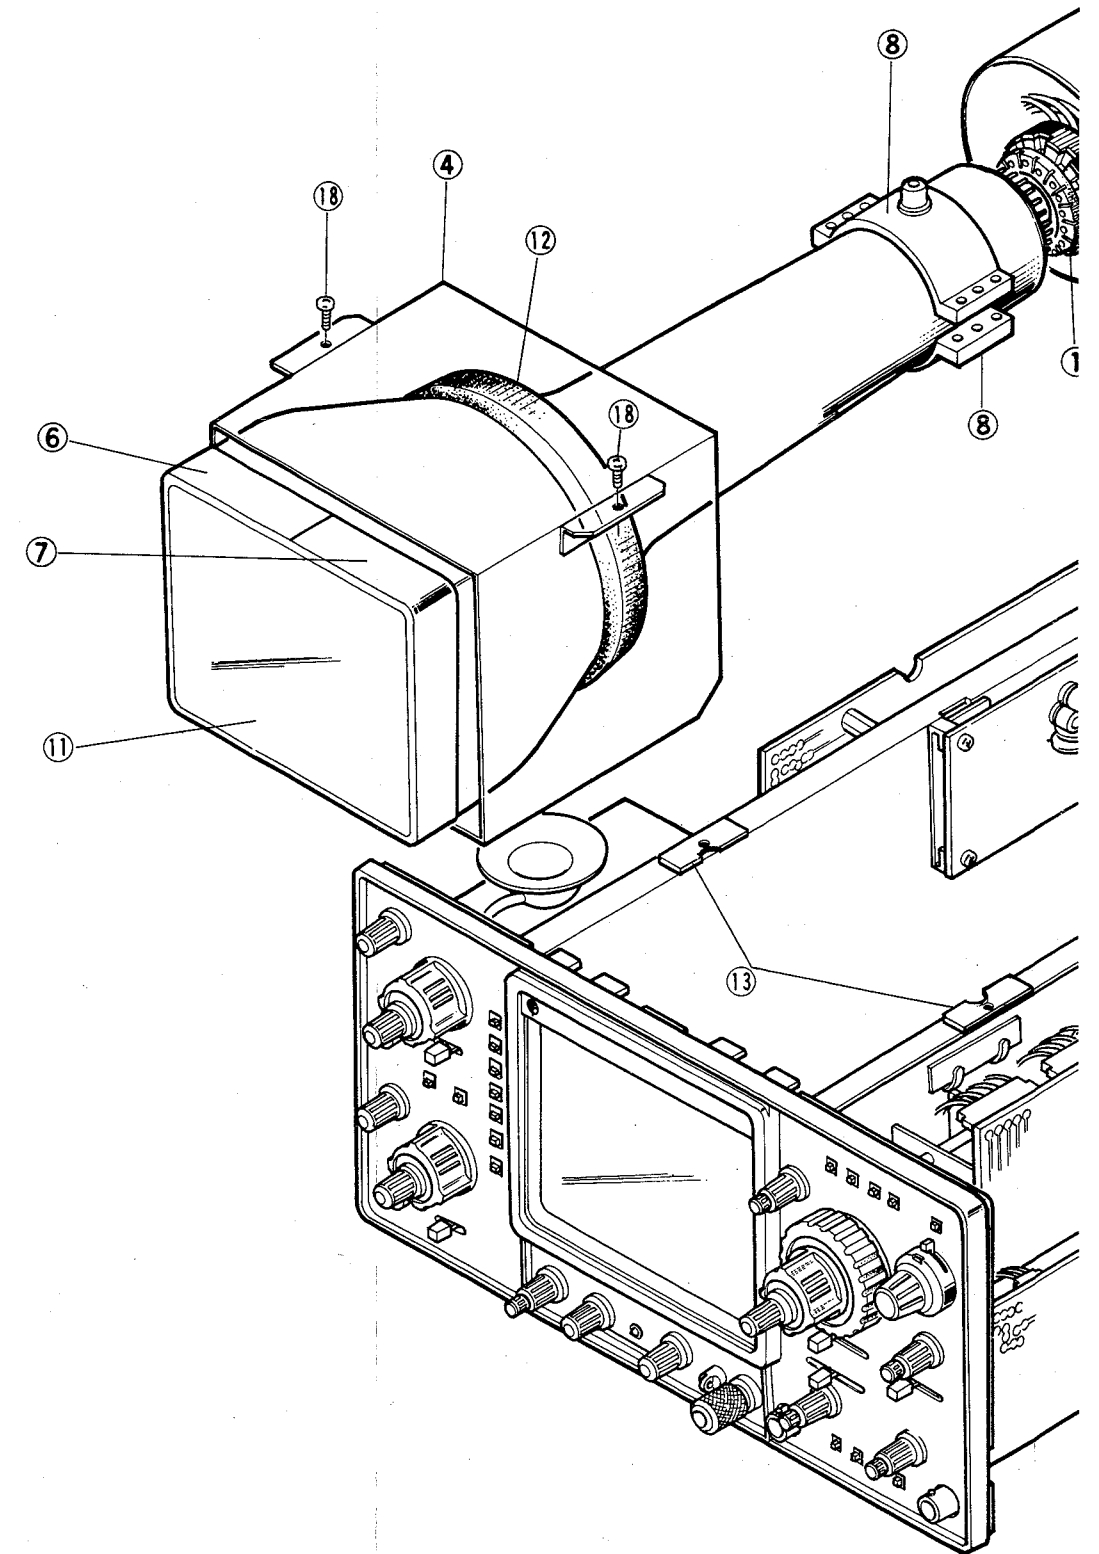

DISASSEMBLY

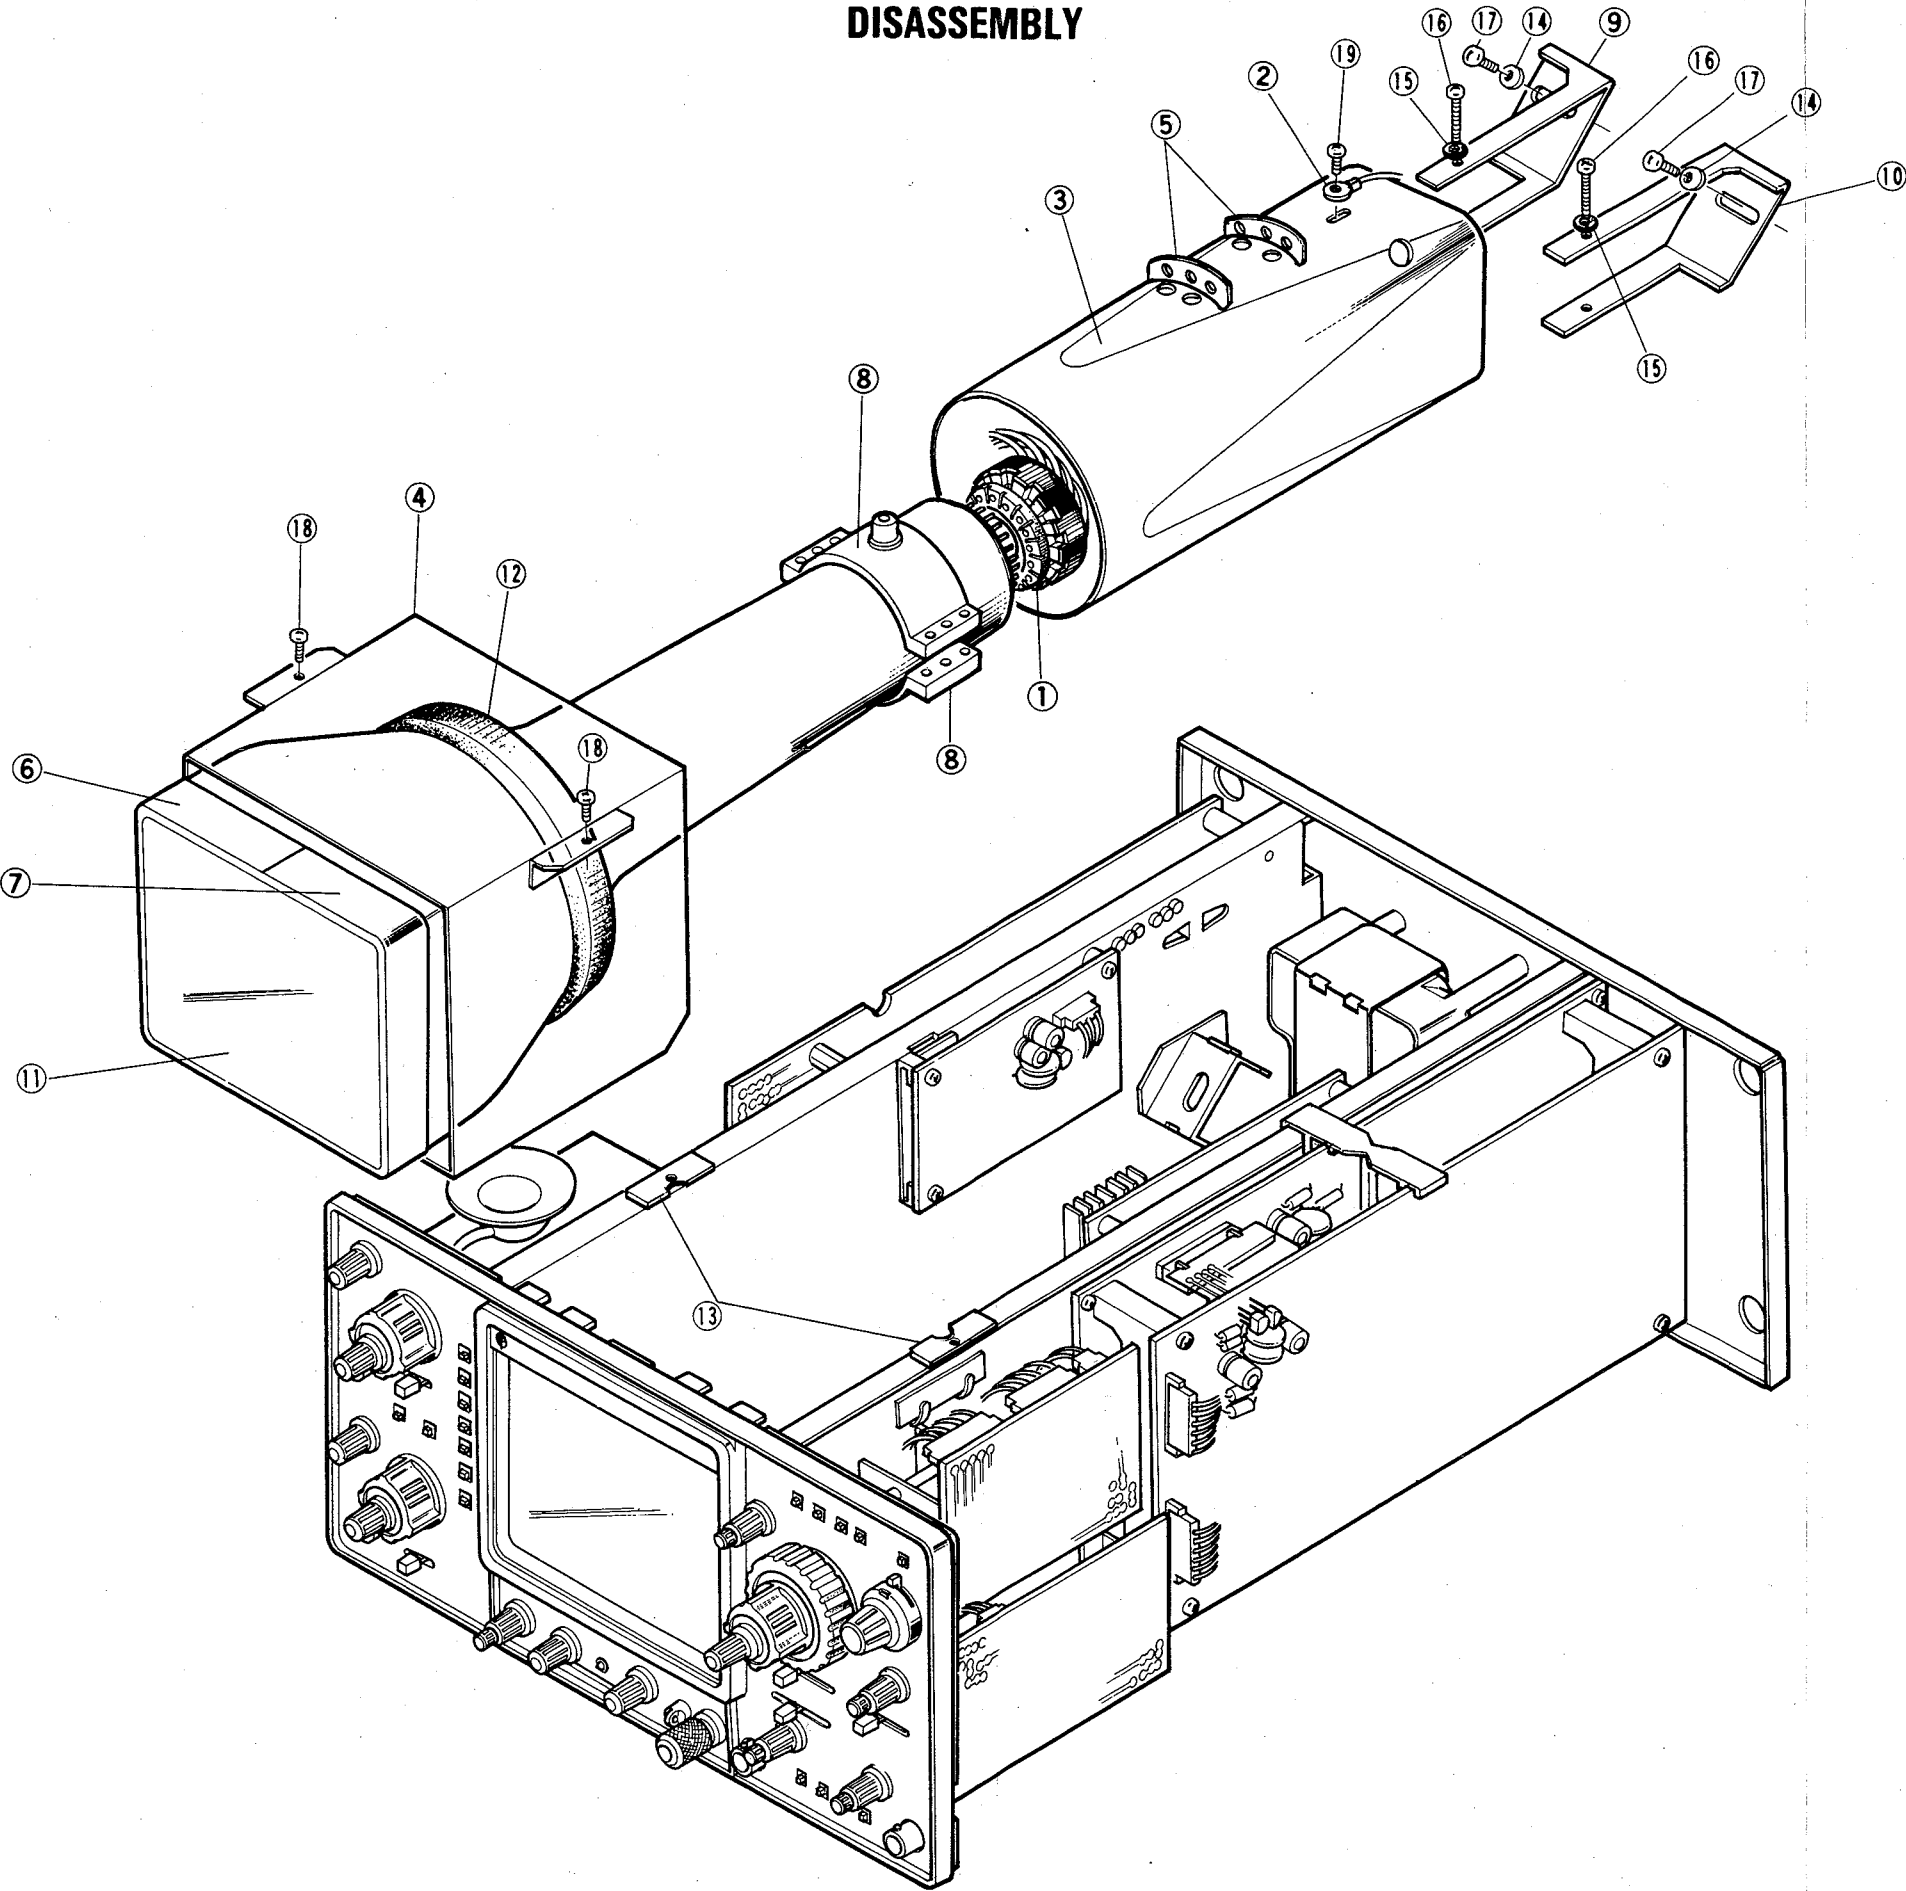

DISASSEMBLY / PARTS LIST

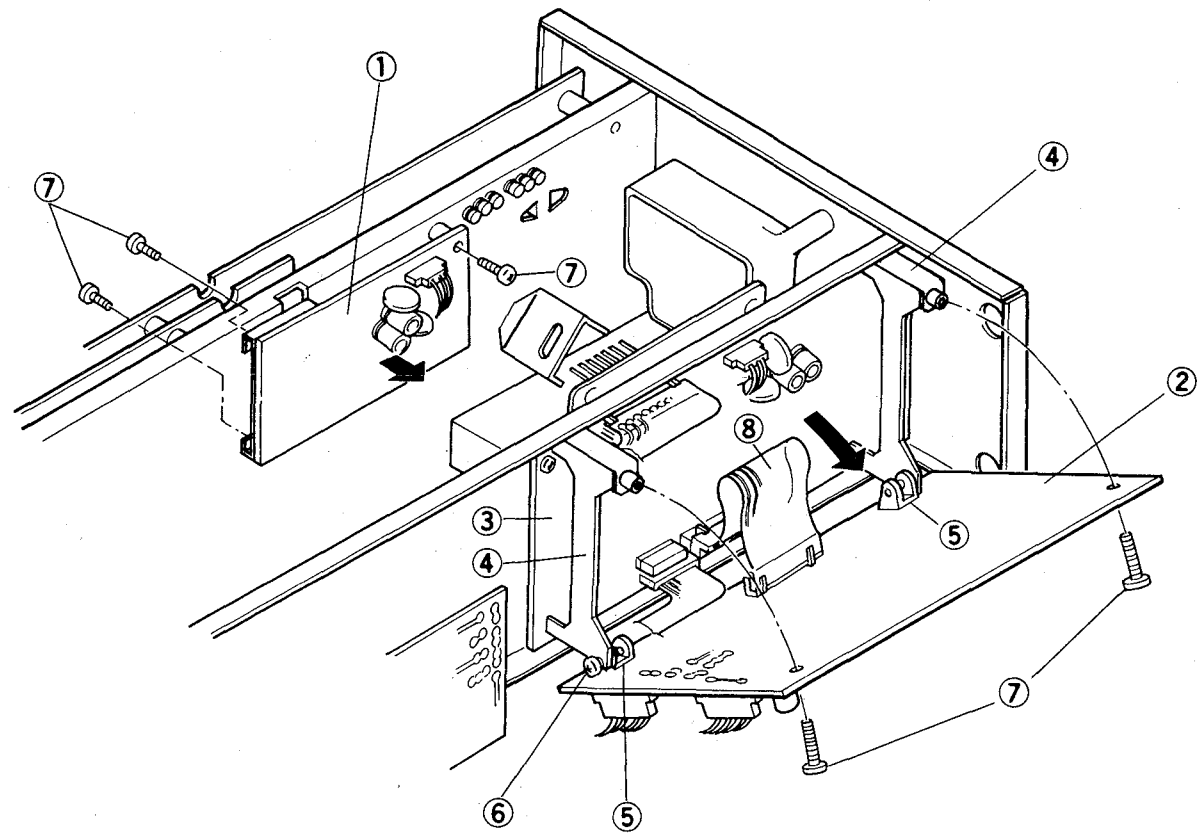


Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
4-1		X73-1330-01	Vertical output unit	
4-2		X74-1320-01	Trig sweep unit	
4-3		X77-1130-01	Horizontal mode control unit	
4-4		J21-2904-24	Bracket (For P.C.B.)	
4-5		J21-2952-04	Bracket (For P.C.B.)	
4-6		J59-0402-05	Screw (Nylon rivet)	
4-7		N30-3006-46	Pan-head screw M3 x 6	
4-8		J25-2904-04	Printed circuit board	

DISASSEMBLY / PARTS LIST

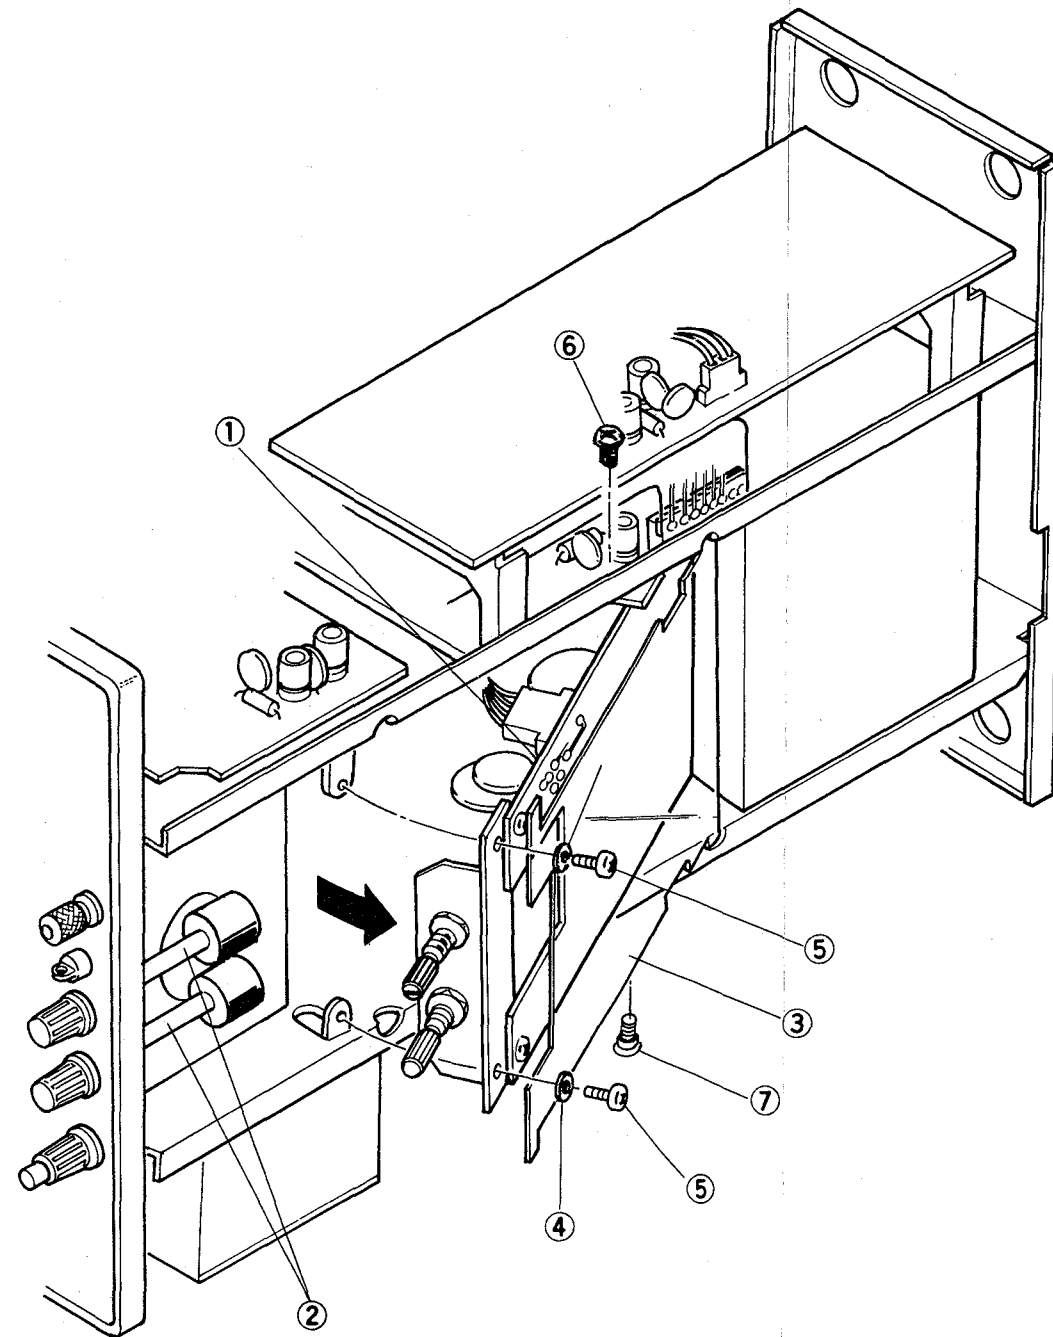


Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
5-1		X68-1310-01	Power blanking unit	
5-2		D21-0903-14	Extension shaft	
5-3		F20-0624-04	Insulator	
5-4		N16-0030-46	Lockwasher	
5-5		N30-3006-46	Pan-head screw M3 x 8	
5-6		N89-3006-46	Screw (Tapping) 3 x 6	
5-7		N09-0402-05	Screw	




Fig. & Index No.

- 6-1
- 6-2
- 6-3
- 6-4
- 6-5
- 6-6
- 6-7
- 6-8
- 6-9
- 6-10
- 6-11
- 6-12
- 6-13
- 6-14
- 6-15
- 6-16
- 6-17
- 6-18
- 6-19

Note: When

DISASSEMBLY/PARTS LIST

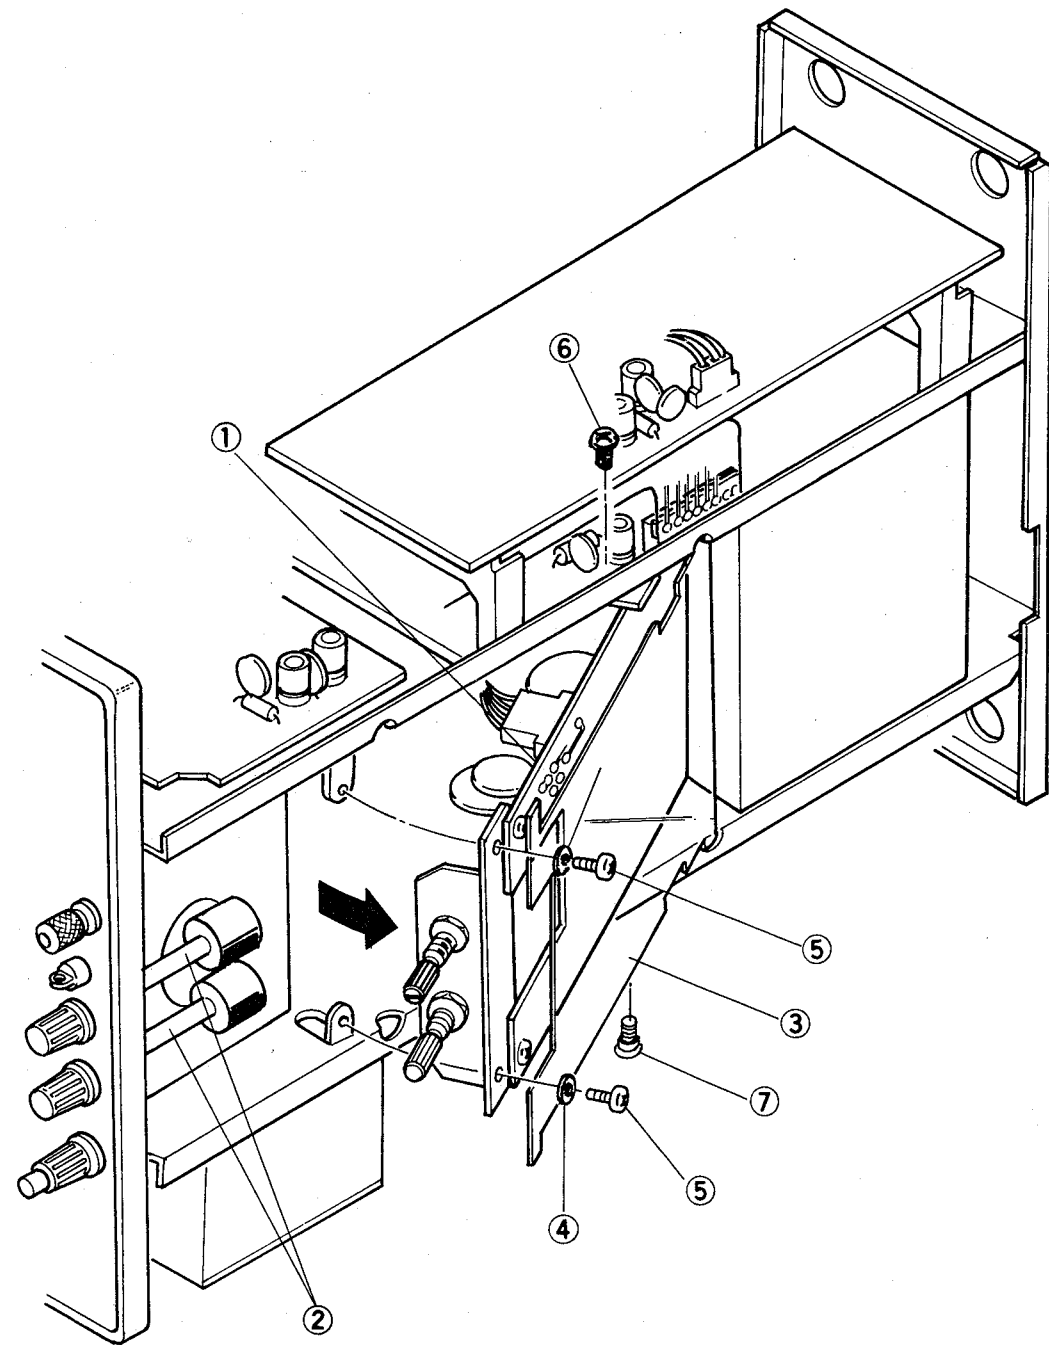


Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
5-1		X68-1310-01	Power blanking unit	
5-2		D21-0903-14	Extension shaft	
5-3		F20-0624-04	Insulator	
5-4		N16-0030-46	Lockwasher	
5-5		N30-3006-46	Pan-head screw M3 x 8	
5-6		N89-3006-46	Screw (Tapping) 3 x 6	
5-7		N09-0402-05	Screw	

DISASSEMBLY/PARTS LIST

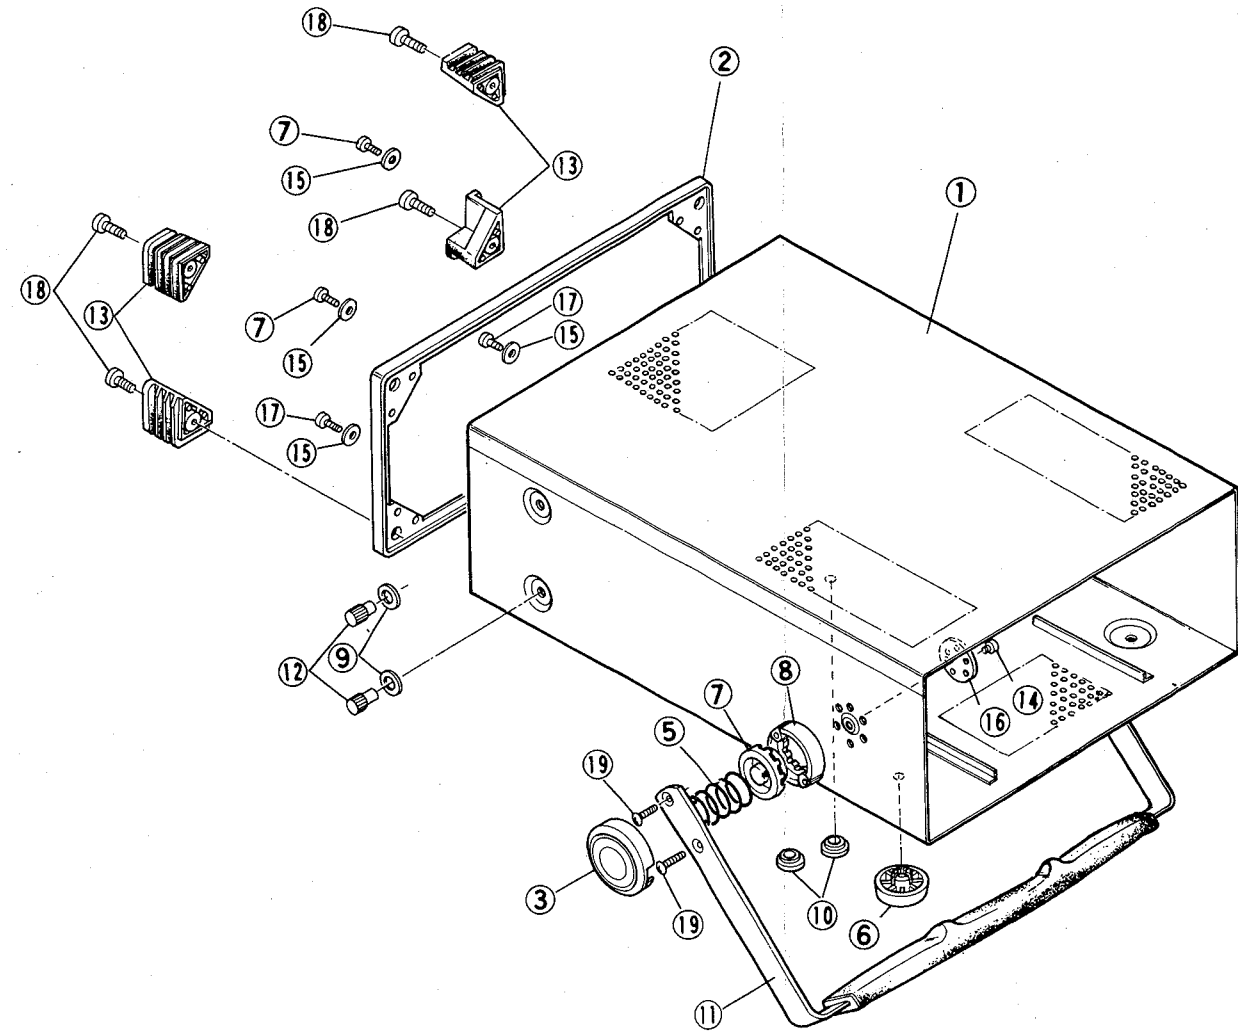


Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
6-1		A01-0872-22	Case	
6-2		B07-0710-02	Rear escutcheon	
6-3		F07-0908-14	Handle cover	
6-4		No use		
6-5		G02-0606-14	Spring (For handle)	
6-6		J02-0507-05	Rubber leg	
6-7		J21-2906-05	Gear	
6-8		J21-2907-05	Ring	
6-9		J39-0505-04	Spacer	
6-10		J42-0038-04	Bushing	
6-11		K01-0512-05	Handle	
6-12		K23-0802-14	Knob	*Note:
6-13		W01-0503-04	Cord wrap	
6-14		N09-0705-05	Hex socket Flat-head screw	
6-15		N17-1030-41	Lockwasher	
6-16		N19-0710-05	Washer	
6-17		N30-3008-41	Pan-head screw M3 x 8	
6-18		N08-0611-04	Flat head screw M6 x 11	
6-19		N32-3008-41	Flat-head screw M3 x 8	

Note: When replacing R01-0512-05 with R01-0512-15, use the knob (K23-0802-14) simultaneously.

PACKING/PARTS LIST

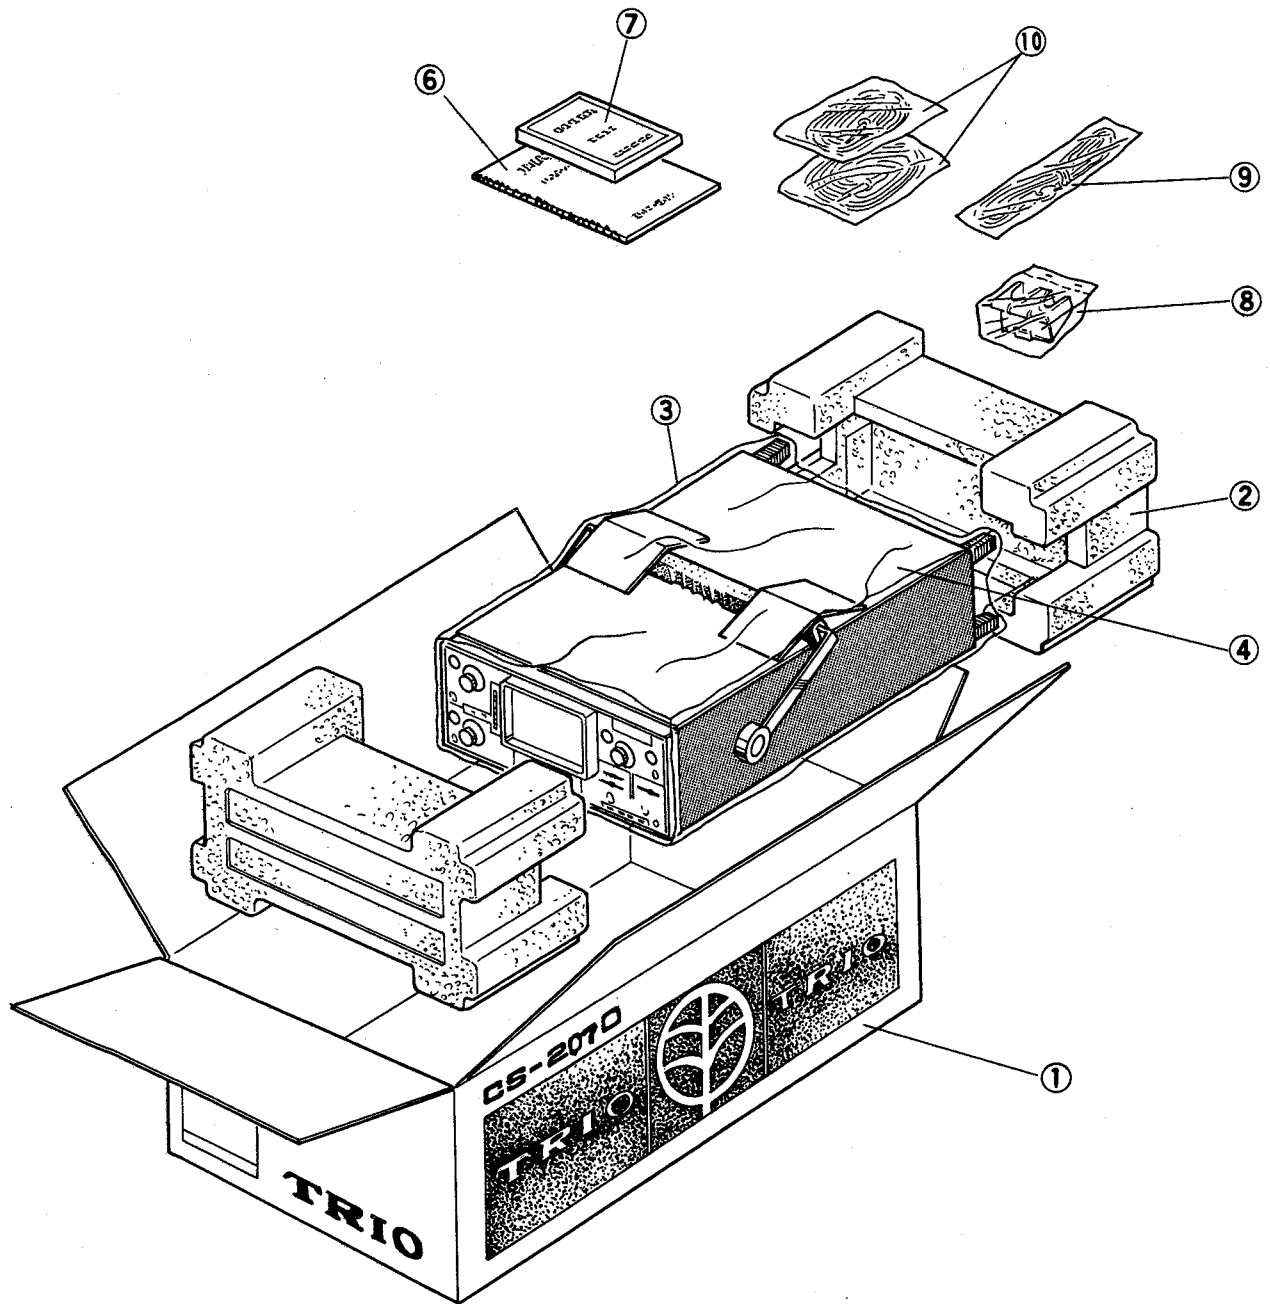


Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
7-1		H01-2978-04	Carton box	
7-2		H10-2812-12	Pad (Formed styrene)	
7-3		H20-1713-14	Polyethylene bag	
7-4		H12-0531-04	Protective cover	
7-5		No use		
7-6		B50-2967-20	Instruction manual	
7-7		B50-2966-20	Instruction hand book	
7-8		J21-2903-03	Probe holder	
7-9		E30-1818-05	Power cord (JIS)	
		E30-1819-05	Power cord (CEE)	
		E30-1821-05	Power cord (SAA)	
7-10		Y87-1250-00	Probe (PC-29)	

PARTS LIST

Fig. & Index No.	Ref. No.	Parts No.	Name & Description	Serial No. Eff.
	R1	No use	Thermister 4W-25V	
	R2	No use		
	R3	RD14BB2E105J	Carbon resistor, 1M Ω , \pm 5%, 1/4W	
	R4	RD14BB2E105J	Carbon resistor, 1M Ω , \pm 5%, 1/4W	
	R5	RD14BB2E220J	Carbon resistor, 22 Ω , \pm 5%, 1/4W	
	R6	RD14BB2E220J	Carbon resistor, 22 Ω , \pm 5%, 1/4W	
	R7	RD14BB2E220J	Carbon resistor, 22 Ω , \pm 5%, 1/4W	
	R8	RD14BB2E220J	Carbon resistor, 22 Ω , \pm 5%, 1/4W	
	R9	RD14BB2C220J	Carbon resistor, 22 Ω , \pm 5%, 1/8W	
	R10	RD14BB2C220J	Carbon resistor, 22 Ω , \pm 5%, 1/8W	
	R11	RD14BB2E471J	Carbon resistor, 470 Ω , \pm 5%, 1/4W	
	R12	RD14BB2E471J	Carbon resistor, 470 Ω , \pm 5%, 1/4W	
	R13	RD14BB2E153J	Carbon resistor, 15 k Ω , \pm 5%, 1/4W	
	C1	C91-0501-05	Metalised film capacitor, 0.047 μ F, 630 WV	
	C2	C91-0501-05	Metalised film capacitor, 0.047 μ F, 630 WV	
	C3	No use		
	C4	CK45E3D472P	Ceramic capacitor, 4700pF, 2000 WV	
	C5	CK45E3D472P	Ceramic capacitor, 4700pF, 2000 WV	
	C6	CC45CH1H101J	Ceramic capacitor 100pF, \pm 5%	
	C7	CC45CH1H030C	Ceramic capacitor, 3pF, \pm 0.25pF	
	C8	CC45CH1H680J	Ceramic capacitor, 68pF, \pm 5%	
	C9	CC45CH1H680J	Ceramic capacitor, 68pF, \pm 5%	
	C10	C91-0551-05	Metalised film capacitor, 0.22 μ F, 630 WV	
		E23-0015-04	Earth lyg (For A TRIG, V ATT)	
		B40-2765-04	Name plate	
		B41-0730-04	Caution sheet	
		B41-0739-04	Caution sheet	
		B42-1835-04	Voltage indication sheet	
		B42-1836-04	Voltage indication sheet	
	J7	E31-0748-15	Leadwire with connector	
	J8	E31-0749-15	Leadwire with connector	
	J9	E31-0750-15	Leadwire with connector	
	J10	E31-0751-25	Leadwire with connector	
	J12	E31-0797-25	Leadwire with connector	
		E31-2340-05	Leadwire with connector	
	J31	E31-0752-05	Leadwire with connector	
	J32	E31-2321-05	Leadwire with connector	
	J33	E31-0754-05	Leadwire with connector	
	J40	E31-2337-05	Leadwire with connector	
	J41	E31-2338-05	Leadwire with connector	
	J48	E31-2339-15	Leadwire with connector	
	J51	E31-2341-15	Leadwire with connector	
	J56	E31-0790-05	Leadwire with connector	
	J57	E31-0799-05	Leadwire with connector	
		E31-0564-05	Leadwire with connector	
		E31-2320-05	Leadwire with connector	
		E31-2323-05	Leadwire with connector	
		E31-2319-45	Wire harness	
		E40-0711-05	Pin connector 7P	
		E40-1811-05	Pin connector 18P	
		E40-1216-05	Pin connector 12P	
		E40-1516-05	Pin connector 15P	
		F11-0963-03	Shield case (for switching power supply)	
	L4, 5	L92-0103-05	Ferrite core	
		L40-2282-13	Axial coil	
		J61-0501-05	Supporter (For P.C.B.)	
		J19-1620-05	Cord keeper	
		J42-0520-04	Edging	
		J61-0049-05	Cable band	

PARTS LIST

VERTICAL ATTENUATOR UNIT X75-1120-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
	R1	RD14BB2C470J	RD 47 Ω
	R2	RD14BB2C100J	RD 10 Ω
	R3	RD14BB2C220J	RD 22 Ω
B-2	R4	RN14BK2E5003F	RN 500k Ω \pm 1% 1/4W
B-2	R5	RN14BK2E1004F	RN 1M Ω \pm 1% 1/4W
B-3	R6	RD14BB2C560J	RD 56 Ω
B-3	R7	RN14BK2E7503F	RN 750k Ω \pm 1% 1/4W
B-3	R8	R92-0795-05	RD 333k Ω \pm 1% 1/2W
B-3	R9	RD14BB2C220J	RD 22 Ω
A-3	R10	RN14BK2E9003F	RN 900k Ω \pm 1% 1/4W
A-2	R11	RN14BK2E1113F	RN 111k Ω \pm 1% 1/4W
A-3	R12	RD14BB2C680J	RD 68 Ω
A-3	R13	RD14BB2C100J	RD 10 Ω
A-3	R14	RD14BB2C470J	RD 47 Ω
B-3	R15	RD14BB2C472J	RD 4.7k Ω
C-2	R16	RD14BB2C472J	RD 4.7k Ω
B-2	R17	RD14BB2C912J	RD 9.1k Ω
B-2	R18	RD14BB2C470J	RD 47 Ω
C-3	R19	RD14BB2C181J	RD 180 Ω
B-3	R20	RN14BK2E9903F	RN 990k Ω \pm 1% 1/4W
B-3	R21	RN14BK2E1012F	RN 10.1k Ω \pm 1% 1/4W
B-3	R22	RN14BB2C101J	RD 100 Ω
B-3	R23	RD14BB2C220J	RD 22 Ω
B-3	R24	RD14BB2C820J	RD 82 Ω
B-3	R25	RD14BB2C122J	RD 1.2k Ω
B-3	R26	RN14BK2E1004F	RN 1M Ω \pm 1% 1/4W
B-3	R27	RD14BB2E104J	RD 100k Ω \pm 5% 1/4W
C-2	R28	RN14BK2B1000F	RN 100 Ω \pm 1% 1/8W
C-3	R29	RN14BK2B1000F	RN 100 Ω \pm 1% 1/8W
C-3	R30	RD14BB2C101J	RD 100 Ω
C-2	R31	RD14BB2C101J	RD 100 Ω
C-3	R32	RN14BK2B7500F	RN 750 Ω \pm 1% 1/8W
C-3	R33	RN14BK2B7500F	RN 750 Ω \pm 1% 1/8W
C-3	R34	RN14BK2B7500F	RN 750 Ω \pm 1% 1/8W
C-3	R35	RN14BK2B3300F	RN 330 Ω \pm 1% 1/8W
	R36	No use	
	R37	No use	
	R38	No use	
	R39	No use	
	R40	No use	
	R41	No use	
C-3	R42	RD14BB2C121J	RD 120 Ω
	R43	RD14BB2C470J	RD 47 Ω
	R44	RD14BB2C100J	RD 10 Ω
	R45	RD14BB2C220J	RD 22 Ω
B-1	R46	RN14BK2E5003F	RN 500k Ω \pm 1% 1/4W
B-1	R47	RN14BK2E1004F	RN 1M Ω \pm 1% 1/4W
B-1	R48	RD14BB2C560J	RD 56 Ω
B-1	R49	RN14BK2E7503F	RN 750k Ω \pm 1% 1/4W
B-2	R50	R92-0795-05	RD 333k Ω \pm 1% 1/2W
B-1	R51	RD14BB2C220J	RD 22 Ω
A-1	R52	RN14BK2E9003F	RN 900k Ω \pm 1% 1/4W
A-1	R53	RN14BK2E1113F	RN 111k Ω \pm 1% 1/4W
A-1	R54	RD14BB2C680J	RD 68 Ω
A-1	R55	RD14BB2C100J	RD 10 Ω
A-1	R56	RD14BB2C220J	RD 22 Ω
C-1	R57	RD14BB2C181J	RD 180 Ω
B-1	R58	RD14BB2C912J	RD 9.1k Ω
B-1	R59	RD14BB2C470J	RD 47 Ω
C-1	R60	RD14BB2C472J	RD 4.7k Ω
D-1	R61	RD14BB2C472J	RD 4.7k Ω
B-1	R62	RN14BK2E9903F	RN 990k Ω \pm 1% 1/4W
B-2	R63	RN14BK2E1012F	RN 10.1k Ω \pm 1% 1/4W
B-1	R64	RD14BB2C101J	RD 100 Ω
B-2	R65	RD14BB2C220J	RD 22 Ω

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
B-1	R66	RD14BB2C820J	RD 82 Ω
B-1	R67	RD14BB2C122J	RD 1.2k Ω
B-1	R68	RN14BK2E1004F	RN 1M Ω \pm 1% 1/4W
B-1	R69	RD14BB2E104J	RN 100 Ω \pm 1% 1/8W
C-1	R70	RN14BK2B1000F	RN 100 Ω \pm 1% 1/8W
C-1	R71	RN14BK2B1000F	RN 100 Ω \pm 1% 1/8W
C-1	R72	RD14BB2C101J	RD 100 Ω
C-1	R73	RD14BB2C101J	RD 100 Ω
C-2	R74	RN14BK2B7500F	RN 750 Ω \pm 1% 1/8W
C-1	R75	RN14BK2B7500F	RN 750 Ω \pm 1% 1/8W
C-2	R76	RN14BK2B7500F	RN 750 Ω \pm 1% 1/8W
C-2	R77	RN14BK2B3300F	RN 330 Ω \pm 1% 1/8W
	R78	No use	
	R79	No use	
	R80	No use	
	R81	No use	
	R82	No use	
	R83	No use	
C-2	R84	RD14BBsC121J	RD 120 Ω
D-3	R85	RD14BB2C224J	RD 220k Ω
D-3	R86	RD14BB2C224J	RD 220k Ω
D-3	R87	RD14BB2C224J	RD 220k Ω
D-3	R88	RD14BB2C224J	RD 220k Ω
D-3	R89	RD14BB2C224J	RD 220k Ω
E-3	R90	RD14BB2C224J	RD 220k Ω
D-3	R91	RD14BB2C224J	RD 220k Ω
D-2	R92	RD14BB2C224J	RD 220k Ω
B-2	R93	RD14BB2C224J	RD 220k Ω
D-3	R94	RD14BB2C824J	RD 820k Ω
D-3	R95	RD14BB2C824J	RD 820k Ω
D-3	R96	RD14BB2C824J	RD 820k Ω
D-3	R97	RD14BB2C824J	RD 820k Ω
D-3	R98	RD14BB2C824J	RD 820k Ω
D-3	R99	RD14BB2C824J	RD 820k Ω
D-3	R100	RD14BB2C824J	RD 820k Ω
D-1	R101	RD14BB2C824J	RD 820k Ω
D-2	R102	RD14BB2C824J	RD 820k Ω
E-2	R103	RD14BB2C473J	RD 47k Ω
E-2	R104	RD14BB2C473J	RD 47k Ω
E-2	R105	RD14BB2C274J	RD 270k Ω
E-2	R106	RD14BB2C274J	RD 270k Ω
E-2	R107	RD14BB2C274J	RD 270k Ω
E-2	R108	RD14BB2C473J	RD 47k Ω
E-2	R109	RD14BB2C473J	RD 47k Ω
D-2	R110	RD14BB2C473J	RD 47k Ω
D-1	R111	RD14BB2C393J	RD 39k Ω
D-3	R112	RD14BB2C391J	RD 390 Ω
D-3	R113	RD14BB2C391J	RD 390 Ω
D-3	R114	RD14BB2C391J	RD 390 Ω
D-3	R115	RD14BB2C391J	RD 390 Ω
D-3	R116	RD14BB2C391J	RD 390 Ω
D-3	R117	RD14BB2C391J	RD 390 Ω
D-3	R118	RD14BB2C391J	RD 390 Ω
D-1	R119	RD14BB2C391J	RD 390 Ω
D-1	R120	RD14BB2C391J	RD 390 Ω
	R121	No use	
	R122	No use	
D-2	R123	RD14BB2C100J	RD 10 Ω
	R124	RD14BB2C680J	RD 68 Ω
C-3	R125	RN14BK2B1000F	RN 100 Ω \pm 1% 1/8W
	R126	No use	
A-1	R127	RD14BB2C101J	RD 100 Ω
C-1	R128	RN14BK2B1000F	RN 100 Ω \pm 1% 1/8W
E-1	R129	RD14BB2C153J	RD 15k Ω
E-2	R130	RD14BB2C824J	RD 820k Ω

PARTS LIST

X75-1120-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
E-1	R131	RD14BB2C824J	RD	820k Ω	
	R132	No use			
C-1	R133	RN14BK2B47ROF	RN	47 Ω	$\pm 1\%$ 1/8W
C-3	R134	RN14BK2B47ROF	RN	47 Ω	$\pm 1\%$ 1/8W
	R135	RD14BB2C680J	RD	68 Ω	
C-2	R136	RN14BK2B47ROF	RN	47 Ω	$\pm 1\%$ 1/8W
A-3	R137	RD14BB2C101J	RD	100 Ω	
C-3	R138	RN14BK2B47ROF	RN	47 Ω	$\pm 1\%$ 1/8W
A-3	R139	RD14BB2C220J	RD	22 Ω	
A-1	R140	RD14BB2C220J	RD	22 Ω	
C-3	R141	RD14BB2C824J	RD	820k Ω	
C-1	R142	RD14BB2C100J	RD	10 Ω	
C-2	R143	RD14BB2C100J	RD	10 Ω	
	R144	RD14BB2C101J	RD	100 Ω	
	R145	RD14BB2C101J	RD	100 Ω	
C-3	VR1	R12-0421-05	VR	100 Ω	
C-2	VR2	R12-0421-05	VR	100 Ω	
	C1	CC45CH1H470J	CC	47pF	$\pm 5\%$
	C2	CC45CH1H470J	CC	47pF	$\pm 5\%$
	C3	CC45CH1H470J	CC	47pF	$\pm 5\%$
A-2	C4	CM93BD2A100D	CM	10pF	$\pm 0.5pF$ 100WV
B-2	C5	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
B-2	C6	CM93BD2A221J	CM	220pF	$\pm 5\%$ 100WV
	C7	No use			
B-3	C8	C91-0502-05	MF	0.01 μF	630WV
C-2	C9	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
C-3	C10	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
C-2	C11	CE04W1C330M	CE	33 μF	16WV
C-2	C12	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
C-3	C13	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
C-2	C14	CE04W1E101M	CE	100 μF	25WV
C-2	C15	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
C-2	C16	CE04W1E101M	CE	100 μF	25WV
C-3	C17	CC45CH1H100D	CC	10pF	$\pm 0.5pF$
	C18	CC45CH1H470J	CC	47pF	$\pm 5\%$
	C19	CC45CH1H470J	CC	47pF	$\pm 5\%$
	C20	No use			
A-1	C21	CM93BD2A100D	CM	10pF	$\pm 0.5pF$ 100WV
C-1	C22	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
B-1	C23	CM93BD2A221J	CM	220pF	$\pm 5\%$ 100WV
B-1	C24	CC45CH1H390J	CC	39pF	$\pm 5\%$
B-1	C25	C91-0502-05	MF	0.01 μF	630WV
C-1	C26	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
B-2	C27	CC45CH1H330J	CC	33pF	$\pm 5\%$
C-1	C28	CE04W1C330M	CE	33 μF	16WV
C-1	C29	CC45CH1H150J	CC	15pF	$\pm 5\%$
C-2	C30	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
C-2	C31	CE04W1E101M	CE	100 μF	25WV
C-2	C32	CE04W1E101M	CE	100 μF	25WV
C-1	C33	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
C-1	C34	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
C-2	C35	CC45CH1H100D	CC	10pF	$\pm 0.5pF$
D-3	C36	CC45CH1H101J	CC	100pF	$\pm 5\%$
D-3	C37	CC45CH1H101J	CC	100pF	$\pm 5\%$
D-3	C38	CC45CH1H101J	CC	100pF	$\pm 5\%$
D-3	C39	CC45CH1H101J	CC	100pF	$\pm 5\%$
D-3	C40	CC45CH1H101J	CC	100pF	$\pm 5\%$
D-3	C41	CC45CH1H101J	CC	100pF	$\pm 5\%$
D-3	C42	CC45CH1H101J	CC	100pF	$\pm 5\%$
D-2	C43	CC45CH1H101J	CC	100pF	$\pm 5\%$
D-2	C44	CC45CH1H101J	CC	100pF	$\pm 5\%$
E-2	C45	CK45B1H222K	CK	2200pF	$\pm 10\%$
E-2	C46	CK45B1H222K	CK	2200pF	$\pm 10\%$

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
E-2	C47	CK45B1H472K	CK	4700pF	$\pm 10\%$
D-1	C48	CC45CH1H101J	CC	100pF	$\pm 5\%$
C-3	C49	CC45CH1H150J	CC	15pF	$\pm 5\%$
	C50	No use			
B-2	C51	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
D-2	C52	CK45B1H102K	CK	1000pF	$\pm 10\%$
	C53	CC45CH1H470J	CC	47pF	$\pm 5\%$
A-1	C54	CC45CH1H090D	CC	9pF	$\pm 0.5pF$
D-1	C55	CK45B1H102K	CK	1000pF	$\pm 10\%$
B-2	C56	CC45CH1H010C	CC	1pF	$\pm 0.25pF$
B-1	C57	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
B-3	C58	CC45CH1H330J	CC	33pF	$\pm 5\%$
	C59	No use			
	C60	No use			
A-3	C61	CC45CH1H090D	CC	9pF	$\pm 0.5pF$
B-2	C62	CC45CH1H390J	CC	39pF	$\pm 5\%$
	C63	No use			
B-1	C64	CC45CH1H010C	CC	1pF	$\pm 0.25pF$
C-2	C65	CE04W1C330M	CE	33 μF	16WV
	C66	No use			
B-1	C67	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
A-3	C68	CC45CH1H101J	CC	100pF	$\pm 5\%$
A-3	C69	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
A-2	C70	CC45CH1H101J	CC	100pF	$\pm 5\%$
A-2	C71	CK45B1H103K	CK	0.01 μF	$\pm 10\%$
	C72	No use			
C-1	C73	CE04W1C330M	CE	33 μF	16WV
A-3	C74	CC45CH1H020C	CC	2pF	$\pm 0.25pF$
A-1	C75	CC45CH1H020C	CC	2pF	$\pm 0.25pF$
B-3	C76	CC45CH1H030C	CC	3pF	$\pm 0.25pF$
B-2	C77	CC45CH1H030C	CC	3pF	$\pm 0.25pF$
	C78	No use			
	C79	No use			
	C80	No use			
	C81	No use			
	C82	CC45CH1H030C	CC	3pF	$\pm 0.25pF$
	C83	CC45CH1H030C	CC	3pF	$\pm 0.25pF$
B-2	TC1	C05-0030-15	TC	20pF	
B-3	TC2	C05-0030-15	TC	20pF	
A-2	TC3	C05-0030-15	TC	20pF	
B-3	TC4	C05-0030-15	TC	20pF	
B-3	TC5	C05-0062-05	TC	6pF	
A-2	TC6	C05-0062-05	TC	6pF	
A-3	TC7	C05-0309-05	TC	40pF	
B-2	TC8	C05-0030-15	TC	20pF	
	TC9	No use			
B-3	TC10	C05-0062-05	TC	6pF	
C-3	TC11	C05-0030-05	TC	20pF	
B-1	TC12	C05-0030-15	TC	20pF	
B-1	TC13	C05-0030-15	TC	20pF	
A-1	TC14	C05-0030-15	TC	20pF	
B-1	TC15	C05-0030-15	TC	20pF	
B-1	TC16	C05-0062-05	TC	6pF	
A-1	TC17	C05-0062-05	TC	6pF	
A-1	TC18	C05-0309-05	TC	40pF	
B-2	TC19	C05-0030-15	TC	20pF	
	TC20	No use			
B-1	TC21	C05-0062-05	TC	6pF	
C-2	TC22	C05-0030-05	TC	20pF	
B-3	TC23	C05-0062-05	TC	6pF	
B-1	TC24	C05-0062-05	TC	6pF	
C-3	L1	L40-1001-02	Ferri-inductor	10 μH	
C-3	L2	L40-1001-02	Ferri-inductor	10 μH	

PARTS LIST

X75-1120-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
C-1	L3	L40-1001-02	Ferri-inductor 10 μ H
C-1	L4	L40-1001-02	Ferri-inductor 10 μ H
B-2	D1		Diode Silicon 1S1544A
B-2	D2		Diode Silicon 1S1544A
B-1	D3		Diode Silicon 1S1544A
B-1	D4		Diode Silicon 1S1544A
D-2	D5		Diode Silicon DS442X
D-2	D6		Diode Silicon DS442X
D-2	D7		Diode Silicon DS442X
D-2	D8		Diode Silicon DS442X
D-2	D9		Diode Silicon DS442X
D-2	D10		Diode Silicon DS442X
D-2	D11		Diode Silicon DS442X
C-2	D12		Diode Zener YZ-120
C-2	D13		Diode Zener YZ-120
C-1	D14		Diode Zener YZ-120
D-1	D15		Diode Zener YZ-120
C-2	Q1		FET Dual DN1901
C-1	Q2		FET Dual DN1901
D-2	IC1		IC Digital MC14584BCP
D-2	IC2		IC Digital MC14584BCP
D-2	IC3		IC Digital MC10014BCP
D-2	IC4		IC Linear MC14027BCP
E-3	IC5		IC Linear SN7404N
E-2	IC6		IC Digital MC14174BCP
D-1	IC7		IC Digital MC14081BCP
E-2	IC8		IC Linear MC14503BCP
E-2	IC9		IC Digital SN7432N
D-1	IC10		IC Digital MC14027BCP
E-1	IC11		IC Digital MC14503BCP
C-3	IC12		IC Linear ATM-4010
C-1	IC13		IC Linear ATM-4010
D-2	P1	E40-1817-05	Pin connector 18P
D-1	P2	E40-0717-05	Pin connector 7P
C-3	P3	E40-0611-05	Pin connector 6P
C-1	P4	E40-0611-05	Pin connector 6P
E-3	P5	E40-1277-05	Pin connector 12P
E-1	P6	E40-0577-05	Pin connector 5P
		E23-0521-04	Earth terminal
		E29-0504-05	Teflon terminal
A-3	S1a	S01-4503-05	Rotary switch
B-3	S1b	S01-4503-05	Rotary switch
B-3	S1c	S01-4503-05	Rotary switch
B-3	S1d	S01-4503-05	Rotary switch
B-3	S1e	S01-4503-05	Rotary switch
	S1f	S01-4503-05	Rotary switch
	S1g	S01-4503-05	Rotary switch
	S1h	S01-4503-05	Rotary switch
A-1	S2a	S01-4503-05	Rotary switch
B-1	S2b	S01-4503-05	Rotary switch
B-1	S2c	S01-4503-05	Rotary switch
B-1	S2d	S01-4503-05	Rotary switch
B-1	S2e	S01-4503-05	Rotary switch
	S2f	S01-4503-05	Rotary switch
	S2g	S01-4503-05	Rotary switch
	S2h	S01-4503-05	Rotary switch

VERTICAL PREAMPLIFIER UNIT X73-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
B-3	R1	RD14BB2C220J	RD 22 Ω
B-3	R2	RD14BB2C220J	RD 22 Ω
B-3	R3	RN14BK2B1500F	RN 150 Ω \pm 1% 1/8W
B-3	R4	RD14BB2C121J	RD 120 Ω
B-3	R5	RD14BB2C472J	RD 4.7k Ω
B-3	R6	RN14BK2B2700F	RN 270 Ω \pm 1% 1/8W
B-3	R7	RD14BB2C101J	RD 100 Ω
B-3	R8	RN14BK2B2700F	RN 270 Ω \pm 1% 1/8W
B-2	R9	RD14BB2C112J	RD 1.1k Ω
B-2	R10	RD14BB2C392J	RD 3.9k Ω
B-2	R11	RD14BB2C220J	RD 22 Ω
B-3	R12	RD14BB2C220J	RD 22 Ω
B-3	R13	RN14BK2B3001F	RN 3k Ω \pm 1% 1/8W
B-3	R14	RN14BK2B1801F	RN 1.8k Ω \pm 1% 1/8W
B-3	R15	RN14BK2B3000F	RN 300 Ω \pm 1% 1/8W
B-3	R16	RN14BK2B7500F	RN 750 Ω \pm 1% 1/8W
B-2	R17	RN14BK2B7500F	RN 750 Ω \pm 1% 1/8W
B-3	R18	RN14BK2B5601F	RN 5.6k Ω \pm 1% 1/8W
B-3	R19	RN14BK2B5601F	RN 5.6k Ω \pm 1% 1/8W
B-3	R20	RN14BK2B3601F	RN 3.6k Ω \pm 1% 1/8W
B-3	R21	RN14BK2B3601F	RN 3.6k Ω \pm 1% 1/8W
B-3	R22	RN14BK2B1501F	RN 1.5k Ω \pm 1% 1/8W
B-3	R23	RN14BK2B1501F	RN 1.5k Ω \pm 1% 1/8W
B-3	R24	RD14BB2C220J	RD 22 Ω
B-2	R25	RD14BB2C220J	RD 22 Ω
B-3	R26	RD14BB2C821J	RD 820 Ω
B-3	R27	RN14BK2B4700F	RN 470 Ω \pm 1% 1/8W
B-3	R28	RN14BK2B4700F	RN 470 Ω \pm 1% 1/8W
B-3	R29	RN14BK2B5100F	RN 51 Ω \pm 1% 1/8W
C-2	R30	RD14BB2C103J	RD 10k Ω
C-2	R31	RD14BB2C472J	RD 4.7k Ω
C-2	R32	RD14BB2C472J	RD 4.7k Ω
C-2	R33	RD14BB2C103J	RD 10k Ω
C-2	R34	RD14BB2C821J	RD 820 Ω
C-3	R35	RN14BK2B4700F	RN 47 Ω \pm 1% 1/8W
C-3	R36	RN14BK2B4300F	RN 430 Ω \pm 1% 1/8W
C-3	R37	RN14BK2B4300F	RN 430 Ω \pm 1% 1/8W
C-3	R38	RD14BB2C221J	RD 220 Ω
	R39	No use	
C-3	R40	RN14BK2B1500F	RN 150 Ω \pm 1% 1/8W
C-3	R41	RN14BK2B4300F	RN 430 Ω \pm 1% 1/8W
C-3	R42	RN14BK2B4300F	RN 430 Ω \pm 1% 1/8W
	R43	No use	
C-3	R44	RD14BB2C220J	RD 22 Ω
C-3	R45	RD14BB2C220J	RD 22 Ω
C-3	R46	RN14BK2B1500F	RN 150 Ω \pm 1% 1/8W
C-3	R47	RD14BB2C123J	RD 12k Ω
C-2	R48	RD14BB2C330J	RD 33 Ω
D-2	R49	RD14BB2C472J	RD 4.7k Ω
C-3	R50	RN14BK2B9100F	RN 910 Ω \pm 1% 1/8W
C-2	R51	RN14BK2B9100F	RN 910 Ω \pm 1% 1/8W
C-3	R52	RD14BB2C470J	RD 47 Ω
C-2	R53	RD14BB2C470J	RD 47 Ω
C-3	R54	RN14BK2B3000F	RN 300 Ω \pm 1% 1/8W
C-2	R55	RD14BB2C103J	RD 10k Ω
C-3	R56	RN14BK2B8200F	RN 820 Ω \pm 1% 1/8W
C-2	R57	RN14BK2B8200F	RN 820 Ω \pm 1% 1/8W
C-3	R58	RD14BB2C682J	RD 6.8k Ω
C-3	R59	RN14BK2B3600F	RN 360 Ω \pm 1% 1/8W
C-3	R60	RN14BK2B4700F	RN 470 Ω \pm 1% 1/8W
C-3	R61	RN14BK2B4700F	RN 470 Ω \pm 1% 1/8W
C-3	R62	RN14BK2B1801F	RN 1.8k Ω \pm 1% 1/8W
C-3	R63	RD14BB2C220J	RD 22 Ω
C-3	R64	RD14BB2C220J	RD 22 Ω
D-3	R65	RD14BB2C820J	RD 820 Ω

PARTS LIST

X73-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
D-3	R66	RD14BB2C430J	RD 43Ω
D-2	R67	RN14BK2B4700F	RN 470Ω ±1% 1/8W
C-2	R68	RN14BK2B4700F	RN 470Ω ±1% 1/8W
C-2	R69	RN14BK2B3600F	RN 360Ω ±1% 1/8W
C-2	R70	RN14BK2B1601F	RN 1.6kΩ ±1% 1/8W
C-2	R71	RD14BB2C220J	RD 22Ω
D-2	R72	RD14BB2C821J	RD 820Ω
D-2	R73	RD14BB2C430J	RD 43Ω
D-3	R74	RD14BB2C220J	RD 22Ω
D-2	R75	RD14BB2C220J	RD 22Ω
D-2	R76	RD14BB2C132J	RD 1.3kΩ
D-2	R77	RD14BB2C392J	RD 3.9kΩ
D-3	R78	RD14BB2C220J	RD 22Ω
D-2	R79	RD14BB2C220J	RD 22Ω
D-2	R80	RD14BB2C101J	RD 100Ω
D-3	R81	RD14BB2C101J	RD 100Ω
D-2	R82	RD14BB2C101J	RD 100Ω
D-3	R83	RD14BB2C102J	RD 1kΩ
D-2	R84	RD14BB2C432J	RD 4.3kΩ
D-3	R85	RD14BB2C472J	RD 4.7kΩ
D-1	R86	RD14BB2C472J	RD 4.7kΩ
	R87	No use	
D-3	R88	RD14BB2C102J	RD 1kΩ
D-3	R89	RD14BB2C432J	RD 4.3kΩ
D-3	R90	RD14BB2C101J	RD 100Ω
D-3	R91	RD14BB2C101J	RD 100Ω
D-3	R92	RD14BB2C101J	RD 100Ω
D-3	R93	RD14BB2C220J	RD 22Ω
D-3	R94	RD14BB2C220J	RD 22Ω
D-3	R95	RD14BB2C132J	RD 1.3kΩ
D-3	R96	RD14BB2C392J	RD 3.9kΩ
D-3	R97	RD14BB2C220J	RD 22Ω
D-1	R98	RD14BB2C220J	RD 22Ω
E-3	R99	RN14BK2B3600F	RN 360Ω ±1% 1/8W
E-3	R100	RN14BK2B4700F	RN 470Ω ±1% 1/8W
E-3	R101	RN14BK2B4700F	RN 470Ω ±1% 1/8W
E-3	R102	RN14BK2B1801F	RN 1.8kΩ ±1% 1/8W
E-3	R103	RD14BB2C220J	RD 22Ω
E-3	R104	RD14BB2C220J	RD 22Ω
E-3	R105	RD14BB2C821J	RD 820Ω
E-3	R106	RD14BB2C430J	RD 43Ω
E-3	R107	RN14BK2B8200F	RN 820Ω ±1% 1/8W
E-3	R108	RN14BK2B8200F	RN 820Ω ±1% 1/8W
E-3	R109	RD14BB2C391J	RD 390Ω
E-3	R110	RN14BK2B1001F	RN 1kΩ ±1% 1/8W
D-3	R111	RD14BB2C470J	RD 47Ω
D-3	R112	RD14BB2C470J	RD 47Ω
E-3	R113	RN14BK2B7500F	RN 750Ω ±1% 1/8W
D-3	R114	RN14BK2B7500F	RN 750Ω ±1% 1/8W
D-3	R115	RD14BB2C221J	RD 220Ω
D-3	R116	RD14BB2C273J	RD 27kΩ
D-3	R117	RD14BB2C103J	RD 10kΩ
E-3	R118	RN14BK2B2400F	RN 240Ω ±1% 1/8W
D-3	R119	RD14BB2C151J	RD 150Ω
D-3	R120	RD14BB2C151J	RD 150Ω
E-3	R121	RD14BB2C510J	RD 51Ω
E-3	R122	RD14BB2C510J	RD 51Ω
D-2	R123	RD14BB2C103J	RD 10kΩ
D-2	R124	RD14BB2C223J	RD 22kΩ
D-2	R125	RD14BB2C223J	RD 22kΩ
D-2	R126	RD14BB2C472J	RD 4.7kΩ
D-2	R127	RD14BB2C472J	RD 4.7kΩ
D-2	R128	RD14BB2C473J	RD 47kΩ
D-2	R129	RD14BB2C473J	RD 47kΩ
D-2	R130	RD14BB2C331J	RD 330Ω

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
D-2	R131	RD14BB2C472J	RD 4.7kΩ
D-2	R132	RD14BB2C103J	RD 10kΩ
D-2	R133	RN14BK2B4300F	RN 430Ω ±1% 1/8W
D-2	R134	RN14BK2B4300F	RN 430Ω ±1% 1/8W
D-2	R135	RN14BK2B4300F	RN 430Ω ±1% 1/8W
D-2	R136	RN14BK2B4300F	RN 430Ω ±1% 1/8W
E-2	R137	RN14BK2B8200F	RN 820Ω ±1% 1/8W
D-2	R138	RN14BK2B8200F	RN 820Ω ±1% 1/8W
	R139	No use	
E-2	R140	RN14BK2B3900F	RN 390Ω ±1% 1/8W
D-2	R141	RN14BK2B3600F	RN 360Ω ±1% 1/8W
E-2	R142	RN14BK2B4700F	RN 470Ω ±1% 1/8W
E-2	R143	RN14BK2B4700F	RN 470Ω ±1% 1/8W
D-2	R144	RN14BK2B1801F	RN 1.8kΩ ±1% 1/8W
D-2	R145	RD14BB2C220J	RD 22Ω
D-2	R146	RD14BB2C220J	RD 22Ω
D-2	R147	RD14BB2C821J	RD 820Ω
D-2	R148	RD14BB2C430J	RD 43Ω
D-2	R149	RD14BB2C220J	RD 22Ω
E-2	R150	RD14BB2C220J	RD 22Ω
E-2	R151	RN14BK2B1101F	RN 1.1kΩ ±1% 1/8W
E-2	R152	RN14BK2B9100F	RN 910Ω ±1% 1/8W
E-2	R153	RN14BK2B9100F	RN 910Ω ±1% 1/8W
E-2	R154	RN14BK2B1101F	RN 1.1kΩ ±1% 1/8W
E-2	R155	RN14BK2B3300F	RN 330Ω ±1% 1/8W
E-2	R156	RN14BK2B3300F	RN 330Ω ±1% 1/8W
E-2	R157	RN14BK2B1001F	RN 1kΩ ±1% 1/8W
E-2	R158	RN14BK2B2200F	RN 220Ω ±1% 1/8W
E-2	R159	RN14BK2B1001F	RN 1kΩ ±1% 1/8W
E-2	R160	RN14BK2B7500F	RN 750Ω ±1% 1/8W
E-2	R161	RN14BK2B7500F	RN 750Ω ±1% 1/8W
E-2	R162	RD14BB2C470J	RD 47Ω
E-2	R163	RD14BB2C470J	RD 47Ω
B-1	R164	RD14BB2C220J	RD 22Ω
B-1	R165	RD14BB2C220J	RD 22Ω
C21	R166	RN14BK2B1500F	RN 150Ω ±1% 1/8W
B-2	R167	RD14BB2C241J	RD 240Ω
B-2	R168	RD14BB2C681J	RD 680Ω
B-2	R169	RN14BK2B2700F	RN 270Ω ±1% 1/8W
B-2	R170	RN14BK2B2700F	RN 270Ω ±1% 1/8W
B-2	R171	RN14BK2B1801F	RN 1.8kΩ ±1% 1/8W
B-2	R172	RN14BK2B5601F	RN 5.6kΩ ±1% 1/8W
B-2	R173	RN14BK2B1801F	RN 1.8kΩ ±1% 1/8W
B-2	R174	RN14BK2B5101F	RN 5.1kΩ ±1% 1/8W
B-2	R175	RN14BK2B3000F	RN 300Ω ±1% 1/8W
B-2	R176	RD14BB2C331J	RD 330Ω
B-2	R177	RN14BK2B2201F	RN 2.2kΩ ±1% 1/8W
B-2	R178	RN14BK2B6801F	RN 6.8kΩ ±1% 1/8W
B-2	R179	RN14BK2B2201F	RN 2.2kΩ ±1% 1/8W
D-2	R180	RD14BB2C273J	RD 27kΩ
B-1	R181	RD14BB2C220J	RD 22Ω
B-1	R182	RD14BB2C220J	RD 22Ω
B-1	R183	RD14BB2C112J	RD 1.1kΩ
B-1	R184	RD14BB2C392J	RD 3.9kΩ
B-1	R185	RD14BB2C220J	RD 22Ω
B-1	R186	RD14BB2C220J	RD 22Ω
B-1	R187	RD14BB2C112J	RD 1.1kΩ
B-1	R188	RD14BB2C392J	RD 3.9kΩ
B-1	R189	RN14BK2B7500F	RN 750Ω ±1% 1/8W
B-1	R190	RN14BK2B7500F	RN 750Ω ±1% 1/8W
B-1	R191	RN14BK2B5601F	RN 5.6kΩ ±1% 1/8W
B-1	R192	RN14BK2B5601F	RN 5.6kΩ ±1% 1/8W
B-1	R193	RN14BK2B3601F	RN 3.6kΩ ±1% 1/8W
B-1	R194	RN14BK2B3601F	RN 3.6kΩ ±1% 1/8W
B-1	R195	RN14BK2B1501F	RN 1.5kΩ ±1% 1/8W

PARTS LIST

X73-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
B-1	R196	RN14BK2B1501F	RN	1.5k Ω	$\pm 1\%$ 1/8W
B-2	R197	RD14BB2C220J	RD	22 Ω	
B-1	R198	RD14BB2C220J	RD	22 Ω	
B-1	R199	RD14BB2C102J	RD	1k Ω	
B-1	R200	RN14BK2B4700F	RN	470 Ω	$\pm 1\%$ 1/8W
B-1	R201	RN14BK2B4700F	RN	470 Ω	$\pm 1\%$ 1/8W
B-2	R202	RN14BK2B51ROF	RN	51 Ω	$\pm 1\%$ 1/8W
C-2	R203	RD14BB2C103J	RD	10k Ω	
C-2	R204	RD14BB2C472J	RD	4.7k Ω	
C-2	R205	RD14BB2C472J	RD	4.7k Ω	
C-2	R206	RD14BB2C103J	RD	10k Ω	
C-2	R207	RD14BB2C821J	RD	820 Ω	
C-2	R208	RN14BK2B47ROF	RN	47 Ω	$\pm 1\%$ 1/8W
C-1	R209	RN14BK2B4300F	RN	430 Ω	$\pm 1\%$ 1/8W
C-1	R210	RN14BK2B4300F	RN	430 Ω	$\pm 1\%$ 1/8W
C-1	R211	RD14BB2C301J	RD	300 Ω	
	R212	No use			
C-1	R213	RN14BK2B1500F	RN	150 Ω	$\pm 1\%$ 1/8W
C-2	R214	RN14BK2B4300F	RN	430 Ω	$\pm 1\%$ 1/8W
C-1	R215	RN14BK2B4300F	RN	430 Ω	$\pm 1\%$ 1/8W
	R216	No use			
C-2	R217	RD14BB2C220J	RD	22 Ω	
C-1	R218	RD14BB2C220J	RD	22 Ω	
C-1	R219	RN14BK2B1500F	RN	150 Ω	$\pm 1\%$ 1/8W
C-1	R220	RD14BB2C123J	RD	12k Ω	
	R221	RD14BB2C330J	RD	33 Ω	
C-1	R222	RD14BB2C682J	RD	6.8k Ω	
C-1	R223	RN14BK2B9100F	RN	910 Ω	$\pm 1\%$ 1/8W
C-1	R224	RN14BK2B9100F	RN	910 Ω	$\pm 1\%$ 1/8W
C-1	R225	RD14BB2C470J	RD	47 Ω	
C-1	R226	RD14BB2C470J	RD	47 Ω	
C-1	R227	RN14BK2B2000F	RN	200 Ω	$\pm 1\%$ 1/8W
C-1	R228	RD14BB2C471J	RD	470 Ω	
C-1	R229	RN14BK2B8200F	RN	820 Ω	$\pm 1\%$ 1/8W
C-1	R230	RN14BK2B8200F	RN	820 Ω	$\pm 1\%$ 1/8W
C-2	R231	RN14BK2B3600F	RN	360 Ω	$\pm 1\%$ 1/8W
C-2	R232	RN14BK2B4700F	RN	470 Ω	$\pm 1\%$ 1/8W
C-2	R233	RN14BK2B4700F	RN	470 Ω	$\pm 1\%$ 1/8W
C-2	R234	RN14BK2B1801F	RN	1.8k Ω	$\pm 1\%$ 1/8W
C-2	R235	RD14BB2C220J	RD	22 Ω	
C-2	R236	RD14BB2C220J	RD	22 Ω	
D-2	R237	RD14BB2C821J	RD	820 Ω	
D-2	R238	RD14BB2C430J	RD	43 Ω	
D-1	R239	RD14BB2C220J	RD	22 Ω	
D-1	R240	RD14BB2C220J	RD	22 Ω	
D-1	R241	RD14BB2C132J	RD	1.3k Ω	
D-1	R242	RD14BB2C392J	RD	3.9k Ω	
D-1	R243	RD14BB2C220J	RD	22 Ω	
D-1	R244	RD14BB2C220J	RD	22 Ω	
D-1	R245	RD14BB2C101J	RD	100 Ω	
D-1	R246	RD14BB2C101J	RD	100 Ω	
D-1	R247	RD14BB2C101J	RD	100 Ω	
D-1	R248	RD14BB2C102J	RD	1k Ω	
D-1	R249	RD14BB2C432J	RD	4.3k Ω	
D-1	R250	RD14BB2C102J	RD	1k Ω	
D-1	R251	RD14BB2C432J	RD	4.3k Ω	
D-1	R252	RD14BB2C101J	RD	100 Ω	
D-1	R253	RD14BB2C101J	RD	100 Ω	
D-1	R254	RD14BB2C101J	RD	100 Ω	
D-1	R255	RD14BB2C220J	RD	22 Ω	
D-1	R256	RD14BB2C220J	RD	22 Ω	
D-1	R257	RD14BB2C132J	RD	1.3k Ω	
D-1	R258	RD14BB2C392J	RD	3.9k Ω	
D-1	R259	RD14BB2C220J	RD	22 Ω	
D-1	R260	RD14BB2C220J	RD	22 Ω	
E-1	R261	RN14BK2B3600F	RN	360 Ω	$\pm 1\%$ 1/8W
E-1	R262	RN14BK2B4700F	RN	470 Ω	$\pm 1\%$ 1/8W
E-1	R263	RN14BK2B4700F	RN	470 Ω	$\pm 1\%$ 1/8W
E-1	R264	RN14BK2B1801F	RN	1.8k Ω	$\pm 1\%$ 1/8W
E-1	R265	RD14BB2C220J	RD	22 Ω	
E-1	R266	RD14BB2C220J	RD	22 Ω	
E-1	R267	RD14BB2C821J	RD	820 Ω	
E-1	R268	RD14BB2C430J	RD	43 Ω	
E-1	R269	RN14BK2B8200F	RN	820 Ω	$\pm 1\%$ 1/8W
E-1	R270	RN14BK2B8200F	RN	820 Ω	$\pm 1\%$ 1/8W
E-1	R271	RD14BB2C391J	RD	390 Ω	
E-1	R272	RN14BK2B1001F	RN	1k Ω	$\pm 1\%$ 1/8W
D-1	R273	RD14BB2C470J	RD	47 Ω	
D-1	R274	RD14BB2C470J	RD	47 Ω	
E-1	R275	RN14BK2B7500F	RN	750 Ω	$\pm 1\%$ 1/8W
D-1	R276	RN14BK2B7500F	RN	750 Ω	$\pm 1\%$ 1/8W
D-1	R277	RD14BB2C221J	RD	220 Ω	
D-1	R278	RD14BB2C273J	RD	27k Ω	
D-1	R279	RD14BB2C103J	RD	10k Ω	
E-1	R280	RN14BK2B2400F	RN	240 Ω	$\pm 1\%$ 1/8W
D-1	R281	RD14BB2C151J	RD	150 Ω	
D-1	R282	RD14BB2C151J	RD	150 Ω	
E-1	R283	RD14BB2C510J	RD	51 Ω	
E-1	R284	RD14BB2C510J	RD	51 Ω	
E-2	R285	RD14BB2C472J	RD	4.7k Ω	
F-2	R286	RD14BB2C103J	RD	10k Ω	
F-2	R287	RD14BB2C103J	RD	10k Ω	
E-2	R288	RD14BB2C103J	RD	10k Ω	
E-2	R289	RD14BB2C103J	RD	10k Ω	
	R290	RD14BB2C103J	RD	10k Ω	
	R291	RD14BB2C272J	RD	2.7k Ω	
C-2	R292	RD14BB2C220J	RD	22 Ω	
	R293	No use			
	R294	No use			
B-1	R295	RD14BB2C103J	RD	10k Ω	
	R296	No use			
	R297	No use			
	R298	No use			
E-2	R299	RD14BB2C222J	RD	2.2k Ω	
E-2	R300	RD14BB2C222J	RD	2.2k Ω	
E-2	R301	RD14BB2C222J	RD	2.2k Ω	
	R302	No use			
	R303	No use			
E-2	R304	RD14BB2C220J	RD	22 Ω	
E-2	R305	RD14BB2C220J	RD	22 Ω	
	R306	RD14BB2C101J	RD	100 Ω	
B-3	R307	RN14BK2B1501F	RN	1.5k Ω	$\pm 1\%$ 1/8W
B-1	R308	RN14BK2B1501F	RN	1.5k Ω	$\pm 1\%$ 1/8W
C-2	R309	No use			
	R310	No use			
	R311	No use			
	R312	No use			
C-2	R313	RD14BB2C471J	RD	470 Ω	
	R314	No use			
E-2	R315	RD14BB2C470J	RD	47 Ω	
E-2	R316	RD14BB2C470J	RD	47 Ω	
B-2	R317	RD14BB2C473J	RD	47k Ω	
B-1	R318	RD14BB2C473J	RD	47k Ω	
A-2	R319	RD14BB2C103J	RD	10k Ω	
A-2	R320	RD14BB2C822J	RD	8.2k Ω	
A-2	R321	RD14BB2C103J	RD	10k Ω	
A-2	R322	RD14BB2C103J	RD	10k Ω	
A-2	R323	RD14BB2C752J	RD	7.5k Ω	
A-2	R324	RD14BB2C332J	RD	3.3k Ω	
B-3	R325	RD14BB2C271J	RD	270 Ω	

PARTS LIST

X73-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
B-2	R326	RD14BB2C271J	RD 270Ω
	R327	No use	
	R328	No use	
	R329	RD14BB2C471J	RD 470Ω
C-3	R330	RD14BB2C100J	RD 10Ω
C-1	R331	RD14BB2C100J	RD 10Ω
C-3	R332	RD14BB2C1R0J	RD 1Ω
D-3	R333	RD14BB2C470J	RD 47Ω
D-1	R334	RD14BB2C470J	RD 47Ω
E-3	VR1	R01-0512-05	VR 500Ω
E-1	VR2	R01-0512-05	VR 500Ω
B-3	VR3	R12-0421-05	VR 100Ω
E-3	VR4	R12-0421-05	VR 100Ω
C-3	VR5	R12-0421-05	VR 100Ω
C-3	VR6	R12-0421-05	VR 100Ω
C-3	VR7	R12-0540-05	VR 500Ω
C-2	VR8	R12-0539-05	VR 200Ω
C-2	VR9	R12-0540-05	VR 500Ω
E-3	VR10	R12-0540-05	VR 500Ω
E-3	VR11	R12-0421-05	VR 100Ω
	VR12	No use	
E-2	VR13	R12-0421-05	VR 100Ω
B-2	VR14	R12-0421-05	VR 100Ω
B-2	VR15	R12-0421-05	VR 100Ω
C-1	VR16	R12-0421-05	VR 100Ω
C-1	VR17	R12-0421-05	VR 100Ω
C-1	VR18	R12-0539-05	VR 200Ω
C-1	VR19	R12-0540-05	VR 500Ω
E-1	VR20	R12-0540-05	VR 500Ω
E-1	VR21	R12-0421-05	VR 100Ω
D-2	VR22	R12-0540-05	VR 500Ω
B-3	C1	CC45CH1H120J	CC 12pF ± 5%
B-3	C2	CC45CH1H220J	CC 22pF ± 5%
B-3	C3	CK45B1H103K	CK 0.01μF ± 10%
B-3	C4	CK45B1H103K	CK 0.01μF ± 10%
B-3	C5	CC45CH1H030C	CC 3pF ± 0.25pF
	C6	No use	
B-2	C7	CK45B1H103K	CK 0.01μF ± 10%
C-2	C8	CK45B1H103K	CK 0.01μF ± 10%
C-3	C9	CC45CH1H330J	CC 33pF ± 5%
	C10	No use	
C-2	C11	CK45B1H222K	CK 2200pF ± 10%
	C12	No use	
D-3	C13	CC45CH1H270J	CC 27pF ± 5%
C-2	C14	CC45CH1H220J	CC 22pF ± 5%
C-3	C15	CK45B1H103K	CK 0.01μF ± 10%
C-2	C16	No use	
	C17	No use	
	C18	No use	
E-3	C19	CC45CH1H150J	CC 15pF ± 5%
E-3	C20	CC45CH1H070D	CC 7pF ± 0.5pF
D-3	C21	CK45B1H102K	CK 1000pF ± 10%
D-3	C22	CC45CH1H220J	CC 22pF ± 5%
E-3	C23	CC45CH1H680J	CC 68pF ± 5%
D-2	C24	CK45B1H103K	CK 0.01μF ± 10%
E-2	C25	CC45CH1H151J	CC 150pF ± 5%
D-2	C26	CC45CH1H151J	CC 150pF ± 5%
D-2	C27	CK45B1H103K	CK 0.01μF ± 10%
E-2	C28	CC45CH1H220J	CC 22pF ± 5%
	C29	No use	
	C30	No use	
E-2	C31	CC45CH1H020C	CC 2pF ± 0.25pF
E-2	C32	CC45CH1H050C	CC 5pF ± 0.25pF
	C33	No use	
D-3	C34	CC45CH1H100J	CC 10pF ± 5%

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
D-1	C35	CC45CH1H100J	CC 10pF ± 5%
E-2	C36	CC45CH1H070D	CC 7pF ± 0.5pF
E-2	C37	CC45CH1H070D	CC 7pF ± 0.5pF
B-2	C38	CC45CH1H270J	CC 27pF ± 5%
B-2	C39	CC45SL1H220J	CC 22pF ± 5%
B-1	C40	CK45B1H103K	CK 0.01μF ± 10%
B-1	C41	CK45B1H103K	CK 0.01μF ± 10%
B-2	C42	CC45CH1H030C	CC 3pF ± 0.25pF
	C43	No use	
C-2	C44	CK45B1H103K	CK 0.01μF ± 10%
C-2	C45	CK45B1H103K	CK 0.01μF ± 10%
C-1	C46	CC45CH1H330J	CC 33pF ± 5%
	C47	No use	
C-1	C48	CK45B1H222K	CK 2200pF ± 10%
	C49	No use	
C-1	C50	CC45CH1H390J	CC 39pF ± 5%
C-1	C51	CC45CH1H220J	CC 22pF ± 5%
C-1	C52	CC45CH1H120J	CC 12pF ± 5%
C-1	C53	CC45CH1H220J	CC 22pF ± 5%
	C54	No use	
	C55	No use	
E-1	C56	CC45CH1H150J	CC 15pF ± 5%
E-1	C57	CC45CH1H070D	CC 7pF ± 0.5pF
D-1	C58	CK45B1H102K	CK 1000pF ± 10%
D-1	C59	CC45CH1H220J	CC 22pF ± 5%
E-1	C60	CC45CH1H680J	CC 68pF ± 5%
B-2	C61	CK45B1H103K	CK 0.01μF ± 10%
B-3	C62	CK45B1H103K	CK 0.01μF ± 10%
B-2	C63	CE04W1C101M	CE 100μF 16WV
B-3	C64	CK45B1H103K	CK 0.01μF ± 10%
B-3	C65	CE04W1C101M	CE 100μF 16WV
B-2	C66	CK45B1H103K	CK 0.01μF ± 10%
C-2	C67	CE04W1C101M	CE 100μF 16WV
C-3	C68	CK45B1H103K	CK 0.01μF ± 10%
C-3	C69	CE04W1H010M	CE 1μF 50WV
C-3	C70	CE04W1C101M	CE 100μF 16WV
C-2	C71	CK45B1H103K	CK 0.01μF ± 10%
C-2	C72	CK45B1H103K	CK 0.01μF ± 10%
C-3	C73	CK45B1H103K	CK 0.01μF ± 10%
C-2	C74	CK45B1H103K	CK 0.01μF ± 10%
C-2	C75	CE04W1C101M	CE 100μF 16WV
C-2	C76	CE04W1C101M	CE 100μF 16WV
D-2	C77	CE04W1C331M	CE 330μF 16WV
D-3	C78	CE04W1C101M	CE 100μF 16WV
E-3	C79	CK45B1H103K	CK 0.01μF ± 10%
E-2	C80	CE04W1C331M	CE 330μF 16WV
E-3	C81	CE04W1C221M	CE 220μF 16WV
F-3	C82	CE04W1C471M	CE 470μF 16WV
E-2	C83	CE04W1C221M	CE 220μF 16WV
F-3	C84	CE04W1C470M	CE 47μF 16WV
B-1	C85	CK45B1H103K	CK 0.01μF ± 10%
D-1	C86	CK45B1H103K	CK 0.01μF ± 10%
B-1	C87	CK45B1H103K	CK 0.01μF ± 10%
B-1	C88	CE04W1C101M	CE 100μF 16WV
B-2	C89	CK45B1H103K	CK 0.01μF ± 10%
B-2	C90	CK45B1H103K	CK 0.01μF ± 10%
B-2	C91	CE04W1C101M	CE 100μF 16WV
B-1	C92	CK45B1H103K	CK 0.01μF ± 10%
B-1	C93	CE04W1C101M	CE 100μF 16WV
C-2	C94	CK45B1H103K	CK 0.01μF ± 10%
C-1	C95	CE04W1H010M	CE 1μF 50WV
C-2	C96	CK45B1H103K	CK 0.01μF ± 10%
C-2	C97	CK45B1H103K	CK 0.01μF ± 10%
C-2	C98	CE04W1C101M	CE 100μF 16WV
C-2	C99	CE04W1C101M	CE 100μF 16WV

PARTS LIST

X73-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description			Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
C-1	C100	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$		C165	No use			
C-1	C101	CE04W1C101M	CE	100 μ F	16WV		C166	No use			
	C102	No use				D-3	C167	CC45CH1H150J	CC	15pF $\pm 5\%$	
C-2	C103	CE04W1H010M	CE	1 μ F	50WV	C-2	C168	CC45CH1H150J	CC	15pF $\pm 5\%$	
D-1	C104	CE04W1C101M	CE	100 μ F	16WV	D-2	C169	CC45CH1H150J	CC	15pF $\pm 5\%$	
F-1	C105	CE04W1C471M	CE	470 μ F	16WV	E-3	C170	CC45CH1H150J	CC	15pF $\pm 5\%$	
E-1	C106	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$	C-2	C171	CC45CH1H150J	CC	15pF $\pm 5\%$	
E-2	C107	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$	E-1	C172	CC45CH1H150J	CC	15pF $\pm 5\%$	
	C108	No use					C173	No use			
F-1	C109	CE04W1C470M	CE	47 μ F	16WV	C-1	C174	CC45CH1H030C	CC	3pF ± 0.25 pF	
F-2	C110	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$		C175	CC45CH1H050C	CC	5pF ± 0.25 pF	
F-1	C111	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$		C176	CC45CH1H050C	CC	5pF ± 0.25 pF	
E-3	C112	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$		C177	CC45CH1H050C	CC	5pF ± 0.25 pF	
	C113	No use					C178	CC45CH1H101J	CC	100pF $\pm 10\%$	
	C114	No use					C179	CC45CH1H101J	CC	100pF $\pm 10\%$	
	C115	CC45CH1H330J	CC	33pF	$\pm 5\%$		C180	CC45CH1H101J	CC	100pF $\pm 10\%$	
	C116	CC45CH1H080D	CC	8pF	± 0.5 pF		C181	CC45CH1H101J	CC	100pF $\pm 10\%$	
D-3	C117	CC45SL1H101J	CC	100pF	$\pm 5\%$	C-2	C182	CK45B1H103K	CK	0.01 μ F $\pm 10\%$	
E-3	C118	CC45SL1H101J	CC	100pF	$\pm 5\%$	C-3	C183	CC45CH1H101J	CC	100pF $\pm 5\%$	
D-2	C119	CC45SL1H101J	CC	100pF	$\pm 5\%$		C184	No use			
B-1	C120	CC45CH1H220J	CC	22pF	$\pm 5\%$		C185	No use			
	C121	No use					C186	No use			
D-2	C122	CC45SL1H101J	CC	100pF	$\pm 5\%$		C187	No use			
E-1	C123	CC45SL1H101J	CC	100pF	$\pm 5\%$		C188	No use			
D-3	C124	CE04W1H010M	CE	1 μ F	50WV		C189	No use			
D-2	C125	C90-0298-05	SCC	0.1 μ F	12WV	C-2	C190	CC45CH1H030C	CC	3pF ± 0.25 pF	
D-2	C126	CC45SL1H101J	CC	100pF	$\pm 5\%$		C191	No use			
F-3	C127	C90-0298-05	SCC	0.1 μ F	12WV		C192	CC45CH1H030C	CC	3pF ± 0.25 pF	
D-2	C128	C90-0298-05	SCC	0.1 μ F	12WV		C193	CC45CH1H030C	CC	3pF ± 0.25 pF	
D-2	C129	C90-0298-05	SCC	0.1 μ F	12WV		C194	CC45CH1H030C	CC	3pF ± 0.25 pF	
F-1	C130	C90-0298-05	SCC	0.1 μ F	12WV		C195	CC45CH1H030C	CC	3pF ± 0.25 pF	
	C131	No use					C196	CC45CH1H030C	CC	3pF ± 0.25 pF	
B-1	C132	CC45CH1H120J	CC	12pF	$\pm 5\%$		C197	CC45CH1H030C	CC	3pF ± 0.25 pF	
	C133	No use					C198	CC45CH1H030C	CC	3pF ± 0.25 pF	
	C134	No use					C199	CC45CH1H030C	CC	3pF ± 0.25 pF	
E-2	C135	CC45CH1H150J	CC	15pF	$\pm 5\%$		C200	CC45CH1H030C	CC	3pF ± 0.25 pF	
E-2	C136	CC45CH1H150J	CC	15pF	$\pm 5\%$		C201	CC45CH1H030C	CC	3pF ± 0.25 pF	
	C137	No use					C202	No use			
	C138	CC45CH1H150J	CC	15pF	$\pm 5\%$		C203	CC45CH1H030C	CC	3pF ± 0.25 pF	
	C139	No use					C204	CC45CH1H030C	CC	3pF ± 0.25 pF	
D-3	C140	CC45CH1H030C	CC	3pF	± 0.25 pF		C205	CC45CH1H030C	CC	3pF ± 0.25 pF	
C-1	C141	CC45CH1H030C	CC	3pF	± 0.25 pF		C206	CC45CH1H030C	CC	3pF ± 0.25 pF	
D-2	C142	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$		C207	CC45CH1H030C	CC	3pF ± 0.25 pF	
B-1	C143	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$	B-3	TC1	C05-0030-15	TC	20pF	
	C144	No use				B-3	TC2	C05-0030-15	TC	20pF	
	C145	No use				D-3	TC3	C05-0030-15	TC	20pF	
D-3	C146	CC45CH1H030C	CC	3pF	± 0.25 pF	D-3	TC4	C05-0030-15	TC	20pF	
D-1	C147	CC45CH1H030C	CC	3pF	± 0.25 pF	B-1	TC5	C05-0030-15	TC	20pF	
	C148	No use				C-3	TC6	C05-0030-15	TC	20pF	
	C149	No use				D-1	TC7	C05-0030-15	TC	20pF	
A-3	C150	C90-0298-05	SCC	0.1 μ F	12WV	D-1	TC8	C05-0030-15	TC	20pF	
	C151	No use				C-2	TC9	C05-0309-15	TC	40pF	
	C152	No use				C-3	TC10	C05-0030-15	TC	20pF	
	C153	No use				C-1	TC11	C05-0030-15	TC	20pF	
	C154	No use				B-3	L1	L40-2201-03	Ferri-inductor	22 μ H	
	C155	No use				B-3	L2	L40-2201-03	Ferri-inductor	22 μ H	
	C156	No use				C-2	L3	L40-2201-03	Ferri-inductor	22 μ H	
	C157	No use					L4	No use			
	C158	No use					L5	No use			
D-2	C159	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$	D-3	L6	L40-2201-03	Ferri-inductor	22 μ H	
E-2	C160	CC45CH1H050C	CC	5pF	± 0.25 pF	B-1	L7	L40-2201-03	Ferri-inductor	22 μ H	
E-2	C161	CC45CH1H050C	CC	5pF	± 0.25 pF	C-2	L8	L40-2201-03	Ferri-inductor	22 μ H	
A-1	C162	C90-0298-05	SCC	0.1 μ F	12WV	C-1	L9	L40-2201-03	Ferri-inductor	22 μ H	
C-2	C163	CC45SL1H470J	CC	47pF	$\pm 5\%$		L10	No use			
	C164	No use				D-1	L11	L40-2201-03	Ferri-inductor	22 μ H	

PARTS LIST

X73-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
D-3	D1		Diode Silicon DS442X
D-1	D2		Diode Silicon DS442X
D-3	D3		Diode Silicon DS442X
D-1	D4		Diode Silicon DS442X
B-2	D5		Diode Silicon DS442X
B-2	D6		Diode Silicon DS442X
D-3	D7		Diode Silicon DS442X
D-3	D8		Diode Silicon DS442X
	D9	No use	
	D10	No use	
D-2	D11		Diode Zener WZ-071
D-2	D12		Diode Zener WZ-071
D-2	D13		Diode Silicon DS442X
E-2	D14		Diode Silicon DS442X
F-2	D15		Diode Silicon DS442X
E-2	D16		Diode Silicon DS442X
E-2	D17		Diode Silicon DS442X
E-2	D18		Diode Silicon DS442X
F-2	D19		Diode Silicon DS442X
E-2	D20		Diode Silicon DS442X
E-2	D21		Diode Silicon DS442X
E-2	D22		Diode Silicon DS442X
E-2	D23		Diode Silicon DS442X
E-2	D24		Diode Silicon DS442X
F-2	D25		Diode Silicon DS442X
F-2	D26		Diode Silicon DS442X
E-2	D27		Diode Silicon DS442X
F-2	D28		Diode Silicon DS442X
F-2	D29		Diode Silicon DS442X
C-3	D30		Diode Silicon DS442X
C-2	D31		Diode Silicon DS442X
E-3	D32		Diode Silicon DS442X
D-2	D33		Diode Silicon DS442X
C-2	D34		Diode Silicon DS442X
E-1	D35		Diode Silicon DS442X
C-3	D36		Diode Zener WZ-061
C-1	D37		Diode Zener WZ-061
	D38	No use	
	D39	No use	
B-3	D40		Diode Silicon 1S2686
B-3	D41		Diode Silicon 1S2686
B-1	D42		Diode Silicon 1S2686
B-1	D43		Diode Silicon 1S2686
A-2	D44		Diode Silicon DS442X
B-3	Q1		TR NPN 2SC536KNP (F)
B-3	Q2		TR NPN 2SC1215 (T or S)
B-2	Q3		TR NPN 2SC1215 (T or S)
C-3	Q4		TR PNP 2SA838 (C)
C-3	Q5		TR PNP 2SA838 (C)
C-3	Q6		TR PNP 2SA838 (C)
C-3	Q7		TR PNP 2SA838 (C)
B-2	Q8		TR PNP 2SA608KS)
C-2	Q9		TR PNP 2SA608KNP (F)
C-3	Q10		TR NPN 2SC1215 (T or S)
C-2	Q11		TR NPN 2SC1215 (T or S)
C-3	Q12		TR NPN 2SC1215 (T or S)
C-2	Q13		TR NPN 2SC1215 (T or S)
C-3	Q14		TR PNP 2SA838 (C)
D-3	Q15		TR NPN 2SC2671
C-2	Q16		TR PNP 2SA838 (C)
C-2	Q17		TR NPN 2SC2671
D-3	Q18		TR NPN 2SC536KNP (F)
D-3	Q19		TR NPN 2SC536KNP (F)
D-2	Q20		TR NPN 2SC536KNP (F)

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
D-2	Q21		TR NPN 2SC536KNP (F)
	Q22	No use	
D-3	Q23		TR NPN 2SC536KNP (F)
D-3	Q24		TR NPN 2SC536KNP (F)
D-3	Q25		TR NPN 2SC536KNP (F)
D-3	Q26		TR NPN 2SC536KNP (F)
E-3	Q27		TR NPN 2SC536KNP (F)
E-3	Q28		TR NPN 2SC1215 (T or S)
E-3	Q29		TR PNP 2SA838 (C)
E-3	Q30		TR NPN 2SC2671
D-3	Q31		TR NPN 2SC1215 (T or S)
D-3	Q32		TR NPN 2SC1215 (T or S)
D-2	Q33		TR PNP 2SA608KNP (F)
D-2	Q34		TR NPN 2SC536KNP (F)
E-2	Q35		TR NPN 2SC1047 (C)
E-2	Q36		TR NPN 2SC1047 (C)
D-2	Q37		TR PNP 2SA608KNP (F)
E-2	Q38		TR NPN 2SC1215 (T or S)
E-2	Q39		TR NPN 2SC1215 (T or S)
D-2	Q40		TR PNP 2SA838 (C)
D-2	Q41		TR NPN 2SC2671
E-2	Q42		TR NPN 2SC1215 (T or S)
E-2	Q43		TR NPN 2SC1215 (T or S)
E-2	Q44		TR PNP 2SA1161
E-2	Q45		TR PNP 2SA1161
B-2	Q46		TR NPN 2SC536KNP (F)
B-2	Q47		TR NPN 2SC536KNP (F)
B-2	Q48		TR NPN 2SC536KNP (F)
B-2	Q49		TR NPN 2SC536KNP (F)
B-1	Q50		TR NPN 2SC1215 (T or S)
B-1	Q51		TR NPN 2SC1215 (T or S)
C-2	Q52		TR PNP 2SA838 (C)
C-1	Q53		TR PNP 2SA838 (C)
C-2	Q54		TR PNP 2SA838 (C)
C-1	Q55		TR PNP 2SA838 (C)
C-2	Q56		TR PNP 2SA608KNP (F)
C-2	Q57		TR PNP 2SA608KNP (F)
C-2	Q58		TR NPN 2SC1215 (T or S)
C-1	Q59		TR NPN 2SC1215 (T or S)
C-1	Q60		TR NPN 2SC1215 (T or S)
C-1	Q61		TR NPN 2SC1215 (T or S)
C-2	Q62		TR PNP 2SA838 (C)
C-2	Q63		TR NPN 2SC2671
D-1	Q64		TR NPN 2SC536KNP (F)
D-2	Q65		TR NPN 2SC536KNP (F)
D-1	Q66		TR NPN 2SC536KNP (F)
D-1	Q67		TR NPN 2SC536KNP (F)
D-1	Q68		TR NPN 2SC536KNP (F)
D-1	Q69		TR NPN 2SC536KNP (F)
D-1	Q70		TR NPN 2SC536KNP (F)
D-1	Q71		TR NPN 2SC536KNP (F)
E-1	Q72		TR NPN 2SC536KNP (F)
E-1	Q73		TR NPN 2SC536KNP (F)
E-1	Q74		TR PNP 2SA838 (C)
E-1	Q75		TR PNP 2SA2671
D-1	Q76		TR NPN 2SC1215 (T or S)
D-1	Q77		TR NPN 2SC1215 (T or S)
E-2	Q78		TR NPN 2SC536KNP (F)
A-2	Q79		TR NPN 2SC536KNP (F)
B-3	IC1		IC Linear CA3102E
B-1	IC2		IC Linear CA3102E
E-3	IC3		IC Digital SN74LS32N
E-2	IC4		IC Digital SN74LS11N
E-2	IC5		IC Digital SN74LS112AN

PARTS LIST

X73-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
E-1	IC6		IC Digital SN74LS08N
E-1	IC7		IC Digital SN74LS00N
A-2	TH1		Thermistor SDT-1000
A-3	P3	E40-0618-05	Pin connector 6P
A-1	P4	E40-0618-05	Pin connector 6P
F-2	P5	E40-1276-05	Pin connector 12P
	P6	No use	
B-2	P7	E40-0576-05	Pin connector 5P
C-2	P8	E40-0576-05	Pin connector 5P
E-2	P9	E40-0376-05	Pin connector 3P
	P10	No use	
E-1	P11	E40-0476-05	Pin connector 4P
E-1	P12	E40-0476-05	Pin connector 4P
	P13	No use	
F-2	P14	E40-0776-05	Pin connector 7P
D-3	P15	E40-0276-05	Pin connector 2P
D-2	P16	E40-0276-05	Pin connector 2P
F-3	P17	E40-0276-05	Pin connector 2P
F-1	P18	E40-0276-05	Pin connector 2P
D-1	P19	E40-0276-05	Pin connector 2P
F-1	P20	E40-0576-05	Pin connector 5P
D-2	P21	E40-0276-05	Pin connector 2P
D-2	TP	E40-0211-05	Pin connector 2P
		L92-0110-05	Core (beads type)

VERTICAL OUTPUT AMPLIFIER UNIT X73-1330-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
E-3	R1	RN14BK2B91ROF	RN 91Ω ±1% 1/8W
E-3	R2	RN14BK2B91ROF	RN 91Ω ±1% 1/8W
E-2	R3	RD14BB2C220J	RD 22Ω
E-3	R4	RD14BB2C220J	RD 22Ω
D-2	R5	RD14BB2C100J	RD 10Ω
	R6	No use	
E-2	R7	RD14BB2C332J	RD 3.3kΩ
E-2	R8	RN14BK2B27ROF	RN 27Ω ±1% 1/8W
D-2	R9	RN14BK2B27ROF	RN 27Ω ±1% 1/8W
D-2	R10	RD14BB2C220J	RD 22Ω
D-3	R11	RD14BB2C220J	RD 22Ω
D-3	R12	RD14BB2C302J	RD 3kΩ
D-2	R13	RD14BB2C122J	RD 1.2kΩ
D-2	R14	RD14BB2C220J	RD 22Ω
D-3	R15	RD14BB2C220J	RD 22Ω
D-2	R16	RN14BK2E6200F	RN 620Ω ±1% 1/4W
D-3	R17	RN14BK2E6200F	RN 620Ω ±1% 1/4W
C-2	R18	RD14BB2C220J	RD 22Ω
C-3	R19	RD14BB2C220J	RD 22Ω
D-3	R20	RD14BB2C470J	RD 47Ω
D-3	R21	RD14BB2C220J	RD 22Ω
D-3	R22	RD14BB2C220J	RD 22Ω
	R23	No use	
	R24	No use	
C-2	R25	RD14BB2C102J	RD 1kΩ
C-3	R26	RD14BB2C822J	RD 8.2kΩ
C-2	R27	RD14BB2E560J	RD 56Ω ±5% 1/4W
C-3	R28	RD14BB2E560J	RD 56Ω ±5% 1/4W
C-3	R29	RS14AB3D820J	RS 82Ω ±5% 2W
C-2	R30	RD14BB2C100J	RD 10Ω
C-3	R31	RD14BB2C100J	RD 10Ω
C-2	R32	RD14BB2C220J	RD 22Ω
C-3	R33	RD14BB2C220J	RD 22Ω
B-2	R34	RD14BB2C471J	RD 470Ω
B-2	R35	RD14BB2C471J	RD 470Ω
	R36	No use	
B-3	R37	RD14BB2C471J	RD 470Ω
B-3	R38	RD14BB2C471J	RD 470Ω
	R39	No use	
B-2	R40	RS14AB3D151J	RS 150Ω ±5% 2W
B-2	R41	RS14AB3D151J	RS 150Ω ±5% 2W
	R42	No use	
E-3	R43	RN14BK2B5601F	RN 5.6kΩ ±1% 1/8W
D-3	R44	RN14BK2B4301F	RN 4.3kΩ ±1% 1/8W
D-3	R45	RN14BK2B1500F	RN 150Ω ±1% 1/8W
B-3	R46	RS14AB3D151J	RS 150Ω ±5% 2W
B-3	R47	RS14AB3D151J	RS 150Ω ±5% 2W
	R48	No use	
E-2	R49	RN14BK2B4700F	RN 470Ω ±1% 1/8W
D-3	R50	RD14BB2C101J	RD 100Ω
	R51	No use	
	R52	No use	
	R53	No use	
D-2	R54	RD14BB2C332J	RD 3.3kΩ
D-3	VR1	R12-0541-05	VR 100Ω
E-3	C1	CK45B1H103K	CK 0.01μF ±10%
	C2	No use	
D-3	C3	CE04W0J102M	CE 1000μF 6.3WV
C-3	C4	CK45B1H103K	CK 0.01μF ±10%
D-2	C5	CK45B1H103K	CK 0.01μF ±10%
D-3	C6	CK45B1H103K	CK 0.01μF ±10%
C-2	C7	CK45B1H103K	CK 0.01μF ±10%
C-2	C8	CK45B1H103K	CK 0.01μF ±10%

PARTS LIST

X73-1330-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
C-3	C9	CK45B2H472K	CK 4700pF ±10% 500WV
E-2	C10	CK45B1H103K	CK 0.01μF ±10%
E-3	C11	CK45B1H103K	CK 0.01μF ±10%
D-2	C12	CE04W1J330M	CE 33μF 63WV
C-2	C13	CK45B2H472K	CK 4700pF ±10% 500WV
F-3	C14	CE04W1V470M	CE 47μF 35WV
F-3	C15	CK45B1H103K	CK 0.01μF ±10%
E-3	C16	CE04W1C470M	CE 47μF 16WV
E-3	C17	CK45B1H103K	CK 0.01μF ±10%
C-2	C18	CC45CH1H070D	CC 7pF ±0.5pF
C-3	C19	CK45B1H152K	CK 1500pF ±10%
E-2	C20	CC45CH1H100D	CC 10pF ±0.5pF
E-2	C21	CE04W1C331M	CE 330μF 16WV
D-2	TC1	C05-0411-05	TC 10pF
	TC2	No use	
C-2	TC3	C05-0414-15	TC 40pF
B-2	L1	L40-2282-13	Ferri-inductor 0.22μH
A-2	L2	L40-2282-13	Ferri-inductor 0.22μH
	L3	No use	
B-3	L4	L40-2282-13	Ferri-inductor 0.22μH
A-3	L5	L40-2282-13	Ferri-inductor 0.22μH
	L6	No use	
D-2	L7	L40-1011-03	Ferri-inductor 100μH
E-2	L8	L40-1011-03	Ferri-inductor 100μH
F-2	L9	L40-1011-03	Ferri-inductor 100μH
E-2	Q1		TR NPN 2SC2499
E-3	Q2		TR NPN 2SC2499
D-2	Q3		TR NPN 2SC2499
D-3	Q4		TR NPN 2SC2499
D-3	Q5		TR NPN 2SC1047 (C)
	Q6	No use	
C-2	Q7		TR NPN 2SC2644
C-3	Q8		TR NPN 2SC2644
C-2	Q9		TR NPN 2SC1164 (O)
C-3	Q10		TR NPN 2SC1164 (O)
D-3	Q11		TR NPN 2SC536KNP (F)
E-3	Q12		TR NPN 2SC536KNP (F)
C-2	Q13		TR NPN 2SC2644
C-3	Q14		TR NPN 2SC2644
F-2	P10	E40-0377-05	Pin connector 3P
F-3	P13	E40-0277-05	Pin connector 2P
E-2	P20	E40-0576-05	Pin connector 5P
E-2	P22	E40-0776-05	Pin connector 7P
		E23-0512-05	Terminal
		F02-0502-05	Heat sink
		L92-0110-05	Core (beads type)

SWEEP ROTARY UNIT X74-1310-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
C-2	R1	RN14BK2B3603F	RN 360kΩ ±1% 1/8W
C-2	R2	RN14BK2B1203F	RN 120kΩ ±1% 1/8W
C-2	R3	RN14BK2B3002F	RN 30kΩ ±1% 1/8W
C-2	R4	RN14BK2B3002F	RN 30kΩ ±1% 1/8W
C-2	R5	RN14BK2B3602F	RN 36kΩ ±1% 1/8W
D-2	R6	RN14BK2B1202F	RN 12kΩ ±1% 1/8W
D-2	R7	RN14BK2B3001F	RN 3kΩ ±1% 1/8W
D-2	R8	RN14BK2B3001F	RN 3kΩ ±1% 1/8W
D-2	R9	RN14BK2B3601F	RN 3.6kΩ ±1% 1/8W
C-2	R10	RD14BB2C124J	RD 120kΩ
C-2	R11	RD14BB2C393J	RD 39kΩ
C-2	R12	RD14BB2C203J	RD 20kΩ
C-2	R13	RD14BB2C123J	RD 12kΩ
D-2	R14	RD14BB2C392J	RD 3.9kΩ
D-2	R15	RD14BB2C202J	RD 2kΩ
D-2	R16	RD14BB2C202J	RD 2kΩ
D-2	R17	RD14BB2C103J	RD 10kΩ
C-1	R18	RD14BB2C103J	RD 10kΩ
C-2	R19	RD14BB2C103J	RD 10kΩ
C-3	R20	RN14BK2B3603F	RN 360kΩ ±1% 1/8W
C-3	R21	RN14BK2B1203F	RN 120kΩ ±1% 1/8W
C-3	R22	RN14BK2B3002F	RN 30kΩ ±1% 1/8W
C-3	R23	RN14BK2B3002F	RN 30kΩ ±1% 1/8W
C-3	R24	RN14BK2B3602F	RN 36kΩ ±1% 1/8W
D-3	R25	RN14BK2B1202F	RN 12kΩ ±1% 1/8W
D-3	R26	RN14BK2B3001F	RN 3kΩ ±1% 1/8W
D-3	R27	RN14BK2B3001F	RN 3kΩ ±1% 1/8W
D-3	R28	RN14BK2B3601F	RN 3.6kΩ ±1% 1/8W
C-3	R29	RD14BB2C124J	RD 120kΩ
C-3	R30	RD14BB2C393J	RD 39kΩ
C-3	R31	RD14BB2C203J	RD 20kΩ
C-3	R32	RD14BB2C123J	RD 12kΩ
D-3	R33	RD14BB2C392J	RD 3.9kΩ
D-3	R34	RD14BB2C202J	RD 2kΩ
D-3	R35	RD14BB2C202J	RD 2kΩ
D-2	R36	RD14BB2C103J	RD 10kΩ
C-2	R37	RD14BB2C103J	RD 10kΩ
C-3	R38	RD14BB2C103J	RD 10kΩ
C-2	C1	CK45B1H103K	CK 0.01μF ±10%
C-2	C2	CK45B1H103K	CK 0.01μF ±10%
C-2	C3	CK45B1H103K	CK 0.01μF ±10%
C-4	C4	CK45B1H103K	CK 0.01μF ±10%
C-2	D1		Diode Silicon GMA-01
C-2	D2		Diode Silicon GMA-01
C-2	D3		Diode Silicon GMA-01
C-2	D4		Diode Silicon GMA-01
D-2	D5		Diode Silicon GMA-01
D-2	D6		Diode Silicon GMA-01
D-2	D7		Diode Silicon GMA-01
	D8	No use	
C-3	D9		Diode Silicon GMA-01
C-3	D10		Diode Silicon GMA-01
C-3	D11		Diode Silicon GMA-01
C-3	D12		Diode Silicon GMA-01
D-3	D13		Diode Silicon GMA-01
D-3	D14		Diode Silicon GMA-01
D-3	D15		Diode Silicon GMA-01
B-3	P15-19	E40-0976-05	Pin connector 9P
		E40-1076-05	Pin connector 10P
B-2	P40	E40-0876-05	Pin connector 8P
B-2	P41	E40-0876-05	Pin connector 8P

PARTS LIST

X74-1310-01

SWEEP UNIT X74-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
C-3	P51	E40-0776-05	Pin connector 7P
B-3	P57	E40-0376-05	Pin connector 3P
		E40-2336-05	Parallel cable

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
	R1	No use	
	R2	No use	
	R3	No use	
	R4	No use	
	R5	RD14BB2C181J	RD 180 Ω
	R6	RD14BB2C332J	RD 3.3k Ω
	R7	RD14BB2C332J	RD 3.3k Ω
A-1	R8	RD14BB2C222J	RD 2.2k Ω
B-1	R9	RD14BB2C470J	RD 47 Ω
B-1	R10	RD14BB2C681J	RD 680 Ω
B-1	R11	RD14BB2C511J	RD 510 Ω
B-2	R12	RD14BB2C511J	RD 510 Ω
D-2	R13	RD14BB2C511J	RD 510 Ω
B-1	R14	RD14BB2C182J	RD 1.8k Ω
B-2	R15	RD14BB2C681J	RD 680 Ω
B-2	R16	RD14BB2C182J	RD 1.8k Ω
B-2	R17	RD14BB2C681J	RD 680 Ω
B-1	R18	RD14BB2C511J	RD 510 Ω
B-2	R19	RD14BB2C181J	RD 180 Ω
B-2	R20	RD14BB2C181J	RD 180 Ω
B-2	R21	RD14BB2C181J	RD 180 Ω
B-2	R22	RD14BB2C332J	RD 3.3k Ω
B-2	R23	RD14BB2C152J	RD 1.5k Ω
B-1	R24	RD14BB2C511J	RD 510 Ω
C-1	R25	RD14BB2C271J	RD 270 Ω
	R26	RD14BB2C472J	RD 4.7k Ω
C-1	R27	RD14BB2C101J	RD 100 Ω
C-1	R28	RD14BB2C103J	RD 10k Ω
C-1	R29	RD14BB2C271J	RD 270 Ω
C-1	R30	RD14BB2C511J	RD 510 Ω
D-1	R31	RD14BB2C361J	RD 360 Ω
D-1	R32	RD14BB2C152J	RD 1.5k Ω
C-2	R33	RD14BB2C511J	RD 510 Ω
	R34	No use	
	R35	No use	
	R36	No use	
	R37	No use	
	R38	No use	
	R39	No use	
C-1	R40	RD14BB2C511J	RD 510 Ω
D-1	R41	RD14BB2C361J	RD 360 Ω
D-1	R42	RD14BB2C220J	RD 22 Ω
D-2	R43	RN14BK2B2401F	RN 2.4k Ω $\pm 1\%$ 1/8W
D-2	R44	RN14BK2B5101F	RN 5.1k Ω $\pm 1\%$ 1/8W
	R45	No use	
	R46	No use	
D-1	R47	RN14BK2B2401F	RN 2.4k Ω $\pm 1\%$ 1/8W
E-1	R48	RD14BB2C123J	RD 12k Ω
E-1	R49	RN14BK2B1502F	RN 15k Ω $\pm 1\%$ 1/8W
E-1	R50	RN14BK2B1202F	RN 12k Ω $\pm 1\%$ 1/8W
E-2	R51	RN14BK2B1002F	RN 10k Ω $\pm 1\%$ 1/8W
E-1	R52	RN14BK2B4302F	RN 43k Ω $\pm 1\%$ 1/8W
E-1	R53	RD14BB2C103J	RD 10k Ω
E-1	R54	RD14BB2C103J	RD 10k Ω
E-2	R55	RN14BK2B3901F	RN 3.9k Ω $\pm 1\%$ 1/8W
E-1	R56	RN14BK2B3901F	RN 3.9k Ω $\pm 1\%$ 1/8W
E-1	R57	RD14BB2C103J	RD 10k Ω
E-2	R58	RD14BB2C104J	RD 100k Ω
E-2	R59	RD14BB2C103J	RD 10k Ω
D-2	R60	RD14BB2C103J	RD 10k Ω
E-2	R61	RD14BB2C104J	RD 100k Ω
D-2	R62	RD14BB2C103J	RD 10k Ω
E-2	R63	RD14BB2C103J	RD 10k Ω
D-2	R64	RD14BB2C104J	RD 100k Ω
D-2	R65	RD14BB2C103J	RD 10k Ω

PARTS LIST

X74-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
E-2	R66	RD14BB2C103J	RD 10 Ω
D-2	R67	RD14BB2C470J	RD 47 Ω
D-2	R68	RD14BB2C101J	RD 100 Ω
D-2	R69	RD14BB2C101J	RD 100 Ω
D-2	R70	RD14BB2C470J	RD 47 Ω
D-2	R71	RD14BB2C470J	RD 47 Ω
D-2	R72	RD14BB2C101J	RD 100 Ω
D-2	R73	RD14BB2C101J	RD 100 Ω
C-2	R74	RD14BB2C242J	RD 2.4k Ω
D-2	R75	RD14BB2C101J	RD 100 Ω
	R76	No use	
D-2	R77	RD14BB2C393J	RD 39k Ω
D-2	R78	RD14BB2C152J	RD 1.5k Ω
C-2	R79	RD14BB2C102J	RD 1k Ω
C-2	R80	RD14BB2C101J	RD 100 Ω
C-1	R81	RD14BB2C511J	RD 510 Ω
C-1	R82	RD14BB2C511J	RD 510 Ω
C-2	R83	RD14BB2C331J	RD 330 Ω
B-1	R84	RD14BB2C511J	RD 510 Ω
C-2	R85	RD14BB2C222J	RD 2.2k Ω
D-1	R86	RD14BB2C100J	RD 10 Ω
C-2	R87	RD14BB2C222J	RD 2.2k Ω
C-2	R88	RD14BB2C273J	RD 27k Ω
C-2	R89	RD14BB2C472J	RD 4.7k Ω
C-2	R90	RD14BB2C102J	RD 1k Ω
C-2	R91	RD14BB2C472J	RD 4.7k Ω
C-2	R92	RD14BB2C302J	RD 3k Ω
C-2	R93	RD14BB2C102J	RD 1k Ω
C-2	R94	RD14BB2C122J	RD 1.2k Ω
C-1	R95	RD14BB2C182J	RD 1.8k Ω
C-1	R96	RD14BB2C152J	RD 1.5k Ω
C-1	R97	RD14BB2C511J	RD 510 Ω
C-2	R98	RN14BK2B5100F	RN 510 Ω $\pm 1\%$ 1/8W
C-2	R99	RD14BB2C221J	RD 220 Ω
	R100	No use	
C-2	R101	RN14BK2B4701F	RN 4.7k Ω $\pm 1\%$ 1/8W
C-2	R102	RN14BK2B4701F	RN 4.7k Ω $\pm 1\%$ 1/8W
C-2	R103	RD14BB2C101J	RD 100 Ω
C-2	R104	RD14BB2C511J	RD 510 Ω
C-3	R105	RD14BB2C511J	RD 510 Ω
C-3	R106	RD14BB2C162J	RD 1.6k Ω
C-3	R107	RD14BB2C222J	RD 2.2k Ω
	R108	No use	
C-1	R109	RD14BB2C102J	RD 1k Ω
D-4	R110	RD14BB2C103J	RD 10k Ω
	R111	No use	
	R112	No use	
C-1	R113	RD14BB2C222J	RD 2.2k Ω
C-4	R114	RD14BB2C222J	RD 2.2k Ω
A-3	R115	RD14BB2C222J	RD 2.2k Ω
B-4	R116	RD14BB2C681J	RD 680 Ω
	R117	RD14BB2C511J	RD 510 Ω
B-4	R118	RD14BB2C470J	RD 47 Ω
B-4	R119	RD14BB2C511J	RD 510 Ω
B-4	R120	RD14BB2C511J	RD 510 Ω
B-4	R121	RD14BB2C511J	RD 510 Ω
B-4	R122	RD14BB2C182J	RD 1.8k Ω
B-4	R123	RD14BB2C681J	RD 680 Ω
B-4	R124	RD14BB2C182J	RD 1.8k Ω
B-4	R125	RD14BB2C681J	RD 680 Ω
B-4	R126	RD14BB2C511J	RD 510 Ω
A-4	R127	RD14BB2C181J	RD 180 Ω
B-4	R128	RD14BB2C181J	RD 180 Ω
B-3	R129	RD14BB2C181J	RD 180 Ω
A-4	R130	RD14BB2C152J	RD 1.5k Ω

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
A-4	R131	RD14BB2C332J	RD 3.3k Ω
B-4	R132	RD14BB2C511J	RD 510 Ω
	R133	No use	
C-4	R134	RD14BB2C101J	RD 100 Ω
C-4	R135	RD14BB2C271J	RD 270 Ω
C-4	R136	RD14BB2C102J	RD 1k Ω
C-4	R137	RD14BB2C271J	RD 270 Ω
C-4	R138	RD14BB2C511J	RD 510 Ω
D-4	R139	RD14BB2C361J	RD 360 Ω
D-4	R140	RD14BB2C152J	RD 1.5k Ω
	R141	No use	
C-4	R142	RD14BB2C511J	RD 510 Ω
D-4	R143	RD14BB2C361J	RD 360 Ω
D-3	R144	RN14BK2B5101F	RN 5.1k Ω $\pm 1\%$ 1/8W
D-3	R145	RN14BK2B7501F	RN 7.5k Ω $\pm 1\%$ 1/8W
B-4	R146	RD14BB2C511J	RD 510 Ω
D-4	R147	RN14BK2B2401F	RN 2.4k Ω $\pm 1\%$ 1/8W
E-4	R148	RD14BB2C123J	RD 12k Ω
E-4	R149	RN14BK2B1502F	RN 15k Ω $\pm 1\%$ 1/8W
E-4	R150	RN14BK2B1202F	RN 12k Ω $\pm 1\%$ 1/8W
E-4	R151	RN14BK2B4302F	RN 43k Ω $\pm 1\%$ 1/8W
E-4	R152	RN14BK2B1002F	RN 10k Ω $\pm 1\%$ 1/8W
E-4	R153	RD14BB2C103J	RD 10k Ω
E-4	R154	RN14BK2B3901F	RN 3.9k Ω $\pm 1\%$ 1/8W
E-4	R155	RN14BK2B3901F	RN 3.9k Ω $\pm 1\%$ 1/8W
E-4	R156	RD14BB2C103J	RD 10k Ω
E-3	R157	RD14BB2C104J	RD 100k Ω
	R158	No use	
E-3	R159	RD14BB2C103J	RD 10k Ω
E-3	R160	RD14BB2C104J	RD 100k Ω
	R161	No use	
E-3	R162	RD14BB2C103J	RD 10k Ω
D-3	R163	RD14BB2C104J	RD 100k Ω
	R164	No use	
E-3	R165	RD14BB2C103J	RD 10k Ω
D-4	R166	RD14BB2C470J	RD 47 Ω
D-3	R167	RD14BB2C101J	RD 100 Ω
D-3	R168	RD14BB2C101J	RD 100 Ω
D-3	R169	RD14BB2C470J	RD 47 Ω
C-3	R170	RD14BB2C472J	RD 4.7k Ω
C-4	R171	RD14BB2C122J	RD 1.2k Ω
C-4	R172	RD14BB2C182J	RD 1.8k Ω
C-4	R173	RD14BB2C152J	RD 1.5k Ω
C-4	R174	RD14BB2C511J	RD 510 Ω
	R175	No use	
	R176	No use	
	R177	No use	
	R178	No use	
	R179	No use	
	R180	No use	
	R181	No use	
	R182	No use	
	R183	No use	
B-4	R184	RD14BB2C511J	RD 510 Ω
	R185	No use	
C-4	R186	RD14BB2C511J	RD 510 Ω
	R187	No use	
C-4	R188	RD14BB2C362J	RD 3.6k Ω
	R189	RD14BB2C102J	RD 1k Ω
C-3	R190	RD14BB2C162J	RD 1.6k Ω
C-3	R191	RD14BB2C362J	RD 3.6k Ω
	R192	No use	
E-4	R193	RD14BB2C103J	RD 10k Ω
D-4	R194	RD14BB2C220J	RD 22 Ω
D-4	R195	RD14BB2C100J	RD 10 Ω

PARTS LIST

X74-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
F-3	R196	RD14BB2C470J	RD 47 Ω
F-3	R197	RD14BB2C470J	RD 47 Ω
F-2	R198	RN14BK2B4701F	RN 4.7k Ω \pm 1% 1/8W
F-2	R199	RD14BB2C472J	RD 4.7k Ω
E-3	R200	RN14BK2B3301F	RN 3.3k Ω \pm 1% 1/8W
E-3	R201	RN14BK2B1201F	RN 1.2k Ω \pm 1% 1/8W
E-2	R202	RD14BB2C392J	RD 3.9k Ω
E-3	R203	RD14BB2C102J	RD 1k Ω
E-2	R204	RD14BB2C132J	RD 1.3k Ω
E-2	R205	RD14BB2C470J	RD 47 Ω
	R206	RN14BK2B3301F	RN 3.3k Ω \pm 1% 1/8W
F-2	R207	RN14BK2B6201F	RN 6.2k Ω \pm 1% 1/8W
E-2	R208	RD14BB2C472J	RD 4.7k Ω
F-2	R209	RD14BB2C472J	RD 4.7k Ω
E-2	R210	RN14BK2B4700F	RN 470 Ω \pm 1% 1/8W
F-2	R211	RN14BK2B4700F	RN 470 Ω \pm 1% 1/8W
E-2	R212	RN14BK2B2201F	RN 2.2k Ω \pm 1% 1/8W
E-2	R213	RD14BB2C621J	RD 620 Ω
F-2	R214	RN14BK2B2201F	RN 2.2k Ω \pm 1% 1/8W
E-2	R215	RN14BK2B1601F	RN 1.6k Ω \pm 1% 1/8W
F-2	R216	RN14BK2B1601F	RN 1.6k Ω \pm 1% 1/8W
F-2	R217	RD14BB2C470J	RD 47 Ω
F-2	R218	RD14BB2C470J	RD 47 Ω
E-1	R219	RN14BK2B1001F	RN 1k Ω \pm 1% 1/8W
E-2	R220	RN14BK2B1001F	RN 1k Ω \pm 1% 1/8W
E-2	R221	RN14BK2B1500F	RN 150 Ω \pm 1% 1/8W
E-1	R222	RN14BK2B1001F	RN 1k Ω \pm 1% 1/8W
E-2	R223	RN14BK2B1001F	RN 1k Ω \pm 1% 1/8W
E-3	R224	RN14BK2B4701F	RN 4.7k Ω \pm 1% 1/8W
E-3	R225	RN14BK2B2001F	RN 2k Ω \pm 1% 1/8W
F-1	R226	RD14BB2C102J	RD 1k Ω
F-2	R227	RD14BB2C102J	RD 1k Ω
F-1	R228	RD14BB2C472J	RD 47k Ω
F-2	R229	RD14BB2C470J	RD 47k Ω
F-2	R230	RD14BB2C470J	RD 47k Ω
F-2	R231	RD14BB2C470J	RD 47k Ω
E-2	R232	RD14BB2C472J	RD 4.7k Ω
E-2	R233	RD14BB2C103J	RD 10k Ω
E-2	R234	RD14BB2C472J	RD 4.7k Ω
E-2	R235	RD14BB2C103J	RD 10k Ω
F-3	R236	RD14BB2C470J	RD 47 Ω
F-3	R237	RN14BK2B4701F	RN 4.7k Ω \pm 1% 1/8W
F-3	R238	RD14BB2C472J	RD 4.7k Ω
E-3	R239	RN14BK2B1201F	RN 1.2k Ω \pm 1% 1/8W
E-3	R240	RN14BK2B3301F	RN 3.3k Ω \pm 1% 1/8W
E-3	R241	RN14BK2B2201F	RN 2.2k Ω \pm 1% 1/8W
C-3	R242	RN14BK2B6801F	RN 6.8k Ω \pm 1% 1/8W
C-2	R243	RN14BK2B6801F	RN 6.8k Ω \pm 1% 1/8W
F-3	R244	RD14BB2C223J	RD 22k Ω
F-3	R245	RD14BB2C102J	RD 1k Ω
F-3	R246	RD14BB2C122J	RD 1.2k Ω
F-3	R247	RD14BB2C751J	RD 750 Ω
F-3	R248	RD14BB2C472J	RD 4.7k Ω
B-2	R249	RD14BB2C511J	RD 510 Ω
B-2	R250	RD14BB2C511J	RD 510 Ω
B-2	R251	RD14BB2C471J	RD 470 Ω
A-2	R252	RD14BB2C101J	RD 100 Ω
A-2	R253	RD14BB2C331J	RD 330 Ω
A-2	R254	RD14BB2C220J	RD 22 Ω
A-2	R255	RD14BB2C272J	RD 2.7k Ω
A-2	R256	RD14BB2C470J	RD 47 Ω
C-3	R257	RD14BB2C2R7J	RD 2.7 Ω
	R258	No use	
B-2	R259	RD14BB2C511J	RD 510 Ω
B-2	R260	RD14BB2C511J	RD 510 Ω

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
B-2	R261	RD14BB2C471J	RD 470 Ω
A-2	R262	RD14BB2C101J	RD 100 Ω
	R263	RD14BB2C331J	RD 330 Ω
A-2	R264	RD14BB2C220J	RD 22 Ω
A-2	R265	RD14BB2C272J	RD 2.7k Ω
A-2	R266	RD14BB2C470J	RD 47 Ω
B-2	R267	RD14BB2C911J	RD 910 Ω
B-2	R268	RD14BB2C432J	RD 4.3k Ω
B-3	R269	RD14BB2C202J	RD 2k Ω
B-3	R270	RD14BB2C102J	RD 1k Ω
B-3	R271	RD14BB2C102J	RD 1k Ω
B-3	R272	RD14BB2C202J	RD 2k Ω
B-2	R273	RD14BB2C222J	RD 2.2k Ω
B-2	R274	RD14BB2C222J	RD 2.2k Ω
B-2	R275	RD14BB2C511J	RD 510 Ω
B-2	R276	RD14BB2C511J	RD 510 Ω
	R277	RD14BB2C561J	RD 560 Ω
	R278	No use	
	R279	No use	
B-2	R280	RD14BB2C511J	RD 510 Ω
	R281	No use	
	R282	No use	
	R283	No use	
	R284	RD14BB2C472J	RD 4.7k Ω
C-2	R285	RD14BB2C222J	RD 2.2k Ω
B-3	R286	RD14BB2C511J	RD 510 Ω
B-2	R287	RD14BB2C220J	RD 22 Ω
A-2	R288	RD14BB2C101J	RD 100 Ω
A-3	R289	RD14BB2C331J	RD 330 Ω
C-2	R290	RD14BB2C152J	RD 1.5k Ω
A-4	R291	RD14BB2C222J	RD 2.2k Ω
	R292	RD14BB2C472J	RD 4.7k Ω
B-3	R293	RD14BB2C222J	RD 2.2k Ω
C-3	R294	RD14BB2C511J	RD 510 Ω
C-3	R295	RD14BB2C220J	RD 22 Ω
C-3	R296	RD14BB2C101J	RD 100 Ω
C-3	R297	RD14BB2C331J	RD 330 Ω
C-3	R298	RD14BB2C220J	RD 22 Ω
C-3	R299	RD14BB2C121J	RD 120 Ω
E-2	R300	RD14BB2C102J	RD 1k Ω
	R301	No use	
E-3	R302	RD14BB2C101J	RD 100 Ω
	R303	No use	
	R304	No use	
E-2	R305	RD14BB2C331J	RD 330 Ω
E-3	R306	RD14BB2C101J	RD 100 Ω
E-3	R307	RD14BB2C220J	RD 22 Ω
E-3	R308	RD14BB2C220J	RD 22 Ω
E-3	R309	RD14BB2C331J	RD 330 Ω
	R310	No use	
D-2	R311	RD14BB2C222J	RD 2.2k Ω
	R312	No use	
	R313	No use	
	R314	No use	
B-3	R315	RD14BB2C222J	RD 2.2k Ω
A-4	R316	RD14BB2C202J	RD 2k Ω
A-3	R317	RD14BB2C202J	RD 2k Ω
B-3	R318	RD14BB2C222J	RD 2.2k Ω
E-1	VR1	R12-3521-05	VR 20k Ω
E-1	VR2	R12-3521-05	VR 20k Ω
E-4	VR3	R12-3521-05	VR 20k Ω
E-4	VR4	R12-3521-05	VR 20k Ω
C-2	VR5	R12-2512-05	VR 5k Ω

PARTS LIST

X74-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
C-2	VR6	R12-0539-05	VR 200Ω
C-2	VR7	R12-1517-05	VR 1kΩ
C-4	VR8	R12-1517-05	VR 1kΩ
F-2	VR9	R12-2512-05	VR 5kΩ
F-3	VR10	R12-2512-05	VR 5kΩ
F-3	VR11	R12-1518-05	VR 2kΩ
F-3	VR12	R12-1518-05	VR 2kΩ
E-1	VR13	R12-0421-05	VR 100Ω
E-2	VR14	R12-0539-05	VR 200Ω
F-3	VR15	R12-2512-05	VR 5kΩ
	C1	No use	
	C2	CE04W1C472M	CE 4700μF 16WV
C-3	C3	CC45SL1H101J	CC 100pF ±5%
C-3	C4	CK45FB1H103K	CK 0.01μF ±5%
B-1	C5	CC45SL1H101J	CC 100pF ±5%
B-2	C6	CE04W1E100M	CE 10μF 25WV
	C7	No use	
B-2	C8	CE04W1E100M	CE 10μF 25WV
D-2	C9	CE04W1H010M	CE 1μF 50WV
E-2	C10	CE04W1V220M	CE 22μF 35WV
D-1	C11	CE04W1H3R3M	CE 3.3μF 50WV
D-2	C12	CK45FB1H103K	CK 0.01μF ±10%
D-2	C13	CE04W1H3R3M	CE 3.3μF 50WV
D-2	C14	C91-0567-05	Polyester 10μF ±10% 100WV
E-2	C15	CK45FB1H103K	CK 0.01μF ±10%
E-2	C16	CK45FB1H103K	CK 0.01μF ±10%
D-2	C17	CQ93BP2A104F	CQ 0.1μF ±1% 100WV
D-2	C18	CK45FB1H103K	CK 0.01μF ±10%
D-2	C19	CQ93M1H333K	CQ 0.033μF ±10%
E-2	C20	CK45FB1H103K	CK 0.01μF ±10%
D-2	C21	CQ93BP2A102F	CQ 1000pF ±1% 100WV
D-2	C22	CK45FB1H103K	CK 0.01μF ±10%
D-2	C23	CC45SL1H331J	CC 330pF ±5%
D-2	C24	CC45SL1H470J	CC 47pF ±5%
D-2	C25	CM93BD2A680J	CM 68pF ±5% 100WV
C-2	C26	CK45FB1H103K	CK 0.01μF ±10%
C-2	C27	CC45CH1H330J	CC 33pF ±5%
C-2	C28	CE04W1E100M	CE 10μF 25WV
C-3	C29	CC45SL1H330J	CC 33pF ±5%
	C30	No use	
	C31	No use	
B-4	C32	CC45SL1H101J	CC 100pF ±5%
B-4	C33	CE04W1E100M	CE 10μF 25WV
B-4	C34	CE04W1E100M	CE 10μF 25WV
	C35	No use	
D-4	C36	CE04W1H3R3M	CE 3.3μF 50WV
D-3	C37	C91-0567-05	Polyester 10μF ±10% 100WV
	C38	No use	
D-3	C39	CQ93BP2A104F	CQ 0.1μF ±1% 100WV
	C40	No use	
D-3	C41	CQ93BP2A102F	CQ 1000pF ±1% 100WV
	C42	No use	
	C43	No use	
D-4	C44	CM93BD2A680J	CM 68pF ±5% 100WV
	C45	No use	
F-3	C46	CK45FB1H103K	CK 0.01μF ±10%
	C47	CE04W1A100M	CE 10μF 10WV
F-2	C48	CE04W1C470M	CE 47μF 16WV
E-2	C49	CK45FB1H103K	CK 0.01μF ±10%
E-2	C50	CK45FB1H103K	CK 0.01μF ±10%
B-2	C51	CC45SL1H331J	CC 330pF ±5%
B-3	C52	CQ93M1H102J	CQ 1000pF ±5%
B-3	C53	CQ93M1H102J	CQ 1000pF ±5%
C-2	C54	CE04W1H010M	CE 1μF 50WV

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
C-2	C55	CK45FB1H103K	CK 0.01μF ±10%
	C56	No use	
	C57	CC45SL1H470J	CC 47pF ±5%
	C58	No use	
F-4	C59	CK45FB1H103K	CK 0.01μF ±10%
F-4	C60	CK45FB1H103K	CK 0.01μF ±10%
F-4	C61	CK45FB1H103K	CK 0.01μF ±10%
F-4	C62	CK45FB1H103K	CK 0.01μF ±10%
D-2	C63	CK45FB1H103K	CK 0.01μF ±10%
E-1	C64	CK45B2H472K	CK 4700pF ±10% 500WV
D-1	C65	CK45FB1H103K	CK 0.01μF ±10%
F-4	C66	CK45B2H472K	CK 4700pF ±10% 500WV
D-4	C67	CE04W1V220M	CE 22μF 35WV
A-2	C68	CK45FB1H103K	CK 0.01μF ±10%
A-2	C69	CK45FB1H103K	CK 0.01μF ±10%
A-4	C70	CK45FB1H103K	CK 0.01μF ±10%
D-1	C71	CK45B1H103K	CK 0.01μF ±10%
E-4	C72	CK45FB2H472K	CK 4700pF ±10% 500WV
D-4	C73	CK45FB1H103K	CK 0.01μF ±10%
B-2	C74	CK45FB1H103K	CK 0.01μF ±10%
	C75	No use	
	C76	No use	
B-1	C77	C90-0298-05	SCC 0.1μF 12WV
B-1	C78	C90-0298-05	SCC 0.1μF 12WV
C-1	C79	C90-0298-05	SCC 0.1μF 12WV
B-2	C80	C90-0298-05	SCC 0.1μF 12WV
B-2	C81	C90-0298-05	SCC 0.1μF 12WV
C-2	C82	C90-0298-05	SCC 0.1μF 12WV
B-3	C83	C90-0298-05	SCC 0.1μF 12WV
B-3	C84	C90-0298-05	SCC 0.1μF 12WV
C-3	C85	C90-0298-05	SCC 0.1μF 12WV
B-3	C86	C90-0298-05	SCC 0.1μF 12WV
B-3	C87	C90-0298-05	SCC 0.1μF 12WV
C-3	C88	C90-0298-05	SCC 0.1μF 12WV
B-2	C89	C90-0298-05	SCC 0.1μF 12WV
	C90	No use	
	C91	No use	
B-1	C92	CE04W1A101M	CE 100μF 10WV
B-2	C93	CE04W1A101M	CE 100μF 10WV
B-3	C94	CE04W1A470M	CE 47μF 10WV
B-3	C95	CE04W1A101M	CE 100μF 10WV
	C96	No use	
F-4	C97	CE04W1A221M	CE 220μF 10WV
D-2	C98	CE04W1C470M	CE 47μF 16WV
D-3	C99	CE04W1C470M	CE 47μF 16WV
C-2	C100	CE04W1C470M	CE 47μF 16WV
C-3	C101	CE04W1C331M	CE 330μF 16WV
F-3	C102	CE04W1C101M	CE 100μF 16WV
F-4	C103	CE04W1C101M	CE 100μF 16WV
D-2	C104	CE04W1E220M	CE 22μF 25WV
D-3	C105	CE04W1E330M	CE 33μF 25WV
D-3	C106	CE04W1E220M	CE 22μF 25WV
F-3	C107	CE04W1E101M	CE 100μF 25WV
	C108	No use	
	C109	No use	
E-1	C110	CE04W1J100M	CE 10μF 63WV
E-4	C111	CE04W1J100M	CE 10μF 63WV
F-2	C112	CE04W1C330M	CE 33μF 16WV
F-2	C113	CE04W1E220M	CE 22μF 25WV
A-4	C114	CE04W1C330M	CE 33μF 16WV
A-2	C115	CE04W1C330M	CE 33μF 16WV
D-3	C116	CE04W1H010M	CE 1μF 50WV
	C117	No use	
	C118	No use	
	C119	No use	

PARTS LIST

X74-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description			Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
	C120	No use				E-2	Q29		TR	PNP	2SA838 (C)
E-3	C121	CK45FB1H103K	CK	0.01 μ F	\pm 10%	E-3	Q30		TR	PNP	2SA838 (C)
E-3	C122	CK45FB1H103K	CK	0.01 μ F	\pm 10%		Q31	No use			
E-3	C123	CK45FB1H103K	CK	0.01 μ F	\pm 10%	B-4	Q32		TR	NPN	2SC536KNP (F)
	C124	No use				A-4	Q33		TR	NPN	2SC536KNP (F)
	C125	No use				C-4	Q34		TR	PNP	2SA838 (C)
	C126	No use				D-4	Q35		TR	NPN	2SC1215 (T or S)
A-1	C127	C90-0298-05	SCC	0.1 μ F	12WV	D-4	Q36		TR	NPN	2SC1973 (T)
A-4	C128	C90-0298-05	SCC	0.1 μ F	12WV	D-4	Q37		TR	PNP	2SA838 (C)
A-2	C129	CE04W1C330M	CE	33 μ F	16WV	E-4	Q38		TR	NPN	2SD438 (F)
	C130	CC45SL1H390J	CC	39pF	\pm 5%	E-4	Q39		TR	NPN	2SC536KNP (F)
						E-4	Q40		TR	NPN	2SC536KNP (F)
D-1	TC1	C05-0030-15	TC	20pF		E-4	Q41		TR	NPN	2SC536KNP (F)
D-4	TC2	C05-0030-15	TC	20pF			Q42	No use			
C-2	TC3	C05-0062-05	TC	6pF		E-3	Q43		TR	NPN	2SC536KNP (F)
C-3	TC4	C05-0006205	TC	6pF			Q44	No use			
						E-3	Q45		TR	NPN	2SC536KNP (F)
D-2	L1	L40-1001-01	Ferri-inductor	10 μ H			Q46	No use			
D-4	L2	L40-1001-01	Ferri-inductor	10 μ H		E-3	Q47		TR	NPN	2SC536KNP (F)
						D-4	Q48		FET	Dual	M74F (C)
B-1	IC1		IC	Digital	MC10103L	D-3	Q49		TR	NPN	2SC1047 (C)
B-1	IC2		IC	Digital	MC10131L		Q50	No use			
D-1	IC3		IC	Linear	TL082CP	D-3	Q51		FET	Dual	M74F (C)
B-4	IC4		IC	Digital	MC10103L		Q52	No use			
B-4	IC5		IC	Digital	MC10131L	F-2	Q53		TR	NPN	2SC536KNP (F)
D-4	IC6		IC	Linear	TL082CP	F-3	Q54		TR	NPN	2SC536KNP (F)
C-1	IC7		IC	Digital	MC10104L	E-3	Q55		TR	NPN	2SC1047 (C)
C-2	IC8		IC	Digital	MC10103L	E-3	Q56		TR	NPN	2SC1047 (C)
	IC9	No use				E-3	Q57		TR	NPN	2SC1047 (C)
C-4	IC10		IC	Digital	MC10104L	E-3	Q58		TR	NPN	2SC1047 (C)
B-2	IC11		IC	Digital	MC10104L	E-3	Q59		TR	NPN	2SC1047 (C)
B-3	IC12		IC	Digital	MC10102L	E-2	Q60		TR	NPN	2SC1047 (C)
B-2	IC13		IC	Digital	MC10131L	F-2	Q61		TR	NPN	2SC1047 (C)
A-3	IC14		IC	Digital	SN7405N	E-2	Q62		TR	PNP	2SA838 (C)
B-3	IC15		IC	Digital	MC10104L	F-2	Q63		TR	PNP	2SA838 (C)
D-2	IC16		IC	Regulator	MC78L15CP		Q64	No use			
	Q1	No use					Q65	No use			
	Q2	No use					Q66	No use			
B-2	Q3		TR	NPN	2SC536KNP (F)		Q67	No use			
B-2	Q4		TR	NPN	2SC536KNP (F)	E-2	Q68		TR	NPN	2SC536KNP (F)
C-1	Q5		TR	PNP	2SA838 (C)	E-2	Q69		TR	NPN	2SC536KNP (F)
D-1	Q6		TR	NPN	2SC1215 (T or S)	F-1	Q70		TR	NPN	2SC1047 (C)
D-1	Q7		TR	NPN	2SC1973 (T)	F-2	Q71		TR	NPN	2SC1047 (C)
D-1	Q8		TR	PNP	2SA838 (C)	A-2	Q72		TR	PNP	2SA838 (C)
E-1	Q9		TR	NPN	2SD438 (F)	A-2	Q73		TR	NPN	2SC1215 (T or S)
E-1	Q10		TR	NPN	2SC536KNP (F)	A 2	Q74		TR	PNP	2SA838 (C)
E-2	Q11		TR	NPN	2SC536KNP (F)	A-2	Q75		TR	NPN	2SC1215 (T or S)
E-1	Q12		TR	NPN	2SC536KNP (F)		Q76	No use			
D-2	Q13		TR	NPN	2SC536KNP (F)	A-3	Q77		TR	PNP	2SA838 (C)
E-2	Q14		TR	NPN	2SC536KNP (F)	C-3	Q78		TR	PNP	2SA838 (C)
D-2	Q15		TR	NPN	2SC536KNP (F)	C-3	Q79		TR	NPN	2SC536KNP (F)
E-2	Q16		TR	NPN	2SC536KNP (F)	C-2	Q80		TR	PNP	2SA838 (C)
D-2	Q17		TR	NPN	2SC536KNP (F)	C-2	Q81		TR	NPN	2SC536KNP (F)
E-2	Q18		TR	NPN	2SC536KNP (F)						
D-2	Q19		FET	Dual	M74F (C)	A-1	D1		Diode	Varistor	SV-03Y
D-2	Q20		TR	NPN	2SC1047 (C)	B-2	D2		Diode	Silicon	GMA-01
D-2	Q21		FET	Dual	M74F (C)	C-2	D3		Diode	Silicon	GMA-01
C-2	Q22		TR	PNP	2SA838 (C)		D4		Diode	Silicon	GMA-01
D-2	Q23		TR	NPN	2SC1407 (C)	C-1	D5		Diode	Silicon	GMA-01
C-2	Q24		TR	NPN	2SC536KNP (F)	C-1	D6		Diode	Silicon	DS442X
C-2	Q25		TR	NPN	2SC536KNP (F)	C-1	D7		Diode	Silicon	DS442X
C-2	Q26		TR	NPN	2SC536KNP (F)	D-1	D8		Diode	Silicon	GMA-01
	Q27	No use				D-1	D9		Diode	Silicon	GMA-01
	Q28	No use				D-1	D10		Diode	Silicon	GMA-01
							D11		Diode	Silicon	GMA-01

PARTS LIST

X74-1320-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
E-1	D12		Diode	Zener	WZ-150
E-1	D13		Diode	Silicon	DS442X
	D14	No use			
D-2	D15		Diode	Silicon	GMA-01
C-2	D16		Diode	Silicon	GMA-01
	D17		Diode	Zener	YZ-030
	D18		Diode	Silicon	GMA-01
A-4	D19		Diode	Varistor	SV-03Y
B-4	D20		Diode	Silicon	GMA-01
	D21		Diode	Silicon	GMA-01
	D22		Diode	Silicon	GMA-01
C-4	D23		Diode	Silicon	GMA-01
C-4	D24		Diode	Silicon	DS442X
C-4	D25		Diode	Silicon	GS442X
D-4	D26		Diode	Silicon	GMA-01
	D27	No use			
E-4	D28		Diode	Zener	WZ-150
E-4	D29		Diode	Silicon	DS442X
	D30	No use			
	D31	No use			
A-3	D32		Diode	Silicon	GMA-01
E-3	D33		Diode	Silicon	GMA-01
E-3	D34		Diode	Silicon	GMA-01
E-3	D35		Diode	Silicon	GMA-01
E-3	D36		Diode	Silicon	GMA-01
E-2	D37		Diode	Zener	WZ-120
E-2	D38		Diode	Zener	WZ-120
	D39	No use			
B-3	D40		Diode	Silicon	GMA-01
B-3	D41		Diode	Silicon	GMA-01
B-3	D42		Diode	Silicon	GMA-01
B-3	D43		Diode	Silicon	GMA-01
	D44		Diode	Silicon	DS442X
	D45		Diode	Varistor	SV-06Y
A-3	D46		Diode	Silicon	GMA-01
	D47		Diode	Silicon	DS442X
A-3	D48		Diode	Silicon	GMA-01
A-3	D49		Diode	Silicon	GMA-01
A-3	D50		Diode	Silicon	GMA-01
C-3	D51		Diode	Zener	WZ-100
C-2	D52		Diode	Silicon	GMA-01
E-3	D53		Diode	Silicon	GMA-01
E-3	D54		Diode	Silicon	GMA-01
D-4	D55		Diode	Silicon	GMA-01
D-4	D56		Diode	Silicon	GMA-01
C-4	D57		Diode	Silicon	GMA-01
A-3	D58		Diode	Silicon	GMA-01
C-2	D59		Diode	Silicon	DS442X
A-3	D60		Diode	Silicon	GMA-01
A-3	D61		Diode	Silicon	GMA-01
B-3	D62		Diode	Silicon	GMA-01
B-1	D63		Diode	Silicon	GMA-01
E-1	D64		Diode	Silicon	GMA-01
E-1	D65		Diode	Varistor	SV-06Y
E-1	D66		Diode	Silicon	GMA-01
C-3	P13	E40-0276-05	Pin connector		2P
A-3	P14	E40-0776-05	Pin connector		7P
A-2	P28	E40-0476-05	Pin connector		4P
F-1	P35	E40-0476-05	Pin connector		4P
F-2	P37	E40-0776-05	Pin connector		7P
C-2	P38	E40-0376-05	Pin connector		3P
D-2	P39	E40-0776-05	Pin connector		7P
E-2	P40	E40-0876-05	Pin connector		8P
E-3	P41	E40-0876-05	Pin connector		8P

Fig. & Index No.	Ref. No.	Parts No.	Name & Description	
	P42	No use		
F-2	P43	E40-0276-05	Pin connector	2P
A-4	P44	E40-0276-05	Pin connector	2P
E-4	P45	E40-0676-05	Pin connector	6P
A-1	P46	E40-0276-05	Pin connector	2P
E-4	P47	E40-0476-05	Pin connector	4P
A-3	P48	E40-1811-05	Pin connector	18P
F-4	P49	E40-0676-05	Pin connector	6P
	P50	No use		
D-2	P57	E40-0376-05	Pin connector	3P

PARTS LIST

HORIZONTAL OUTPUT AMPLIFIER UNIT X74-1230-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
C-1	R1	RD14BB2C272J	RD	2.7k Ω	
C-3	R2	RD14BB2C272J	RD	2.7k Ω	
C-2	R3	RD14BB2C470J	RD	47 Ω	
C-3	R4	RD14BB2C470J	RD	47 Ω	
C-2	R5	RD14BB2C152J	RD	1.5k Ω	
C-2	R6	RD14BB2H473J	RD	47k Ω	$\pm 5\%$ 1/2W
C-2	R7	RD14BB2H473J	RD	47k Ω	$\pm 5\%$ 1/2W
D-2	R8	RD14BB2C821J	RD	820 Ω	
C-2	R9	RD14BB2C821J	RD	820 Ω	
D-2	R10	RD14BB2C102J	RD	1k Ω	
D-2	R11	RD14BB2C102J	RD	1k Ω	
	R12	No use			
	R13	No use			
C-1	R14	RS14GB3A223J	RS	22k Ω	$\pm 5\%$ 1W
C-3	R15	RS14GB3A223J	RS	22k Ω	$\pm 5\%$ 1W
D-1	R16	RD14BB2C134J	RD	130k Ω	
D-3	R17	RD14BB2C134J	RD	130k Ω	
E-2	R18	RD14BY2H123J	RD	12k Ω	$\pm 5\%$ 1/2W
E-2	R19	RD14BB2C102J	RD	1k Ω	
E-2	R20	RD14BB2C102J	RD	1k Ω	
E-1	R21	RD14BB2C220J	RD	22 Ω	
E-3	R22	RD14BB2C220J	RD	22 Ω	
F-2	R23	RD14BB2C471J	RD	470 Ω	
E-2	R24	RD14BB2C471J	RD	470 Ω	
	R25	No use			
B-2	R26	RD14BB2C472J	RD	4.7k Ω	
B-2	R27	RD14BB2C472J	RD	4.7k Ω	
B-2	R28	RD14BB2C271J	RD	270 Ω	
B-2	R29	RD14BB2C512J	RD	5.1k Ω	
C-2	C1	CK45B2H472K	CK	4700pF	$\pm 10\%$ 500WV
D-2	C2	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$
	C3	No use			
	C4	No use			
D-2	C5	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$
D-2	C6	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$
	C7	No use			
	C8	No use			
C-3	C9	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$
C-1	C10	CC45CH2H010C	CC	1pF	± 0.25 pF500WV
D-1	C11	CC45CH2H010C	CC	1pF	± 0.25 pF500WV
C-3	C12	CC45CH2H010C	CC	1pF	± 0.25 pF500WV
D-3	C13	CC45CH2H010C	CC	1pF	± 0.25 pF500WV
B-3	C14	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$
E-2	C15	CK45B2H472K	CK	4700pF	$\pm 10\%$ 500WV
E-2	C16	CK45B2H472K	CK	4700pF	$\pm 10\%$ 500WV
D-2	C17	CK45B2H472K	CK	4700pF	$\pm 10\%$ 500WV
D-3	C18	C92-0549-05	Tantalum	1 μ F	35WV
E-2	C19	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$
E-2	C20	C91-0549-05	Tantalum	1 μ F	35WV
F-2	C21	CK45B2H472K	CK	4700pF	$\pm 10\%$ 500WV
B-2	C22	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$
B-2	C23	CE04W1C101M	CE	100 μ F	16WV
B-3	C24	CE04W1C101M	CE	100 μ F	16WV
	C25	No use			
B-2	C26	CE04W2A100M	CE	10 μ F	100WV
D-2	C27	CE04W2C2R2M	CE	2.2 μ F	160WV
D-2	C28	CK45B1H103K	CK	0.01 μ F	$\pm 10\%$
B-2	L1	L40-1011-04	Ferri-inductor	100 μ H	
B-3	L2	L40-1011-04	Ferri-inductor	100 μ H	
	L3	No use			
B-2	L4	L40-1011-04	Ferri-inductor	100 μ H	

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
B-3	L5	L40-1011-04	Ferri-inductor	100 μ H	
	D1	No use			
	D2	No use			
	D3	No use			
	D4	No use			
	D5	No use			
	D6	No use			
	D7	No use			
	D8	No use			
E-2	D9		Diode	Silicon	DS442X
E-2	D10		Diode	Silicon	DS442X
E-2	D11		Diode	Silicon	DS442X
	D12	No use			
E-2	D13		Diode	Zener	WZ-050
C-2	Q1		TR	PNP	2SA838 (C)
C-2	Q2		TR	PNP	2SA838 (C)
	Q3	No use			
	Q4	No use			
D-2	Q5		TR	PNP	2SA838 (C)
D-2	Q6		TR	PNP	2SA838 (C)
D-1	Q7		TR	NPN	2SC805A-2 (2, 3)
D-3	Q8		TR	NPN	2SC805A-2 (2, 3)
E-1	Q9		TR	PNP	2SA923-2 (2, 3)
E-3	Q10		TR	PNP	2SA923-2 (2, 3)
B-2	Q11		TR	NPN	2SC536KNP (F)
B-2	Q12		TR	NPN	2SC536KNP (F)
		E31-0747-05	Lead wire with connector		
B-2	P27	E40-0876-05	Pin connector	8P	
B-1	P35	E40-0476-05	Pin connector	4P	
B-1	P36	E40-0676-05	Pin connector	6P	

PARTS LIST

HORIZONTAL MODE CONTROL UNIT X-77-1130-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
B-1	R1	RD14BB2C393J	RD 39k Ω
B-1	R2	RD14BB2C393J	RD 39k Ω
B-1	R3	RD14BB2C393J	RD 39k Ω
B-1	R4	RD14BB2C393J	RD 39k Ω
	R5	No use	
B-1	R6	RD14BB2C393J	RD 39k Ω
B-2	R7	RD14BB2C824J	RD 820k Ω
B-1	R8	RD14BB2C393J	RD 39k Ω
B-2	R9	RD14BB2C824J	RD 820k Ω
B-1	R10	RD14BB2C393J	RD 39k Ω
B-2	R11	RD14BB2C824J	RD 820k Ω
B-1	R12	RD14BB2C393J	RD 39k Ω
B-1	R13	RD14BB2C473J	RD 47k Ω
B-1	R14	RD14BB2C473J	RD 47k Ω
B-1	R15	RD14BB2C184J	RD 180k Ω
C-1	R16	RD14BB2C391J	RD 390 Ω
C-1	R17	RD14BB2C391J	RD 390 Ω
C-1	R18	RD14BB2C391J	RD 390 Ω
C-1	R19	RD14BB2C391J	RD 390 Ω
	R20	No use	
C-1	R21	RD14BB2C391J	RD 390 Ω
C-2	R22	RD14BB2C393J	RD 39k Ω
C-2	R23	RD14BB2C393J	RD 39k Ω
C-2	R24	RD14BB2C393J	RD 39k Ω
C-2	R25	RD14BB2C393J	RD 39k Ω
B-2	R26	RD14BB2C824J	RD 820k Ω
B-2	R27	RD14BB2C393J	RD 39k Ω
A-2	R28	RD14BB2C824J	RD 820k Ω
B-2	R29	RD14BB2C393J	RD 39k Ω
B-2	R30	RD14BB2C824J	RD 820k Ω
B-2	R31	RD14BB2C393J	RD 39k Ω
B-1	R32	RD14BB2C473J	RD 47k Ω
B-1	R33	RD14BB2C473J	RD 47k Ω
B-1	R34	RD14BB2C184J	RD 180k Ω
C-2	R35	RD14BB2C391J	RD 390 Ω
C-2	R36	RD14BB2C391J	RD 390 Ω
C-2	R37	RD14BB2C391J	RD 390 Ω
C-2	R38	RD14BB2C562J	RD 5.6k Ω
C-2	R39	RD14BB2C562J	RD 5.6k Ω
C-2	R40	RD14BB2C562J	RD 5.6k Ω
C-2	R41	RD14BB2C184J	RD 180k Ω
C-2	R42	RD14BB2C223J	RD 22k Ω
C-1	R43	RD14BB2C473J	RD 47k Ω
E-1	R44	RD14BB2C103J	RD 10k Ω
D-2	R45	RD14BB2C472J	RD 4.7k Ω
D-2	R46	RD14BB2C332J	RD 3.3k Ω
D-2	R47	RD14BB2C272J	RD 2.7k Ω
D-2	R48	RD14BB2C331J	RD 330 Ω
C-2	R49	RD14BB2C561J	RD 560 Ω
D-2	R50	RD14BB2C272J	RD 2.7k Ω
D-2	R51	RD14BB2C222J	RD 2.2k Ω
	R52	No use	
	R53	No use	
	R54	No use	
	R55	No use	
	R56	No use	
	R57	No use	
	R58	No use	
	R59	No use	
	R60	No use	
	R61	No use	
	R62	No use	
	R63	No use	
	R64	No use	
	R65	No use	

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
	R66	No use	
	R67	No use	
	R68	No use	
	R69	No use	
E-1	R70	RN14BK2B3600F	RN 360 Ω \pm 1% 1/8W
E-1	R71	RN14BK2B30R0F	RN 30 Ω \pm 1% 1/8W
	R72	No use	
E-1	R73	RD14BB2C223J	RD 22k Ω
E-1	R74	RD14BB2C103J	RD 10k Ω
E-1	R75	RD14BB2C103J	RD 10k Ω
E-1	R76	RN14BK2B1003F	RN 100k Ω \pm 1% 1/8W
E-1	R77	RN14BK2B9102F	RN 91k Ω \pm 1% 1/8W
E-1	R78	RD14BB2C472J	RD 4.7k Ω
A-3	R79	RD14BB2E470J	RD 47 Ω \pm 5% 1/4W
	R80	No use	
	R81	No use	
	R82	No use	
B-3	R83	RN14BK2H1004F	RN 1M Ω \pm 1% 1/2W
	R84	RD14BB2C104J	RD 100k Ω
B-2	R85	RD14BB2C101J	RD 100 Ω
B-2	R86	RN14BK2B2701F	RN 2.7k Ω \pm 1% 1/8W
B-2	R87	RN14BK2B2701F	RN 2.7k Ω \pm 1% 1/8W
B-2	R88	RD14BB2C220J	RD 22 Ω
B-2	R89	RD14BB2C220J	RD 22 Ω
B-2	R90	RD14BB2C220J	RD 22 Ω
B-2	R91	RN14BK2B8200F	RN 820 Ω \pm 1% 1/8W
B-2	R92	RN14BK2B8200F	RN 820 Ω \pm 1% 1/8W
B-2	R93	RD14BB2C220J	RD 22 Ω
A-2	R94	RN14BK2B39R0F	RN 39 Ω \pm 1% 1/8W
A-2	R95	RN14BK2B39R0F	RN 39 Ω \pm 1% 1/8W
A-2	R96	RD14BB2C122J	RD 1.2k Ω
C-3	R97	RD14BB2E470J	RD 47 Ω \pm 5% 1/4W
	R98	No use	
	R99	No use	
	R100	No use	
C-3	R101	RN14BK2H1004F	RN 1M Ω \pm 1% 1/2W
C-2	R102	RD14BB2C104J	RD 100k Ω
B-2	R103	RD14BB2C101J	RD 100 Ω
B-2	R104	RN14BK2B2701F	RN 2.7k Ω \pm 1% 1/8W
B-2	R105	RN14BK2B2701F	RN 2.7k Ω \pm 1% 1/8W
B-2	R106	RD14BB2C220J	RD 22 Ω
B-2	R107	RD14BB2C220J	RD 22 Ω
B-2	R108	RD14BB2C220J	RD 22 Ω
B-2	R109	RN14BK2B8200F	RN 820 Ω \pm 1% 1/8W
B-2	R110	RN14BK2B8200F	RN 820 Ω \pm 1% 1/8W
B-2	R111	RD14BB2C220J	RD 22 Ω
C-2	R112	RN14BK2B39R0F	RN 39 Ω \pm 1% 1/8W
C-2	R113	RN14BK2B39R0F	RN 39 Ω \pm 1% 1/8W
	R114	No use	
	R115	No use	
	R116	No use	
C-1	R117	RD14BB2C472J	RD 4.7k Ω
D-1	R118	RD14BB2C472J	RD 4.7k Ω
C-1	R119	RD14BB2C472J	RD 4.7k Ω
C-1	R120	RD14BB2C563J	RD 56k Ω
	R200	RD14BB2C561J	RD 560 Ω
E-1	VR1	R12-0542-05	VR 200 Ω
E-1	VR2	R12-5517-05	VR 100k Ω
B-1	C1	CC45SL1H101J	CC 100pF \pm 5%
A-1	C2	CC45SL1H101J	CC 100pF \pm 5%
A-1	C3	CC45SL1H101J	CC 100pF \pm 5%

PARTS LIST

X77-1130-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description			Fig. & Index No.	Ref. No.	Parts No.	Name & Description			
A-1	C4	CC45SL1H101J	CC	100pF	±5%	C-2	IC7		IC	Digital	MC14013BCP	
	C5	No use				D-2	IC8		IC	Digital	MC14011BCP	
B-1	C6	CC45SL1H101J	CC	100pF	±5%	E-2	IC9		IC	Digital	SN74LS04N	
B-1	C7	CK45FB1H103K	CK	0.01μF	±10%		IC10	No use				
C-2	C8	CC45SL1H101J	CC	100pF	±5%		IC11	No use				
C-2	C9	CC45SL1H101J	CC	100pF	±5%		IC12	No use				
C-2	C10	CC45SL1H101J	CC	100pF	±5%		IC13	No use				
C-2	C11	CC45SL1H101J	CC	100pF	±5%		IC14	No use				
B-1	C12	CK45FB1H103K	CK	0.01μF	±10%		IC15	No use				
E-2	C13	CK45FB1H103K	CK	0.01μF	±10%		IC16	No use				
D-1	C14	CK45FB1H103K	CK	0.01μF	±10%	E-2	IC17		IC	Regulator	MC78L05C	
D-1	C15	CE04W1C471M	CE	470μF	16WV							
	C16	No use				B-1	D1		Diode	Silicon	DS442X	
	C17	No use				B-1	D2		Diode	Silicon	DS442X	
	C18	No use					D3	No use				
	C19	No use				B-1	D4		Diode	Silicon	DS442X	
	C20	No use				B-1	D5		Diode	Silicon	DS442X	
	C21	No use				B-1	D6		Diode	Silicon	DS442X	
E-1	C22	CC45SL1H471J	CC	470pF	±5%	A-1	D7		Diode	Silicon	DS442X	
	C23	No use					D8	No use				
	C24	No use				B-1	D9		Diode	Silicon	DS442X	
	C25	No use				B-1	D10		Diode	Silicon	DS442X	
E-1	C26	CE04W1C471M	CE	470μF	16WV	B-1	D11		Diode	Silicon	DS442X	
E-1	C27	CQ93BP2A472F	CQ	4700pF	±1%	100WV	B-1	D12		Diode	Silicon	DS442X
E-1	C28	CQ93BP2A472F	CQ	4700pF	±1%	100WV	C-2	D13		Diode	Silicon	DS442X
	C29	No use				C-2	D14		Diode	Silicon	DS442X	
B-2	C30	C91-0501-05	MF	0.047μF	630WV	C-2	D15		Diode	Silicon	DS442X	
	C31	No use				B-1	D16		Diode	Silicon	DS442X	
B-2	C32	CK45FB1H103K	CK	0.01μF	±10%	B-1	D17		Diode	Silicon	DS442X	
	C33	No use				D-1	D18		Diode	Silicon	DS442X	
	C34	CK45FB1H103K	CK	0.01μF	±10%	D-1	D19		Diode	Silicon	DS442X	
	C35	No use				D-1	D20		Diode	Silicon	DS442X	
B-1	C36	C91-0501-05	MF	0.047μF	630WV	D-2	D21		Diode	Silicon	DS442X	
	C37	No use				D-2	D22		Diode	Silicon	DS442X	
E-2	C38	CE04W1C471M	CE	470μF	16WV	D-2	D22		Diode	Silicon	DS442X	
E-1	C39	CK45FB1H103K	CK	0.01μF	±10%	D-2	D23		Diode	Silicon	DS442X	
E-2	C40	CK45FB1H103K	CK	0.01μF	±10%		D24	No use				
E-2	C41	CE04W1C471M	CE	470μF	16WV		D25	No use				
E-2	C42	CK45FB1H103K	CK	0.01μF	±10%		D26	No use				
F-2	C43	CE04W1C471M	CE	470μF	16WV		D27	No use				
E-2	C44	CK45FB1H103K	CK	0.01μF	±10%		D28	No use				
F-2	C45	CE04W1C471M	CE	470μF	16WV		D29	No use				
	C46	No use					D30	No use				
	C47	CC45CH1H100D	CC	10pF	±0.5pF	D-1	D31		Diode	Silicon	DS442X	
	C48	CC45CH1H100D	CC	10pF	±0.5pF		D32	No use				
D-1	C100	CE04W1A102M	CE	1000μF	10WV		D33	No use				
							D34	No use				
B-3	TC1	C05-0411-05	TC	10pF			D35	No use				
	TC2	No use					D36	No use				
	TC3	No use					D37	No use				
C-3	TC4	C05-0411-05	TC	10pF		E-1	D38		Diode	Germanium	IN60	
E-1	L1	L40-4701-03	Ferri inductor	47μH		E-1	D39		Diode	Silicon	DS442X	
F-1	L2	L40-1011-04	Ferri inductor	100μH		B-2	D40		Diode	Silicon	DS442X	
E-1	L3	L40-4701-03	Ferri inductor	47μH		B-2	D41		Diode	Silicon	1S1544A	
F-1	L4	L40-1011-03	Ferri inductor	100μH		B-2	D42		Diode	Silicon	DS442X	
F-1	L5	L40-1011-03	Ferri inductor	100μH		B-2	D43		Diode	Silicon	DS442X	
						B-2	D44		Diode	Silicon	DS442X	
B-2	IC1		IC	Digital	MC14584BCP	B-2	D45		Diode	Silicon	DS442X	
C-1	IC2		IC	Digital	MC14069UBCP		D46	No use				
C-2	IC3		IC	Digital	MC14001BCP	B-2	D47		Diode	Silicon	1S1544A	
C-1	IC4		IC	Digital	MC14174BCP	C-2	D48		Diode	Silicon	DS442X	
D-1	IC5		IC	Digital	MC14503BCP	C-2	D49		Diode	Silicon	DS442X	
D-2	IC6		IC	Digital	SN7442AN	C-2	D50		Diode	Silicon	DS442X	
						C-2	D51		Diode	Silicon	DS442X	
							D52	No use				

PARTS LIST

X77-1130-01

A TRIGGER SWITCH UNIT X77-1110-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
B-2	D53		Diode	Silicon	DS442X
B-2	D54		Diode	Silicon	DS442X
	D100		Diode	Silicon	DS442X
C-2	Q1		TR	NPN	2SC536KNP (F)
C-2	Q2		TR	NPN	2SC536KNP (F)
C-2	Q3		TR	NPN	2SC536KNP (F)
D-1	Q4		TR	NPN	2SC536KNP (F)
D-2	Q5		TR	PNP	2SA608KNP (F)
D-2	Q6		TR	PNP	2SA608KNP (F)
D-2	Q7		TR	NPN	2SC536KNP (F)
	Q8	No use			
	Q9	No use			
E-1	Q10		TR	PNP	2SA608KNP (F)
E-1	Q11		TR	PNP	2SA608KNP (F)
E-1	Q12		TR	PNP	2SA608KNP (F)
B-2	Q13		FET	Dual	DN1901
B-2	Q14		TR	NPN	2SC1215 (T or S)
B-2	Q15		TR	NPN	2SC1215 (T or S)
	Q16	No use			
B-2	Q17		FET	Dual	DN1901
B-2	Q18		TR	NPN	2SC1215 (T or S)
B-2	Q19		TR	NPN	2SC1215 (T or S)
D-1	P6	E40-0576-05	Pin connector		5P
A-2	P11	E40-0477-05	Pin connector		4P
C-2	P12	E40-0476-05	Pin connector		4P
F-1	P36	E40-0676-05	Pin connector		6P
D-3	P48	E40-1811-05	Pin connector		18P
F-1	P49	E40-0676-05	Pin connector		6P
E-1	P52	E40-0276-05	Pin connector		2P
C-3	P54	E40-1211-05	Pin connector		12P
B-1	P55	E40-1511-05	Pin connector		15P
A-3	P56	E40-0277-05	Pin connector		2P
C-1	TP1	E23-0508-04	Test terminal		
E-1	TP2	E40-0211-05	Pin connector		2P
		E23-0503-05	Terminal		

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
B-1	R1	RD14BB2C510J	RD		51Ω
B-1	R2	RD14BB2C101J	RD		100Ω
B-2	R3	RD14BB2C101J	RD		100Ω
A-2	R4	RD14BB2C510J	RD		51Ω
	R5	No use			
	R6	No use			
C-3	R7	RD14BB2C473J	RD		47kΩ
B-3	R8	RD14BB2C473J	RD		47kΩ
	R9	No use			
	R10	No use			
	R11	No use			
	R12	No use			
B-4	R13	RD14BB2C103J	RD		10kΩ
B-4	R14	RD14BB2C103J	RD		10kΩ
C-3	R15	RD14BB2C471J	RD		470Ω
	R16	No use			
C-2	R17	RD14BB2C123J	RD		12kΩ
C-2	R18	RD14BB2C103J	RD		10kΩ
C-2	R19	RD14BB2C103J	RD		10kΩ
D-1	R20	RD14BB2C473J	RD		47kΩ
D-1	R21	RD14BB2C223J	RD		22kΩ
C-3	R22	RD14BB2C220J	RD		22Ω
C-3	R23	RD14BB2C101J	RD		100Ω
C-3	R24	RD14BB2E105J	RD	±5%	1/4W
D-3	R25	RD14BB2E105J	RD	±5%	1/4W
D-3	R26	RN14BK2B3001F	RN	±1%	1/8W
D-3	R27	RN14BK2B3001F	RN	±1%	1/8W
D-3	R28	RD14BB2C220J	RD		22Ω
D-3	R29	RD14BB2C220J	RD		22Ω
D-3	R30	RD14BB2C562J	RD		5.6kΩ
D-3	R31	RD14BB2C562J	RD		5.6kΩ
D-3	R32	RN14BK2B2200F	RN	±1%	1/8W
D-3	R33	RN14BK2B2200F	RN	±1%	1/8W
C-1	R34	RN14BK2B1501F	RN	±1%	1/8W
E-2	R35	RN14BK2B1001F	RN	±1%	1/8W
C-1	R36	RN14BK2B7500F	RN	±1%	1/8W
C-1	R37	RN14BK2B2700F	RN	±1%	1/8W
E-2	R38	RN14BK2B2700F	RN	±1%	1/8W
C-1	R39	RD14BB2C220J	RD		22Ω
C-1	R40	RD14BB2C220J	RD		22Ω
E-2	R41	RD14BB2C100J	RD		10Ω
E-1	R42	RD14BB2C680J	RD		68Ω
E-2	R43	RD14BB2C680J	RD		68Ω
	R44	No use			
	R45	No use			
D-1	R46	RD14BB2C220J	RD		22Ω
D-2	R47	RD14BB2C220J	RD		22Ω
D-2	R48	RD14BB2C473J	RD		47kΩ
D-2	R49	RD14BB2C473J	RD		47kΩ
D-2	R50	RD14BB2C220J	RD		22Ω
D-2	R51	RD14BB2C220J	RD		22Ω
D-2	R52	RD14BB2C271J	RD		270Ω
D-2	R53	RD14BB2C271J	RD		270Ω
D-2	R54	RD14BB2C102J	RD		1kΩ
C-2	R55	RD14BB2C220J	RD		22Ω
C-2	R56	RD14BB2C470J	RD		47Ω
	R57	No use			
	R58	No use			
C-2	R59	RD14BB2C243J	RD		24kΩ
C-2	R60	RD14BB2C363J	RD		36kΩ
B-3	VR1	RO1-2510-05	VR	(attached S3a, b, 4) 5kΩ	
B-3	VR2	R12-3516-05	VR		10kΩ
B-4	VR3	R12-0532-05	VR		100Ω
B-1	C1	C91-0502-05	MF	0.01μF	630WV
B-3	C2	CC45CH1H680J	CC	68pF	±5%

PARTS LIST

X77-1110-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
B-3	C3	CC45CH1H680J	CC	68pF	±5%
	C4	No use			
	C5	No use			
C-3	C6	CK45B1H103K	CK	0.01μF	±10%
C-2	C7	CE04W1H3R3M	CE	3.3μF	50WV
C-2	C8	CK45B1H103K	CK	0.01μF	±10%
D-3	C9	CC45CH1H220J	CC	22pF	±5%
D-3	C10	CC45CH1H220J	CC	22pF	±5%
	C11	No use			
	C12	No use			
D-2	C13	CC45CH1H220J	CC	22pF	±5%
D-4	C14	CK45B1H103K	CK	0.01μF	±10%
B-3	C15	C91-0549-05	Tantalum	1μF	35WV
D-4	C16	CE04W1C330M	CE	33μF	16WV
D-4	C17	CE04W1C330M	CE	33μF	16WV
D-4	C18	CK45B1H103K	CK	0.01μF	±10%
D-3	C19	CK45B1H103K	CK	0.01μF	±10%
D-1	C20	CK45B1H103K	CK	0.01μF	±10%
E-1	C21	CK45B1H103K	CK	0.01μF	±10%
D-3	C22	CK45B1H103K	CK	0.01μF	±10%
B-4	C23	C91-0549-05	Tantalum	1μF	35WV
E-4	C24	CE04W1C330M	CE	33μF	16WV
E-3	C25	CE04W1C330M	CE	33μF	16WV
C-2	C26	CK45B1H103K	CK	0.01μF	±10%
D-2	C27	CK45B1H103K	CK	0.01μF	±10%
E-2	C28	CK45B1H103K	CK	0.01μF	±10%
	C29	No use			
D-2	C30	CK45B1H103K	CK	0.01μF	±10%
	C31	CK45B1H103K	CK	0.01μF	±10%
E-2	TC1	C05-0412-05	TC	20pF	
D-3	L1	L40-2201-03	Ferri-inductor	22μH	
E-3	L2	L40-2201-03	Ferri-inductor	22μH	
C-2	D1		Diode Silicon	DS442X	
E-1	D2		Diode Silicon	DS442X	
E-2	D3		Diode Silicon	DS442X	
E-1	D4		Diode Silicon	DS442X	
E-2	D5		Diode Silicon	DS442X	
	Q1	No use			
	Q2	No use			
C-2	Q3		TR NPN	2SC536KNP (F)	
C-2	Q4		TR NPN	2SC536KNP (F)	
C-3	Q5		FET Dual	DN1901	
D-3	Q6		TR NPN	2SC1215 (T or S)	
D-3	Q7		TR PNP	2SC1215 (T or S)	
D-2	Q8		TR PNP	2SA1161	
E-2	Q9		TR PNP	2SA1161	
C-2	Q10		TR NPN	2SC2671	
D-2	IC1		IC Linear	CA3102E	
B-1	P15	E40-1077-05	Pin connector	10P	
C-1	P46	E40-0276-05	Pin connector	2P	
E-2	P47	E40-0476-05	Pin connector	4P	

B TRIGGER SWITCH UNIT X77-1120-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
C-3	R1	RD14BB2C101J	RD	100Ω	
C-3	R2	RD14BB2C101J	RD	100Ω	
	R3	No use			
	R4	No use			
	R5	No use			
B-2	R6	RD14BB2C103J	RD	10kΩ	
B-2	R7	RD14BB2C103J	RD	10kΩ	
C-2	R8	RD14BB2C471J	RD	470Ω	
C-3	R9	RD14BB2C220J	RD	22Ω	
C-2	R10	RD14BB2C101J	RD	100Ω	
C-3	R11	RD14BB2E105J	RD	1MΩ	±5% 1/4W
C-2	R12	RD14BB2E105J	RD	1MΩ	±5% 1/4W
C-3	R13	RN14BK2B3001F	RN	3kΩ	±1% 1/8W
C-3	R14	RN14BK2B3001F	RN	3kΩ	±1% 1/8W
C-2	R15	RD14BB2C220J	RD	22Ω	
C-2	R16	RD14BB2C220J	RD	22Ω	
C-2	R17	RD14BB2C562J	RD	5.6kΩ	
C-2	R18	RD14BB2C562J	RD	5.6kΩ	
C-2	R19	RN14BK2B2200F	RN	220Ω	±1% 1/8W
C-2	R20	RN14BK2B2200F	RN	220Ω	±1% 1/8W
D-2	R21	RN14BK2B1501F	RN	1.5kΩ	±1% 1/8W
D-2	R22	RN14BK2B1501F	RN	1.5kΩ	±1% 1/8W
D-2	R23	RN14BK2B7500F	RN	750Ω	±1% 1/8W
D-2	R24	RN14BK2B2700F	RN	270Ω	±1% 1/8W
D-2	R25	RN14BK2B2700F	RN	270Ω	±1% 1/8W
D-2	R26	RD14BB2C220J	RD	22Ω	
D-2	R27	RD14BB2C220J	RD	22Ω	
E-2	R28	RD14BB2C100J	RD	10Ω	
E-2	R29	RD14BB2C680J	RD	68Ω	
E-2	R30	RD14BB2C680J	RD	68Ω	
	R31	No use			
	R32	No use			
D-2	R33	RD14BB2C220J	RD	22Ω	
D-2	R34	RD14BB2C220J	RD	22Ω	
D-2	R35	RD14BB2C473J	RD	47kΩ	
D-2	R36	RD14BB2C473J	RD	47kΩ	
D-2	R37	RD14BB2C220J	RD	22Ω	
D-2	R38	RD14BB2C220J	RD	22Ω	
D-2	R39	RD14BB2C271J	RD	270Ω	
D-2	R40	RD14BB2C271J	RD	270Ω	
D-3	R41	RD14BB2C220J	RD	22Ω	
D-3	R42	RD14BB2C470J	RD	47Ω	
C-3	R43	RD14BB2C510J	RD	51Ω	
C-3	R44	RD14BB2C222J	RD	2.2kΩ	
D-3	R45	RD14BB2C470J	RD	47Ω	
C-3	R46	RD14BB2C821J	RD	820Ω	
C-2	VR1	R01-2511-05	VR	5kΩ	
B-2	VR2	R12-3516-05	VR	10kΩ	
E-2	VR3	R12-0532-05	VR	100Ω	
B-3	C1	C91-0502-05	MF	0.01μF	630WV
	C2	No use			
	C3	No use			
C-2	C4	CK45B1H103K	CK	0.01μF	±10%
C-2	C5	CC45CH1H220J	CC	22pF	±5%
C-2	C6	CC45CH1H220J	CC	22pF	±5%
	C7	No use			
	C8	No use			
D-3	C9	CK45B1H103K	CK	0.01μF	±10%
C-3	C10	CK45B1H103K	CK	0.01μF	±10%
B-2	C11	C91-0549-05	Tantalum	1μF	35WV
E-3	C12	CE04W1C330M	CE	33μF	16WV
E-3	C13	CE04W1C330M	CE	33μF	16WV
E-3	C14	CK45B1H103K	CK	0.01μF	±10%

PARTS LIST

X77-1120-01

POWER BLANKING UNIT X68-1310-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description		
D-2	C15	CK45B1H103K	CK	0.01 μ F	\pm 10%
C-3	C16	CK45B1H103K	CK	0.01 μ F	\pm 10%
D-3	C17	CK45B1H103K	CK	0.01 μ F	\pm 10%
B-2	C18	C91-0549-05	Tantalum	1 μ F	35WV
D-3	C19	CE04W1C330M	CE	33 μ F	16WV
E-3	C20	CE04W1C330M	CE	33 μ F	16WV
F-3	C21	CK45B1H103K	CK	0.01 μ F	\pm 10%
D-2	C22	CK45B1H103K	CK	0.01 μ F	\pm 10%
C-2	C23	CK45B1H103K	CK	0.01 μ F	\pm 10%
C-3	C24	CE04W1C100M	CE	10 μ F	16WV
E-2	TC1	C05-0412-05	TC	20pF	
E-3	L1	L40-2201-03	Ferri-inductor	22 μ H	
E-3	L2	L40-2201-03	Ferri-inductor	22 μ H	
C-3	D1		Diode Zener	WZ-081	
C-3	Q1		TR	NPN	2SC1215 (T or S)
C-2	Q2		FET	Dual	DN1901
C-2	Q3		TR	NPN	2SC1215 (T or S)
C-2	Q4		TR	NPN	2SC1215 (T or S)
D-2	Q5		TR	PNP	2SA1161
D-2	Q6		TR	PNP	2SA1161
D-3	Q7		TR	NPN	2SC2499
E-2	IC1		IC	Linear	CA3102E
D-3	P43	E40-0276-06	Pin connector	2P	
D-3	P44	E40-0276-05	Pin connector	2P	
F-3	P45	E40-0676-05	Pin connector	6P	
C-4	P51	E40-0576-05	Pin connector	5P	

Fig. & Index No.	Ref. No.	Parts No.	Name & Description			
C-6	R1	RN14BK2B5102F	RN	51k Ω	\pm 1%	1/8W
C-6	R2	RN14BK2B5101F	RN	5.1k Ω	\pm 1%	1/8W
B-5	R3	RD14BB2C102J	RD	1k Ω		
	R4	No use				
B-5	R5	RD14BB2C101J	RD	100 Ω		
B-5	R6	RD14BB2C102J	RD	1k Ω		
C-5	R7	RN14BK2B1303F	RN	130k Ω	\pm 1%	1/8W
C-5	R8	RN14BK2B5601F	RN	5.6k Ω	\pm 1%	1/8W
C-4	R9	RD14BB2C561J	RD	560 Ω		
C-4	R10	RD14BB2C392J	RD	3.9k Ω		
C-4	R11	RN14BK2B5101F	RN	5.1k Ω	\pm 1%	1/8W
C-4	R12	RN14BK2B5101F	RN	5.1k Ω	\pm 1%	1/8W
C-4	R13	RD14BB2C561J	RD	560 Ω		
C-4	R14	RD14BB2C392J	RD	3.9k Ω		
C-4	R15	RN14BK2B1301F	RN	1.3k Ω	\pm 1%	1/8W
C-4	R16	RN14BK2B3901F	RN	3.9k Ω	\pm 1%	1/8W
C-5	R17	RD14BB2C561J	RD	560 Ω		
C-5	R18	RD14BB2C222J	RD	2.2k Ω		
B-6	R19	RD14BB2E100J	RD	10 Ω	\pm 5%	1/4W
B-6	R20	RN14BK2B1302F	RN	13k Ω	\pm 1%	1/8W
B-6	R21	RN14BK2B8201F	RN	8.2k Ω	\pm 1%	1/8W
	R22	No use				
	R23	No use				
	R24	No use				
	R25	No use				
D-6	R26	RD14BB2C682J	RD	6.8k Ω		
D-5	R27	RD14BB2C332J	RD	3.3k Ω		
D-6	R28	RD14BB2C332J	RD	3.3k Ω		
E-6	R29	RD14BB2C510J	RD	51 Ω		
E-6	R30	RD14BB2C510J	RD	51 Ω		
E-6	R31	RD14BB2C471J	RD	470 Ω		
E-6	R32	RD14BB2C222J	RD	2.2k Ω		
E-5	R33	RD14BB2C222J	RD	2.2k Ω		
E-5	R34	RD14BB2C471J	RD	470 Ω		
F-6	R35	RD14BB2C332J	RD	3.3k Ω		
F-6	R36	RD14BB2C102J	RD	1k Ω		
F-6	R37	RD14BB2C102J	RD	1k Ω		
E-5	R38	RD14BB2C332J	RD	3.3k Ω		
E-5	R39	RD14BB2C122J	RD	1.2k Ω		
E-5	R40	RD14BB2E101J	RD	100 Ω	\pm 5%	1/4W
E-4	R41	RD14BB2C221J	RD	220 Ω		
E-4	R42	RD14BB2C332J	RD	33k Ω		
D-4	R43	RD14BB2C432J	RD	4.3k Ω		
D-4	R44	RD14BB2C471J	RD	470 Ω		
E-4	R45	RD14BB2C753J	RD	75k Ω		
D-4	R46	RD14BB2C124J	RD	120k Ω		
D-4	R47	RD14BB2C562J	RD	5.6k Ω		
D-4	R48	RD14BB2C561J	RD	560 Ω		
E-3	R49	RD14BB2C470J	RD	47 Ω		
E-4	R50	RD14BB2C104J	RD	100k Ω		
E-5	R51	RD14BB2C221J	RD	220 Ω		
E-5	R52	RD14BB2C562J	RD	5.6k Ω		
E-4	R53	RD14BB2C154J	RD	150k Ω		
E-4	R54	RD14BB2C124J	RD	120k Ω		
E-3	R55	RD14BB2C470J	RD	47 Ω		
E-4	R56	RD14BB2C332J	RD	3.3k Ω		
E-3	R57	RD14BB2C561J	RD	560 Ω		
C-3	R58	RD14BB2C683J	RD	68k Ω		
C-3	R59	RD14BB2C683J	RD	68k Ω		
C-3	R60	RD14BB2C102J	RD	1k Ω		
C-3	R61	RD14BB2C102J	RD	1k Ω		
C-3	R62	RD14BB2C103J	RD	10k Ω		
C-4	R63	RD14BB2C102J	RD	1k Ω		
C-2	R64	RD14BB2C683J	RD	68k Ω		
B-2	R65	RD14BB2C103J	RD	10k Ω		

PARTS LIST

X68-1310-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description			Fig. & Index No.	Ref. No.	Parts No.	Name & Description			
B-2	R66	RD14BB2C103J	RD	10k Ω		D-3	C36	CK45E3D103P	CK	0.01 μ F	+100%, -0%	
C-2	R67	RD14BB2C102J	RD	1k Ω							2kVV	
B-2	R68	RD14BB2C472J	RD	4.7k Ω		D-3	C37	CK45E3D103P	CK	0.01 μ F	+100%, -0%	
B-1	R69	RD14BB2C330J	RD	33 Ω							2kVV	
D-3	R70	R92-0793-05	MG	15M Ω	\pm 5%	1/2W	E-3	C38	CK45E3D103P	CK	0.01 μ F	+100%, -0%
F-2	R71	RC05GF2H825J	RC	8.2M Ω	\pm 5%	1/2W					2kVV	
F-2	R72	RC05GF2H156J	RC	15M Ω	\pm 5%	1/2W	E-3	C39	CK45E3D103P	CK	0.01 μ F	+100%, -0%
E-2	R73	R92-0755-05	MG	3M Ω	\pm 5%	1/2W					2kVV	
E-2	R74	R92-0756-05	MG	47M Ω	\pm 5%	1/2W	D-2	C40	CK45B3D102K	CK	1000pF	\pm 10%
A-4	R75	RD14BB2C562J	RD	5.6k Ω			C-2	C41	CQ93M1H154K	CQ	0.15 μ F	\pm 10%
	R76	No use					C-2	C42	CK45B1H103K	CK	0.01 μ F	\pm 10%
	R77	No use					C-2	C43	CK45B1H472K	CK	4700pF	\pm 10%
B-3	R78	RD14BB2E101J	RD	100 Ω	\pm 5%	1/4W	C-2	C44	CE04W1E470M	CE	47 μ F	25WV
	R79	No use					B-2	C45	CK45B1H103K	CK	0.01 μ F	\pm 10%
F-5	R80	RD14BB2C221J	RD	220 Ω			B-2	C46	CE04W1E470M	CE	47 μ F	25WV
C-3	R81	RD14BB2C102J	RD	1k Ω			B-2	C47	CK45B1H103K	CK	0.01 μ F	\pm 10%
	R82	RD14BB2C102J	RD	1k Ω			B-1	C48	CE04W1E470M	CE	47 μ F	25WV
	R83	RN14BK2B2200F	RN	220 Ω	\pm 1%	1/8W	B-2	C49	CQ93M1H472K	CQ	4700pF	\pm 10%
	R84	RN14BK2B5101F	RN	5.1k Ω	\pm 1%	1/8W	C-3	C50	CE04W1E470M	CE	47 μ F	25WV
							C-3	C51	CK45B1H472K	CK	4700pF	\pm 10%
F-5	VR1	R03-3502-15	VR	10k Ω			D-1	C52	CK45E3D103P	CK	0.01 μ F	+100%, -0%
C-3	VR2	R12-3041-05	VR	10k Ω							2kVV	
C-3	VR3	R12-3041-05	VR	10k Ω			F-2	C53	CK45E3D103P	CK	0.01 μ F	+100%, -0%
G-3	VR4	R23-1501-05	VR	1k Ω							2kVV	
D-5	VR5	R12-1028-05	VR	4.7k Ω			F-1	C54	CK45B3D102K	CK	1000pF	\pm 10%
E-6	VR6	R12-3041-05	VR	10k Ω			B-3	C55	CK45B2H222K	CK	2200pF	\pm 10%
C-2	VR7	R12-3042-05	VR	47k Ω				C56	No use			500WV
G-2	VR8	R05-8001-05	VR	3M Ω			E-6	C57	CC45CH1H101J	CC	100pF	\pm 5%
A-4	VR9	R12-5501-05	VR	150k Ω			E-5	C58	CC45CH1H101J	CC	100pF	\pm 5%
C-6	C1	CK45B1H103K	CK	0.01 μ F	\pm 10%		D-6	TC1	C05-0405-05	TC	20pF	
B-5	C2	CE04W1V100M	CE	10 μ F		35WV	E-4	TC2	C05-0405-05	TC	20pF	
C-6	C3	CE04W1J330M	CE	33 μ F		63WV	E-4	TC3	C05-0403-05	TC	6pF	
B-5	C4	CE04W2C3R3M	CE	3.3 μ F		160WV						
C-5	C5	CE04W2C3R3M	CE	3.3 μ F		160WV	C-6	L1	L40-1011-04	Ferri-inductor	100 μ H	
C-4	C6	CE04W1C330M	CE	33 μ F		16WV	C-4	L2	L40-1001-01	Ferri-inductor	10 μ H	
C-4	C7	C91-0549-05	Tantalum	1 μ F		35WV	C-6	L3	L40-1011-04	Ferri-inductor	100 μ H	
C-4	C8	CE04W1E101M	CE	100 μ F		25WV	D-5	L4	L40-1011-04	Ferri-inductor	100 μ H	
C-4	C9	CE04W1E101M	CE	100 μ F		25WV	D-4	L5	L40-1011-04	Ferri-inductor	100 μ H	
C-5	C10	CE04W1A221M	CE	220 μ F		10WV	D-4	L6	L40-1011-04	Ferri-inductor	100 μ H	
B-6	C11	CE04W1V100M	CE	10 μ F		35WV	B-2	L7	L40-1011-04	Ferri-inductor	100 μ H	
B-6	C12	CK45B1H103K	CK	0.01 μ F	\pm 10%		B-2	L8	L40-1011-04	Ferri-inductor	100 μ H	
C-5	C13	CE04W1V470M	CE	47 μ F		35WV	B-2	L9	L40-1011-04	Ferri-inductor	100 μ H	
B-3	C14	CK45B1H103K	CK	0.01 μ F	\pm 10%							
B-3	C15	CK45B1H103K	CK	0.01 μ F	\pm 10%		B-5	D1		Diode Silicon	DS442X	
	C16	No use					B-4	D2		Diode Zener	WZ-120	
E-6	C17	CC45CH1H680J	CC	68pF	\pm 5%		B-4	D3		Diode Zener	WZ-120	
F-6	C18	CC45CH1H680J	CC	68pF	\pm 5%		E-5	D4		Diode Zener	WZ-032	
E-5	C19	CK45B1H472K	CK	4700pF	\pm 10%		E-5	D5		Diode Silicon	DS442X	
E-5	C20	CK45B1H472K	CK	4700pF	\pm 10%			D6	No use			
F-5	C21	C91-0549-05	Tantalum	1 μ F		35WV	E-5	D7		Diode Zener	WZ-090	
F-5	C22	C91-0549-05	Tantalum	1 μ F		35WV	D-3	D8		Diode Silicon	1SS83	
	C23	CC45CH1H220J	CC	22pF	\pm 5%		E-3	D9		Diode Silicon	1SS83	
E-4	C24	CC45CH2H010C	CC	1pF	\pm 0.25pF	500WV	D-2	D10		Diode Silicon	W06C	
D-4	C25	CK45B2H472K	CK	4700pF	\pm 10%	500WV	D-2	D11		Diode Silicon	W06C	
D-4	C26	CK45B1H103K	CK	0.01 μ F	\pm 10%		F-2	D12		Diode Silicon	W06C	
E-4	C27	CC45CH2H010C	CC	1pF	\pm 0.25pF	500WV	F-1	D13		Diode Silicon	W06C	
E-3	C28	CK45B2H472K	CK	4700pF	\pm 10%	500WV	C-2	D14		Diode Silicon	DS442X	
E-3	C29	CK45B1H103K	CK	0.01 μ F	\pm 10%		C-2	D15		Diode Silicon	DS442X	
D-4	C30	CE04W2C3R3M	CE	3.3 μ F		160WV	C-2	D16		Diode Zener	WZ-032	
D-3	C31	CK45B2H472K	CK	4700pF	\pm 10%	500WV	B-2	D17		Diode Silicon	DS442X	
D-5	C32	CE04W1A221M	CE	220 μ F		10WV						
D-5	C33	CK45B1H103K	CK	0.01 μ F	\pm 10%		B-5	Q1		TR NPN	2SC1913 (Q or R)	
D-4	C34	CE04W1E101M	CE	100 μ F		25WV	B-5	Q2		TR NPN	2SC1505 (L)	
D-4	C35	CK45B1H103K	CK	0.01 μ F	\pm 10%		C-4	Q3		TR PNP	2SB633 (E)	

PARTS LIST

X68-1310-01

Fig. & Index No.	Ref. No.	Parts No.	Name & Description
C-4	Q4		TR NPN 2SD613 (E)
C-5	Q5		TR PNP 2SB633 (E)
B-6	Q6		TR NPN 2SC1505 (L)
B-6	Q7		TR NPN 2SC536KNP (F)
B-4	Q8		TR NPN 2SC1505 (L)
B-3	Q9		TR NPN 2SC536KNP (F)
B-3	Q10		TR PNP 2SA608KNP (F)
	Q11	No use	
	Q12	No use	
E-5	Q13		TR NPN 2SC1215 (T or S)
E-5	Q14		TR NPN 2SC1215 (T or S)
E-5	Q15		TR NPN 2SC1215 (T or S)
	Q16	No use	
D-5	Q17		TR NPN 2SC1047 (C)
D-4	Q18		TR PNP 2SA838 (C)
E-3	Q19		TR NPN 2SC805A-2(2,3)
D-4	Q20		TR PNP 2SA923-2 (2, 3)
	Q21		TR NPN 2SC2910 S or T
	Q22		TR PNP 2SA1208 S or T
C-3	Q23		TR NPN 2SC2910 S or T
C-3	Q24		TR NPN 2SC2910 S or T
B-2	Q25		TR NPN 2SC536KNP (F)
C-2	Q26		TR NPN 2SC536KNP (F)
B-2	Q27		TR PNP 2SA608KNP (F)
C-2	Q28		FETN-channel 2SK19 (BL)
B-1	Q29		TR NPN 2SD613 (E)
B-4	IC1		IC Linear NJM4558D
B-5	IC2		IC Linear NJM4558D
D-6	P22	E40-0776-05	Pin connector 7P
F-5	P23a	E40-0476-05	Pin connector 4P
F-3	P23b	E40-0476-05	Pin connector 4P
C-3	P25	E40-0276-05	Pin connector 2P
F-6	P26a	E40-0576-05	Pin connector 5P
F-3	P26b	E40-0576-05	Pin connector 5P
D-5	P27	E40-0876-05	Pin connector 8P
E-6	P28	E40-0476-05	Pin connector 4P
A-2	P29	E40-0703-05	Pin connector 7P
A-5	P30	E40-0746-05	Pin connector 7P
A-3	P32	E40-0476-05	Pin connector 4P
E-1	P33	E40-0332-05	Pin connector 3P
E-6	P34	E40-0276-05	Pin connector 2P
		E31-0762-05	Lead wire with connector
		F02-0414-04	Heat sink
		F20-0516-05	Sheet (Insulator)
		F20-0623-05	Sheet (insulator)
F-3	PL1	B30-0927-05	Pilot lamp
F-3	PL2	B30-0927-05	Pilot lamp
F-3	PL3	B30-0927-05	Pilot lamp
F-3	PL4	B30-0927-05	Pilot lamp
D-2	NL1		Neon lamp NE-2B
D-2	NL2		Neon lamp NE-2B
E-2	NL3		Neon lamp NE-2B
E-2	NL4		Neon lamp NE-2B
		J30-0605-05	Spacer (For TR)

VOLTAGES AND WAVEFORMS

The voltages and waveforms are measured on each schematic diagram as follows:

TEST EQUIPEMENT

- Digital multimeter : DL-720 (TRIO)
- Oscilloscope : 475A (TEKTRONIX)
- Sine wave generator : SG-502 (TEKTRONIX)

CONTROL SETTINGS

A INTENSITY	Midrange
FOCUS	Midrange
AC-GND-DC	GND for voltage measurement DC for waveform measurement
POSITION	Midrange
X5GAIN	OFF
VOLTS/DIV	0.2V
V. VARIABLE	CAL
CH 2 INV	OFF
V. MODE	Unless otherwise specified CH 1
COUPLING	AC
SLOPE	+
TRIG. MODE	AUTO
HOLDOFF	NORM
A SWEEP TIME/DIV	0.2ms
B SWEEP TIME/DIV	50μs
A. VARIABLE	CAL
POSITION	Midrange
H. DISPLAY	A
X 10 MAG	OFF

NOTE:


In differential circuit, the voltages and waveforms are shown only CH 1 and CH 3.


Voltage Measurements

Voltage measurements are taken with no signal applied and the trace positioned to the center horizontal graticule line. The digital multimeter common should be connected to chassis ground at the nearest measurement point.

Waveform Condition

Waveforms are measured with 1 kHz 1Vp-p sine wave applied CH 1 input and 1 kHz 500m Vp-p applied CH3 input.

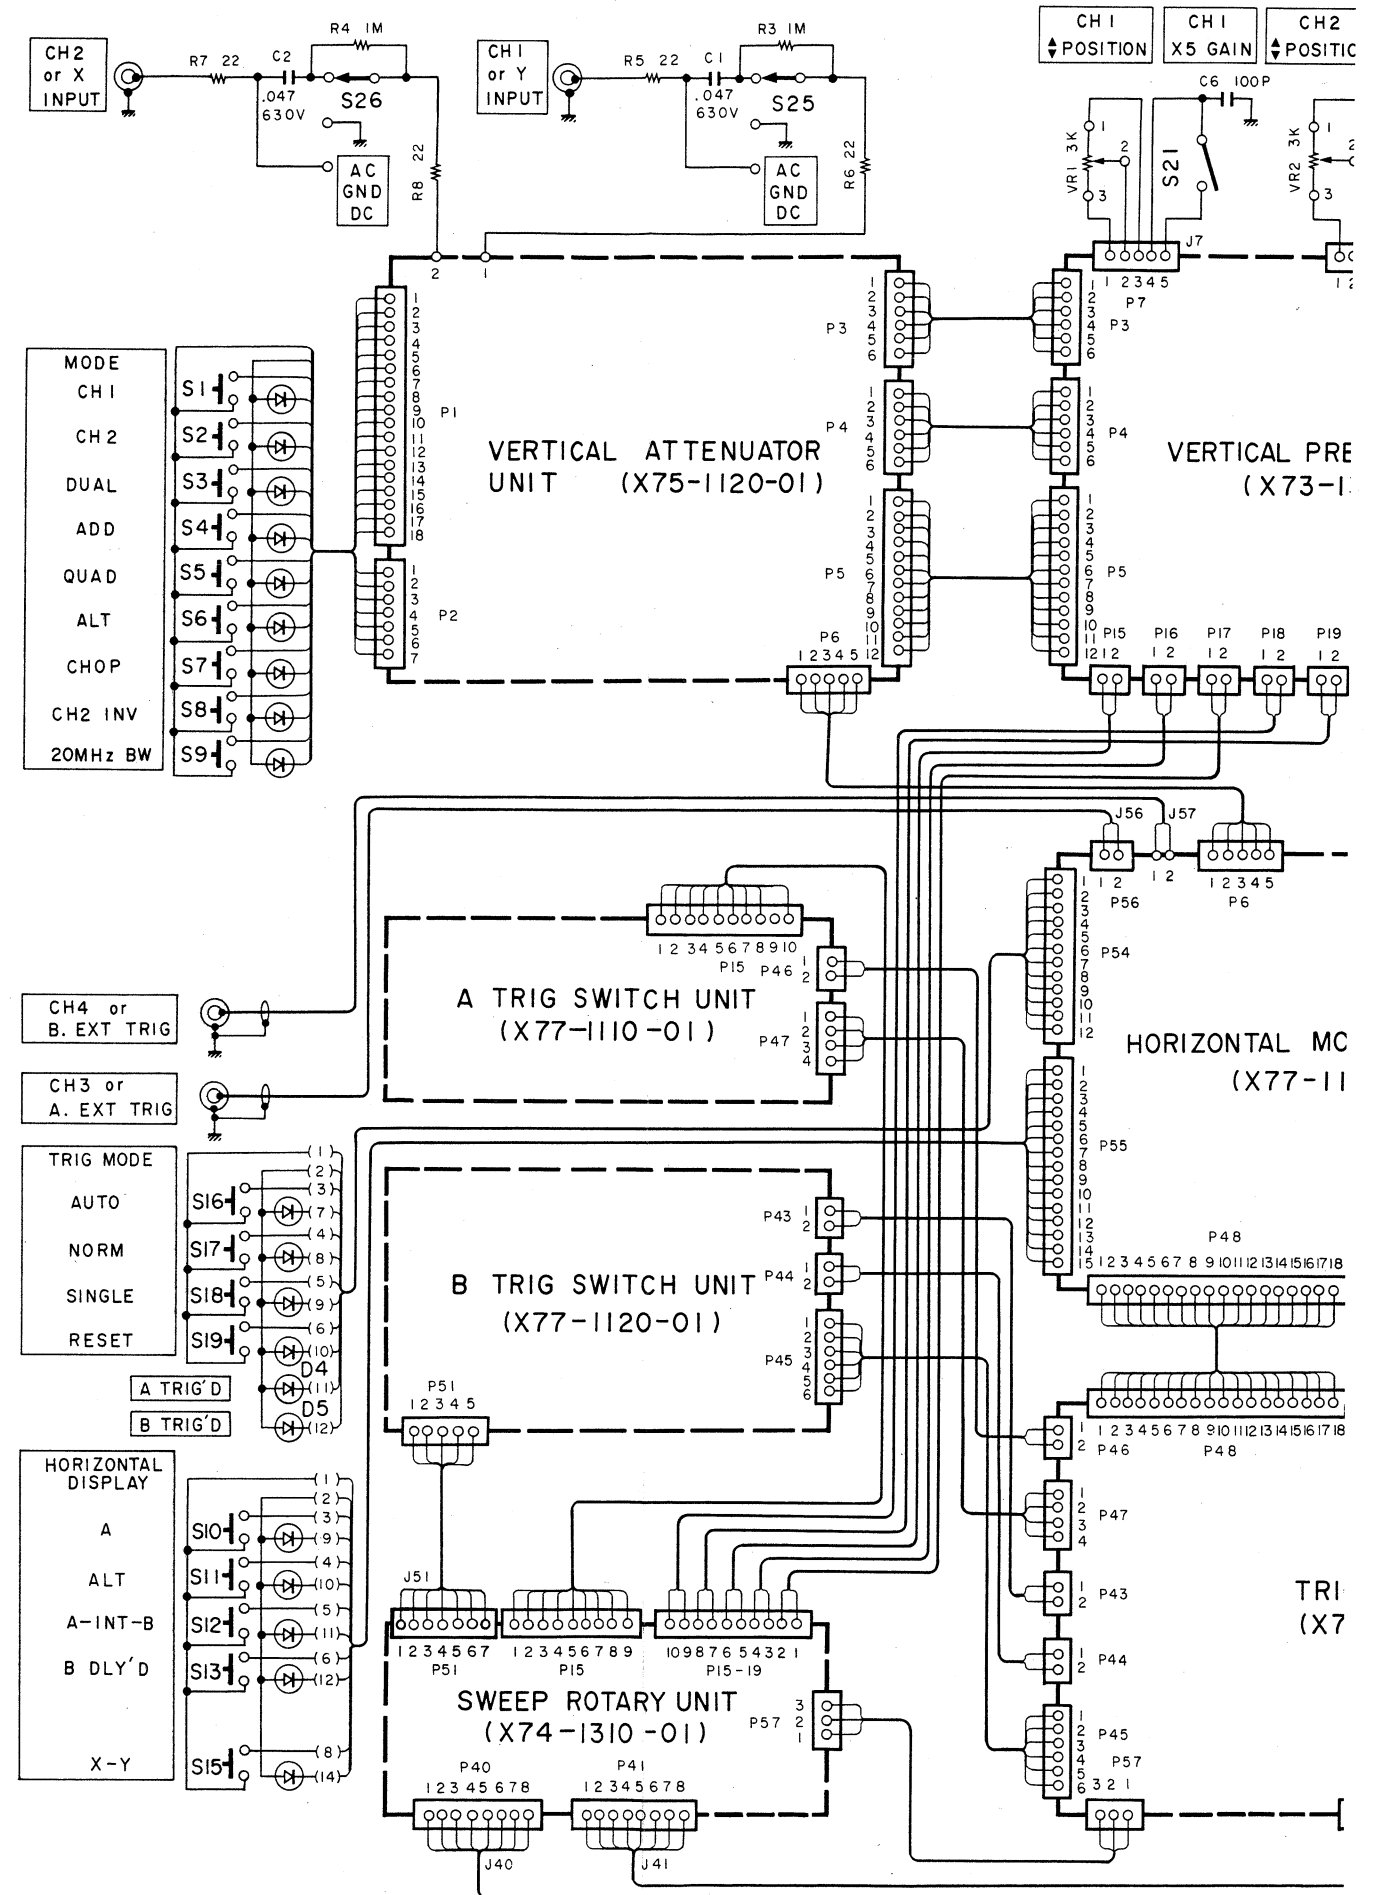


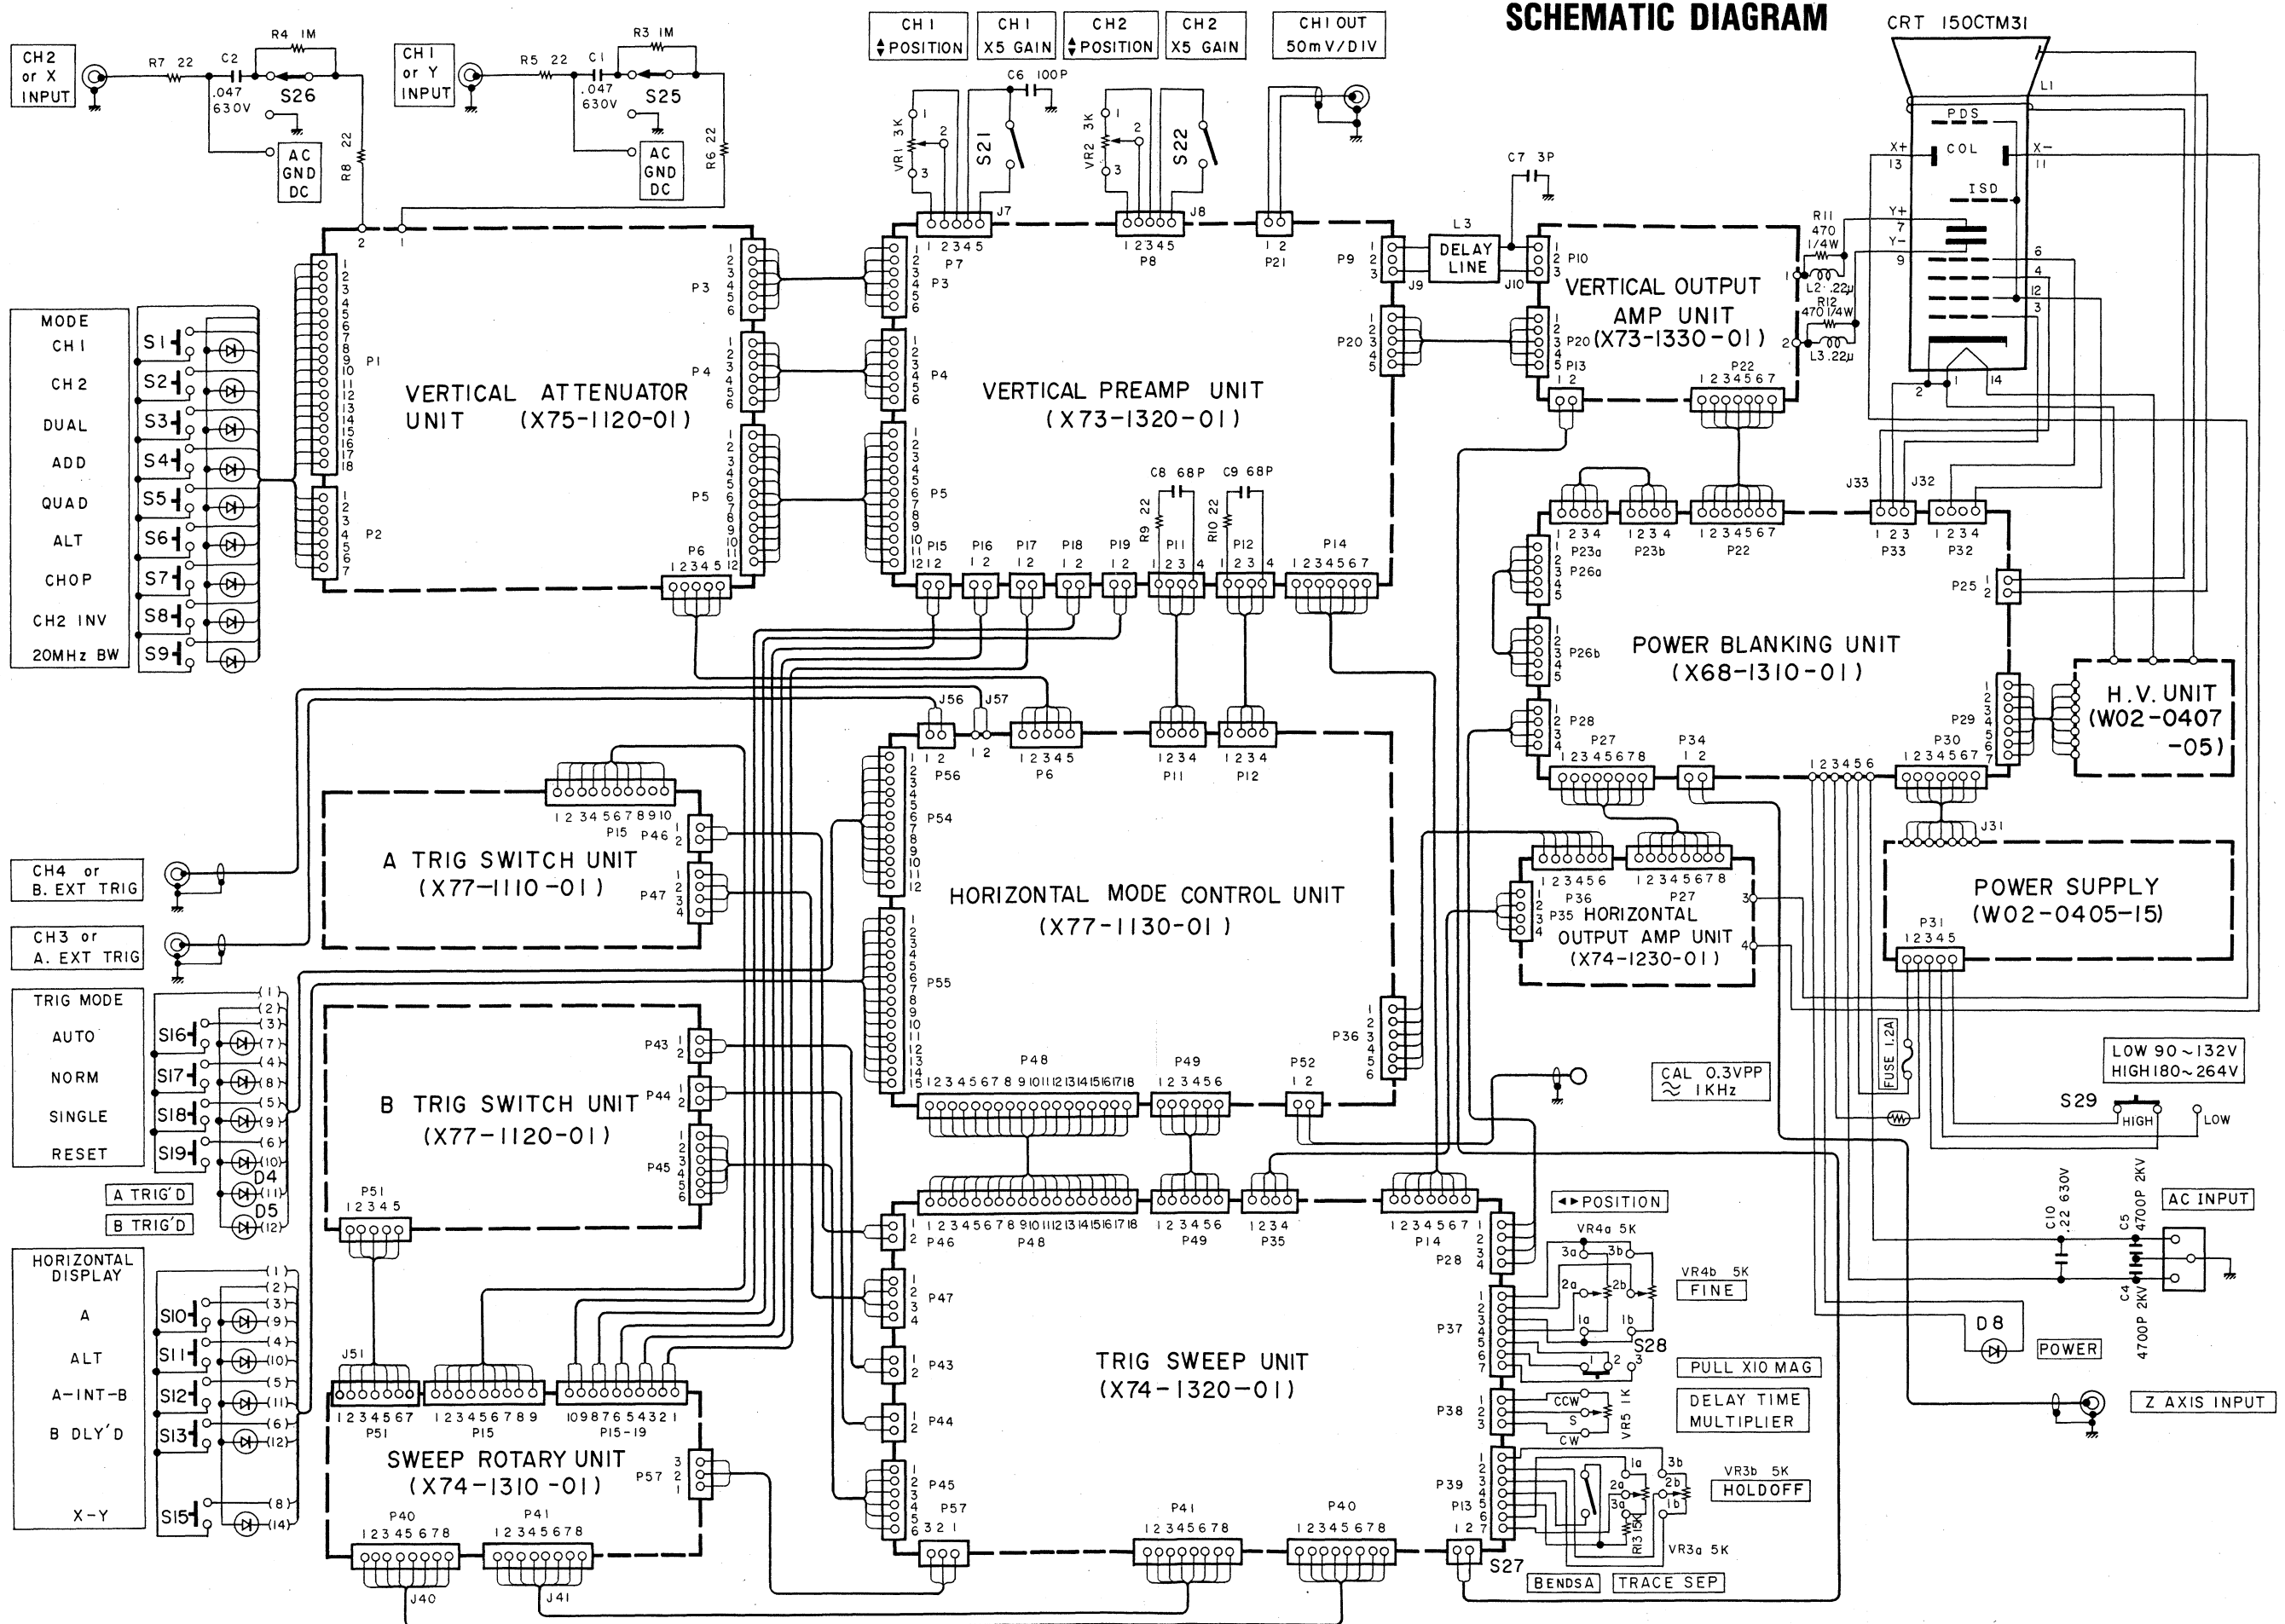

SCHEMATIC DIAGRAM


PC BOARD

X75-1120-01


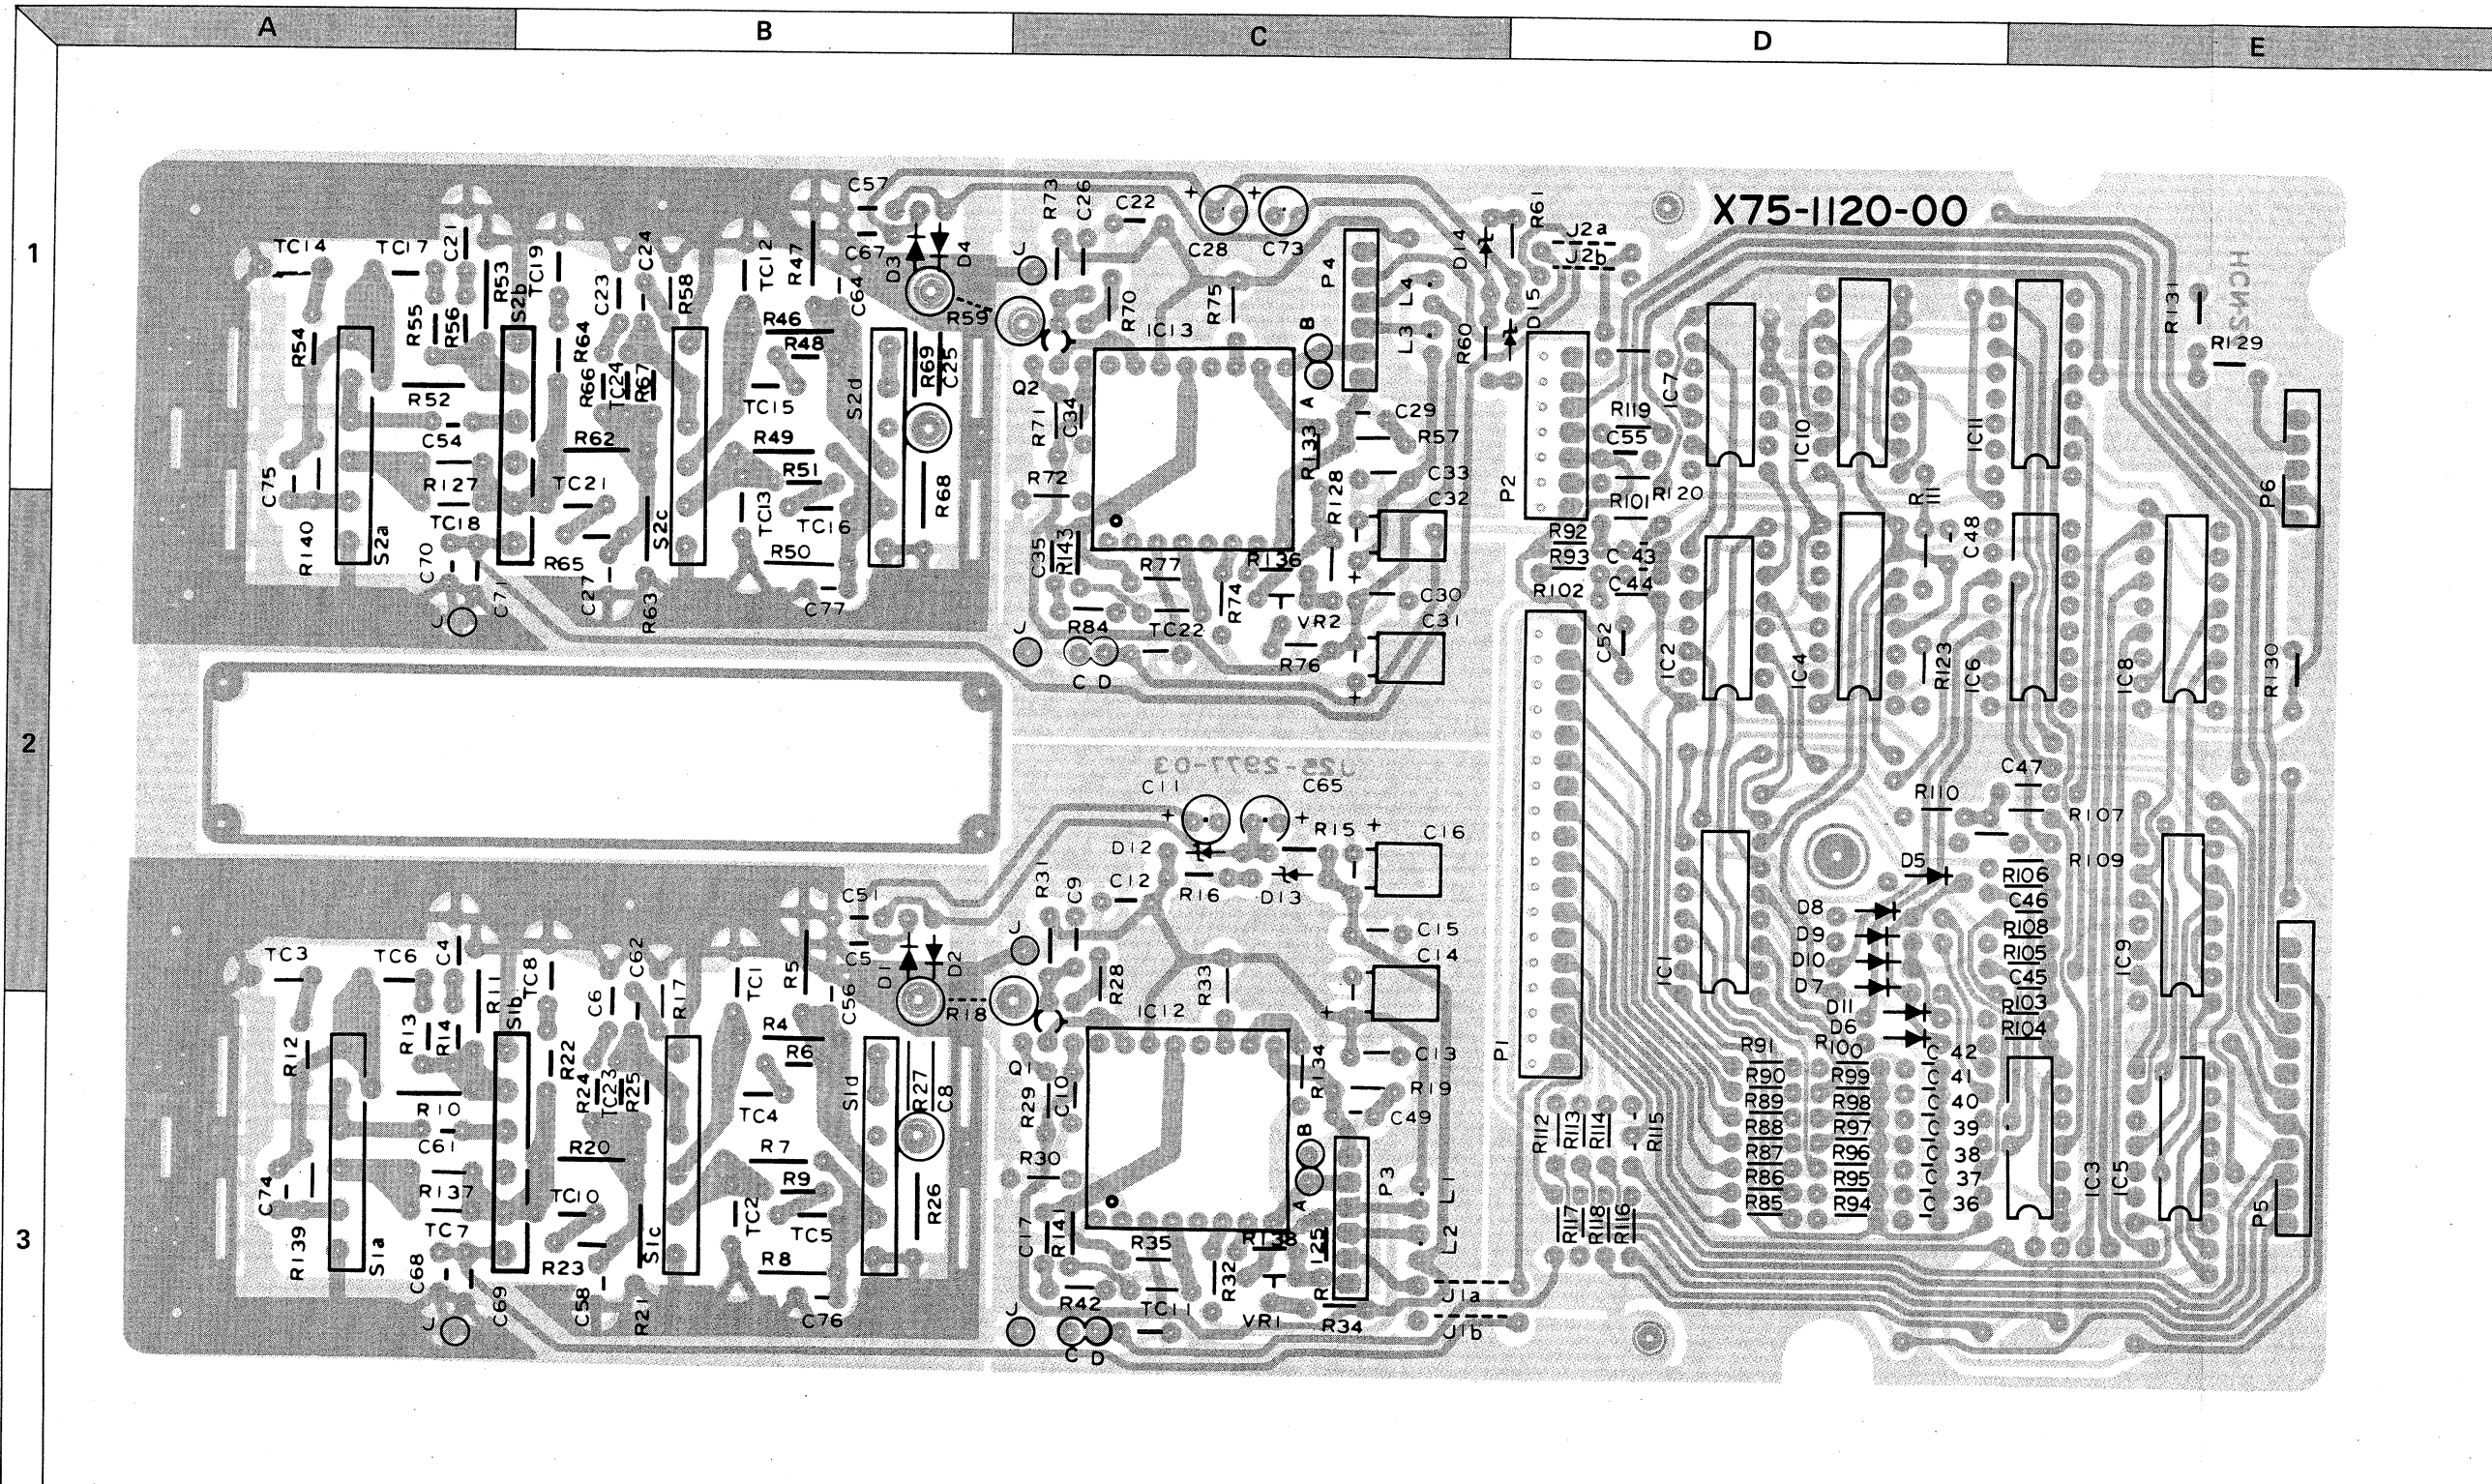


BOARD

D E




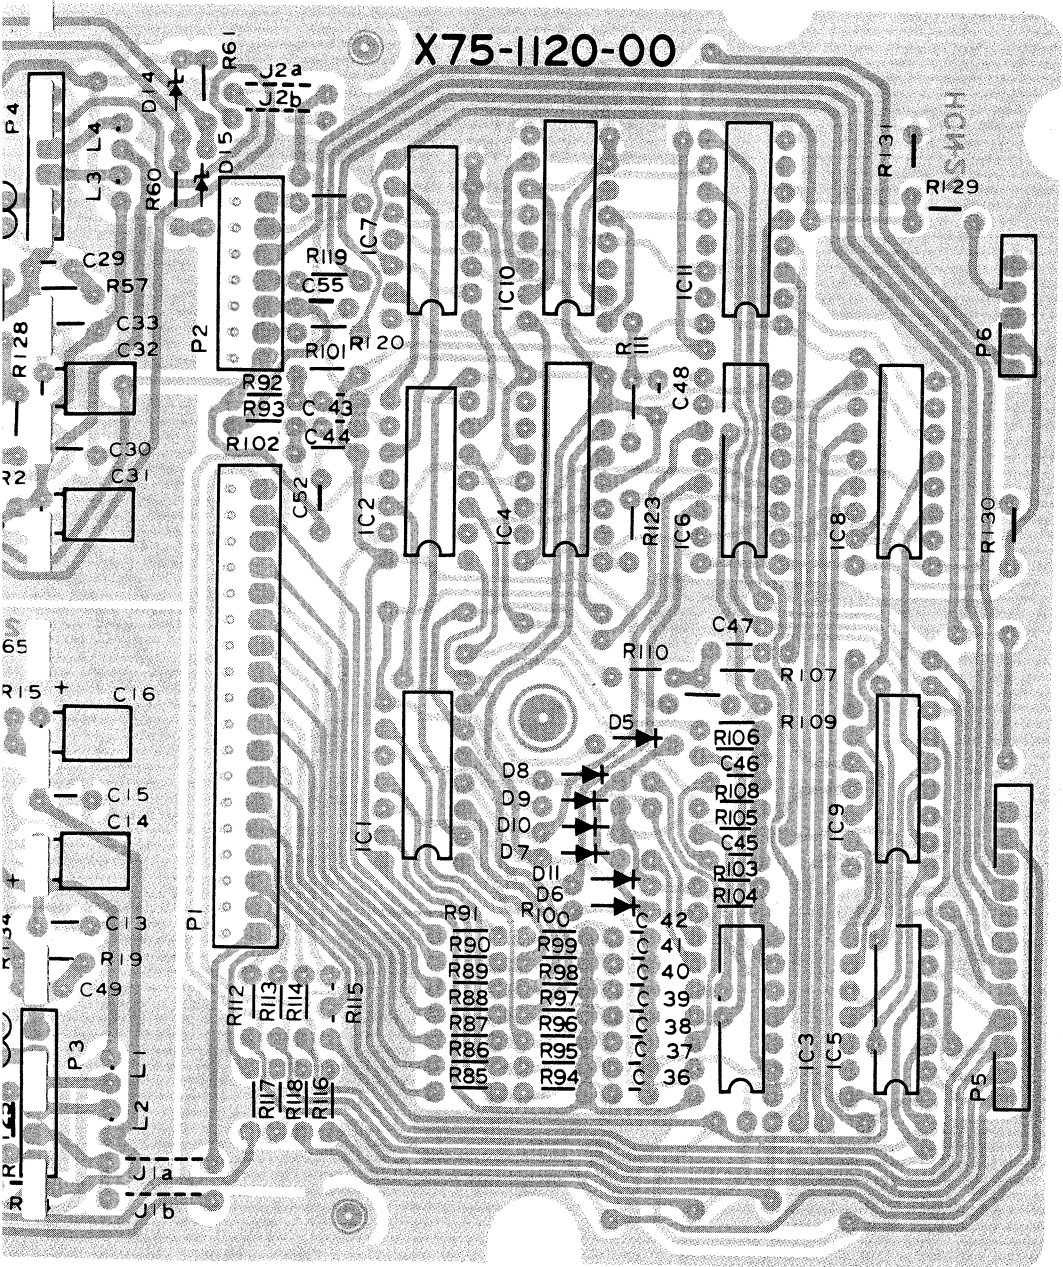


X75-1120-01 (VERTICAL ATTENUATOR UNIT)

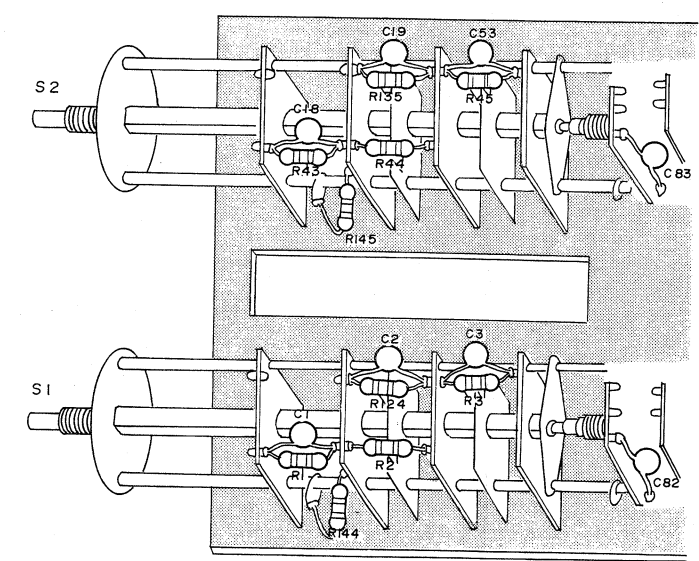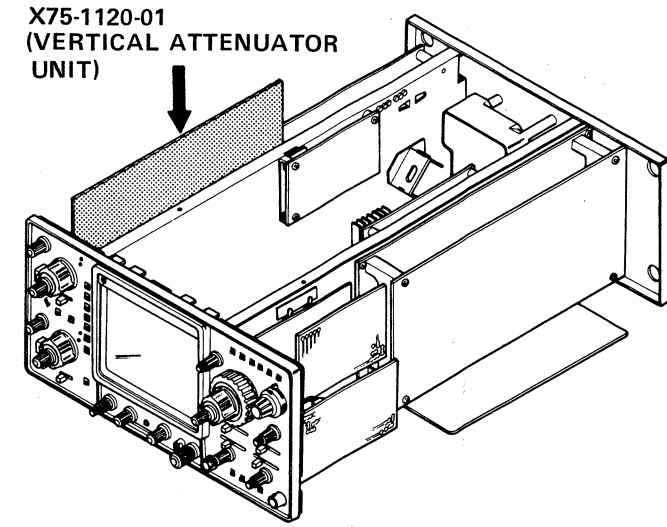


Location of Parts in the Rotary Switch

WAVEFORMS

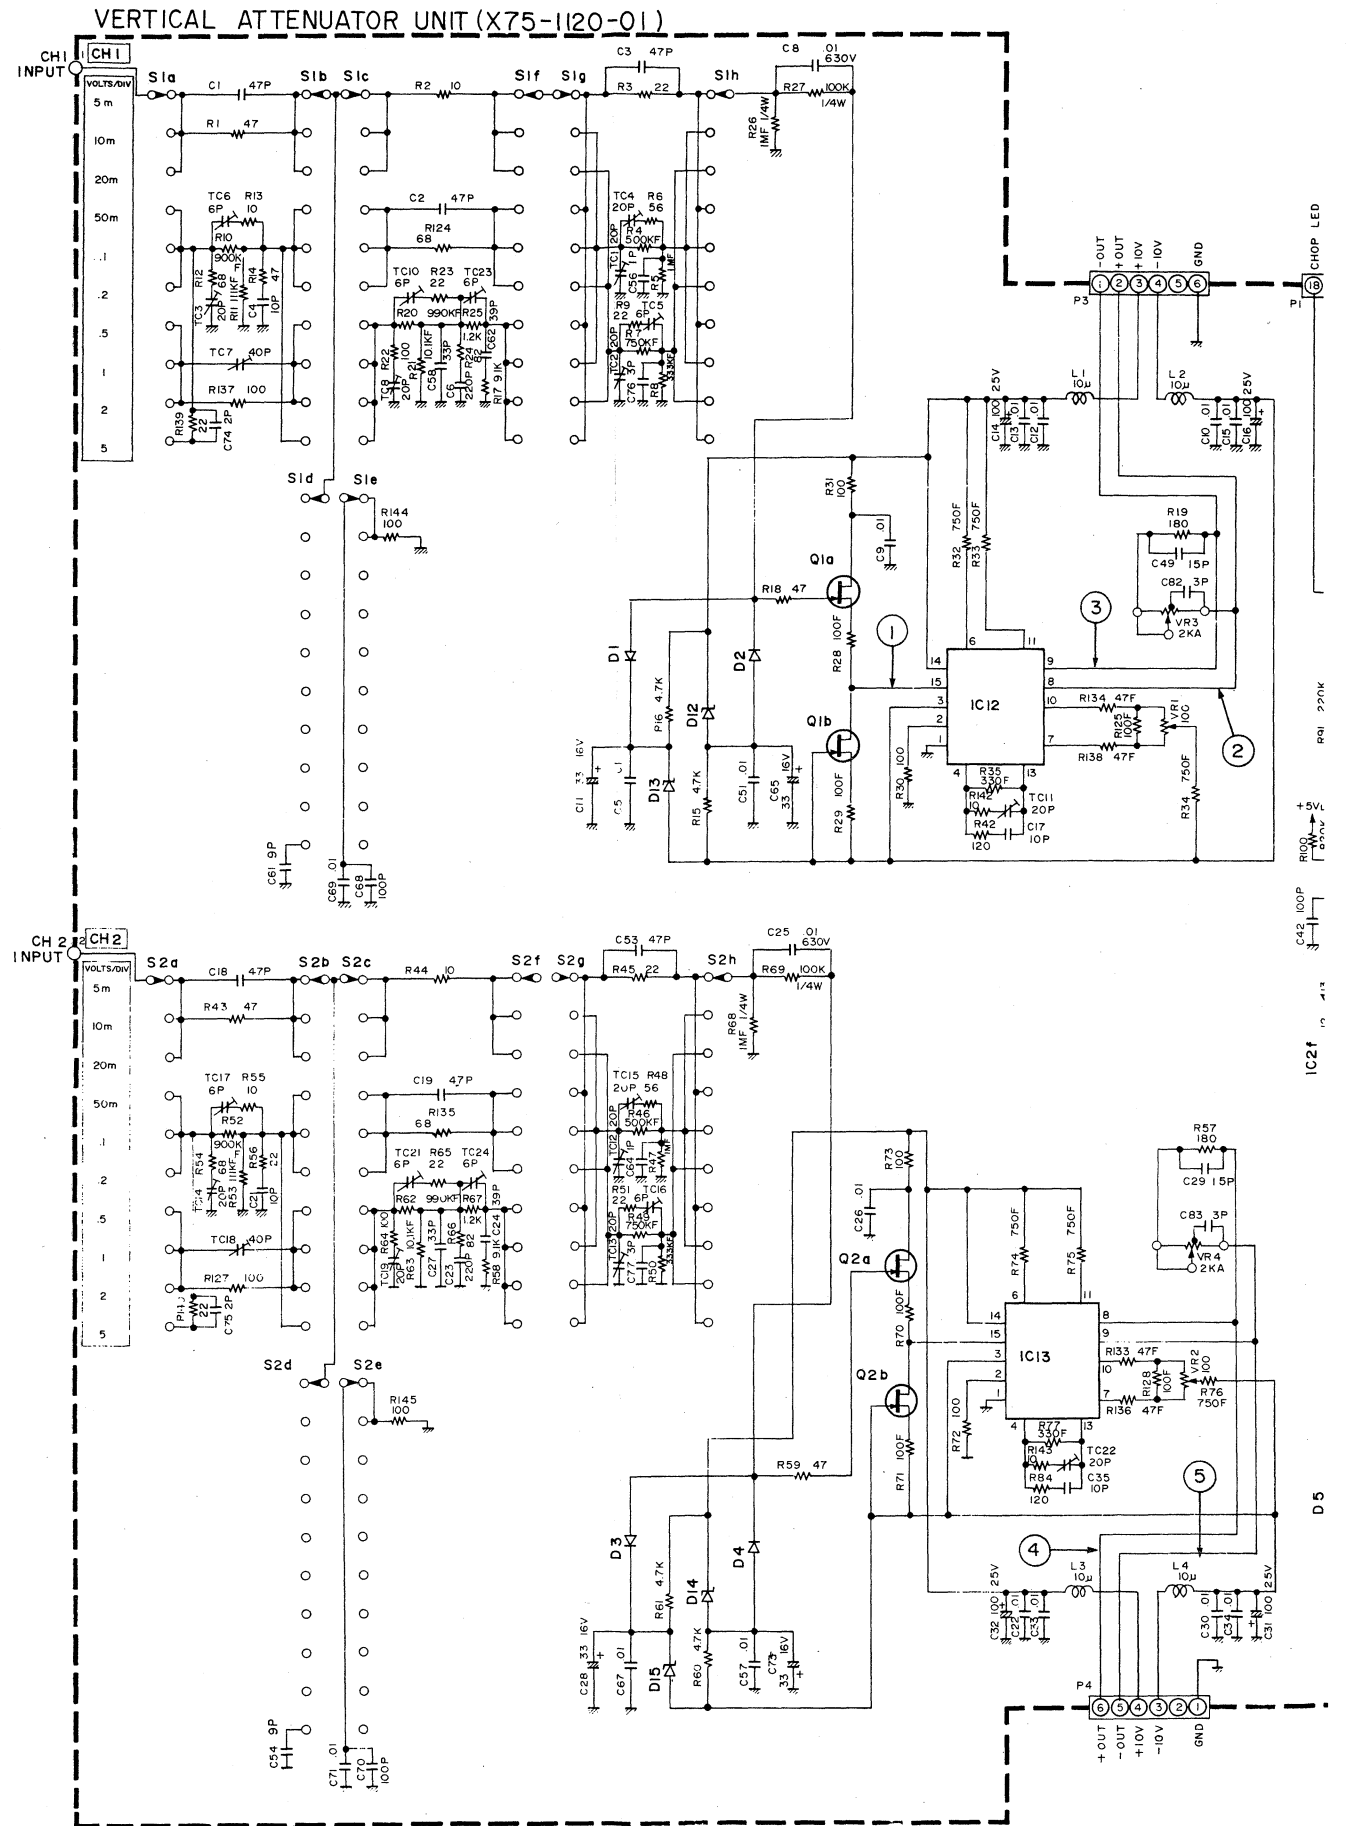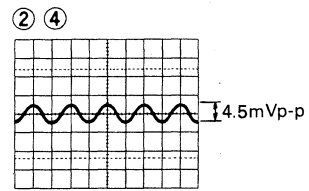

SCHEMATIC DIAGRAM


VERTICAL ATTENUATOR UNIT (X75-1120-01)

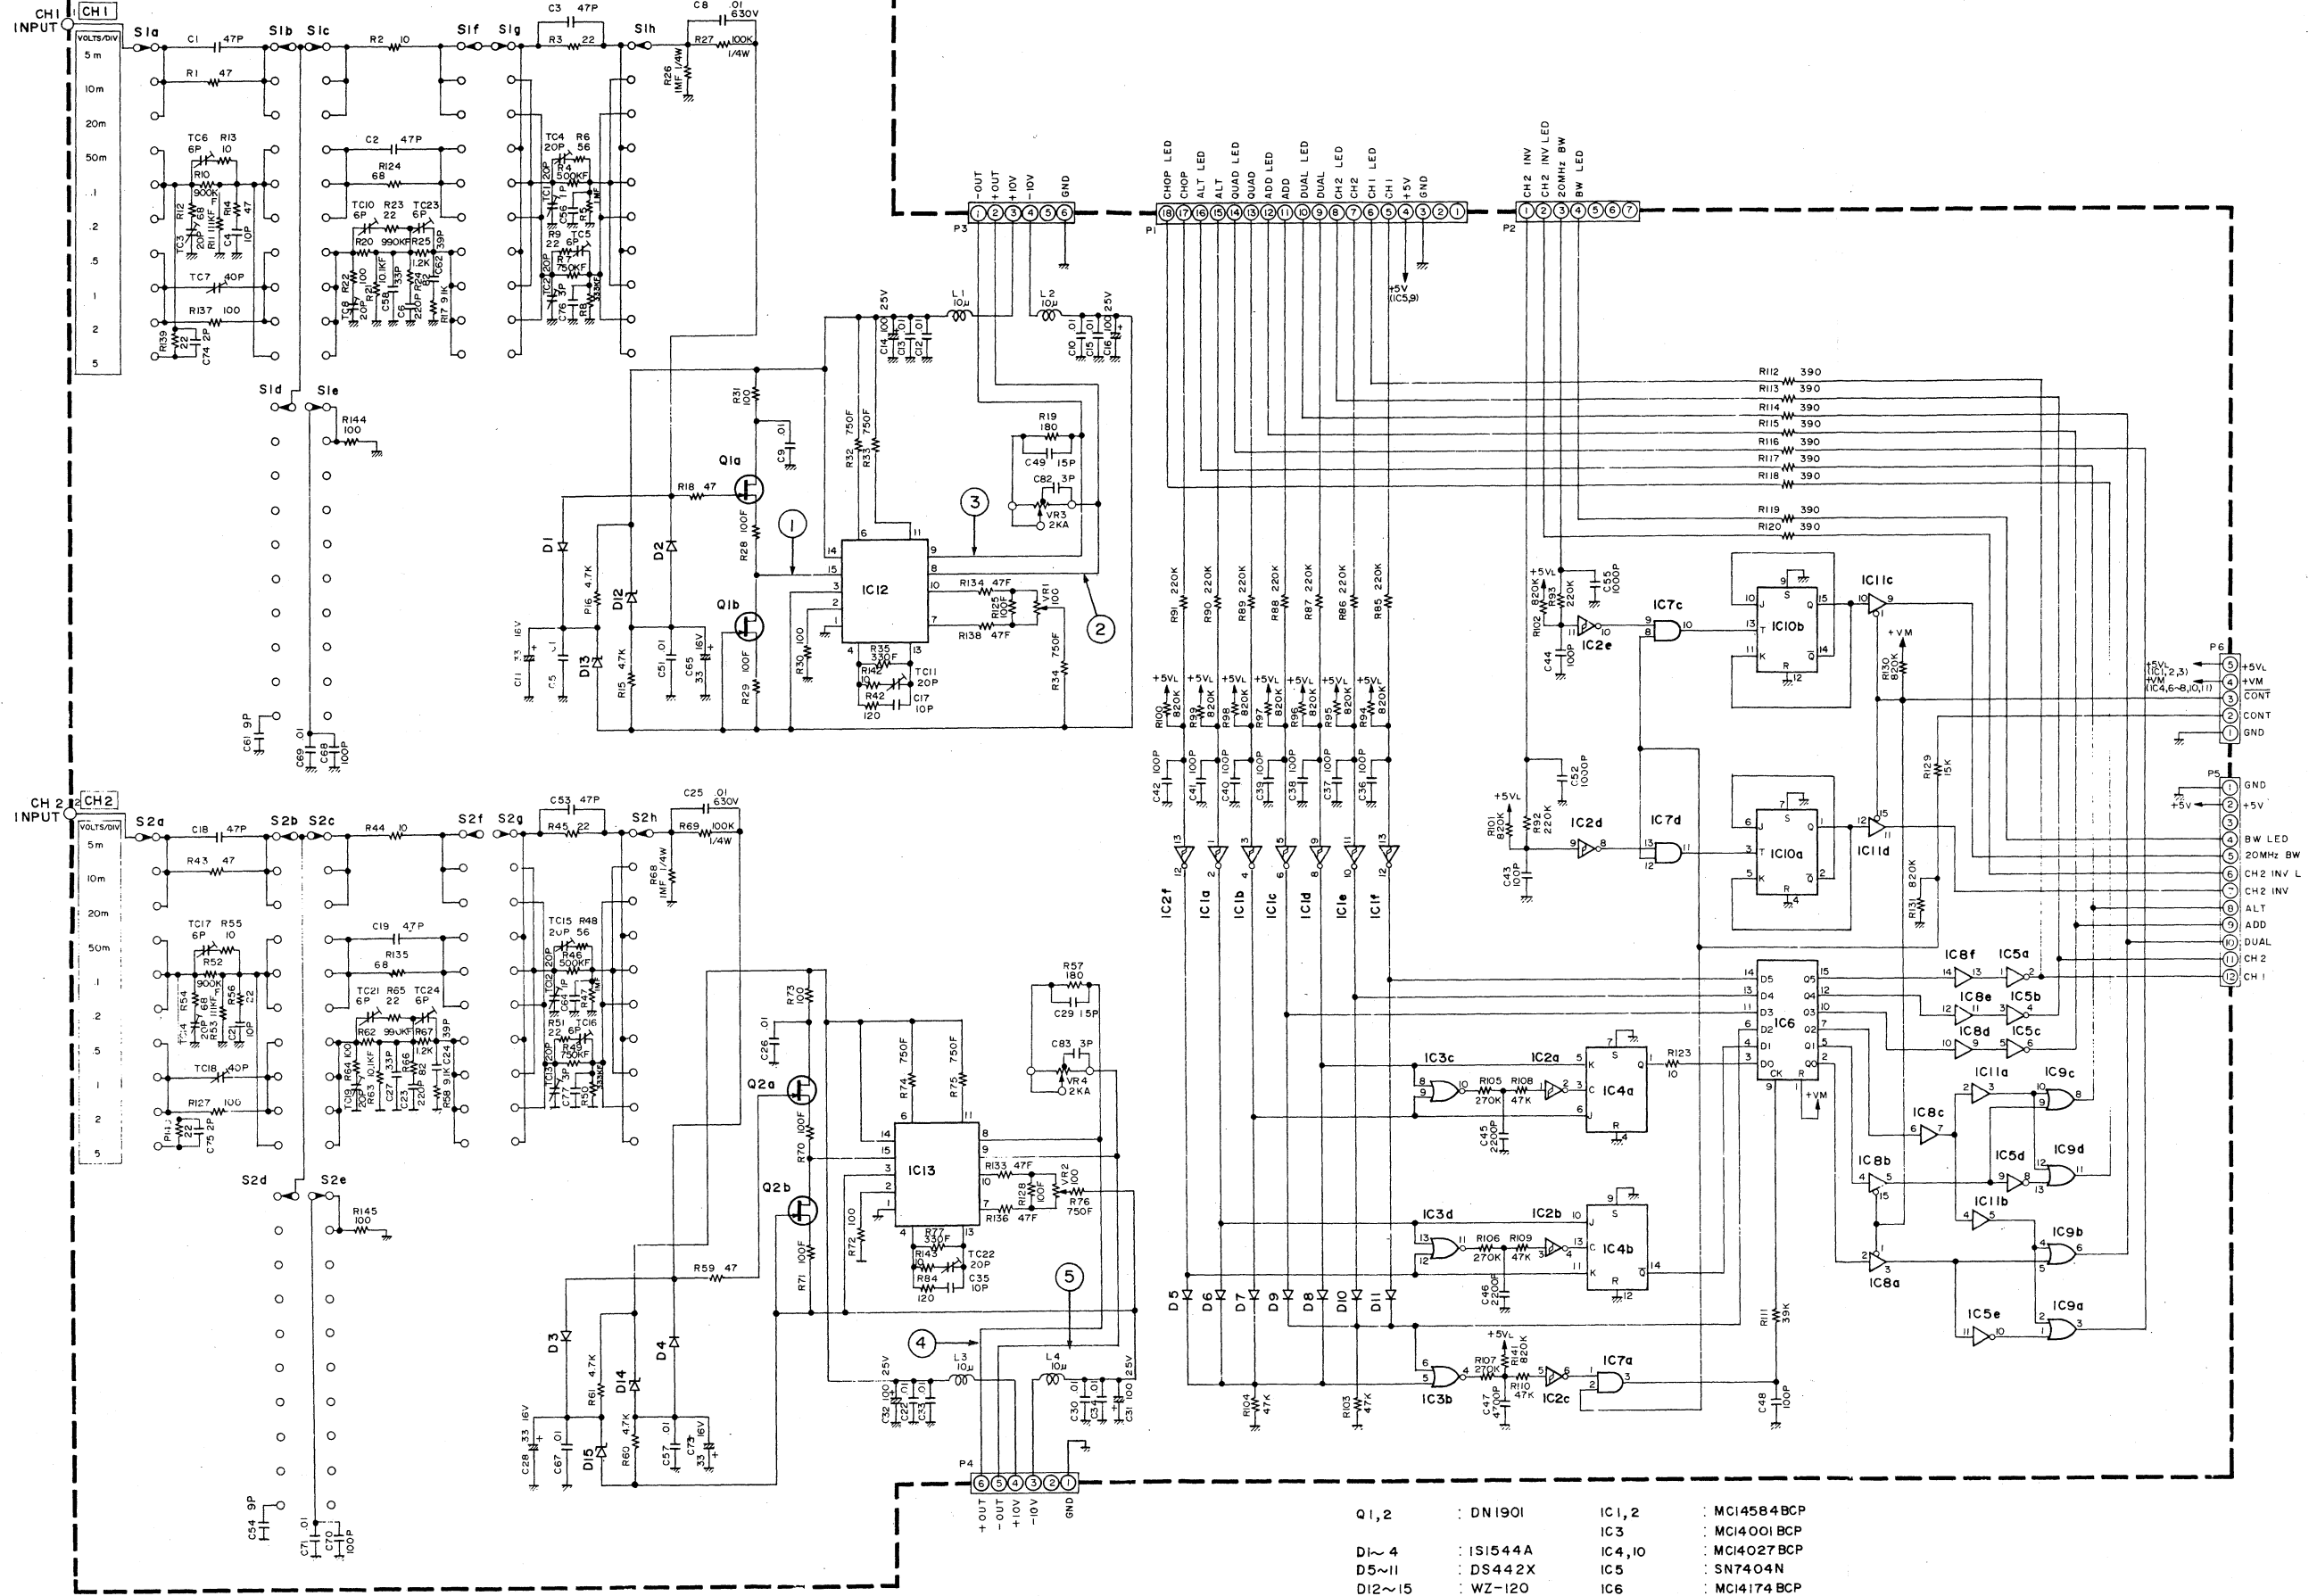


PC BOARD

X73-1320-01

X73-132


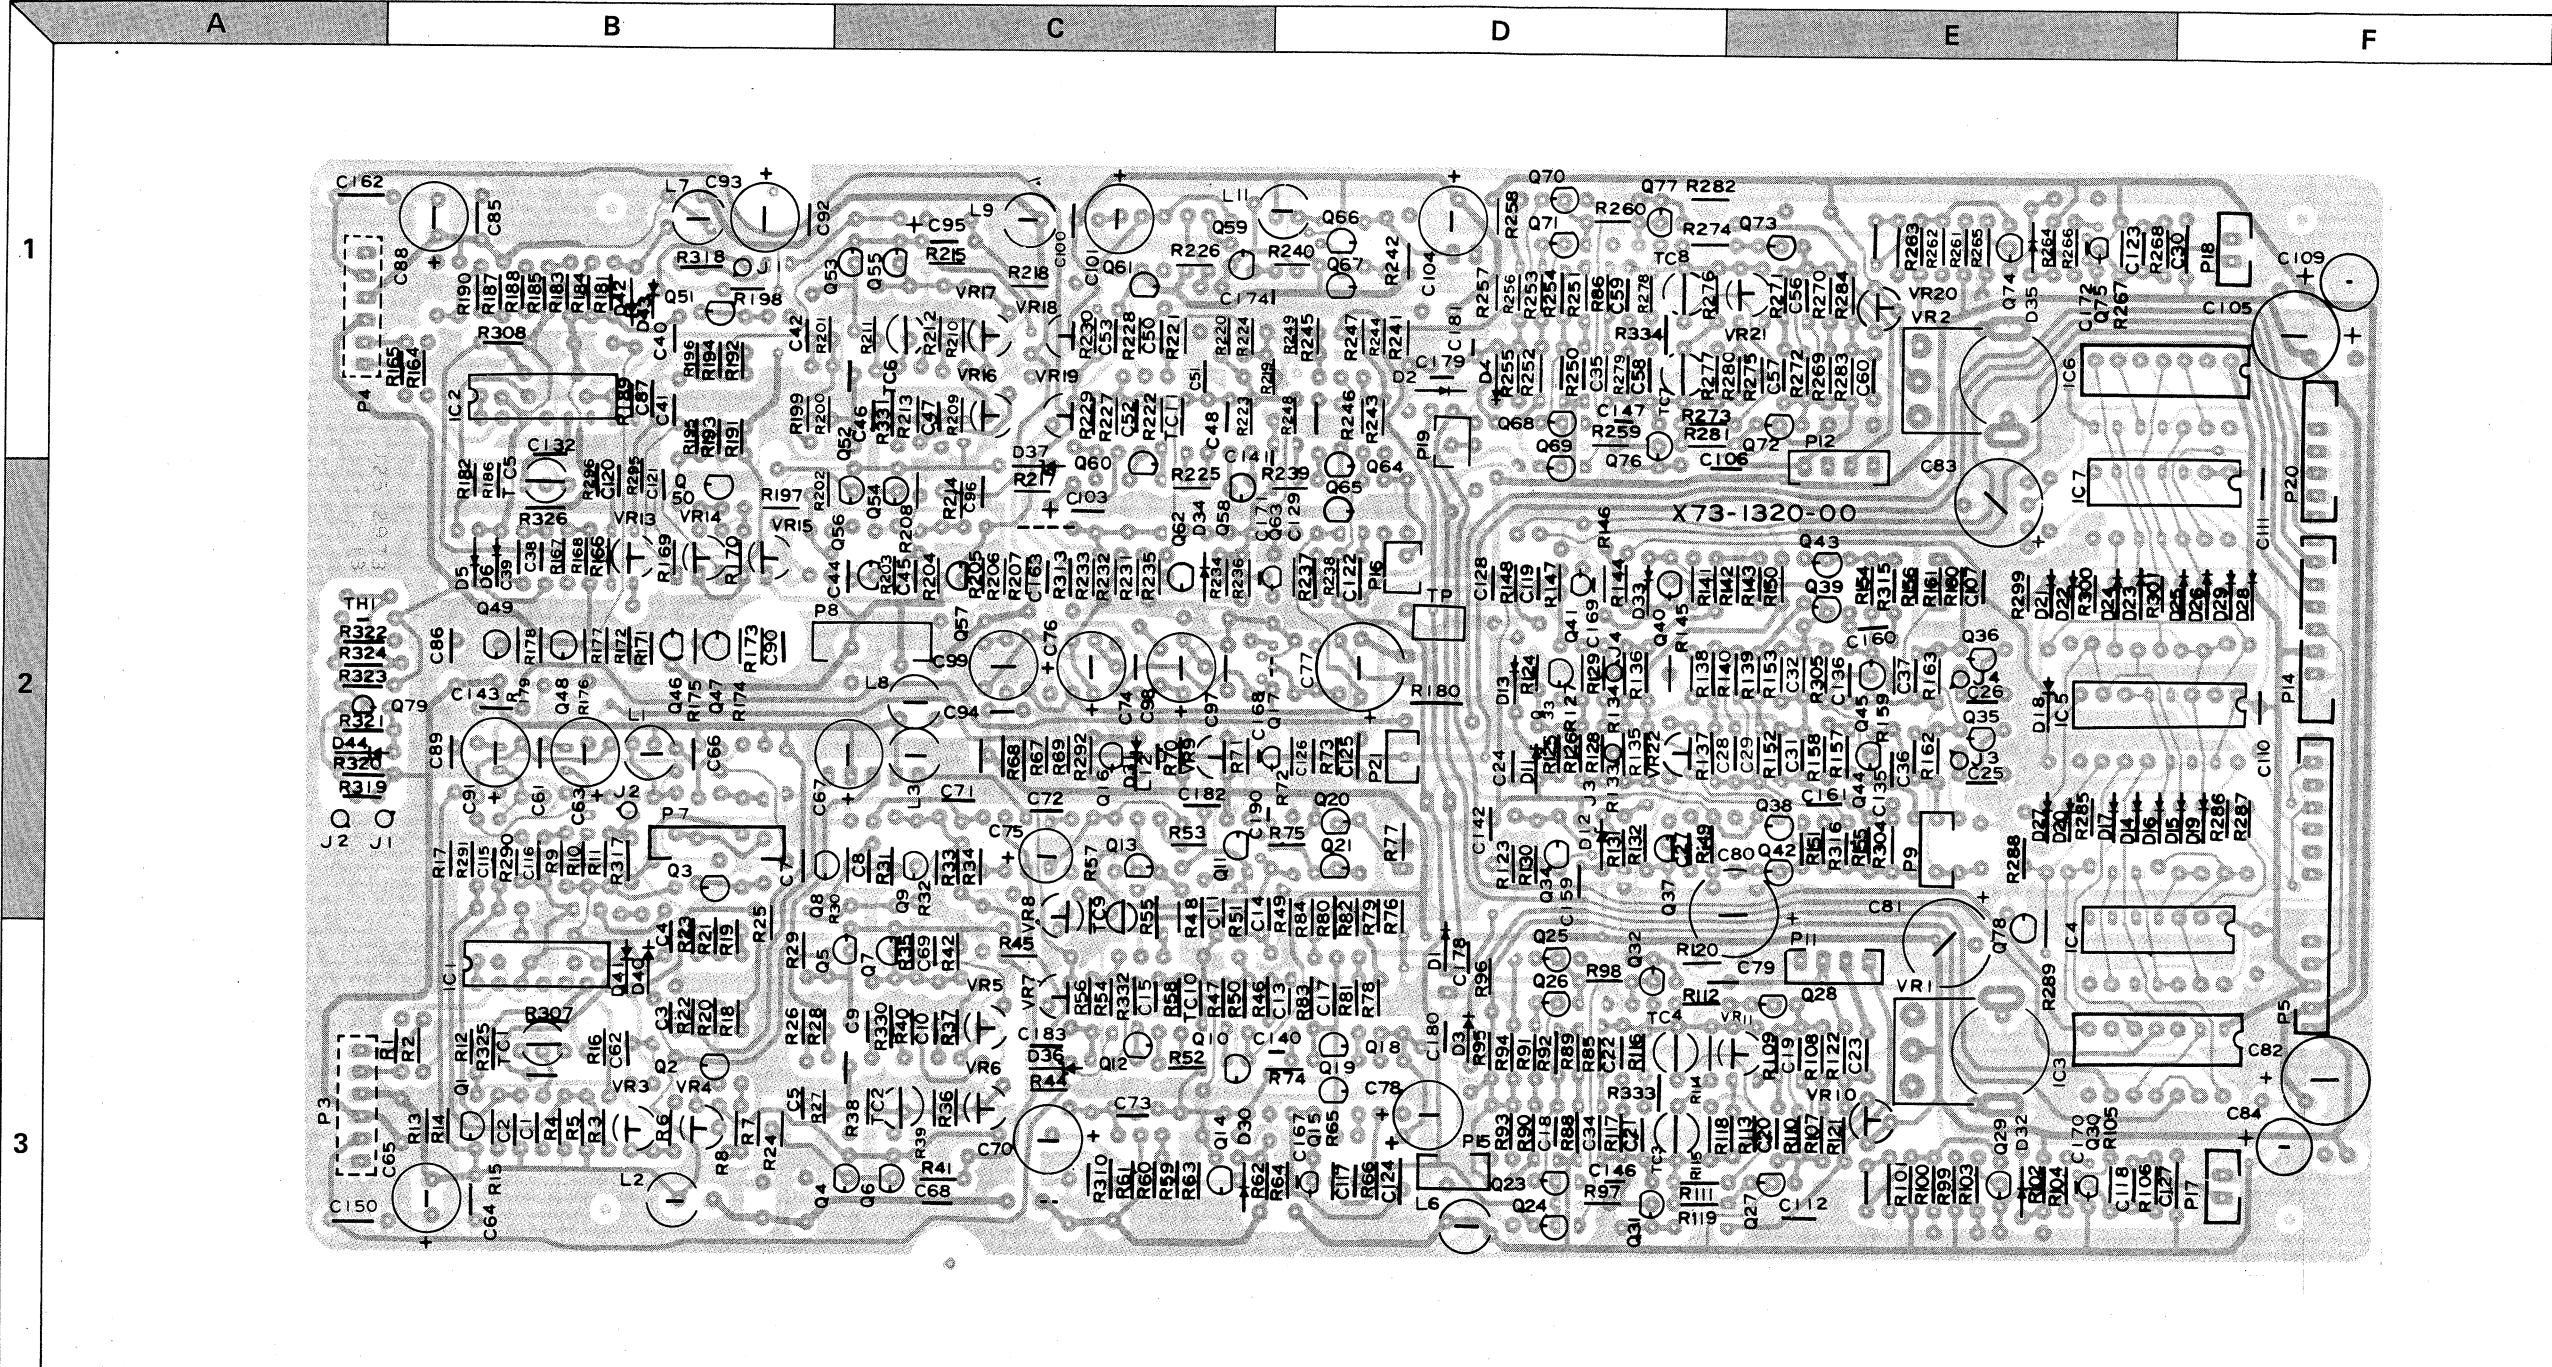


X73-1320-01
(V. PRE AMP UNIT)

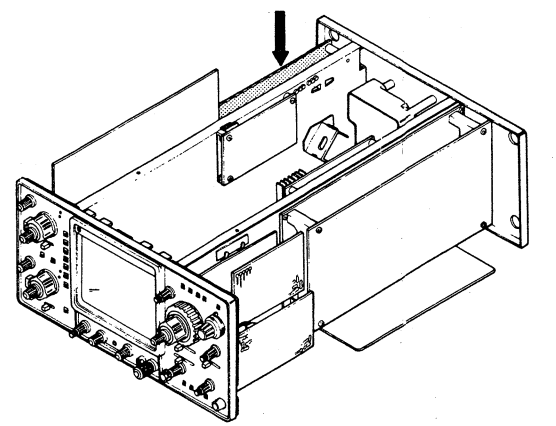


X73-1320-01

D E F

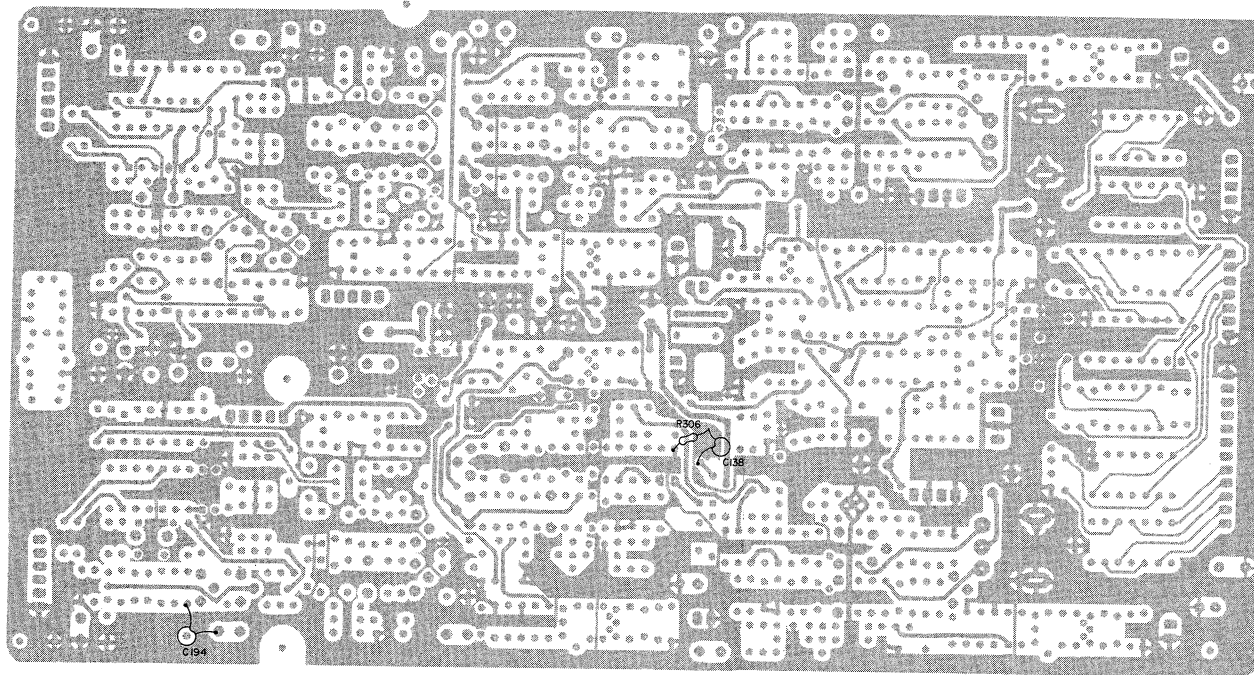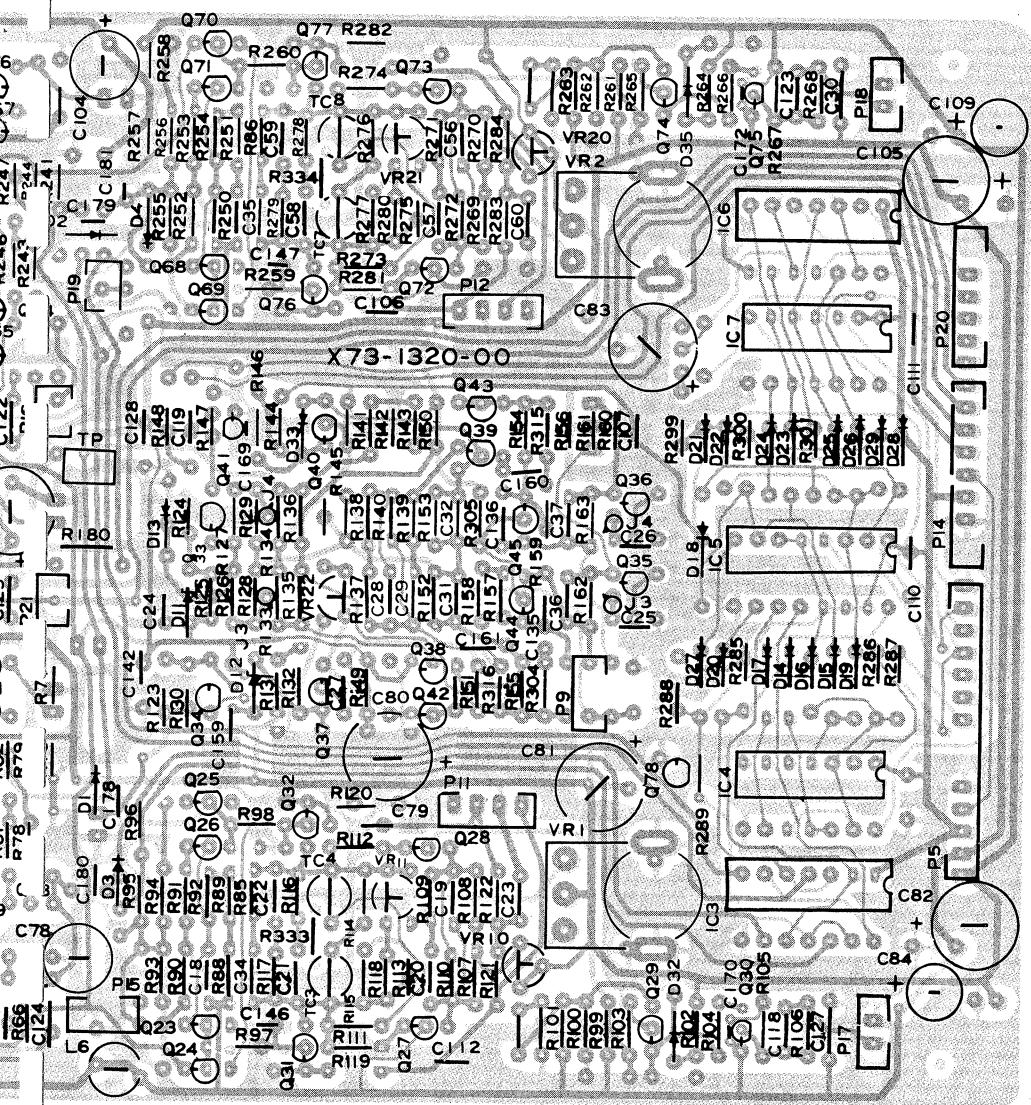


(Parts Side View)

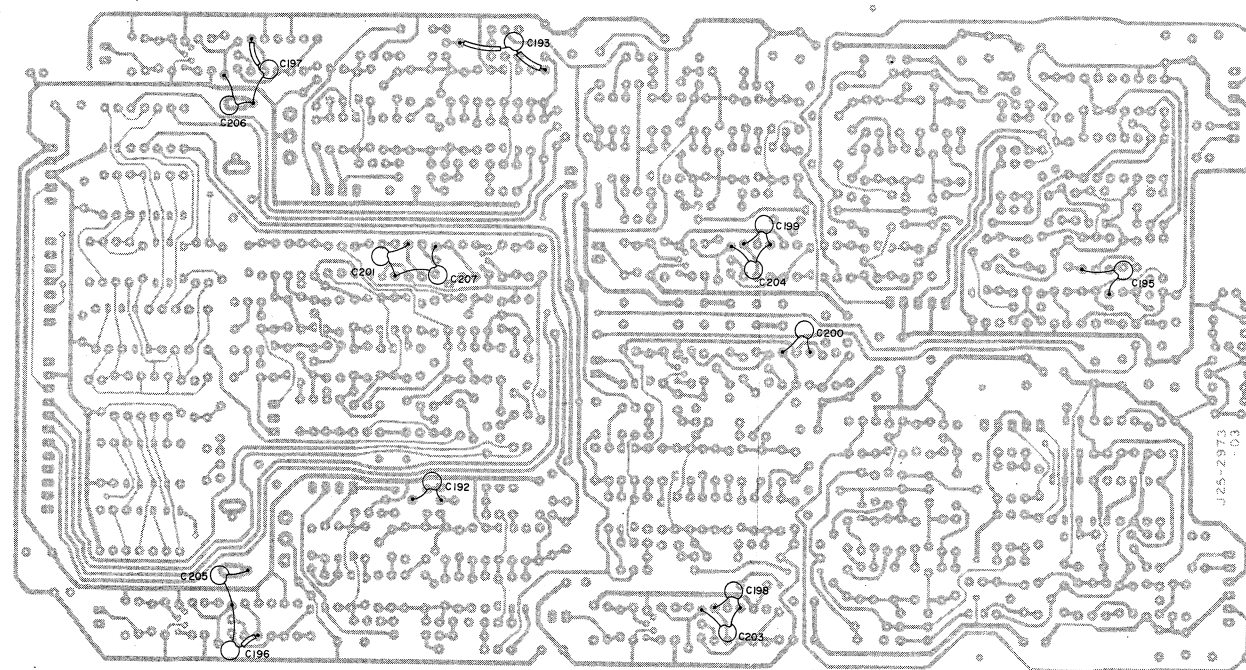















(Foil Side View)

X73-1320-01 (V. PRE AMP UNIT)

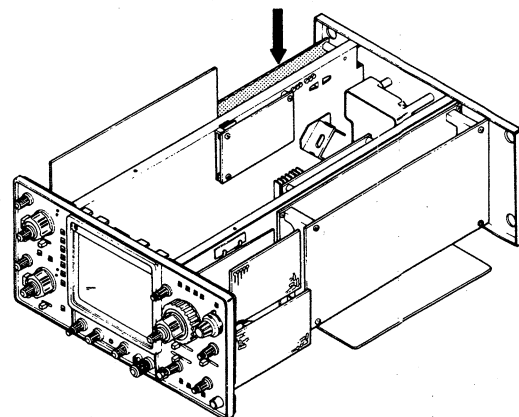


WAVEFORMS

SCHEMATIC I

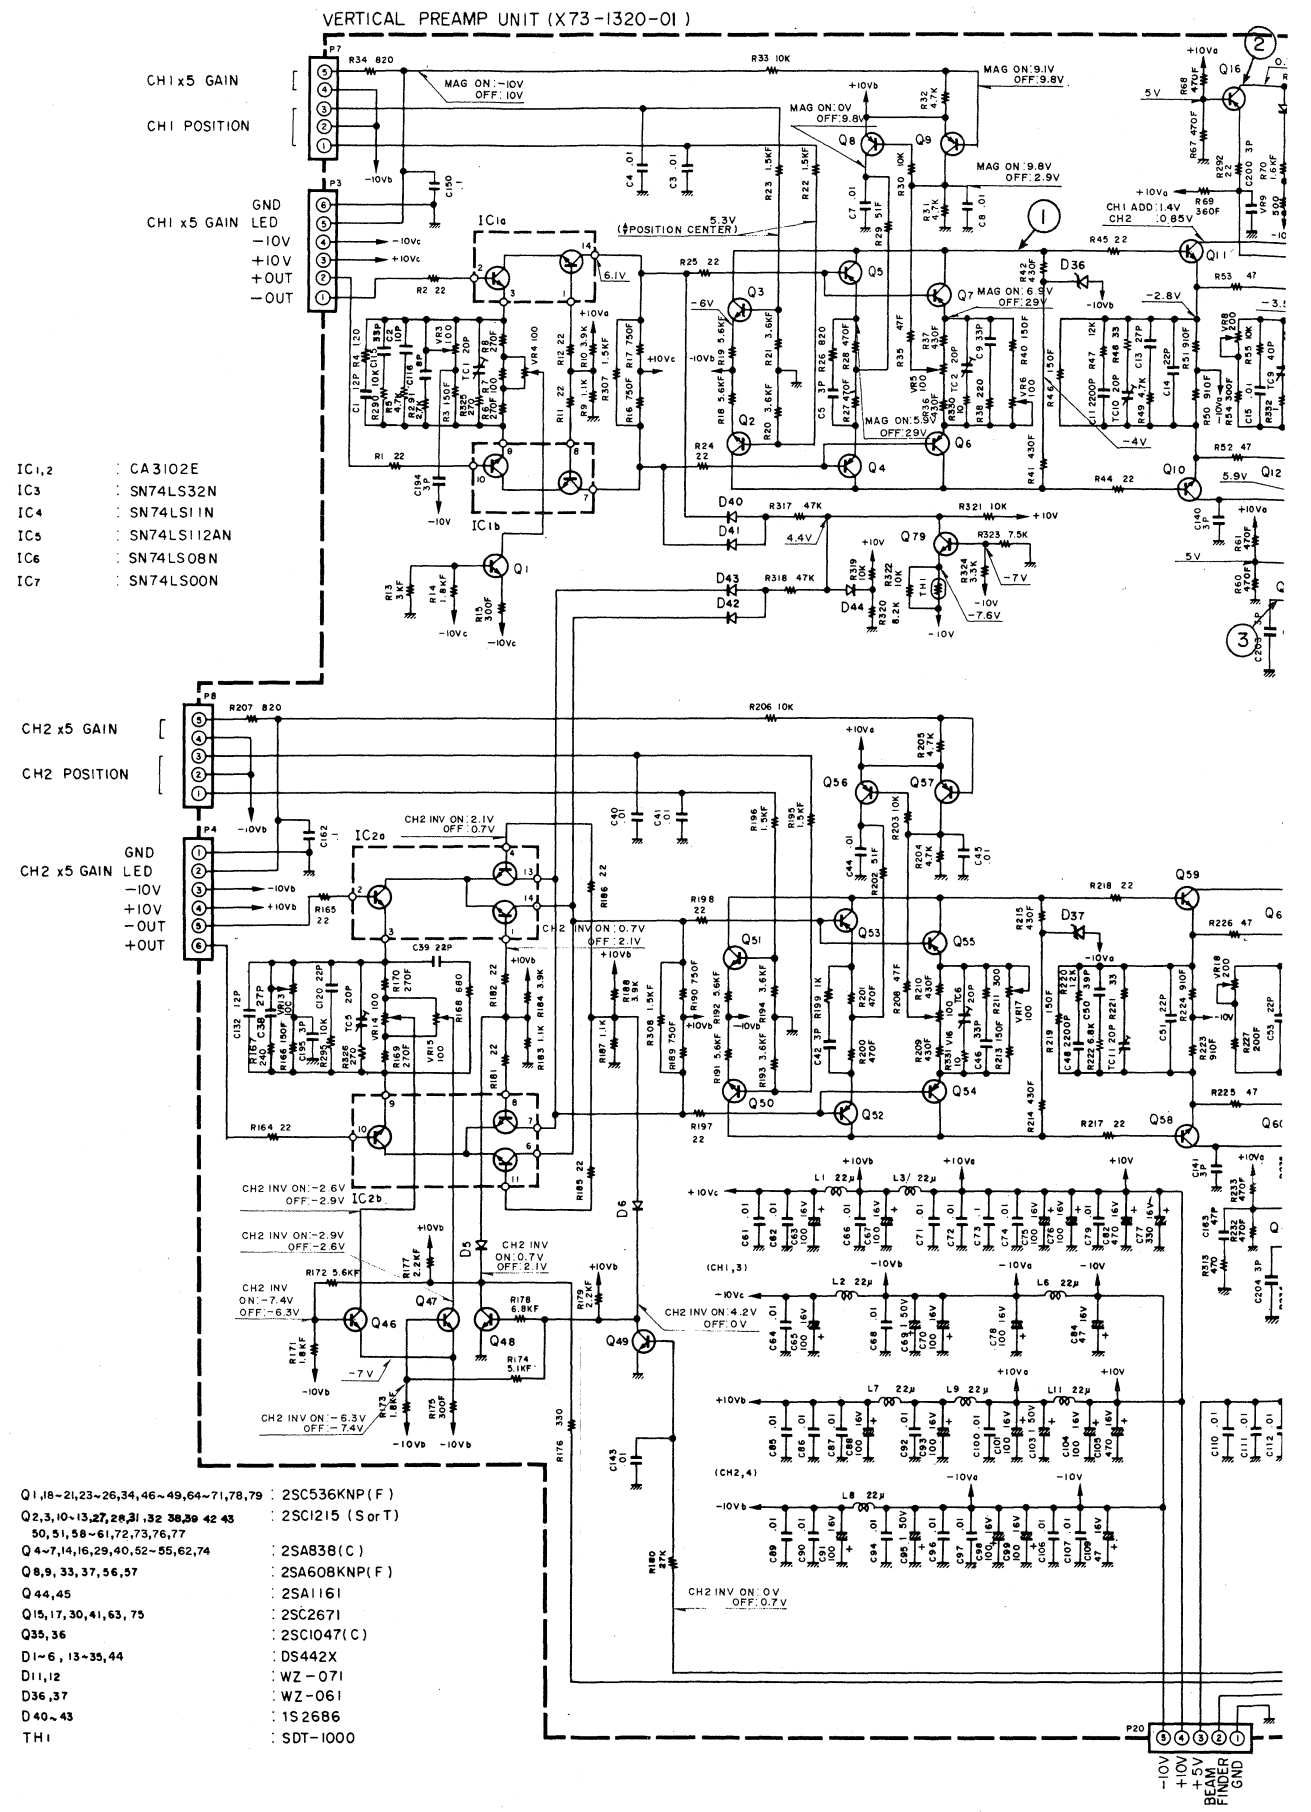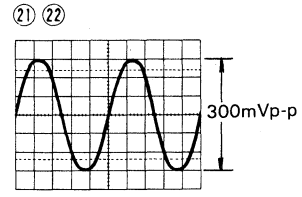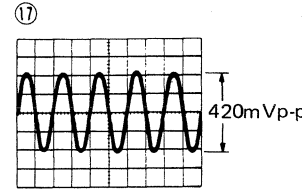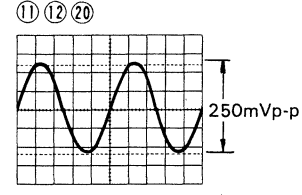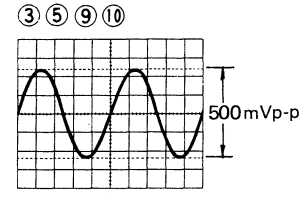




SCHEMATIC DIAGRAM

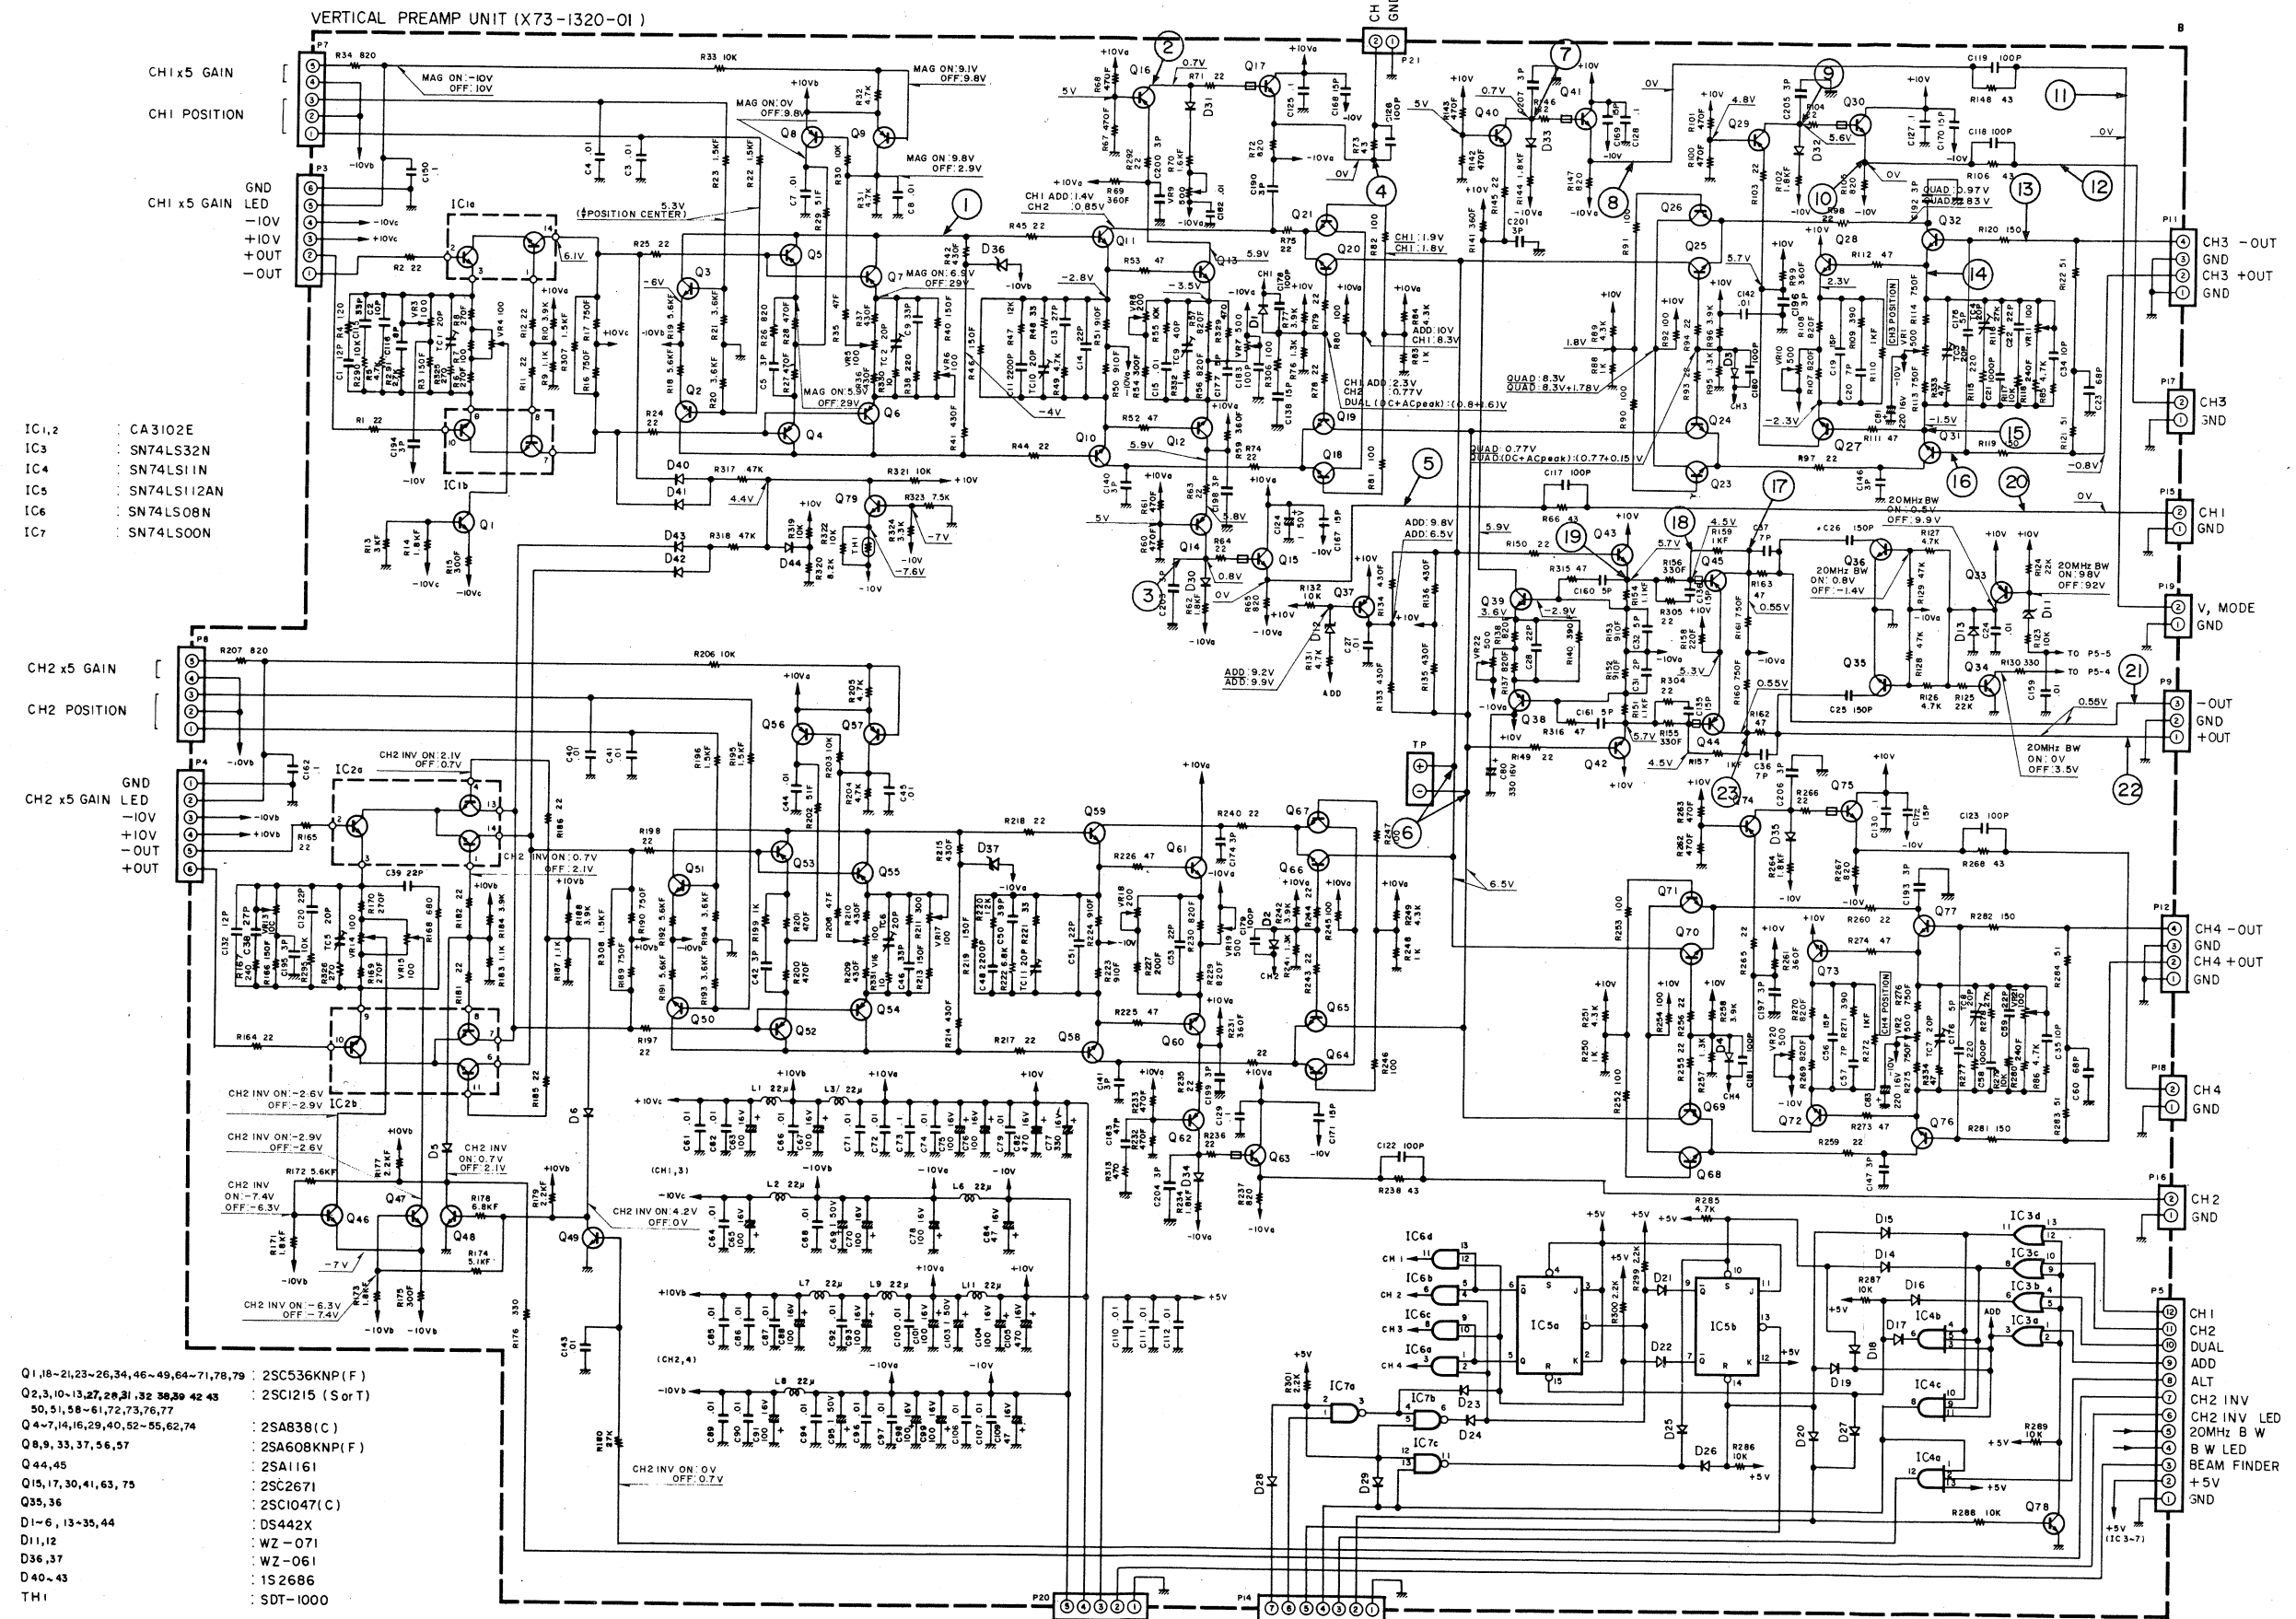






PC BOARD

X73-1330-01

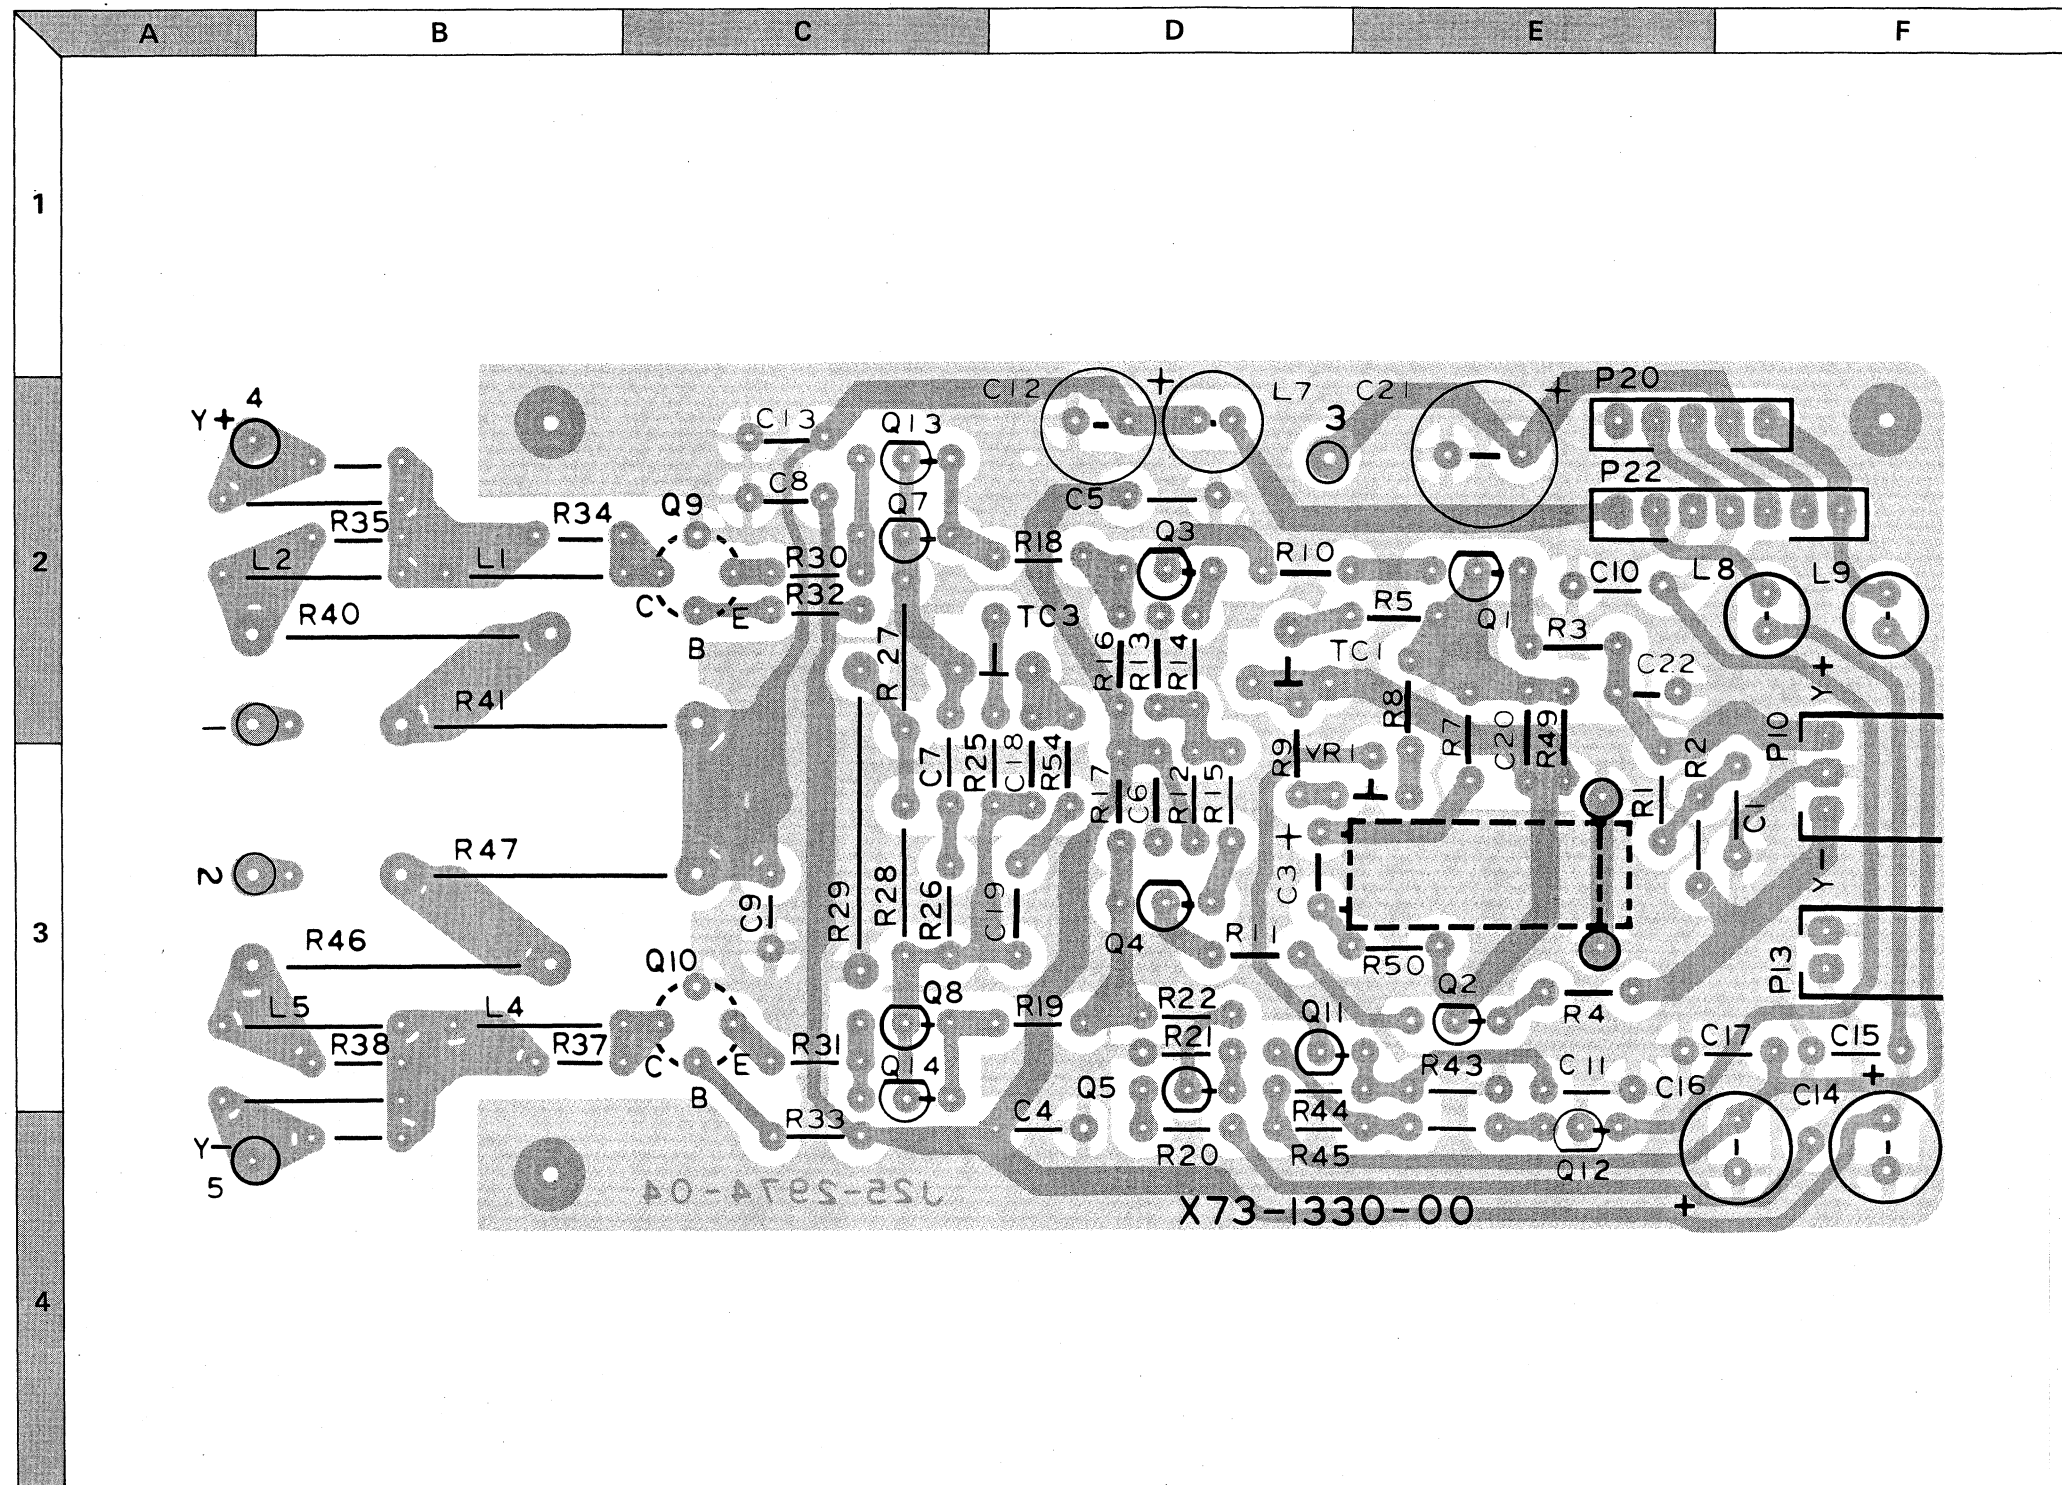


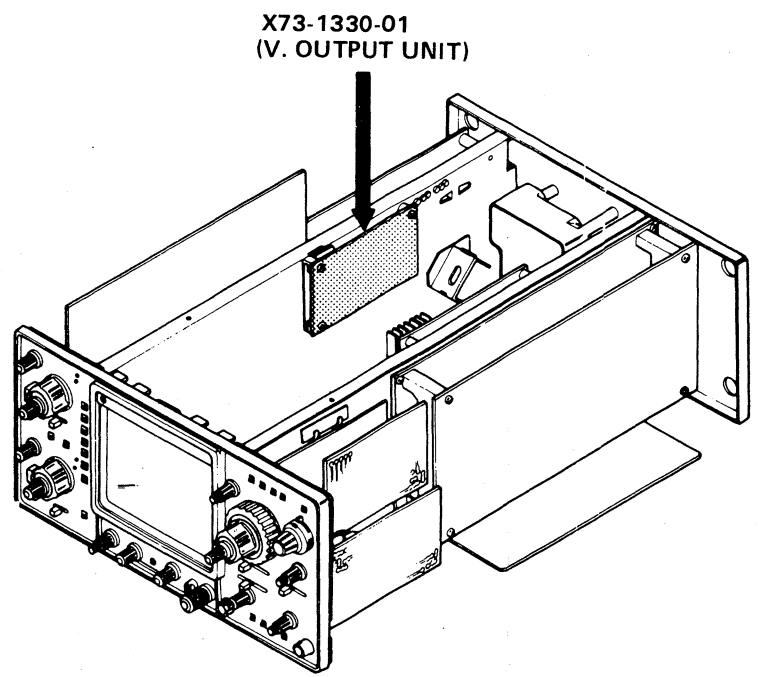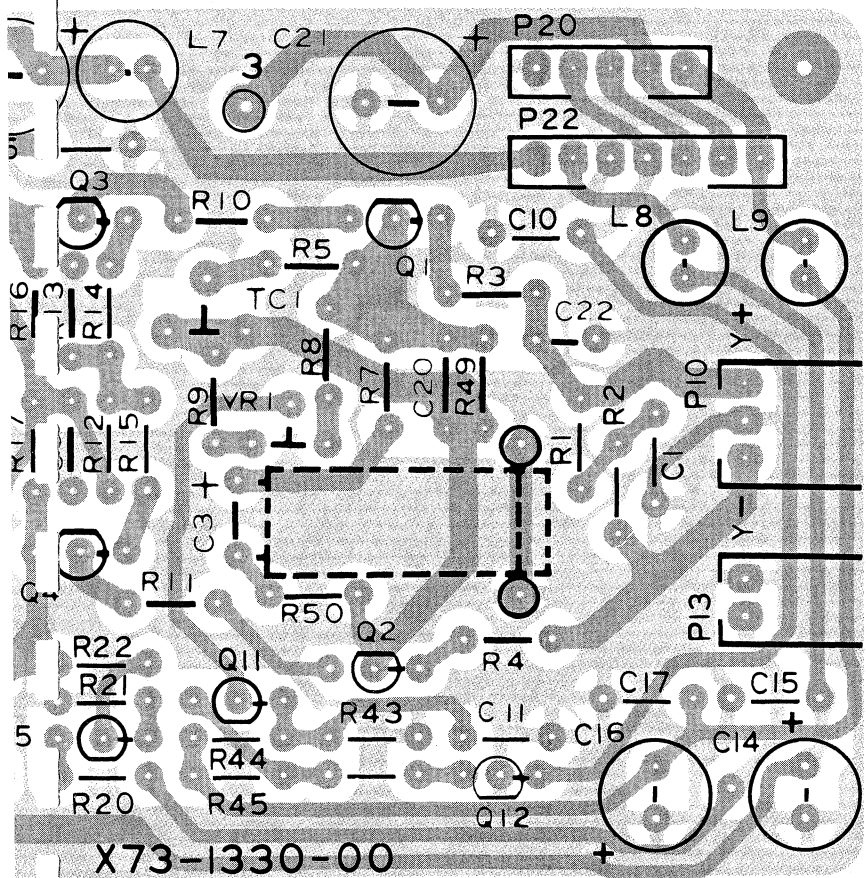


WAVEFORMS

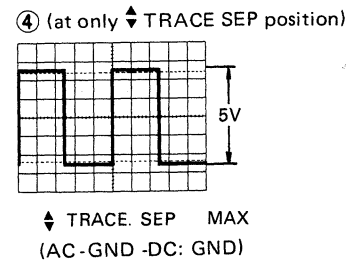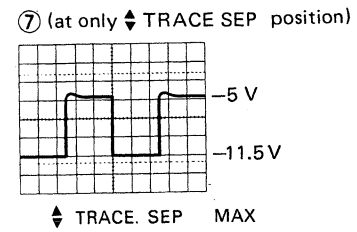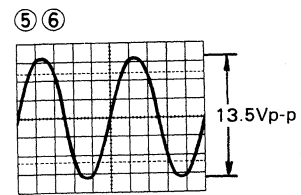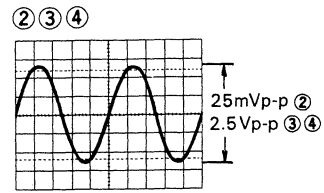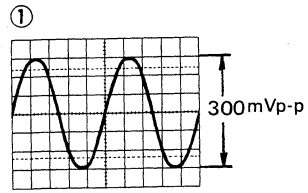

VERTICAL OUTPUT AMP UNIT (X73-1330-01)

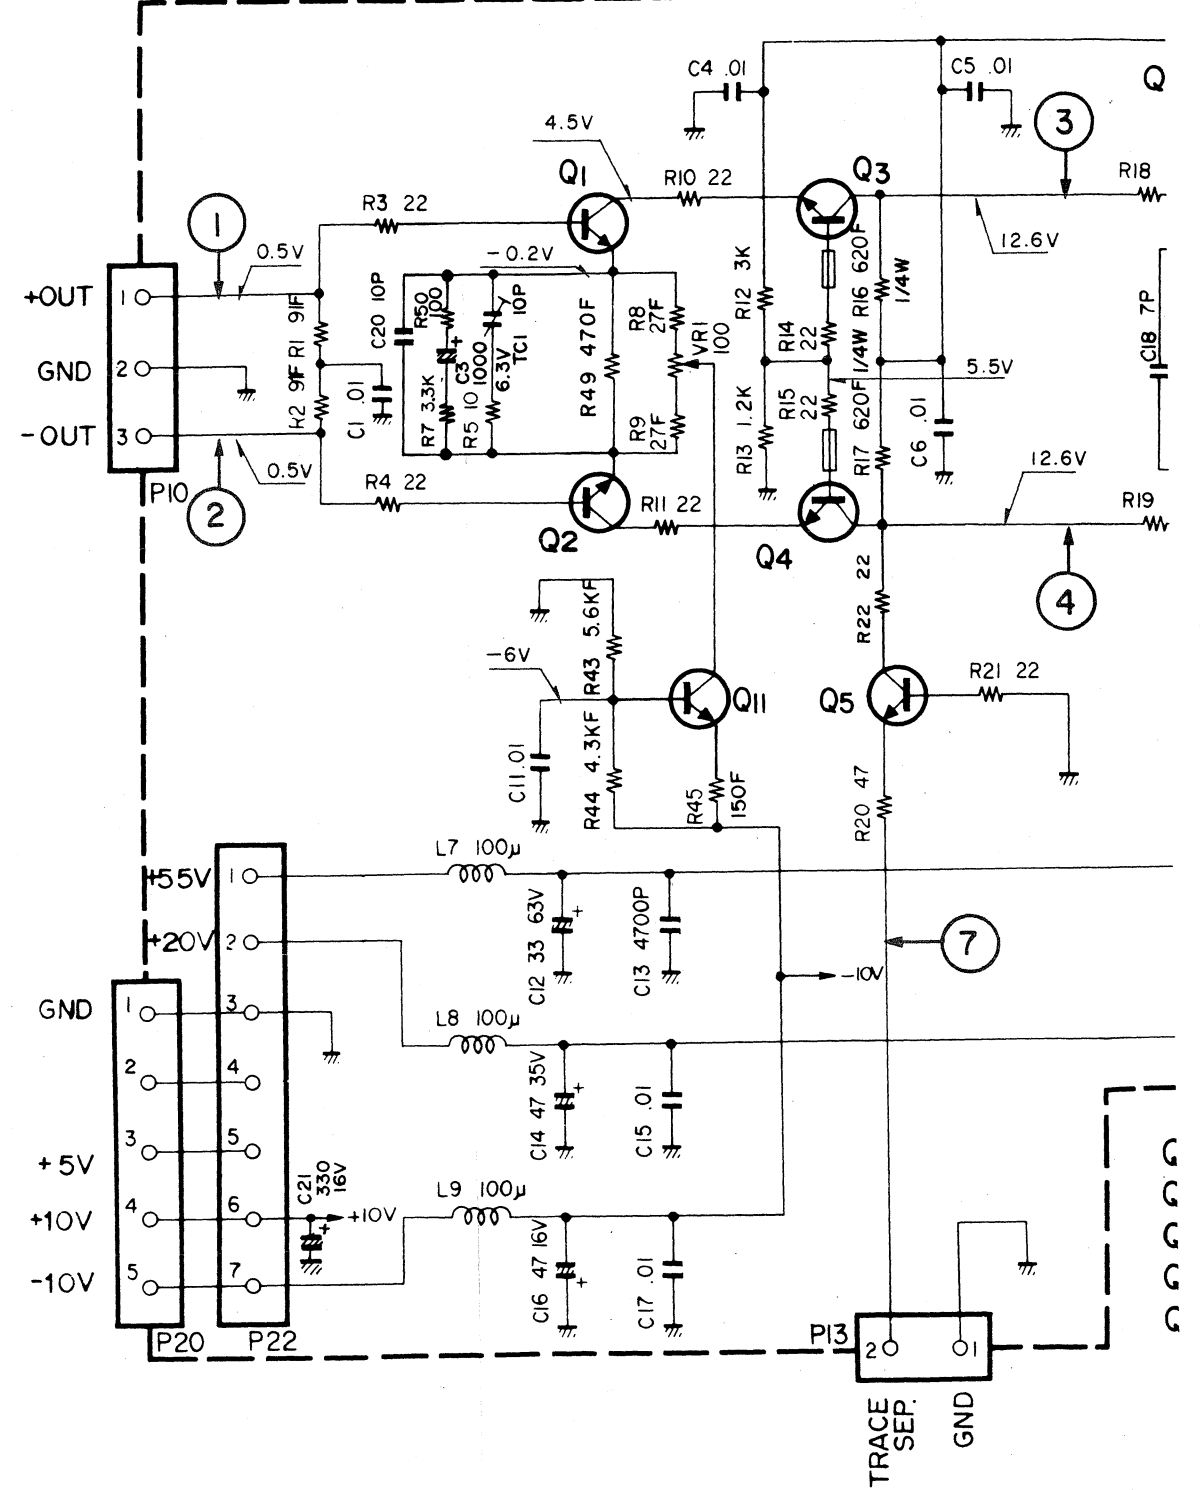


SCHEMATIC DIAGRAM

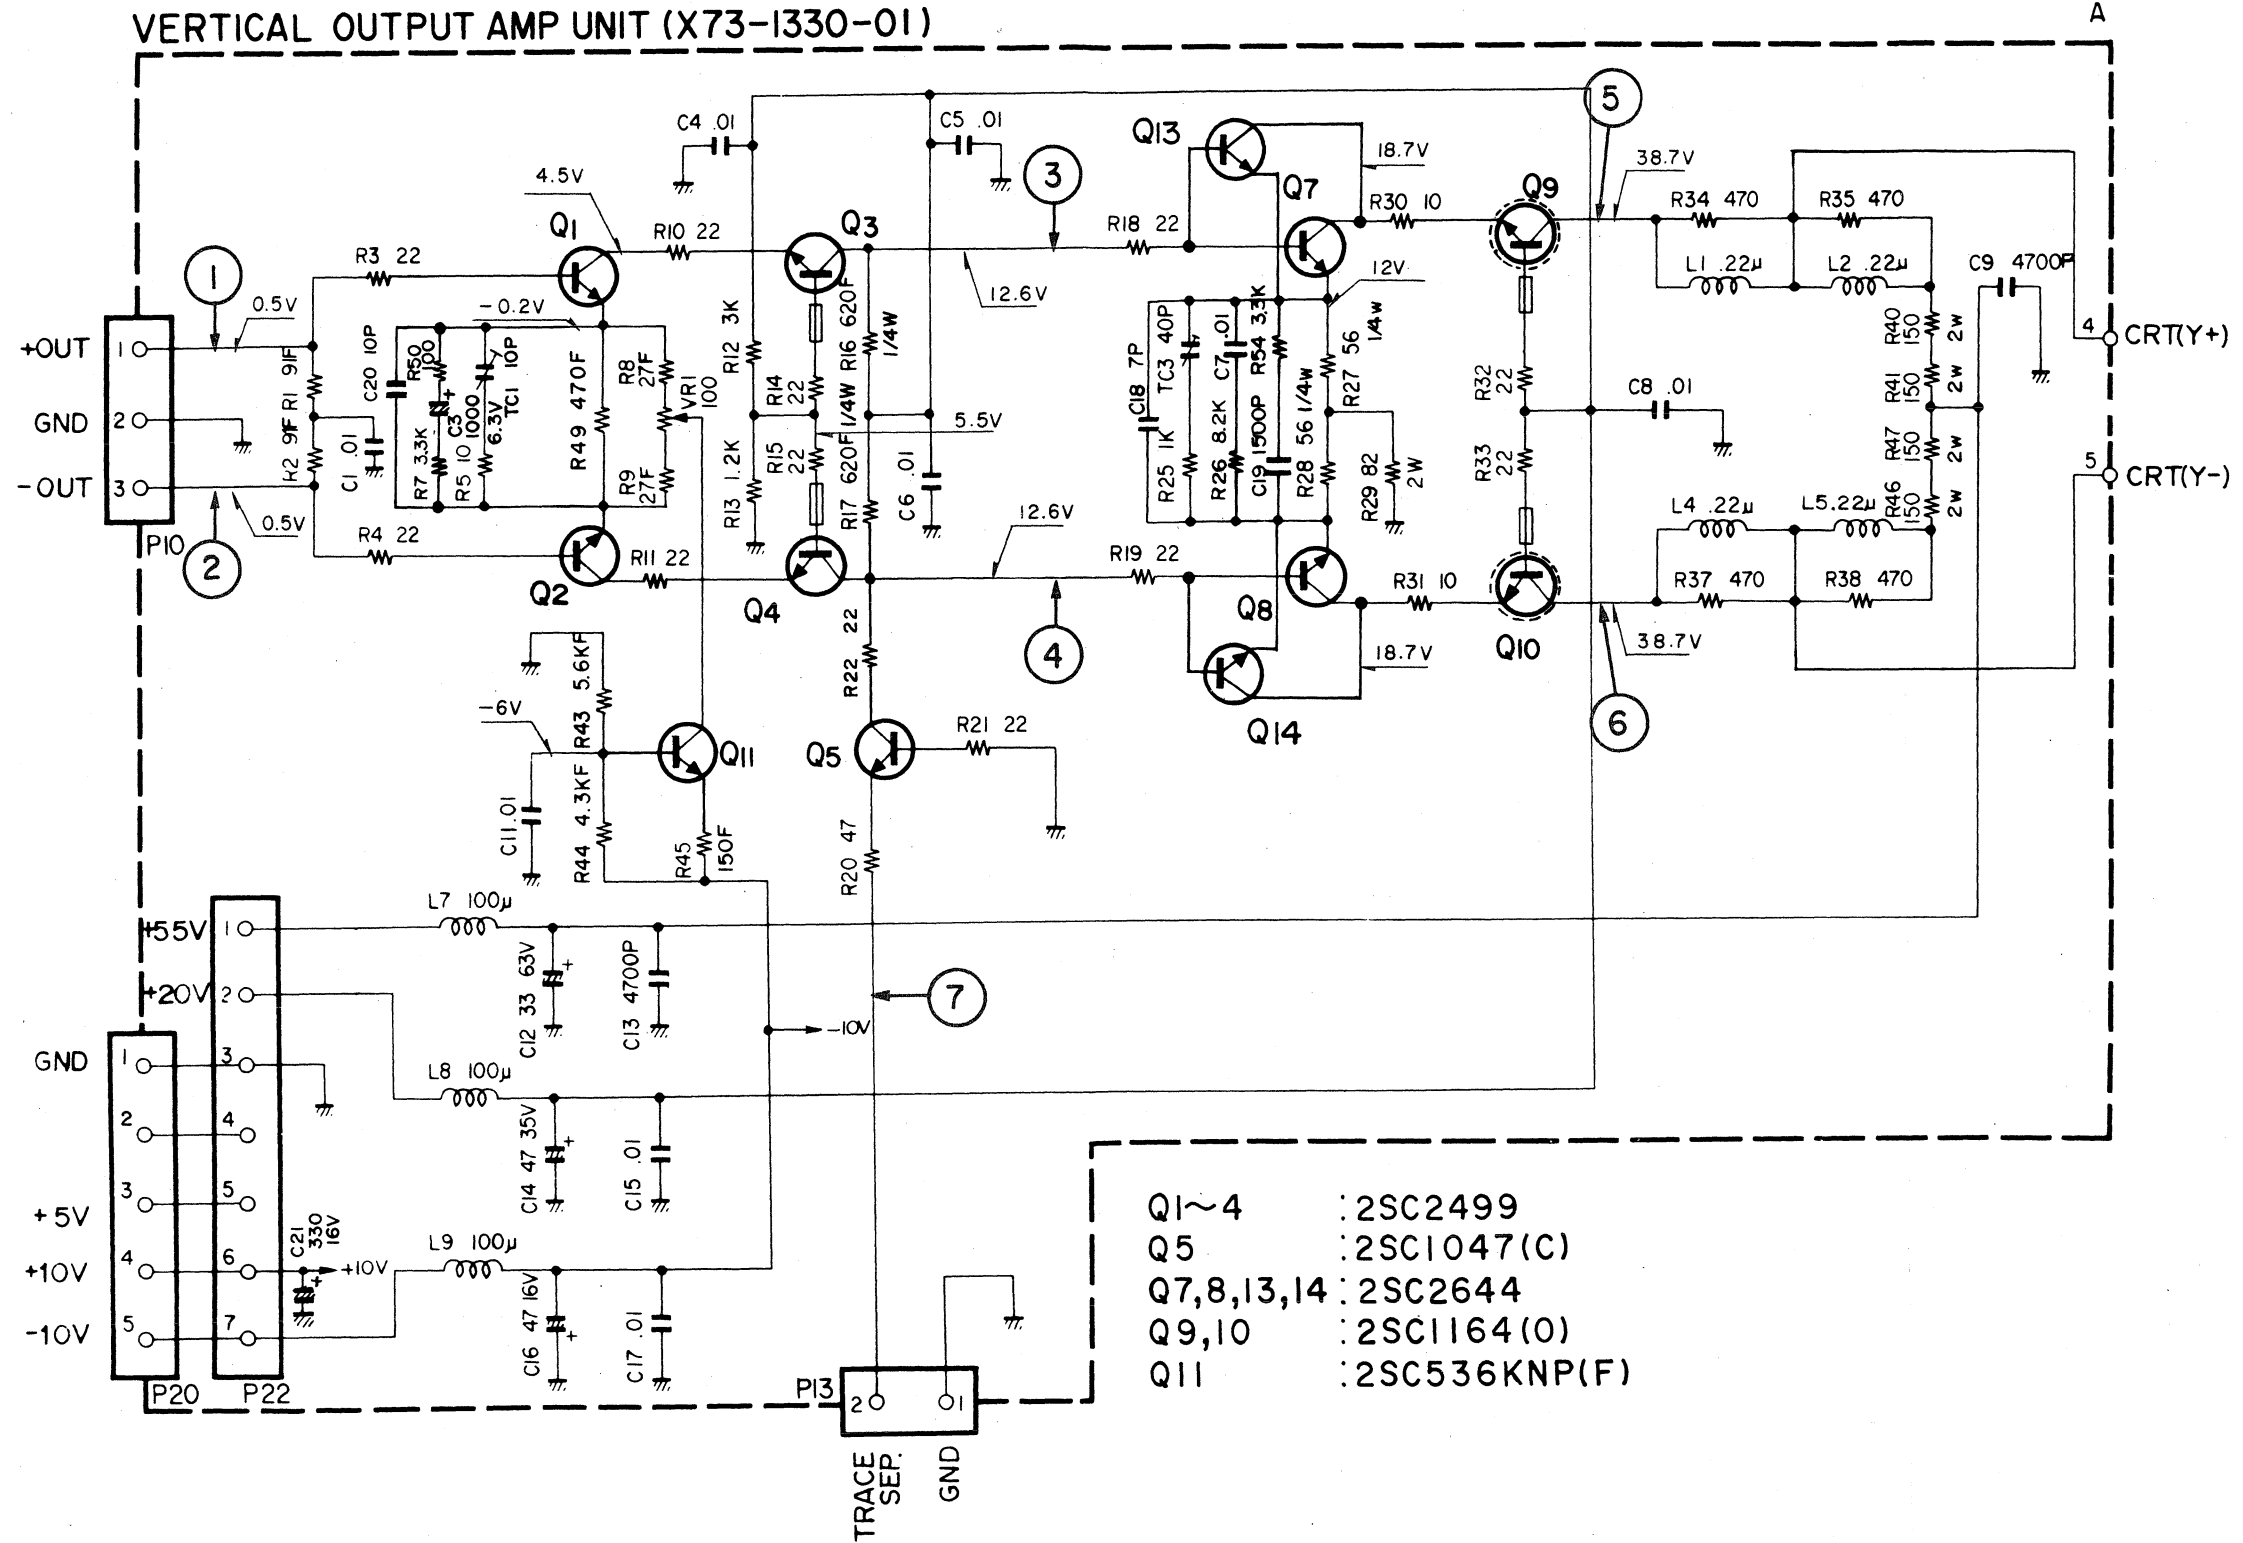



PC BOARD

X74-1310-01

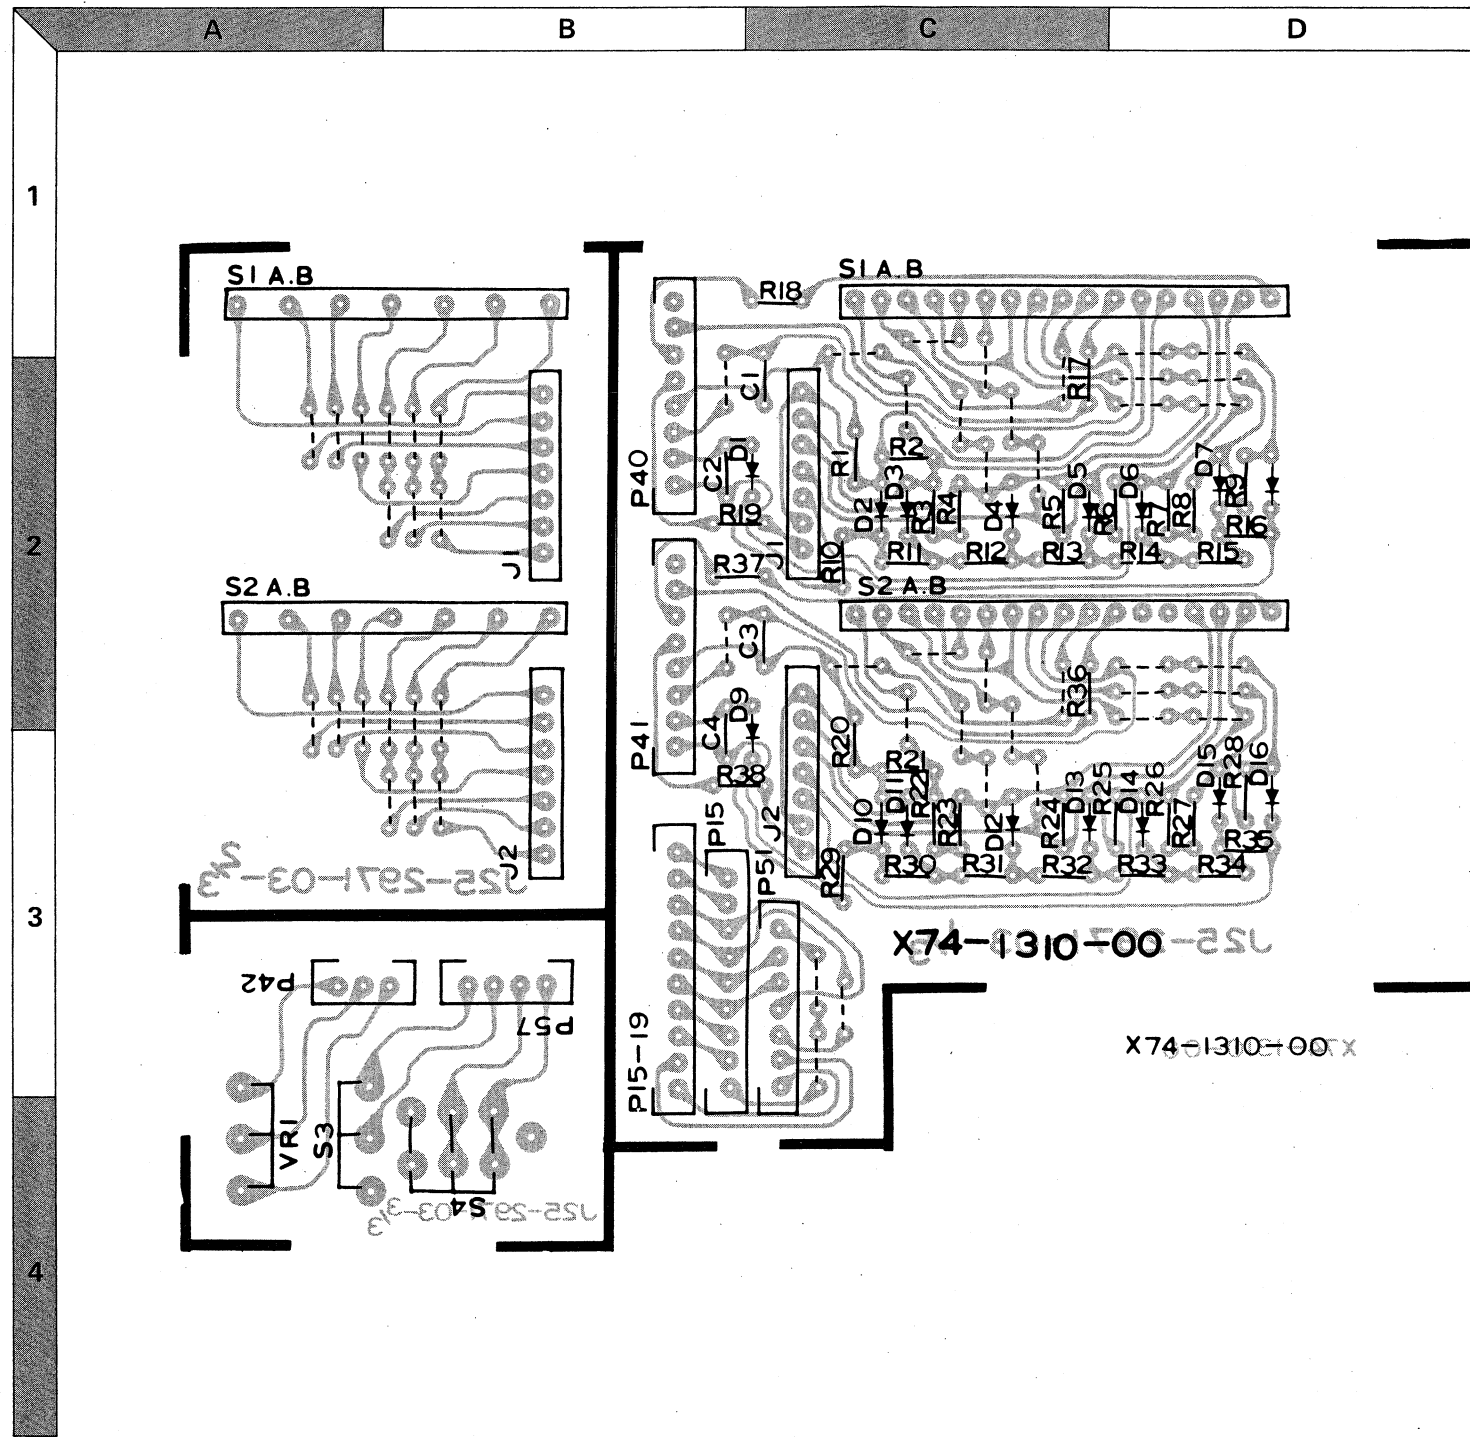


CAUTION
 Because the silk symbols in P42 and P57 are reversed,
 please refer to the Schematic Diagram.

PC BOARD

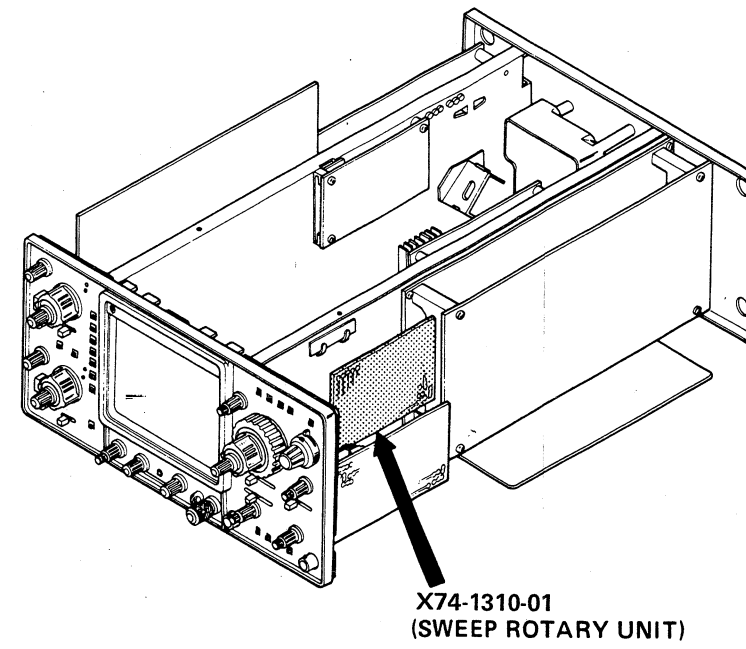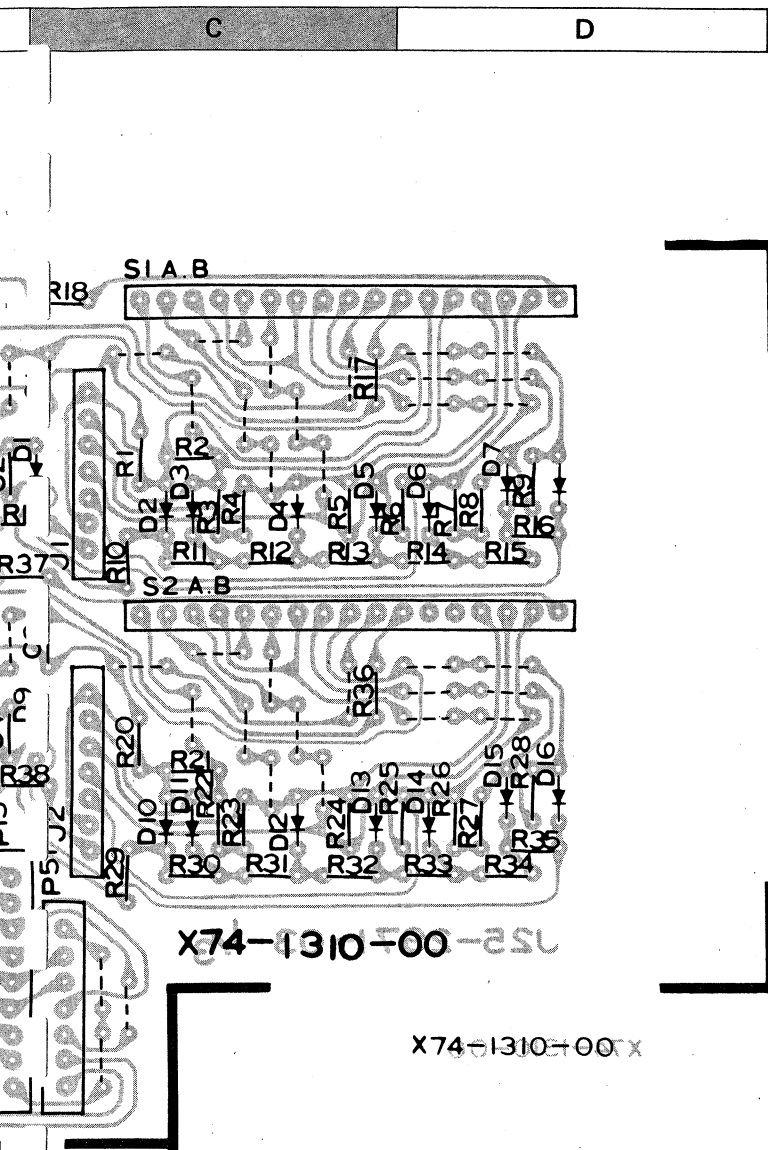

CAUTION
Because the silk symbols in P42 and P57 are reversed,
please refer to the Schematic Diagram.



SCHEMATIC DIAGRAM

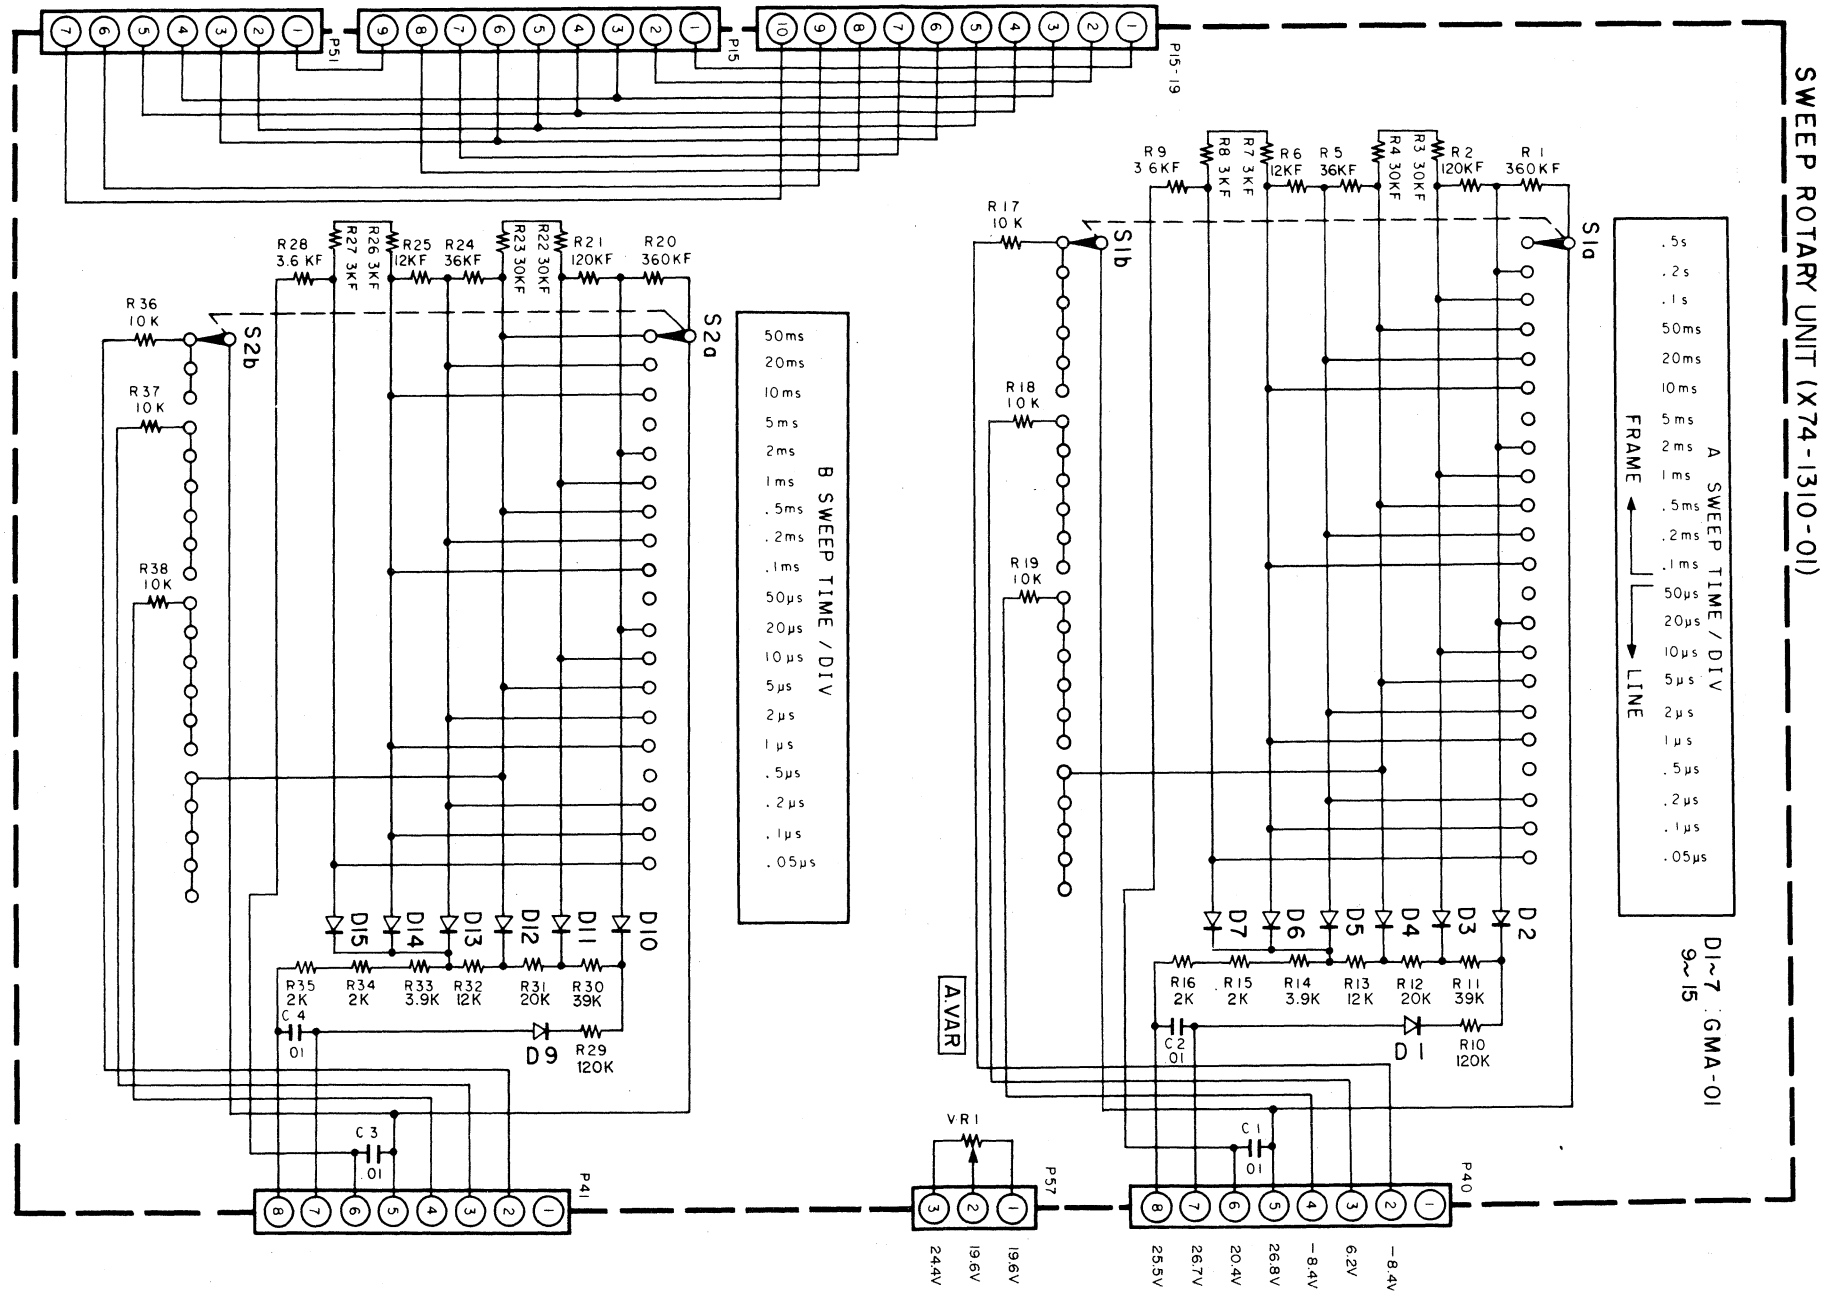



PC BOARD

X74-1320-01


X74-

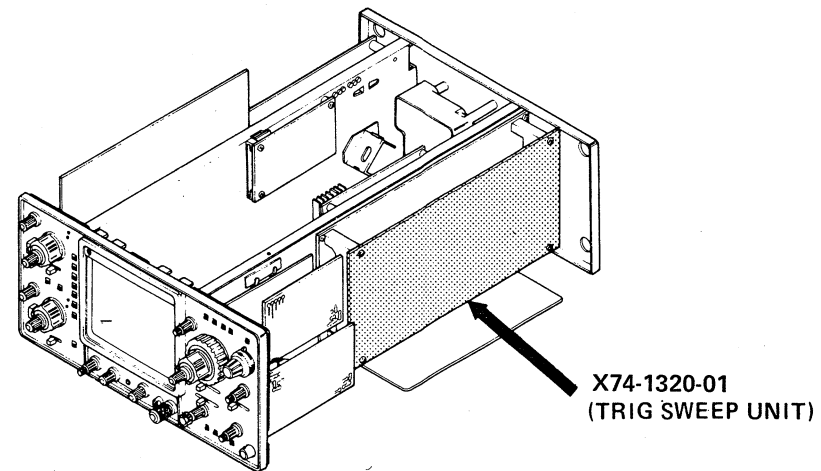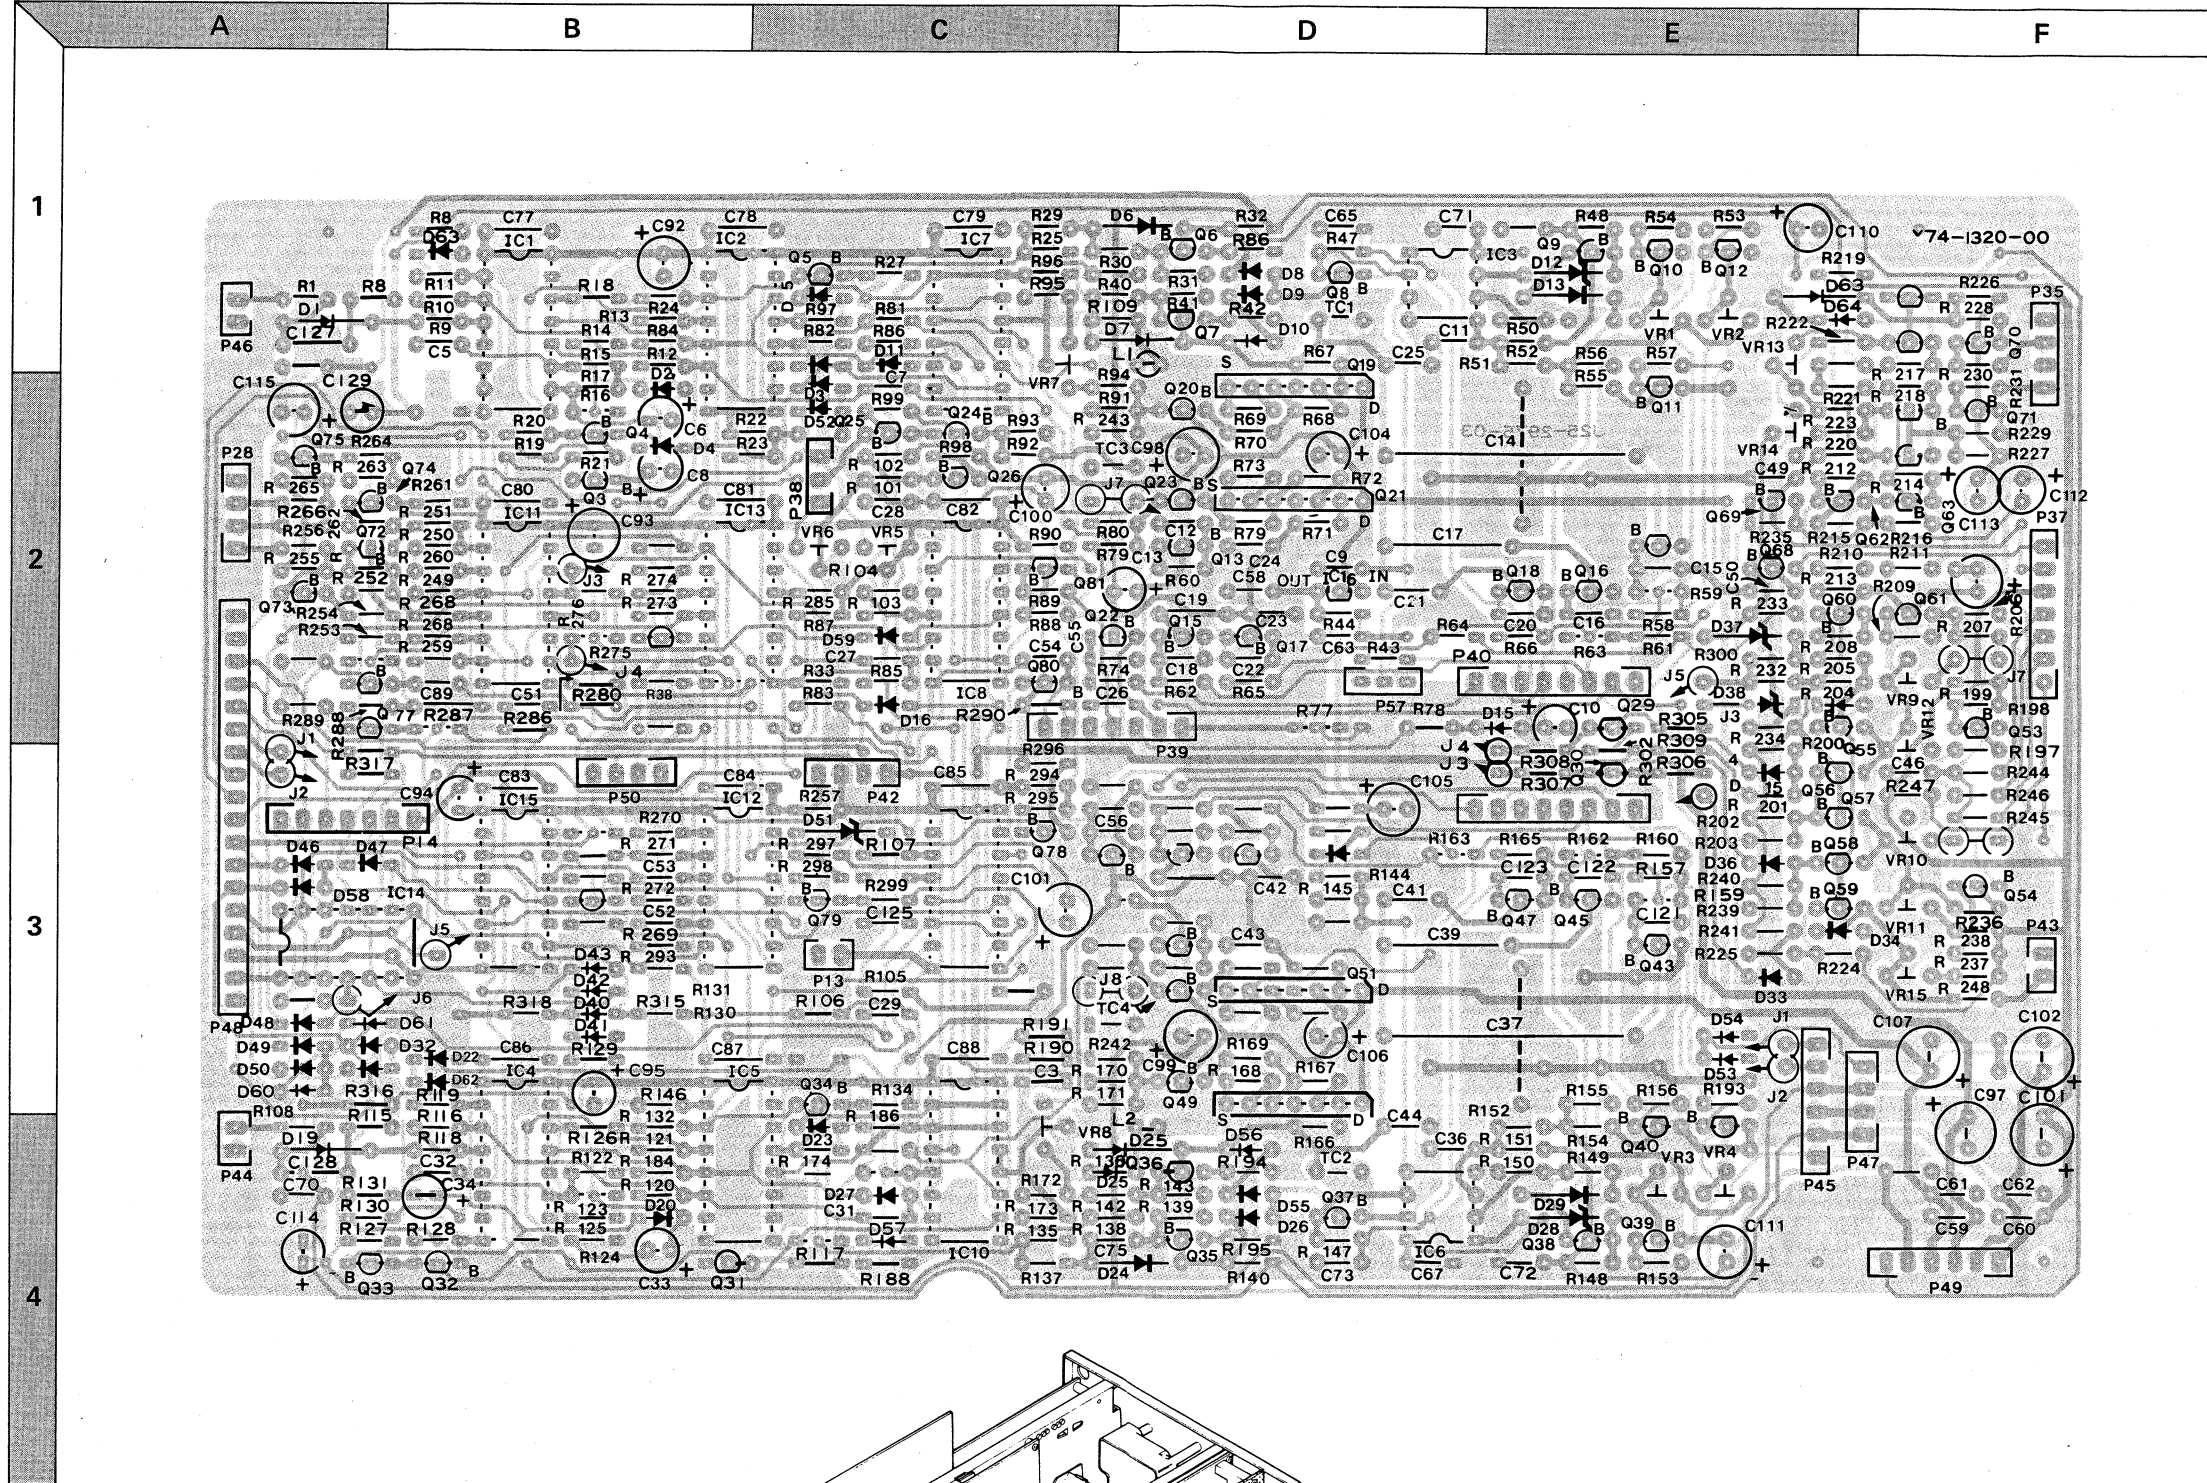

D E F

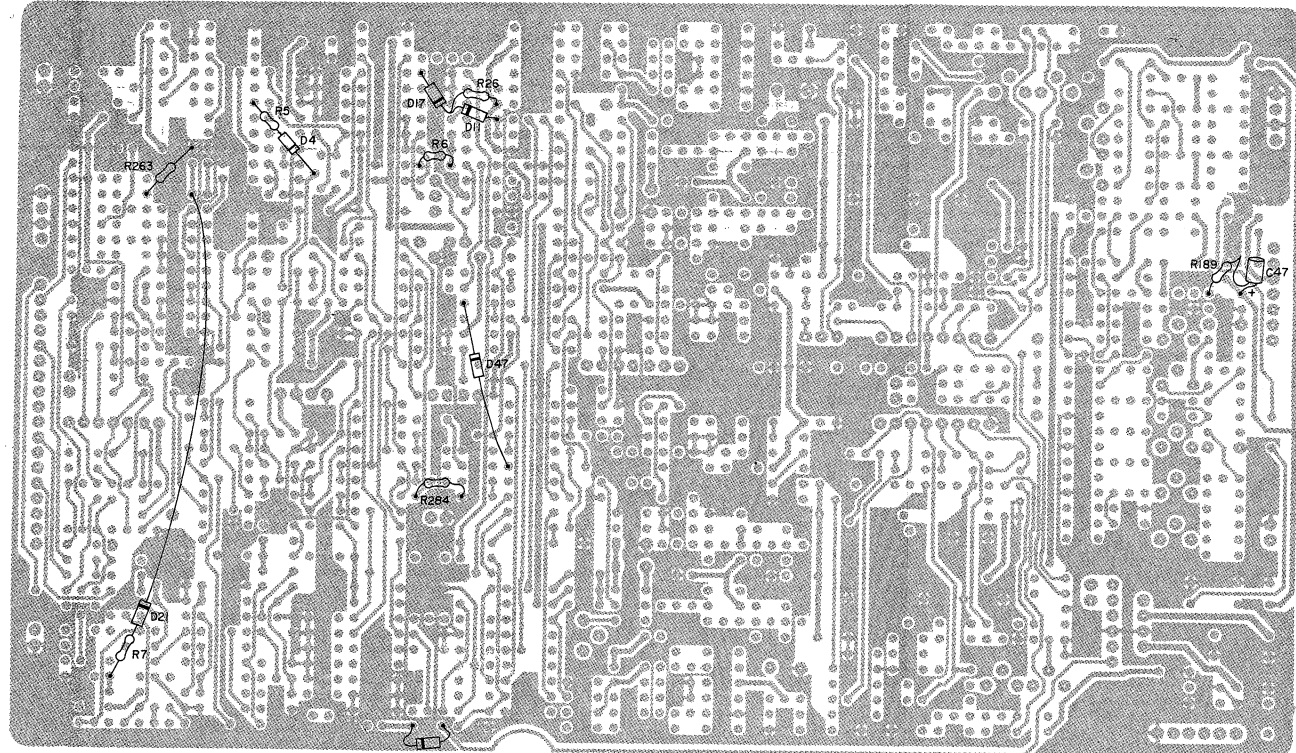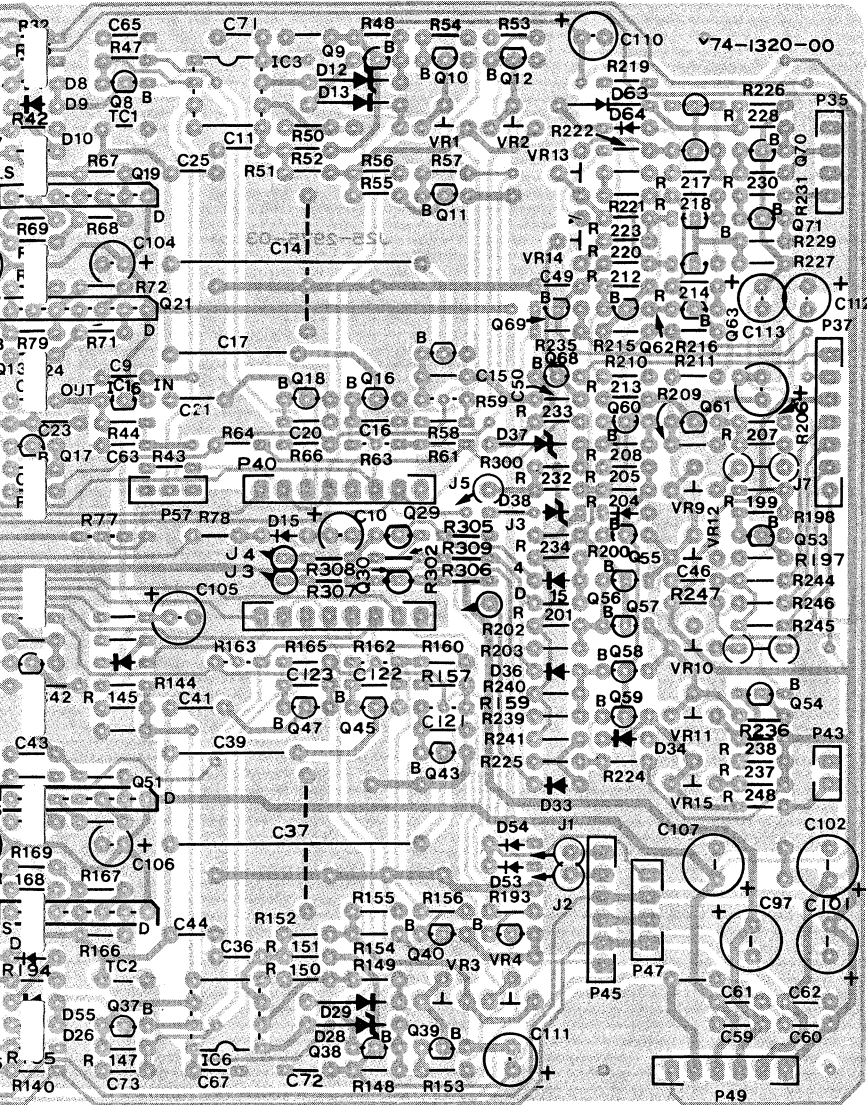



(Parts Side View)

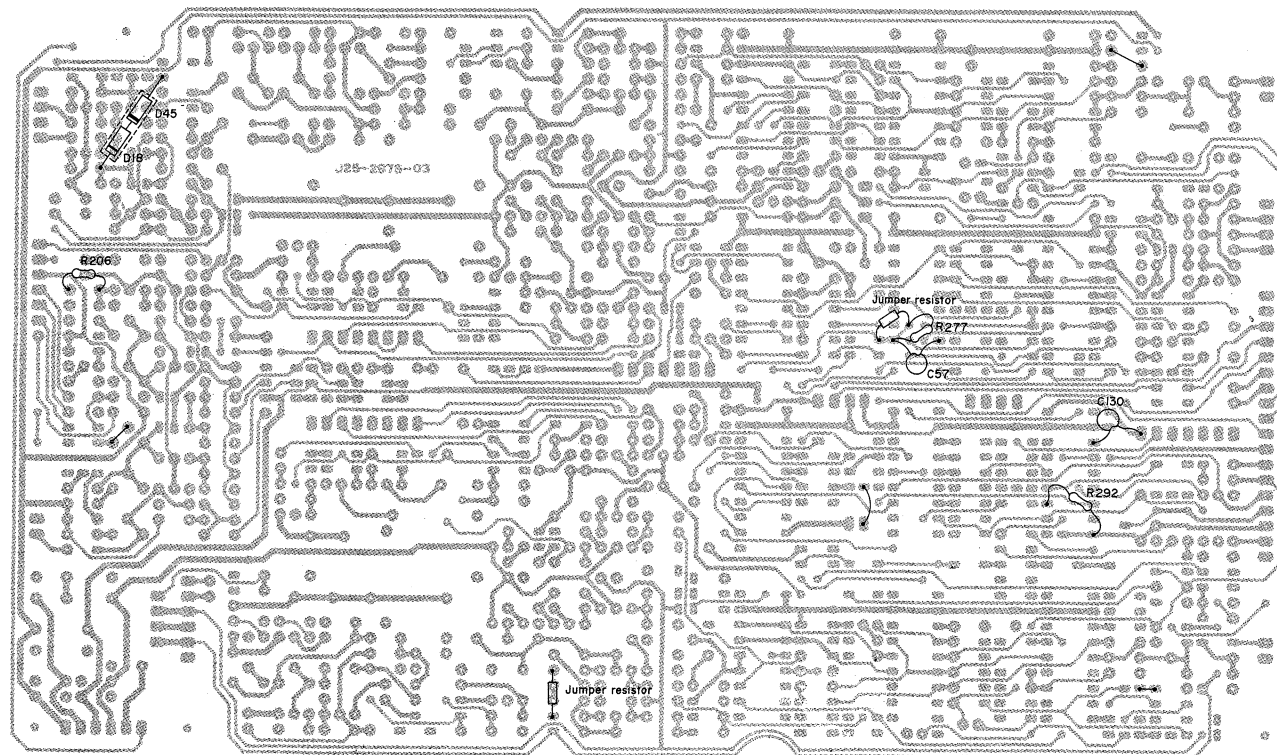

(Foil Side View)


WAVEFORMS

SCHEMATIC DIA

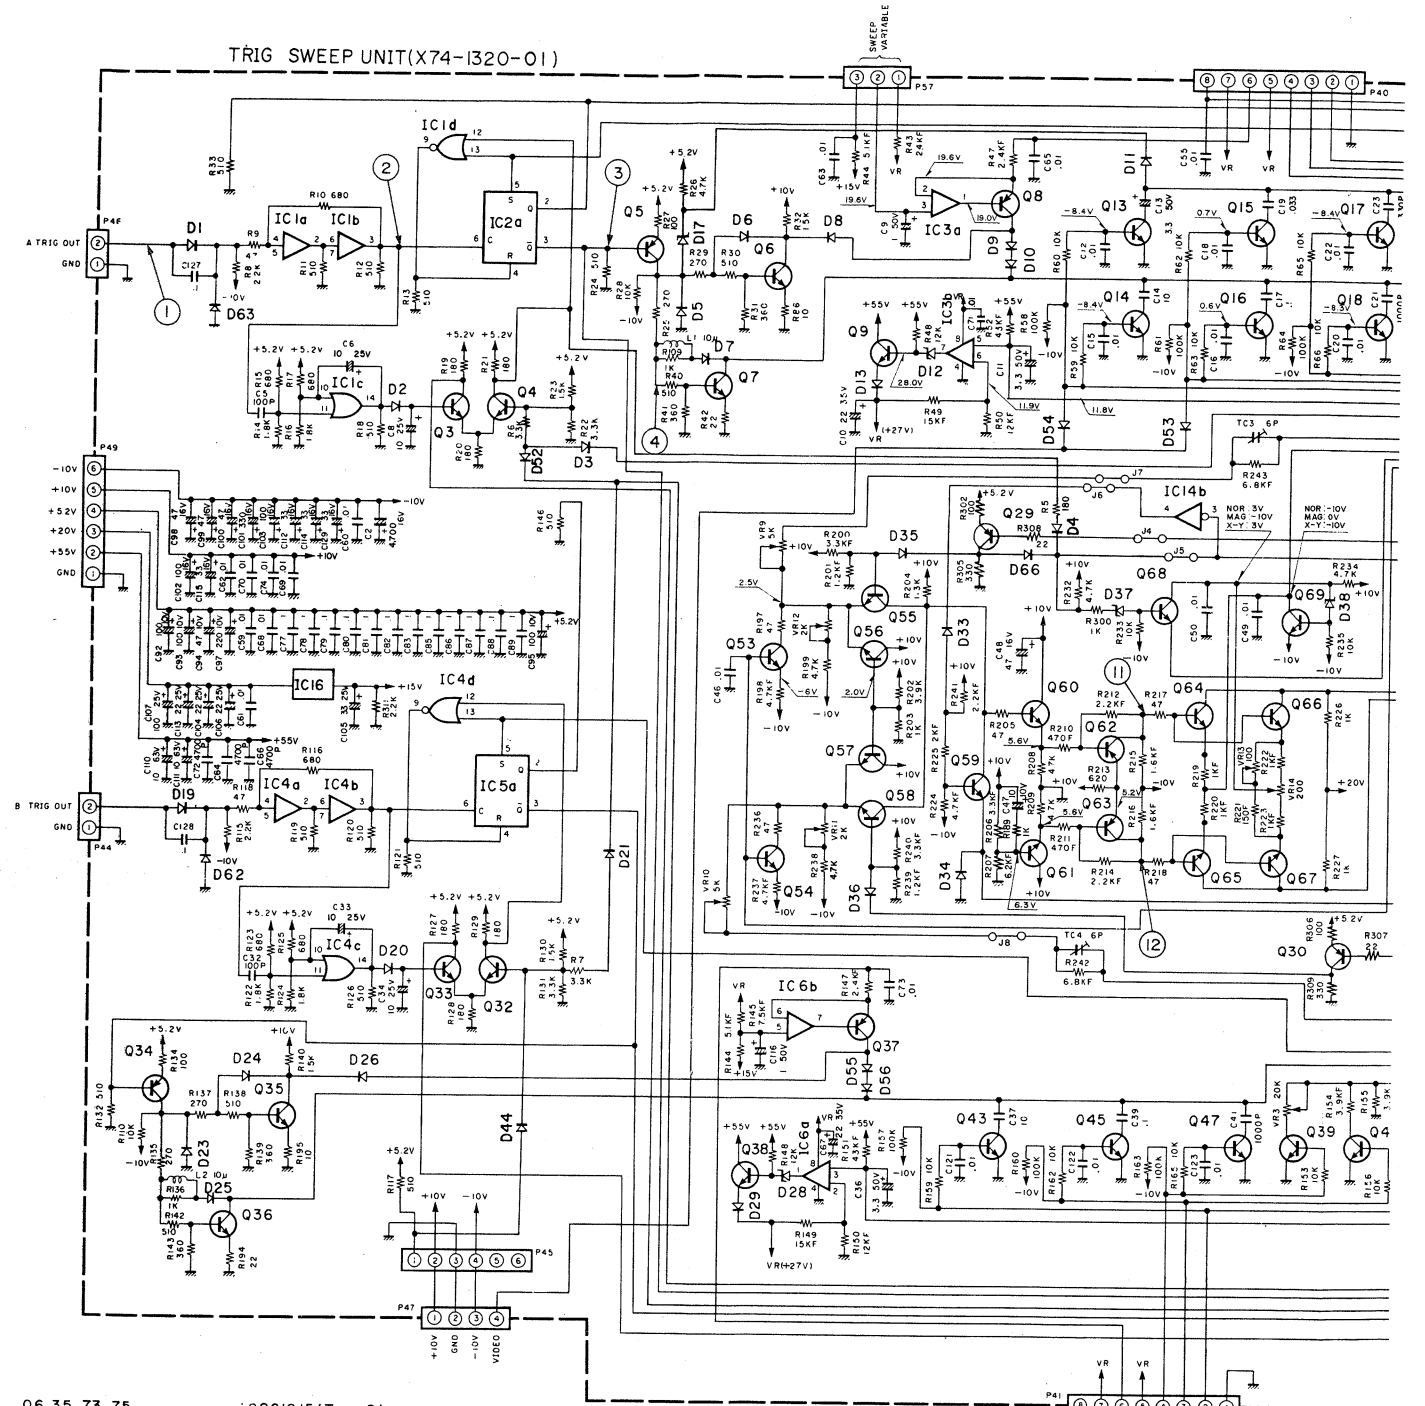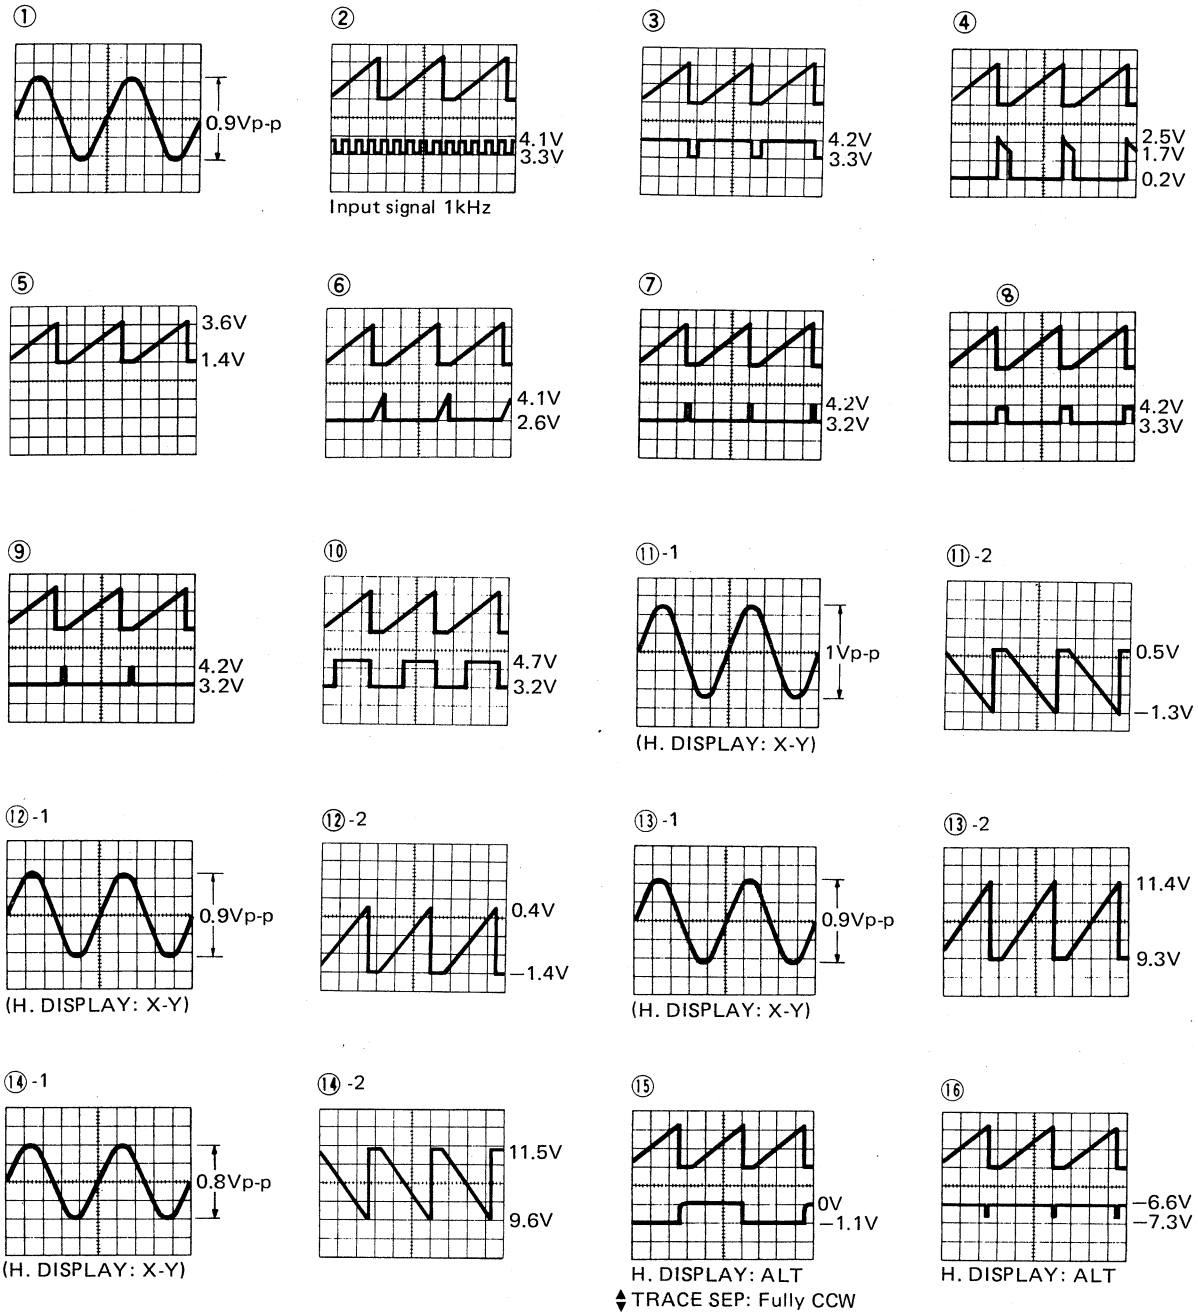

Q6,35,73,75	:2SC1215(T or S)	IC1,4,8	:MC10103L	D17	:YZ-030
Q5,8,22, 29,30,34,37,62,63,72,74,77,78,80	:2SAB38(C)	IC2,5,13	:MC10131L	D1,19	:SV03Y
Q3,4,10~18,24~26,32,33,39~41,43,45,47,53,54	:2SC536KNP(F)	IC3,6	:TL082CP	D2 ~ 5, 8~11,15,16,18,20,21,23,26,32~36,40~43,22	:GMA-01
Q7,36	:2SC1973(T)	IC7,10,11,15	:MC10104L	46,48~50,52~58,60~64,66	:DS-442X
Q9,38	:2SD438(F)	IC12	:MC10102L	D6,7,13,24,25,29,44,47,59	:WZ-150
Q19,21,48,51	:M47F(C)	IC14	:SN7405N	D12,28	:WZ-120
Q20,23,49,55~61,64~67,70,71	:2SC1047(C)	IC16	:MC78L15CP	D37,38	:WZ-100
				D51	:WZ-100
				D65,45	:SV06Y


SCHEMATIC DIAGRAM

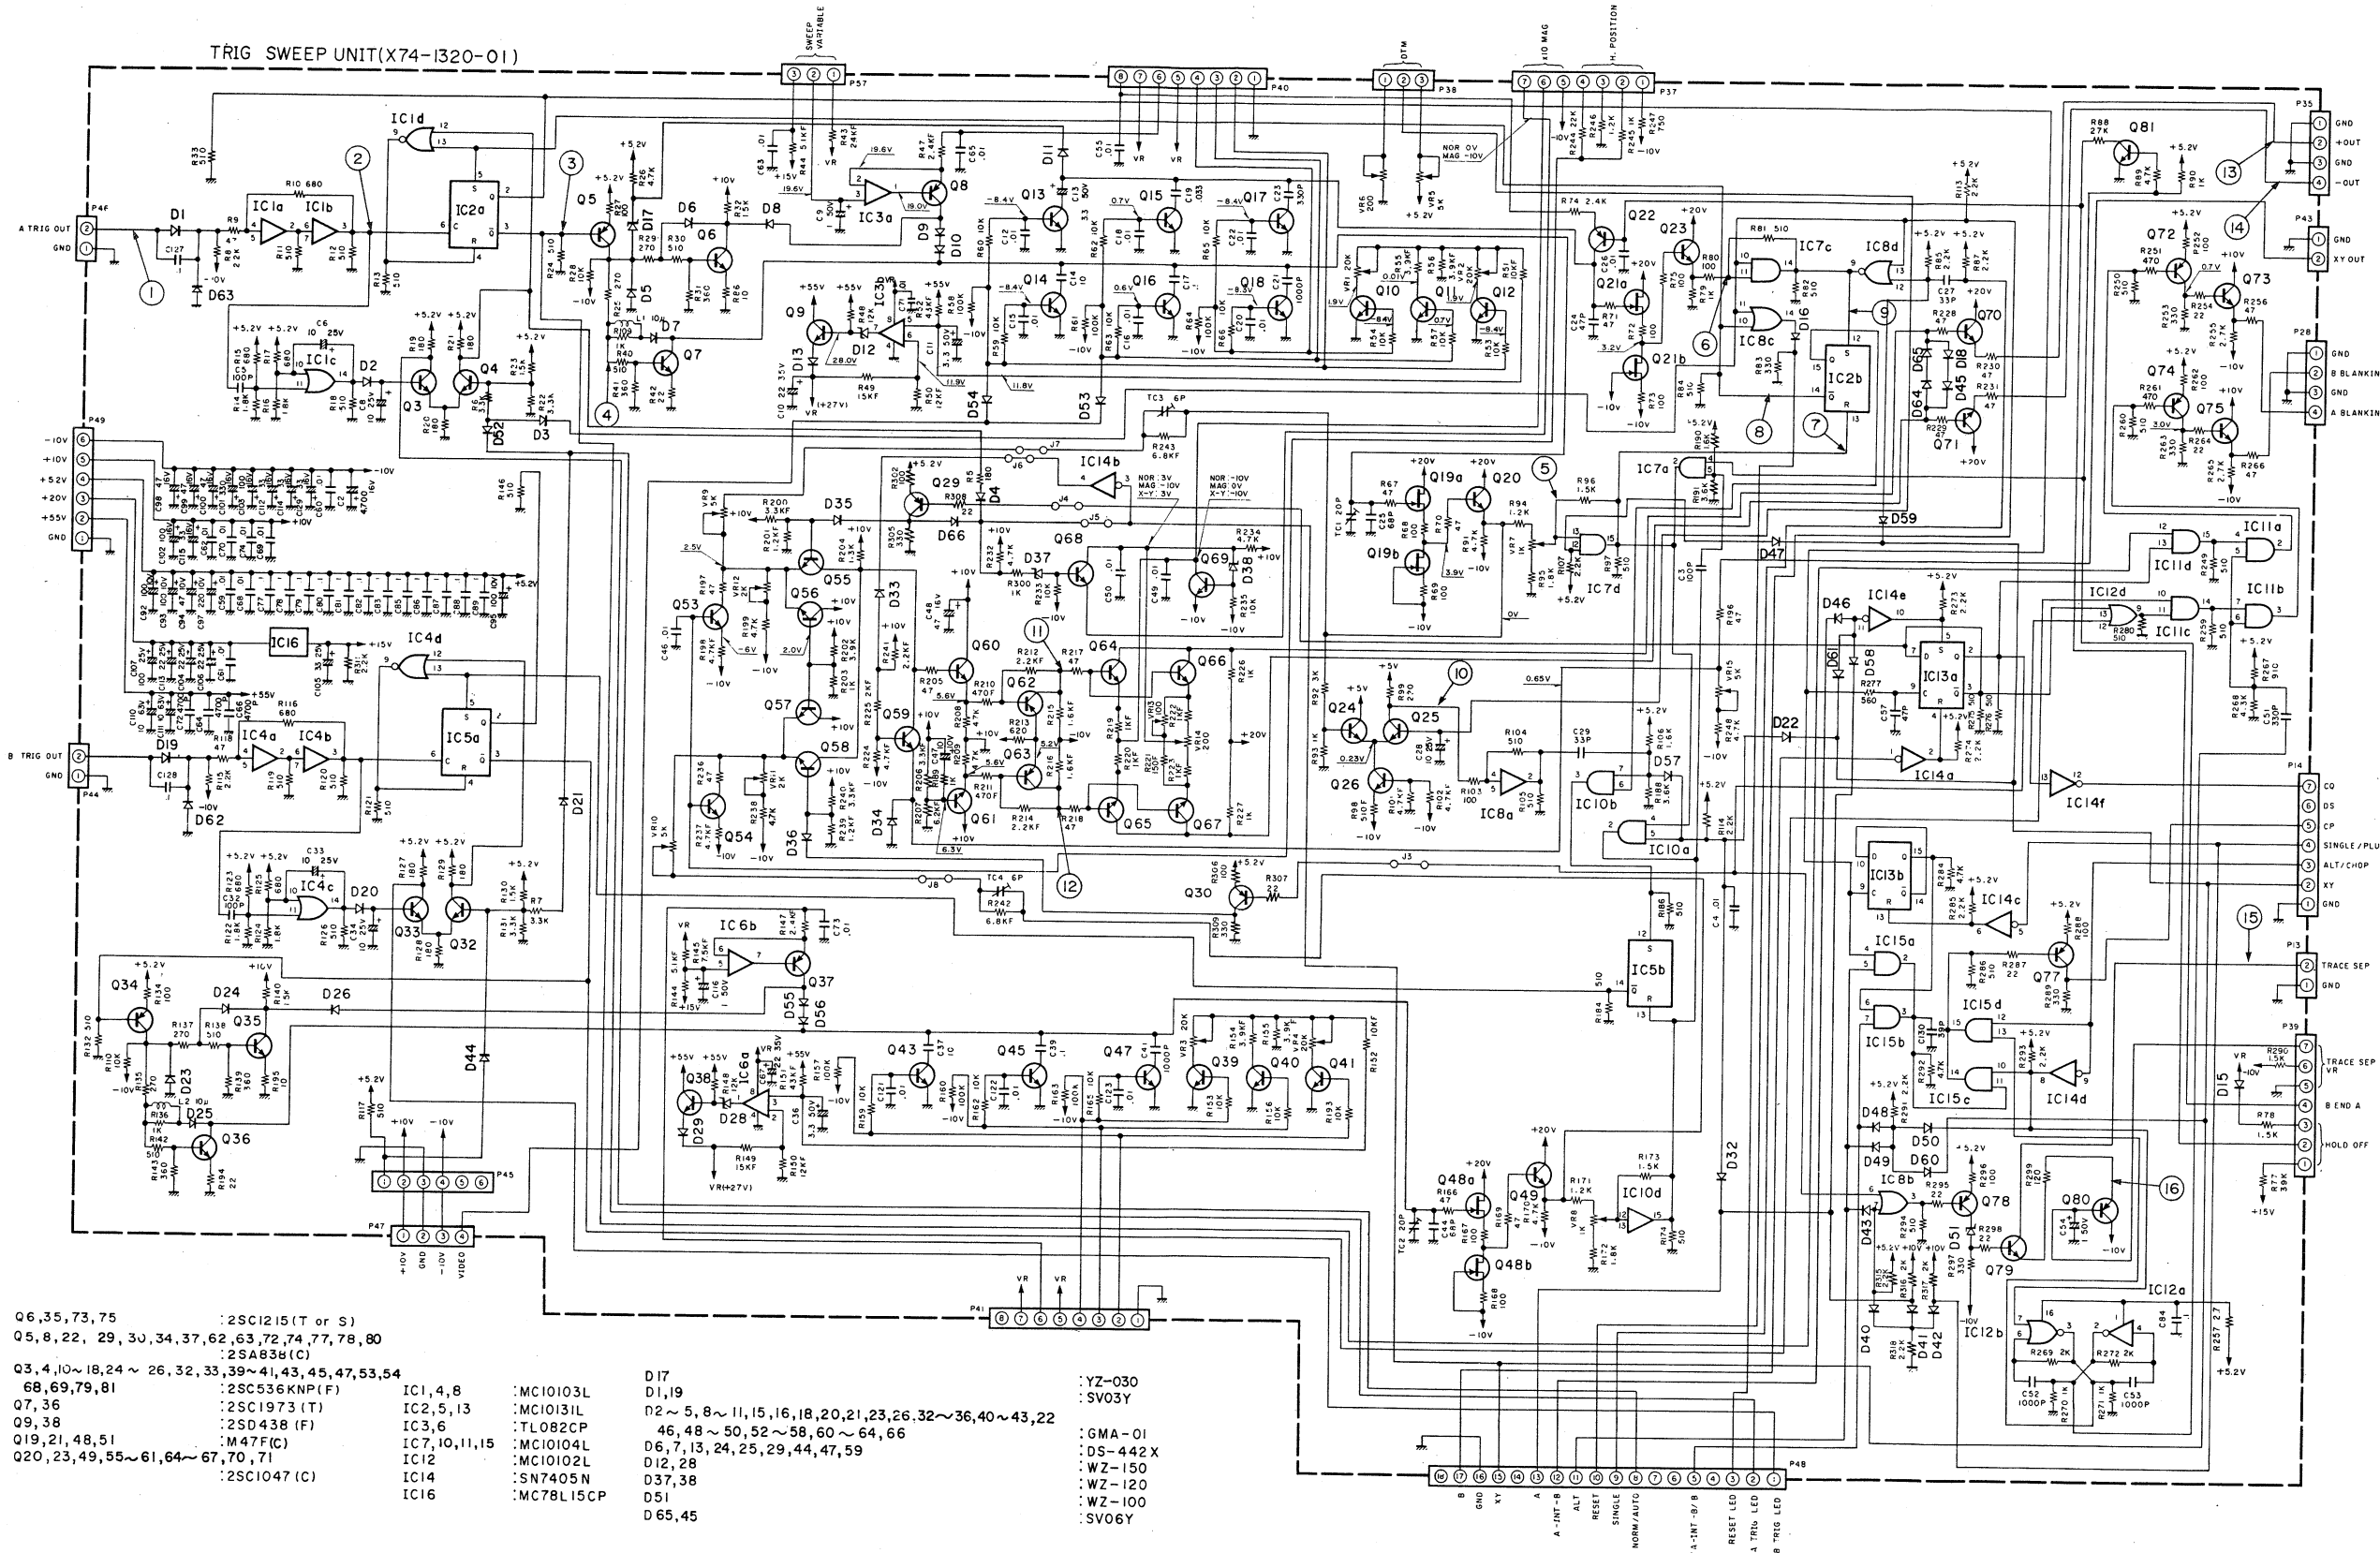




- | | | | | | |
|---|------------------|--------------|------------|---|----------|
| Q6,35,73,75 | :2SC1215(T or S) | IC1,4,8 | :MC10103L | D17 | :YZ-030 |
| Q5,8,22,29,30,34,37,62,63,72,74,77,78,80 | :2SA83B(C) | IC2,5,13 | :MC10131L | D1,19 | :SV03Y |
| Q3,4,10~18,24~26,32,33,39~41,43,45,47,53,54 | :2SC536KNP(F) | IC3,6 | :TL082CP | D2~5,8~11,15,16,18,20,21,23,26,32~36,40~43,22 | :GMA-01 |
| Q7,36 | :2SC1973(T) | IC7,10,11,15 | :MC10104L | 46,48~50,52~58,60~64,66 | :DS-442X |
| Q9,38 | :2SD438(F) | IC12 | :MC10102L | D6,7,13,24,25,29,44,47,59 | :WZ-150 |
| Q19,21,48,51 | :M47F(C) | IC14 | :SN7405N | D37,38 | :WZ-120 |
| Q20,23,49,55~61,64~67,70,71 | :2SC1047(C) | IC16 | :MC78L15CP | D51 | :WZ-100 |
| | | | | D65,45 | :SV06Y |

PC BOARD








X74-1230-01

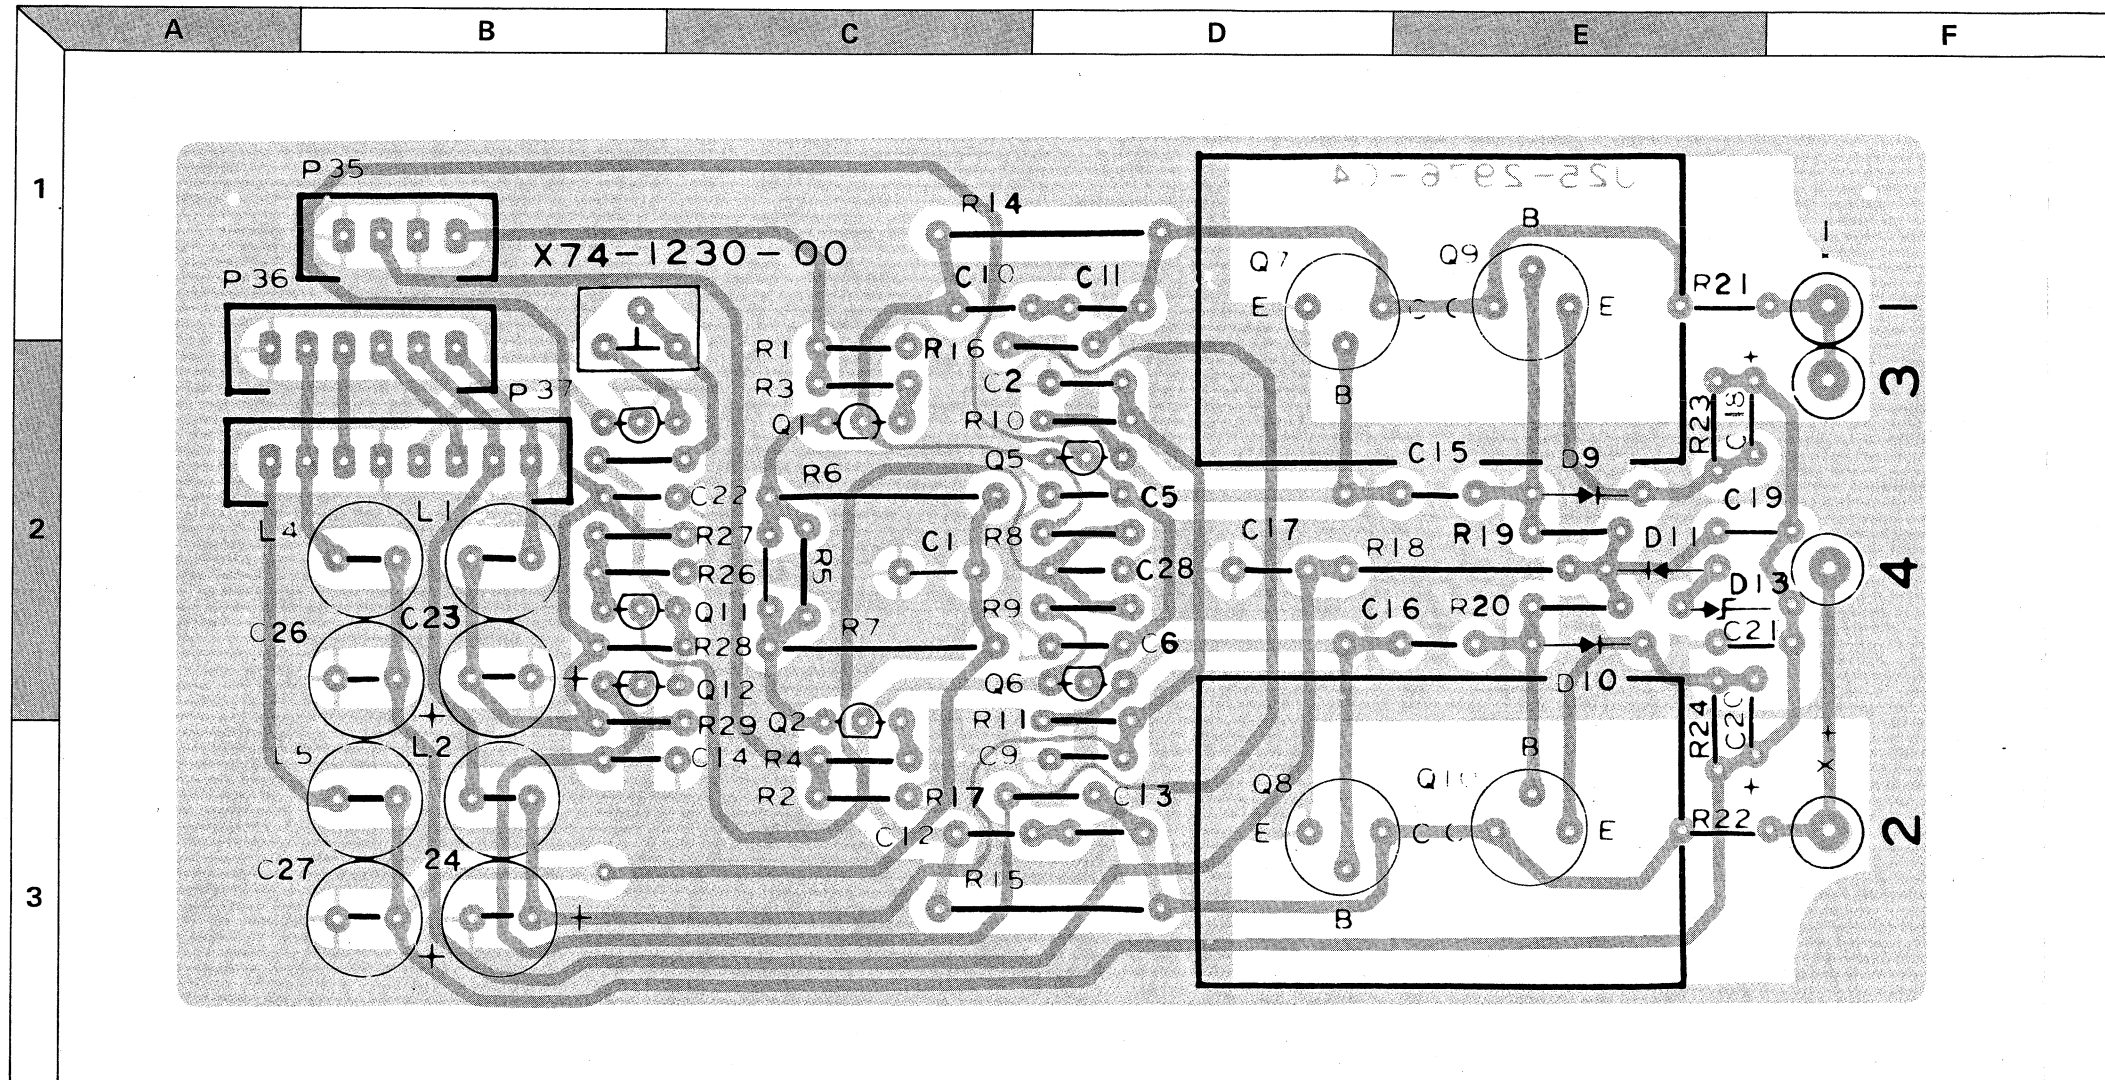


BOARD

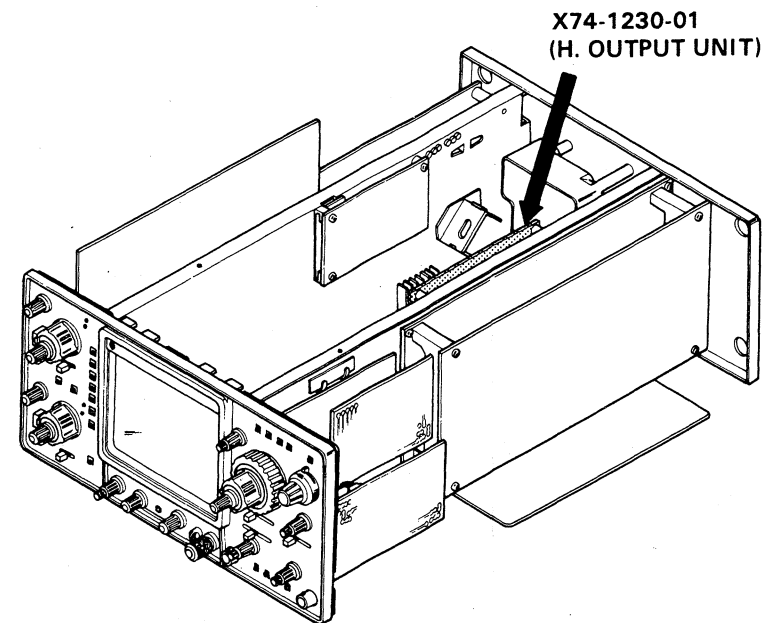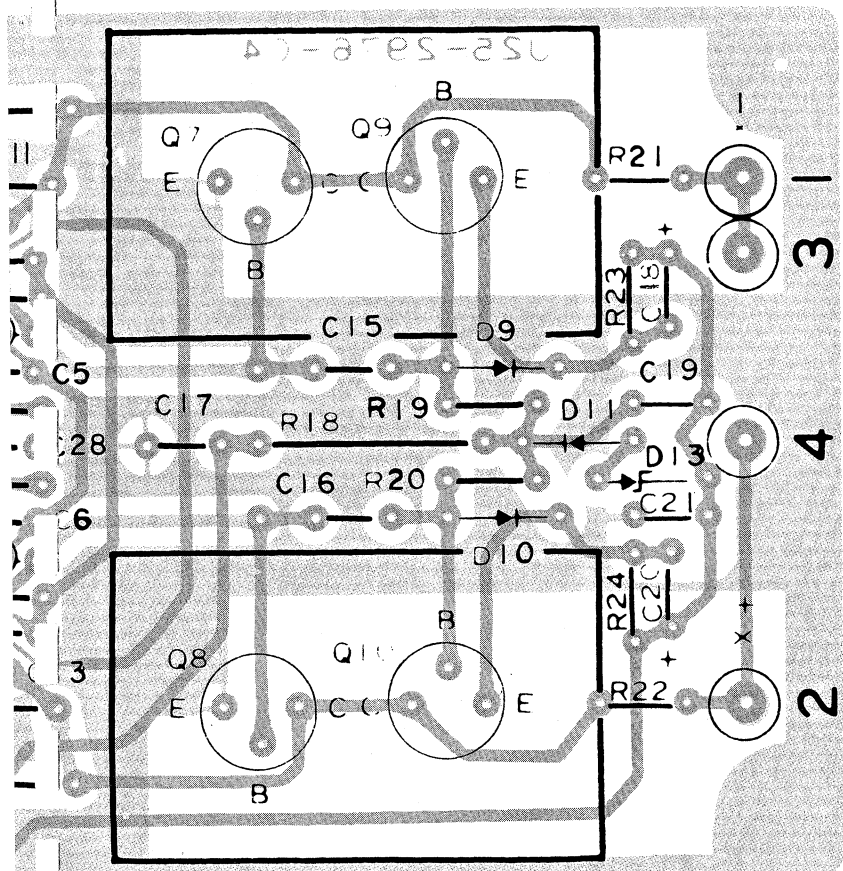

WAVEFORMS

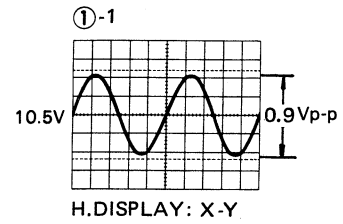


SCHEMATIC DIA

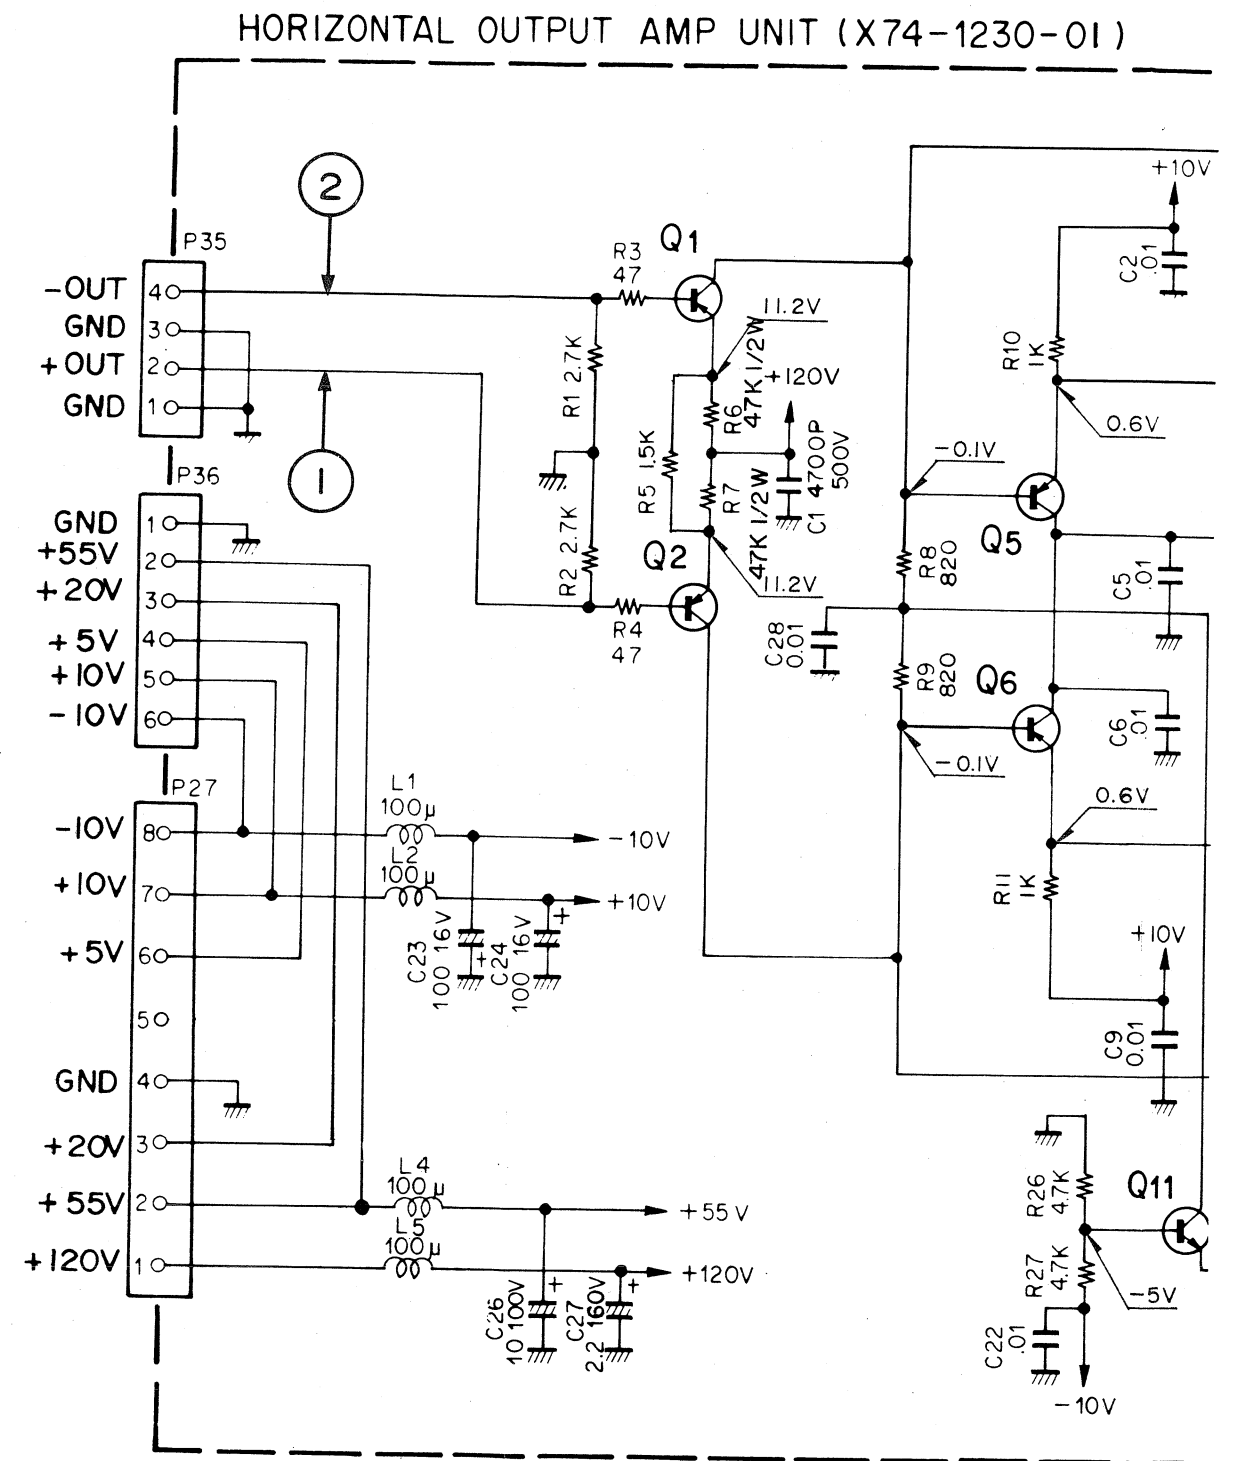

SCHEMATIC DIAGRAM


HORIZONTAL OUTPUT AMP UNIT (X74-1230-01)

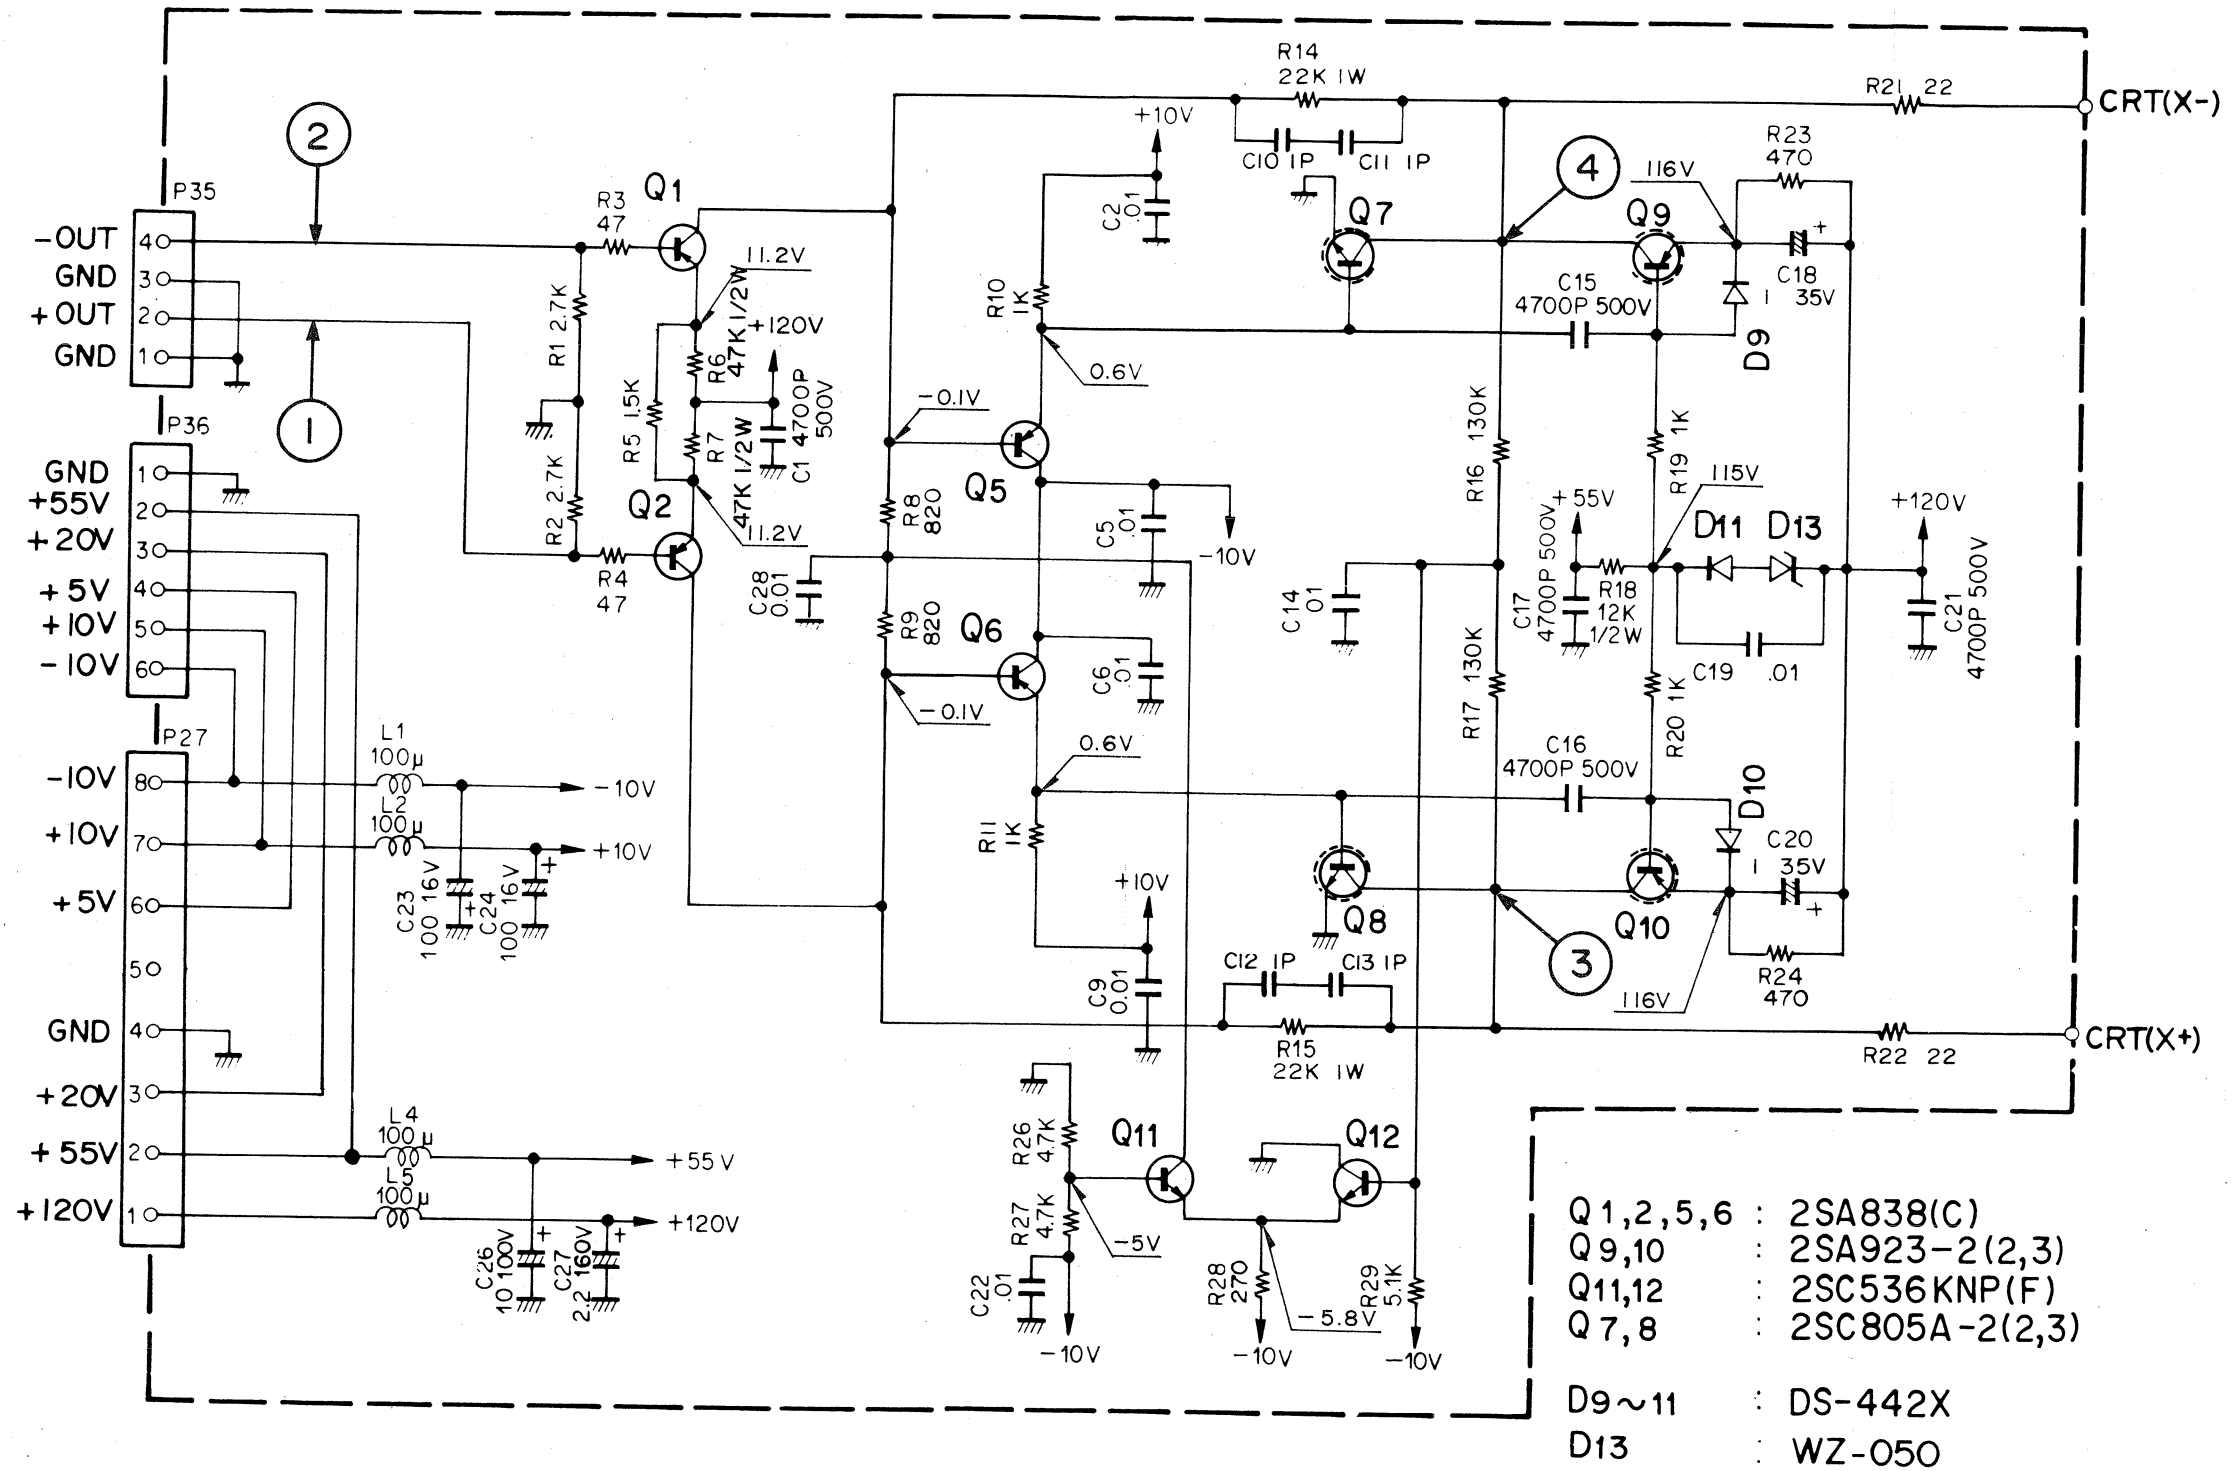

PC BOARD



X77-1130-01

X77-113

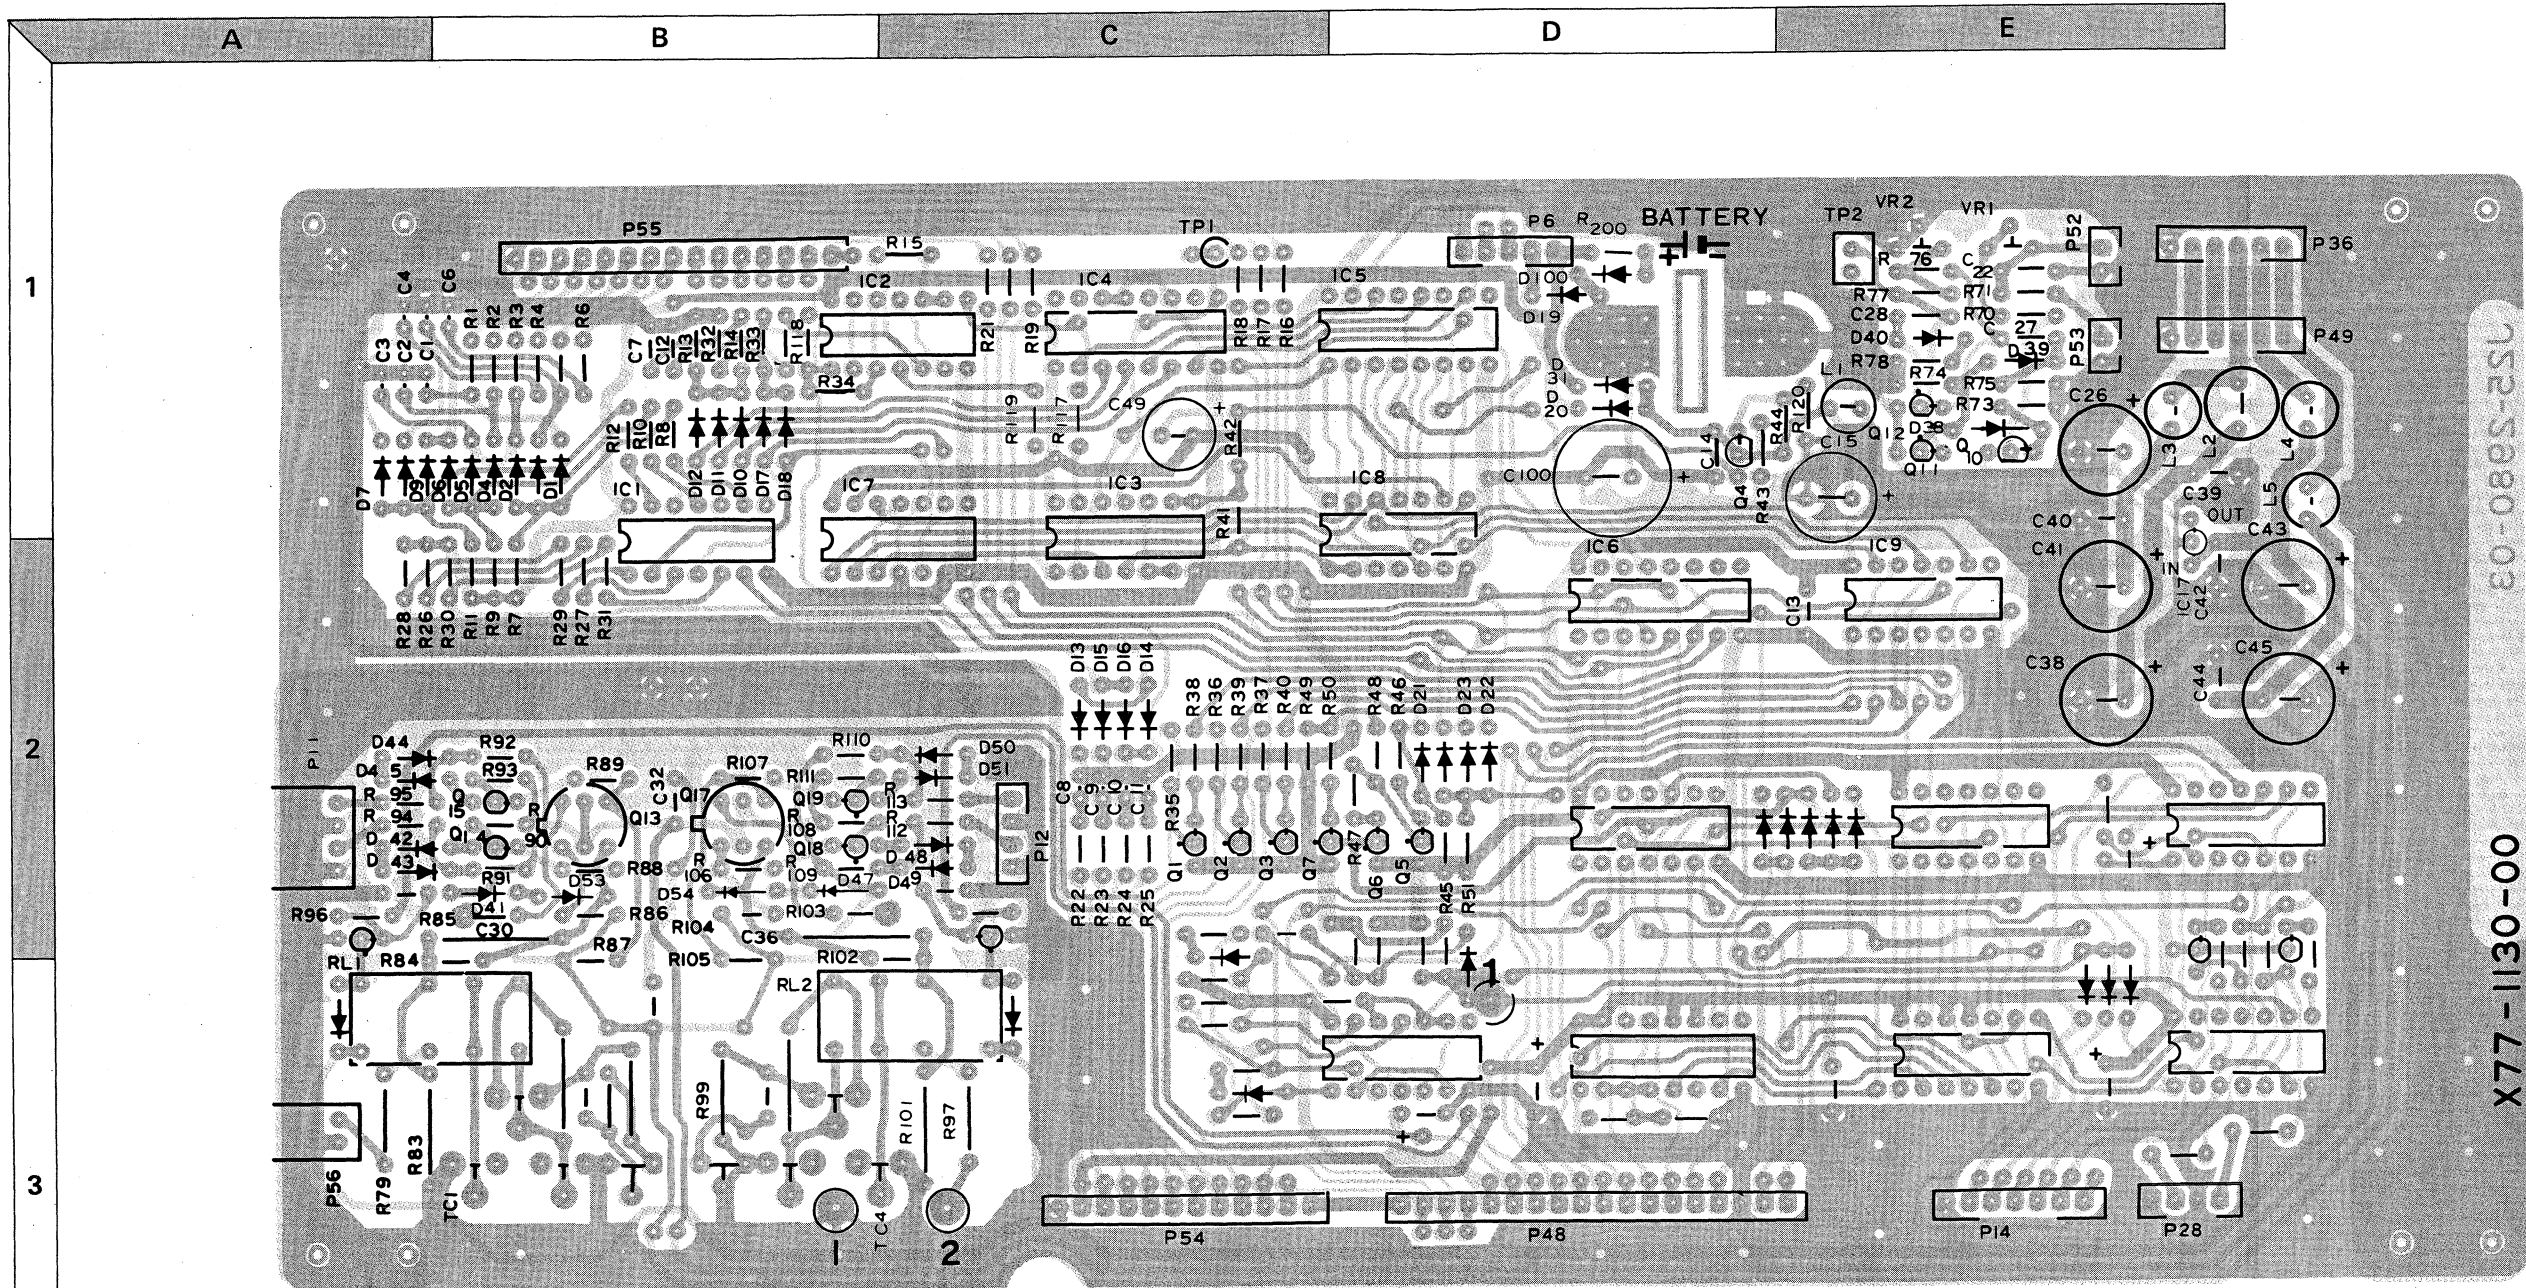


ARD




X77-1130-01

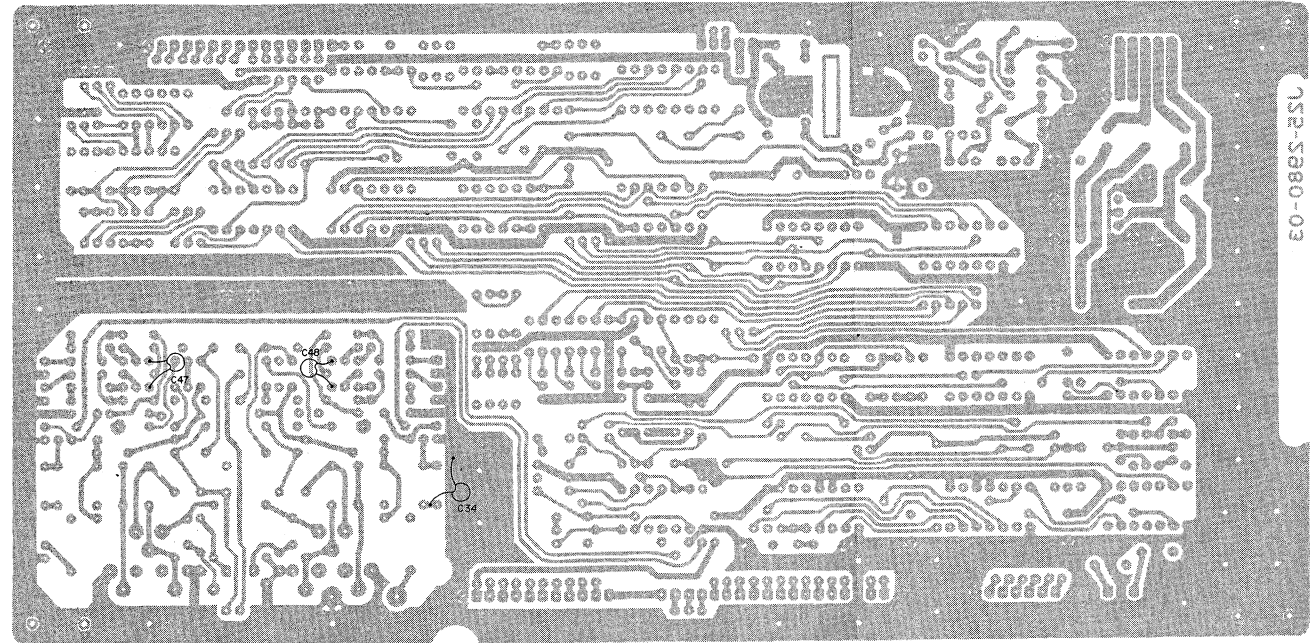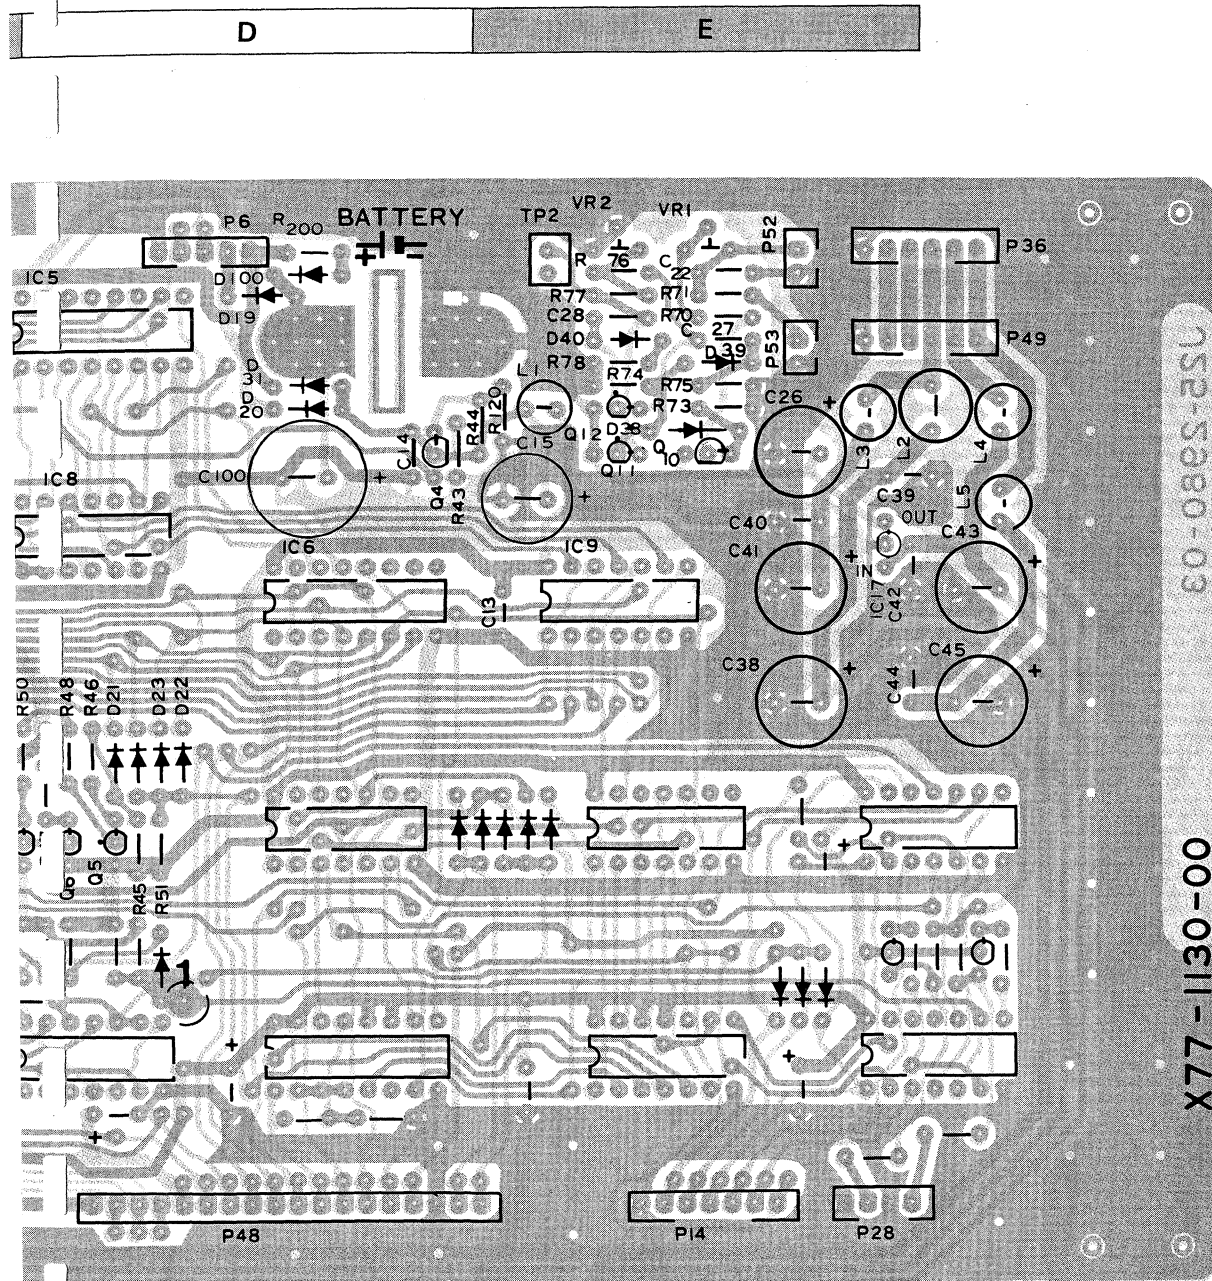

(Foil Side View)

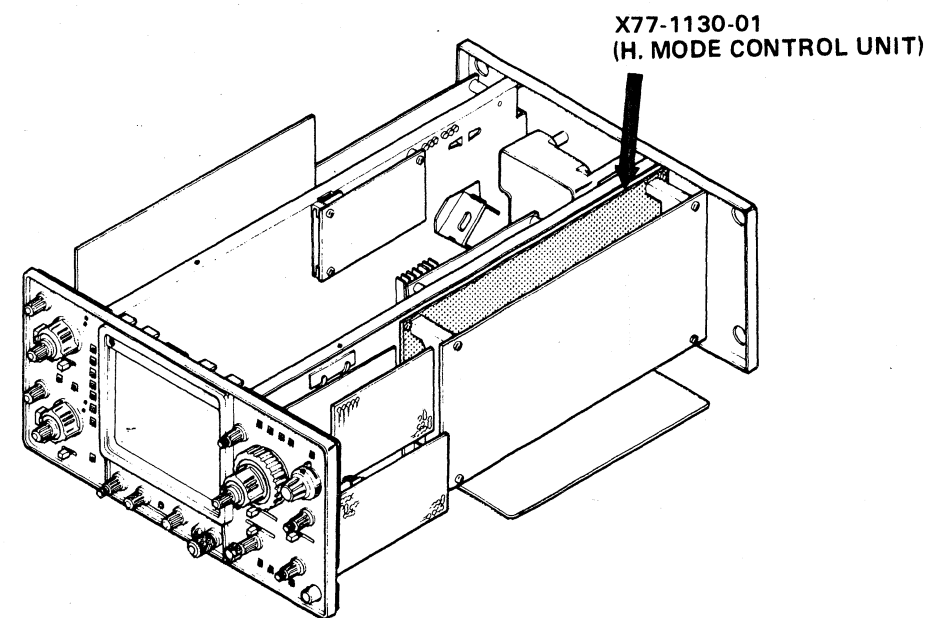


WAVEFORMS

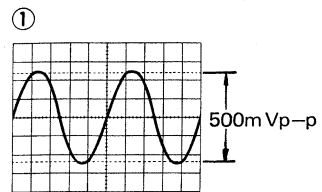

SCHEMATIC DIA

HORIZONTAL MODE CONTROL UNIT (X77-1130-01)

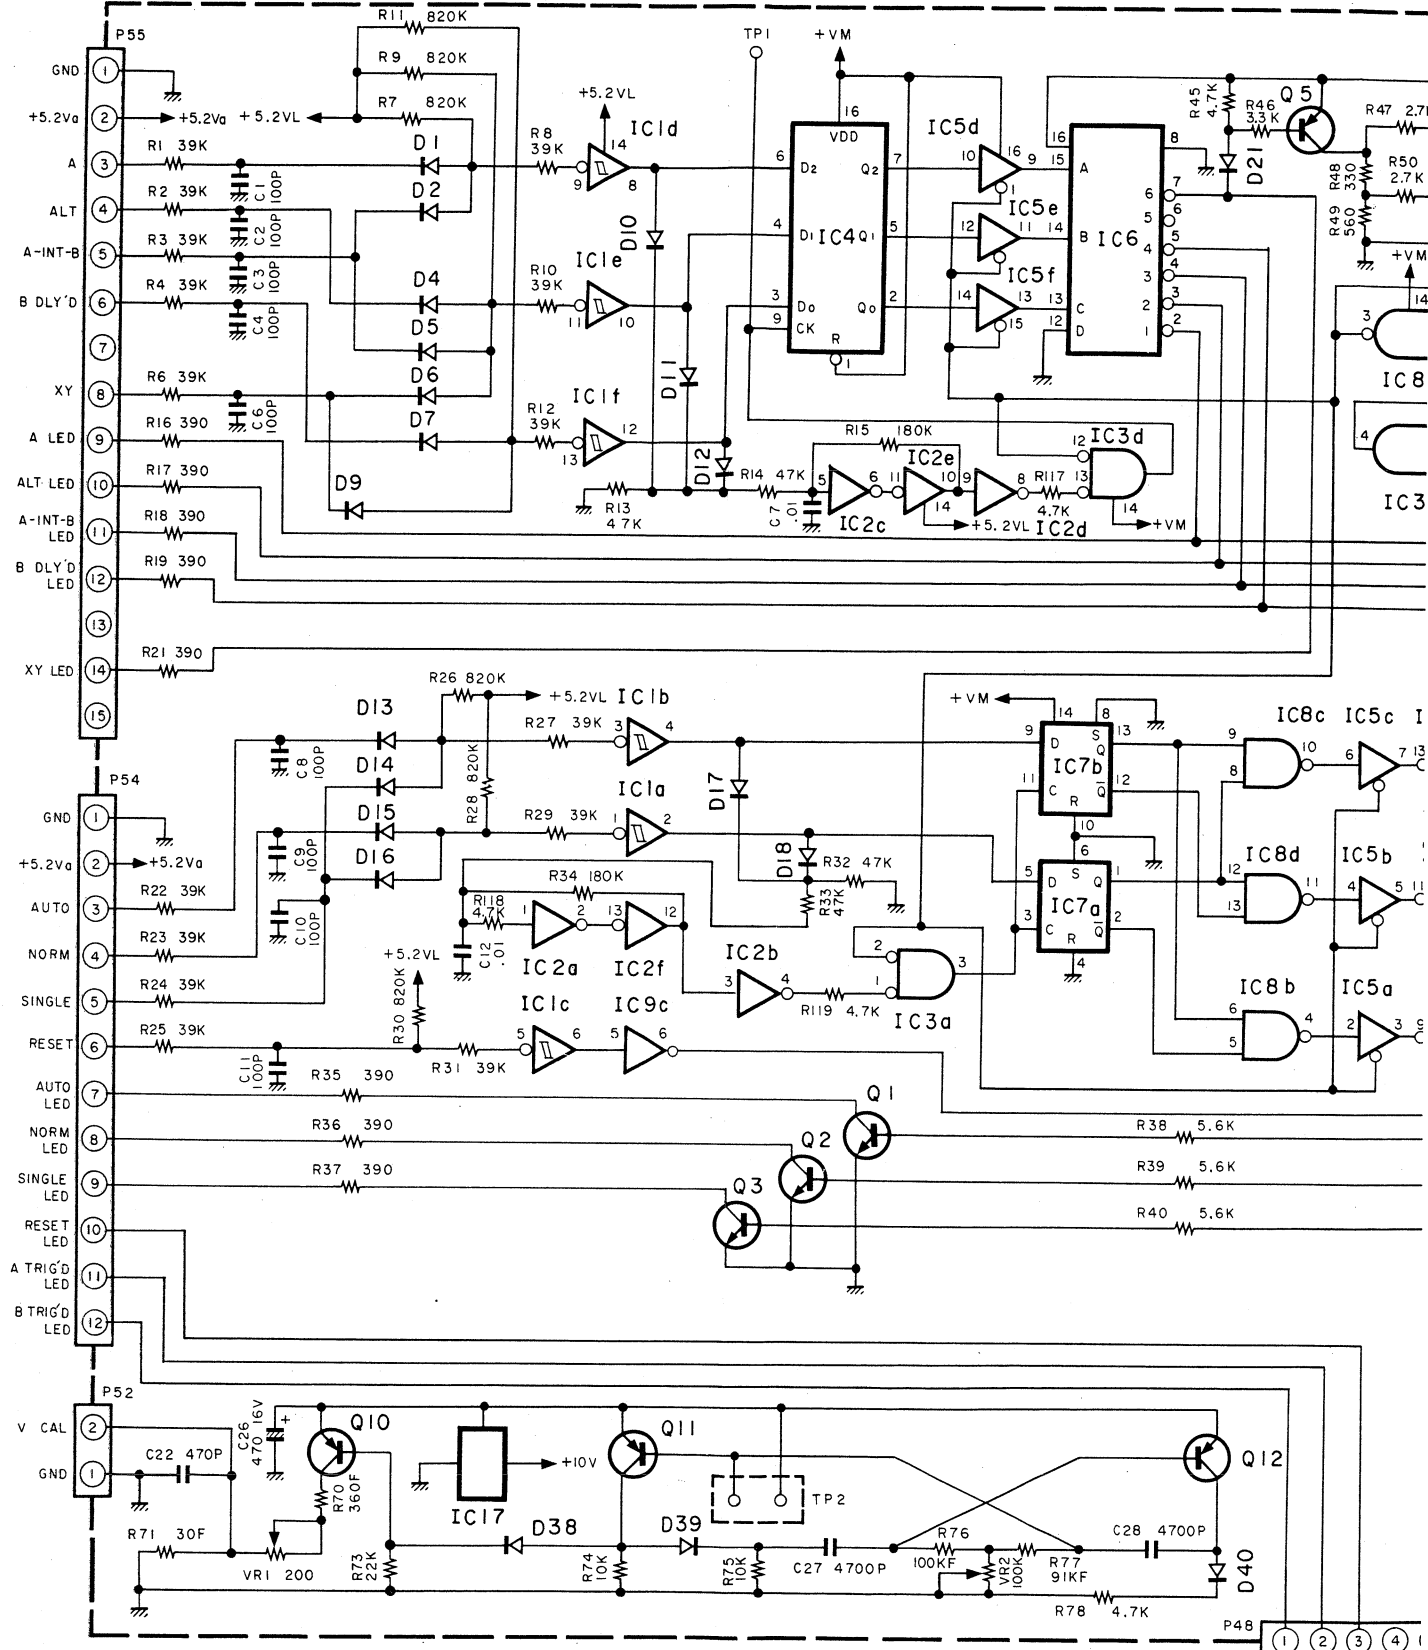


- | | | |
|-------------------|-----------------------------|---------------------------------|
| IC1 : MCI4584BCP | IC6 : SN7442AN | Q1~4,7 : 2SC536KNP(F) |
| IC2 : MCI4069UBCP | IC7 : MCI4013BCP | Q5,6,10~12 : 2SA608KNP(F) |
| IC3 : MCI4001BCP | IC8 : MCI4011BCP | Q13,17 : DNI901 |
| IC4 : MCI4174BCP | IC9 : SN74LS04N | Q14,15,18,19 : 2SC1215 (T or S) |
| IC5 : MCI4503BCP | IC17 : FS7805L or MC78L05CP | |

P48
1 2 3 4
B TRIG LED
A TRIG LED
RESET LED

SCHEMATIC DIAGRAM

HORIZONTAL MODE CONTROL UNIT (X77-1130-01)

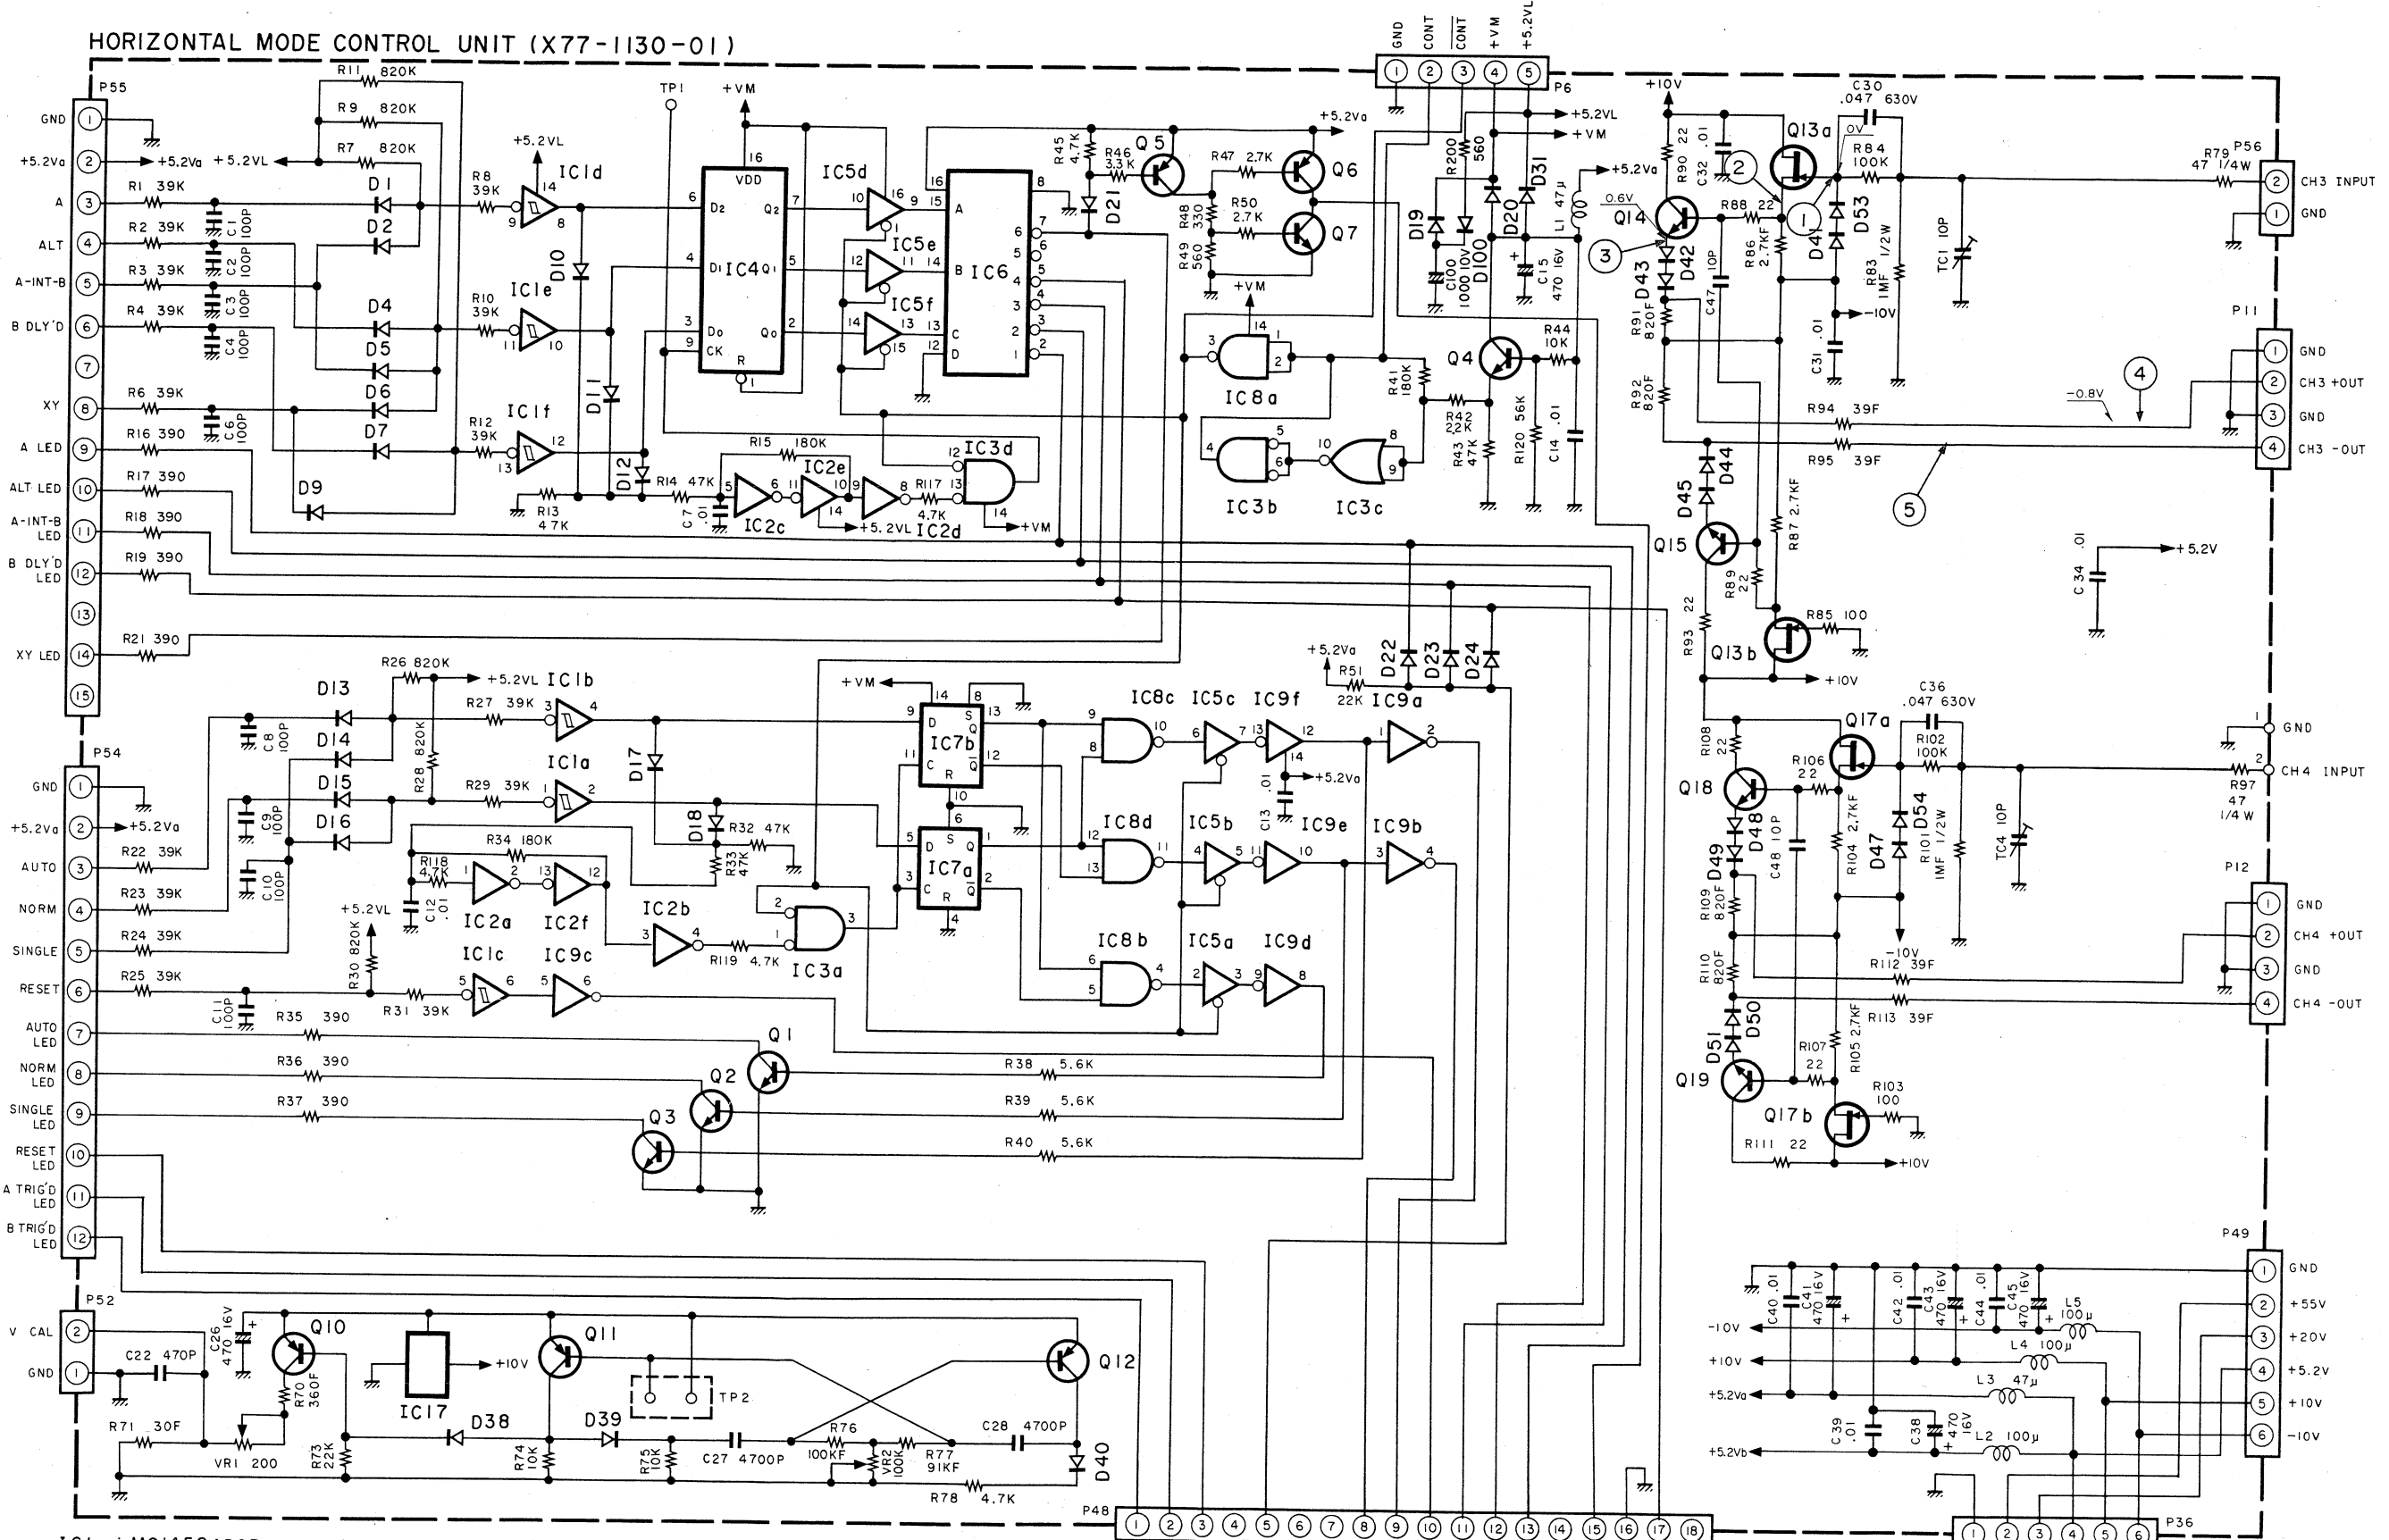


- | | | |
|-------------------|-----------------------------|---------------------------------|
| IC1 : MCI4584BCP | IC6 : SN7442AN | Q1~4,7 : 2SC536KNP(F) |
| IC2 : MCI4069UBCP | IC7 : MCI4013BCP | Q5,6,10~12 : 2SA608KNP(F) |
| IC3 : MCI4001BCP | IC8 : MCI4011BCP | Q13,17 : DNI901 |
| IC4 : MCI4174BCP | IC9 : SN74LS04N | Q14,15,18,19 : 2SC1215 (T or S) |
| IC5 : MCI4503BCP | IC17 : FS7805L or MC78L05CP | |




- D1, 2, 4~7, 9~24, 31, 39, 40, 42~45, 48~51, 53, 54, 100 : DS442 X
 D38 : IN60
 D41, 47 : IS1544A

PC BOARD






X77-1110-01

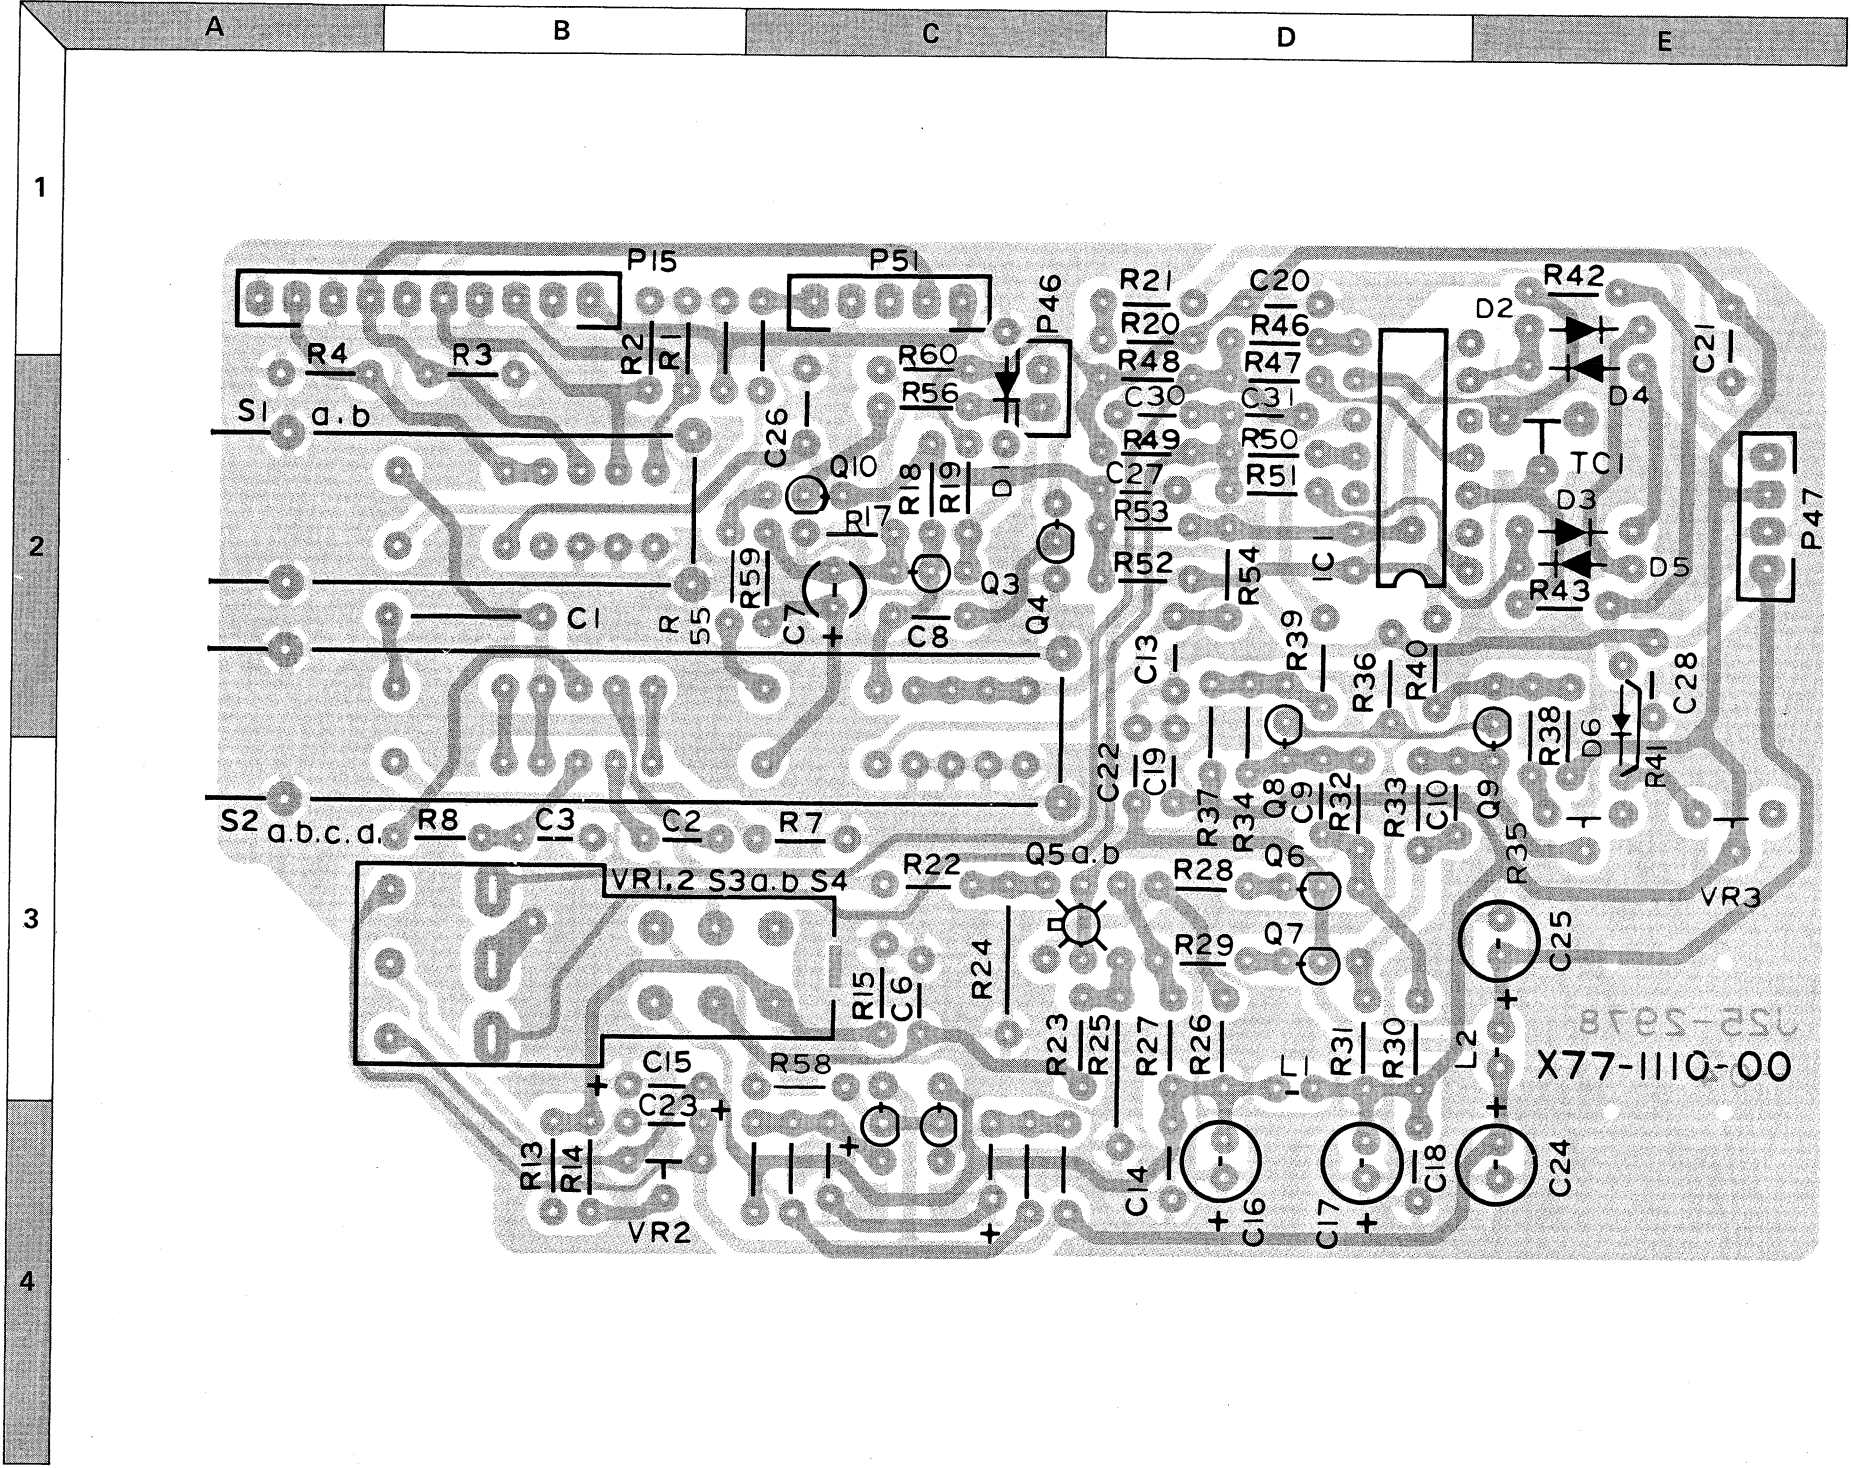


BOARD

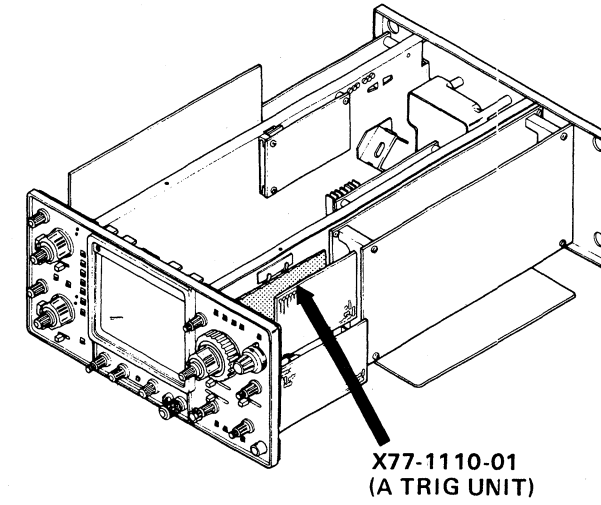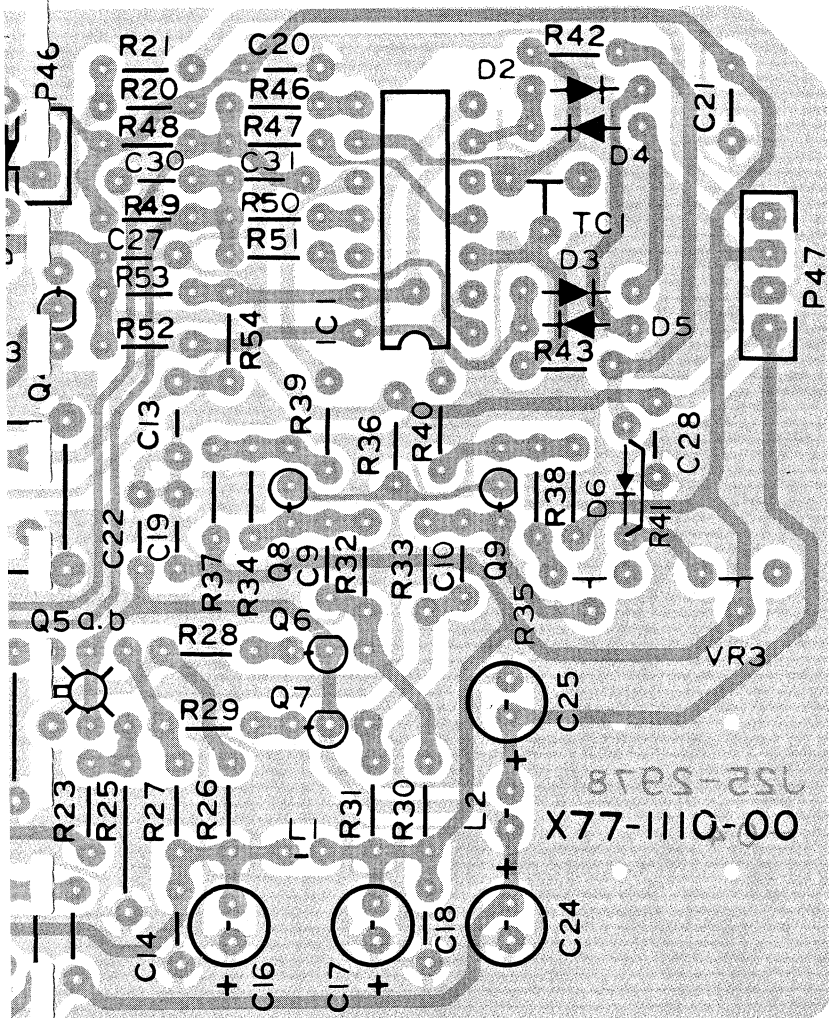

WAVEFORMS

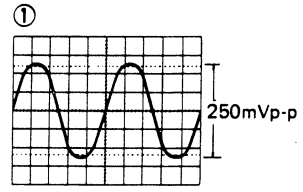


SCHEMATIC

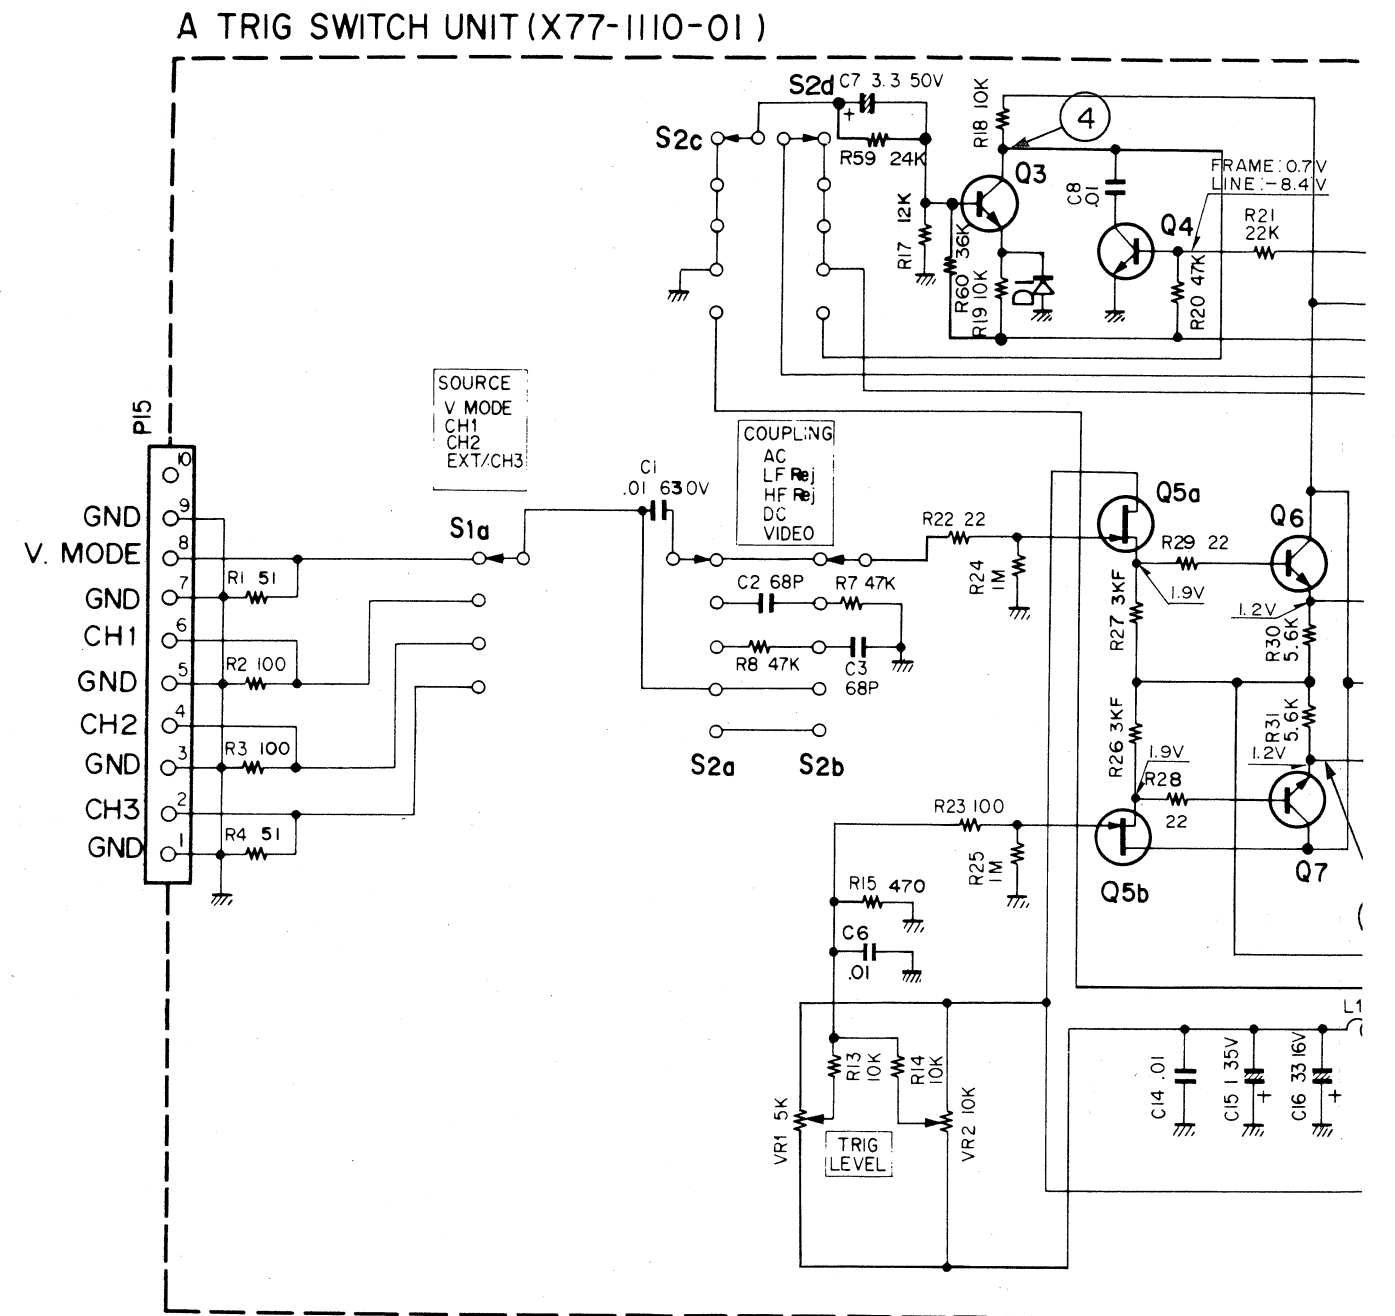

SCHEMATIC DIAGRAM


A TRIG SWITCH UNIT (X77-1110-01)

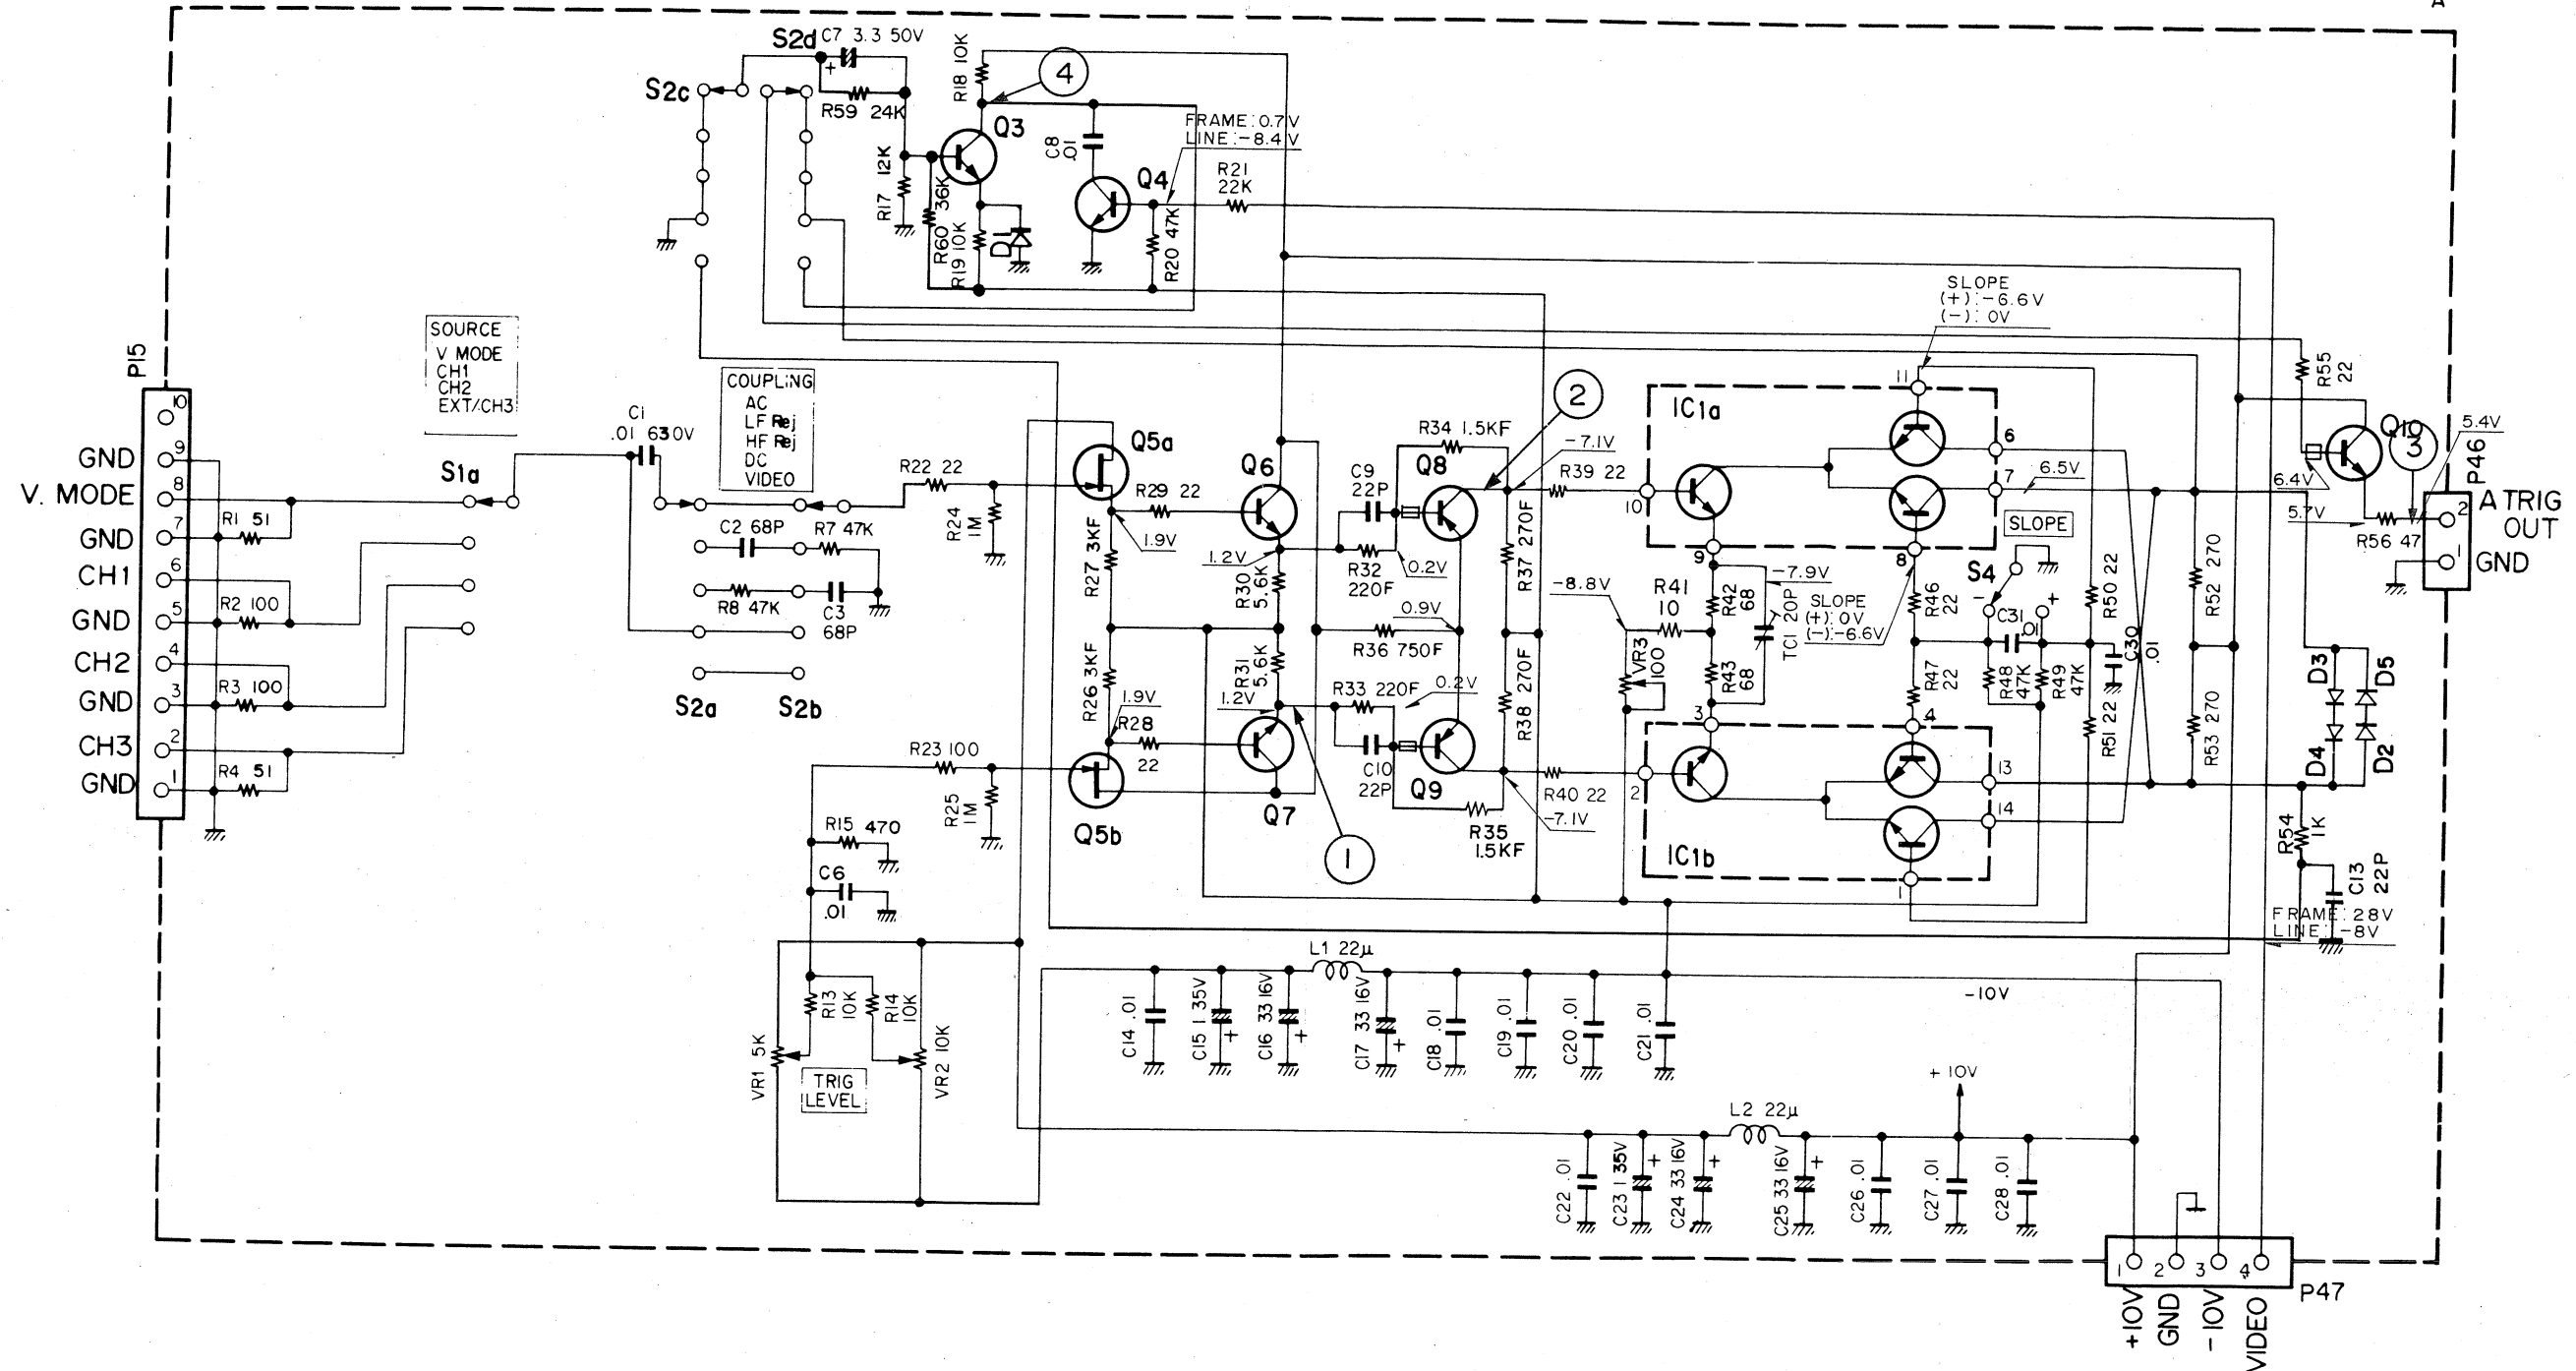

- IC1 : CA3102E
- Q3,4 : 2SC536KNP(F)
- Q5 : DN190I
- Q6,7 : 2SC1215(T or S)
- Q8,9 : 2SA116I
- Q10 : 2SC267I
- D1~5 : DS442X



PC BOARD

X77-1120-01





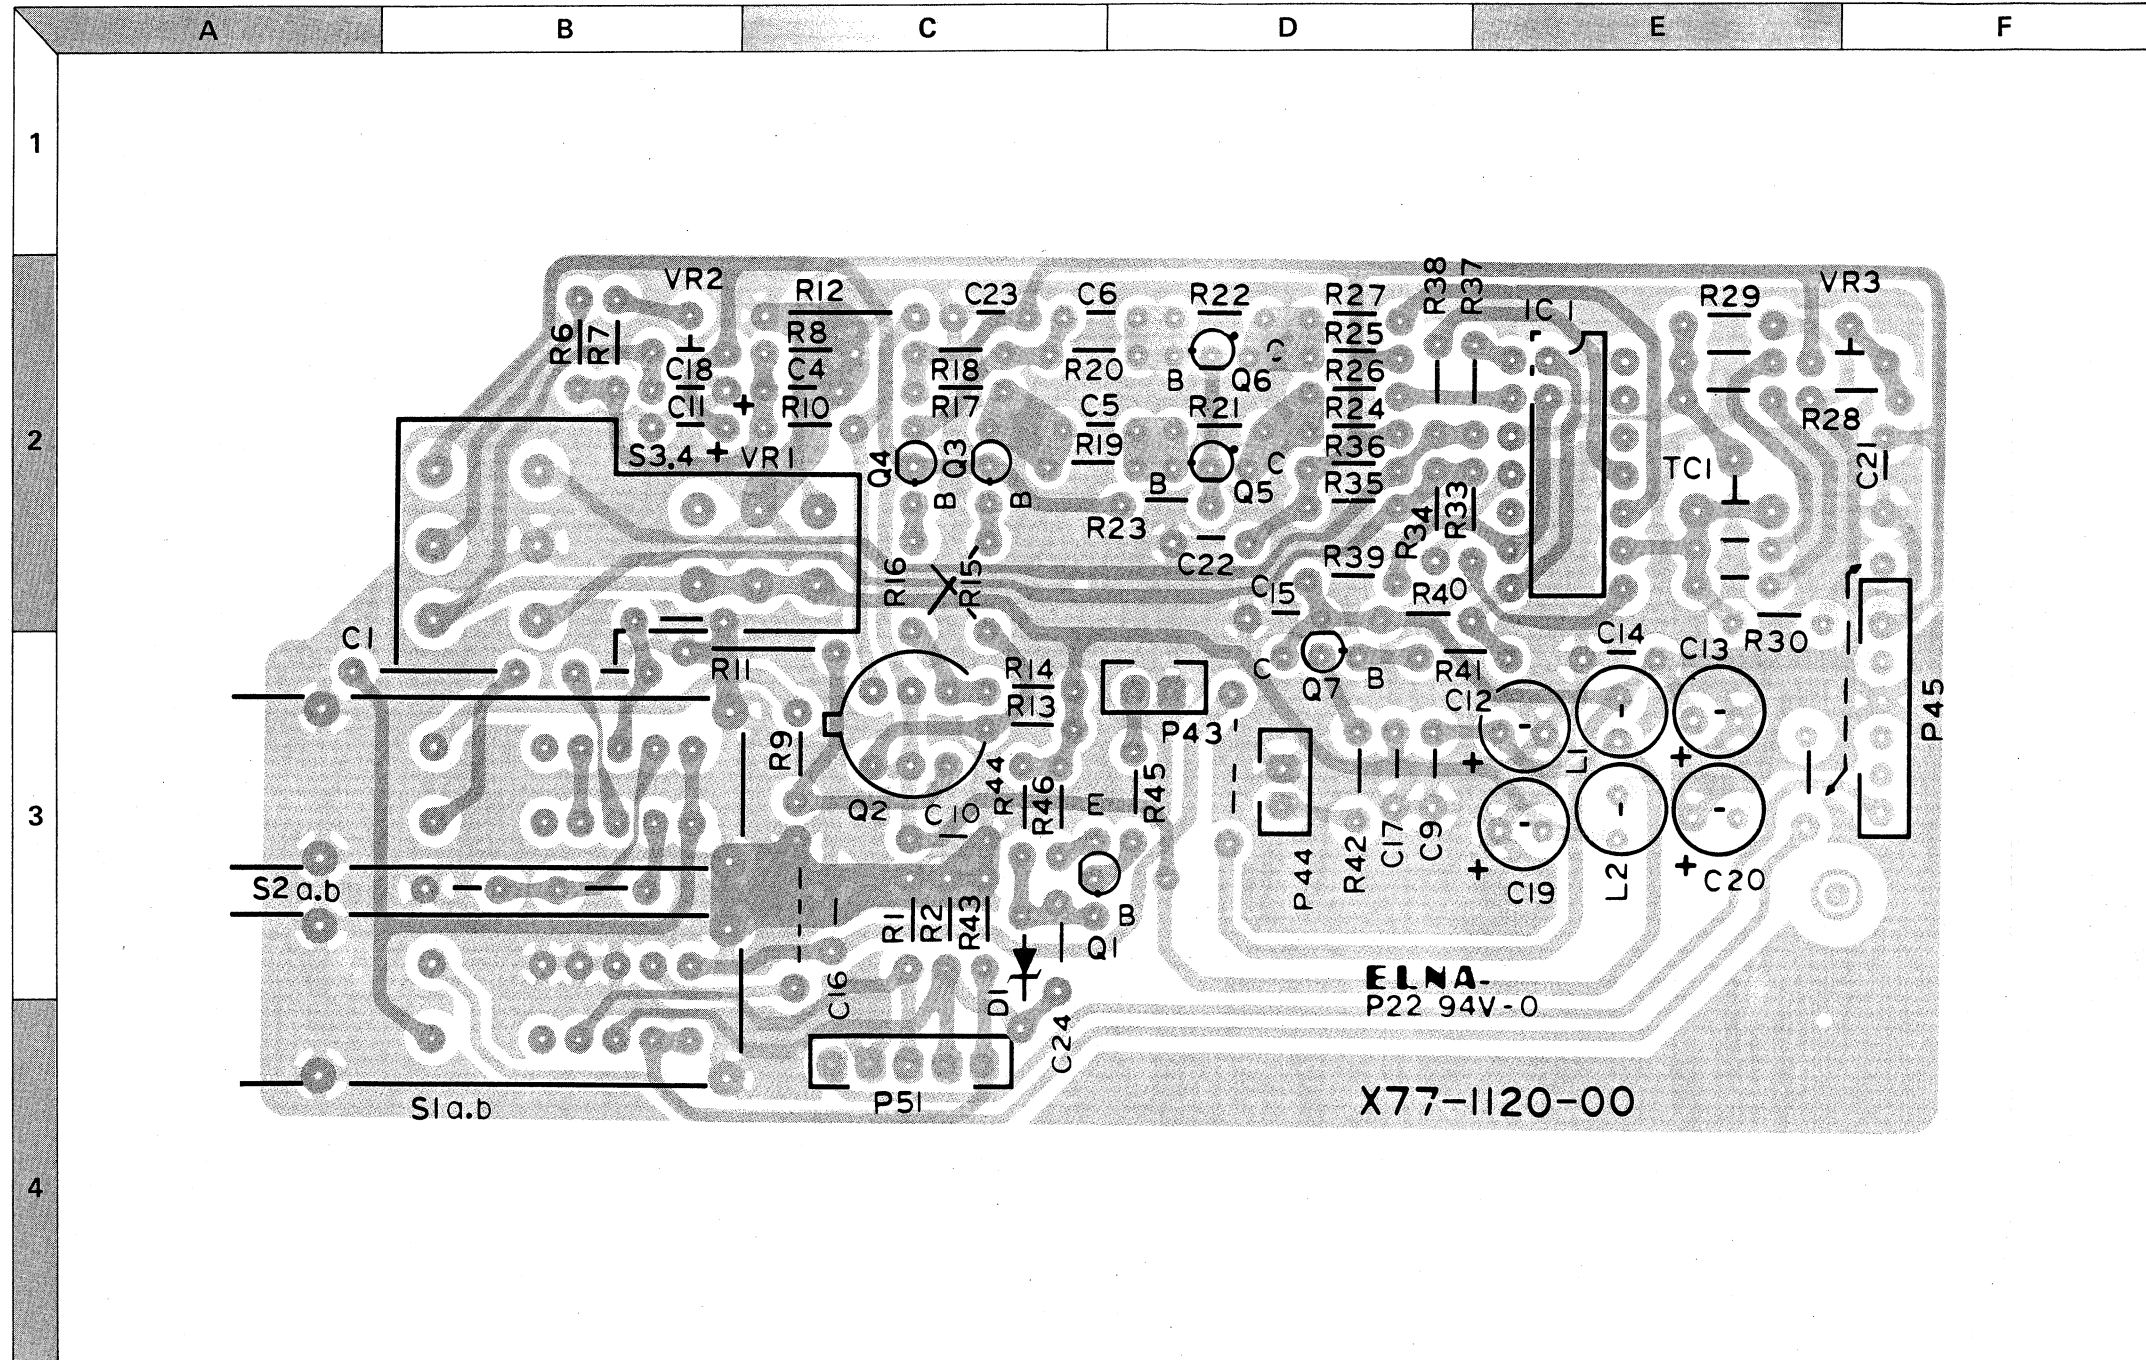


BOARD


D E F

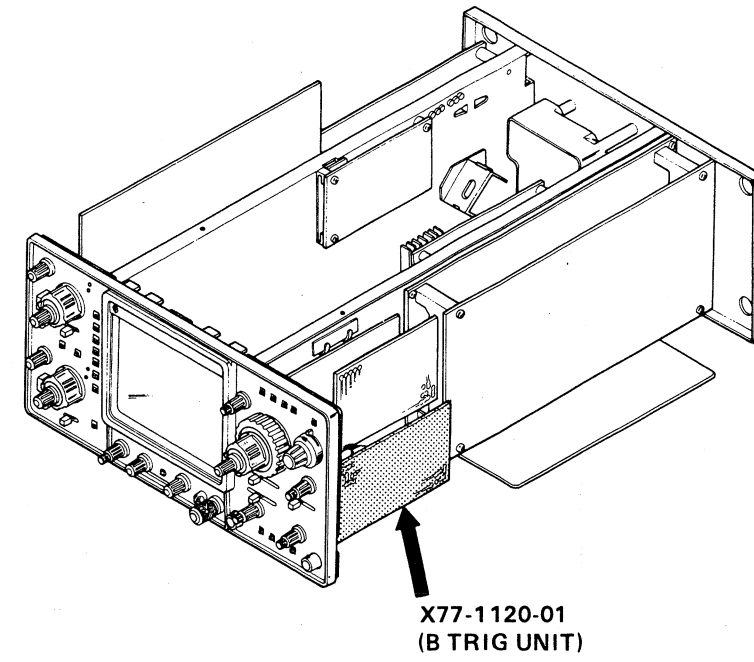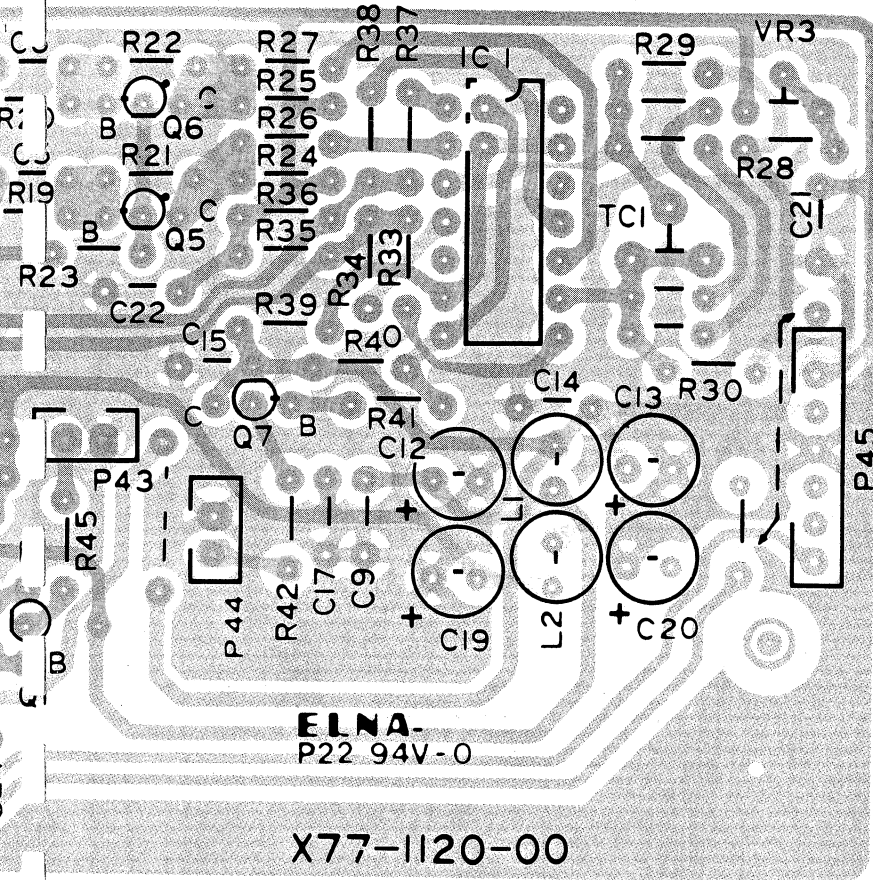

WAVEFORMS

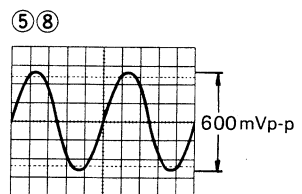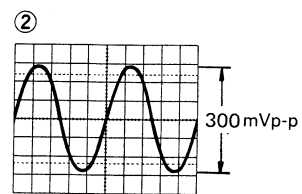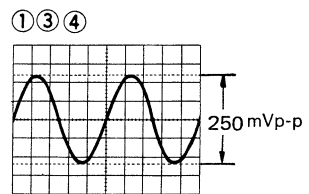


SCHEMATIC I

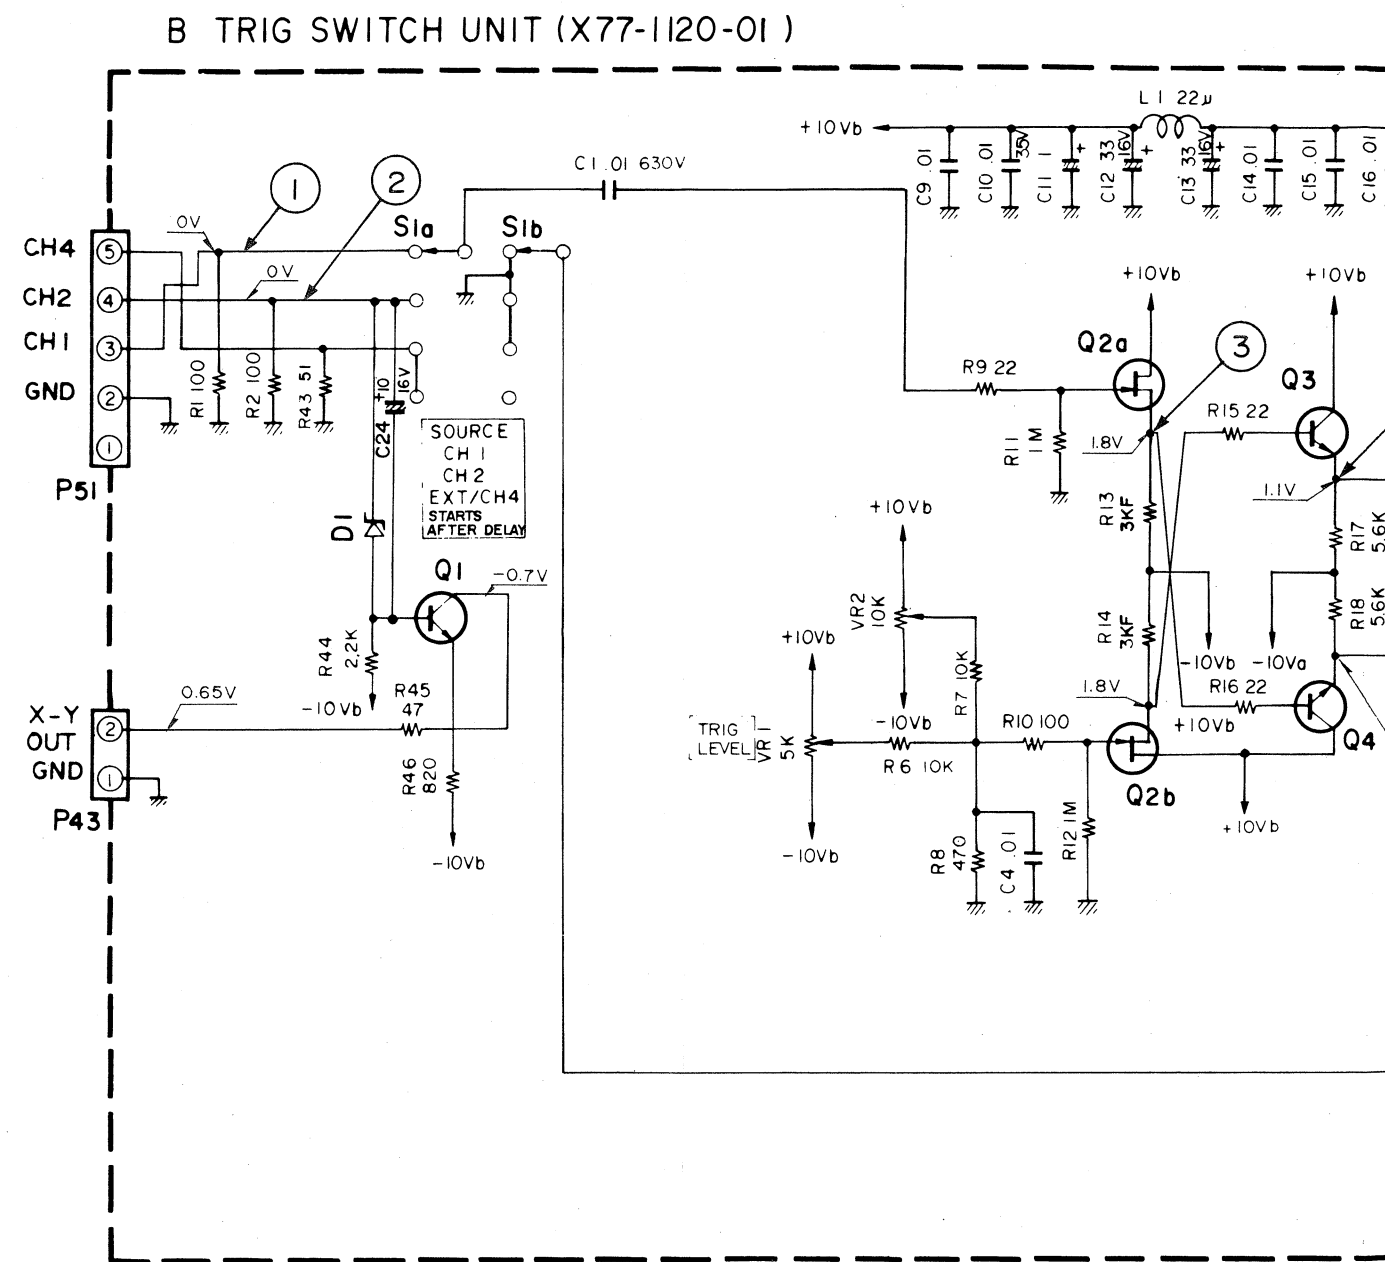

- IC1 : CA3102E Q5,6 : 2SA1161
- Q1,3,4 : 2SC1215TorS D1 : WZ-081
- Q2 : DNI901
- Q7 : 2SC2499

SCHEMATIC DIAGRAM

B TRIG SWITCH UNIT (X77-1120-01)


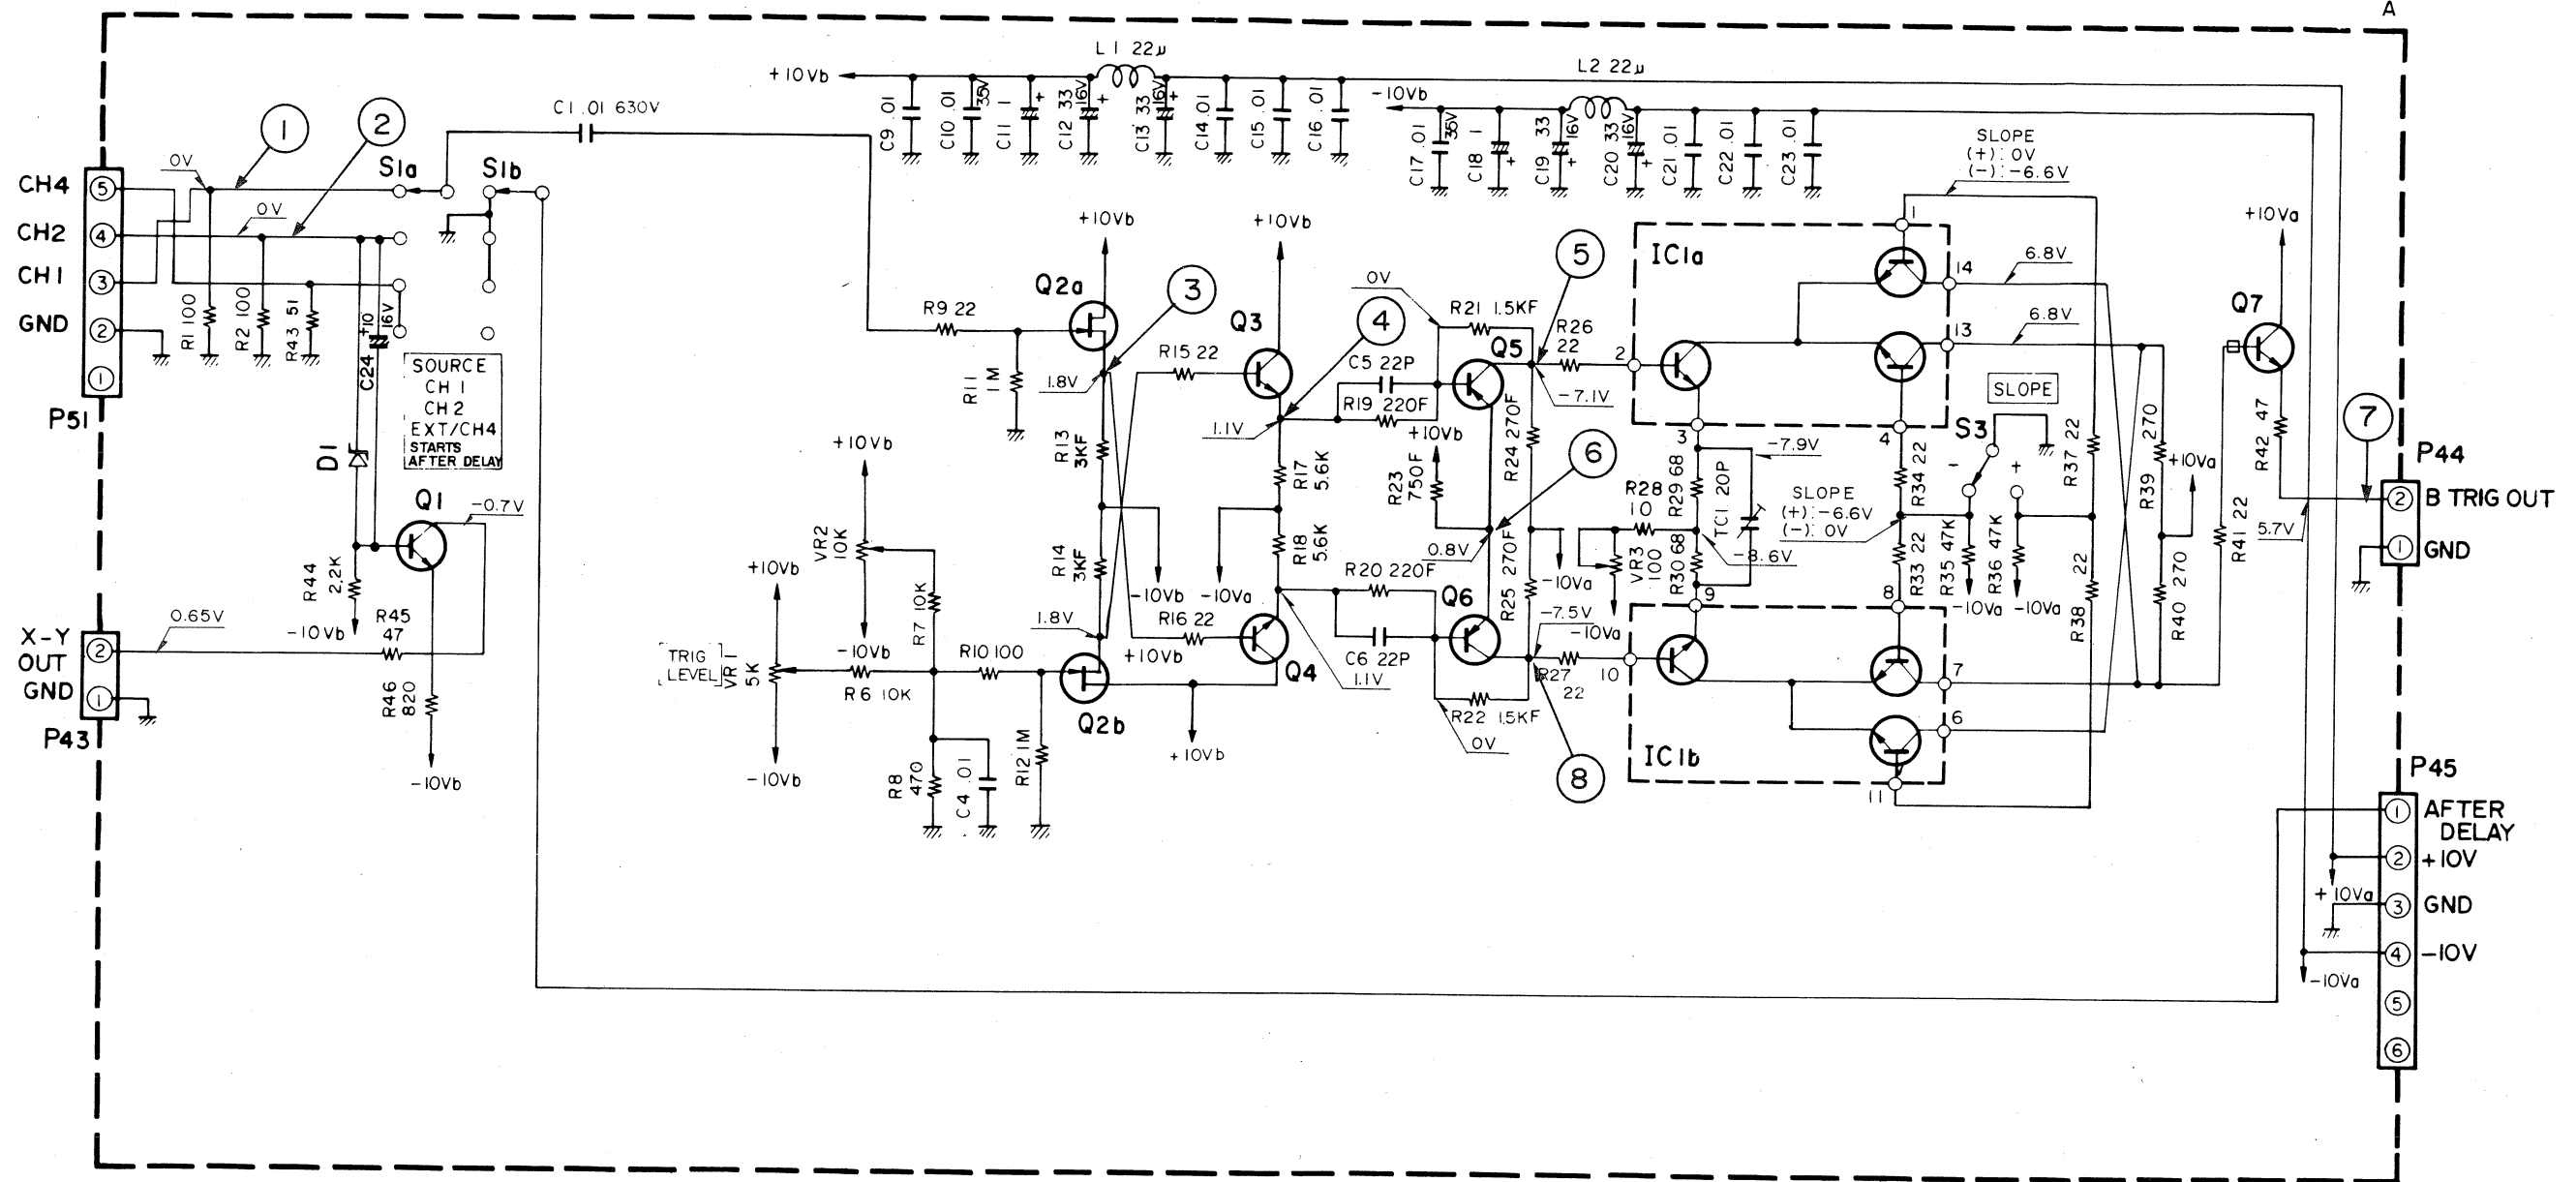


- | | |
|----------------------|----------------|
| IC1 : CA3102E | Q5,6 : 2SA1161 |
| Q1,3,4 : 2SC1215TorS | DI : WZ-081 |
| Q2 : DNI901 | |
| Q7 : 2SC2499 | |

PC BOARD

X68-1310-01



X68-1:

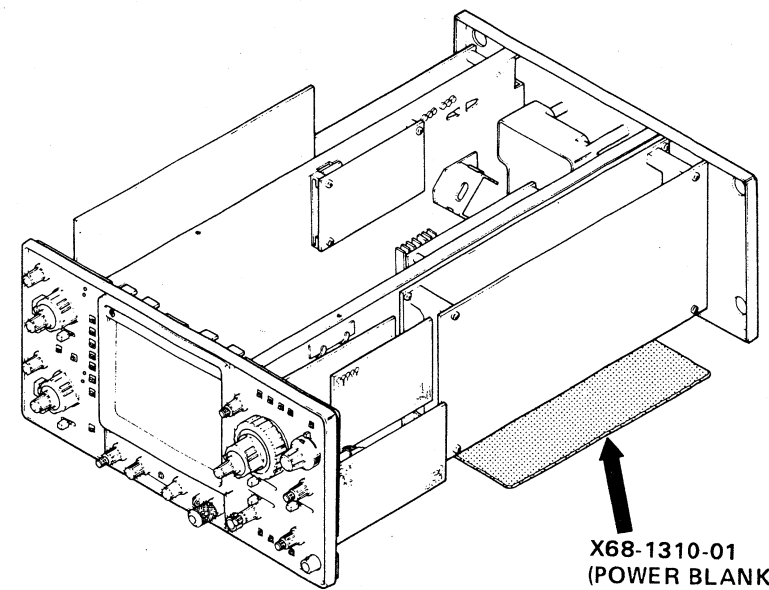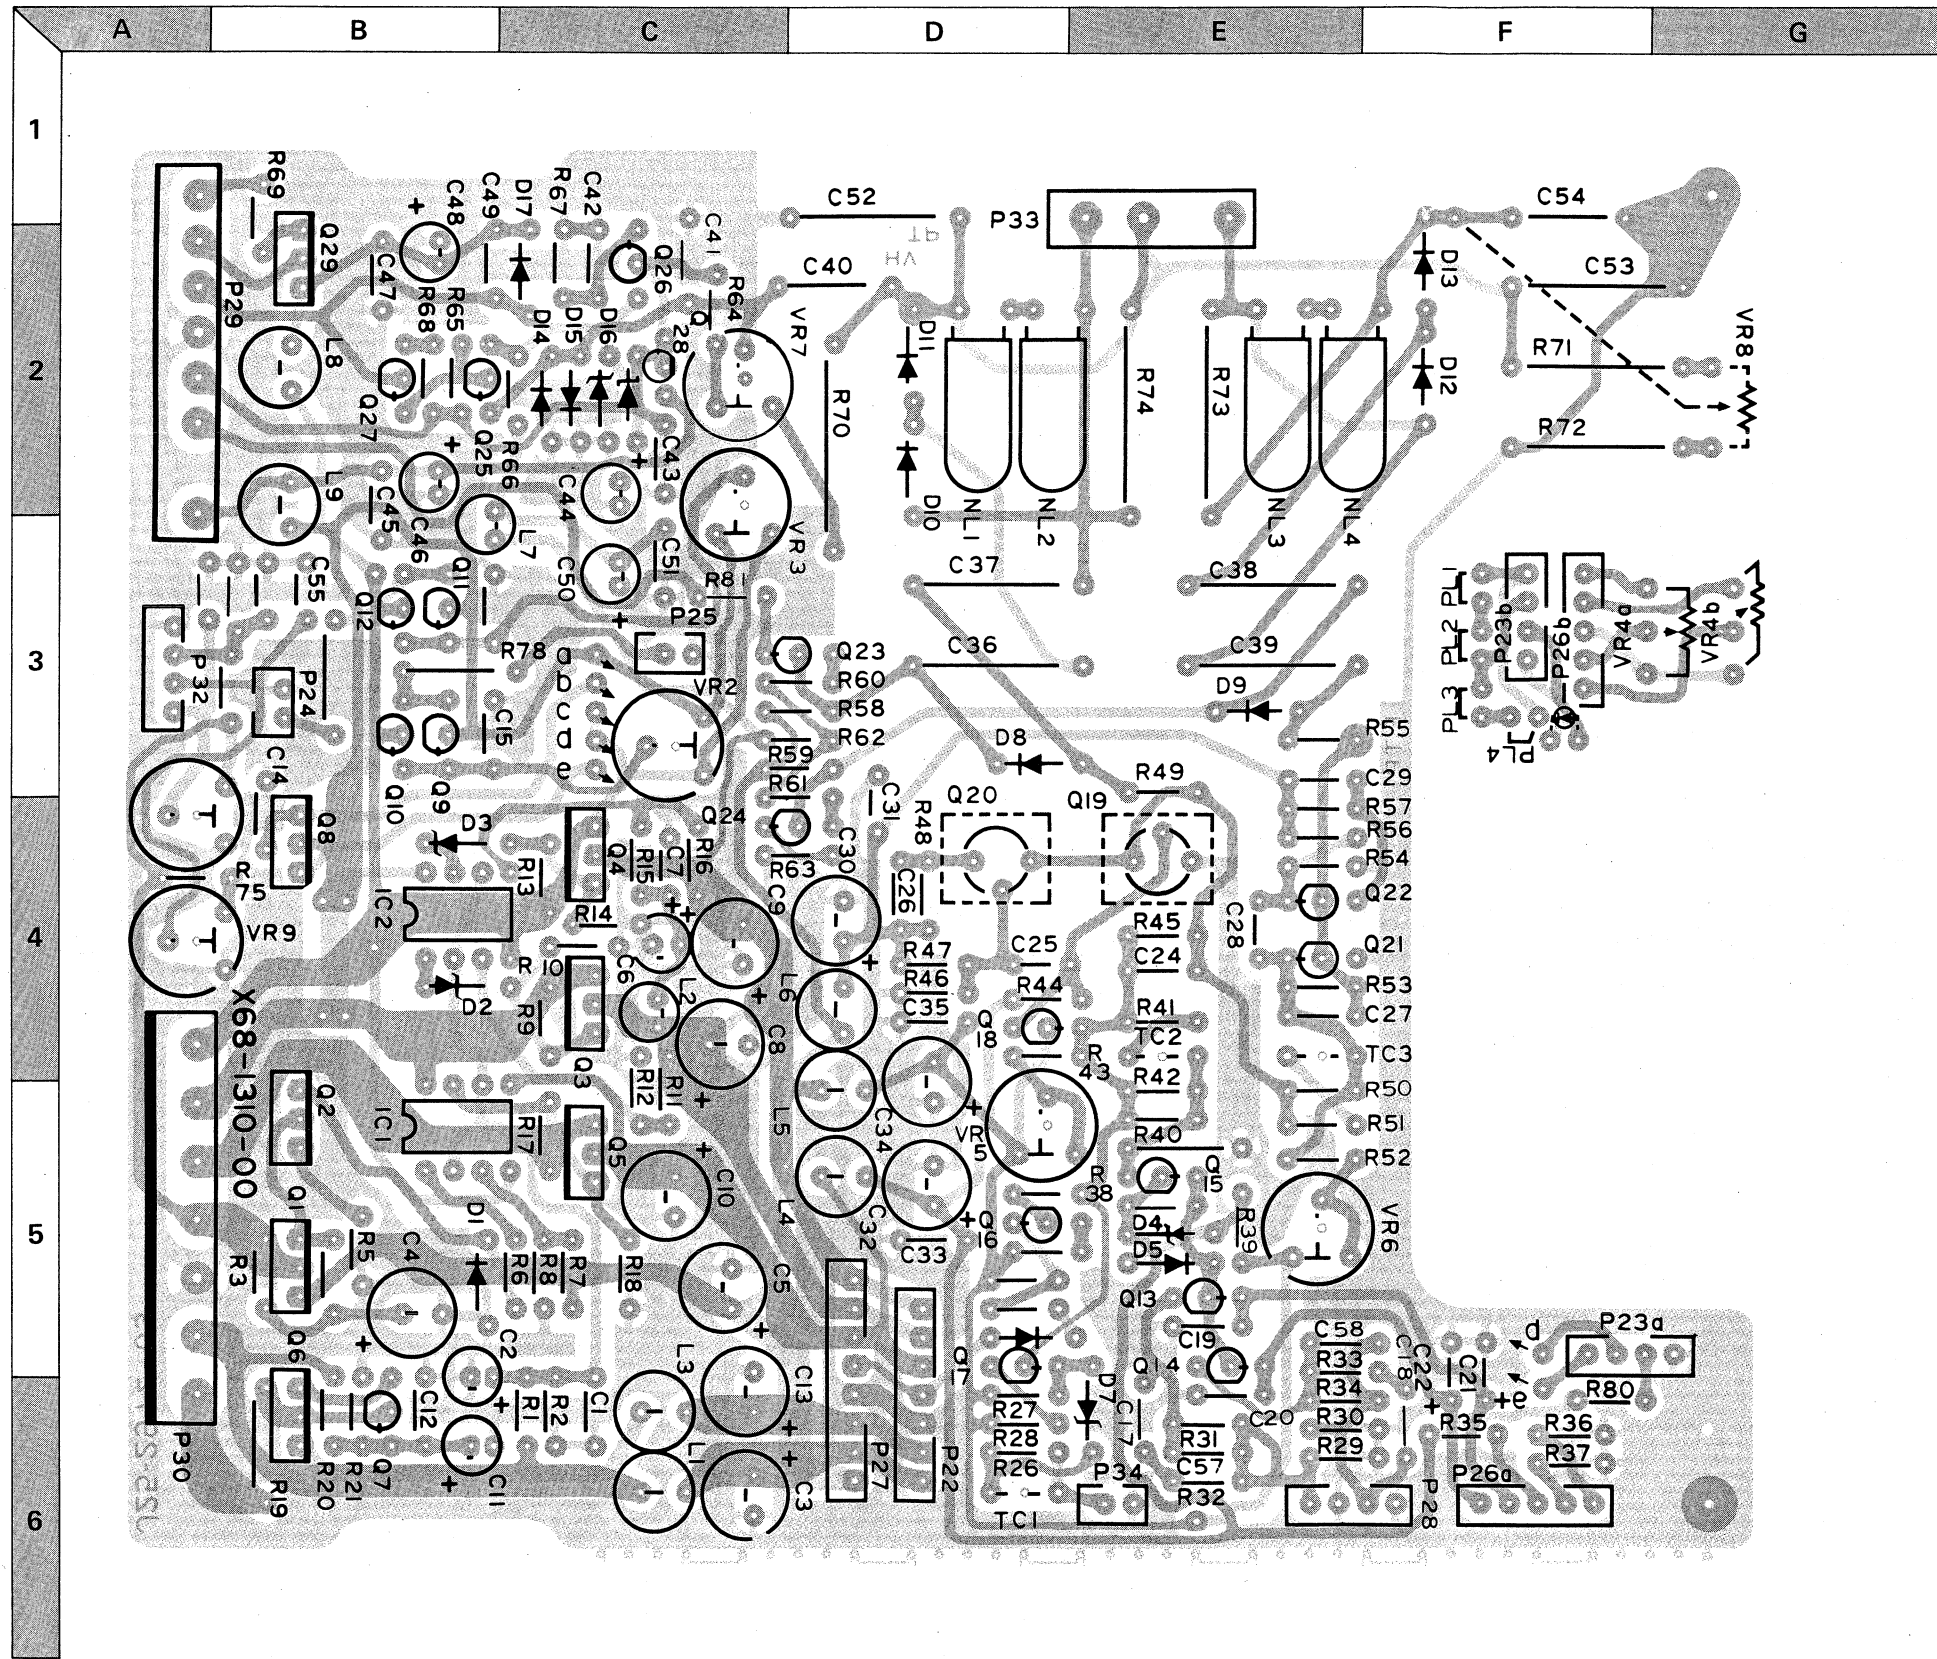



X68-1310-01
(POWER BLANKING UNIT)

BOARD


X68-1310-01

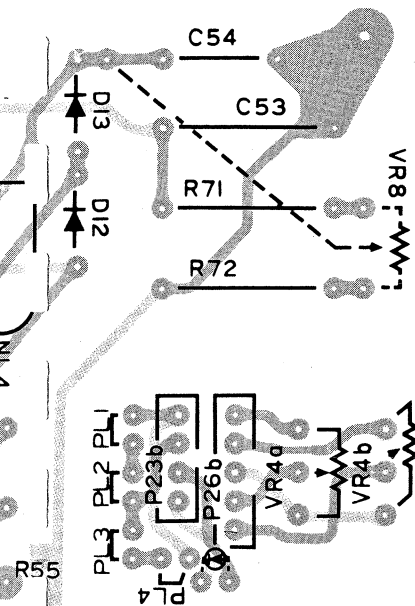


R55
C 9
R57
R56
F 4
C 2
Q21
F 3
C 7
TC3
F 0
R51
R52

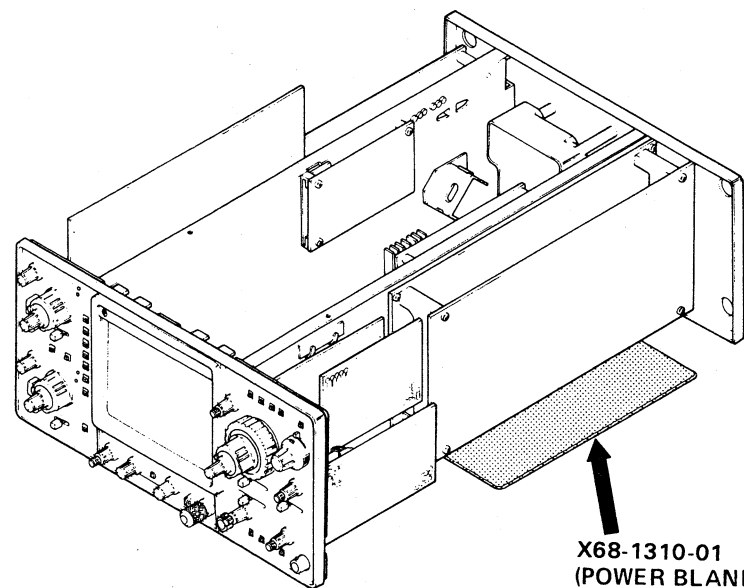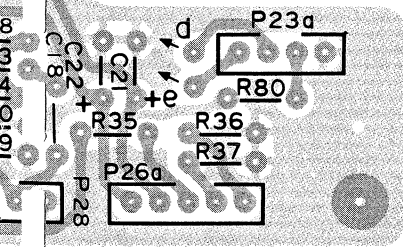

X68-1310-01
(POWER BLANKING UNIT)






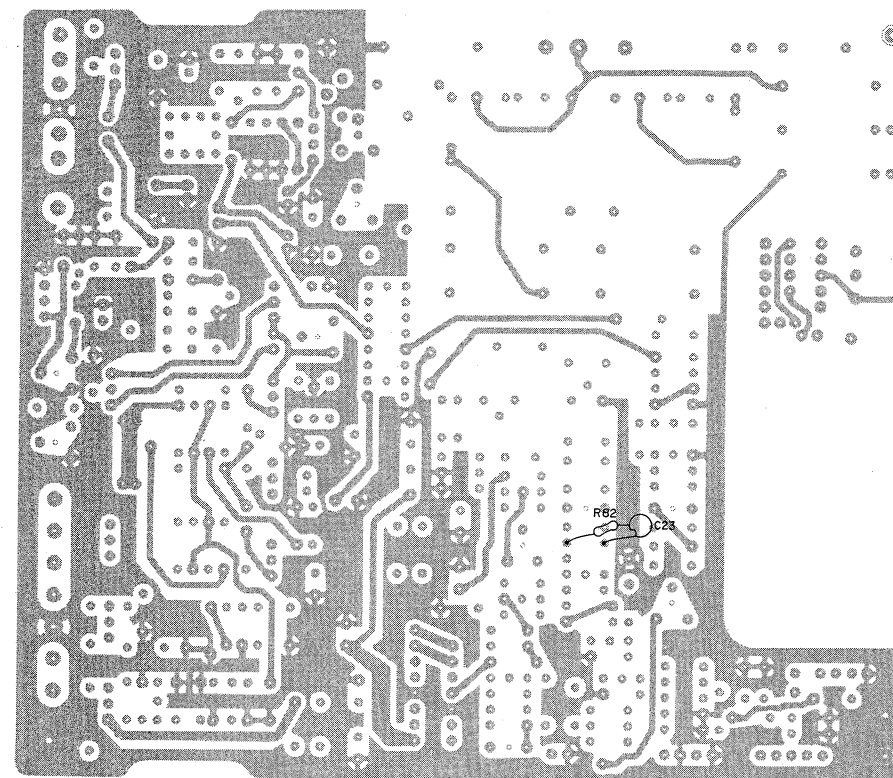



(Parts Side View)

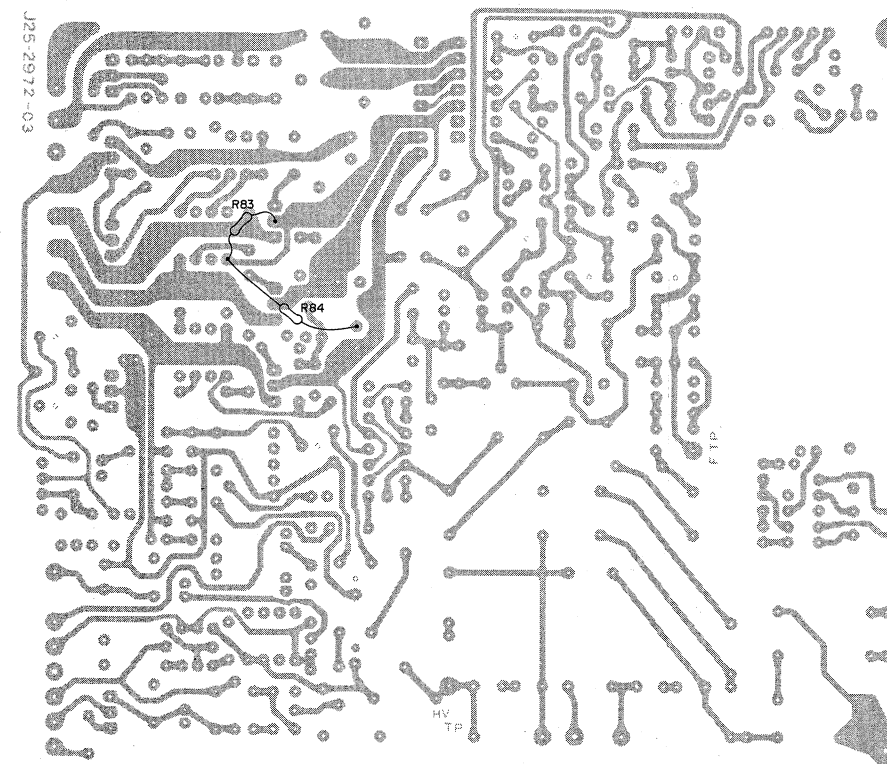


(Foil Side View)

WAVEFORMS

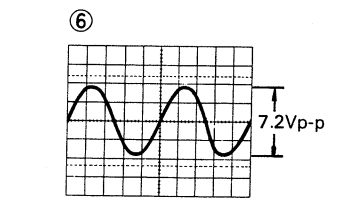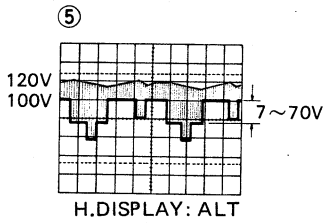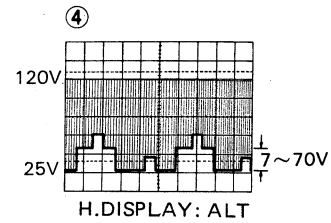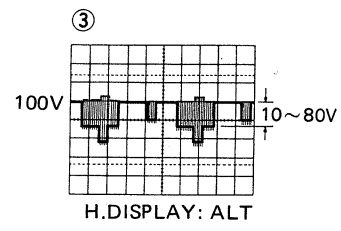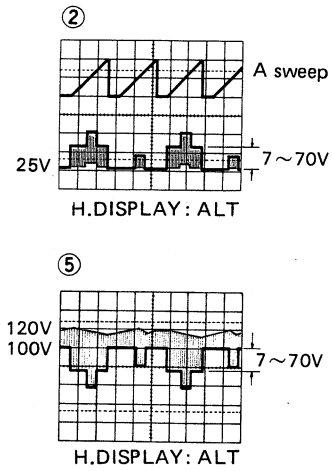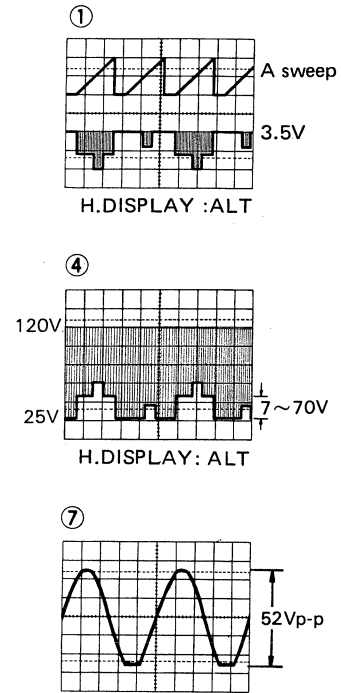


Note:  : CHOP Operation

SCHEMATIC

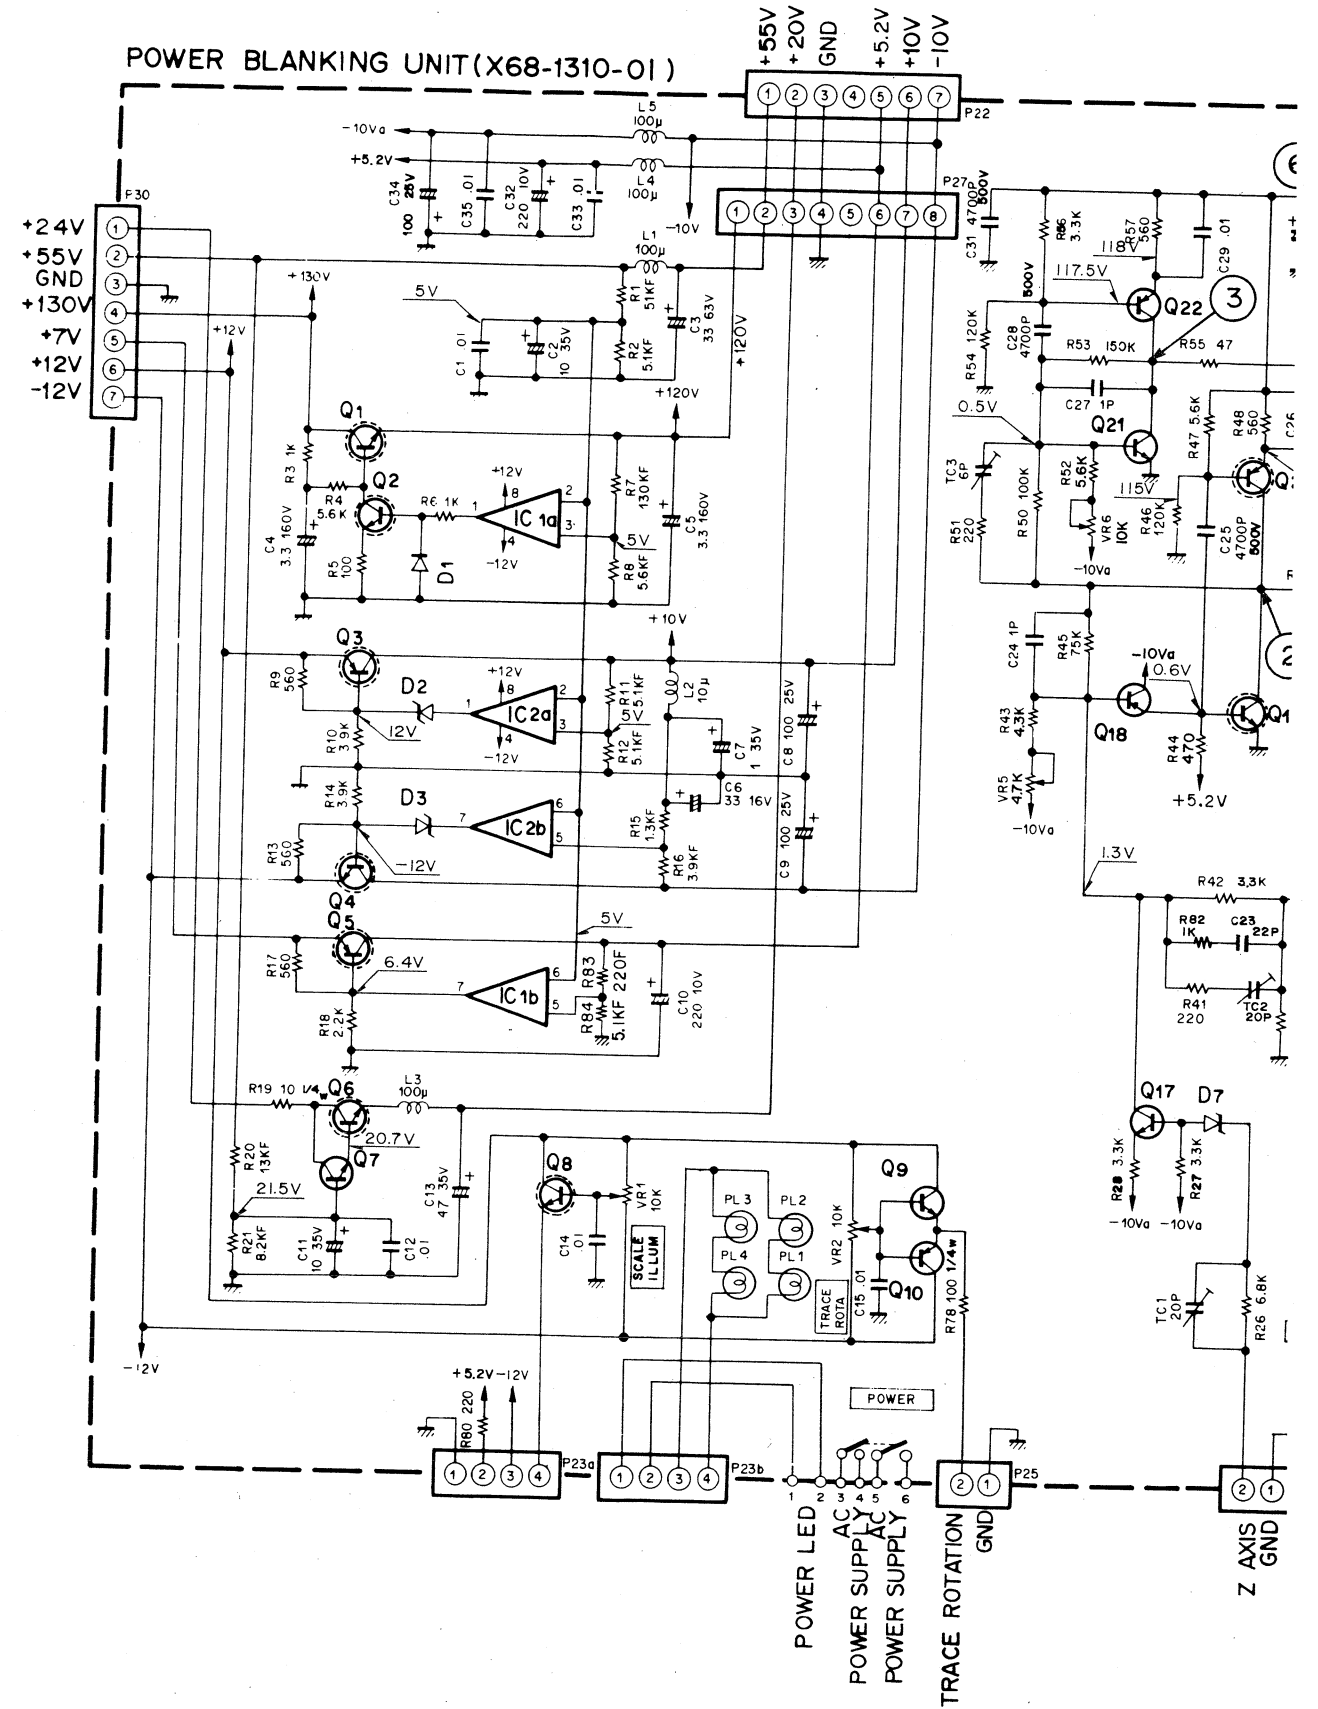


SCHEMATIC DIAGRAM

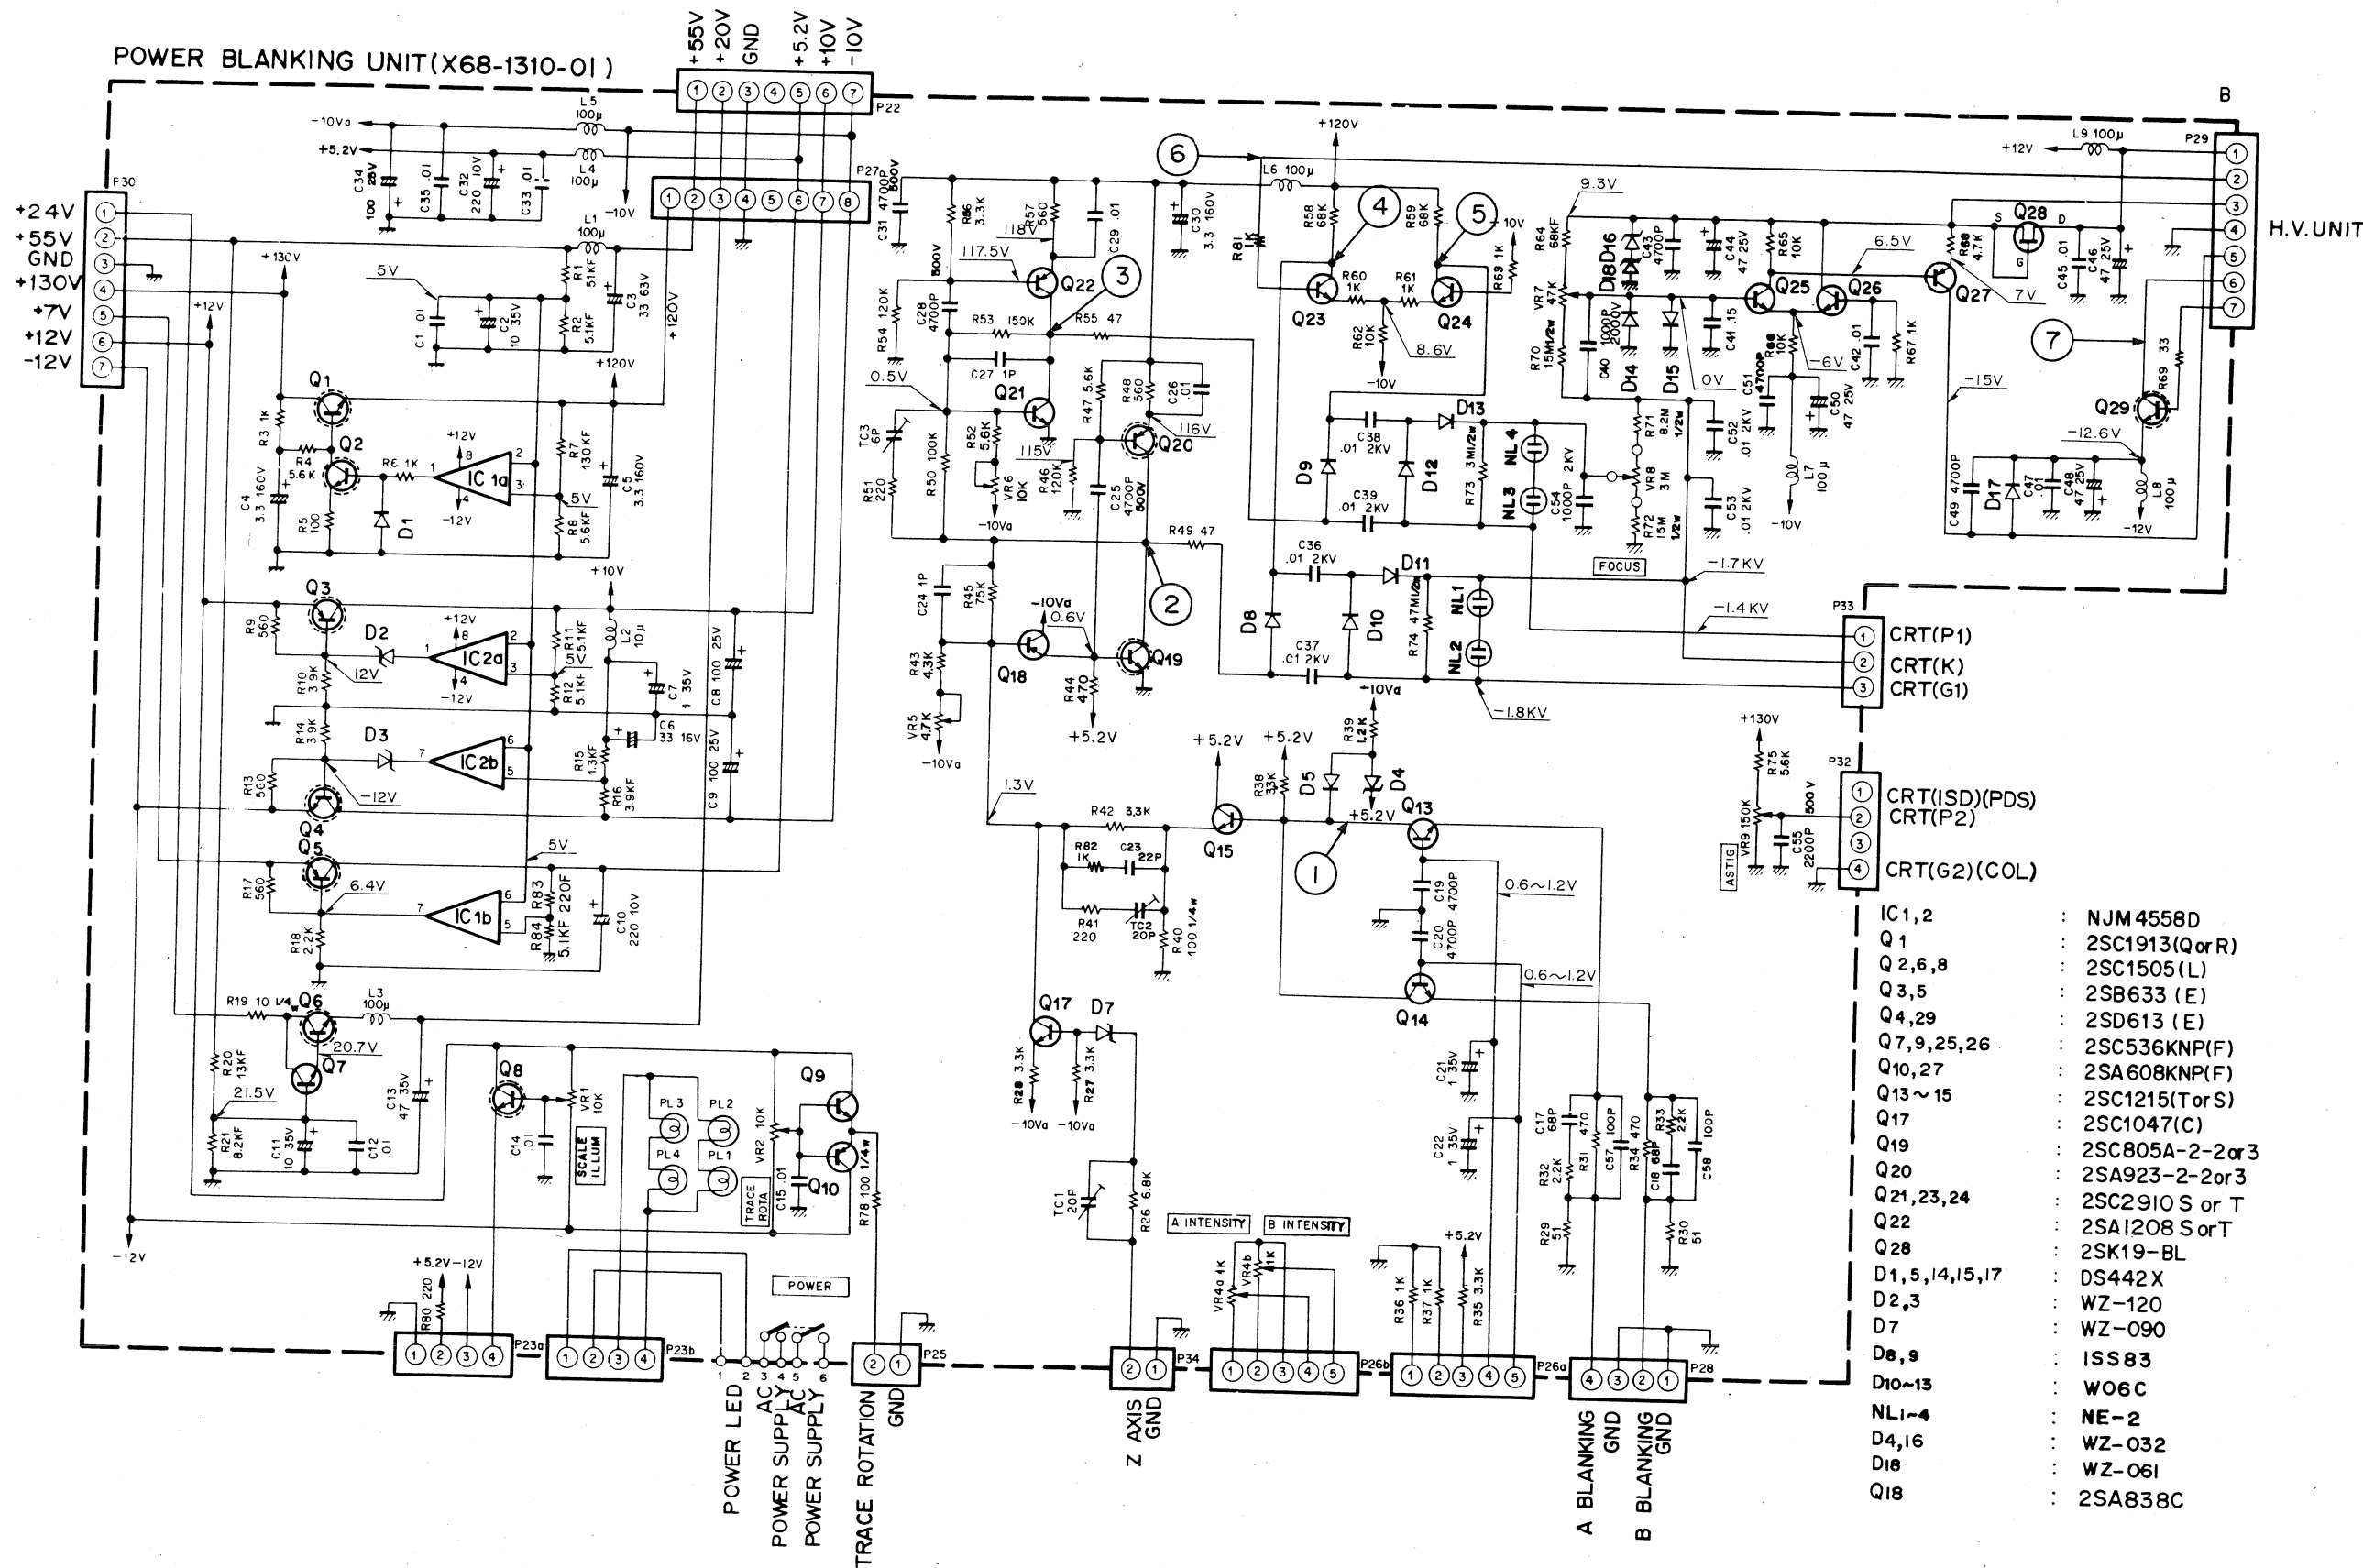


- IC 1, 2 : NJM 4558D
- Q 1 : 2SC1913(Q or R)
- Q 2, 6, 8 : 2SC1505(L)
- Q 3, 5 : 2SB633 (E)
- Q 4, 29 : 2SD613 (E)
- Q 7, 9, 25, 26 : 2SC536KNP(F)
- Q 10, 27 : 2SA608KNP(F)
- Q 13 ~ 15 : 2SC1215(T or S)
- Q 17 : 2SC1047(C)
- Q 19 : 2SC805A-2-2 or 3
- Q 20 : 2SA923-2-2 or 3
- Q 21, 23, 24 : 2SC2910 S or T
- Q 22 : 2SA1208 S or T
- Q 28 : 2SK19-BL
- D 1, 5, 14, 15, 17 : DS442 X
- D 2, 3 : WZ-120
- D 7 : WZ-090
- D 8, 9 : ISS 83
- D 10-13 : WO6C
- NL 1-4 : NE-2
- D 4, 16 : WZ-032
- D 18 : WZ-061
- Q 18 : 2SA838C

SEMICONDUCTORS


C-MOS IC

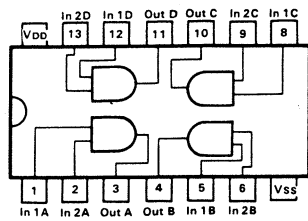


Top view
MC14081BCP

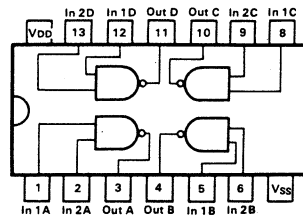


Top view
MC14011BCP

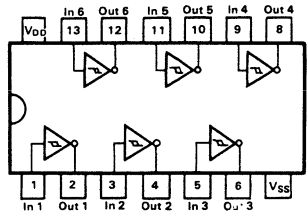


Top view
MC14584BCP

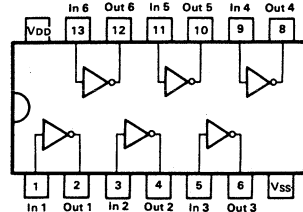


Top view
MC14069UBCP

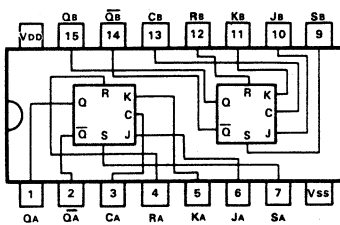


Top view
MC14027BCP

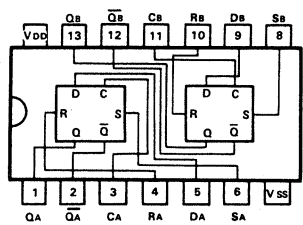


Top view
MC14013BCP

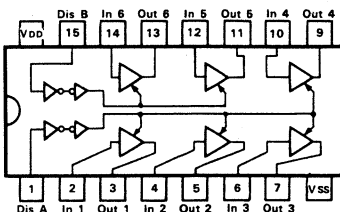


Top view
MC14503BCP

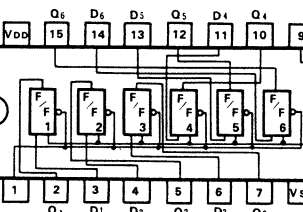


Top view
MC14174BCP

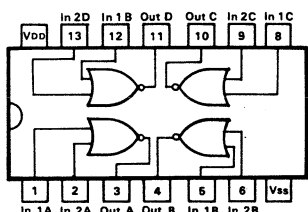


Top view
MC14001BCP

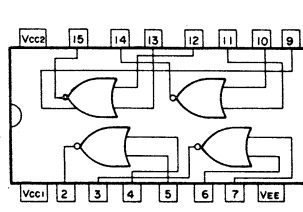


MC10102P

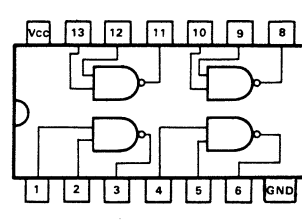


Top view
SN74S00N
SN74LS00N
74F00PC

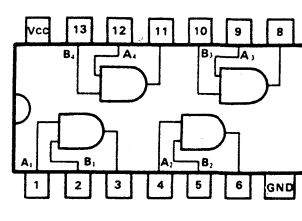


Top view
SN74LS08N
SN74S08N

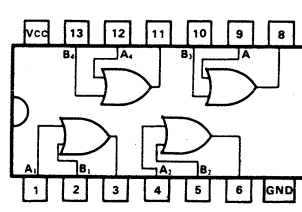


Top view
SN7432N
SN74LS32N
SN74S32N

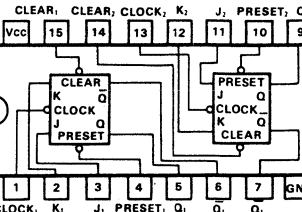


Top view
SN74LS112AN
SN74S112N

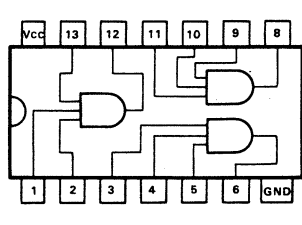


Top view
SN74LS11N

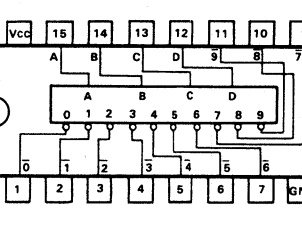


Top view
SN7442AN

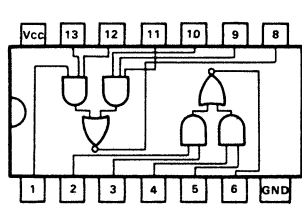

Top view
SN74LS51N

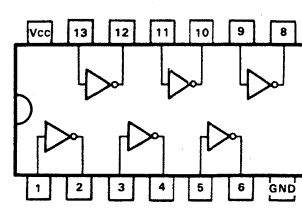

Top view
SN7404N
SN74LS04N

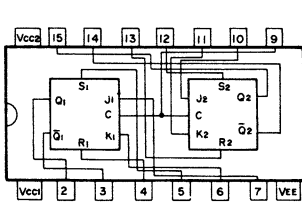


MC10135P

TTL IC


OTHER

TRANSISTOR


FET.

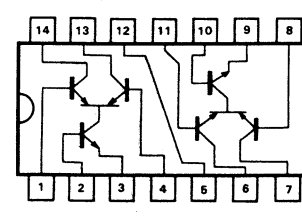


Top view
CA3102E

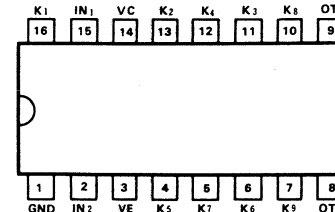


Top view
ATM-4010




Top view
TL082CP
NJM4558D




MC78L05C




- 2SA608KNP (F)
- 2SA838 (C)
- 2SA896-2-2
- 2SD438 (F)
- 2SC536KNP (F)
- 2SC1047 (C)
- 2SC1215 (T or S)
- 2SC1811-2-2
- 2SC1973 (T)
- 2SC2910 (S or T)
- 2SA1208 (S or T)

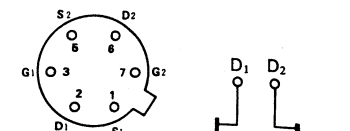


U440 DN1901




- 2SB633 (E)
- 2SD613 (E)
- 2SC1505 (L)




2SK19 (BL)




- 2SA1161
- 2SC2499
- 2SC2644
- 2SC2671
- 2SC2407




2SK30A (O)



- 2SC1913 (Q, R)



- 2SA923-2-2 or 3
- 2SC805A2-2 or 3



- 2SC1164 (O)

CS-2070 SERVICE MANUAL CHANGE INFORMATION:

At Trio, we continually strive to keep up with latest electronic developments by adding circuit and component improvement to our instruments as soon as they are developed and tested.

Sometimes, due to printing and shipping requirements, we can't get these change immediately into printed manual.

Also, a single change may affect several section.

Since the change information sheets are permanently entered, some duplication may occur.

Because of the universal parts procurement problem, some electrical parts in your instrument may be different from those described in the replaceable electrical parts list. (Main chassis)

PARTS LIST

Note: A: Addition
C: Change
D: Deletion

S/No. 2120001 ~ VERTICAL ATTENUATOR (X75-1120-01)

Ref. No.	Parts No.	Name & Description			Note	
R32	RN14BK2B5600F	RN	560Ω	± 1%	1/8W	C
R33	RN14BK2B5600F	RN	560Ω	± 1%	1/8W	C
R74	RN14BK2B5600F	RN	560Ω	± 1%	1/8W	C
R75	RN14BK2B5600F	RN	560Ω	± 1%	1/8W	C
IC12		IC	ATM-4020			C
IC13		IC	ATM-4020			C

S/No. 3010001 ~ POWER BLANKING (X68-1310-01)

Ref. No.	Parts No.	Name & Description			Note	
R53	RD14BB2C753J	RD	75kΩ			C

S/No. 3020001 ~ POWER BLANKING (X68-1310-01)

Ref. No.	Parts No.	Name & Description			Note	
Q1		TR	2SC2591(Q or R)			C

S/No. 3040001 ~ TRIG SWEEP (X74-1320-01)

Ref. No.	Parts No.	Name & Description			Note	
R269	RD14BB2C162J	RD	1.6kΩ			C
R272	RD14BB2C162J	RD	1.6kΩ			C
R287	RD14BB2C471J	RD	470Ω			C
D67		Diode	GMA-01			A
D68		Diode	GMA-01			A
D69		Diode	GMA-01			A
D70		Diode	GMA-01			A
D71		Diode	GMA-01			A

PARTS LIST

S/No. 3050001 ~
VERTICAL PRE AMPLIFIERE (X73-1320-01)

Ref. No.	Parts No.	Name & Description			Note	
C1	CC45CH1H120J	CC	12pF	±5%	D	
C2	CC45CH1H100J	CC	10pF	±5%	D	
C5	CC45CH1H020C	CC	2pF	±0.25pF	C	
C9	CC45CH1H270J	CC	27pF	±5%	C	
C13	CC45CH1H270J	CC	27pF	±5%	D	
C14	CC45CH1H100J	CC	10pF	±5%	C	
C16	CC45CH1H270J	CC	27pF	±5%	A	
C23	CC45CH1H680J	CC	68pF	±5%	D	
C34	CC45CH1H120J	CC	12pF	±5%	C	
C35	CC45CH1H120J	CC	12pF	±5%	C	
C38	CC45CH1H270J	CC	27pF	±5%	D	
C39	CC45CH1H150J	CC	15pF	±5%	D	
C42	CC45CH1H020C	CC	2pF	±0.25pF	C	
C46	CC45CH1H270J	CC	27pF	±5%	C	
C49	CC45CH1H020C	CC	2pF	±0.25pF	A	
C51	CC45CH1H100J	CC	10pF	±5%	C	
C60	CC45CH1H680J	CC	68pF	±5%	D	
C108	CC45CH1H330J	CC	33pF	±5%	A	
C115	CC45CH1H330J	CC	33pF	±5%	D	
C116	CC45CH1H080D	CC	8pF	±0.5pF	D	
C119	CC45CH1H101J	CC	100pF	±5%	D	
C120	CC45CH1H220J	CC	22pF	±5%	D	
C131	CC45CH1H070D	CC	7pF	±0.5pF	A	
C132	CC45CH1H070D	CC	7pF	±0.5pF	A	
C175	CC45CH1H020C	CC	2pF	±0.25pF	C	
C176	CC45CH1H050C	CC	5pF	±0.25pF	D	
C208	CC45CH1H050C	CC	5pF	±0.25pF	A	
C209	CC45CH1H050C	CC	5pF	±0.25pF	A	
C210	CK45B1H103K	CK	0.01μF	±10%	A	
TC12	C05-0062-05	TC	6pF		A	
R3	RN14BK2B2700F	RN	270Ω	±1%	1/8W	C
R4	RD14BB2C121J	RD	120Ω			D
R5	RD14BB2C472J	RD	4.7kΩ			D
R26	RD14BB2C470J	RD	47Ω			C
R38	RD14BB2C151J	RD	150Ω			C
R40	RN14BK2B1800F	RN	180Ω	±1%	1/8W	C
R48	RD14BB2C100J	RD	10Ω			C
R49	RD14BB2C472J	RD	4.7kΩ			D
R54	RN14BK2B2400F	RN	240Ω	±1%	1/8W	C
R58	RD14BB2C682J	RD	6.8kΩ			A
R85	RD14BB2C473J	RD	47kΩ			C
R86	RD14BB2C473J	RD	47kΩ			C
R115	RD14BB2C471J	RD	470Ω			C
R118	RN14BK2B2700F	RN	270Ω	±1%	1/8W	C
R150	RD14BB2C470J	RD	47Ω			C
R166	RN14BK2B2700F	RN	270Ω	±1%	1/8W	C
R167	RD14BB2C330J	RD	33Ω			D
R168	RD14BB2C102J	RD	1kΩ			D
R199	RD14BB2C470J	RD	47Ω			C
R211	RD14BB2C151J	RD	150Ω			C
R213	RN14BK2B1800F	RN	180Ω	±1%	1/8W	C
R221	RD14BB2C100J	RD	10Ω			C
R227	RN14BK2B2000F	RN	200Ω	±1%	1/8W	C
R277	RD14BB2C471J	RD	470Ω			C
R280	RN14BK2B2700F	RN	270Ω	±1%	1/8W	C
R290	RD14BB2C153J	RD	15kΩ			D
R291	RD14BB2C272J	RD	2.7kΩ			D
R293	RD14BB2C331J	RD	330Ω			A
R294	RD14BB2C331J	RD	330Ω			A
R295	RD14BB2C103J	RD	10kΩ			D
R317	RD14BB2C473J	RD	47kΩ			D

PARTS LIST

Ref. No.	Parts No.	Name & Description		Note
R318	RD14BB2C473J	RD	47k Ω	D
R319	RD14BB2C103J	RD	10k Ω	D
R320	RD14BB2C822J	RD	8.2k Ω	-
R321	RD14BB2C103J	RD	10k Ω	D
R322	RD14BB2C103J	RD	10k Ω	D
R323	RD14BB2C752J	RD	7.5k Ω	D
R324	RD14BB2C332J	RD	3.3k Ω	D
R325	RD14BB2C470J	RD	47 Ω	C
R326	RD14BB2C470J	RD	47 Ω	C
R329	RD14BB2C472J	RD	4.7k Ω	A
R333	RD14BB2C620J	RD	62 Ω	C
R334	RD14BB2C620J	RD	62 Ω	C
TH1		Thermister SDT-1000		D
Q79		TR	2SC536KNP (F)	D
D40		Diode	1S2686	D
D41		Diode	1S2686	D
D42		Diode	1S2686	D
D43		Diode	1S2686	D
D44		Diode	DS442X	D

VERTICAL ATTENUATOR (X75-1120-01)

Ref. No.	Parts No.	Name & Description		Note
C7	CC45CH1H030C	CC	3pF ± 0.25 pF	A
C20	CC45CH1H030C	CC	3pF ± 0.25 pF	A
R36	RD14BB2C151J	RD	150 Ω	A
R37	RD14BB2C151J	RD	150 Ω	A
R38	RD14BB2C330J	RD	33 Ω	A
R39	RD14BB2C330J	RD	33 Ω	A

VERTICAL OUTPUT (X73-1330-01)

Ref. No.	Parts No.	Name & Description		Note
C18	CC45CH1H070D	CC	7pF ± 0.5 pF	D
C19	CK45B1H102K	CK	1000pF $\pm 10\%$	C
C20	CC45CH1H070D	CC	7pF ± 0.5 pF	D
C25	CC45CH1H331J	CC	330pF $\pm 5\%$	A
C26	CC45CH1H331J	CC	330pF $\pm 5\%$	A
C27	CC45CH1H020C	CC	2pF ± 0.25 pF	A
R12	RD14BB2C302J	RD	3k Ω	D
R13	RD14BB2C122J	RD	1.2k Ω	D
R16	RN14BK2E6200F	RN	620 Ω $\pm 1\%$ 1/4W	D
R17	RN14BK2E6200F	RN	620 Ω $\pm 1\%$ 1/4W	D
R22	RD14BB2C151J	RD	150 Ω	C
R23	RD14BB2C101J	RD	100 Ω	A
R24	RD14BB2C220J	RD	22 Ω	A
R29	RD14BB2E100J	RD	10 Ω $\pm 5\%$ 1/4W	C
R34	RD14BB2C471J	RD	470 Ω	D
R37	RD14BB2C471J	RD	470 Ω	D
R40	RD14BB2C181J	RD	180 Ω	C
R46	RD14BB2C181J	RD	180 Ω	C
R49	RD14BB2C561J	RD	560 Ω	A
R51	RD14BB2C471J	RD	470 Ω	A
R52	RD14BB2C471J	RD	470 Ω	A
R55	RD14BB2C221J	RD	220 Ω	A
R58	RD14BB2C621J	RD	620 Ω	A
R59	RD14BB2C621J	RD	620 Ω	A
R60	RN14BK2B3600F	RN	360 Ω $\pm 1\%$ 1/8W	A
R61	RN14BK2B3600F	RN	360 Ω $\pm 1\%$ 1/8W	A
R62	RD14BB2C220J	RD	22 Ω	A
R63	RD14BB2C220J	RD	22 Ω	A

PARTS LIST


Ref. No.	Parts No.	Name & Description	Note
L1	L40-2282-13	Ferri inductor 0.22 μ H	D
L2	L33-0806-05	Choke coil 0.7 μ H	C
L4	L40-2282-13	Ferri inductor 0.22 μ H	D
L5	L33-0806-05	Choke coil 0.7 μ H	C
L8	L40-1011-03	Ferri inductor 100 μ H	D
D1		Diode DS442X	A
Q1		TR 2SC2671	C
Q2		TR 2SC2671	C
Q3		TR 2SC1215 (T or S)	C
Q4		TR 2SC1215 (T or S)	C
Q6		TR 2SC1047 (C)	A
Q15		TR 2SA838 (C)	A

TRIG SWEEP (X74-1320-01)

Ref. No.	Parts No.	Name & Description	Note
C11	C91-0549-05	Tantalum 1 μ F 35V	C
C24	CC45CH1H121J	CC 120pF \pm 5%	C
C25	CC45CH1H121J	CC 120pF \pm 5%	C
C36	C91-0549-05	Tantalum 1 μ F 35V	C
C44	CC45CH1H121J	CC 120pF \pm 5%	C
C54	CC45CH1H220J	CC 22pF \pm 5%	C
TC1	C05-0309-05	TC 40pF	C
TC2	C05-0309-05	TC 40pF	C
R49	RN14BK2B2402F	RN 24k Ω \pm 1% 1/8W	C
R50	RN14BK2B3001F	RN 3k Ω \pm 1% 1/8W	C
R51	RN14BK2B1501F	RN 1.5k Ω \pm 1% 1/8W	C
R52	RN14BK2B1202F	RN 12k Ω \pm 1% 1/8W	C
R55	RN14BK2B3001F	RN 3k Ω \pm 1% 1/8W	C
R56	RN14BK2B3001F	RN 3k Ω \pm 1% 1/8W	C
R149	RN14BK2B2402F	RN 24k Ω \pm 1% 1/8W	C
R150	RN14BK2B3001F	RN 3k Ω \pm 1% 1/8W	C
R151	RN14BK2B1202F	RN 12k Ω \pm 1% 1/8W	C
R152	RN14BK2B1501F	RN 1.5k Ω \pm 1% 1/8W	C
R154	RN14BK2B3001F	RN 3k Ω \pm 1% 1/8W	C
R155	RN14BK2B3001F	RN 3k Ω \pm 1% 1/8W	C
R299	RD14BB2C750J	RD 75 Ω	C
R301	RD14BB2C272J	RD 2.7k Ω	A
R303	RD14BB2C152J	RD 1.5k Ω	A
R304	RD14BB2C272J	RD 2.7k Ω	A
VR1	R12-2512-05	VR 5k Ω	C
VR2	R12-2512-05	VR 5k Ω	C
VR3	R12-2512-05	VR 5k Ω	C
VR4	R12-2512-05	VR 5k Ω	C
Q82		TR 2SC536KNP (F)	A
Q83		TR 2SC536KNP (F)	A
IC16		IC MC78L15AC	C


VERTICAL ATTENUATOR UNIT (X75-1120-01)

SCHEMATIC DIAGRAM

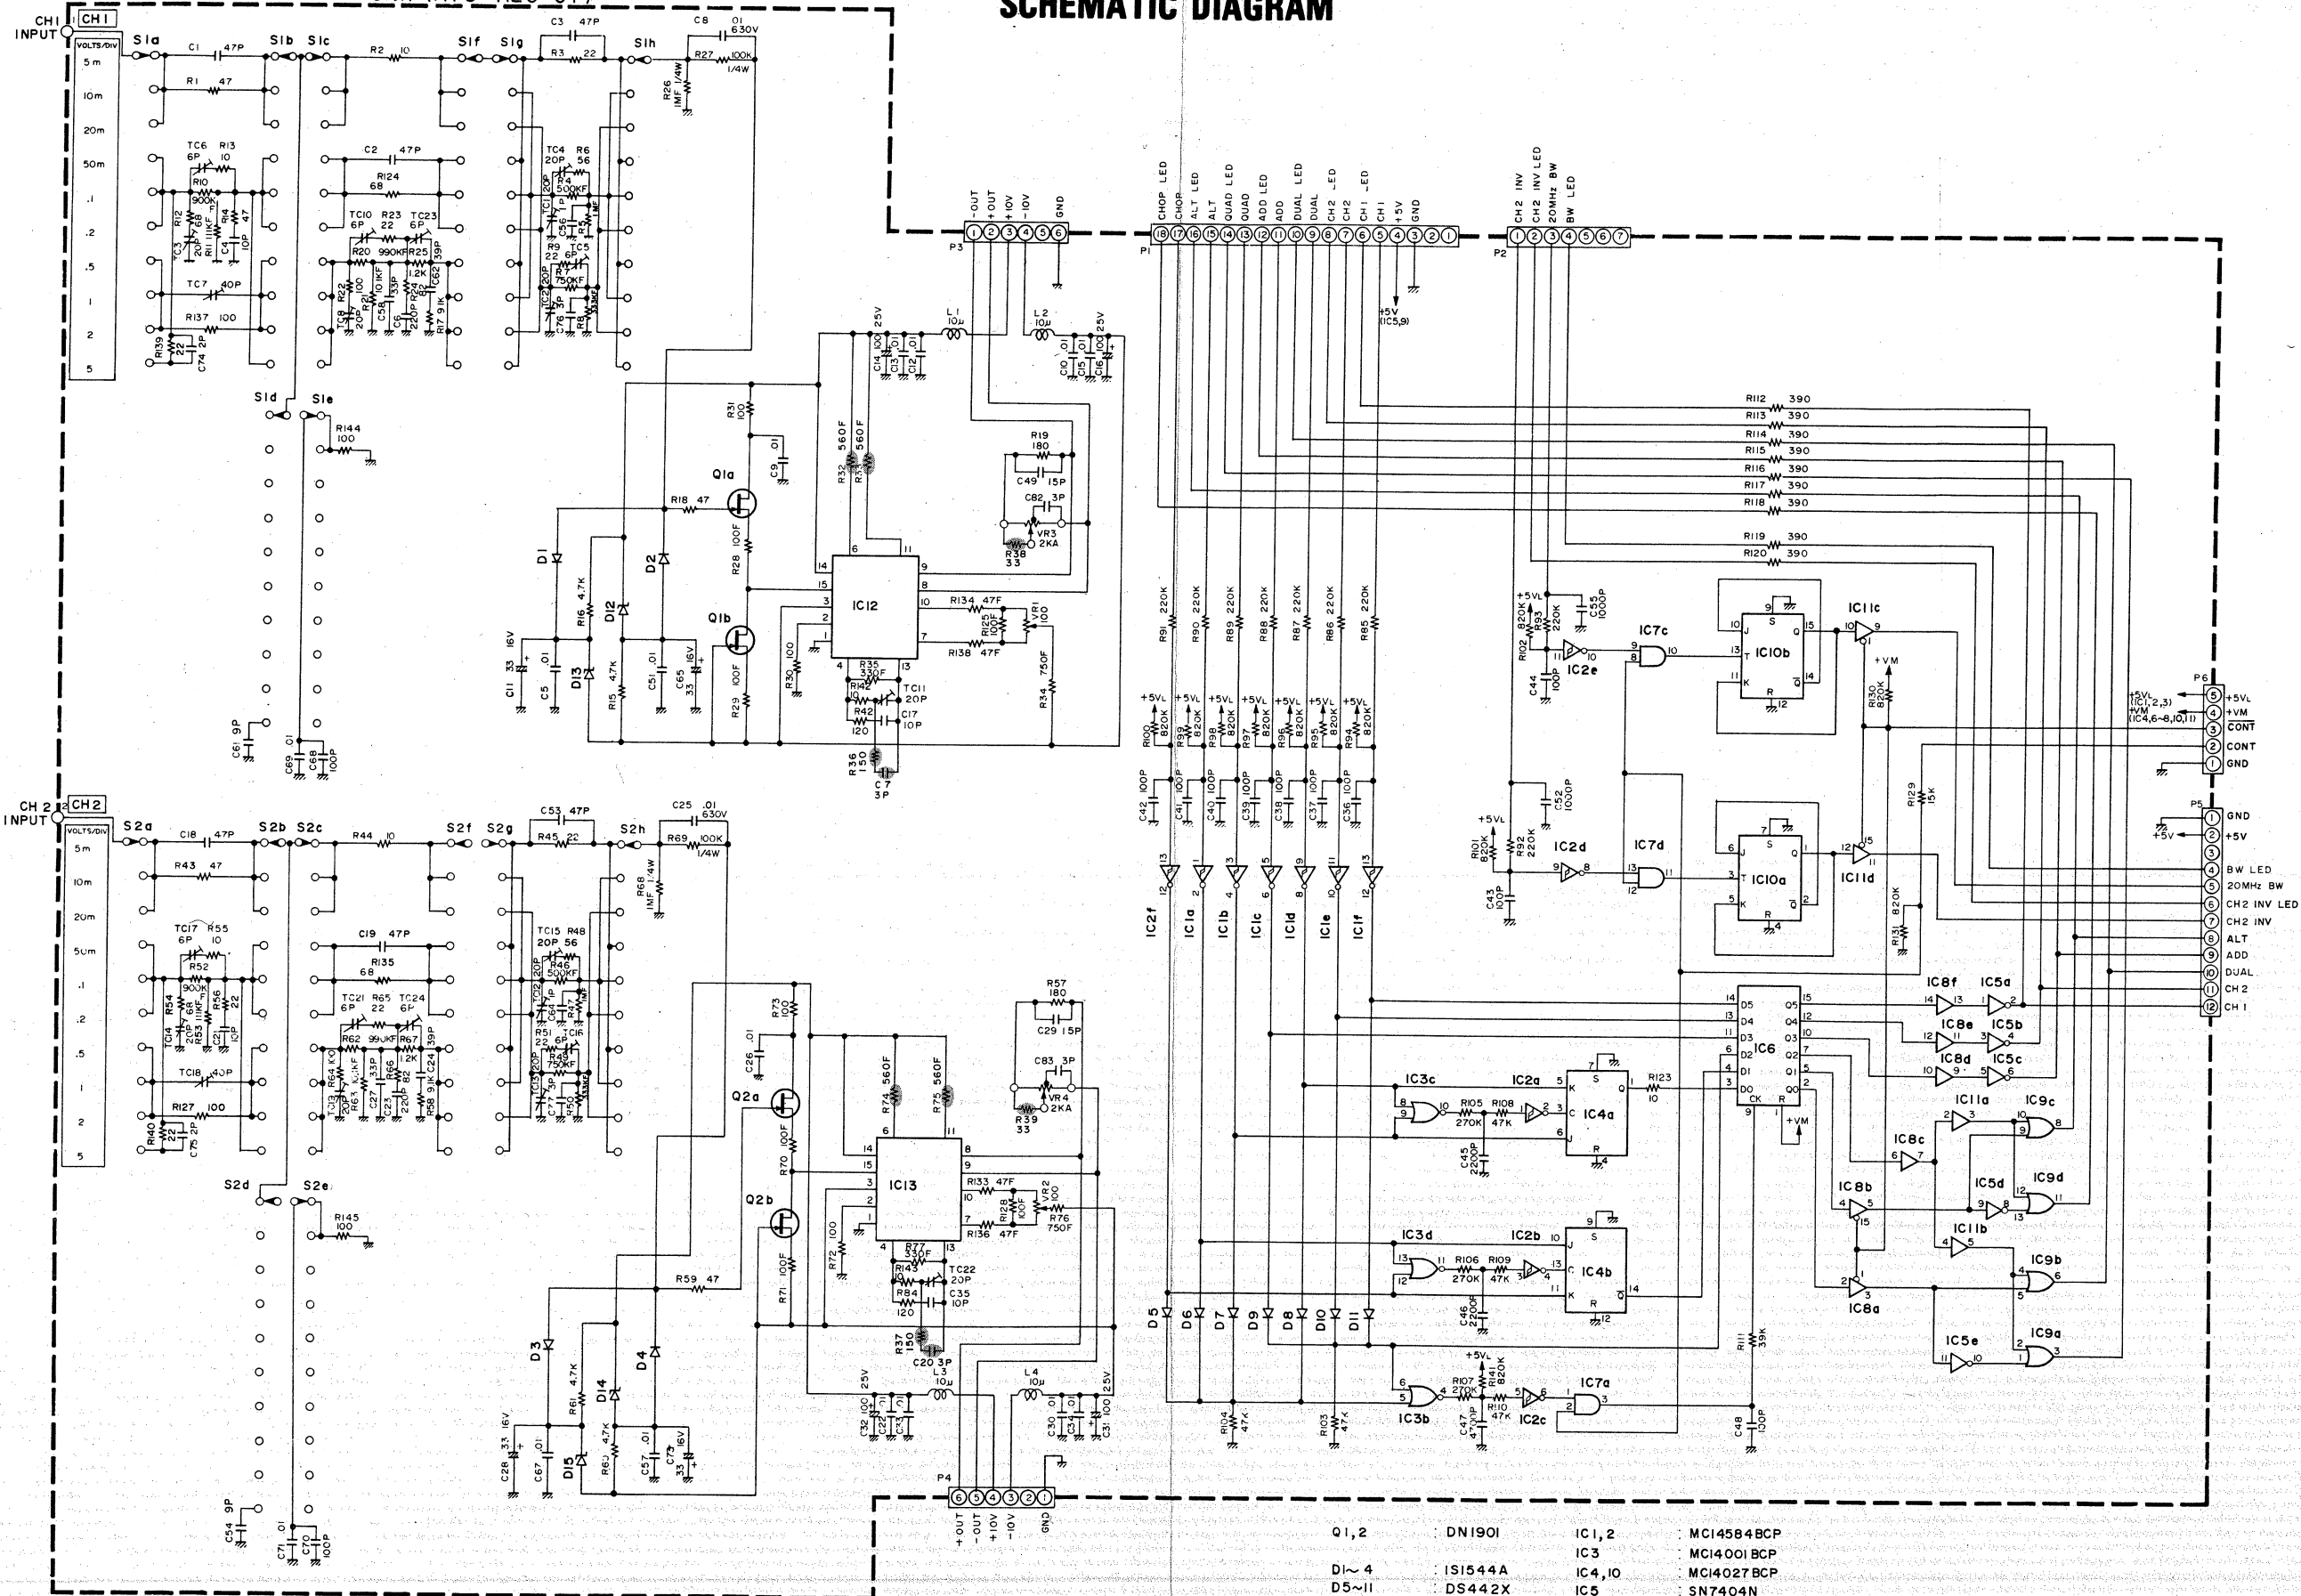


- | | | | |
|----------|---------|----------|------------|
| Q1, 2 | DN1901 | IC1, 2 | MC14584BCP |
| DI ~ 4 | 1S1544A | IC3 | MC14001BCP |
| D5 ~ 11 | DS442X | IC4, 10 | MC14027BCP |
| DI2 ~ 15 | WZ-120 | IC5 | SN7404N |
| | | IC6 | MC14174BCP |
| | | IC7 | MC14081BCP |
| | | IC8, 11 | MC14503BCP |
| | | IC9 | SN7432N |
| | | IC12, 13 | ATM-4020 |

SCHEMATIC DIAGRAM

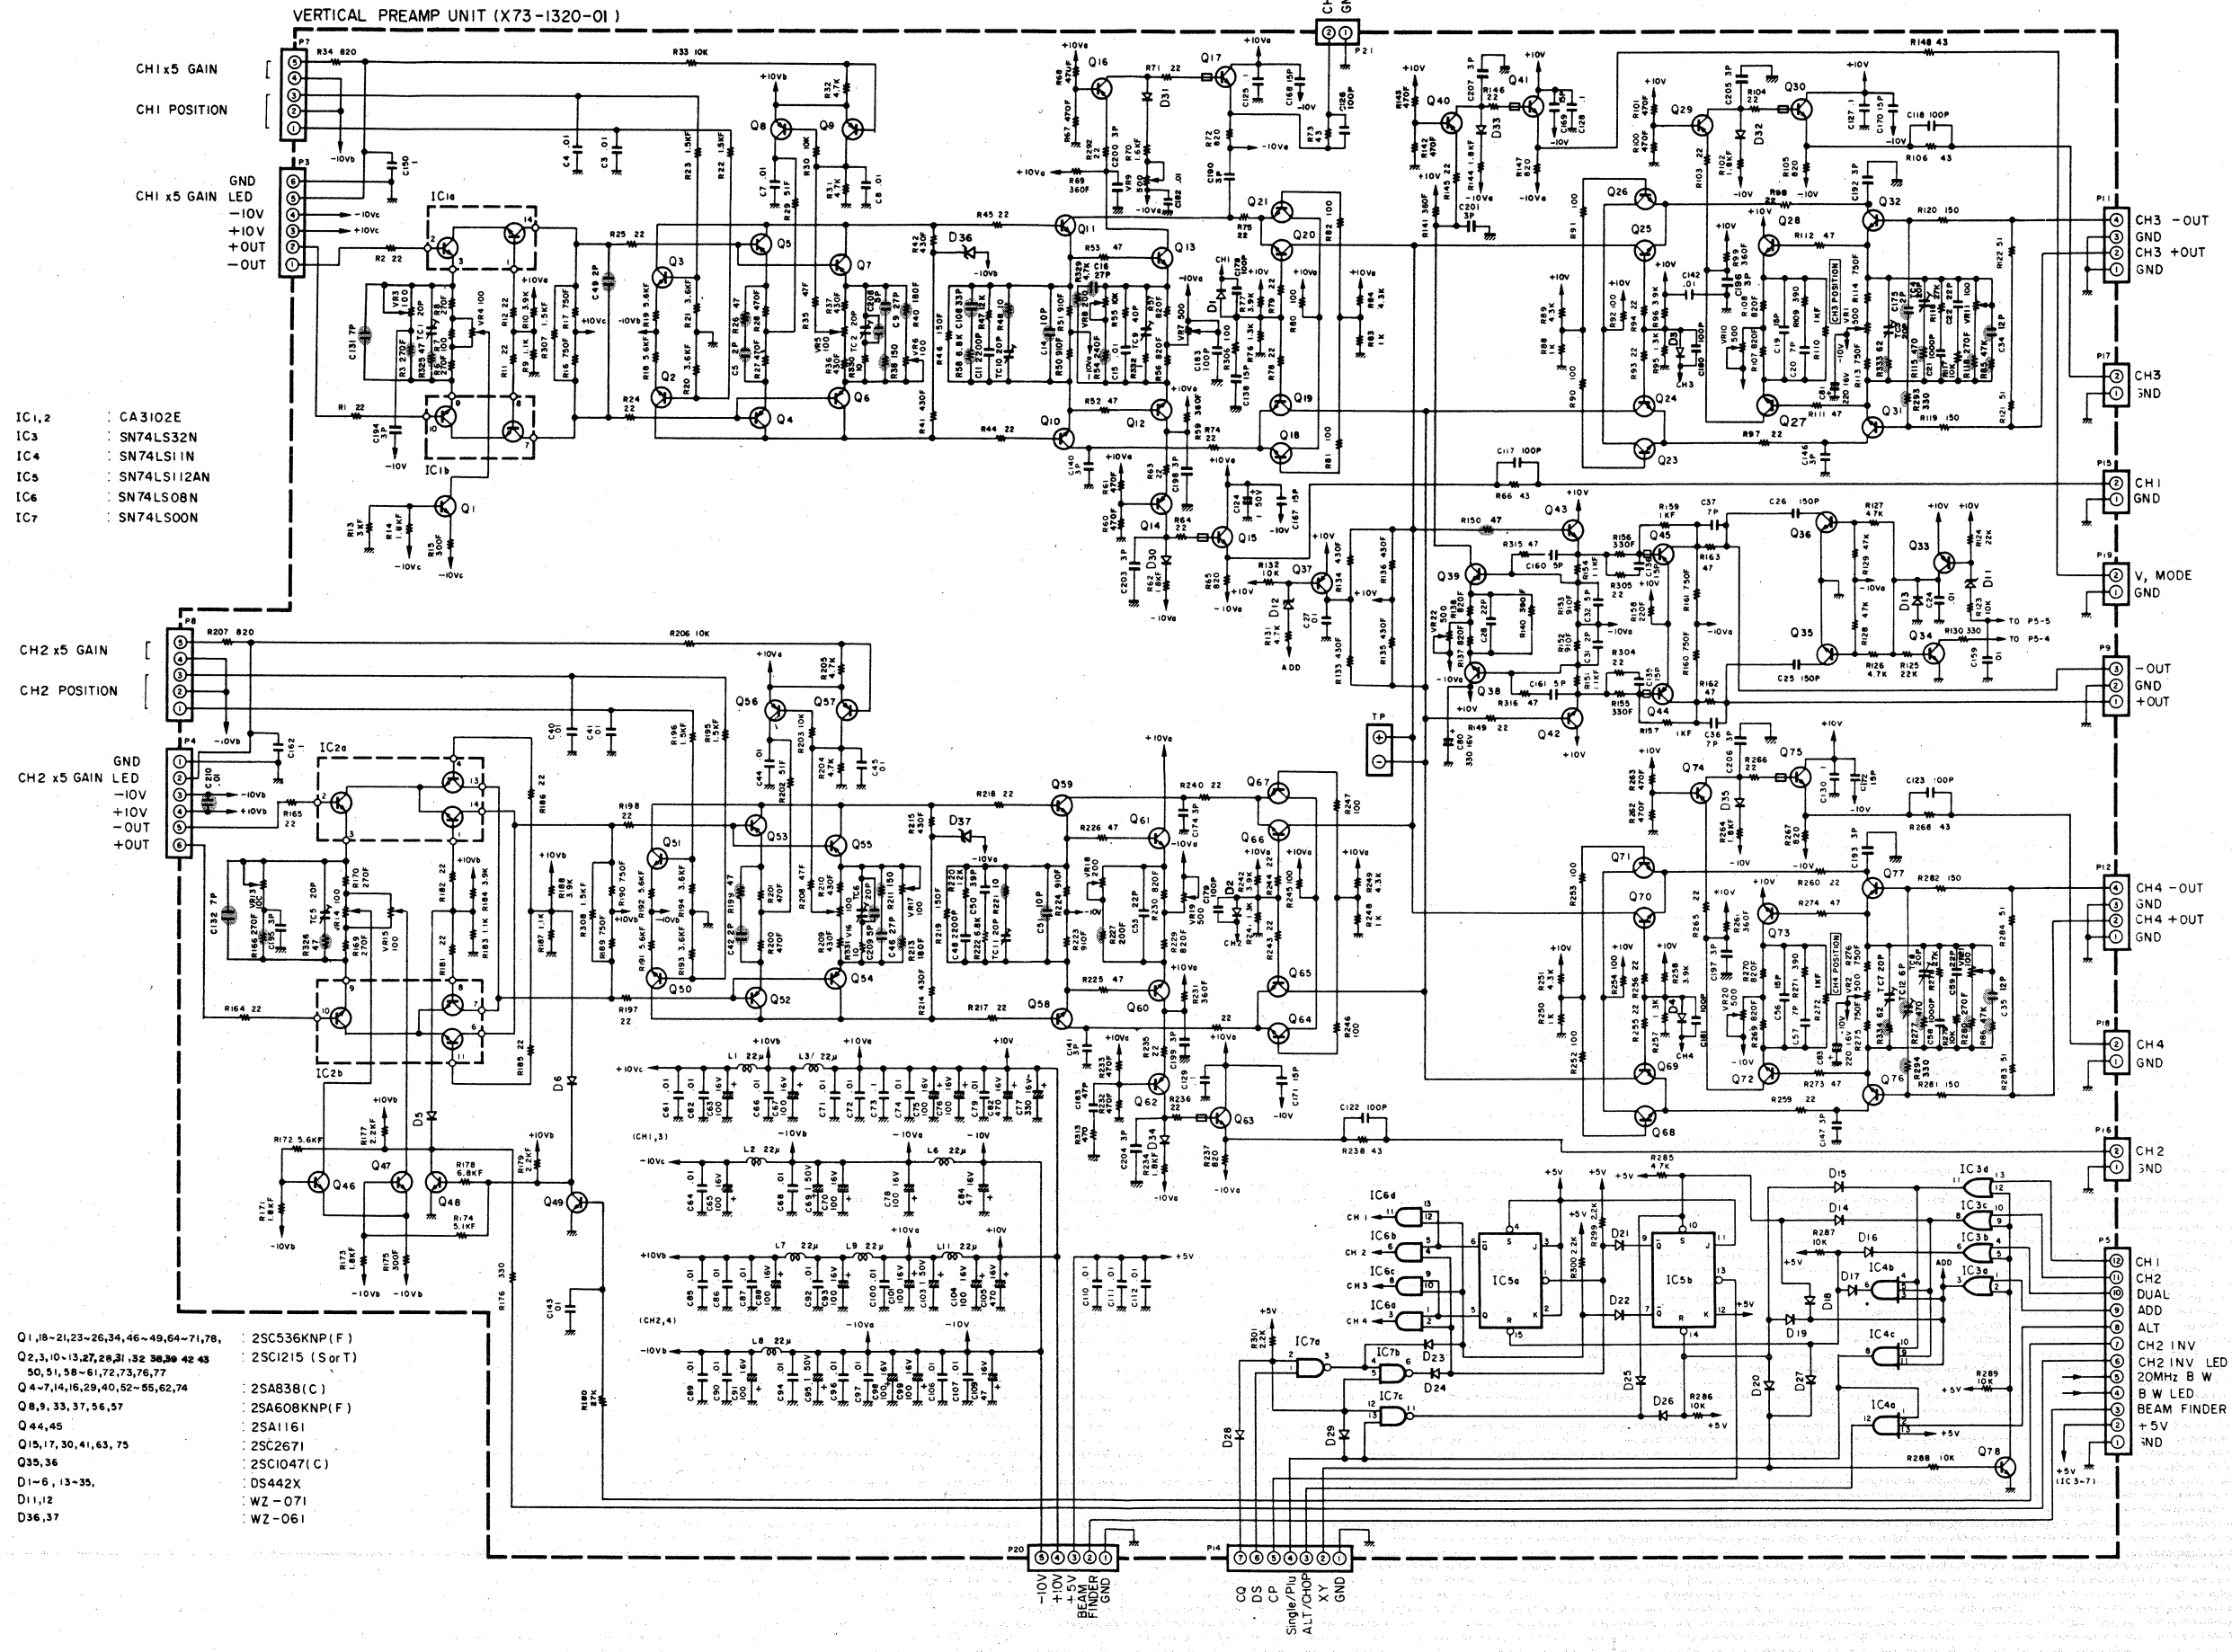


SCHEMATIC DIAGRAM

VERTICAL OUTPUT AMP UNIT (X 73-1330-01)

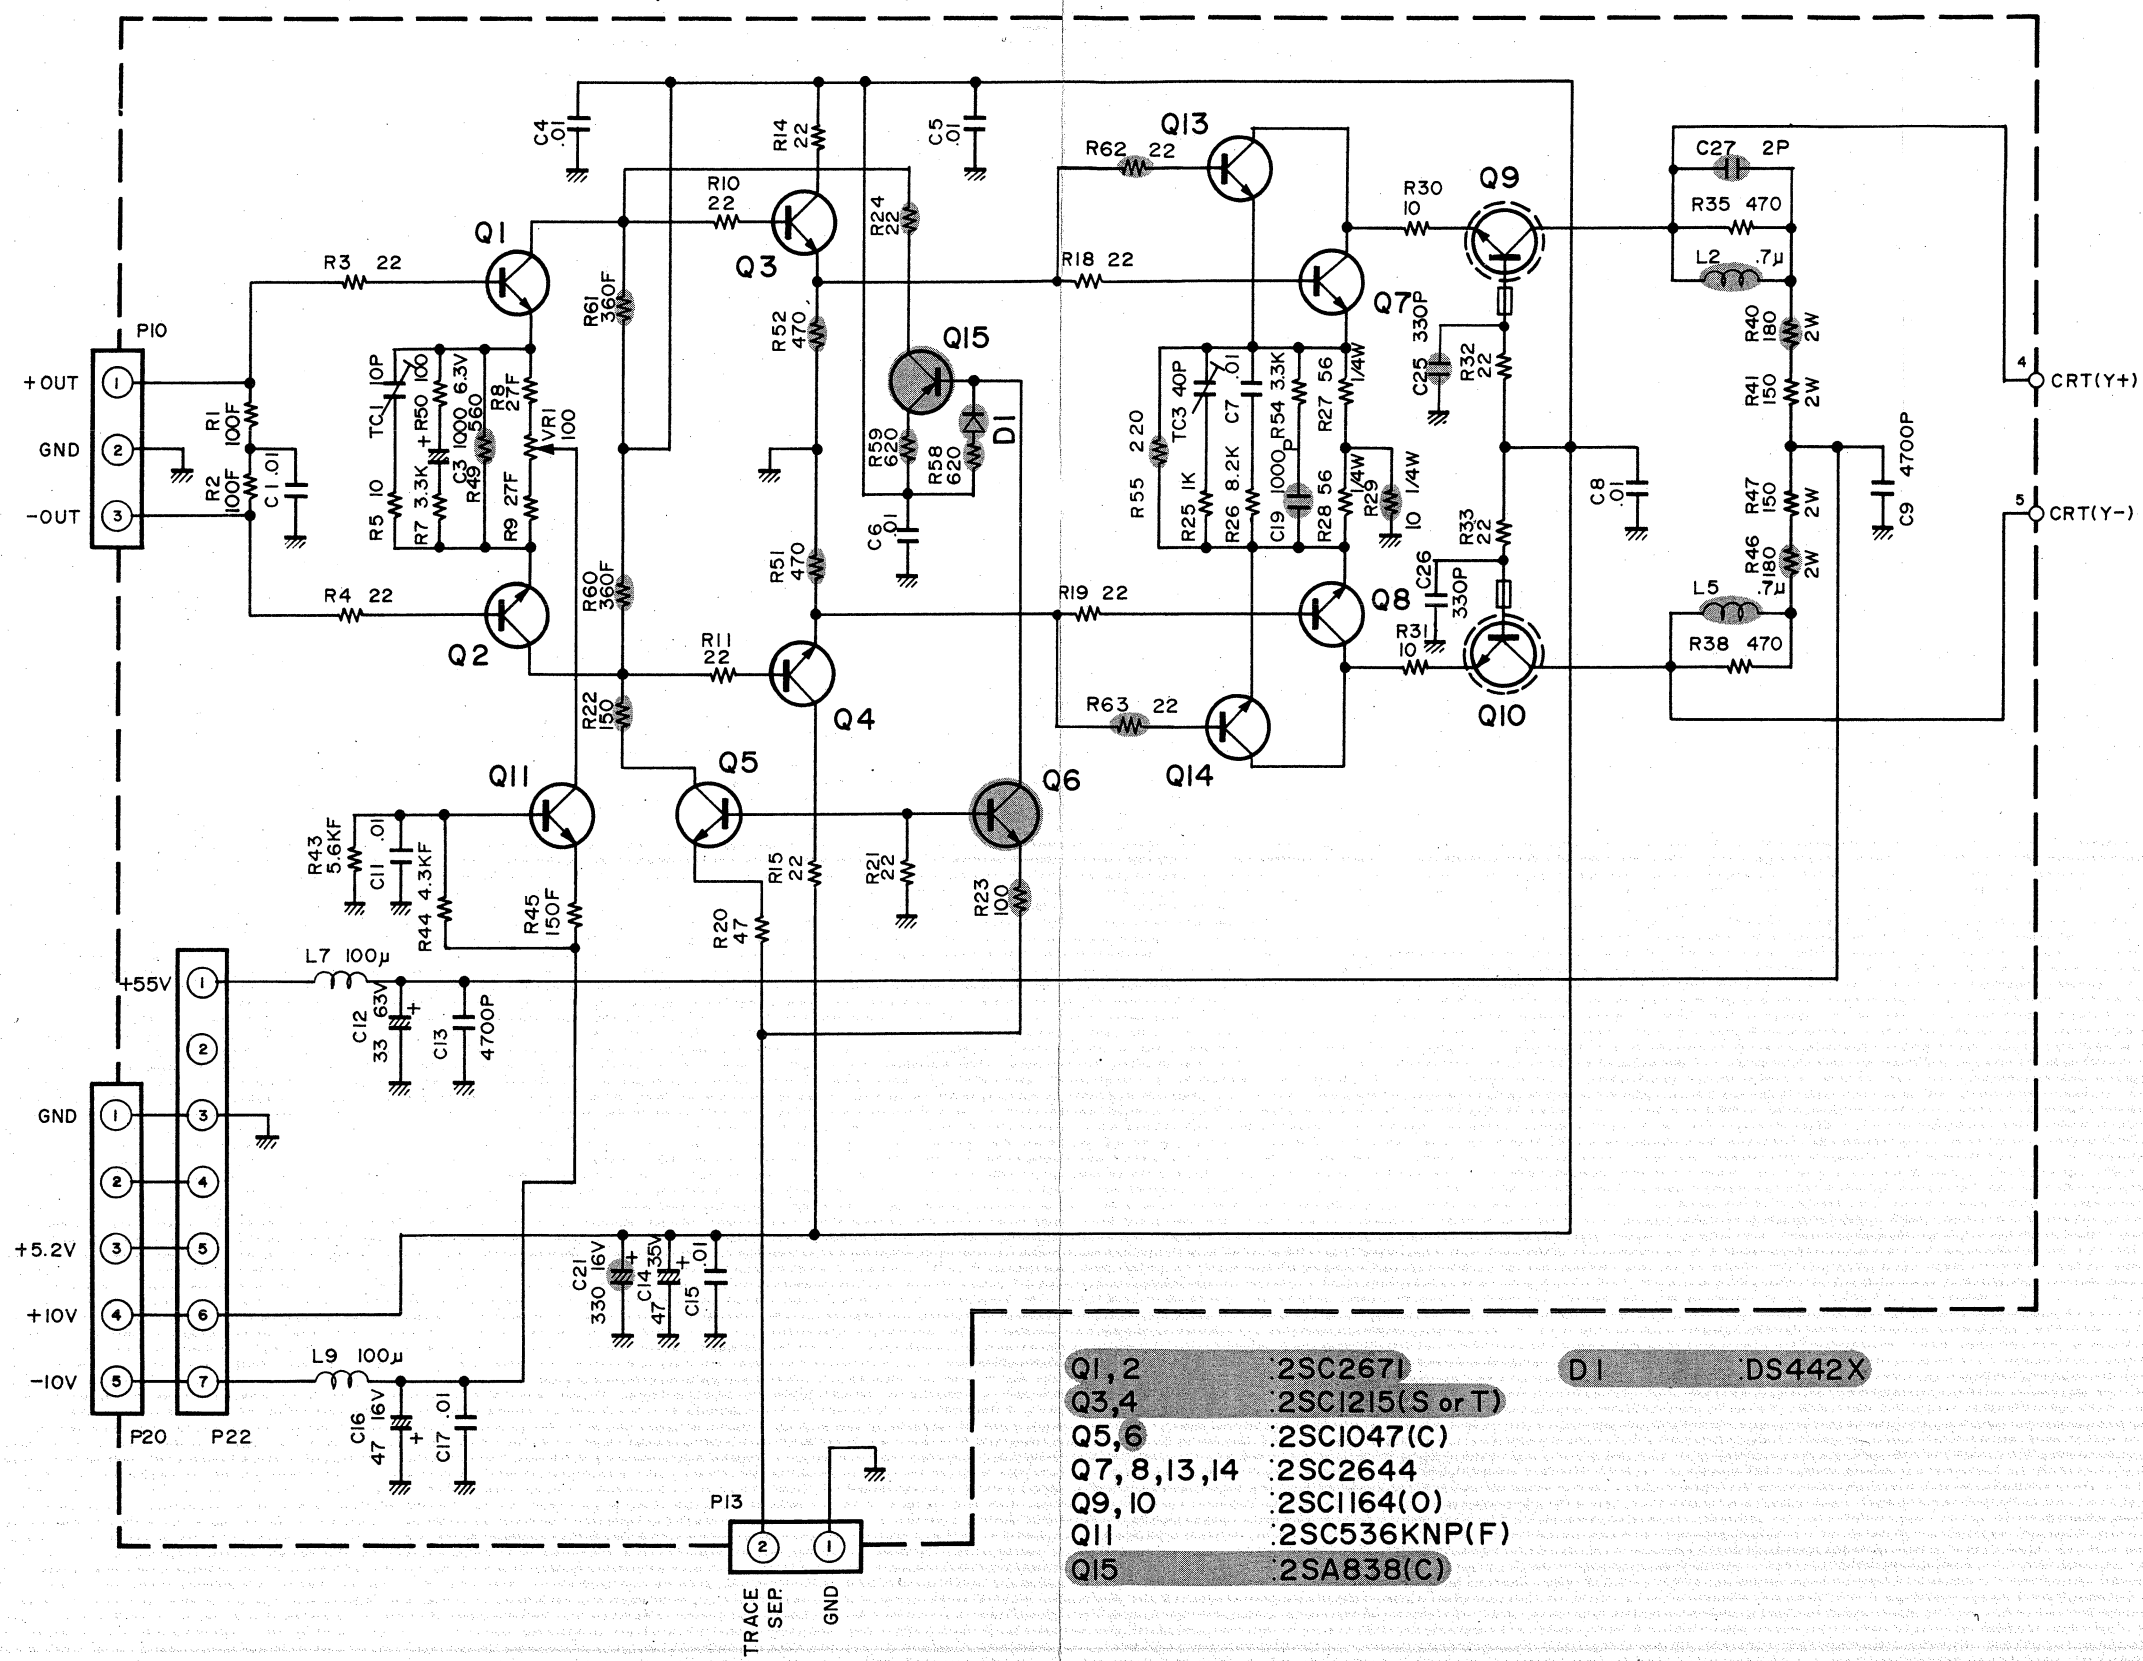

SCHEMATIC DIAGRAM

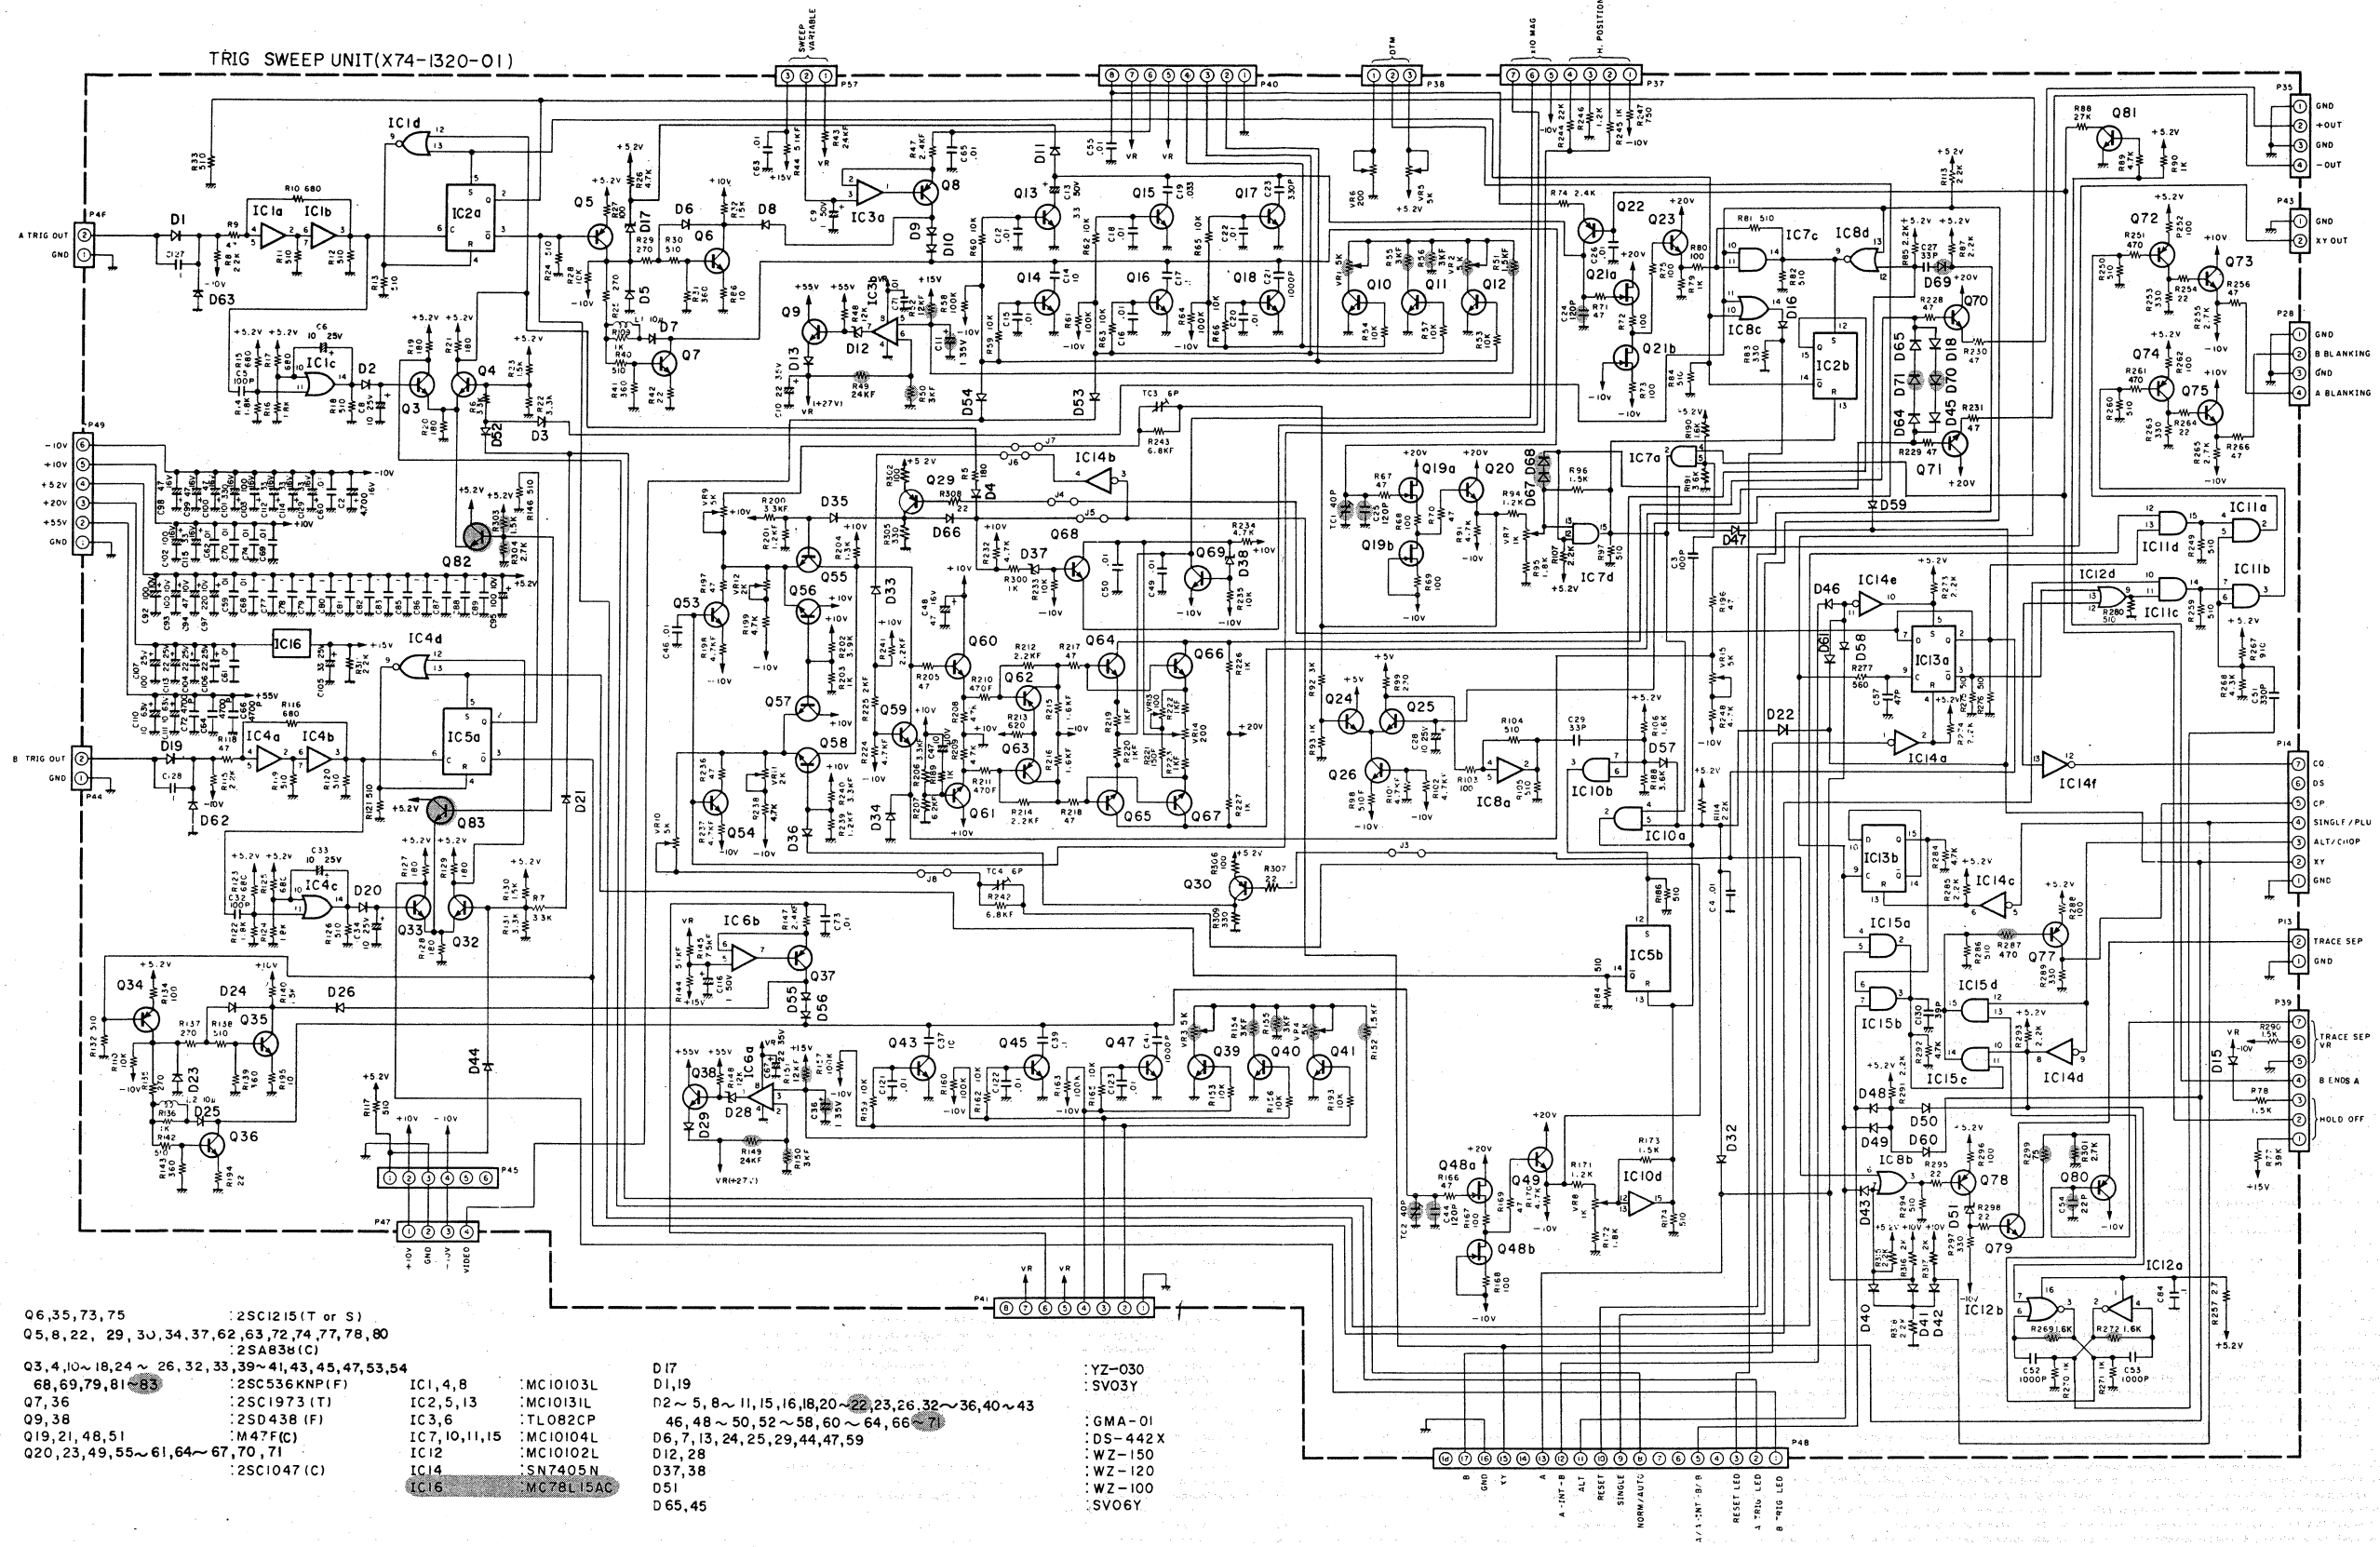


- Q6,35,73,75 :2SC1215(T or S)
- Q5,8,22, 29, 30,34,37,62,63,72,74,77,78,80 :2SA838(C)
- Q3,4,10~18,24~26,32,33,39~41,43,45,47,53,54 :2SC536KNP(F)
- 68,69,79,81~83 :2SC1973(T)
- Q7,36 :2SD438(F)
- Q9,38 :M47F(C)
- Q19,21,48,51 :2SC1047(C)
- Q20,23,49,55~61,64~67,70,71 :2SC1047(C)


- IC1, 4, 8 :MC10103L
- IC2, 5, 13 :MC10131L
- IC3, 6 :TL082CP
- IC7, 10, 11, 15 :MC10104L
- IC12 :MC10102L
- IC14 :SN7405N
- IC16 :MC78L15AC

- D17 :YZ-030
- D1,19 :SV03Y
- D2~5, 8~11, 15, 16, 18, 20~22, 23, 26, 32~36, 40~43 :GMA-01
- 46, 48~50, 52~58, 60~64, 66~71 :DS-442X
- D6, 7, 13, 24, 25, 29, 44, 47, 59 :WZ-150
- D12, 28 :WZ-120
- D37, 38 :WZ-100
- D51 :SV06Y
- D65, 45


SCHEMATIC DIAGRAM

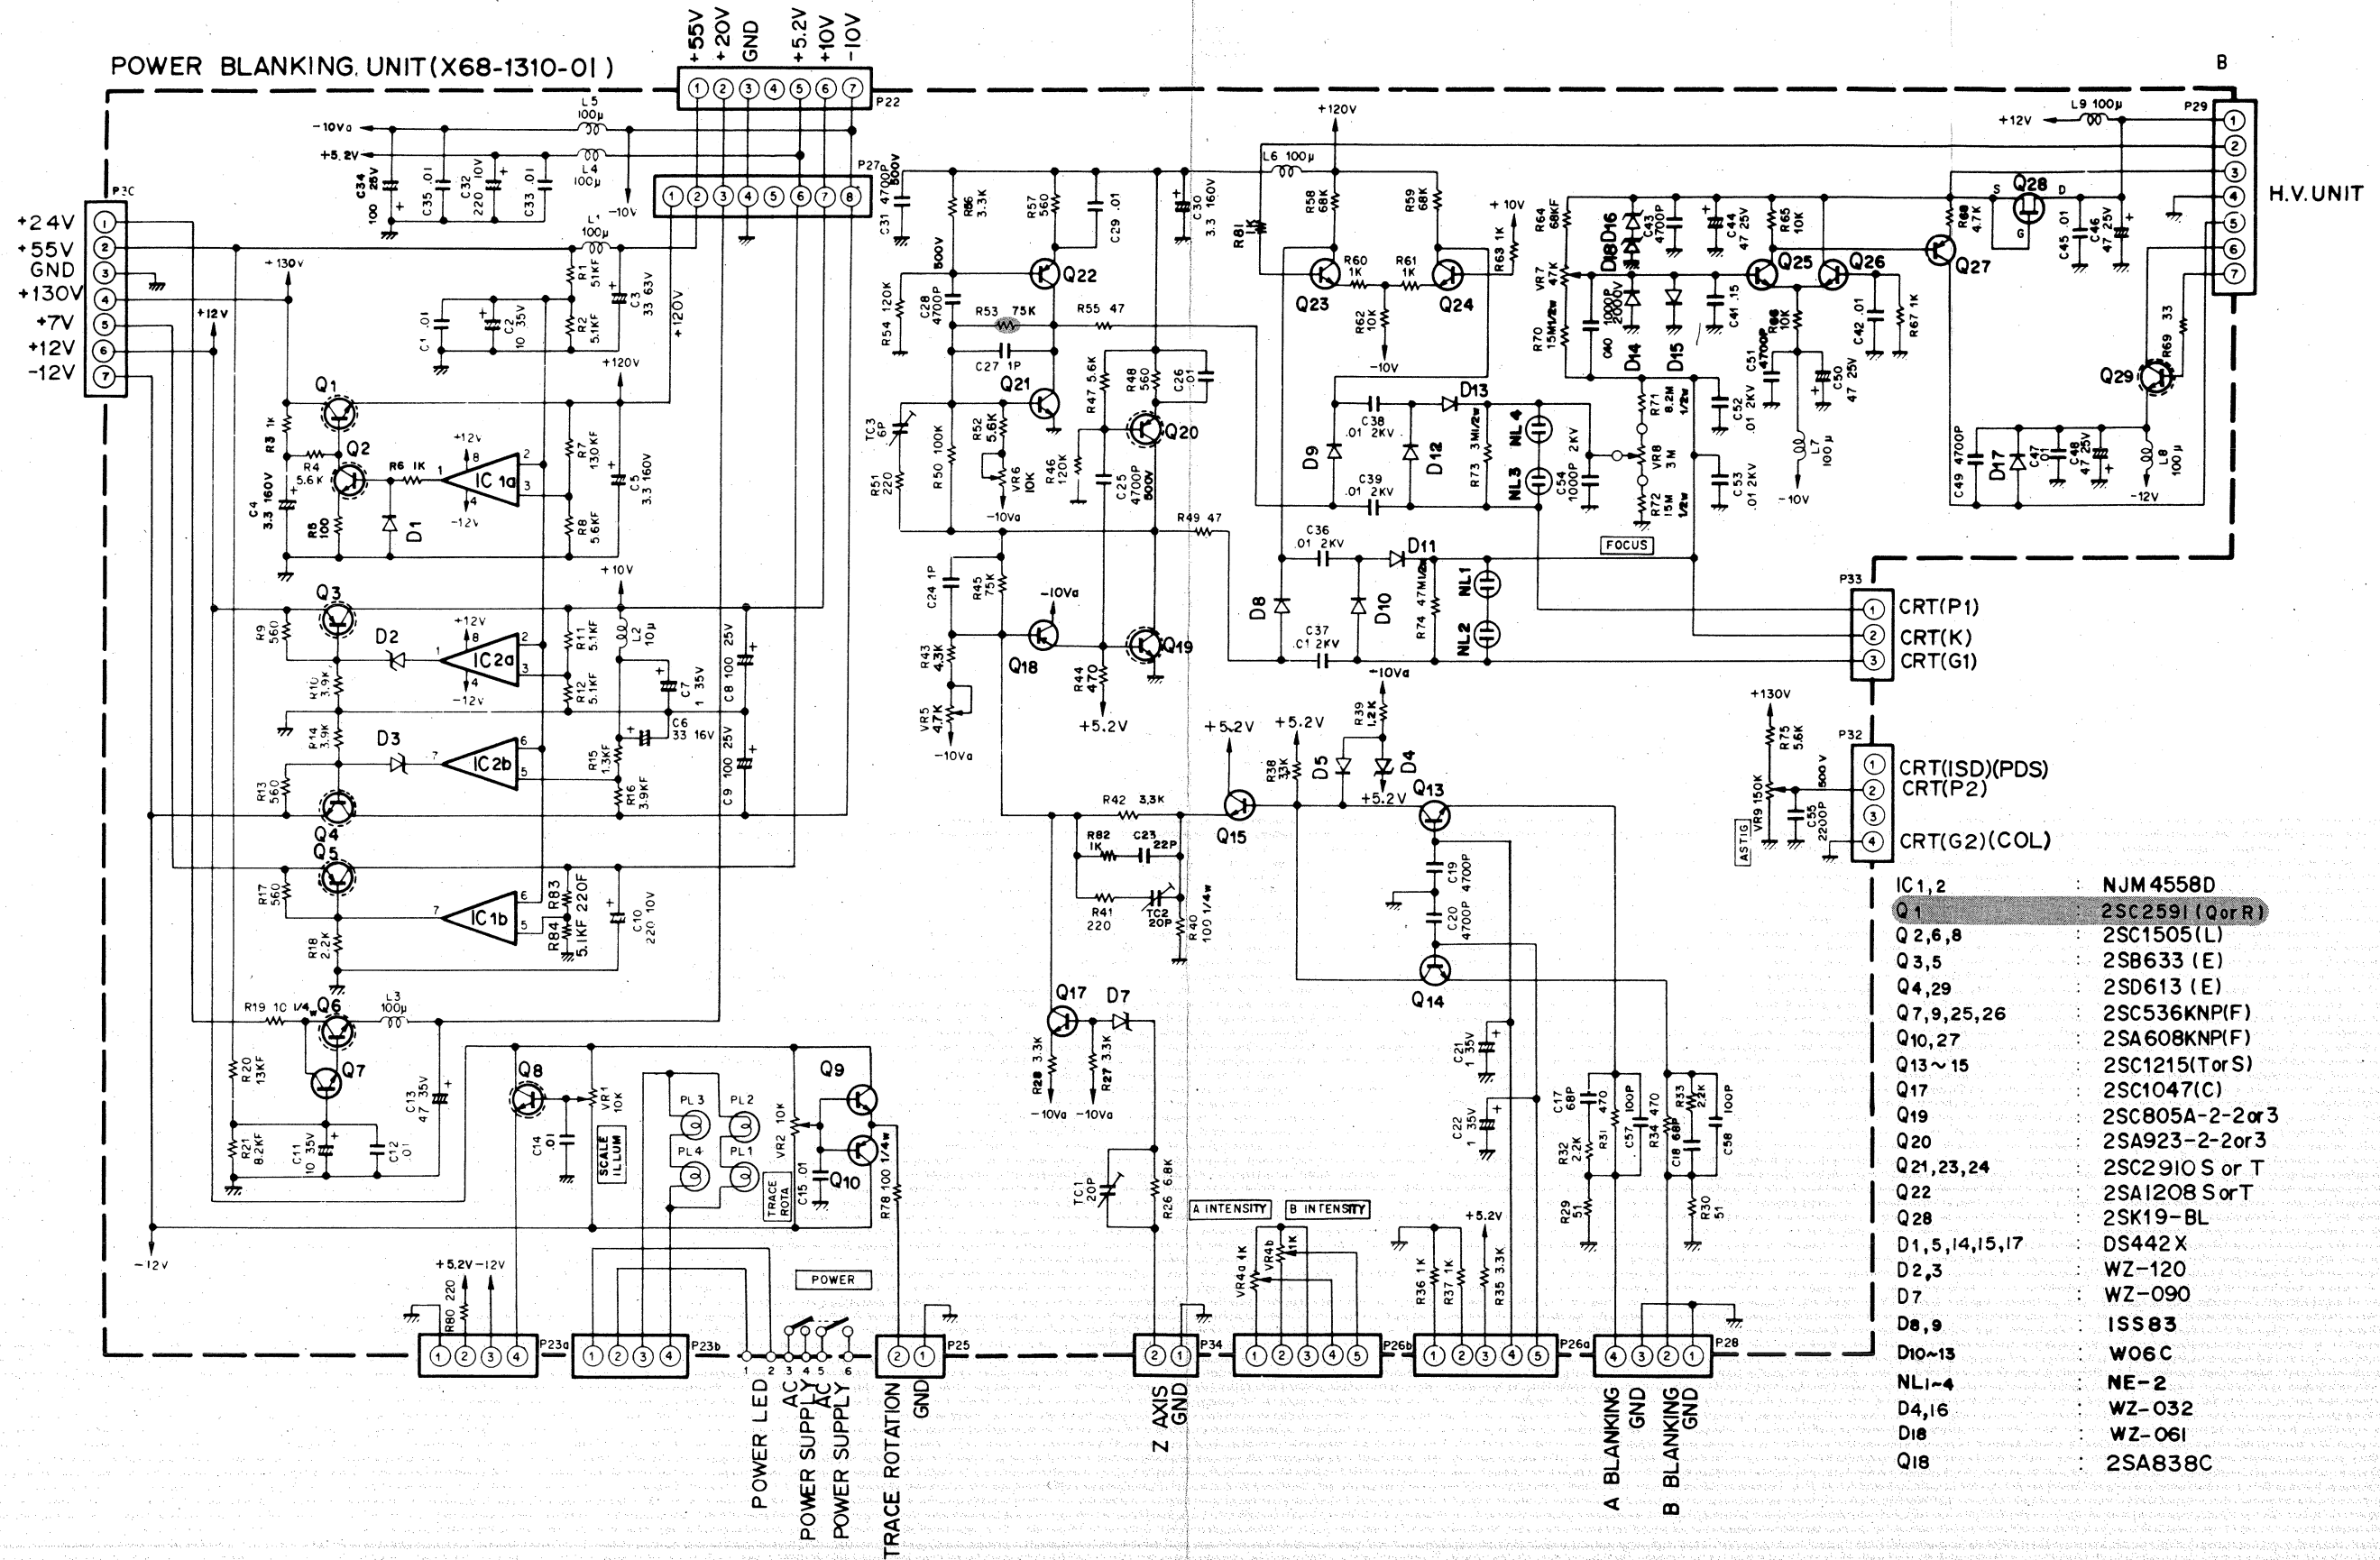

- | | |
|--------------------|-------------------|
| IC 1, 2 | : NJM 4558D |
| Q 1 | : 2SC2591 (Qor R) |
| Q 2, 6, 8 | : 2SC1505 (L) |
| Q 3, 5 | : 2SB633 (E) |
| Q 4, 29 | : 2SD613 (E) |
| Q 7, 9, 25, 26 | : 2SC536KNPI(F) |
| Q 10, 27 | : 2SA608KNPI(F) |
| Q 13 ~ 15 | : 2SC1215 (Tor S) |
| Q 17 | : 2SC1047 (C) |
| Q 19 | : 2SC805A-2-2or3 |
| Q 20 | : 2SA923-2-2or3 |
| Q 21, 23, 24 | : 2SC2910 S or T |
| Q 22 | : 2SA1208 S or T |
| Q 28 | : 2SK19-BL |
| D 1, 5, 14, 15, 17 | : DS442 X |
| D 2, 3 | : WZ-120 |
| D 7 | : WZ-090 |
| D 8, 9 | : ISS 83 |
| D 10 ~ 13 | : W06C |
| NL 1-4 | : NE-2 |
| D 4, 16 | : WZ-032 |
| D 18 | : WZ-061 |
| Q 18 | : 2SA838C |

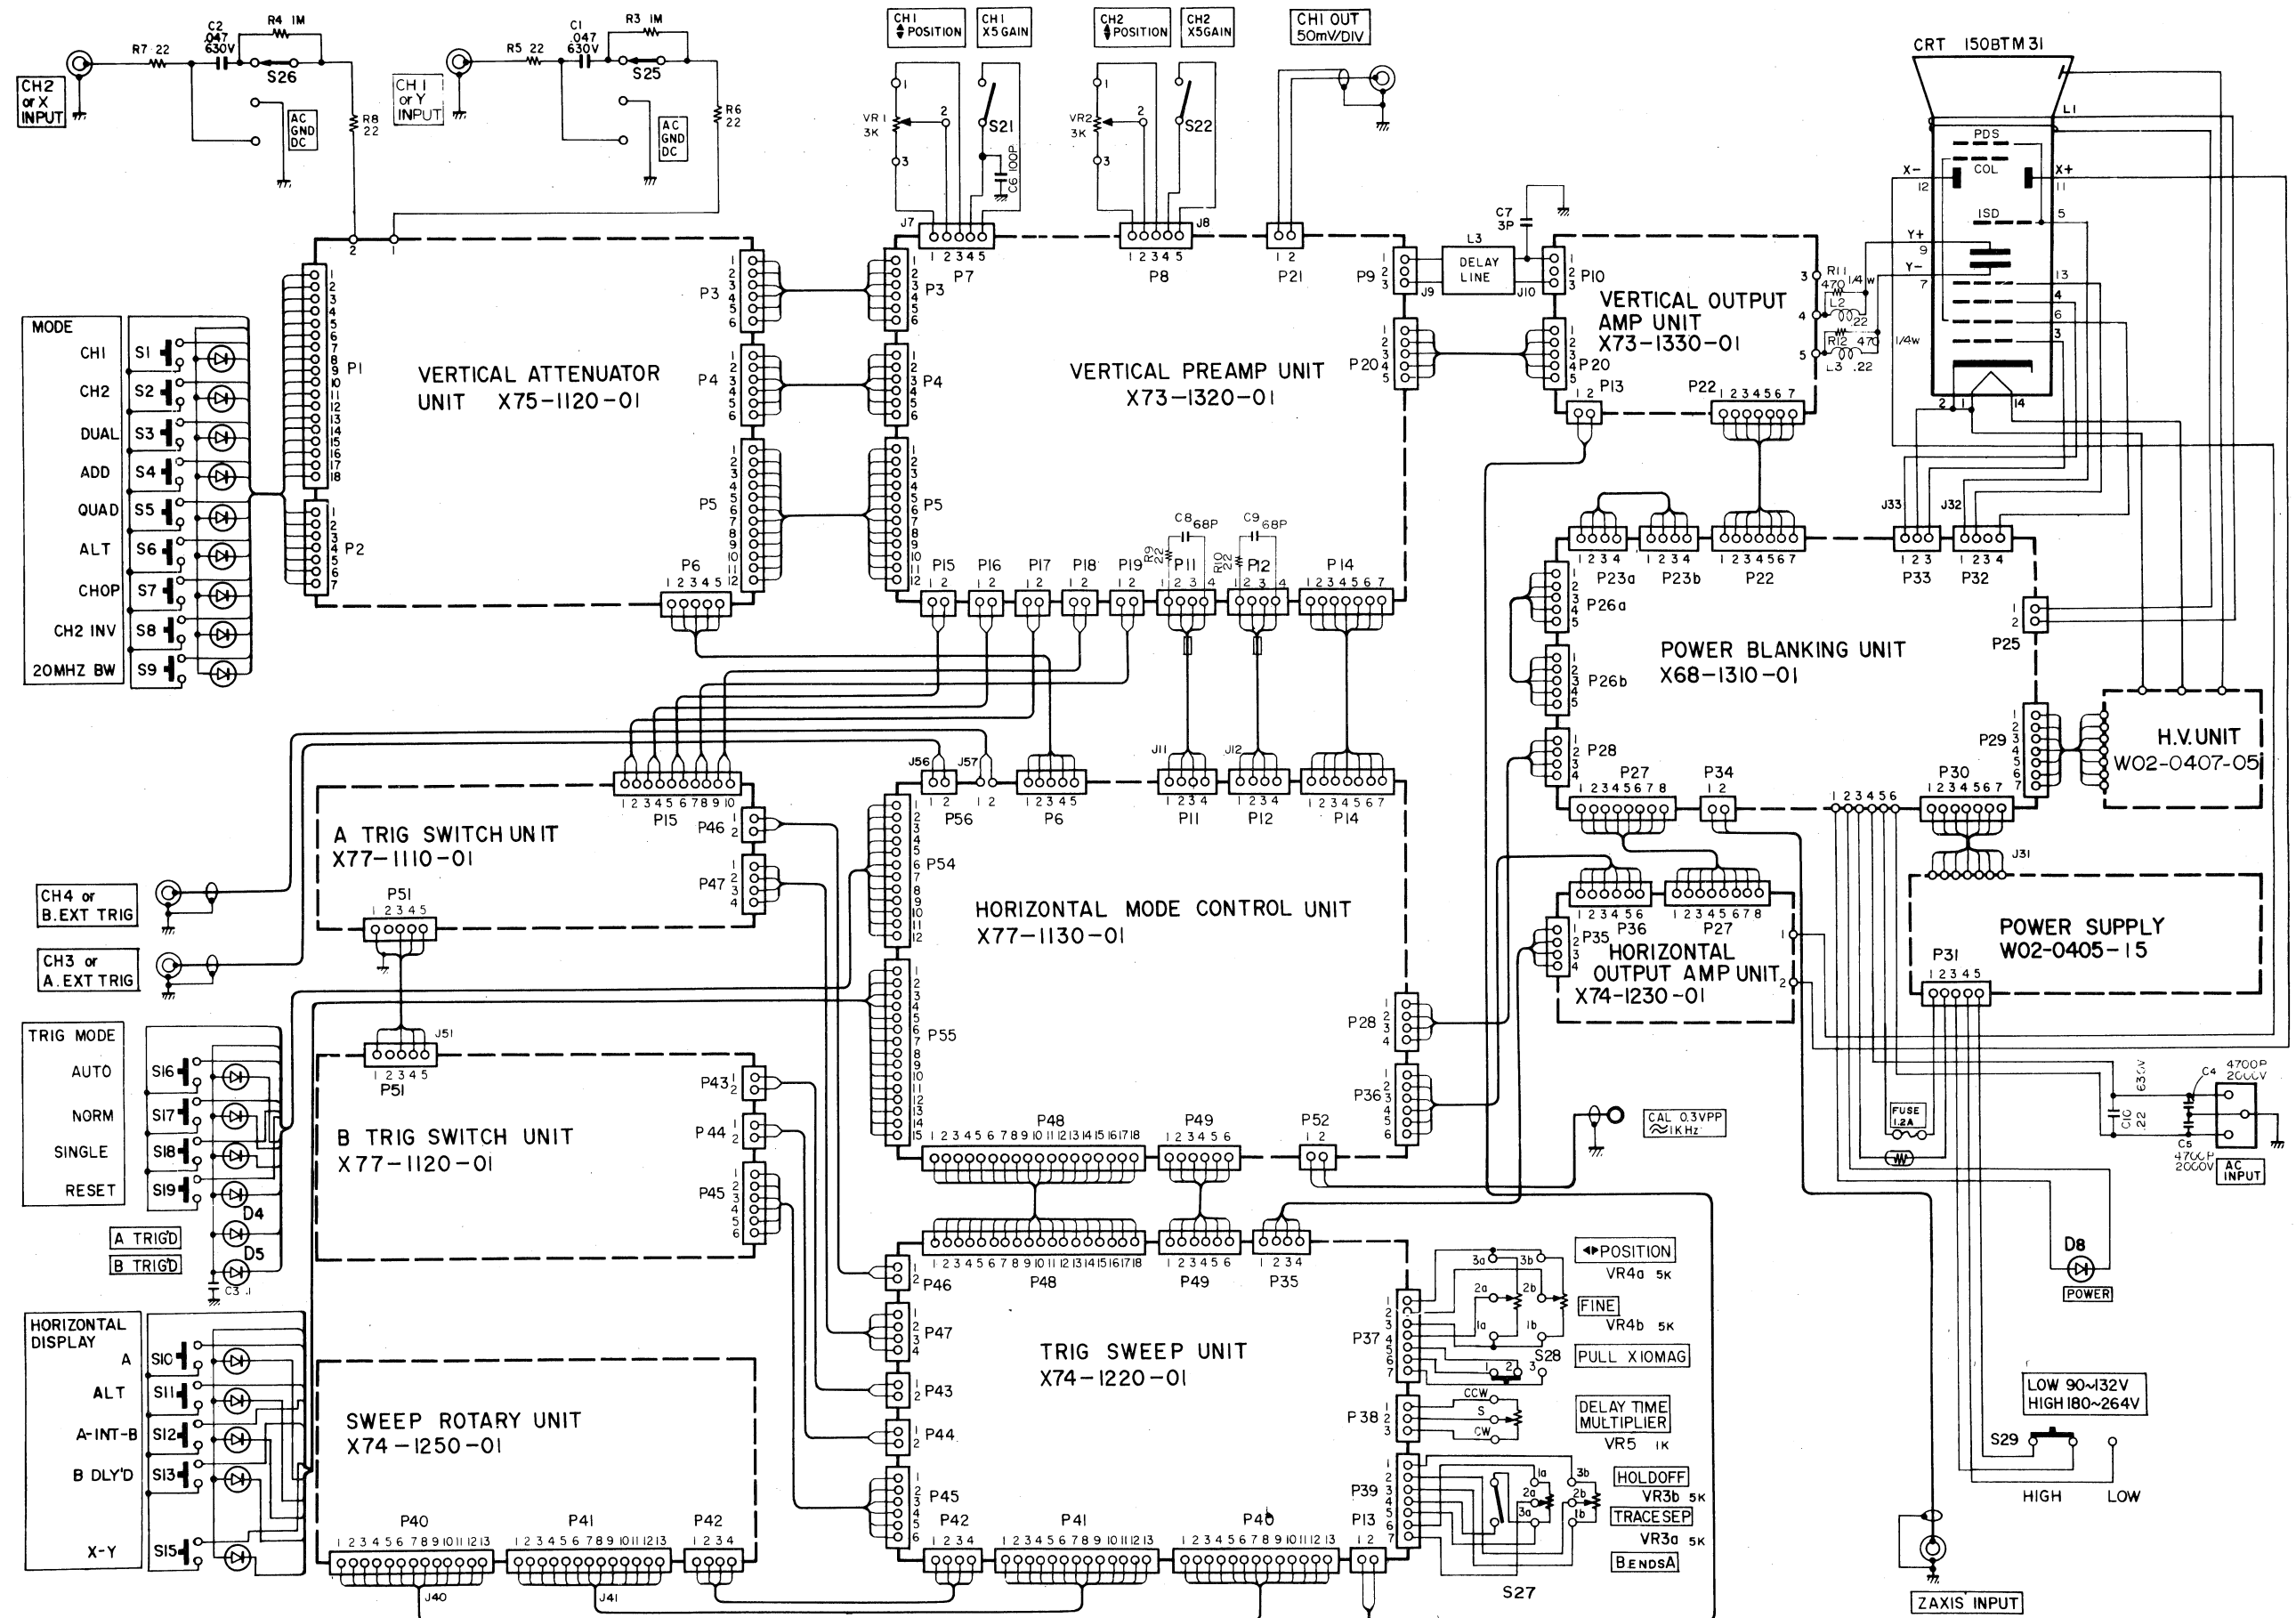


VERTICAL ATTENUATOR UNIT (X75-1120-01)

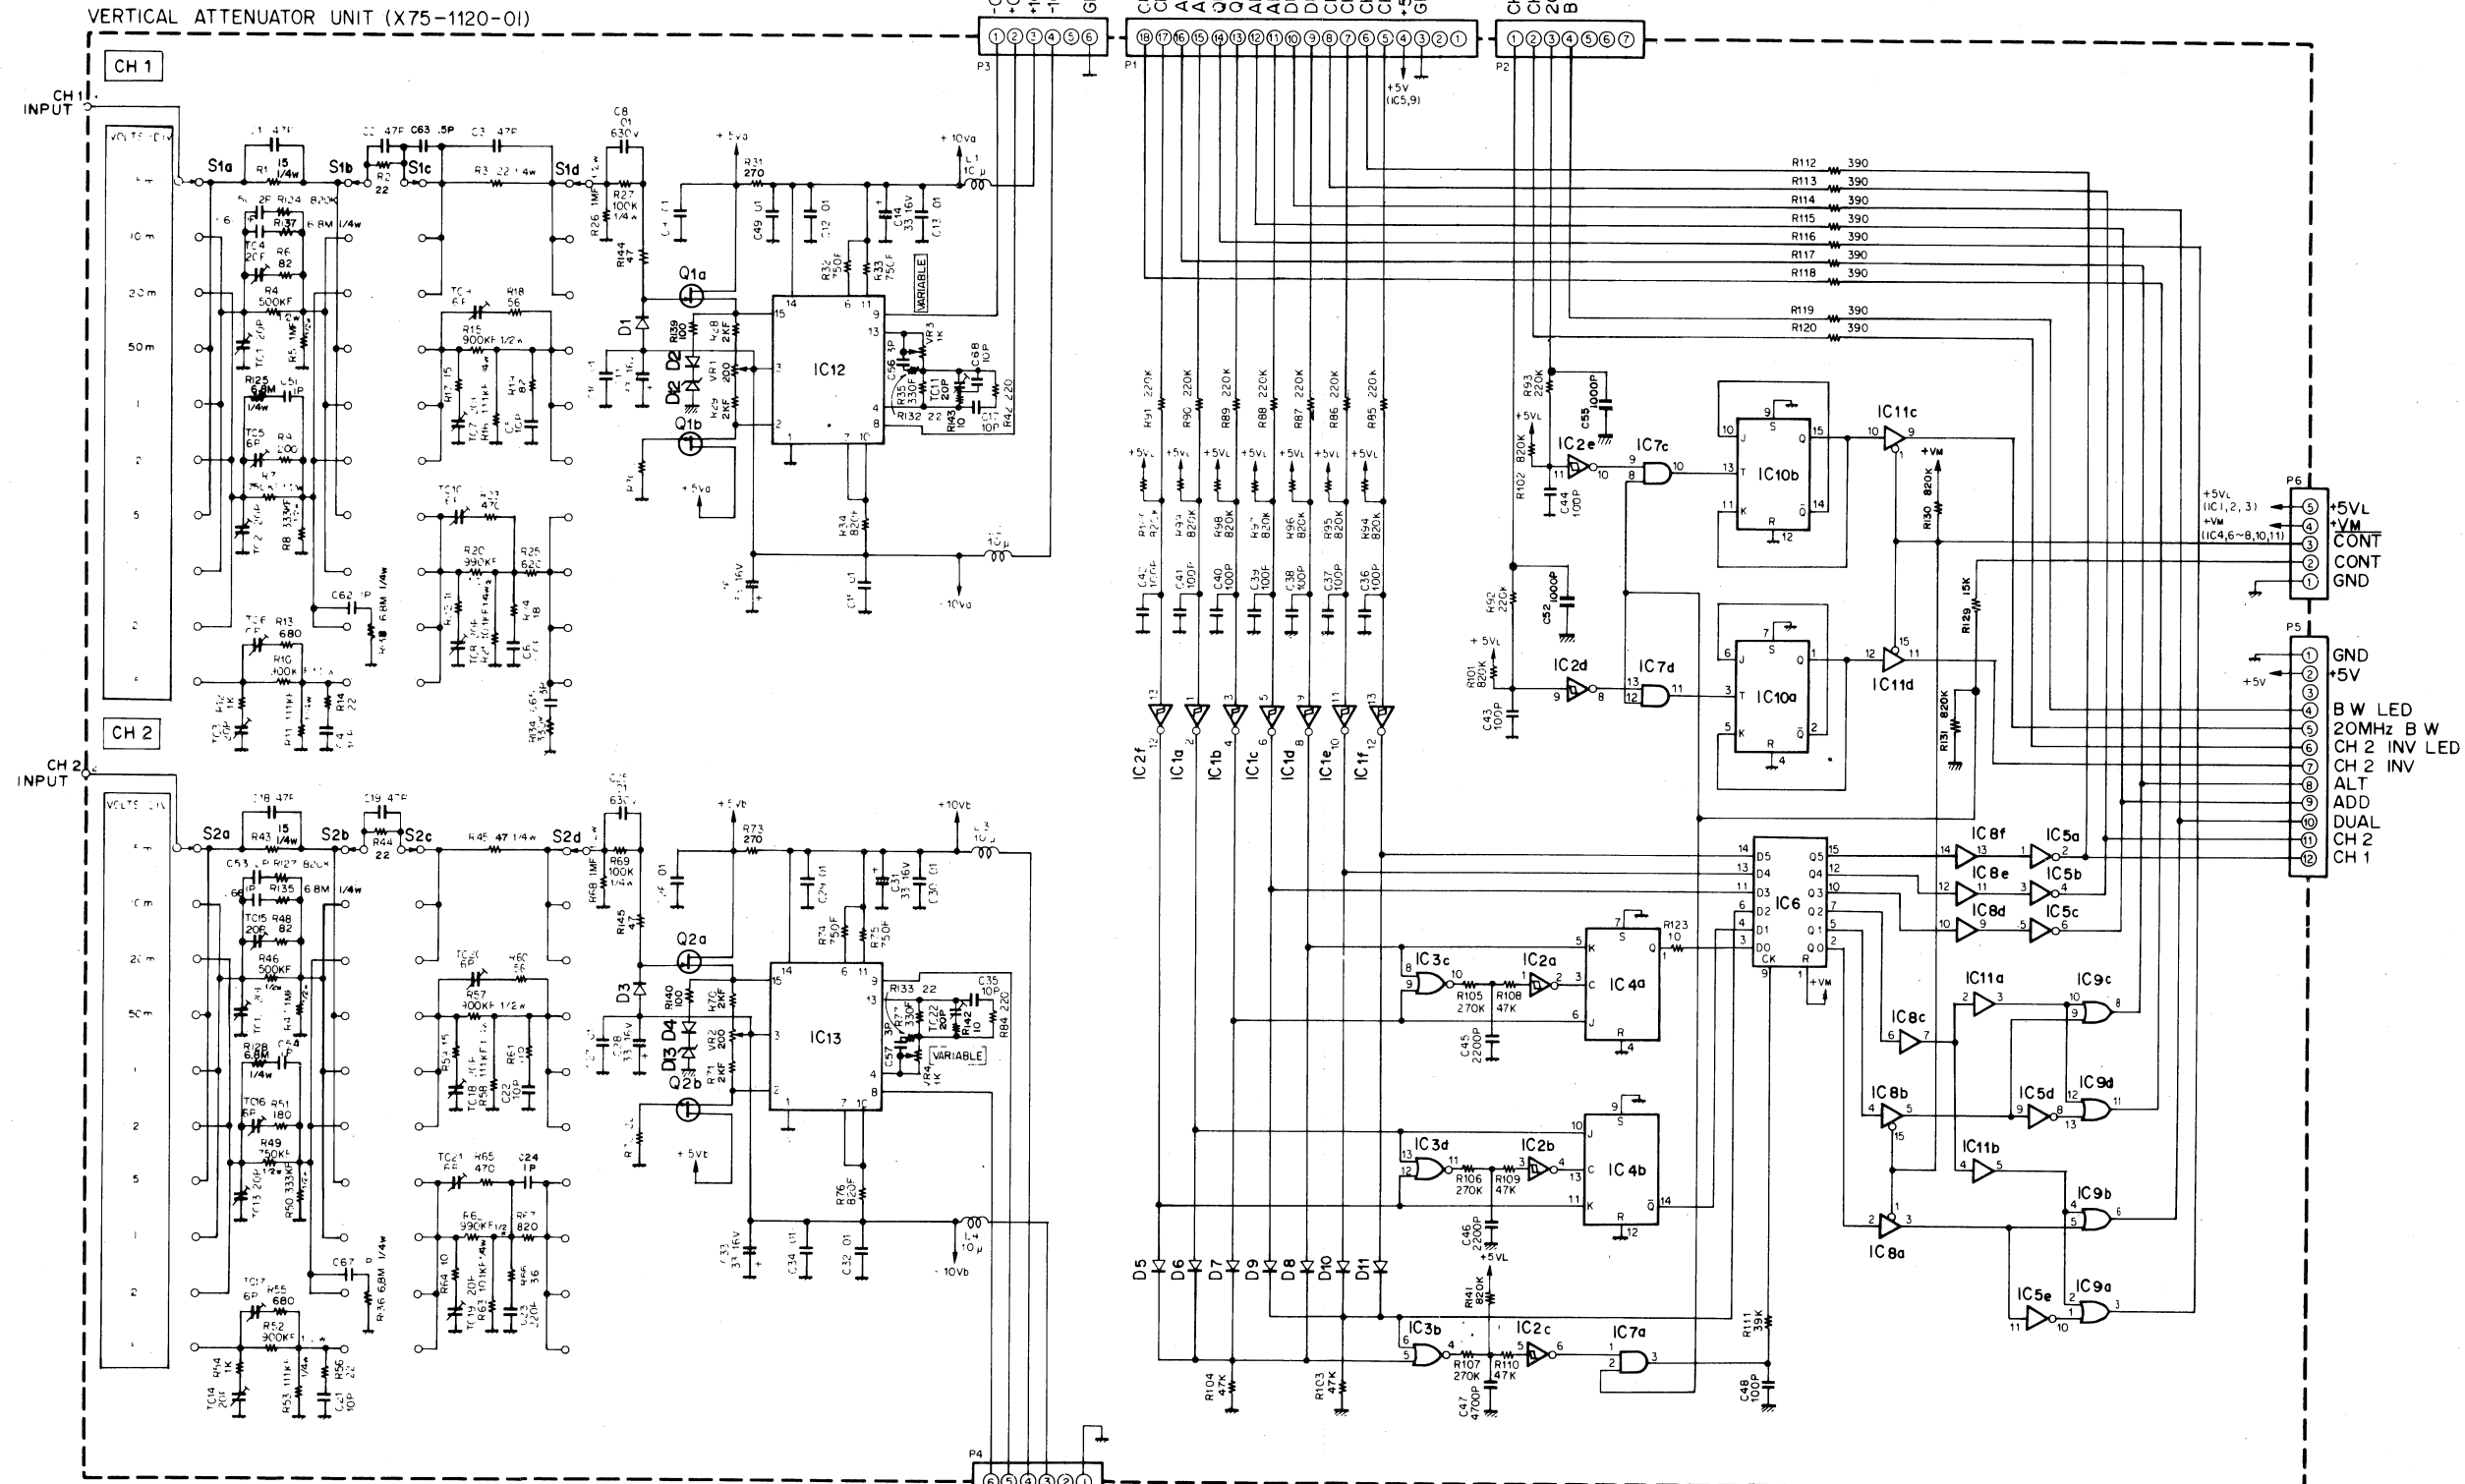


- | | | | |
|-----------|------------------|---------|--------------|
| Q1,2 | : DNI90I or U440 | IC4,10 | : MC14027BPC |
| D1,3 | : 1S1544A | IC5 | : SN7404N |
| D5-11,2,4 | : DS442X | IC6 | : MC14174BPC |
| D12,13 | : YZ-030 | IC7 | : MC14081BPC |
| IC1,2 | : MC14584BPC | IC8,11 | : MC14503BPC |
| IC3 | : MC14001BPC | IC9 | : SN7432N |
| | | IC12,13 | : ATM-4010 |

VERTICAL PREAMP UNIT (X73-1320-01)

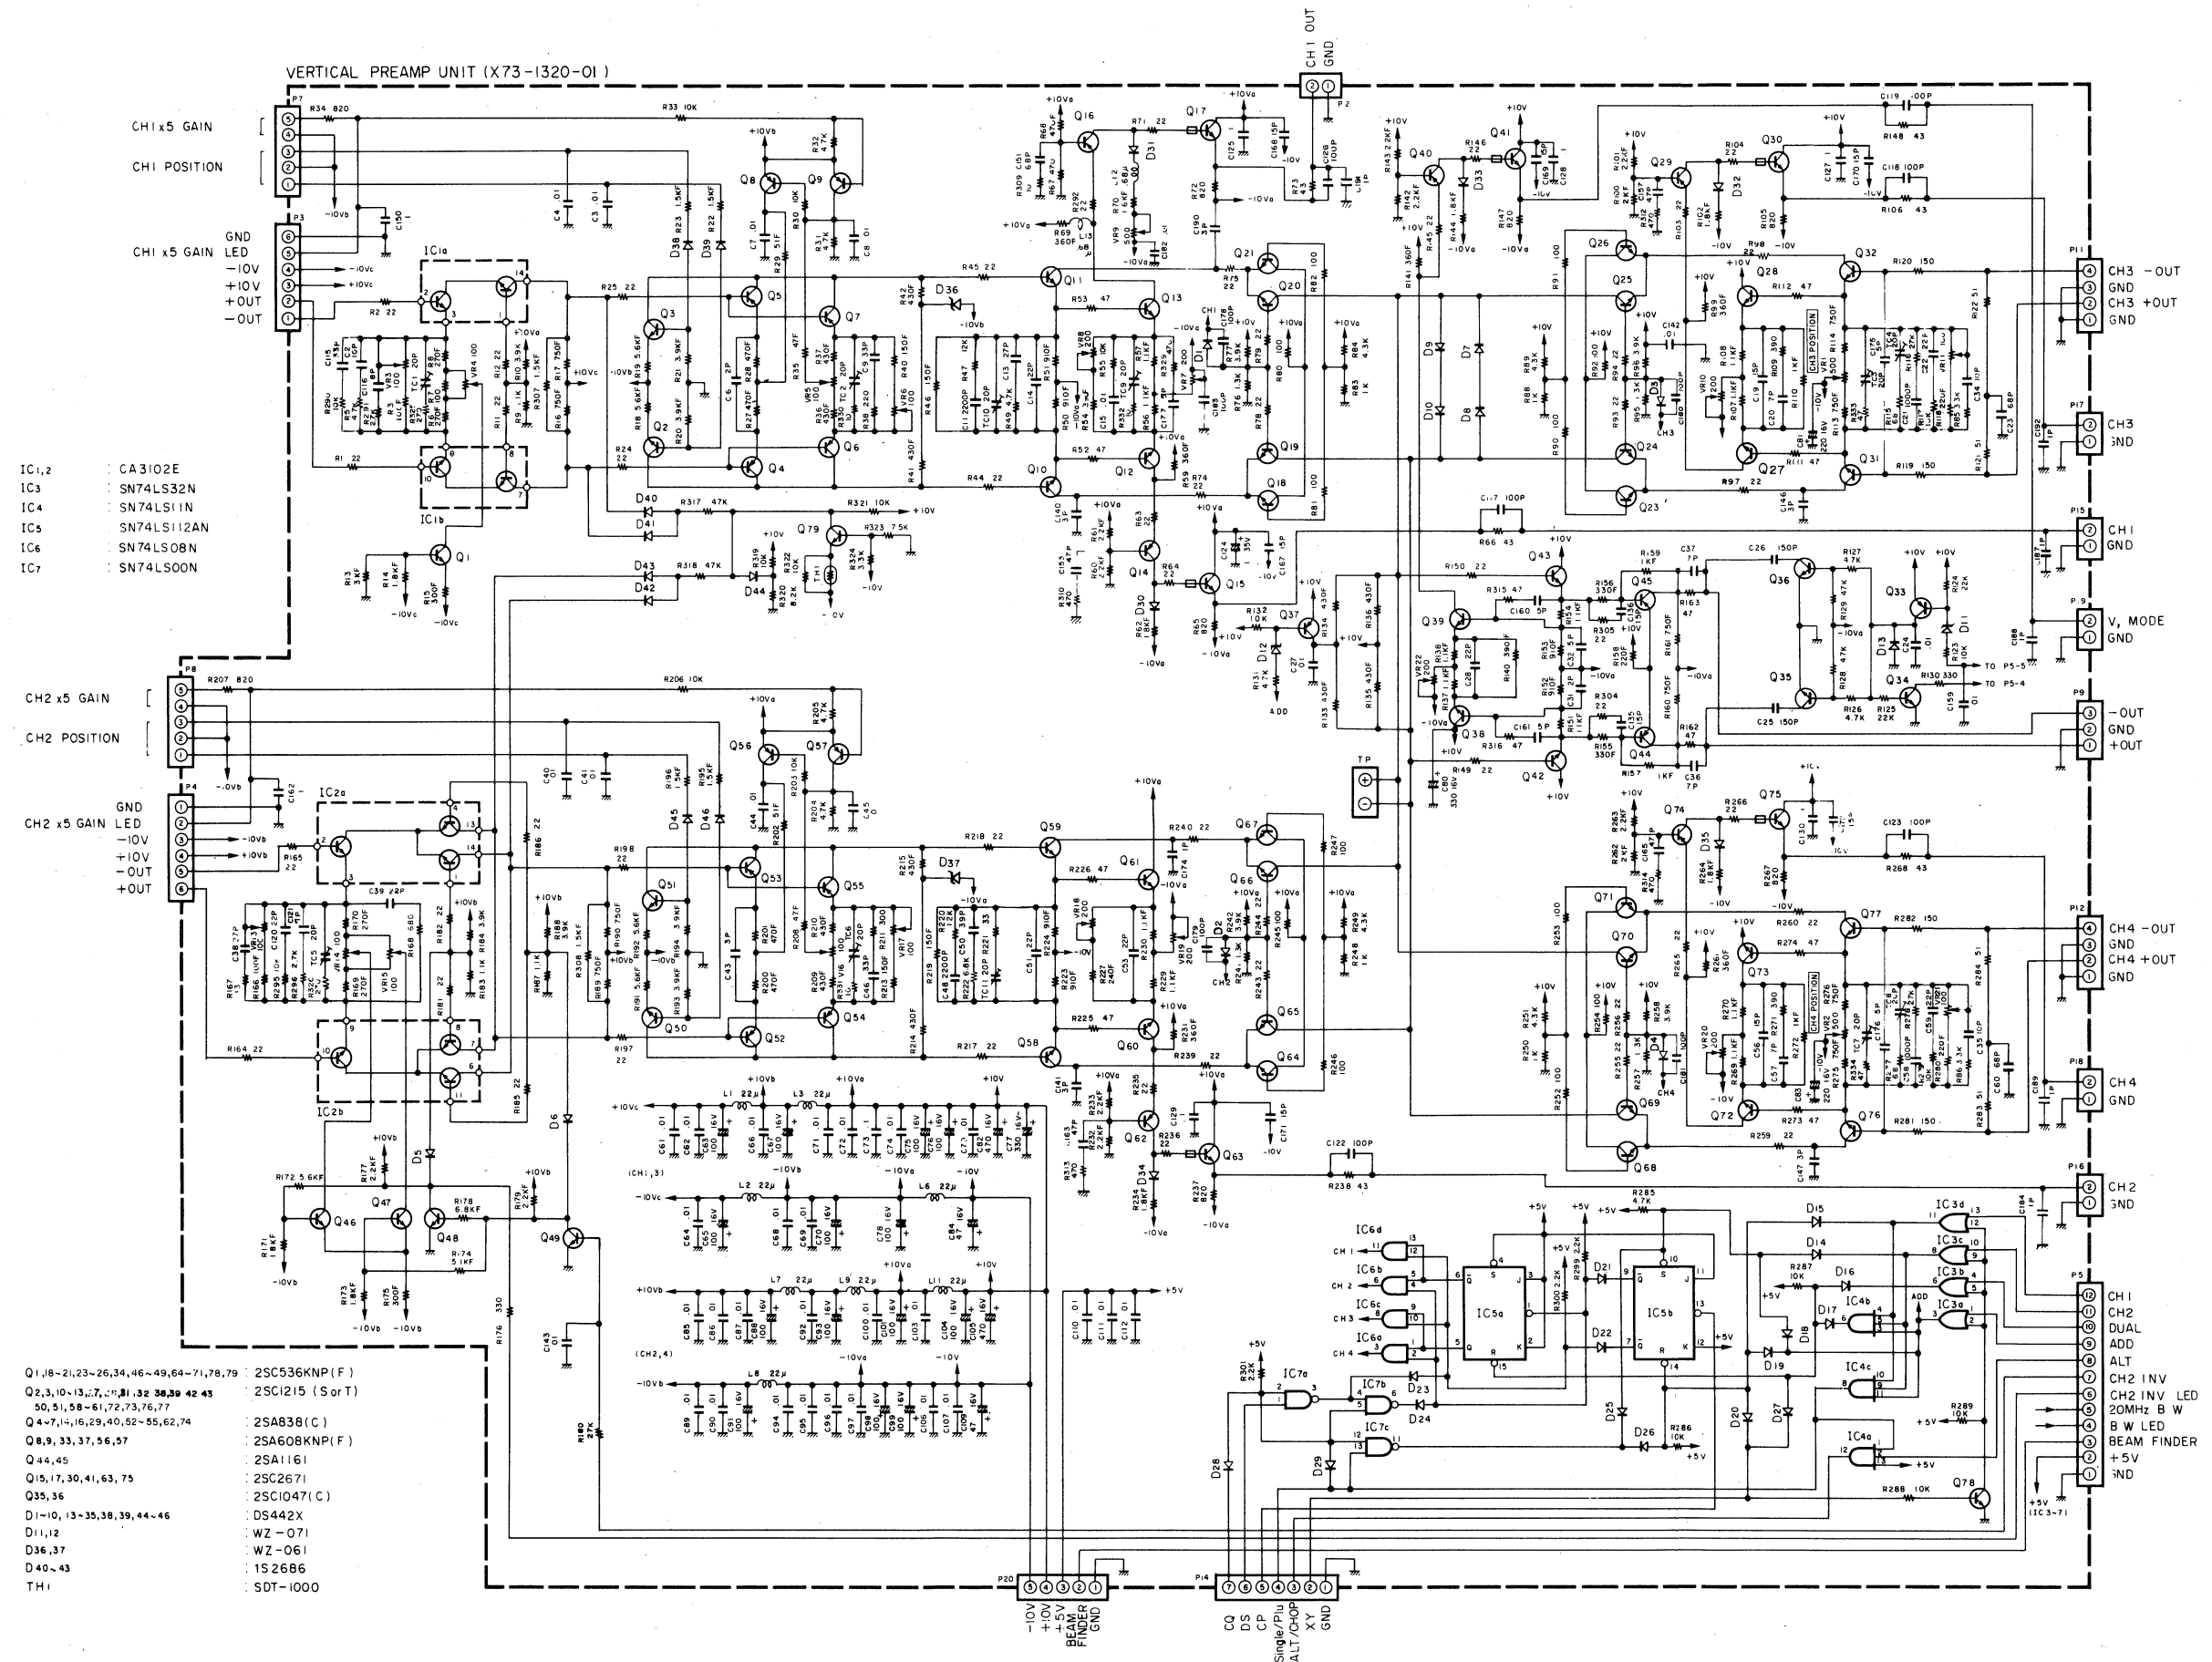


VERTICAL OUTPUT AMP UNIT (X73-1330-01)

VERTICAL OUTPUT AMP UNIT (X73-1330-01)

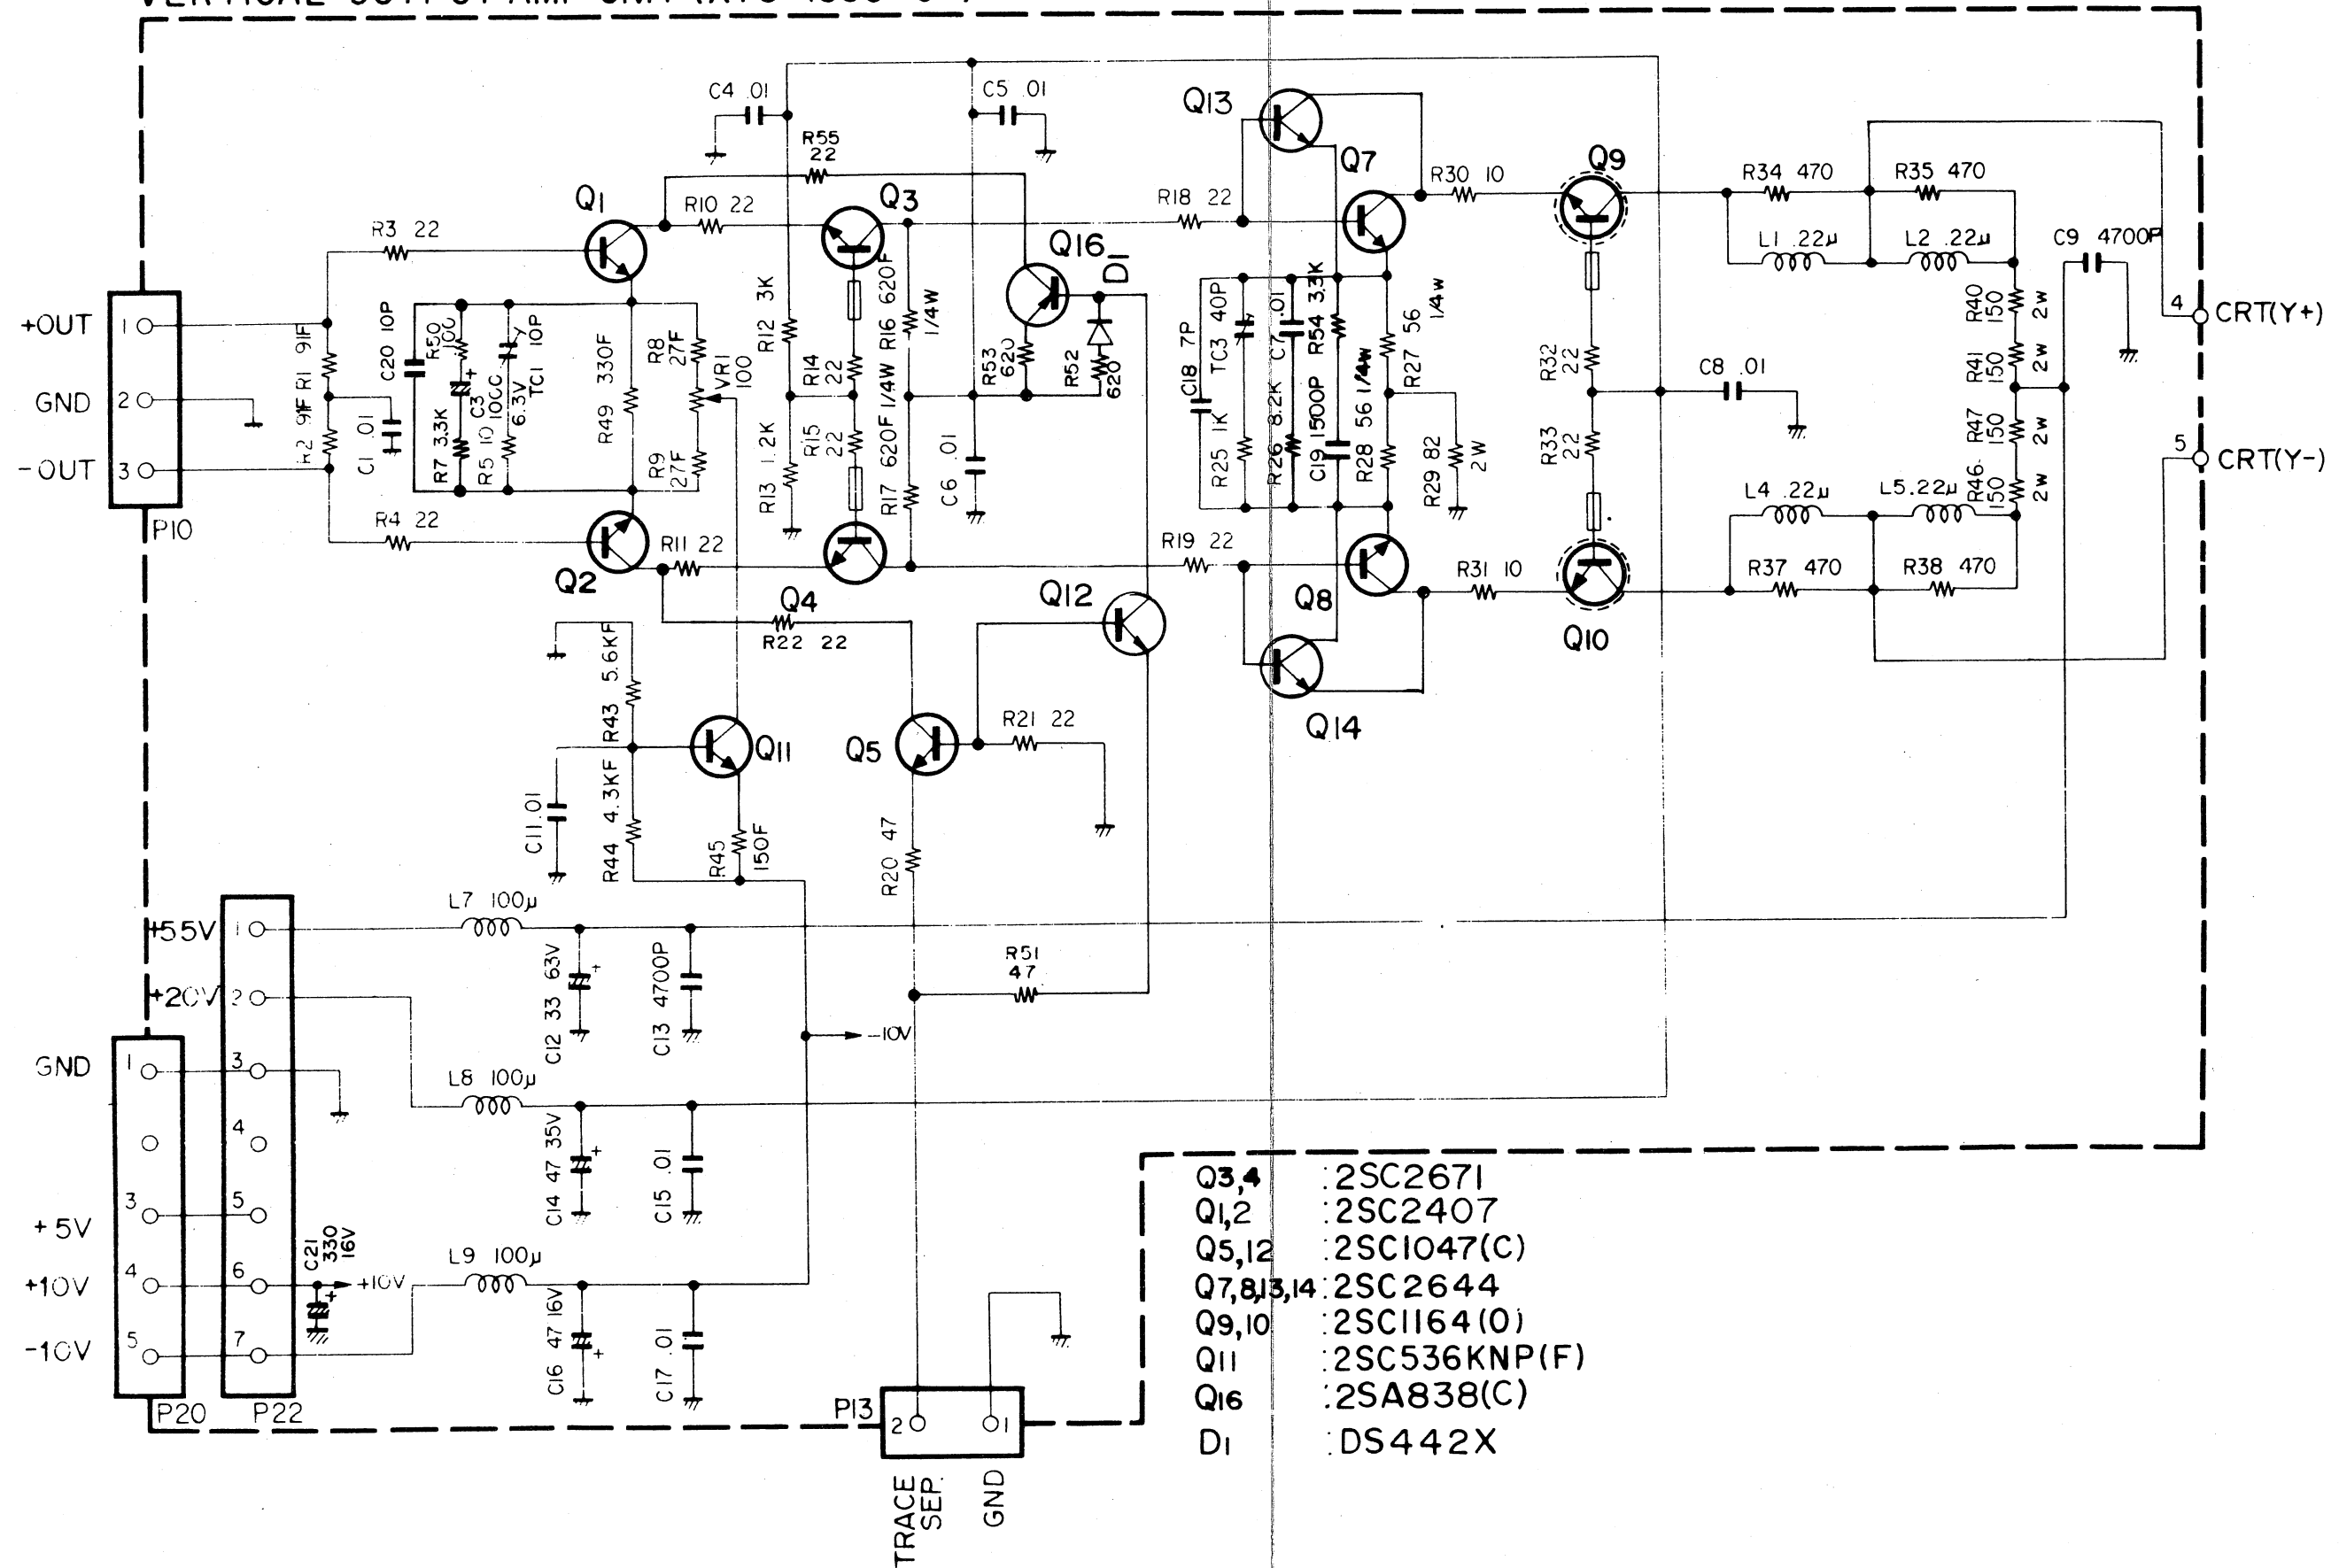


- | | |
|------------|----------------|
| Q3,4 | : 2SC2671 |
| Q1,2 | : 2SC2407 |
| Q5,12 | : 2SC1047(C) |
| Q7,8,13,14 | : 2SC2644 |
| Q9,10 | : 2SC1164(O) |
| Q11 | : 2SC536KNP(F) |
| Q16 | : 2SA838(C) |
| D1 | : DS442X |

TRIG SWEEP UNIT (X74-1220-01)

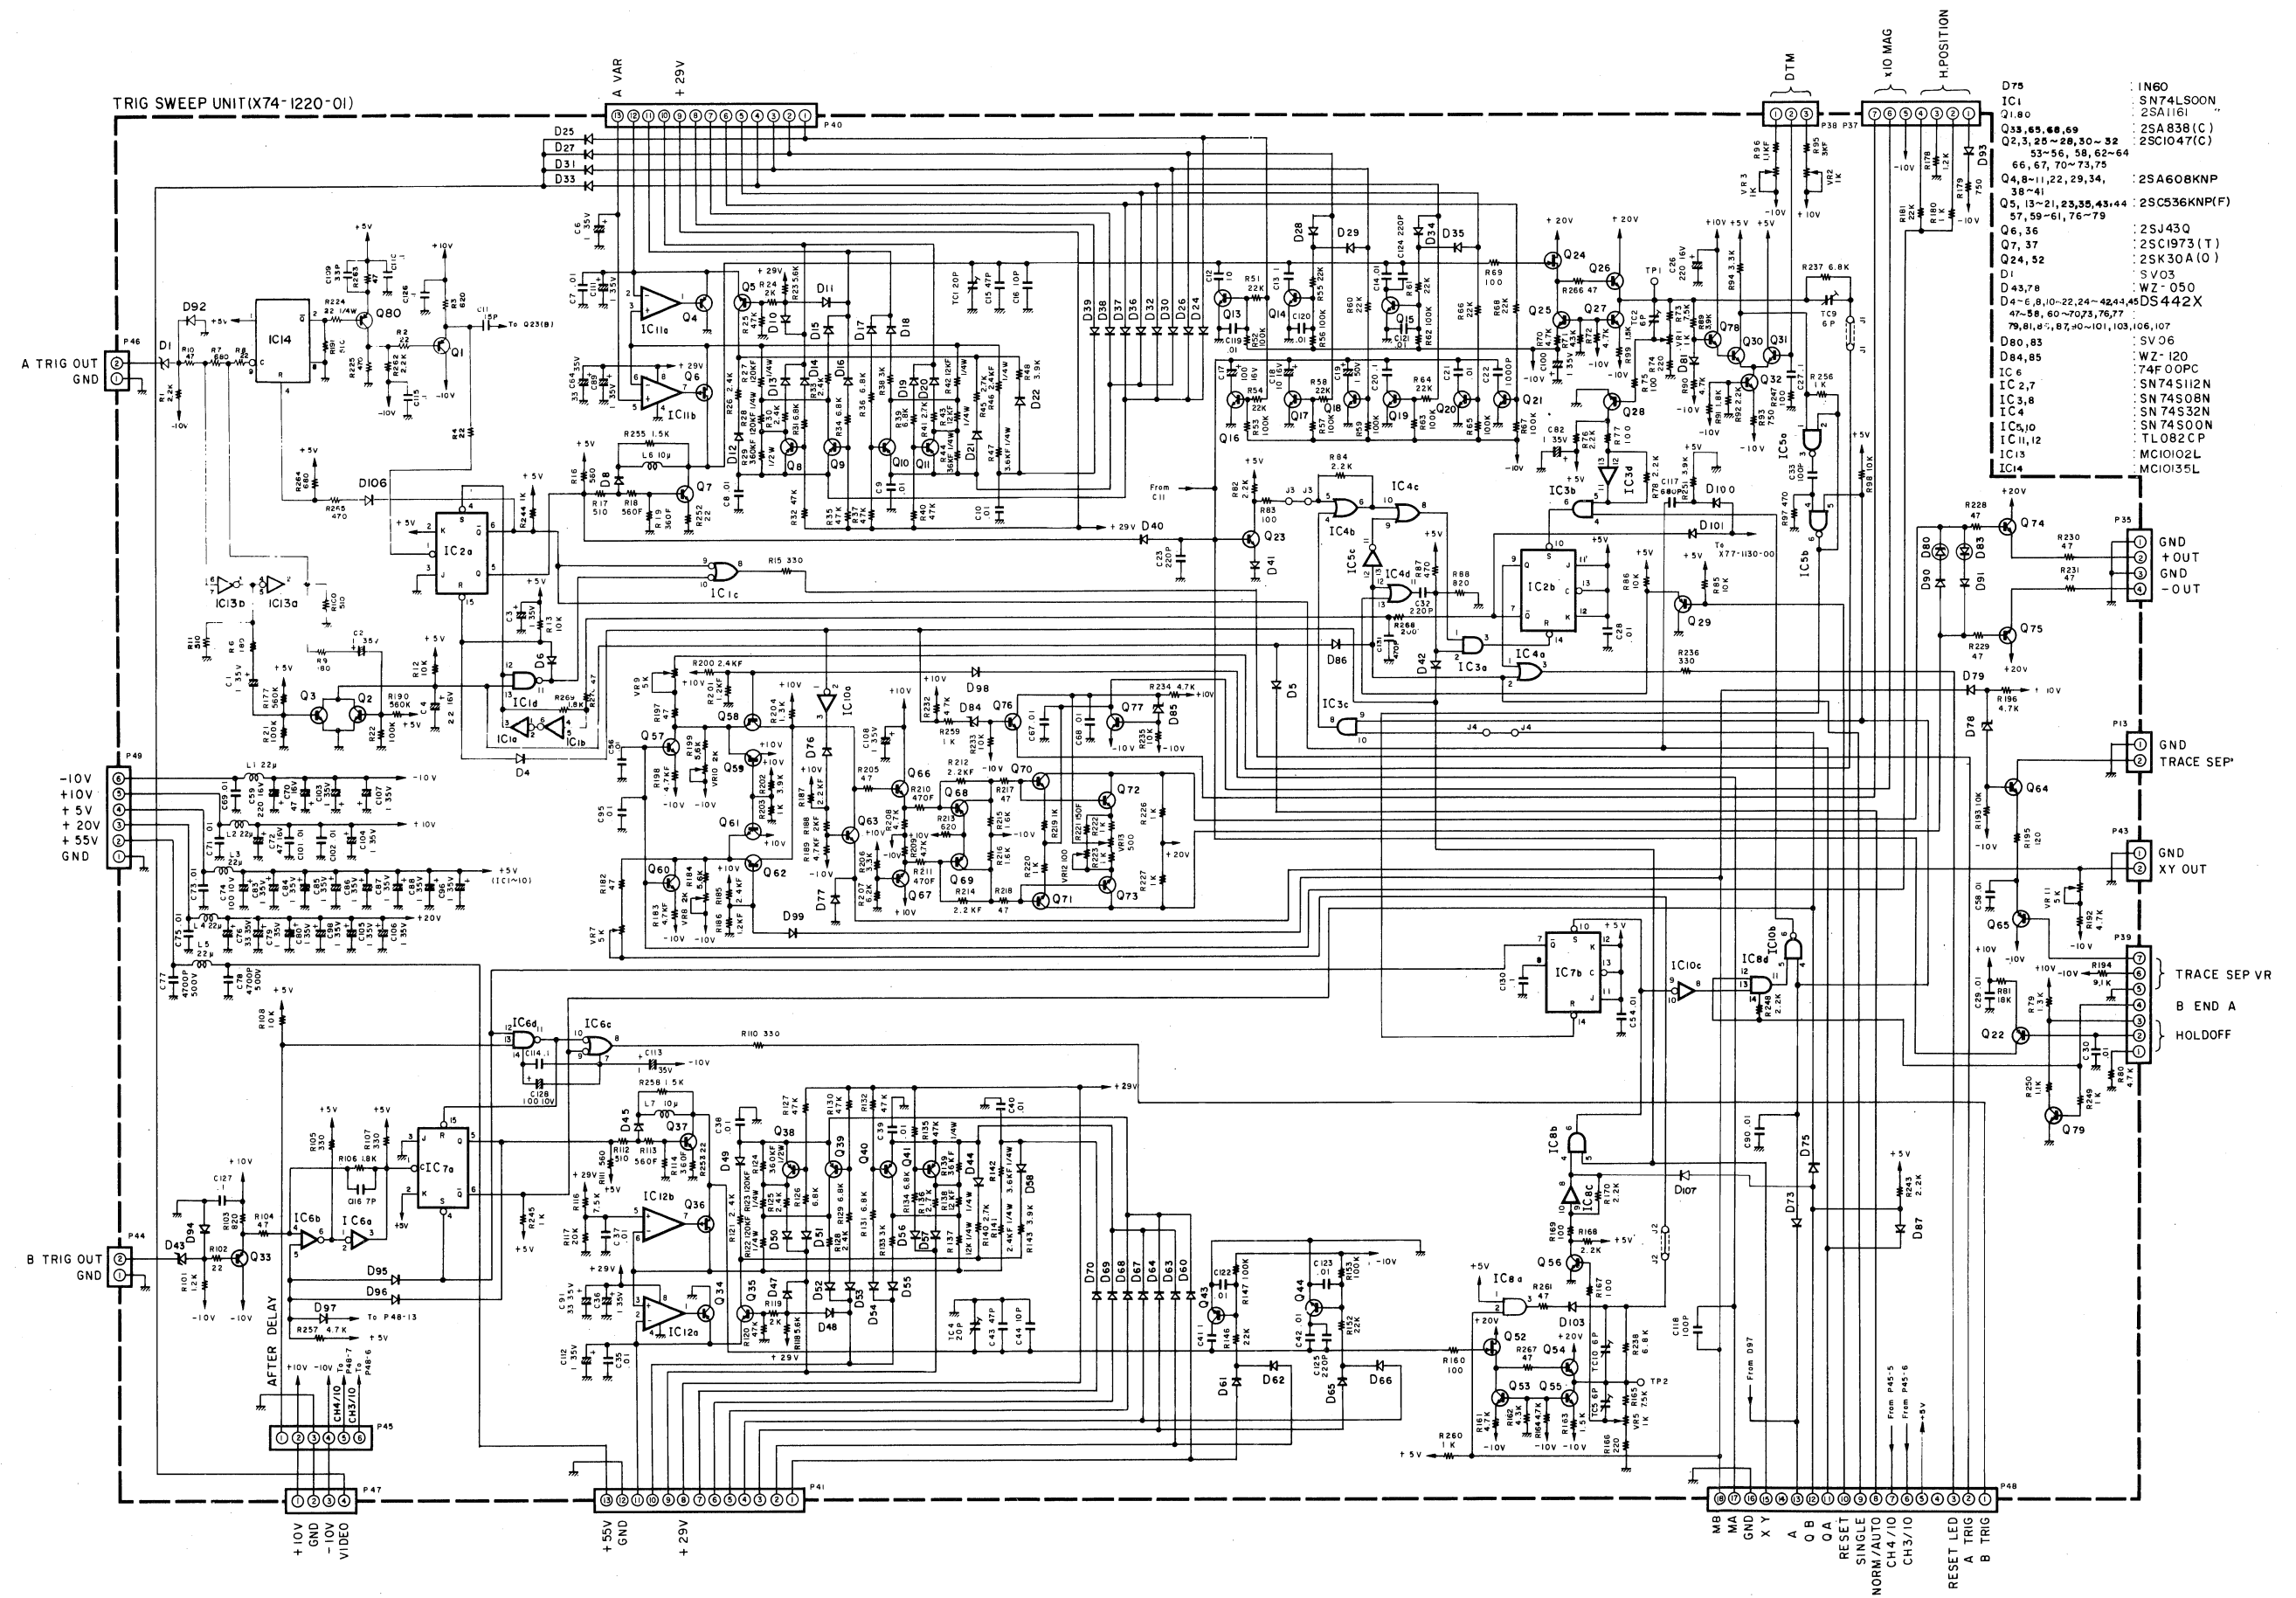


SWEEP ROTARY UNIT (X74-1250-01)

SWEEP ROTARY UNIT (X74-1250-01)

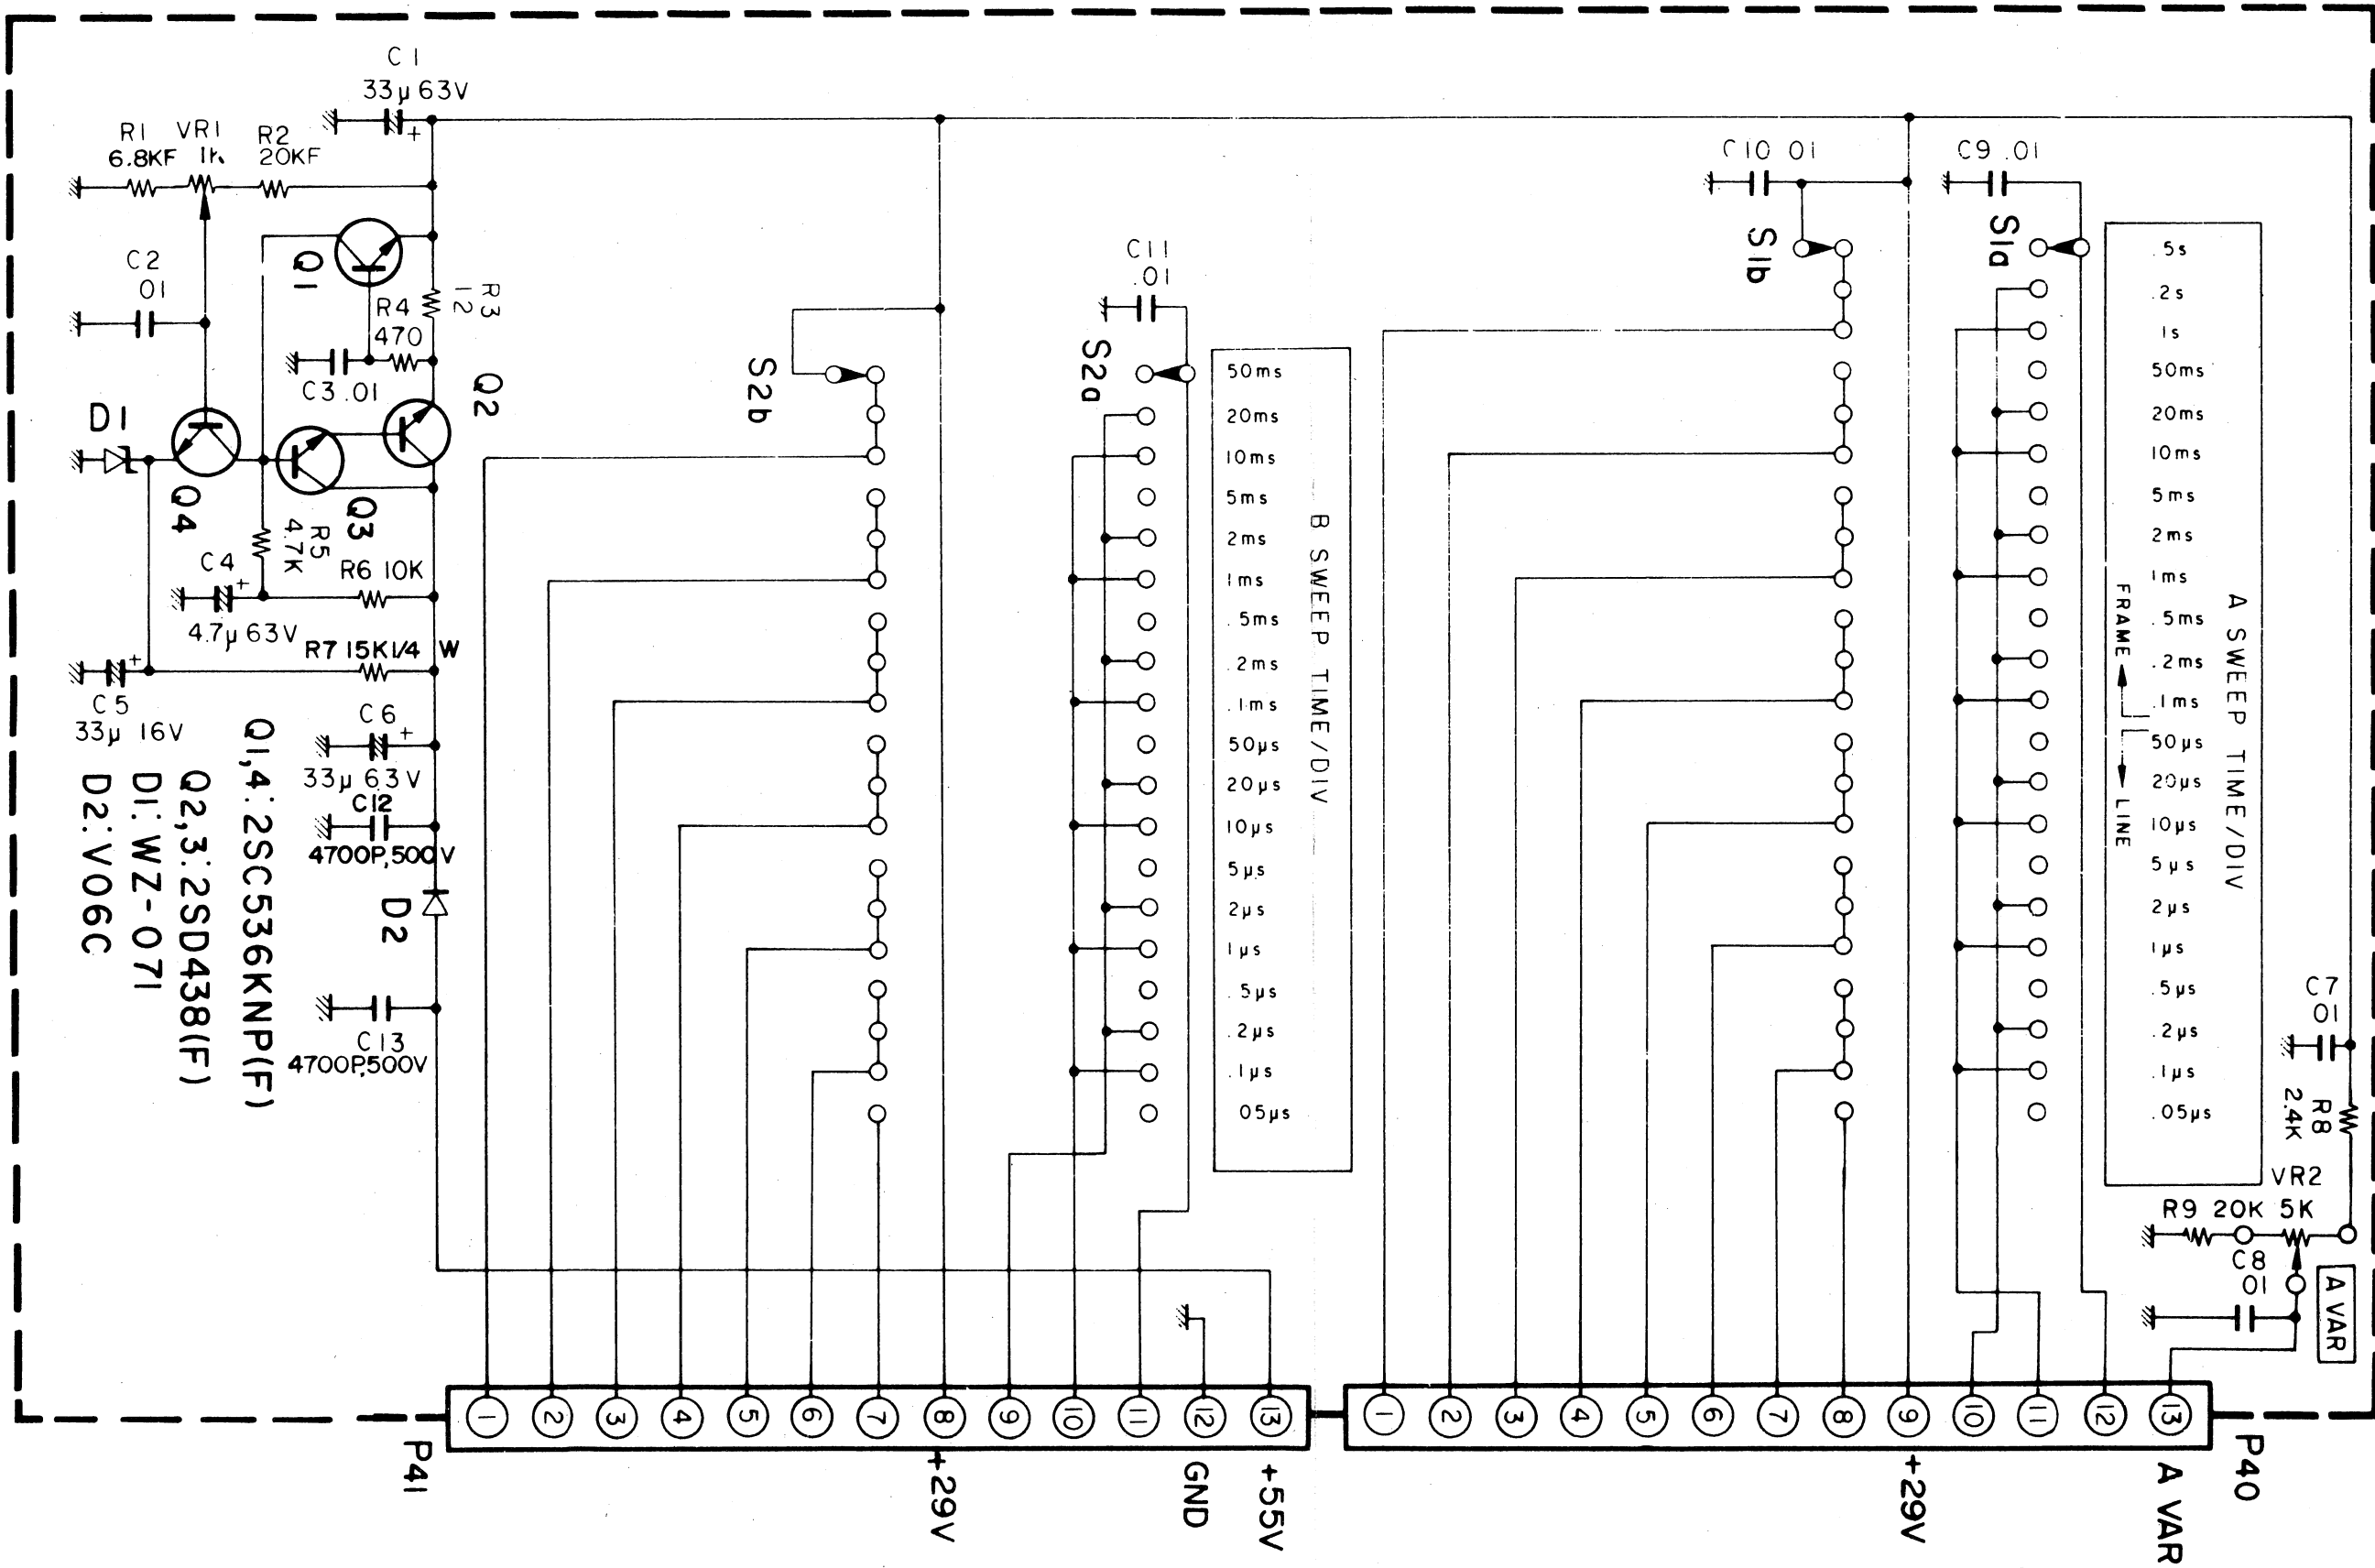


HORIZONTAL MODE CONTROL UNIT (X77-1130-01)

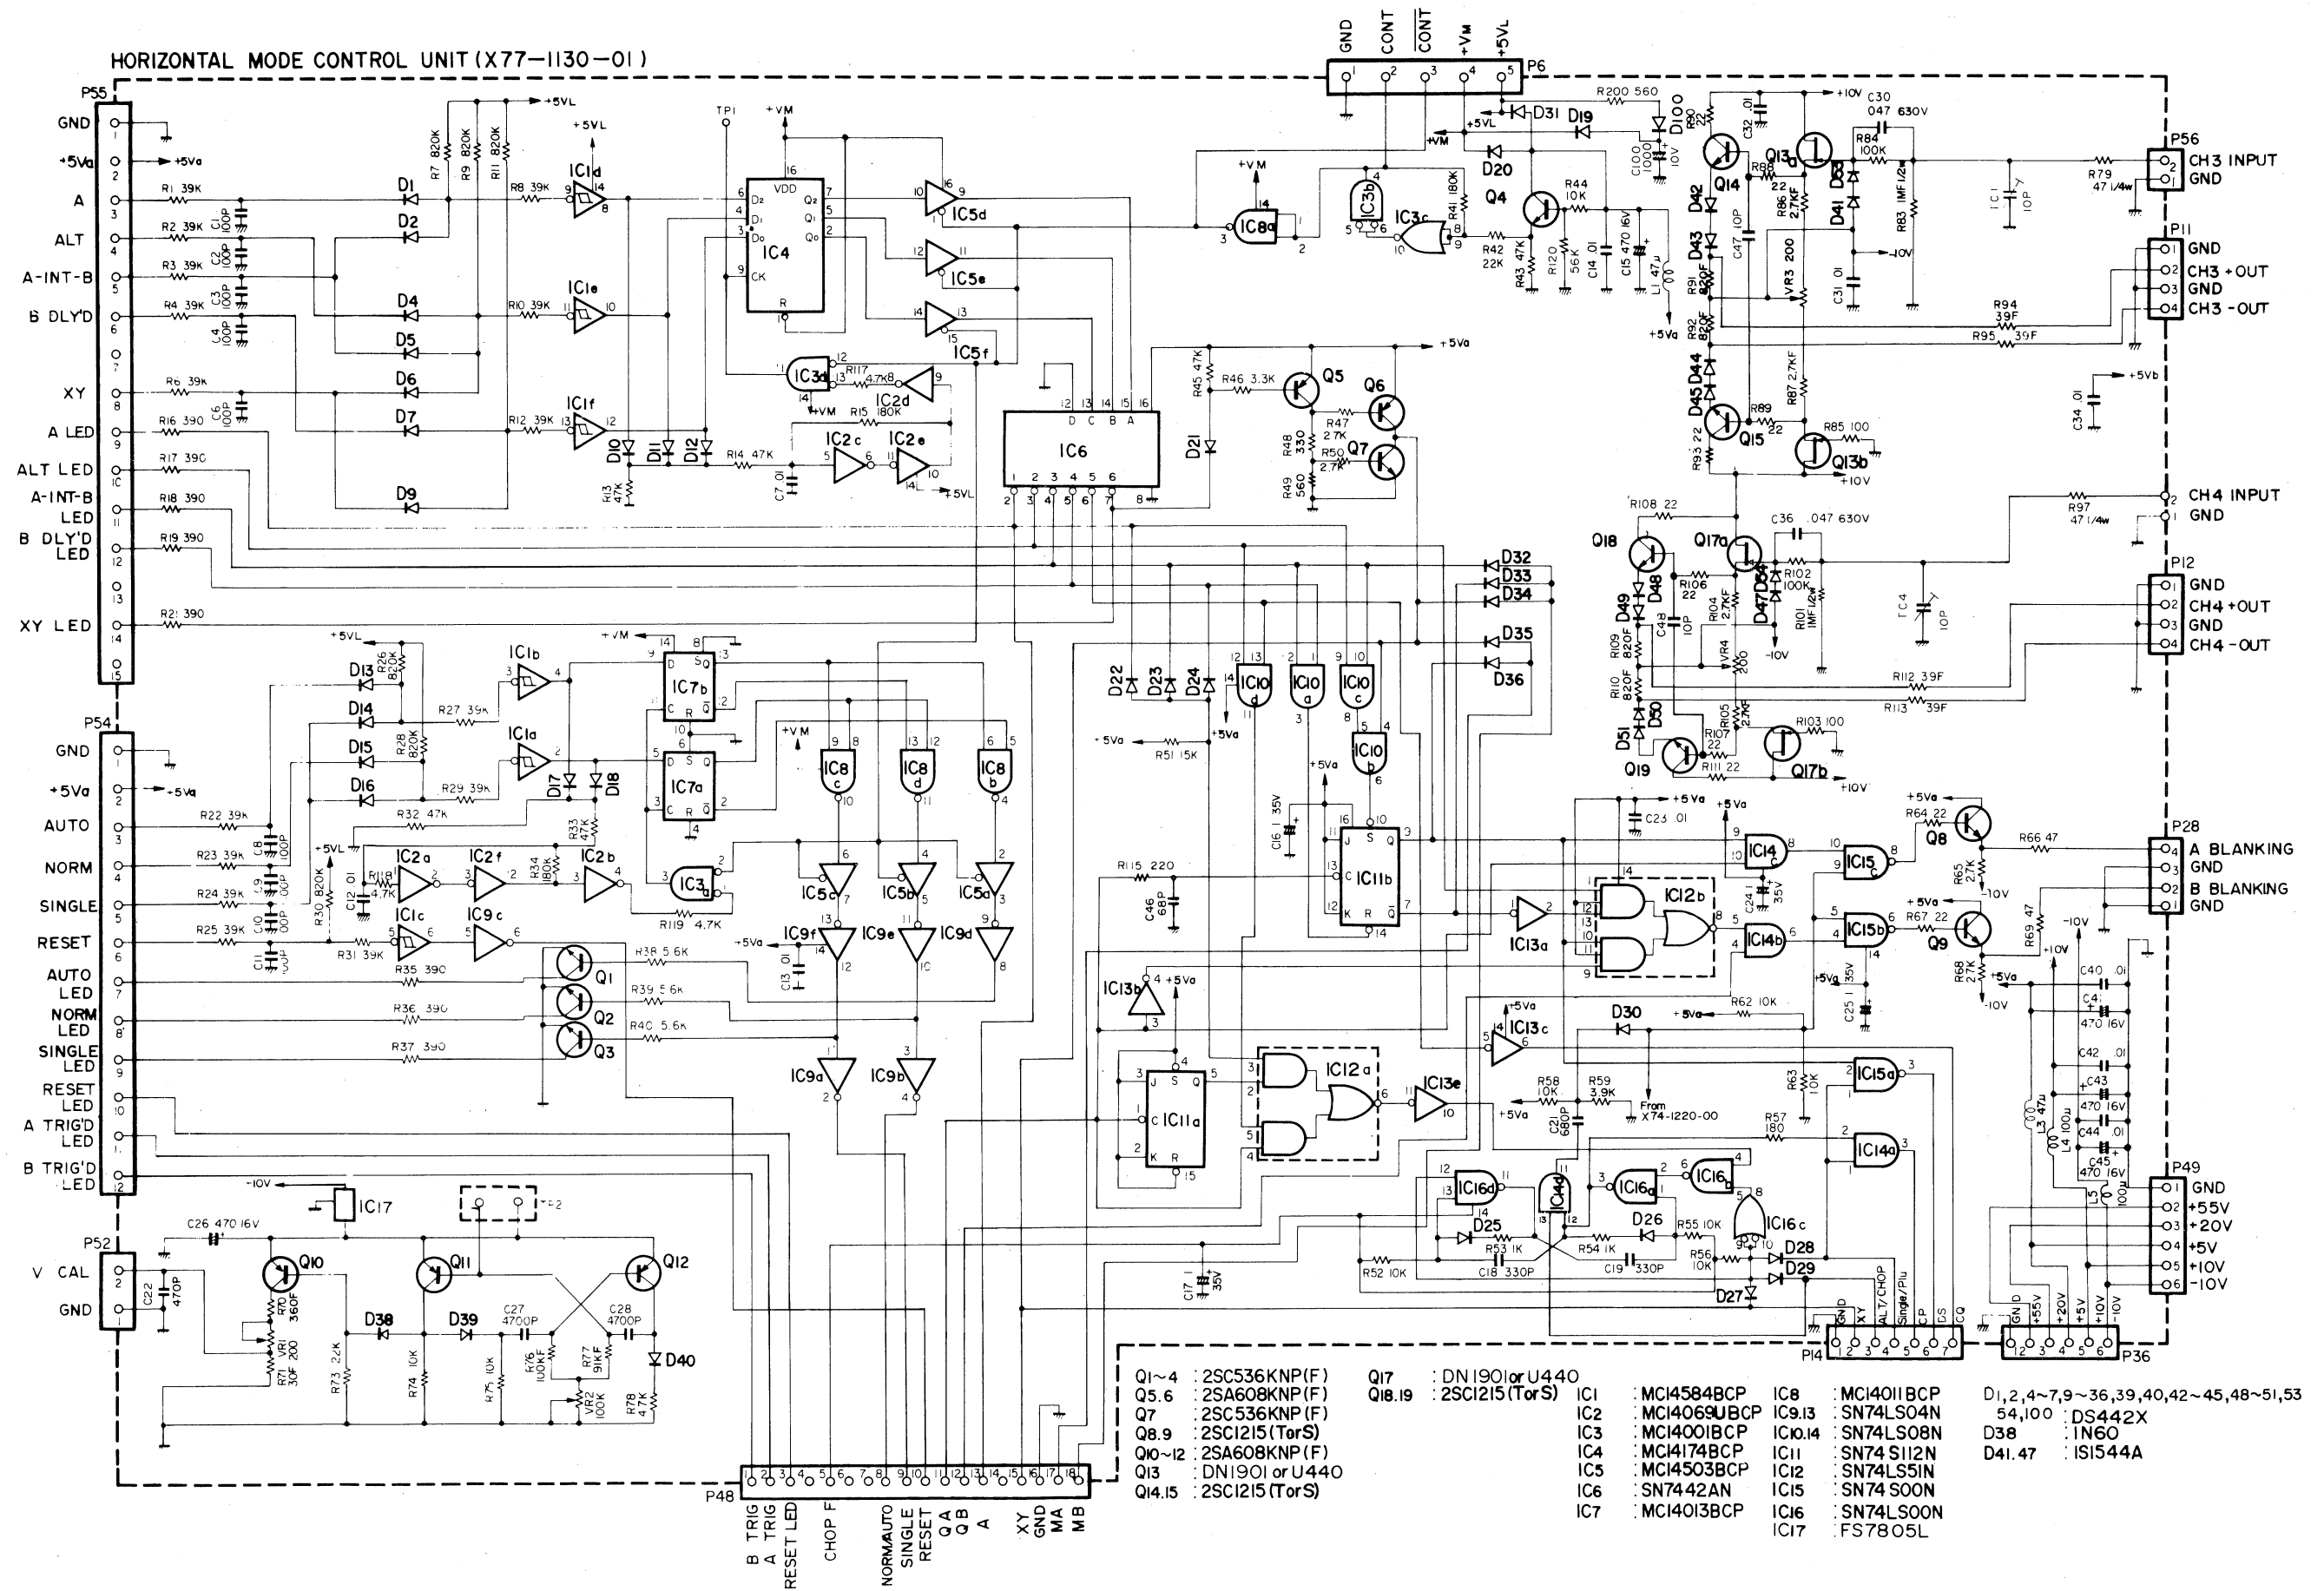


HORIZONTAL OUTPUT AMP UNIT (X74-1230-01)

HORIZONTAL OUTPUT AMP UNIT (X74-1230-01)

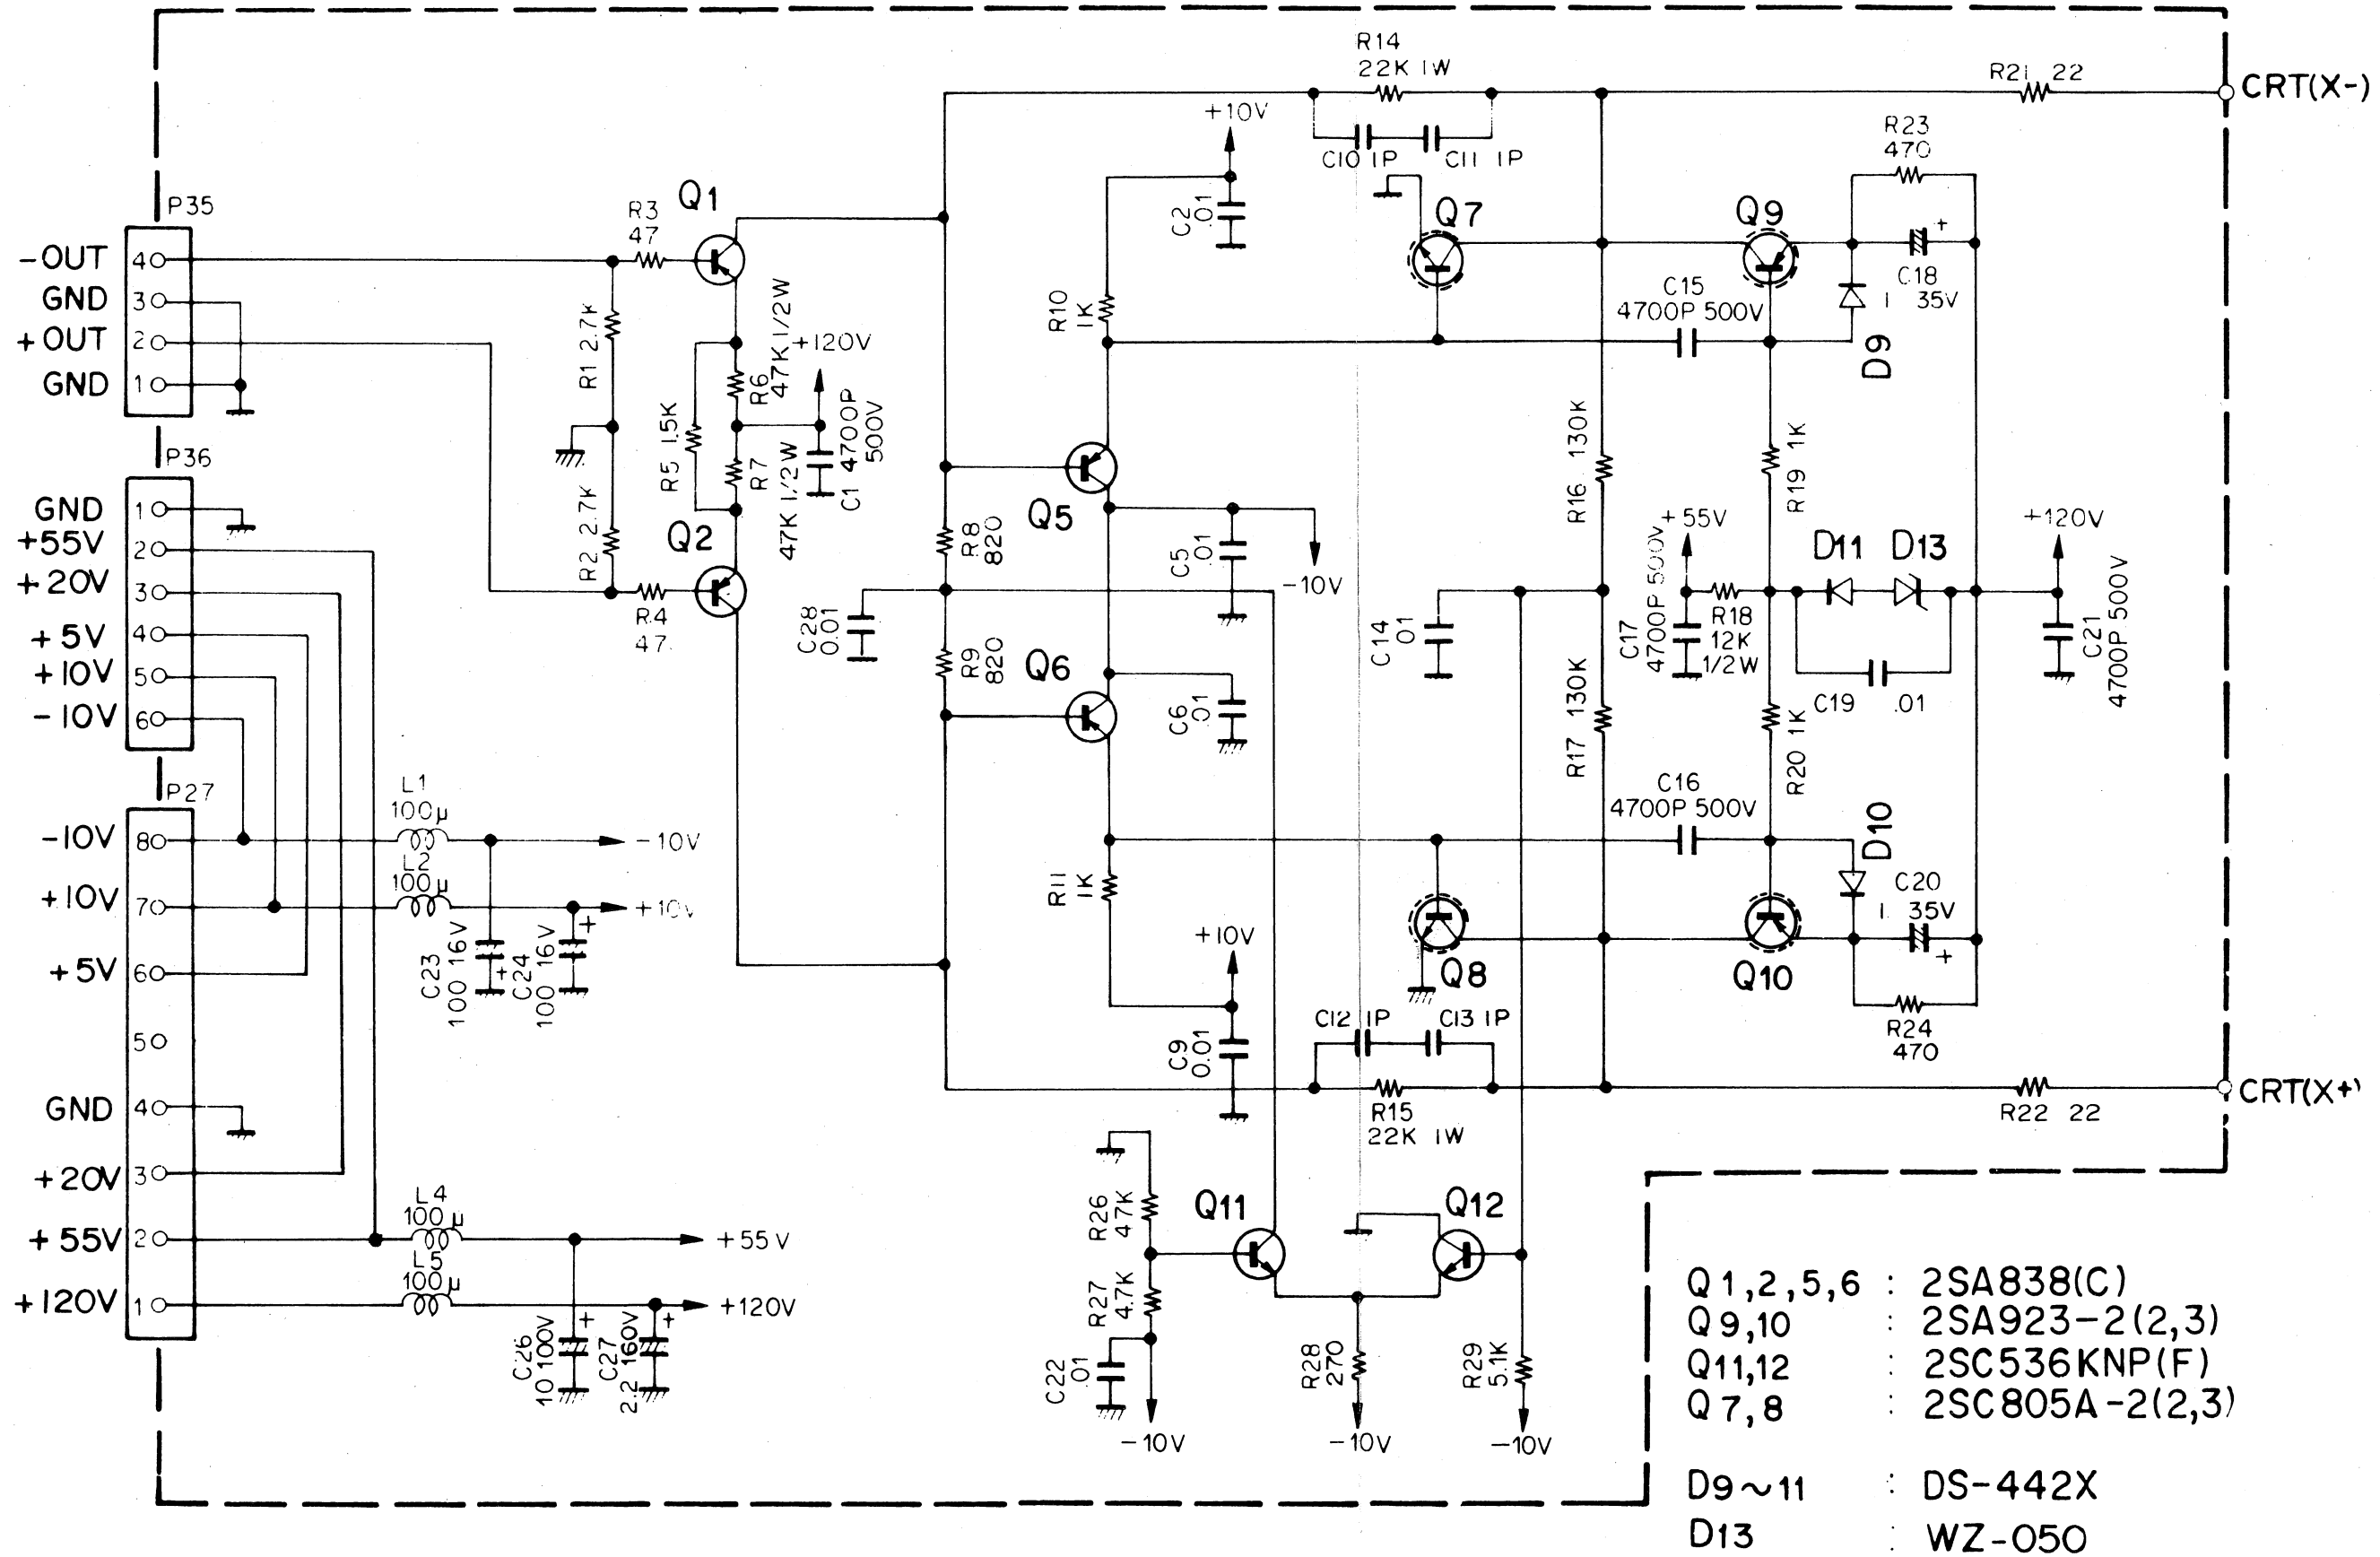


A TRIG SWITCH UNIT (X77-1110-01)

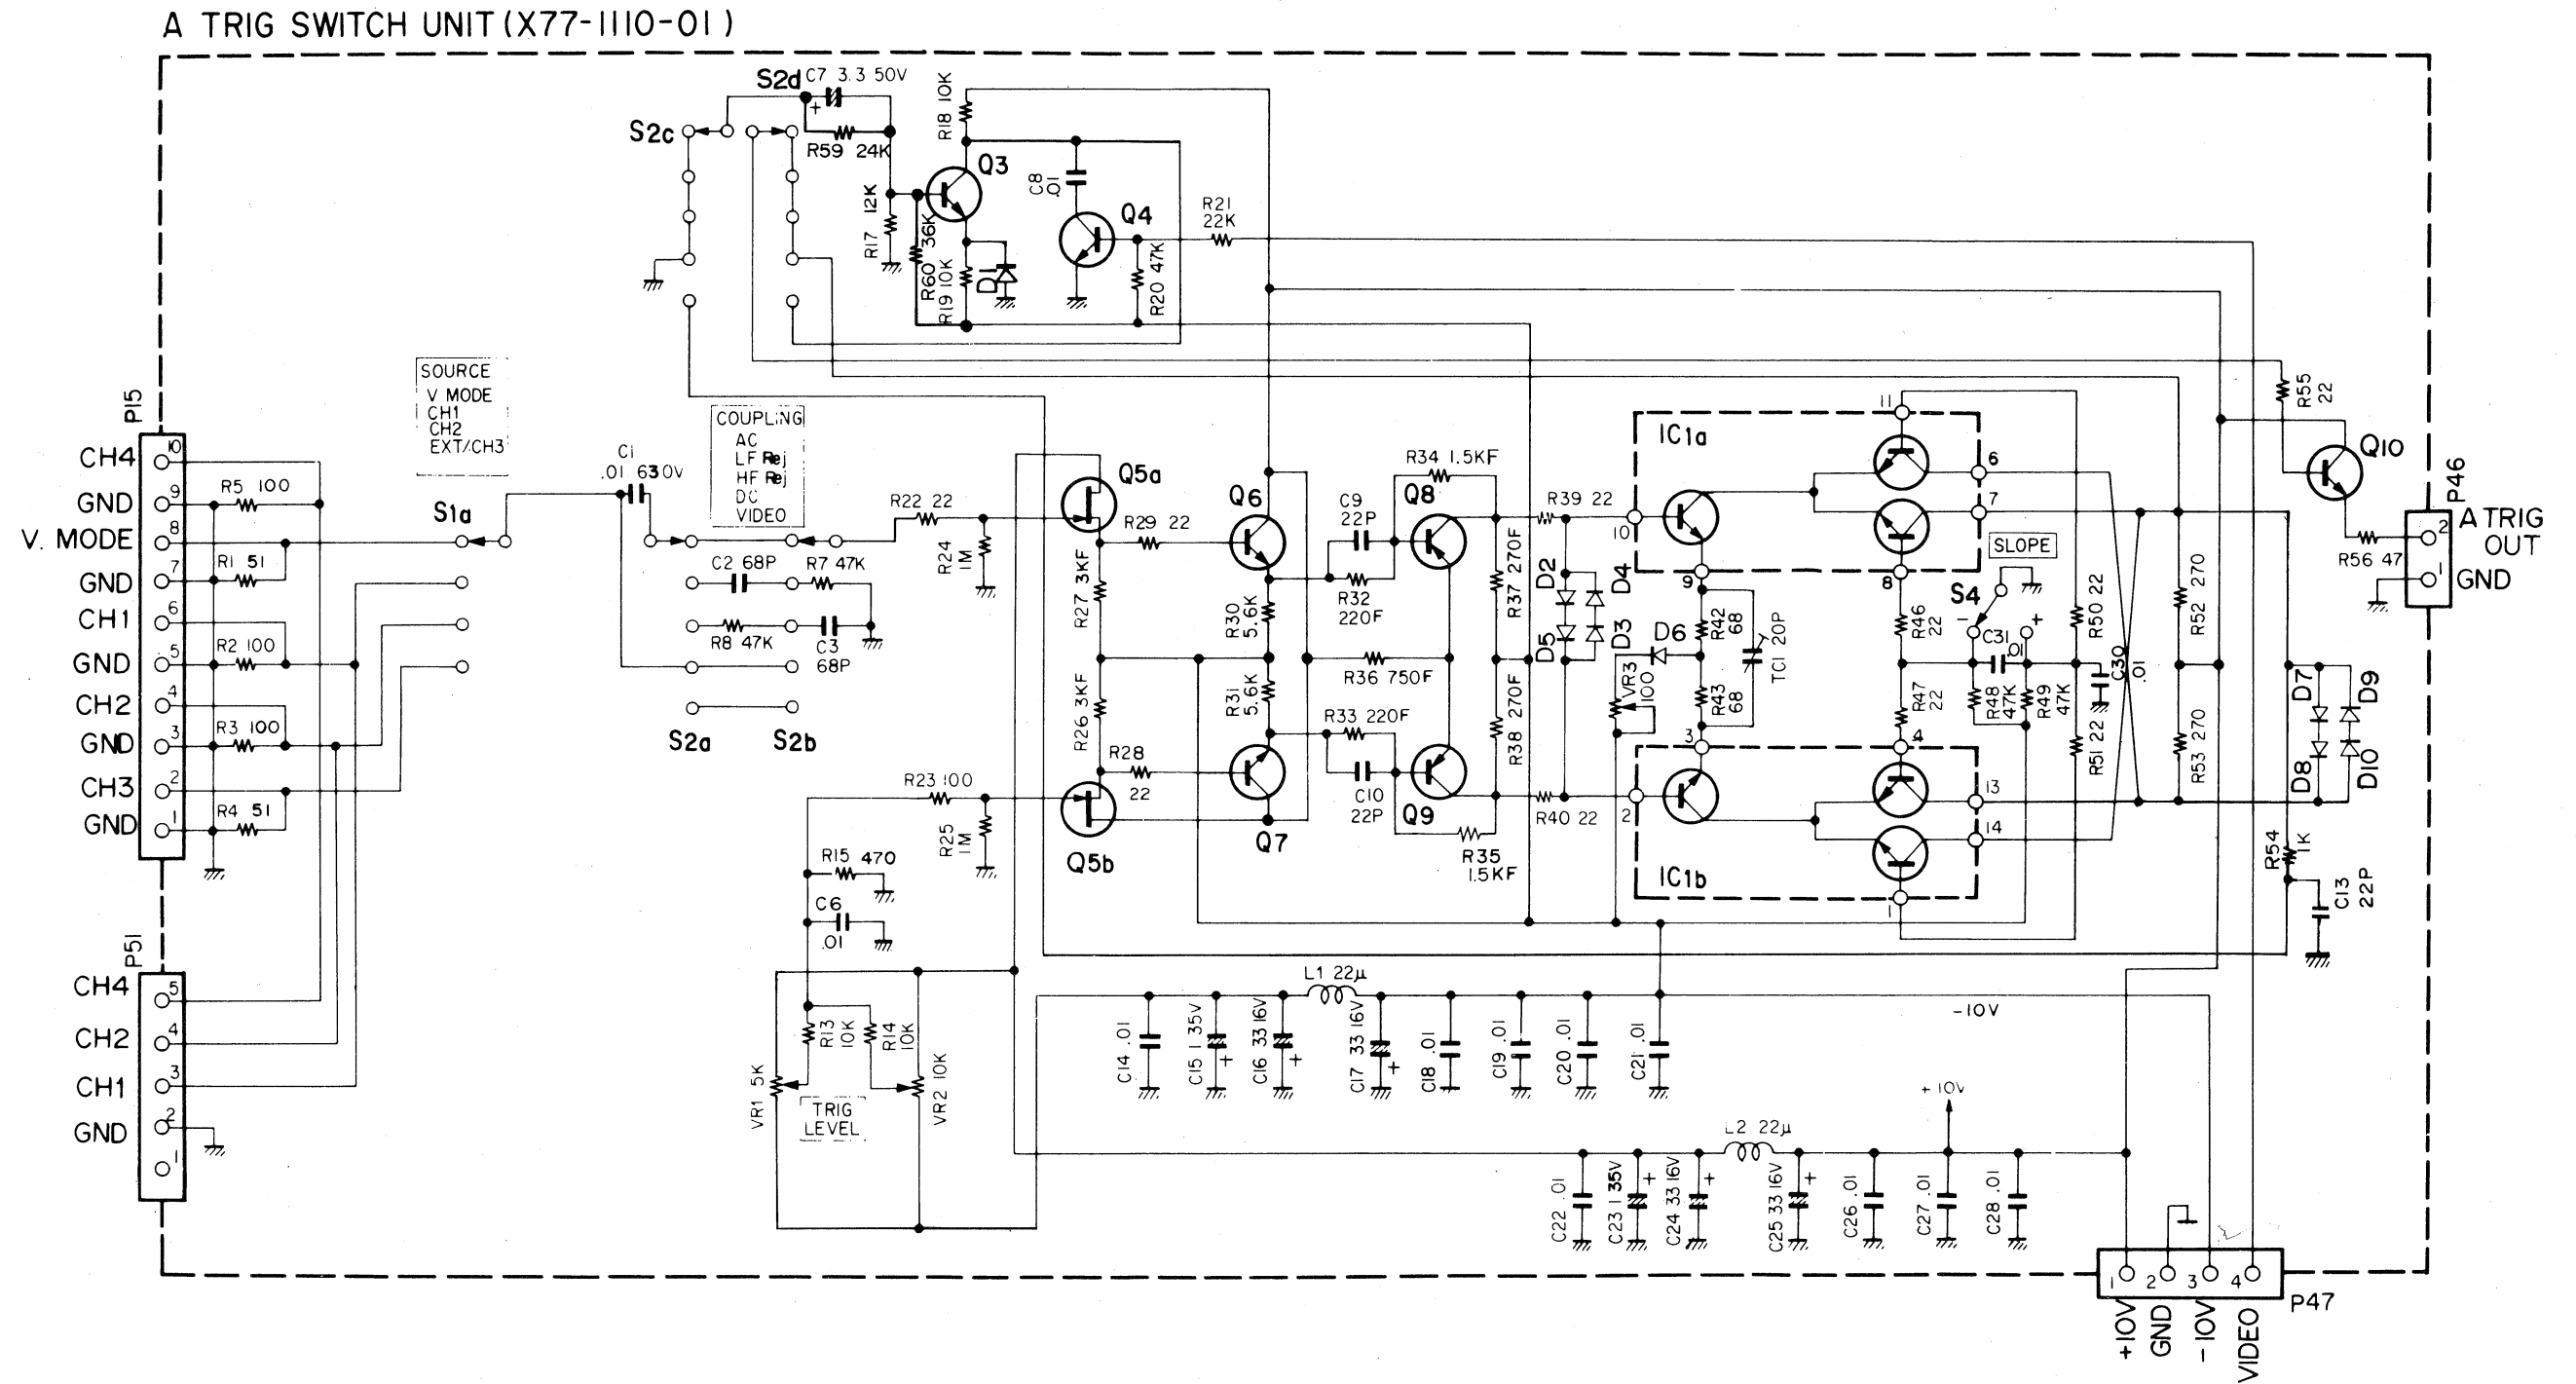

- IC1 : CA3102E DI~10: DS442X
- Q3,4 : 2SC536KNP(F)
- Q5 : DN1901 or U440
- Q6,7 : 2SC1215(T or S)
- Q8,9 : 2SA1161
- Q10 : 2SC2671


B TRIG SWITCH UNIT (X77-1120-01)

B TRIG SWITCH UNIT (X77-1120-01)

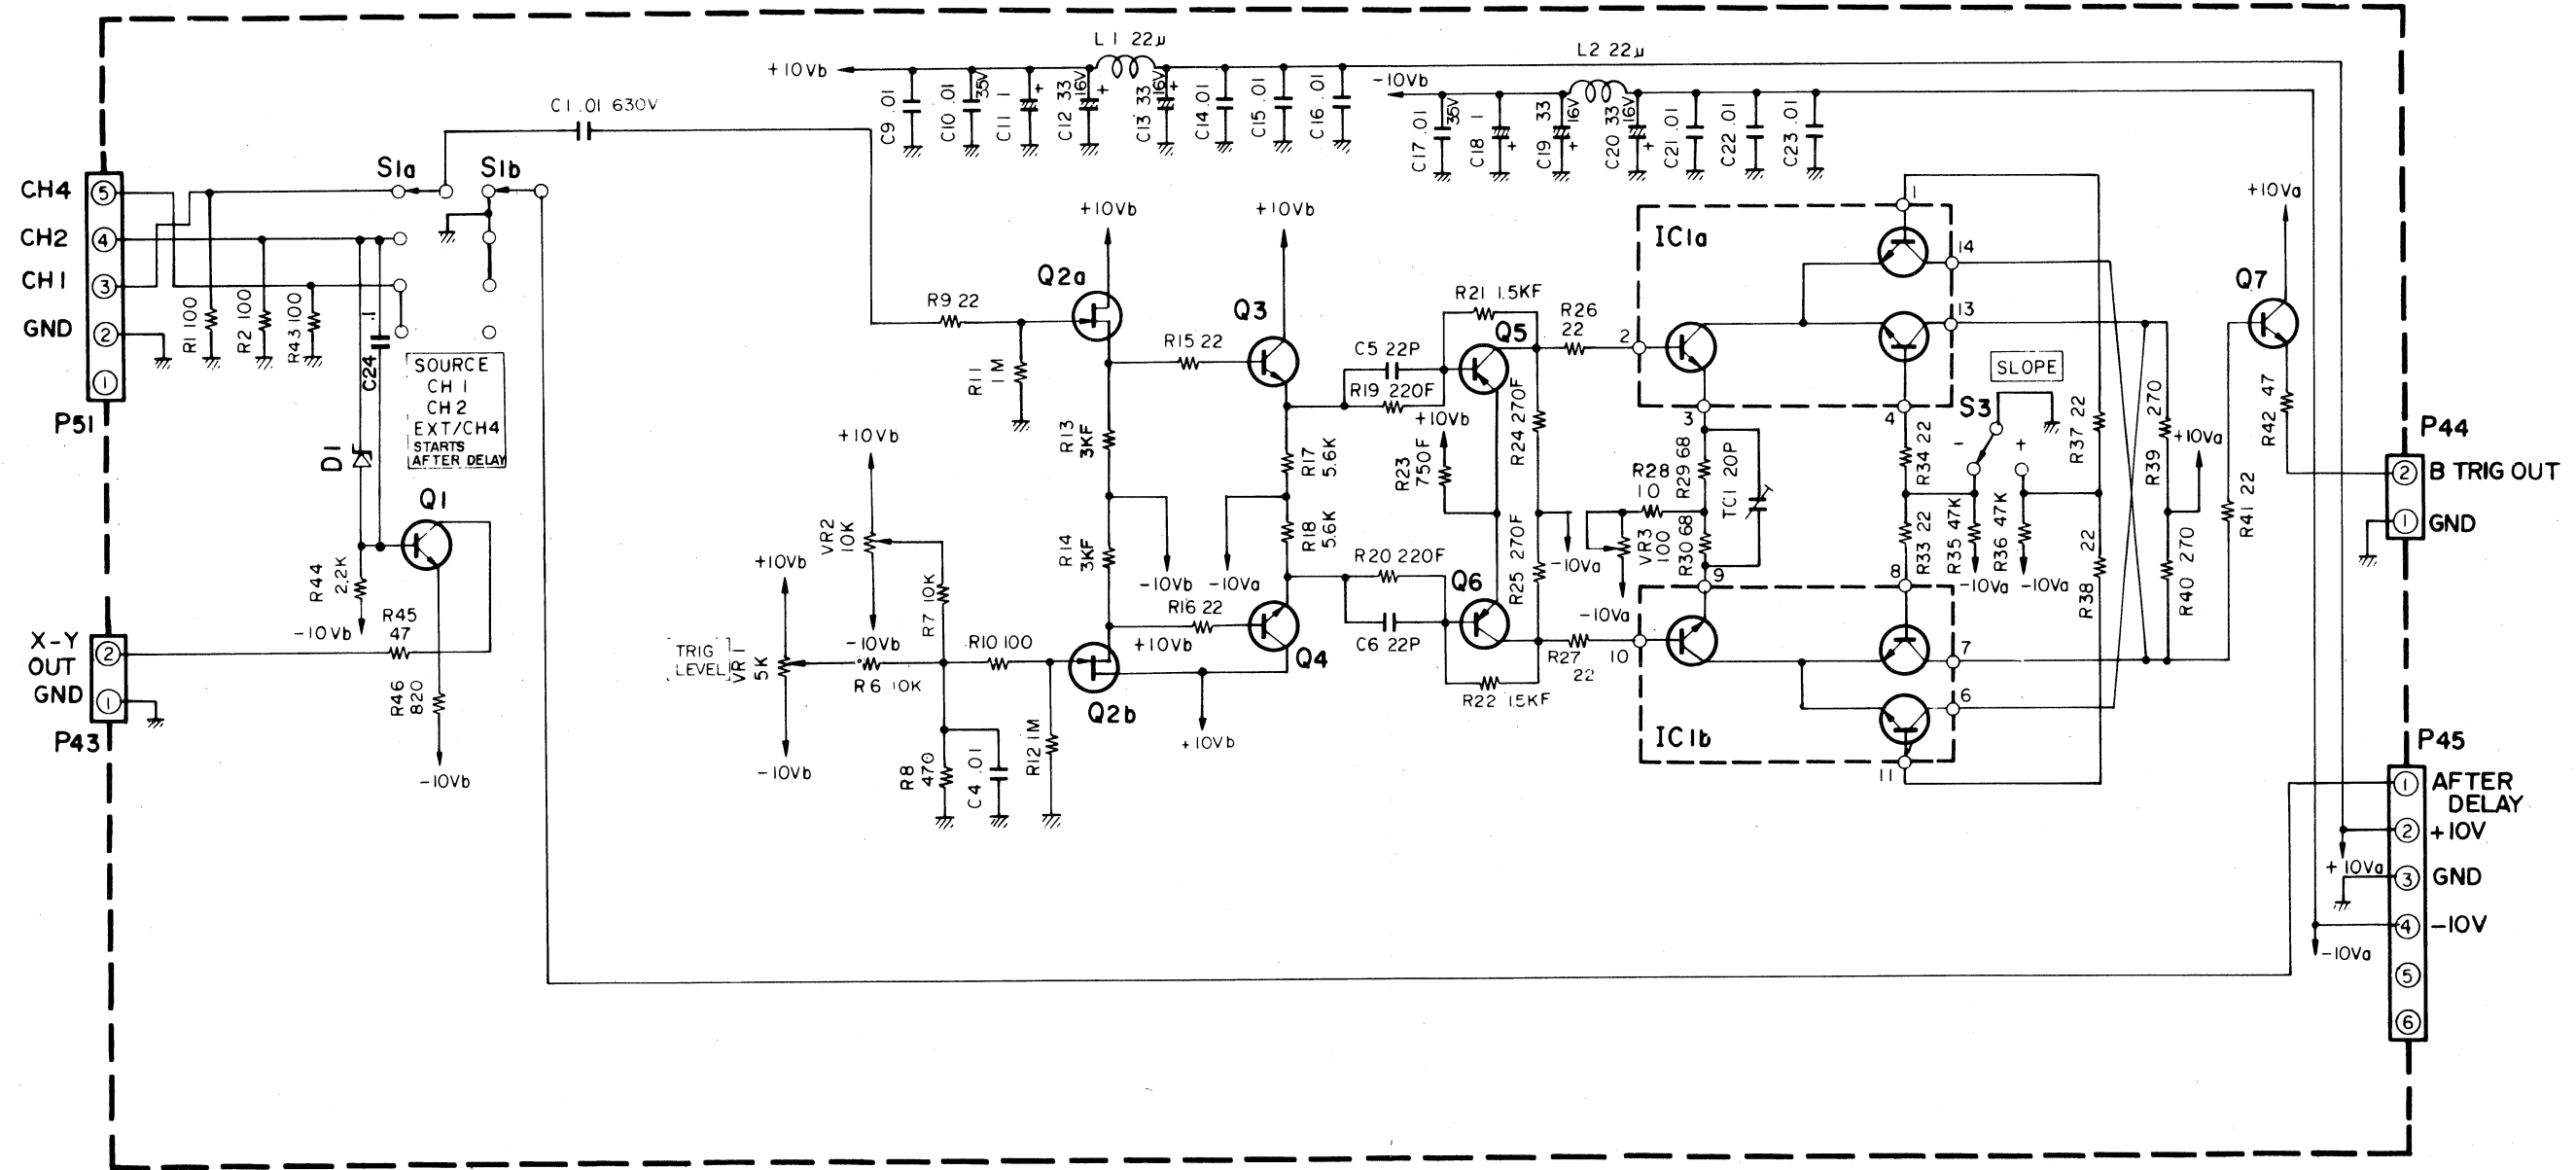

- IC1 : CA3102E Q5,6 : 2SA1161
- Q1,3,4 : 2SC1215TorS DI : WZ-081
- Q2 : DNI901 or U440
- Q7 : 2SC2671


POWER BLANKING UNIT (X68-1310-01)

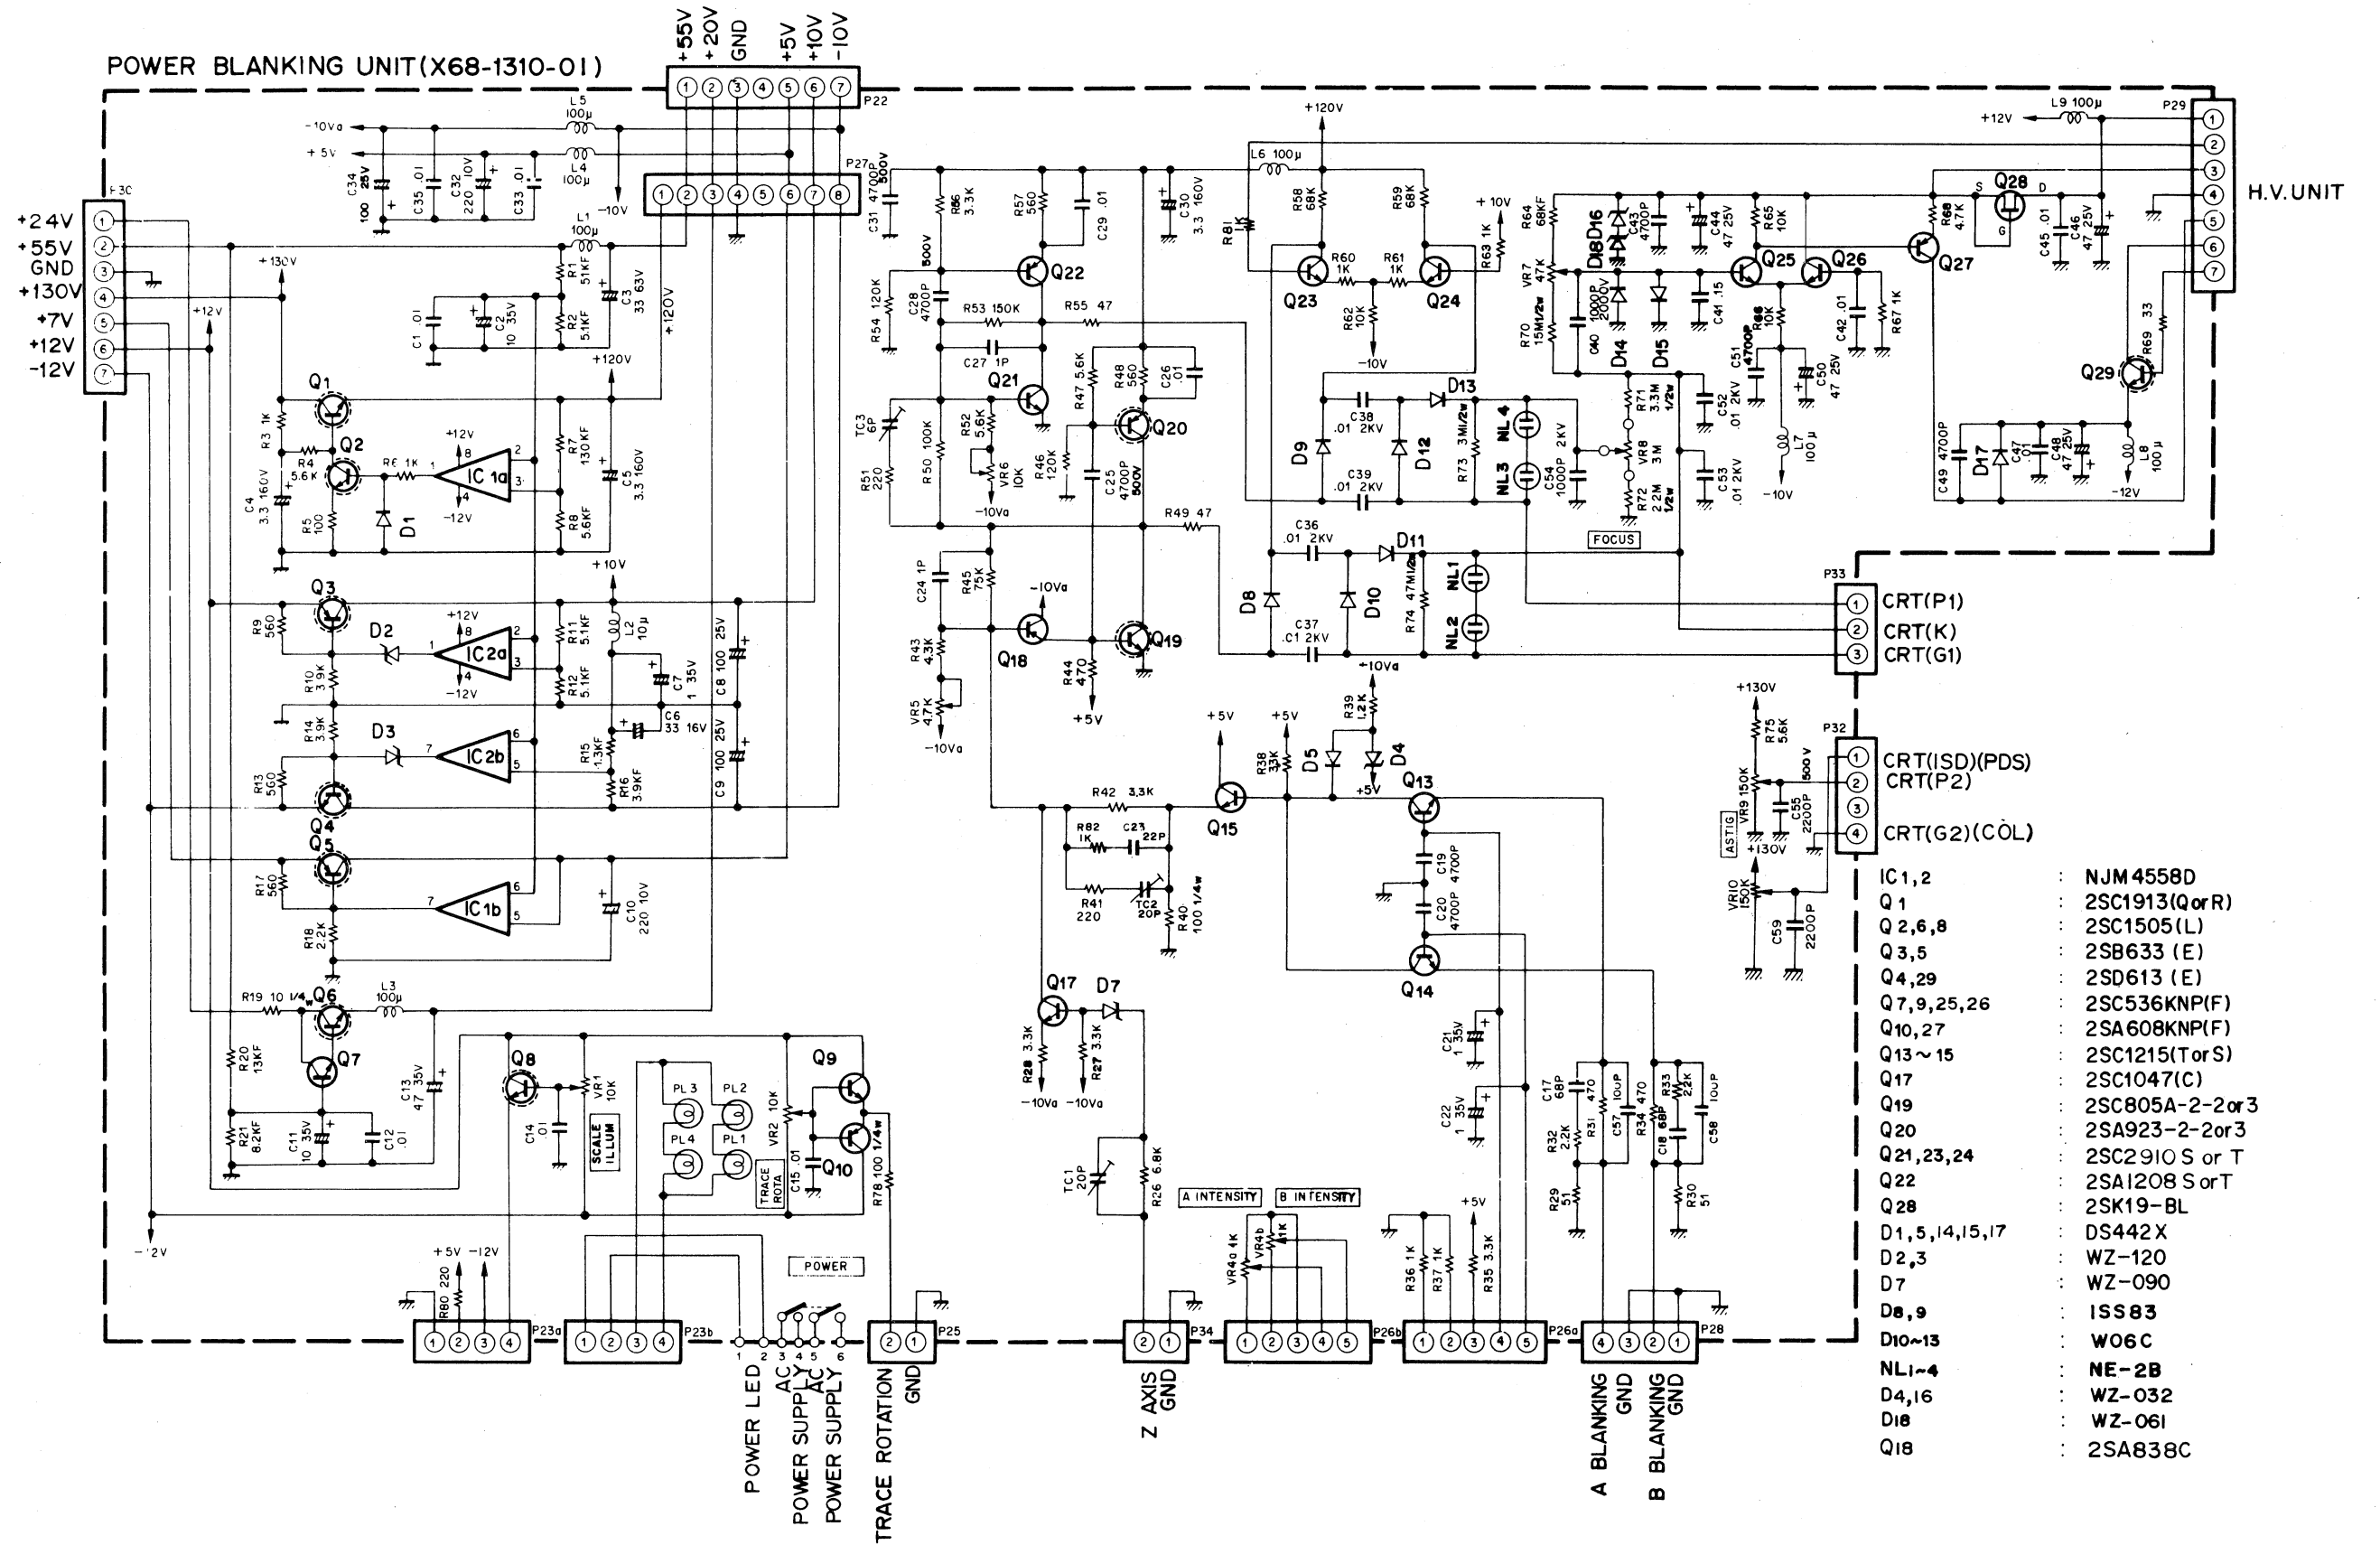

- | | |
|--------------------|--------------------|
| IC 1, 2 | : NJM 4558D |
| Q 1 | : 2SC1913(Q or R) |
| Q 2, 6, 8 | : 2SC1505(L) |
| Q 3, 5 | : 2SB633 (E) |
| Q 4, 29 | : 2SD613 (E) |
| Q 7, 9, 25, 26 | : 2SC536KNP(F) |
| Q 10, 27 | : 2SA608KNP(F) |
| Q 13 ~ 15 | : 2SC1215(Tor S) |
| Q 17 | : 2SC1047(C) |
| Q 19 | : 2SC805A-2-2 or 3 |
| Q 20 | : 2SA923-2-2 or 3 |
| Q 21, 23, 24 | : 2SC2910 S or T |
| Q 22 | : 2SA1208 S or T |
| Q 28 | : 2SK19-BL |
| D 1, 5, 14, 15, 17 | : DS442X |
| D 2, 3 | : WZ-120 |
| D 7 | : WZ-090 |
| D 8, 9 | : ISS83 |
| D 10 ~ 13 | : W06C |
| NL 1 ~ 4 | : NE-2B |
| D 4, 16 | : WZ-032 |
| D 18 | : WZ-061 |
| Q 18 | : 2SA838C |

POWER SUPPLY (W02-0405-15)

SWITCHING POWER SUPPLY(W02-0405-15)

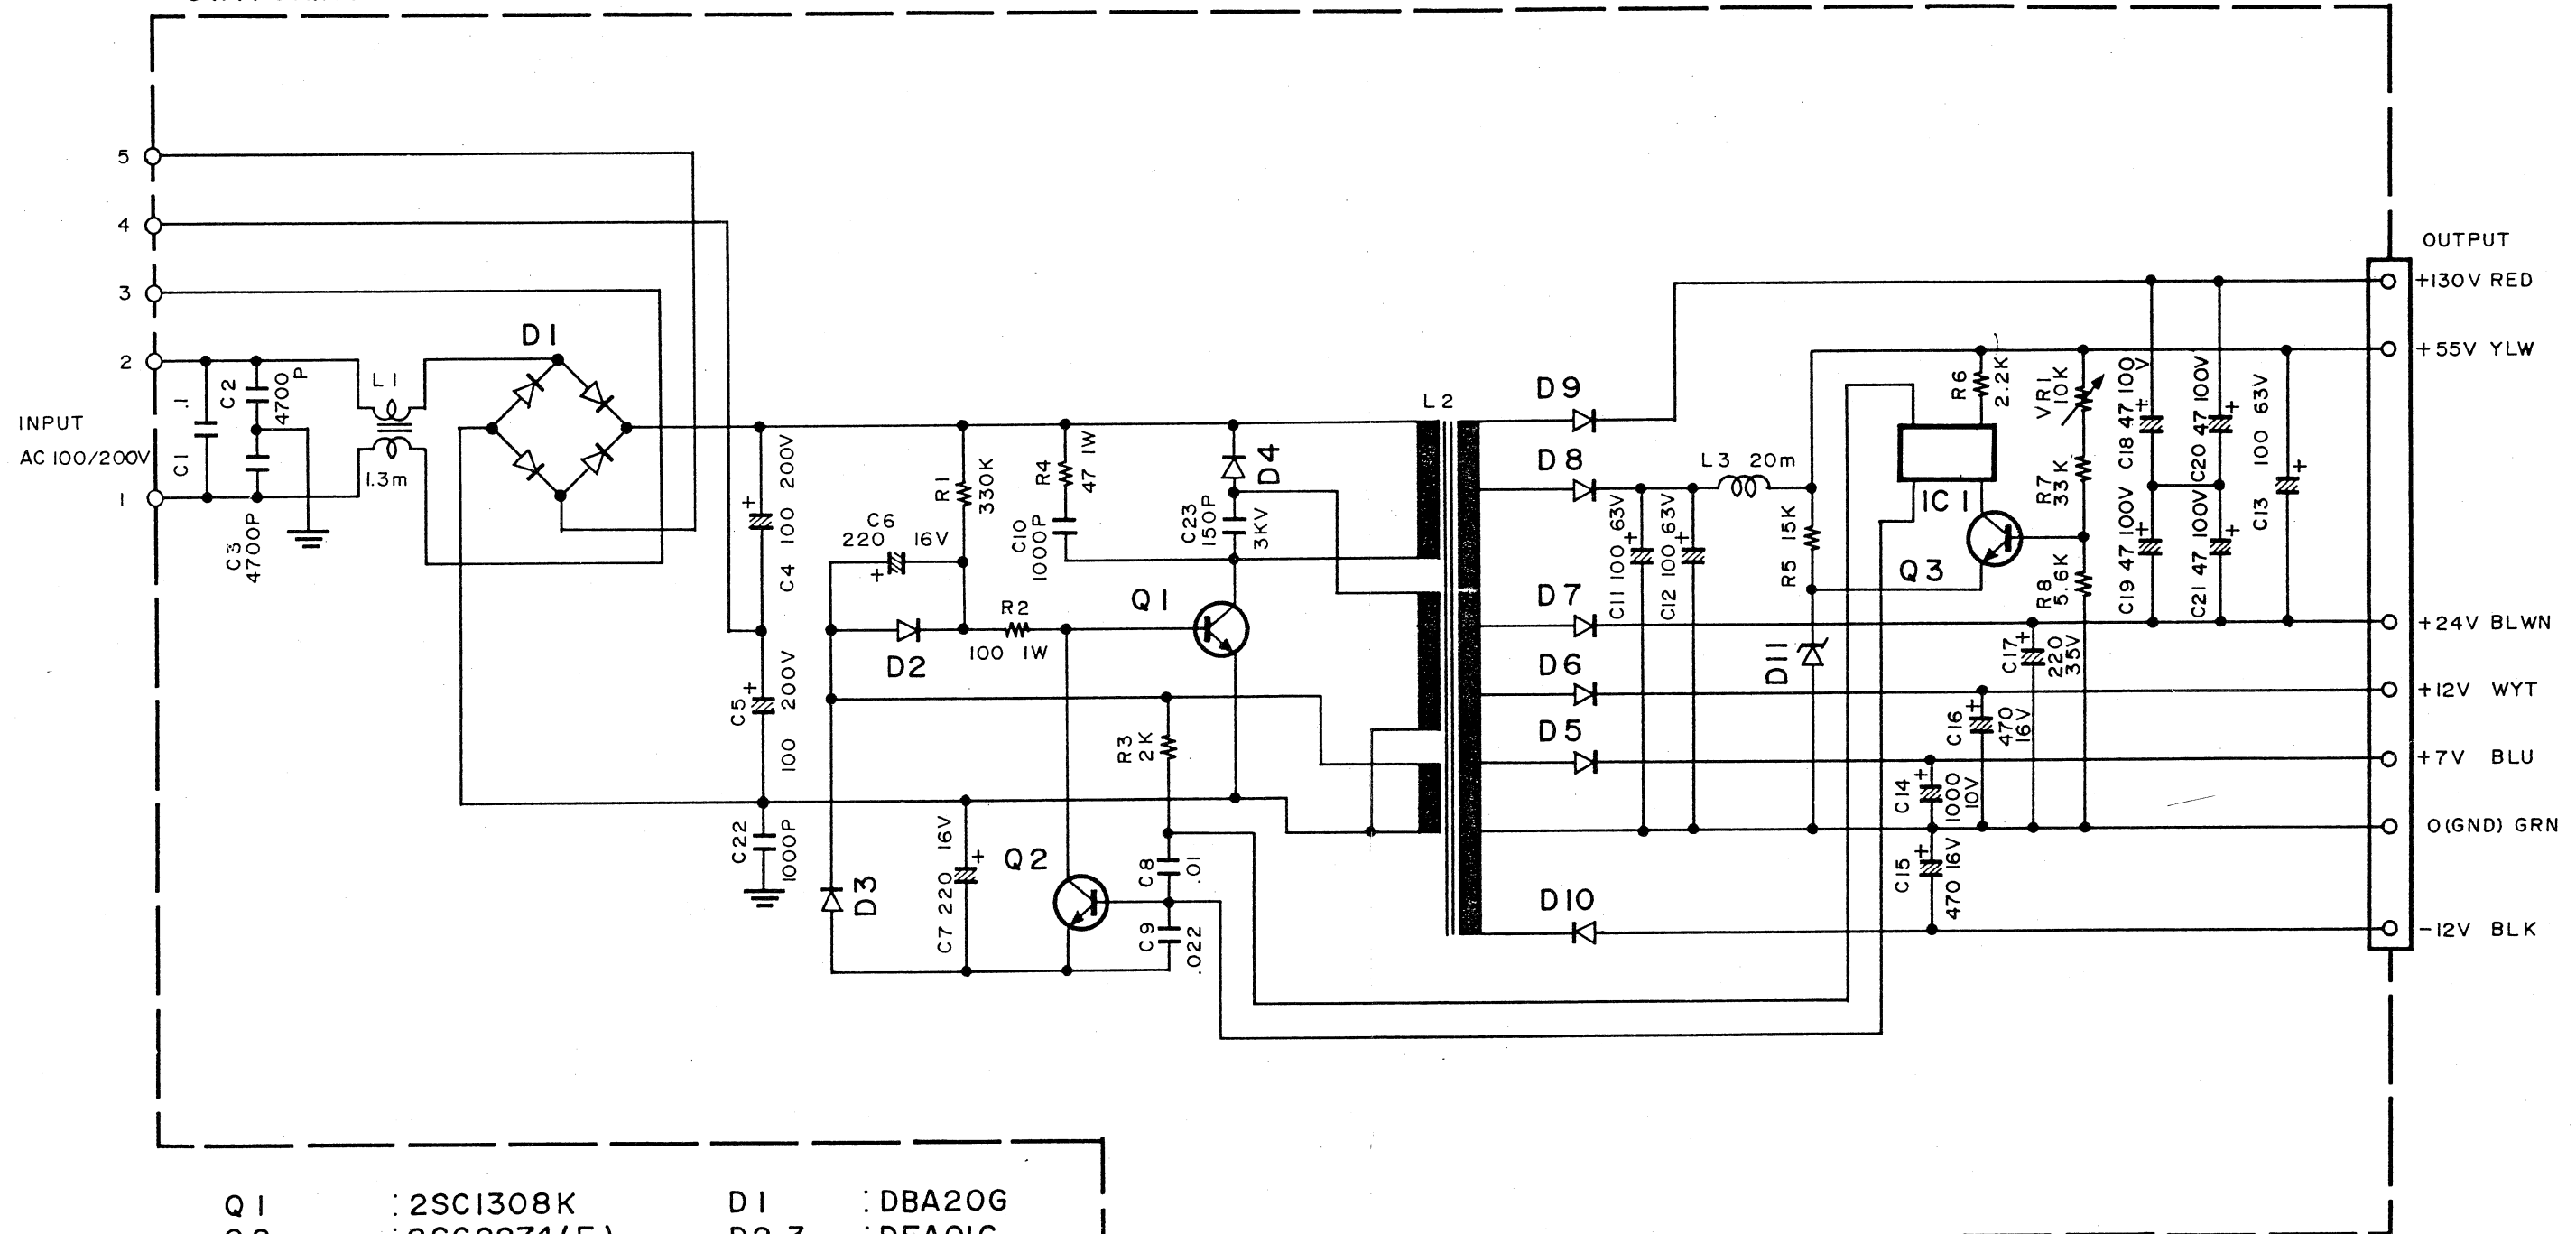

- | | | | |
|-----|--------------|---------|------------|
| Q1 | : 2SC1308K | D1 | : DBA20G |
| Q2 | : 2SC2274(E) | D2,3 | : DFA01C |
| Q3 | : 2SC2363(E) | D4 | : ERC25-06 |
| | | D5,6,10 | : S5KC20 |
| IC1 | : PC714U | D7~9 | : ERC25-04 |
| | | D11 | : GZA6.2Y |

- OUTPUT
- +130V RED
 - +55V YLW
 - +24V BLWN
 - +12V WYT
 - +7V BLU
 - 0 (GND) GRN
 - 12V BLK